

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102025\
 Data File : PS032093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2025 11:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 08:02:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.288	7.755	1653.1E6	431.6E6	346.772	392.229
Target Compounds							
2) T	3,5-DICHL...	6.477f	0.000	795243	0	<MDL	N.D. #
7) T	MCPA	7.811	8.248f	342963	20985666	<MDL	5.563 #
8) T	DICHLORPROP	8.185	0.000	1928027	0	<MDL	N.D. #
10) T	Pentachlo...	8.726	0.000	2803170	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.288	9.848f	4633329	13904788	<MDL	<MDL #
12) T	2,4,5-T	9.619f	10.311	3363904	13643182	<MDL	<MDL #
13) T	2,4-DB	10.159	10.880	1228880	2179794	<MDL	1.687 #
14) T	DINOSEB	11.362	0.000	4174624	0	<MDL	N.D. #
15) T	Picloram	11.217f	12.422f	751357	2690830	<MDL	<MDL #
16) T	DCPA	11.653	0.000	3401739	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102025\
Data File : PS032093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2025 11:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 08:02:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

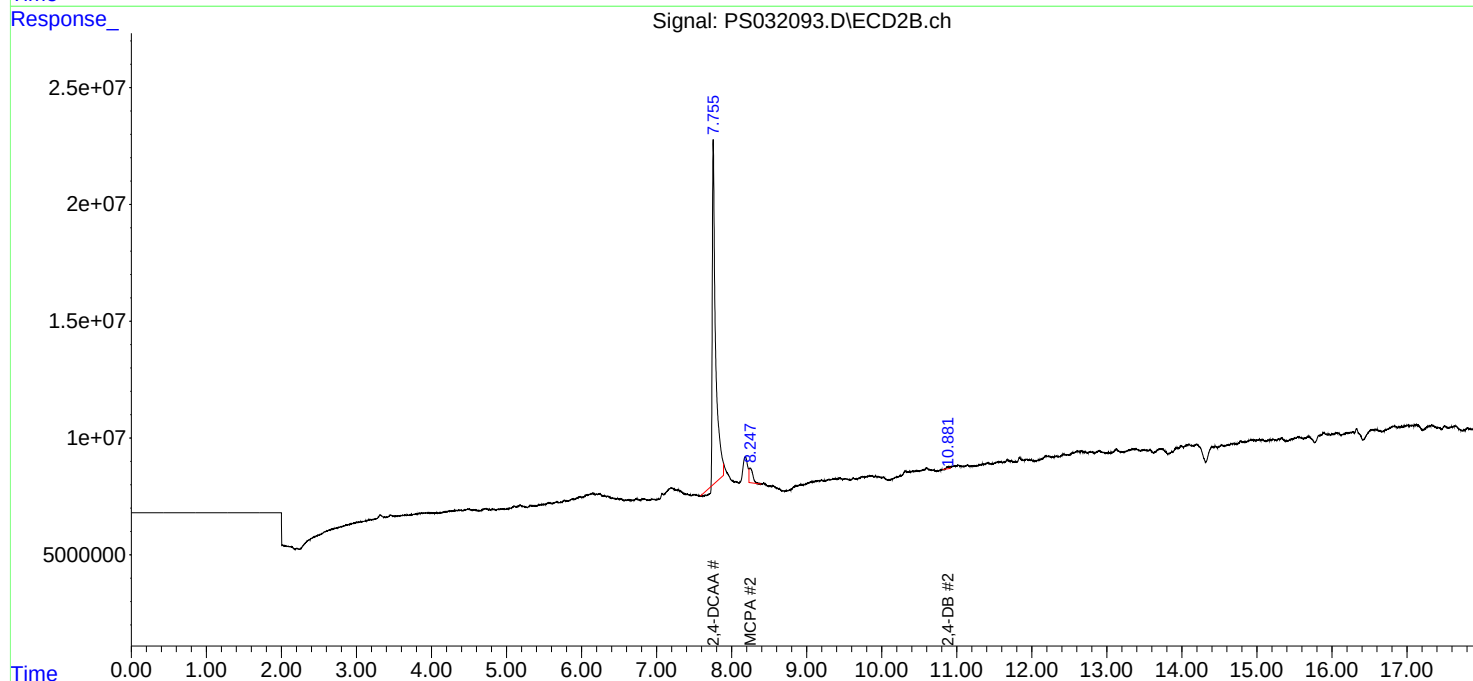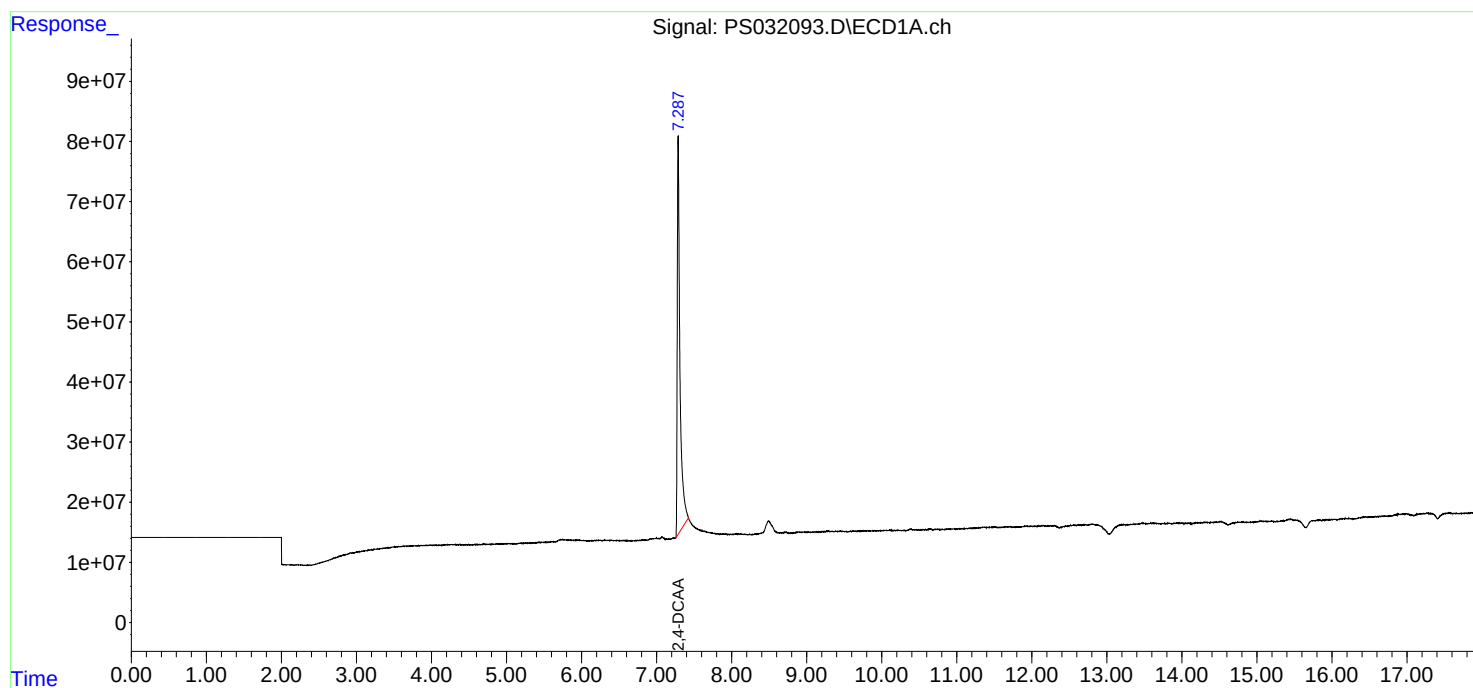


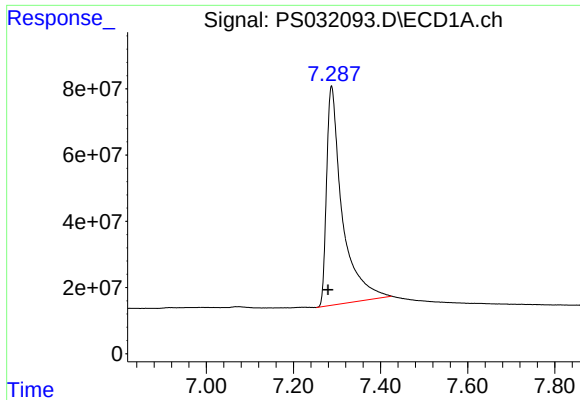

#4 2,4-DCAA


R.T.: 7.288 min
Delta R.T.: 0.008 min
Response: 1653074247
Conc: 346.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

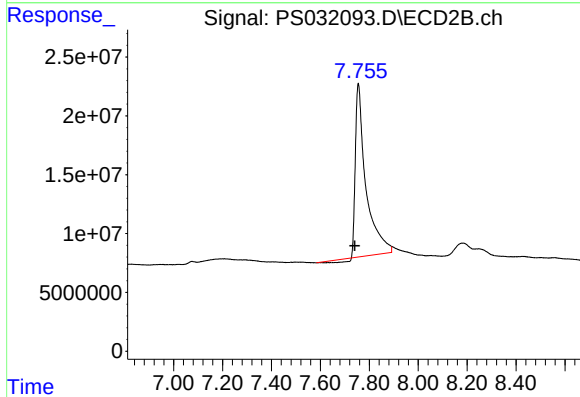


#4 2,4-DCAA

R.T.: 7.755 min
Delta R.T.: 0.014 min
Response: 431584975
Conc: 392.23 ng/ml

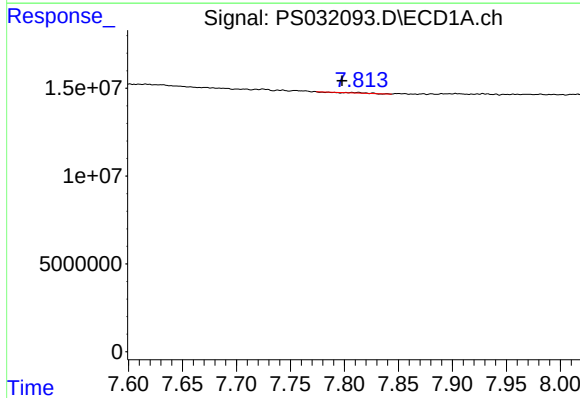


#7 MCPA

R.T.: 7.811 min
Delta R.T.: 0.013 min
Response: 342963
Conc: N.D.

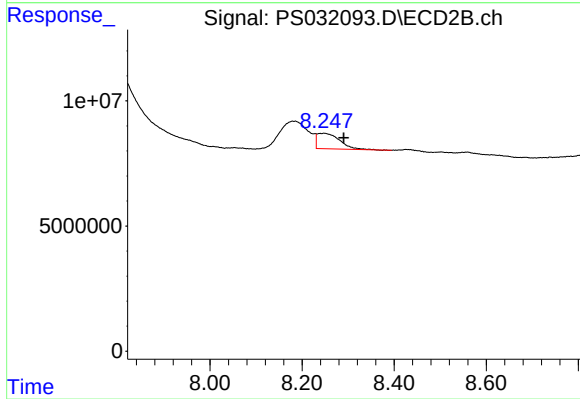

#7 MCPA


R.T.: 8.248 min
Delta R.T.: -0.043 min
Response: 20985666
Conc: 5.56 ug/ml

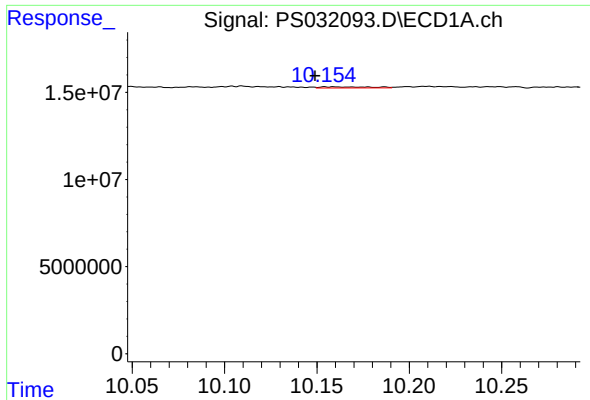

#13 2,4-DB

R.T.: 10.159 min
Delta R.T.: 0.010 min
Response: 1228880
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

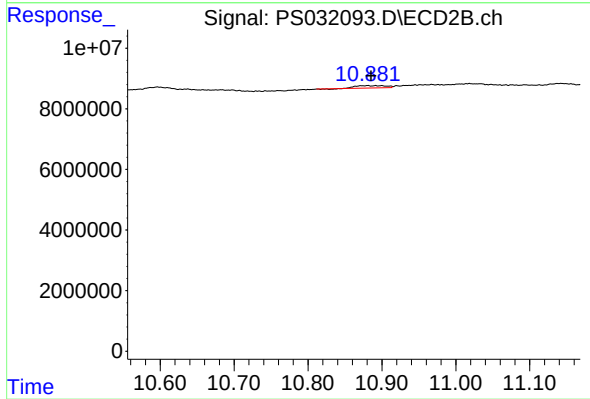

#13 2,4-DB

R.T.: 10.880 min
Delta R.T.: -0.005 min
Response: 2179794
Conc: 1.69 ng/ml