

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102025\
 Data File : PS032095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2025 12:13
 Operator : AR\AJ
 Sample : Q3352-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 08:03:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.292	7.753	611.7E6	181.1E6	128.320	164.580 #
Target Compounds							
1) T	Dalapon	2.639f	2.673	1402.5E6	1265.4E6	181.499	336.693 #
2) T	3,5-DICHL...	6.443	0.000	4535523	0	<MDL	N.D. #
3) T	4-Nitroph...	7.066	7.251f	2612867	-360017	1.958	N.D. #
5) T	DICAMBA	7.468	0.000	1709209	0	<MDL	N.D. #
6) T	MCPD	7.638	8.086f	2030990	4009701	<MDL	1.615 #
7) T	MCPA	7.753f	0.000	148.5E6	0	10.093	N.D. #
8) T	DICHLORPROP	8.183	8.667	1030550	28101729	<MDL	14.350 #
9) T	2,4-D	8.428	8.980	60577115	29970846	12.475	14.421
10) T	Pentachlo...	8.707	9.509	13361761	76411884	<MDL	1.474 #
11) T	2,4,5-TP ...	9.298	9.891	6669777	130.9E6	<MDL	6.522 #
12) T	2,4,5-T	9.555	0.000	134.1E6	0	5.312	N.D. #
13) T	2,4-DB	10.196f	0.000	203.5E6	0	65.644	N.D. #
14) T	DINOSEB	0.000	11.293f	0	22469854	N.D.	1.478
16) T	DCPA	11.644	12.307	31619515	57998705	<MDL	1.746 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102025\
Data File : PS032095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2025 12:13
Operator : AR\AJ
Sample : Q3352-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 08:03:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

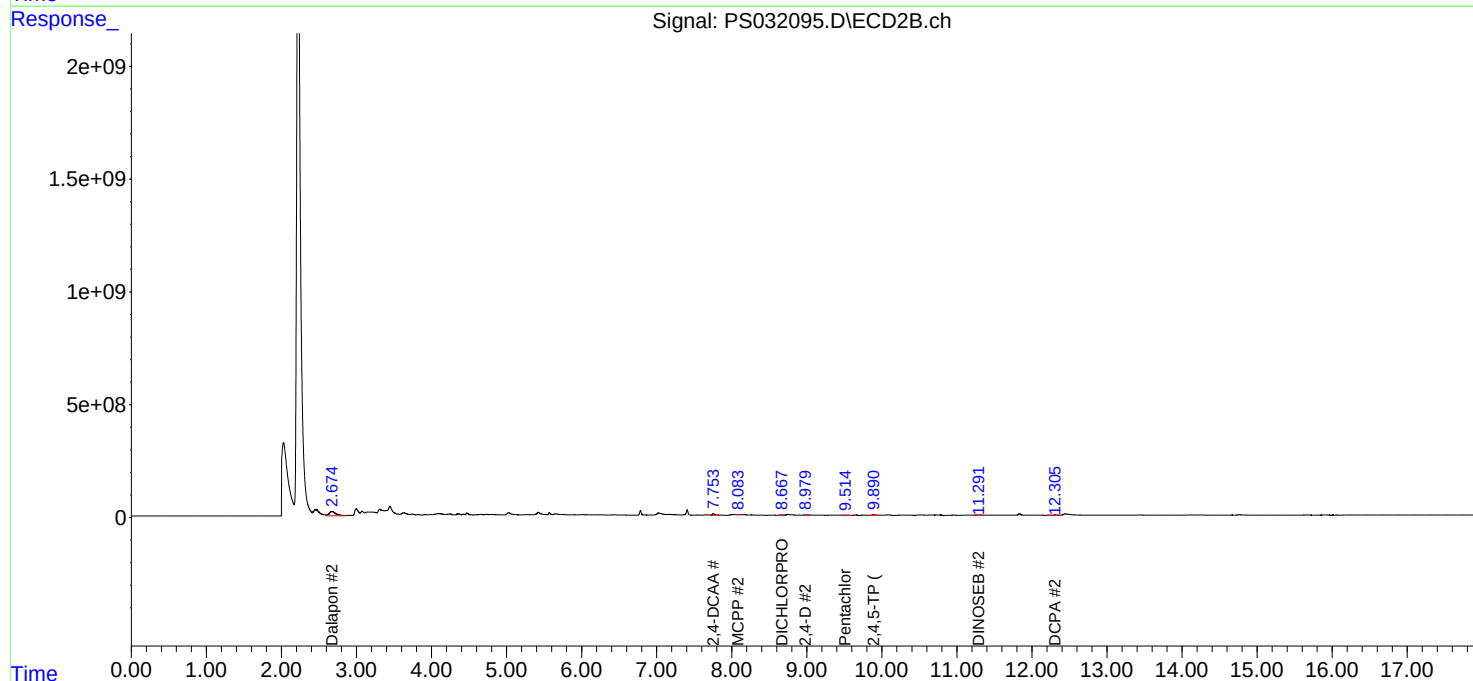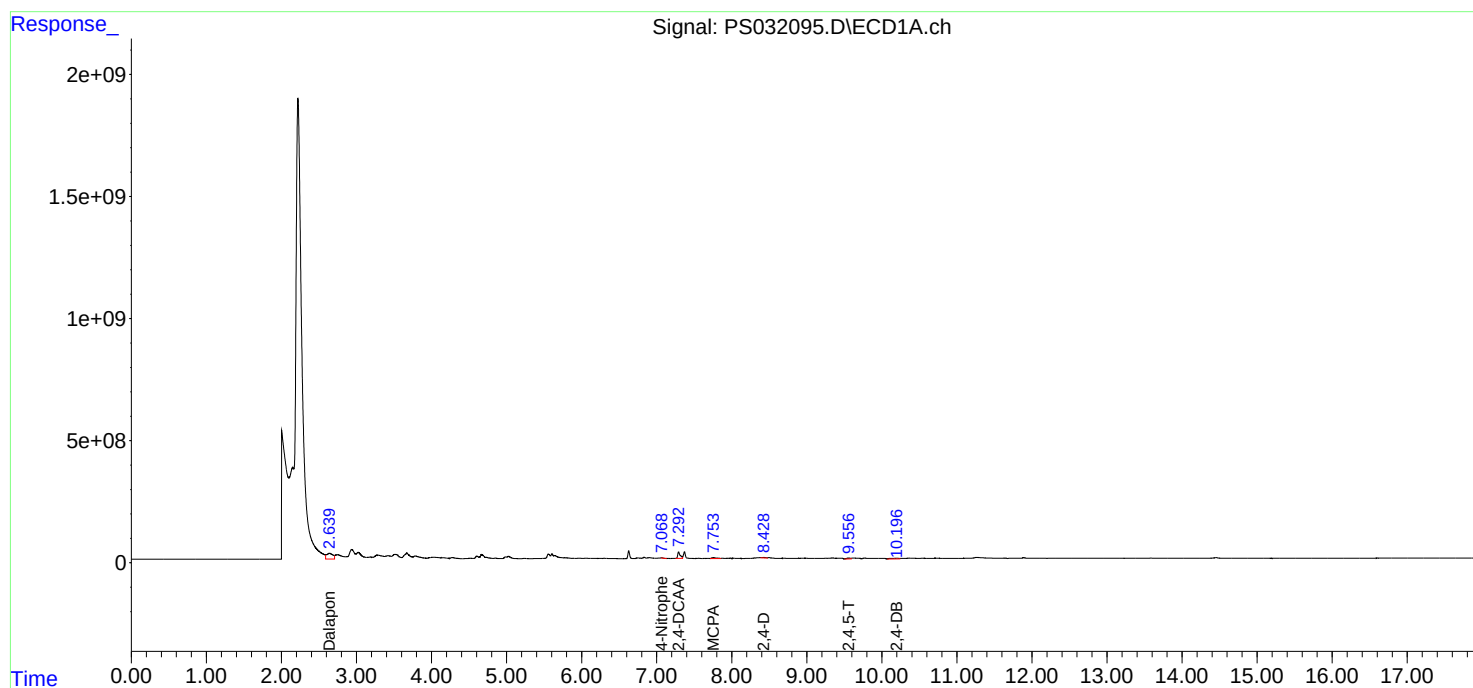


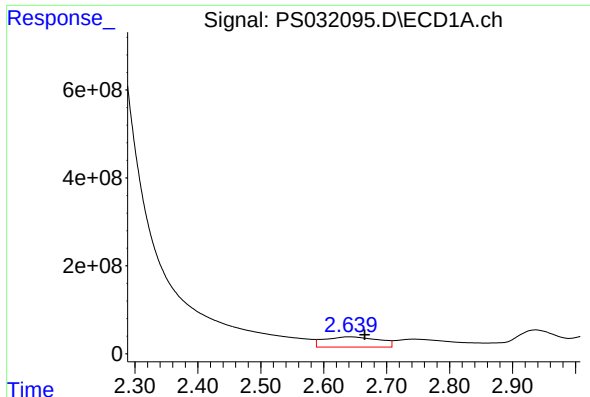

#1 Dalapon


R.T.: 2.639 min
Delta R.T.: -0.026 min
Response: 1402542559
Conc: 181.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

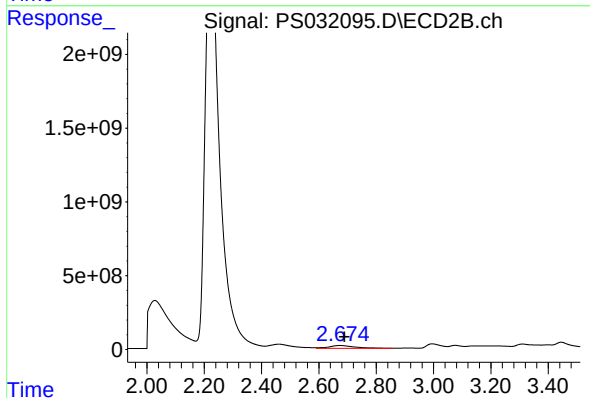


#1 Dalapon

R.T.: 2.673 min
Delta R.T.: -0.016 min
Response: 1265382656
Conc: 336.69 ng/ml

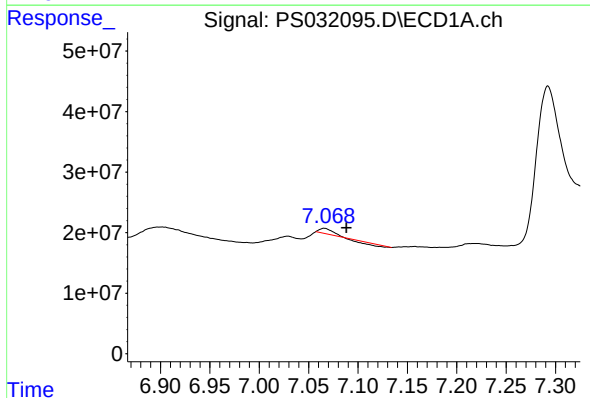


#3 4-Nitrophenol

R.T.: 7.066 min
Delta R.T.: -0.022 min
Response: 2612867
Conc: 1.96 ng/ml

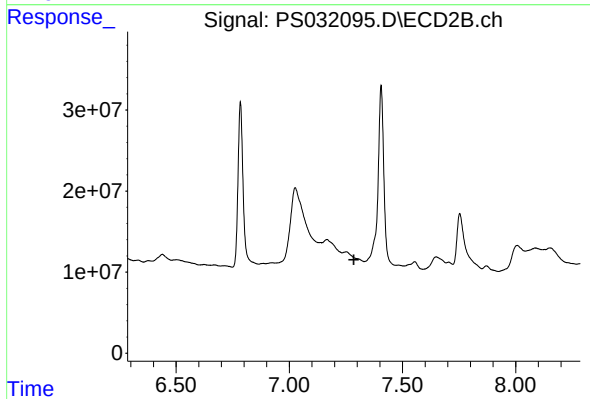

#3 4-Nitrophenol


R.T.: 7.251 min
Delta R.T.: -0.034 min
Response: -360017
Conc: N.D.

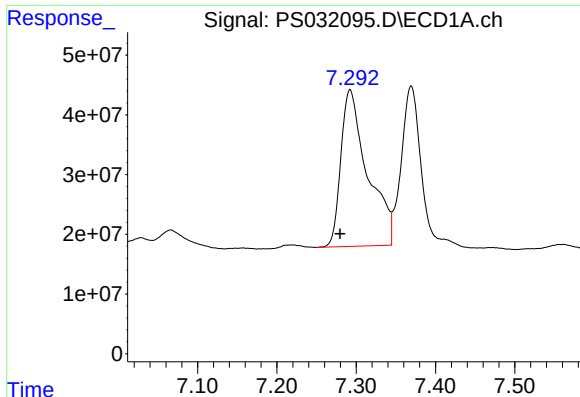

#4 2,4-DCAA


R.T.: 7.292 min
Delta R.T.: 0.013 min
Response: 611703775
Conc: 128.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

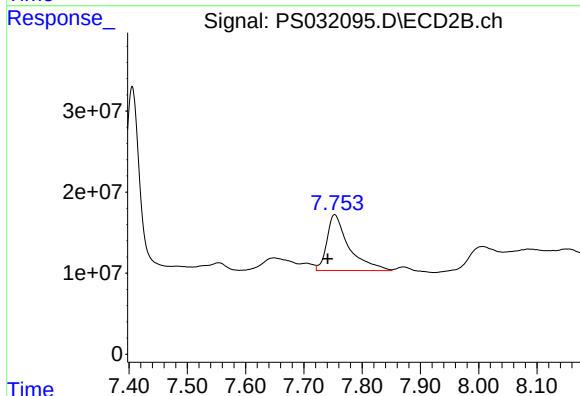


#4 2,4-DCAA

R.T.: 7.753 min
Delta R.T.: 0.012 min
Response: 181093543
Conc: 164.58 ng/ml

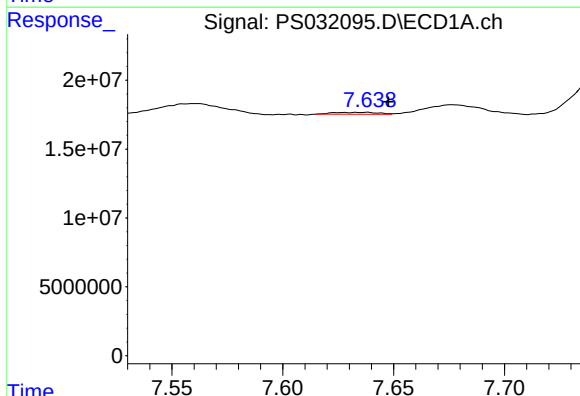


#6 MCP

R.T.: 7.638 min
Delta R.T.: -0.010 min
Response: 2030990
Conc: N.D.

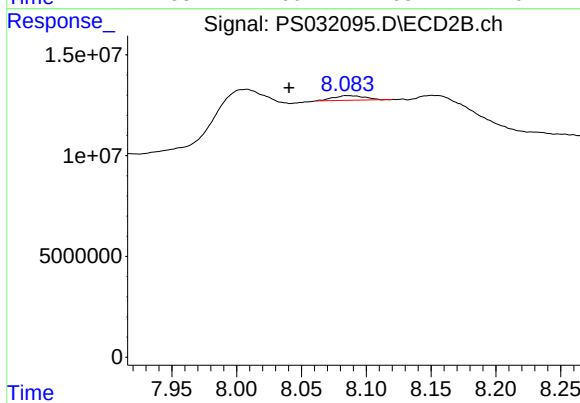

#6 MCP


R.T.: 8.086 min
Delta R.T.: 0.046 min
Response: 4009701
Conc: 1.62 ug/ml

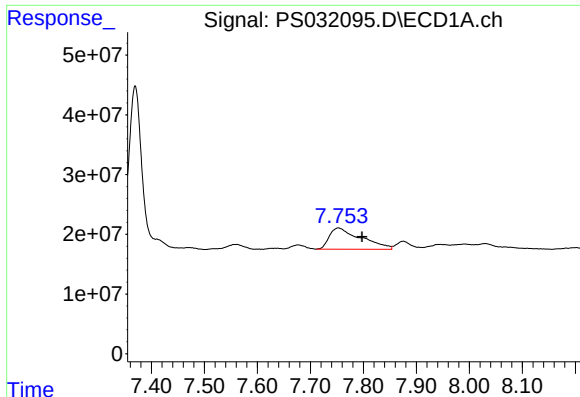

#7 MCPA


R.T.: 7.753 min
Delta R.T.: -0.045 min
Response: 148534512
Conc: 10.09 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

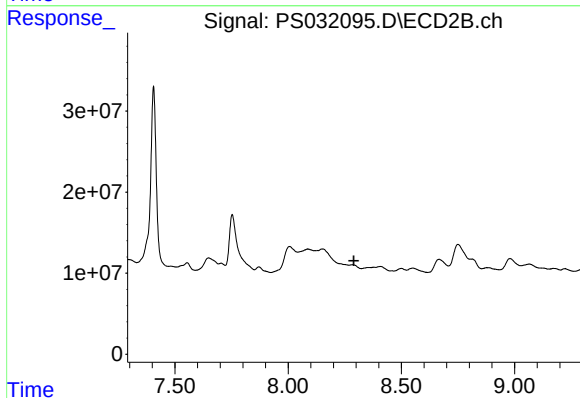


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 8.290 min
Response: 0
Conc: N.D.

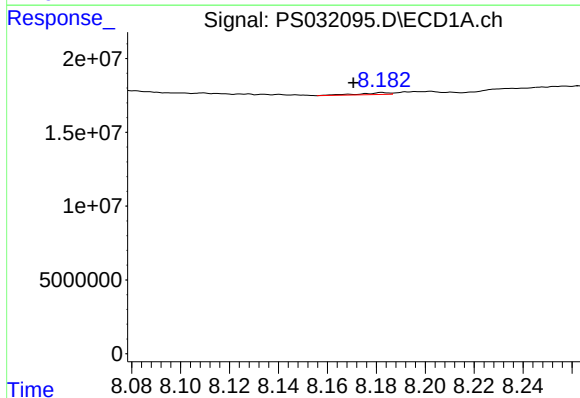


#8 DICHLORPROP

R.T.: 8.183 min
Delta R.T.: 0.012 min
Response: 1030550
Conc: N.D.

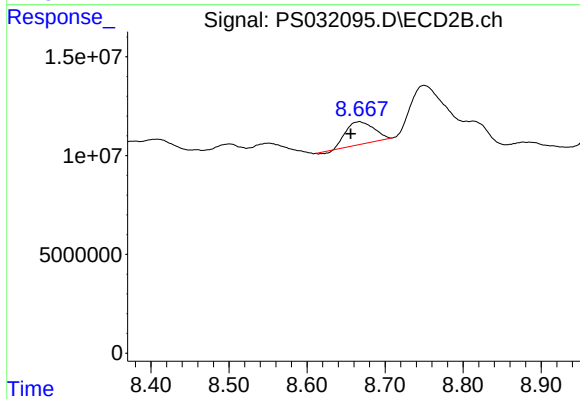

#8 DICHLORPROP


R.T.: 8.667 min
Delta R.T.: 0.010 min
Response: 28101729
Conc: 14.35 ng/ml

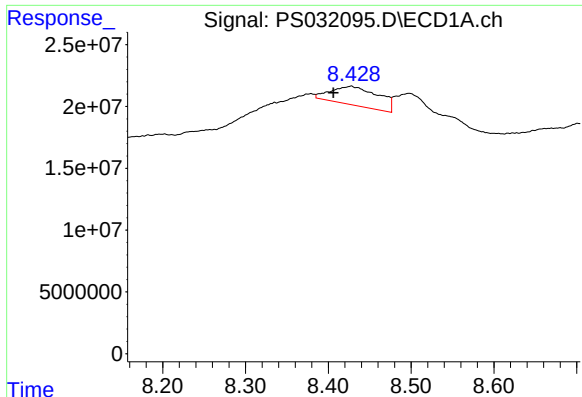

#9 2,4-D


R.T.: 8.428 min
Delta R.T.: 0.021 min
Response: 60577115
Conc: 12.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

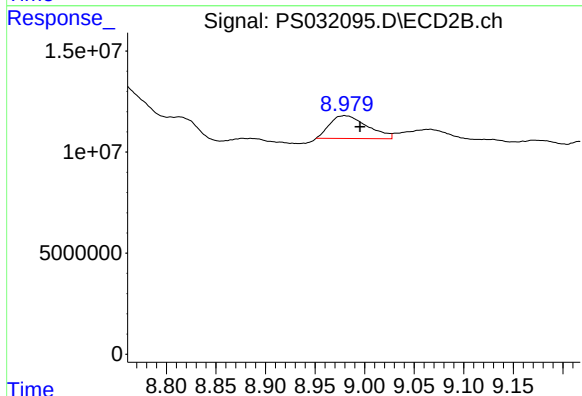


#9 2,4-D

R.T.: 8.980 min
Delta R.T.: -0.015 min
Response: 29970846
Conc: 14.42 ng/ml

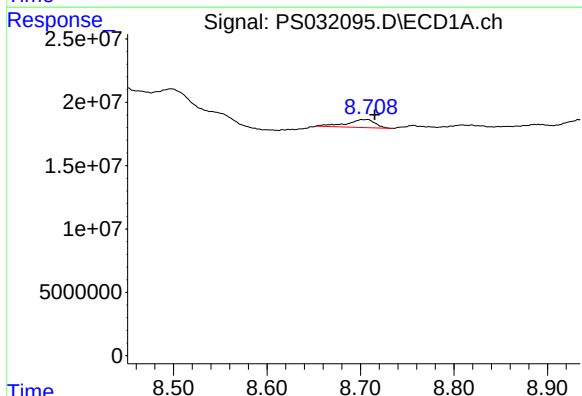


#10 Pentachlorophenol

R.T.: 8.707 min
Delta R.T.: -0.008 min
Response: 13361761
Conc: N.D.

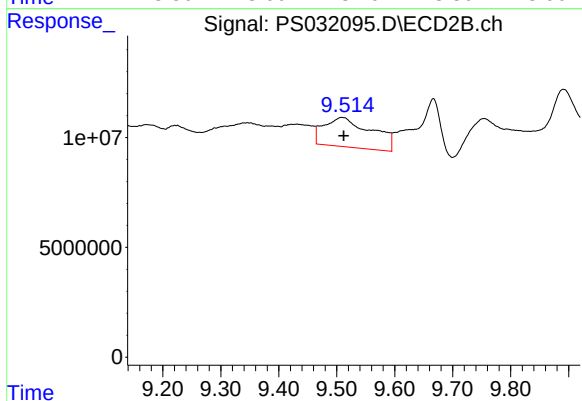

#10 Pentachlorophenol


R.T.: 9.509 min
Delta R.T.: -0.003 min
Response: 76411884
Conc: 1.47 ng/ml

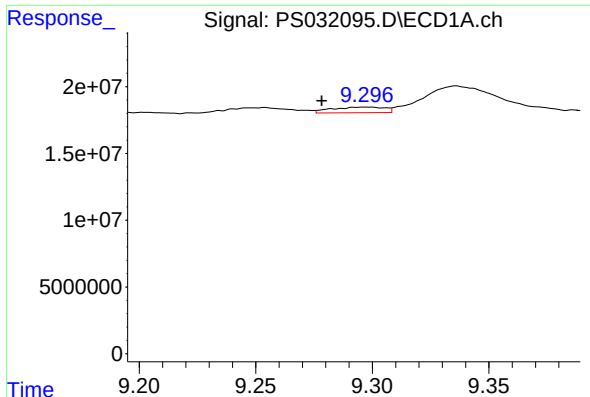

#11 2,4,5-TP (SILVEX)


R.T.: 9.298 min
Delta R.T.: 0.019 min
Response: 6669777
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

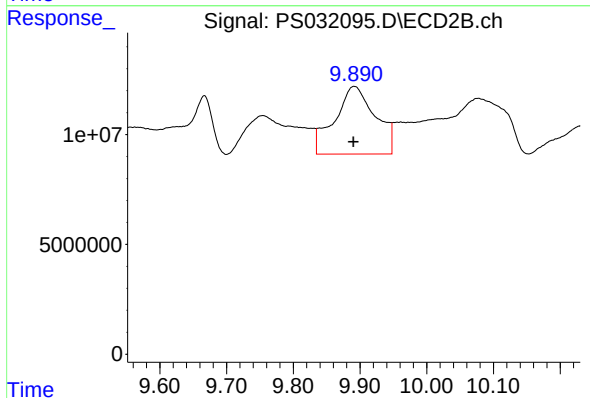


#11 2,4,5-TP (SILVEX)

R.T.: 9.891 min
Delta R.T.: 0.001 min
Response: 130923238
Conc: 6.52 ng/ml

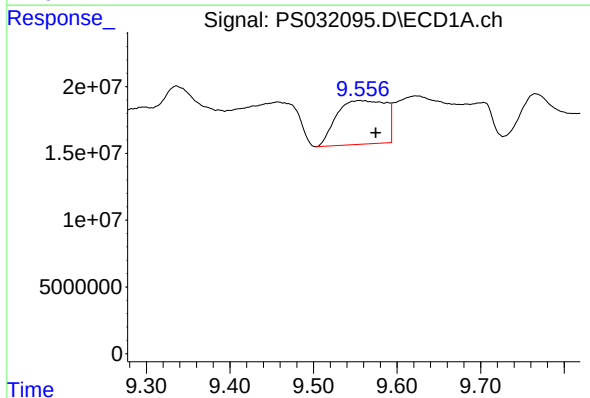


#12 2,4,5-T

R.T.: 9.555 min
Delta R.T.: -0.019 min
Response: 134098228
Conc: 5.31 ng/ml

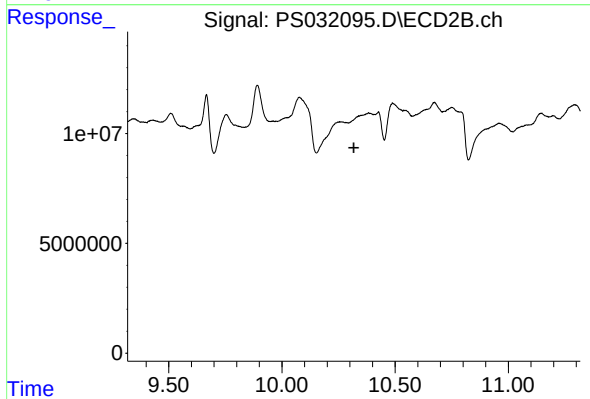

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 10.318 min
Response: 0
Conc: N.D.

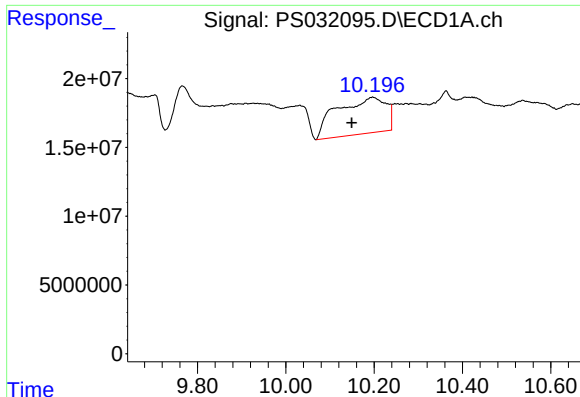

#13 2,4-DB


R.T.: 10.196 min
Delta R.T.: 0.047 min
Response: 203517158
Conc: 65.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

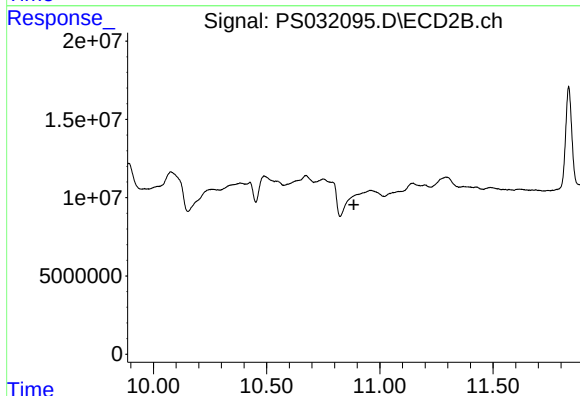


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.885 min
Response: 0
Conc: N.D.

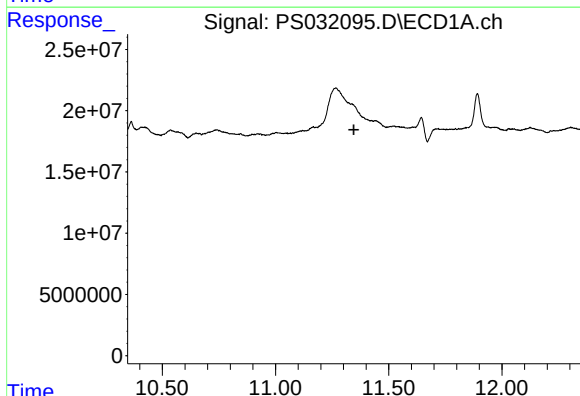


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.346 min
Response: 0
Conc: N.D.

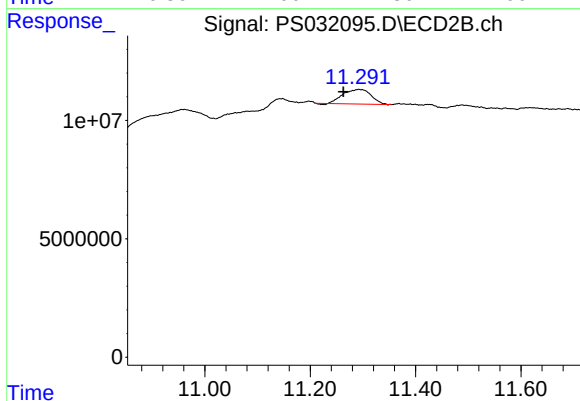

#14 DINOSEB


R.T.: 11.293 min
Delta R.T.: 0.030 min
Response: 22469854
Conc: 1.48 ng/ml

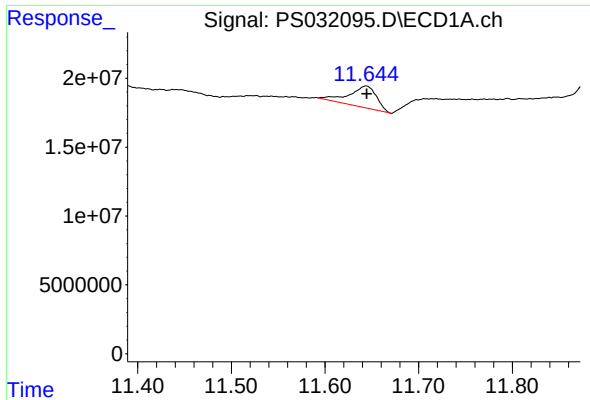

#16 DCPA

R.T.: 11.644 min
Delta R.T.: 0.000 min
Response: 31619515
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

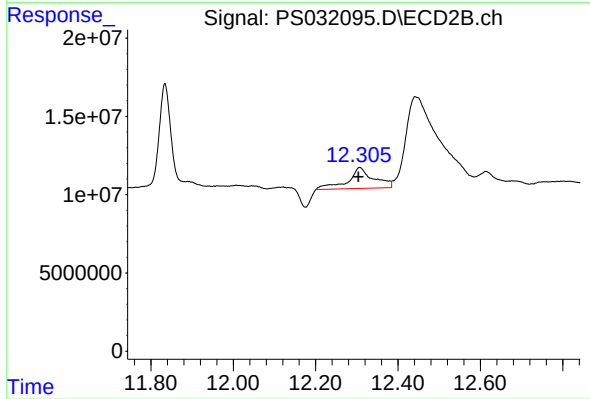

#16 DCPA

R.T.: 12.307 min
Delta R.T.: 0.003 min
Response: 57998705
Conc: 1.75 ng/ml