

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102025\
 Data File : PS032098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2025 16:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 08:03:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.748	1717.9E6	444.9E6	360.371	404.317
Target Compounds							
2) T	3,5-DICHL...	6.458	0.000	848936	0	<MDL	N.D. #
3) T	4-Nitroph...	7.075	0.000	3285491	0	2.462	N.D. #
6) T	MCP	7.647	0.000	192795	0	<MDL	N.D. #
8) T	DICHLORPROP	8.183	0.000	5822549	0	1.225	N.D. #
9) T	2,4-D	8.407	0.000	2518497	0	<MDL	N.D. #
10) T	Pentachlo...	8.718	9.510	2860426	5046129	<MDL	<MDL #
11) T	2,4,5-TP ...	9.288	0.000	2107802	0	<MDL	N.D. #
12) T	2,4,5-T	9.581	10.281f	2856093	97685775	<MDL	5.698 #
13) T	2,4-DB	10.151	0.000	2194178	0	<MDL	N.D. #
14) T	DINOSEB	11.336	0.000	2592643	0	<MDL	N.D. #
15) T	Picloram	11.170	0.000	32861	0	<MDL	N.D. #
16) T	DCPA	11.651	12.319	3061864	5326949	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102025\
Data File : PS032098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2025 16:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 08:03:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

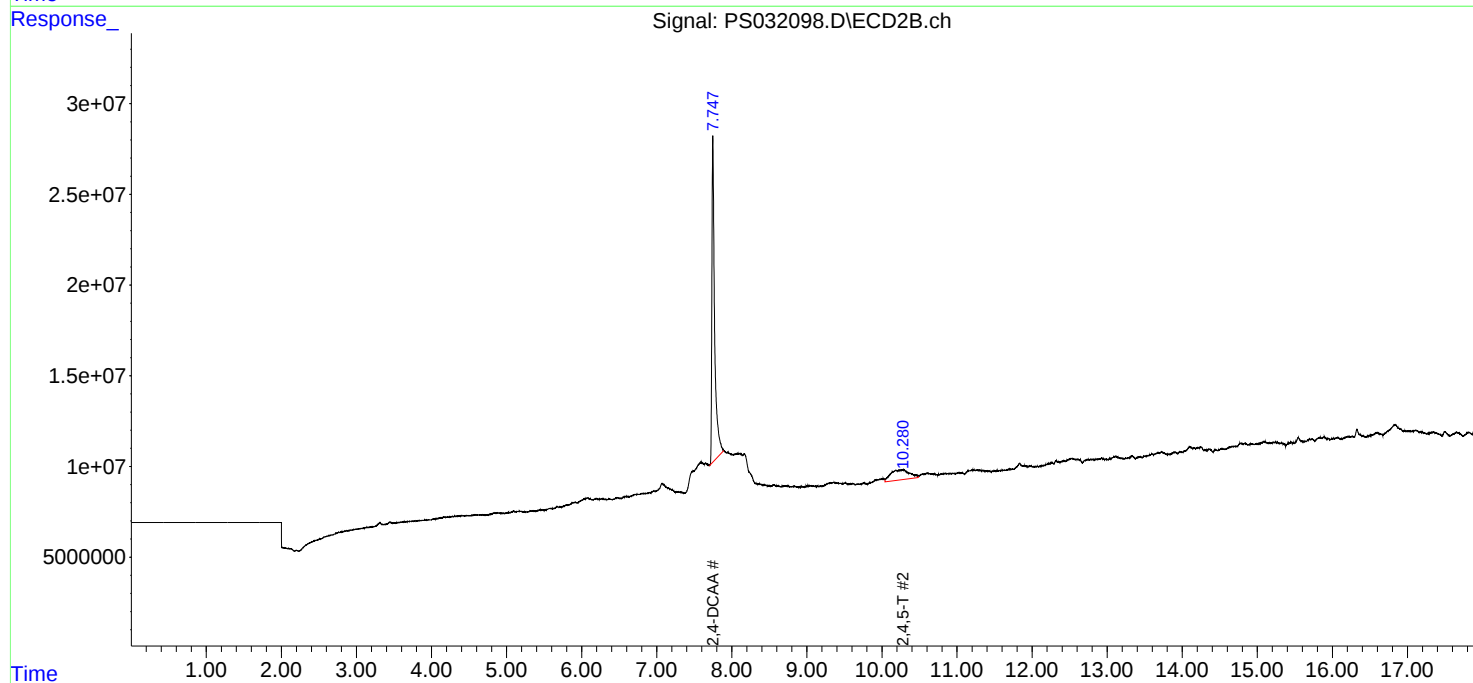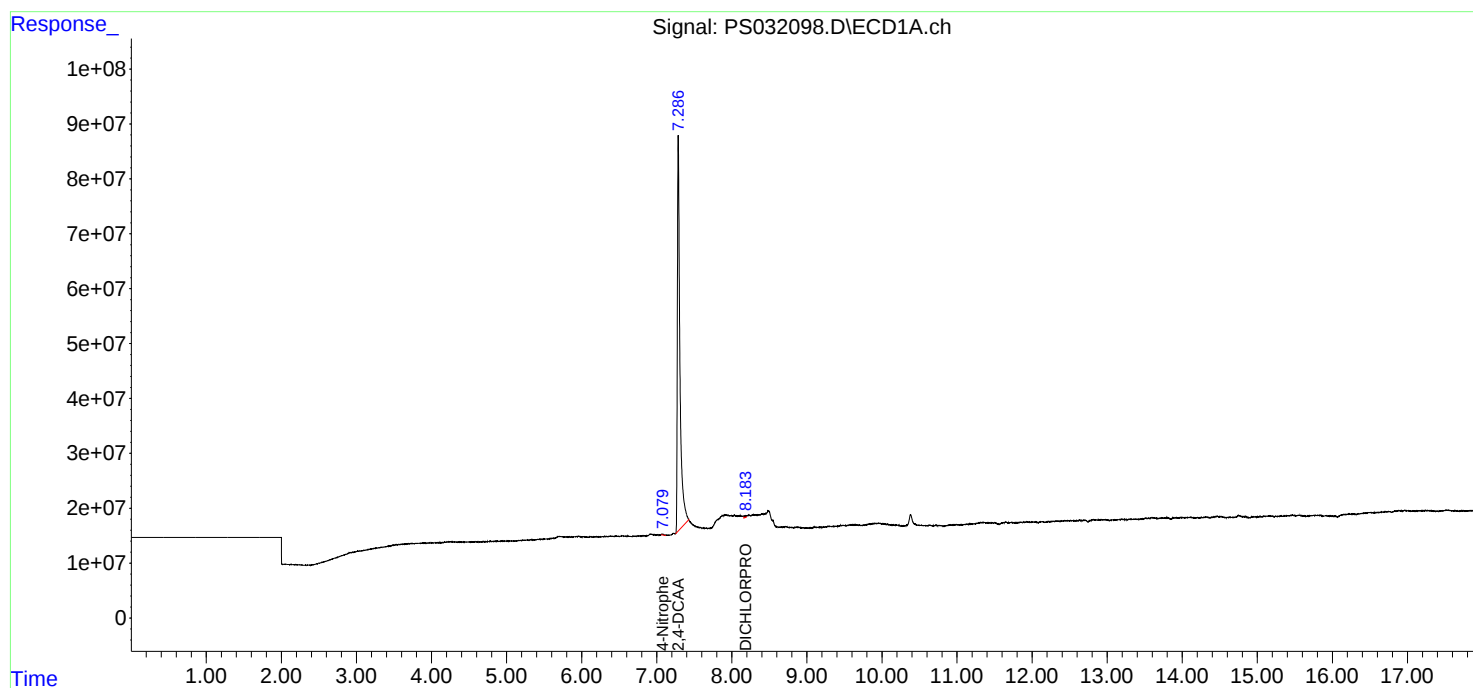


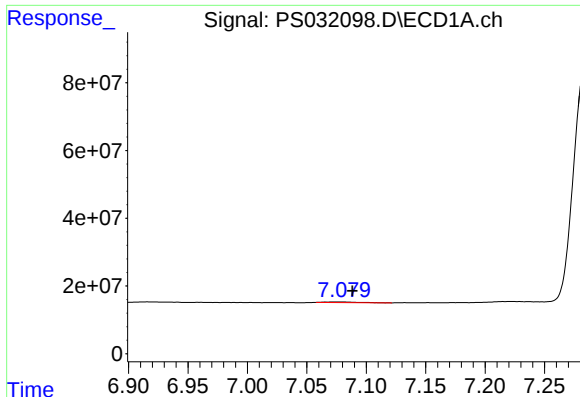

#3 4-Nitrophenol


R.T.: 7.075 min
Delta R.T.: -0.013 min
Response: 3285491
Conc: 2.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

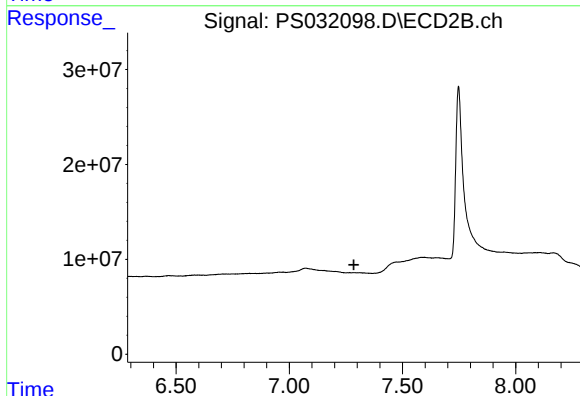


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.285 min
Response: 0
Conc: N.D.

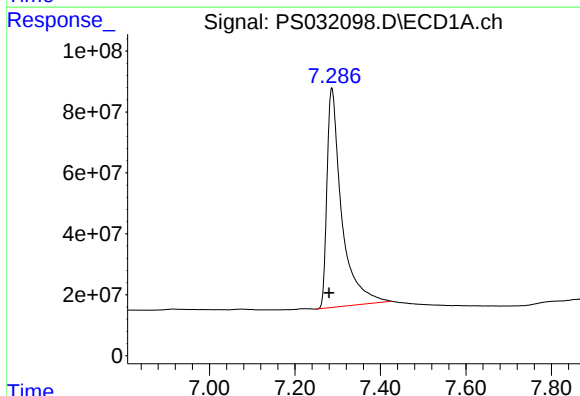


#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: 0.007 min
Response: 1717900293
Conc: 360.37 ng/ml

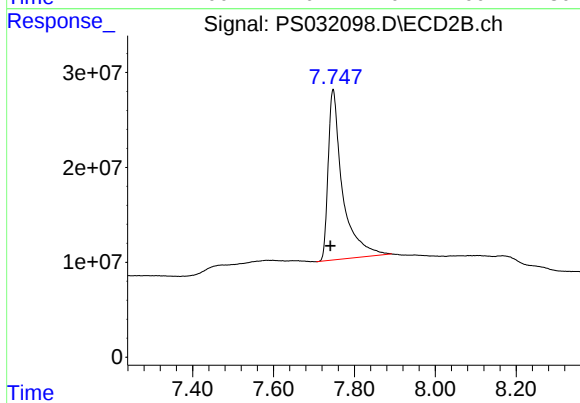

#4 2,4-DCAA


R.T.: 7.748 min
Delta R.T.: 0.007 min
Response: 444886326
Conc: 404.32 ng/ml

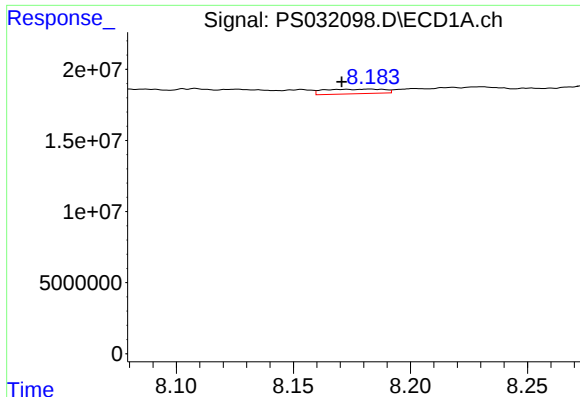

#8 DICHLORPROP


R.T.: 8.183 min
Delta R.T.: 0.012 min
Response: 5822549
Conc: 1.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

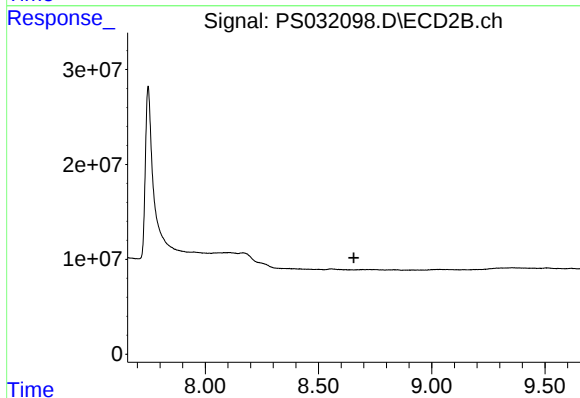


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.656 min
Response: 0
Conc: N.D.

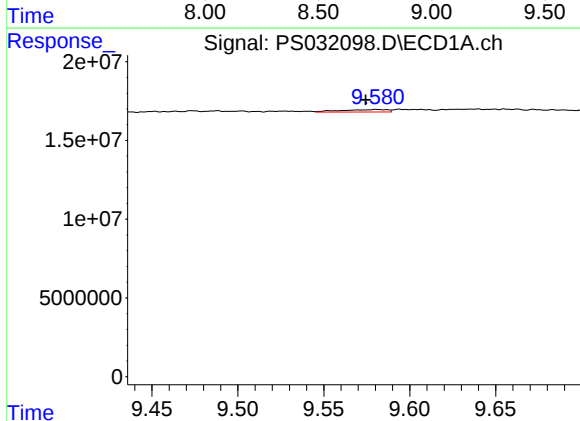

#12 2,4,5-T

R.T.: 9.581 min
Delta R.T.: 0.006 min
Response: 2856093
Conc: N.D.

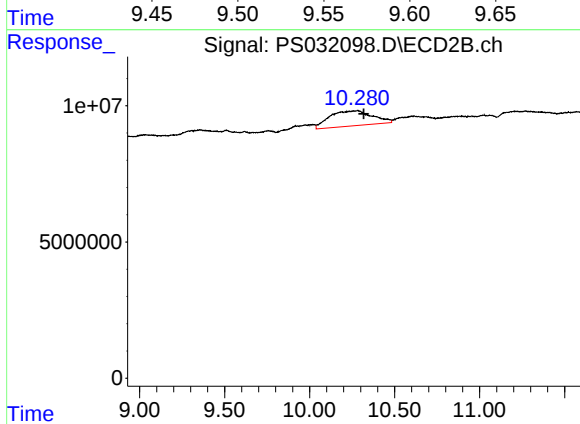

#12 2,4,5-T

R.T.: 10.281 min
Delta R.T.: -0.037 min
Response: 97685775
Conc: 5.70 ng/ml