

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102119\
 Data File : PS007237.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2019 18:45
 Operator : SM\AJ
 Sample : K5420-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 05:13:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.478	5.170	397.4E6	213.8E6	290.350	303.990
Target Compounds							
1) T	Dalapon	2.033	1.705	119.1E6	325.8E6	71.153	357.980 #
2) T	3,5-DICHL...	0.000	4.503	0	40714431	N.D.	47.319
5) T	DICAMBA	5.571	0.000	60890318	0	12.393	N.D. #
7) T	MCPA	0.000	5.541	0	28051675	N.D.	9.649
9) T	2,4-D	0.000	6.107	0	9793713	N.D.	12.276
10) T	Pentachlo...	0.000	6.463	0	20245871	N.D.	2.105
11) T	2,4,5-TP ...	0.000	6.772	0	26158678	N.D.	6.877
12) T	2,4,5-T	7.436	0.000	140.6E6	0	18.389	N.D. #
14) T	DINOSEB	0.000	7.963	0	22900088	N.D.	8.157
15) T	Picloram	0.000	8.922	0	47782529	N.D.	7.782
16) T	DCPA	0.000	8.922	0	47782529	N.D.	9.529



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102119\
Data File : PS007237.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2019 18:45
Operator : SM\AJ
Sample : K5420-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 05:13:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

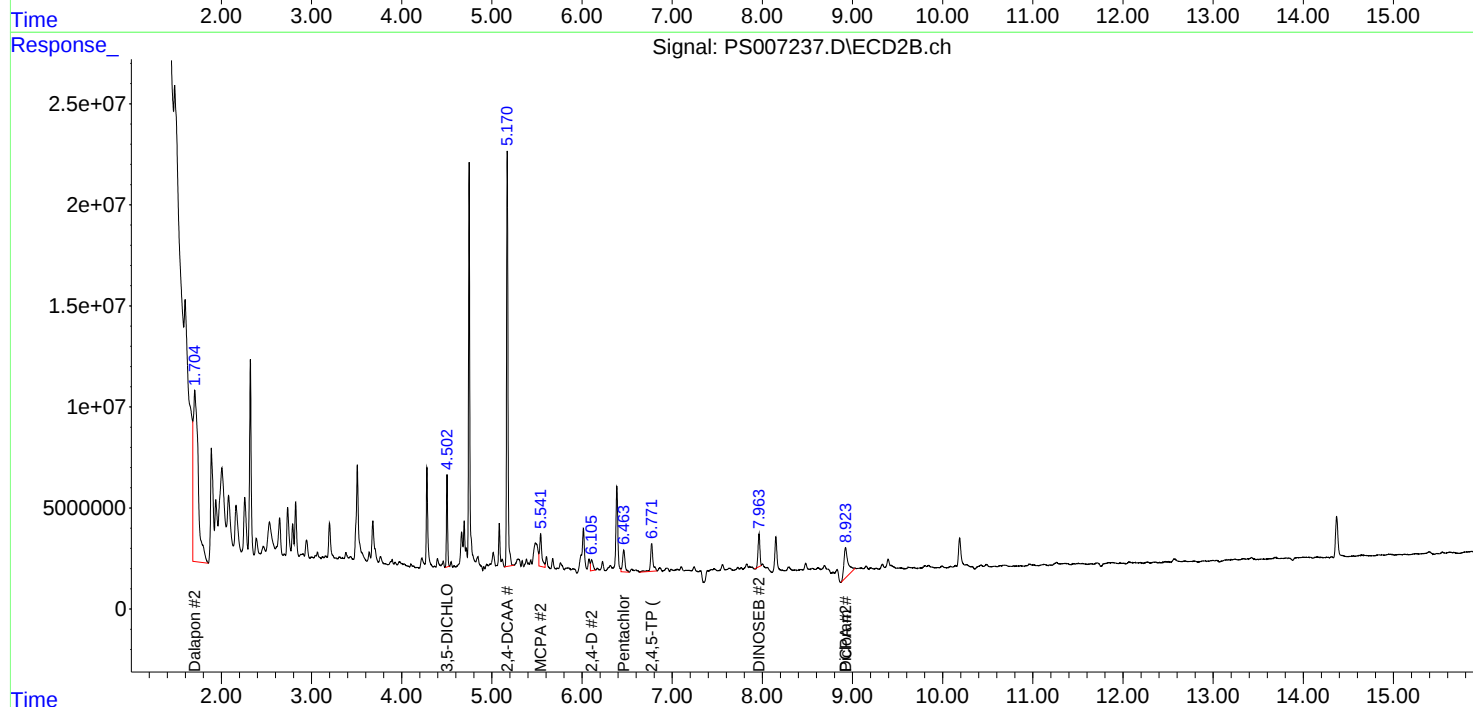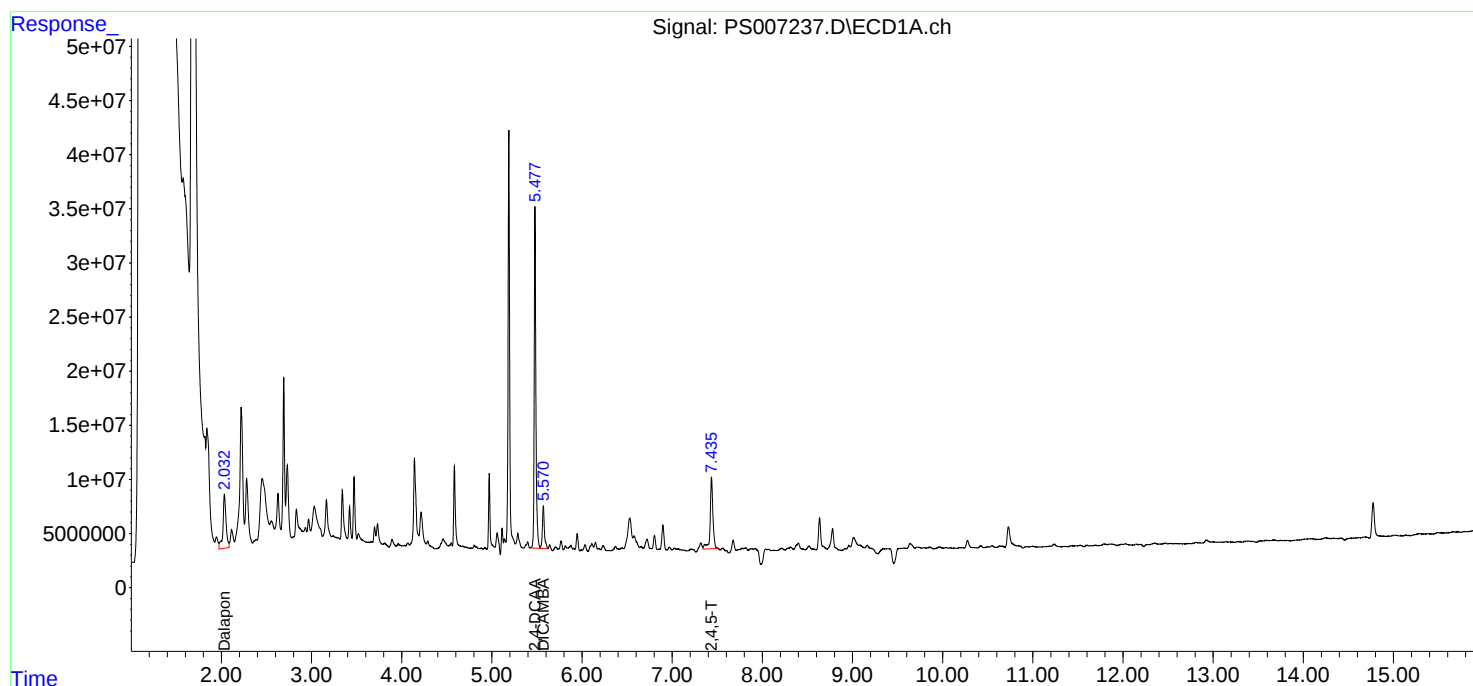


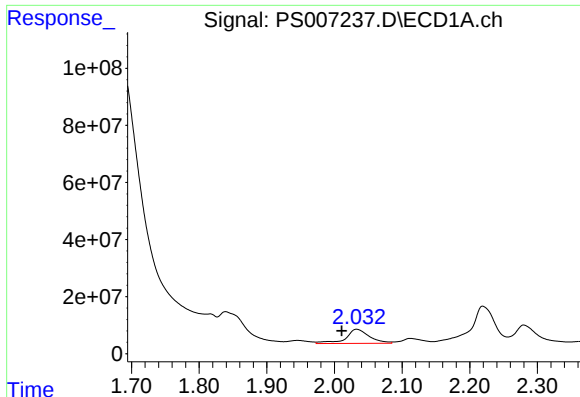

#1 Dalapon


R.T.: 2.033 min
Delta R.T.: 0.022 min
Response: 119058484
Conc: 71.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

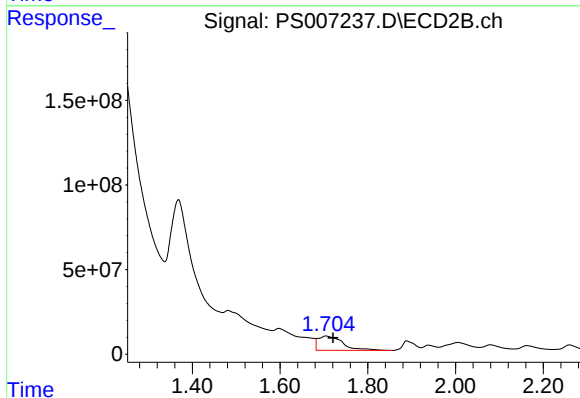


#1 Dalapon

R.T.: 1.705 min
Delta R.T.: -0.016 min
Response: 325763153
Conc: 357.98 ng/ml

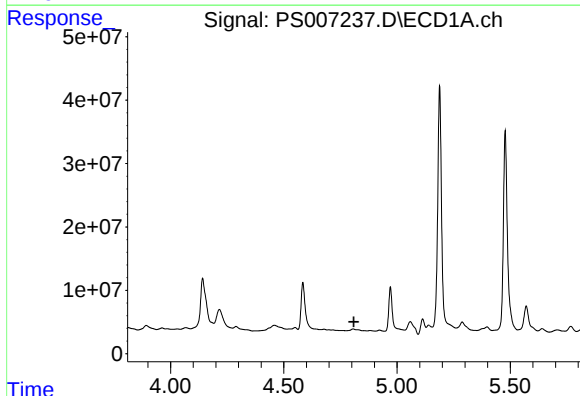


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

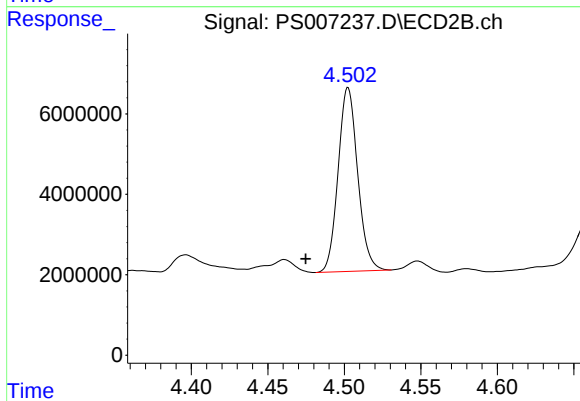

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.503 min
Delta R.T.: 0.028 min
Response: 40714431
Conc: 47.32 ng/ml

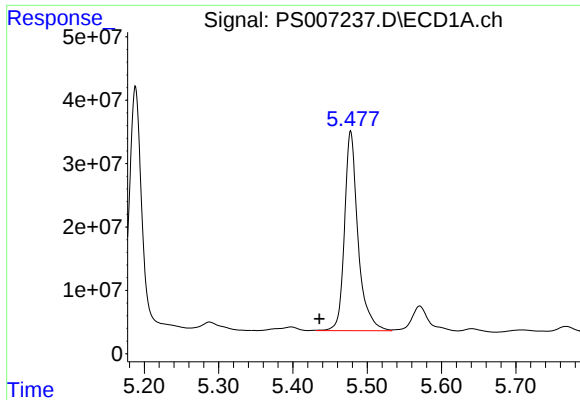

#4 2,4-DCAA


R.T.: 5.478 min
Delta R.T.: 0.042 min
Response: 397392473
Conc: 290.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

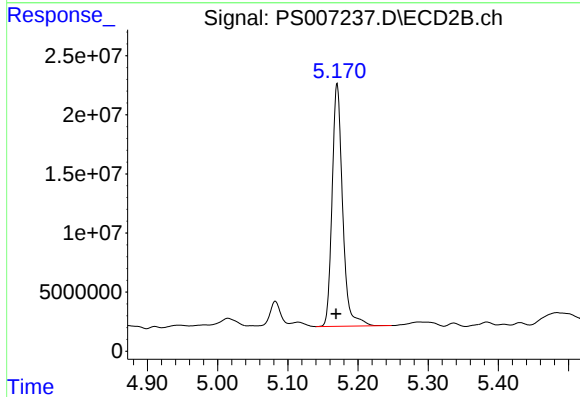


#4 2,4-DCAA

R.T.: 5.170 min
Delta R.T.: 0.002 min
Response: 213798475
Conc: 303.99 ng/ml

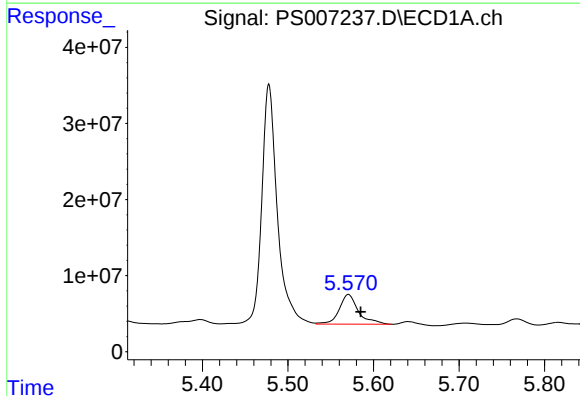


#5 DICAMBA

R.T.: 5.571 min
Delta R.T.: -0.014 min
Response: 60890318
Conc: 12.39 ng/ml

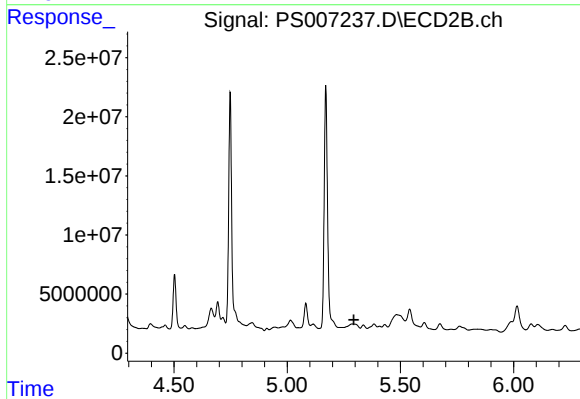

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

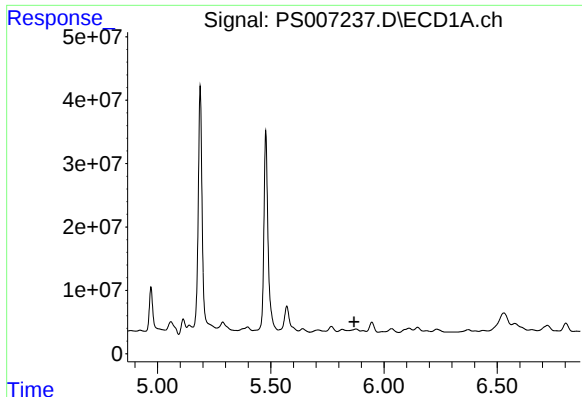

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

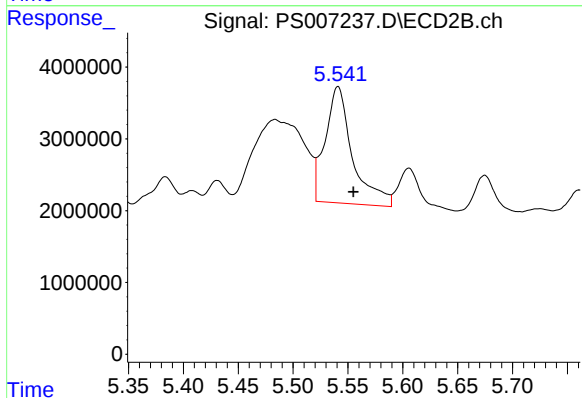


#7 MCPA

R.T.: 5.541 min
Delta R.T.: -0.014 min
Response: 28051675
Conc: 9.65 ug/ml

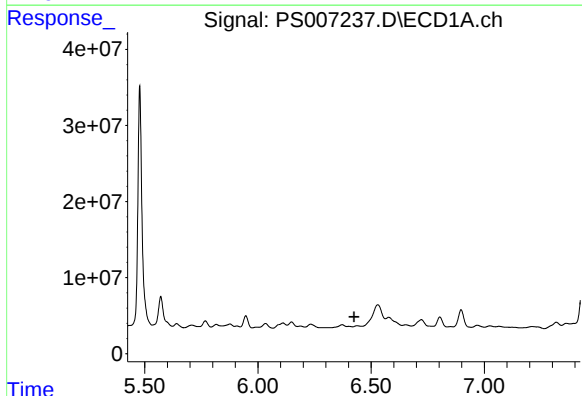


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

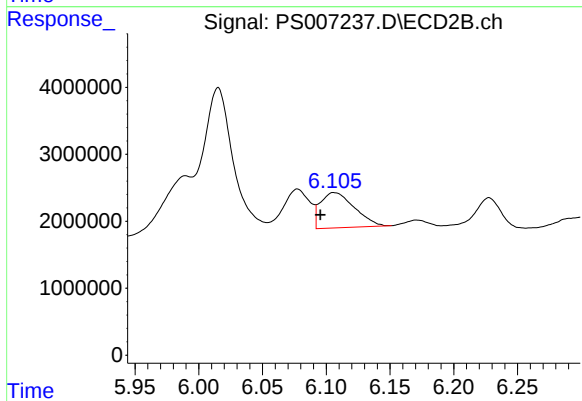

#9 2,4-D


R.T.: 6.107 min
Delta R.T.: 0.011 min
Response: 9793713
Conc: 12.28 ng/ml

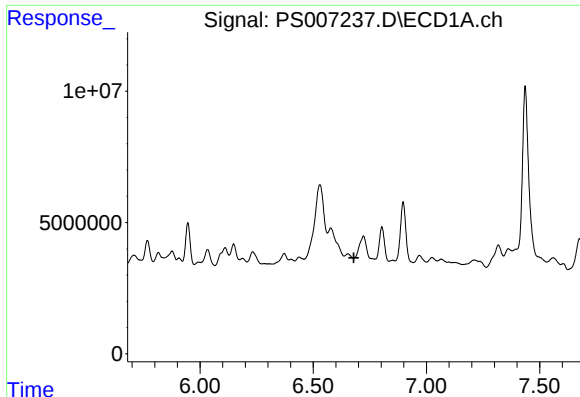

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

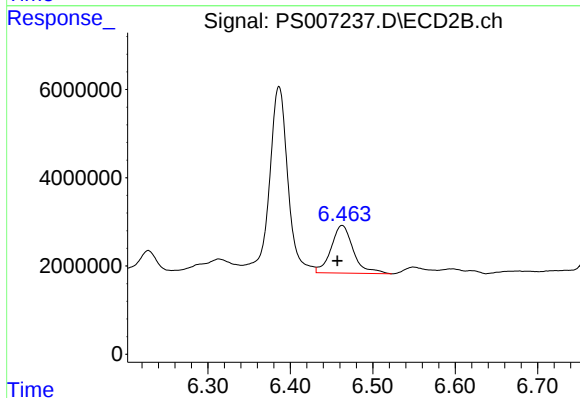


#10 Pentachlorophenol

R.T.: 6.463 min
Delta R.T.: 0.005 min
Response: 20245871
Conc: 2.11 ng/ml

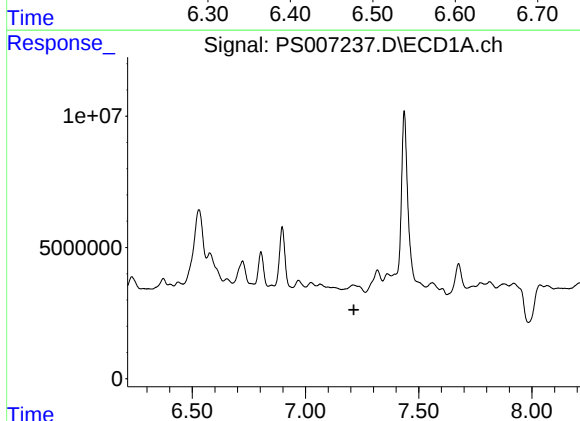


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

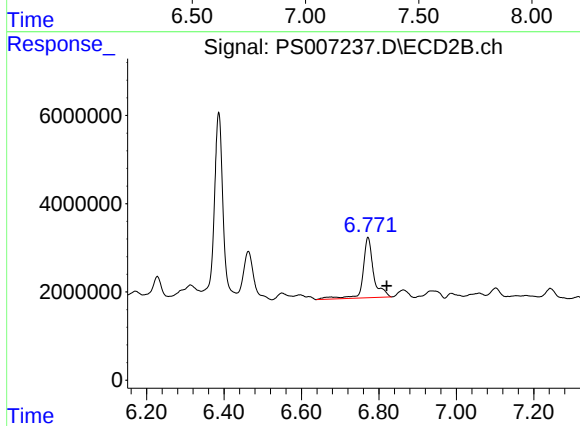

#11 2,4,5-TP (SILVEX)


R.T.: 6.772 min
Delta R.T.: -0.049 min
Response: 26158678
Conc: 6.88 ng/ml

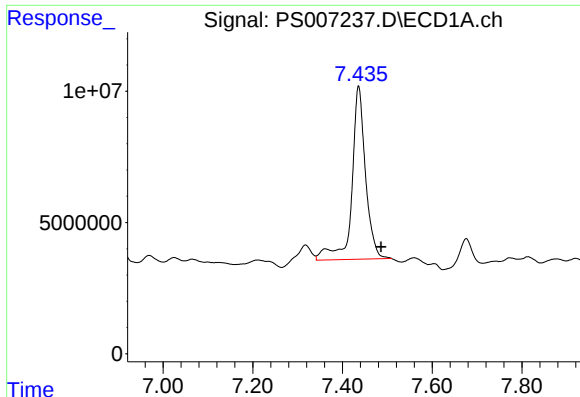

#12 2,4,5-T


R.T.: 7.436 min
Delta R.T.: -0.050 min
Response: 140580359
Conc: 18.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

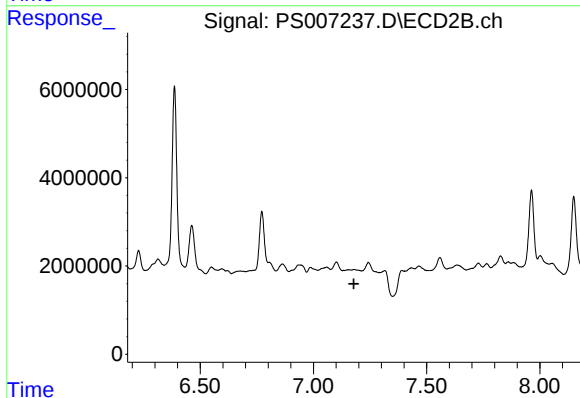


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.178 min
Response: 0
Conc: N.D.

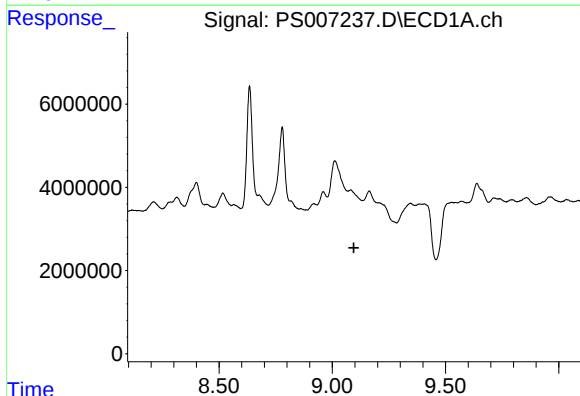


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.095 min
Response: 0
Conc: N.D.

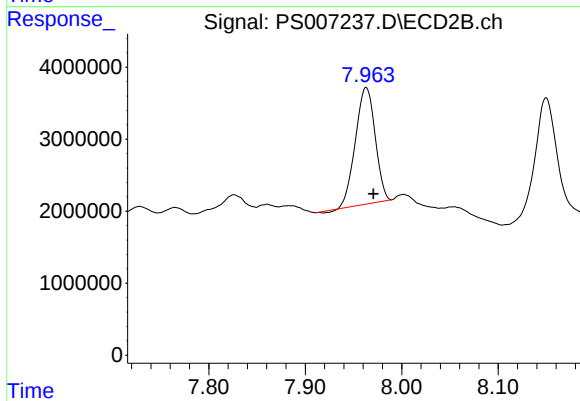

#14 DINOSEB


R.T.: 7.963 min
Delta R.T.: -0.008 min
Response: 22900088
Conc: 8.16 ng/ml

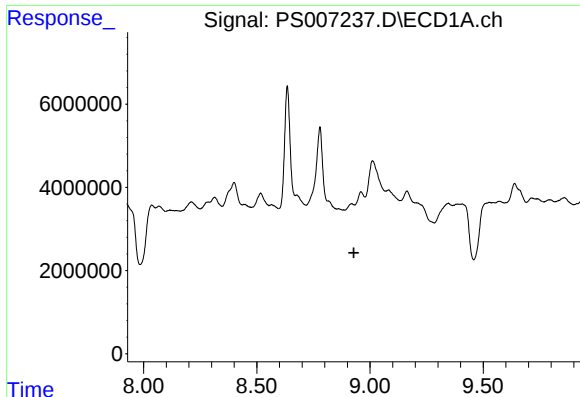

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

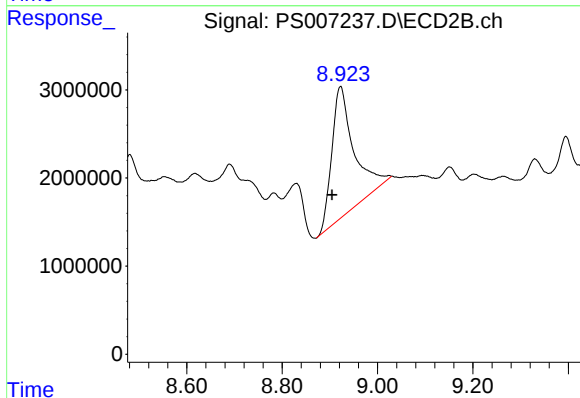


#15 Picloram

R.T.: 8.922 min
Delta R.T.: 0.018 min
Response: 47782529
Conc: 7.78 ng/ml

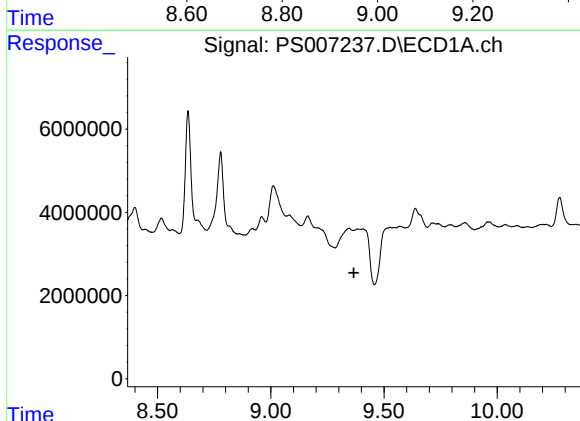

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

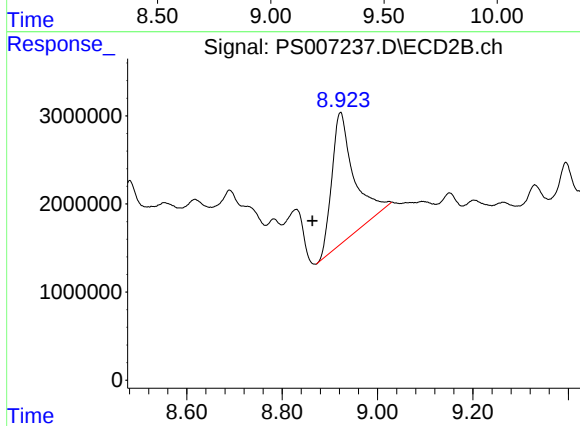

#16 DCPA

R.T.: 8.922 min
Delta R.T.: 0.059 min
Response: 47782529
Conc: 9.53 ng/ml