

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102119\
 Data File : PS007246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2019 22:03
 Operator : SM\AJ
 Sample : PB124159TB
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 05:15:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.455	5.185	466.4E6	275.0E6	340.754	391.038
Target Compounds							
1) T	Dalapon	2.011	1.723	92822457	251.5E6	55.473	276.345 #
2) T	3,5-DICHL...	0.000	4.475	0	9751572	N.D.	11.333
5) T	DICAMBA	0.000	5.315	0	5947406	N.D.	2.286
6) T	MCPD	0.000	5.315	0	5947406	N.D.	3.135
7) T	MCPA	0.000	5.499	0	54580091	N.D.	18.775
9) T	2,4-D	0.000	6.029	0	39328178	N.D.	49.296
10) T	Pentachlo...	0.000	6.477	0	9990662	N.D.	1.039
11) T	2,4,5-TP ...	0.000	6.784	0	41418740	N.D.	10.889
12) T	2,4,5-T	7.426	0.000	107.0E6	0	13.991	N.D. #
14) T	DINOSEB	0.000	8.019	0	9467132	N.D.	3.372



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102119\
Data File : PS007246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2019 22:03
Operator : SM\AJ
Sample : PB124159TB
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 05:15:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

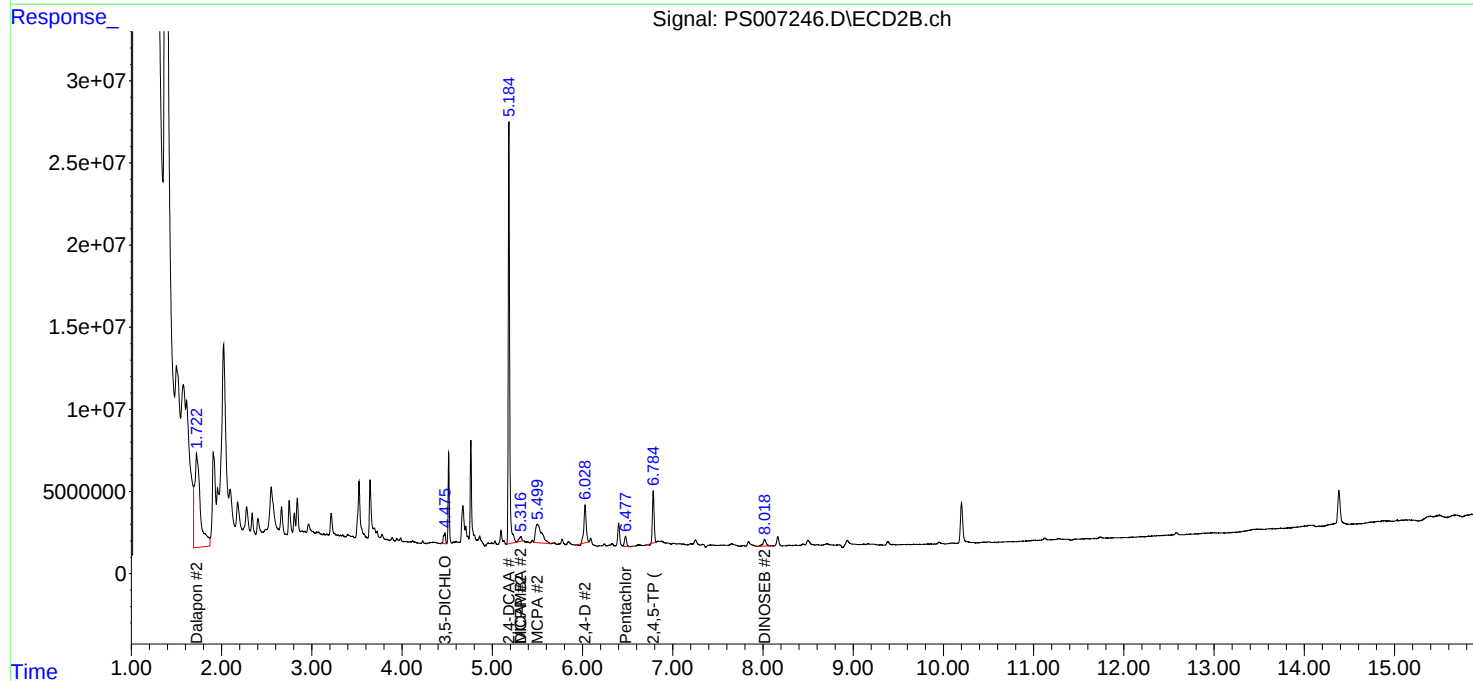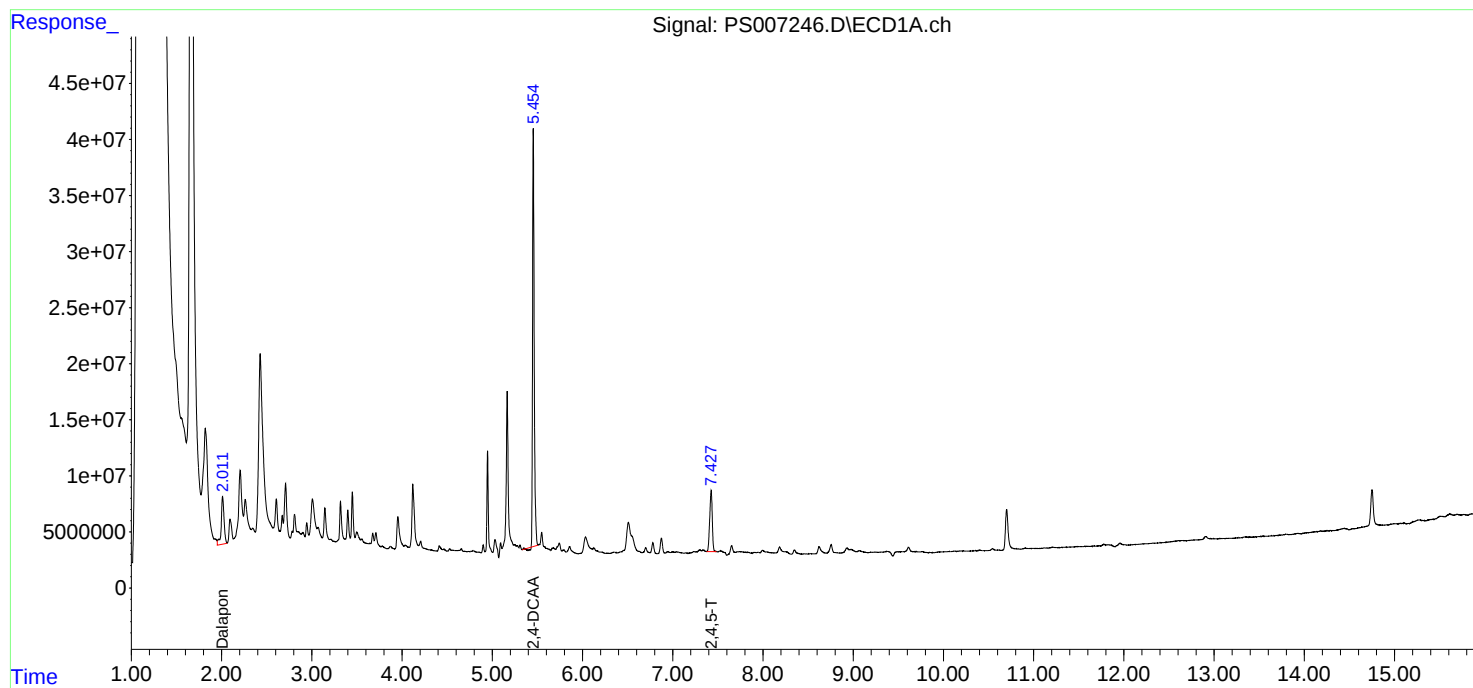


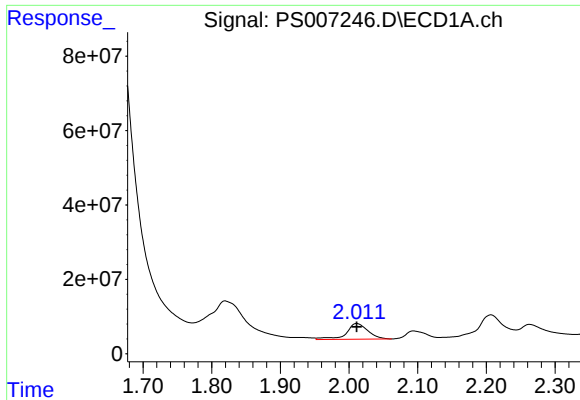

#1 Dalapon


R.T.: 2.011 min
Delta R.T.: 0.000 min
Response: 92822457
Conc: 55.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

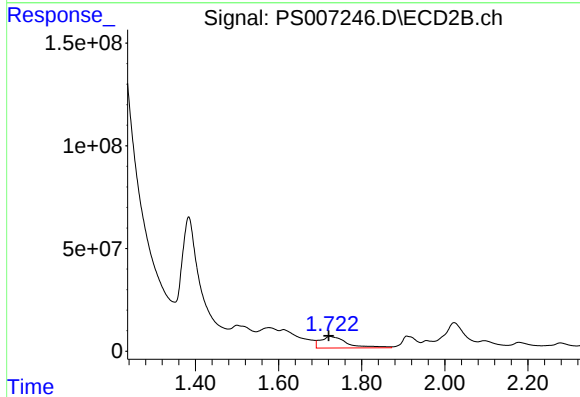


#1 Dalapon

R.T.: 1.723 min
Delta R.T.: 0.003 min
Response: 251475235
Conc: 276.35 ng/ml

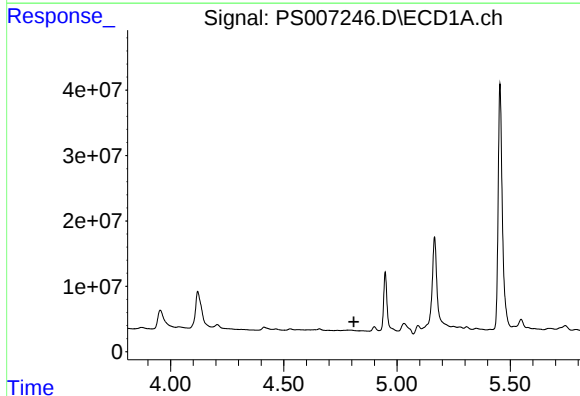


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

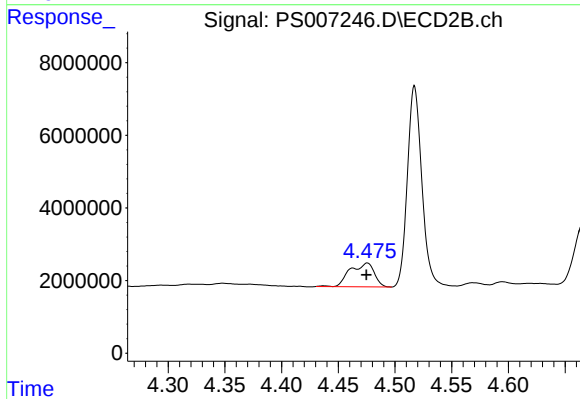

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.475 min
Delta R.T.: 0.000 min
Response: 9751572
Conc: 11.33 ng/ml

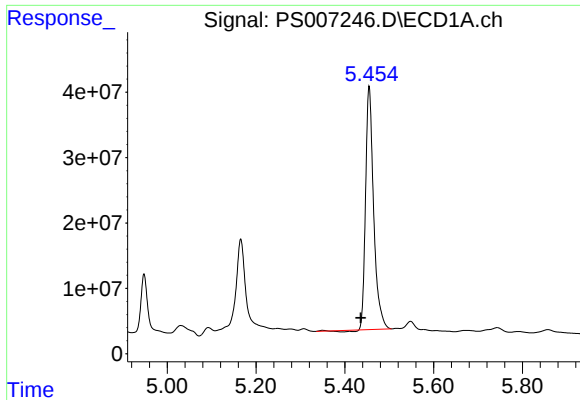

#4 2,4-DCAA


R.T.: 5.455 min
Delta R.T.: 0.019 min
Response: 466378893
Conc: 340.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

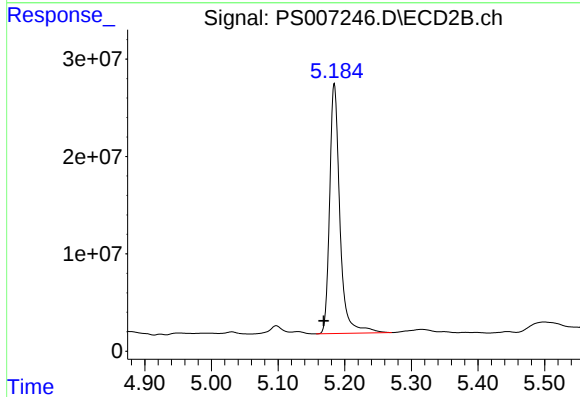


#4 2,4-DCAA

R.T.: 5.185 min
Delta R.T.: 0.016 min
Response: 275019505
Conc: 391.04 ng/ml

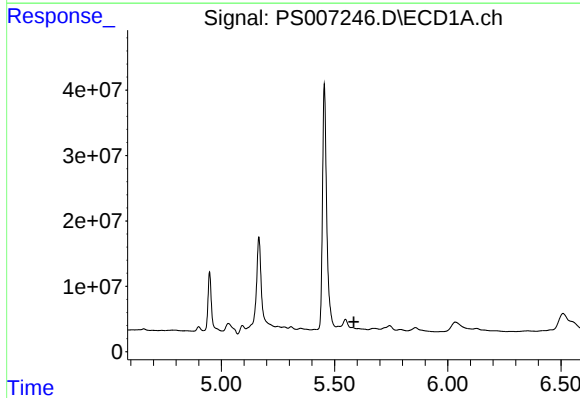


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.585 min
Response: 0
Conc: N.D.

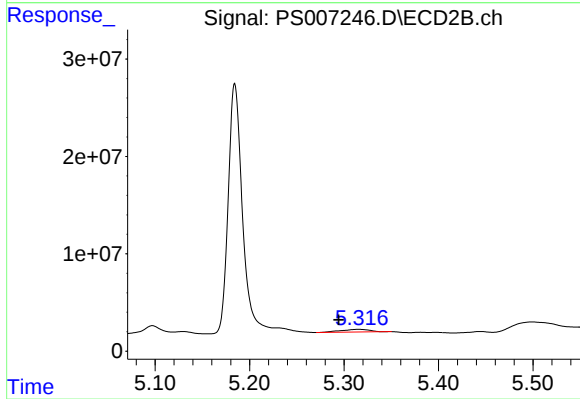

#5 DICAMBA


R.T.: 5.315 min
Delta R.T.: 0.021 min
Response: 5947406
Conc: 2.29 ng/ml

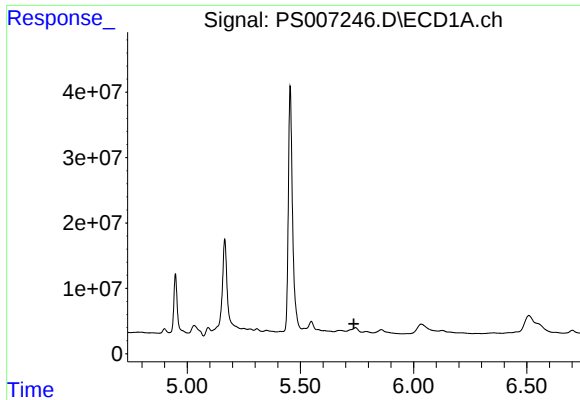

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.736 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

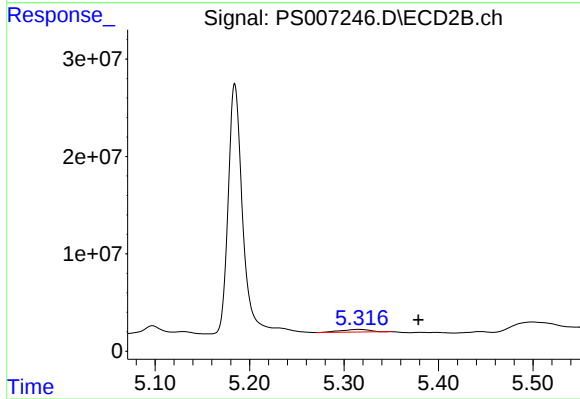


#6 MCPP

R.T.: 5.315 min
Delta R.T.: -0.063 min
Response: 5947406
Conc: 3.14 ug/ml

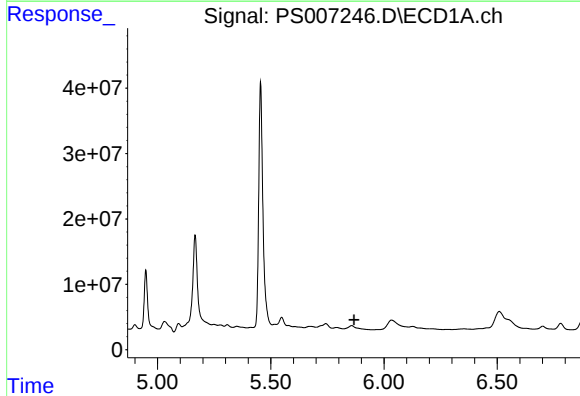


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

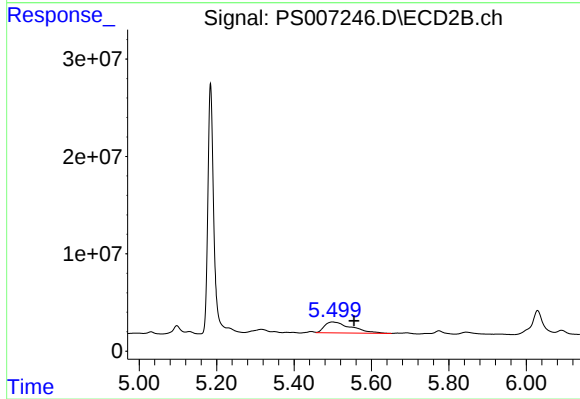

#7 MCPA


R.T.: 5.499 min
Delta R.T.: -0.056 min
Response: 54580091
Conc: 18.77 ug/ml

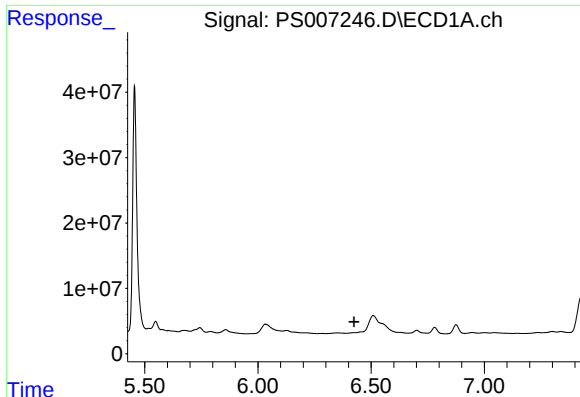

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

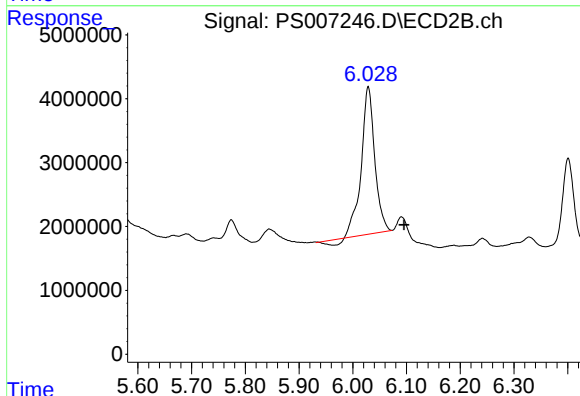


#9 2,4-D

R.T.: 6.029 min
Delta R.T.: -0.066 min
Response: 39328178
Conc: 49.30 ng/ml

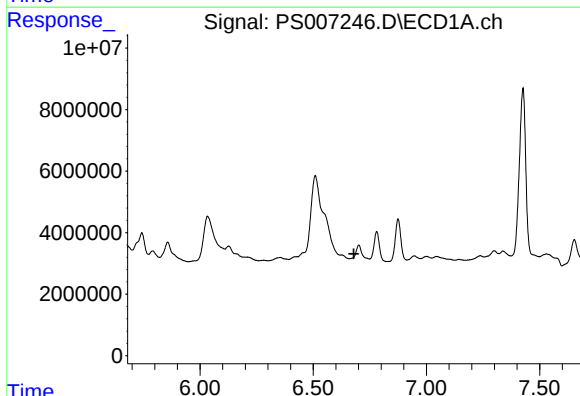


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

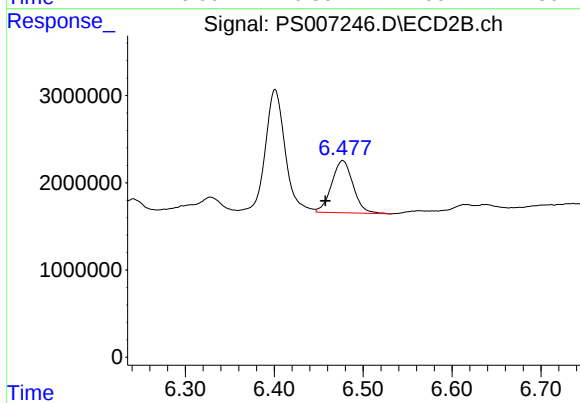

#10 Pentachlorophenol


R.T.: 6.477 min
Delta R.T.: 0.020 min
Response: 9990662
Conc: 1.04 ng/ml

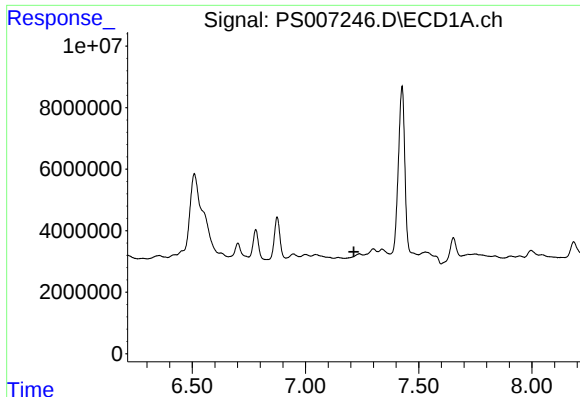

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

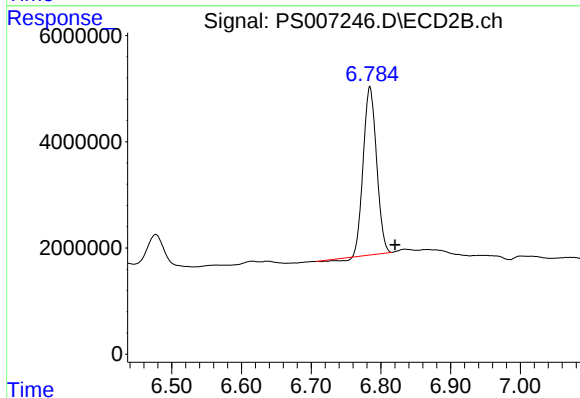


#11 2,4,5-TP (SILVEX)

R.T.: 6.784 min
Delta R.T.: -0.036 min
Response: 41418740
Conc: 10.89 ng/ml

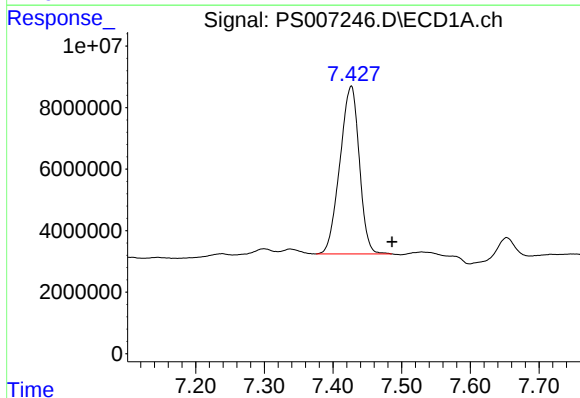


#12 2,4,5-T

R.T.: 7.426 min
Delta R.T.: -0.060 min
Response: 106956162
Conc: 13.99 ng/ml

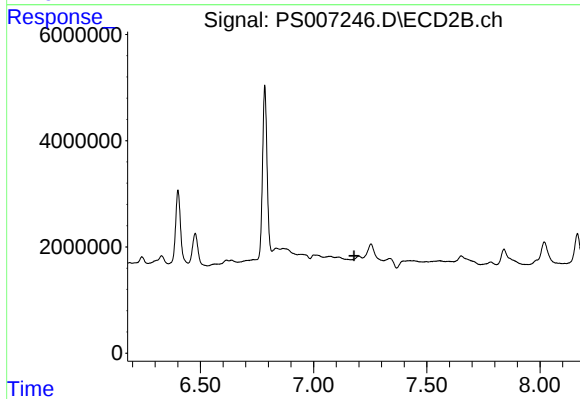

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.178 min
Response: 0
Conc: N.D.

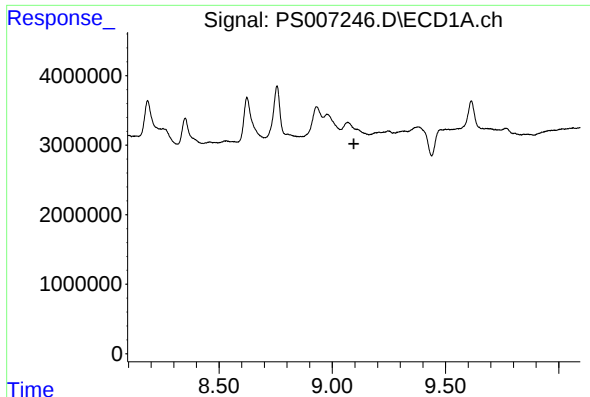

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

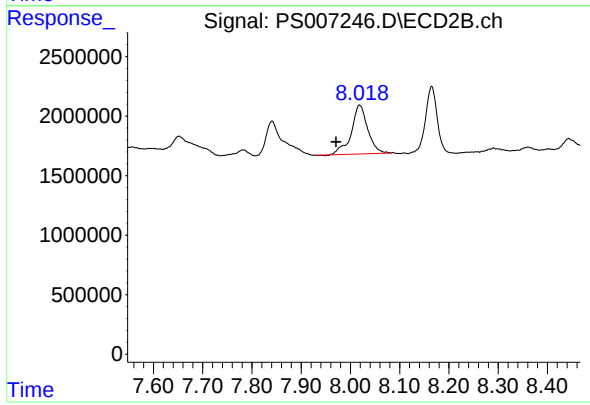

#14 DINOSEB

R.T.: 8.019 min
Delta R.T.: 0.048 min
Response: 9467132
Conc: 3.37 ng/ml