

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102119\
 Data File : PS007252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2019 00:15
 Operator : SM\AJ
 Sample : K5147-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 05:16:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.464	5.194	559.6E6	307.8E6	408.871	437.597
Target Compounds							
1) T	Dalapon	2.021	1.734	70446798	195.9E6	42.101	215.278 #
2) T	3,5-DICHL...	0.000	4.473	0	14789755	N.D.	17.189
5) T	DICAMBA	5.557	5.242	39475711	10516937	8.034	4.042 #
7) T	MCPA	0.000	5.510	0	52690789	N.D.	18.125
9) T	2,4-D	0.000	6.101	0	8336509	N.D.	10.449
10) T	Pentachlo...	0.000	6.486	0	15559381	N.D.	1.618
11) T	2,4,5-TP ...	0.000	6.837	0	36853071	N.D.	9.689
12) T	2,4,5-T	7.434	0.000	163.6E6	0	21.406	N.D. #
15) T	Picloram	0.000	8.945	0	6971973	N.D.	1.135



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102119\
Data File : PS007252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2019 00:15
Operator : SM\AJ
Sample : K5147-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 05:16:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

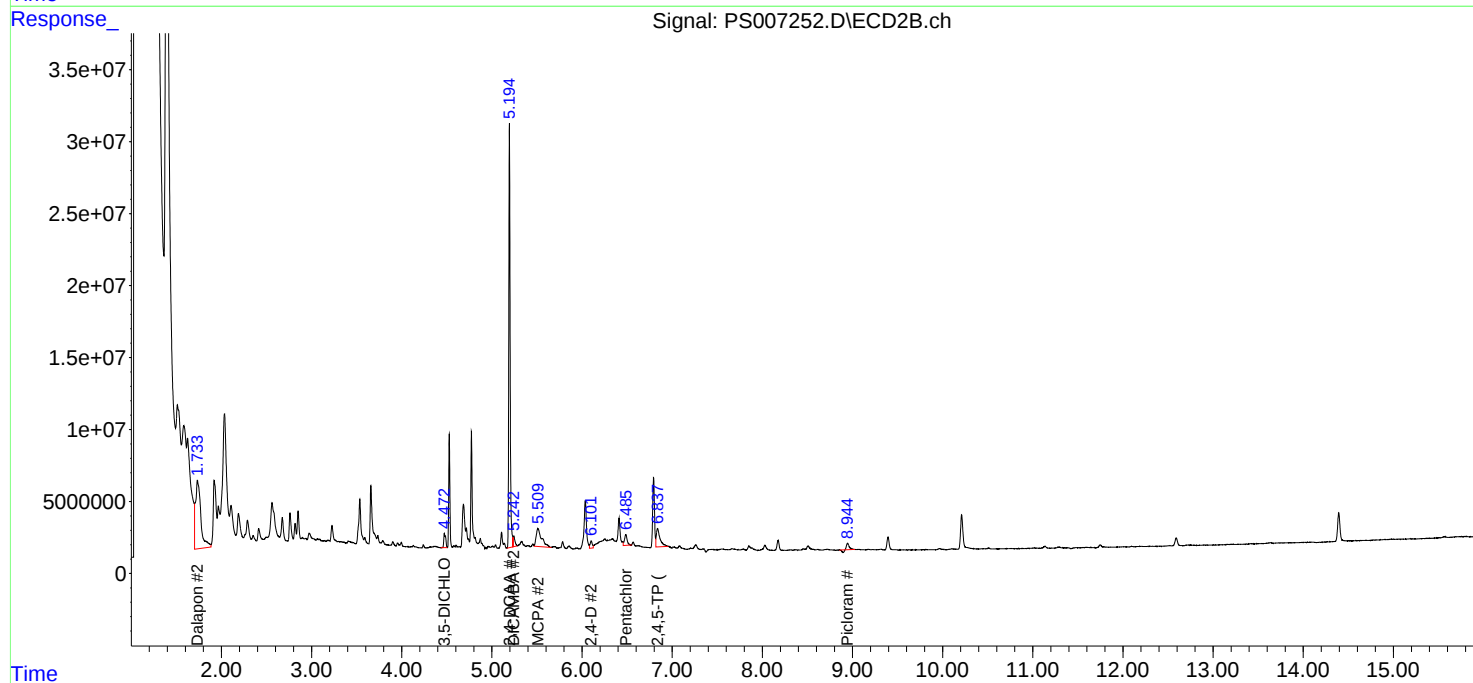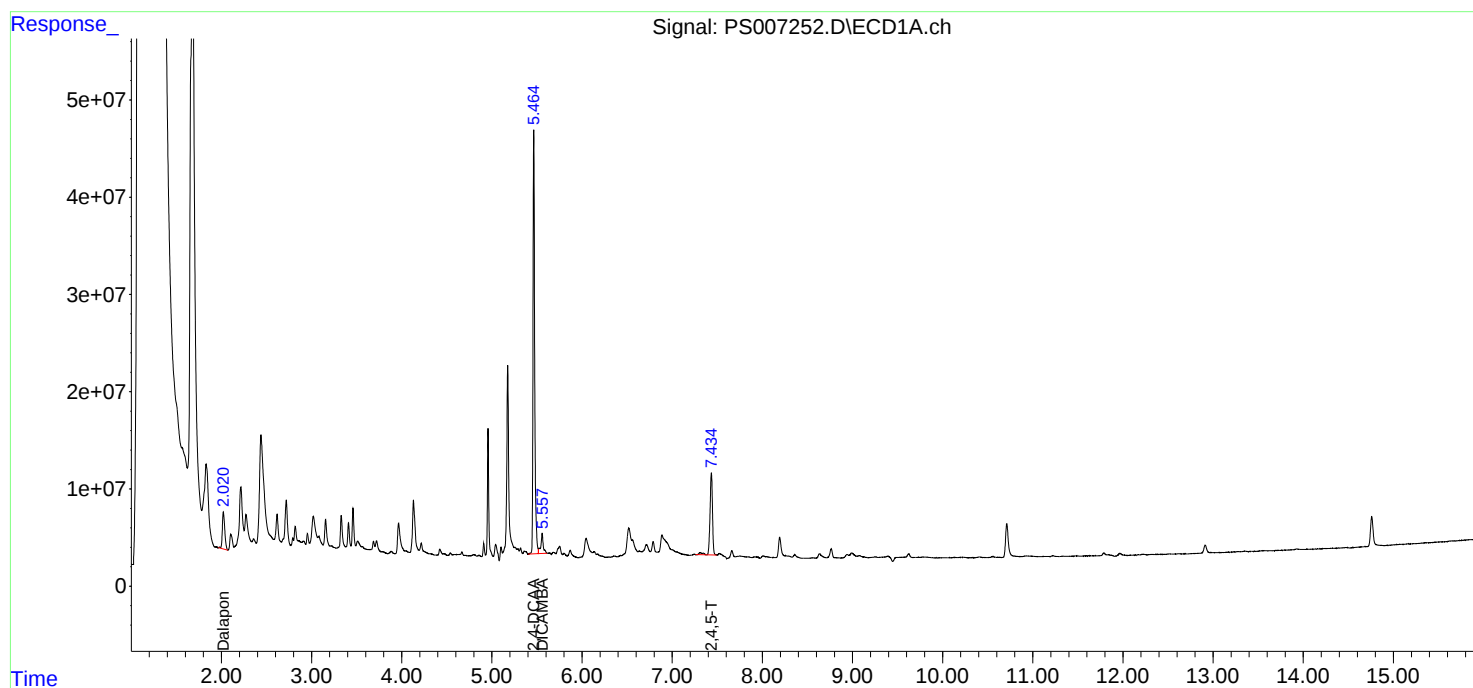


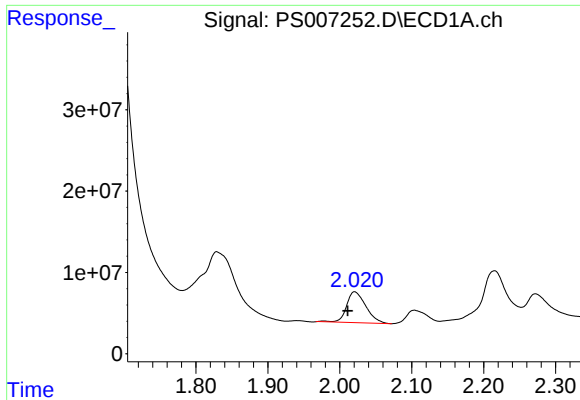

#1 Dalapon


R.T.: 2.021 min
Delta R.T.: 0.010 min
Response: 70446798
Conc: 42.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

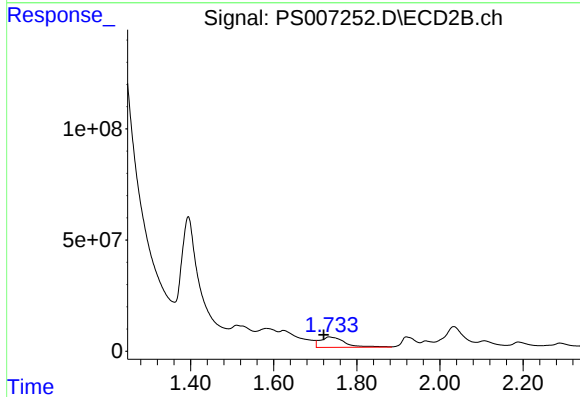


#1 Dalapon

R.T.: 1.734 min
Delta R.T.: 0.013 min
Response: 195903330
Conc: 215.28 ng/ml

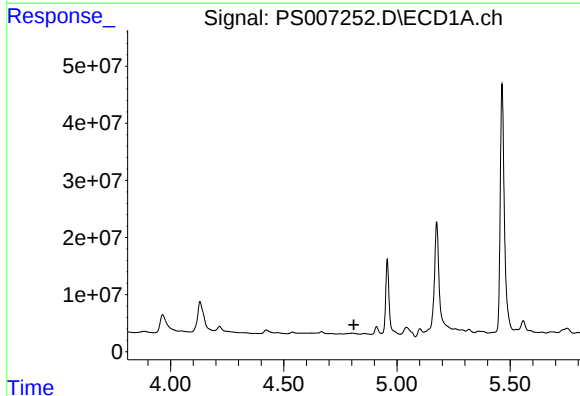


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

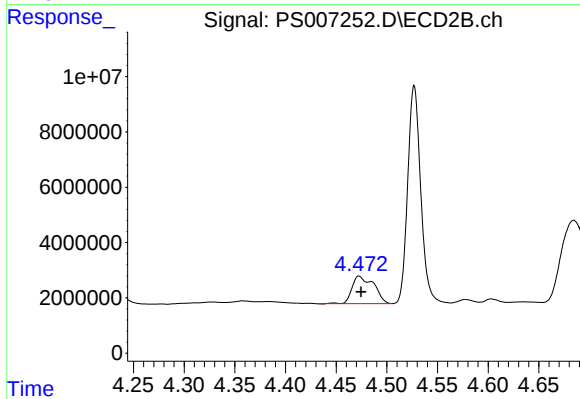

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.473 min
Delta R.T.: -0.002 min
Response: 14789755
Conc: 17.19 ng/ml

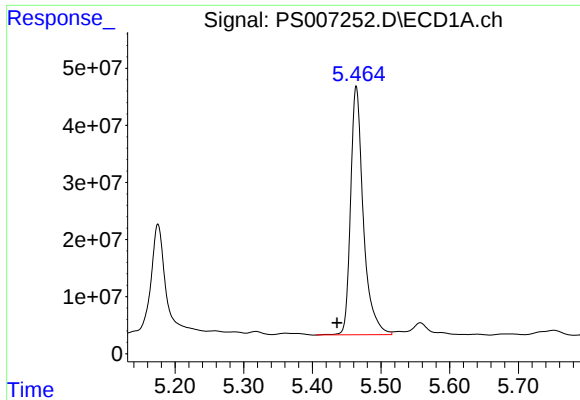

#4 2,4-DCAA


R.T.: 5.464 min
Delta R.T.: 0.028 min
Response: 559609125
Conc: 408.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

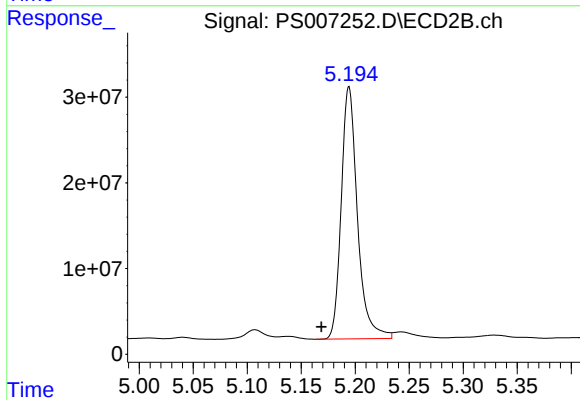


#4 2,4-DCAA

R.T.: 5.194 min
Delta R.T.: 0.026 min
Response: 307764618
Conc: 437.60 ng/ml

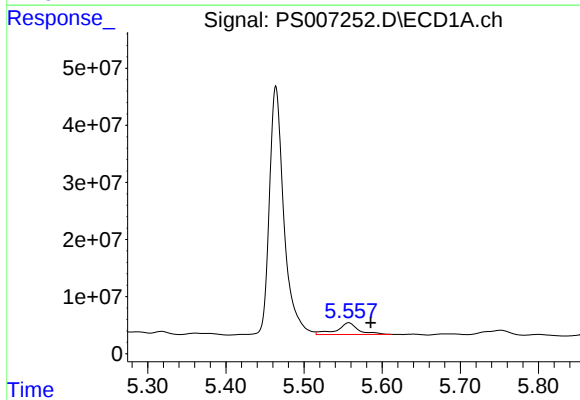


#5 DICAMBA

R.T.: 5.557 min
Delta R.T.: -0.028 min
Response: 39475711
Conc: 8.03 ng/ml

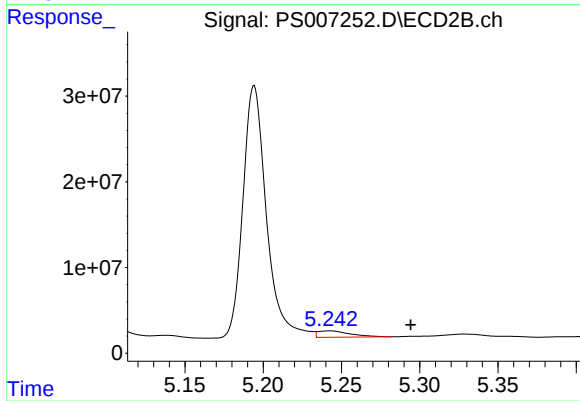

#5 DICAMBA


R.T.: 5.242 min
Delta R.T.: -0.052 min
Response: 10516937
Conc: 4.04 ng/ml

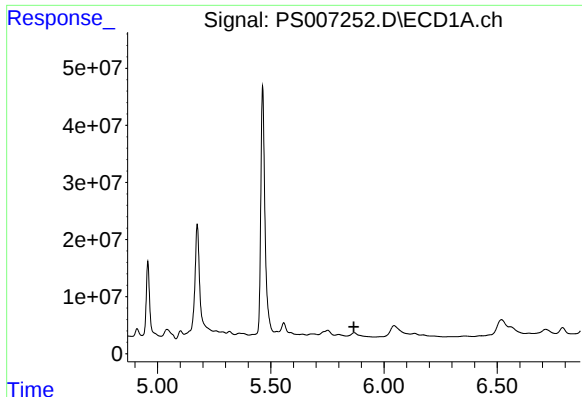

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

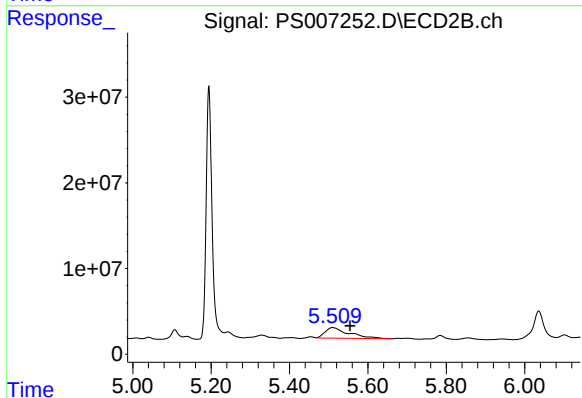


#7 MCPA

R.T.: 5.510 min
Delta R.T.: -0.045 min
Response: 52690789
Conc: 18.12 ug/ml

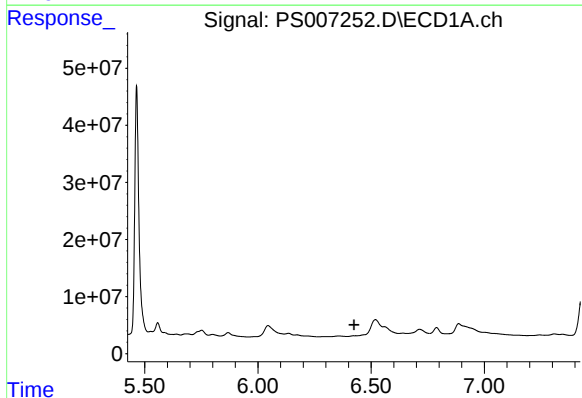


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

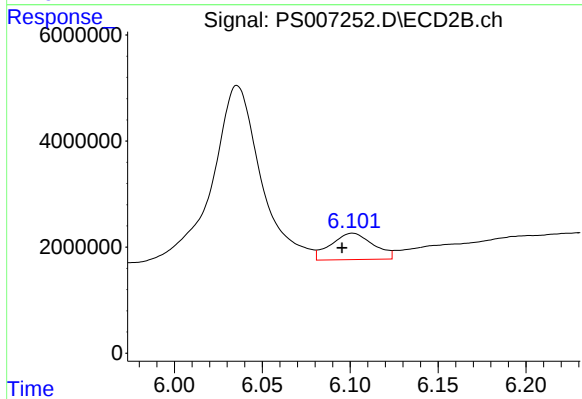

#9 2,4-D


R.T.: 6.101 min
Delta R.T.: 0.006 min
Response: 8336509
Conc: 10.45 ng/ml

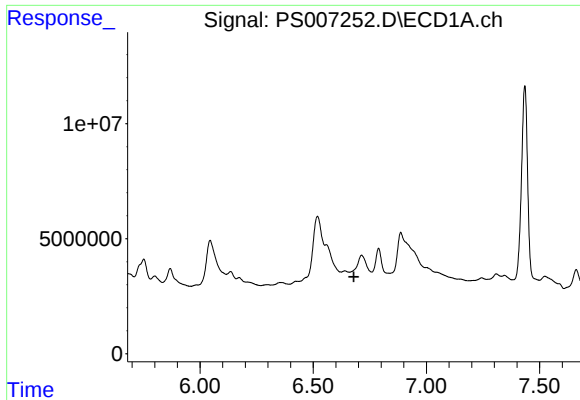

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

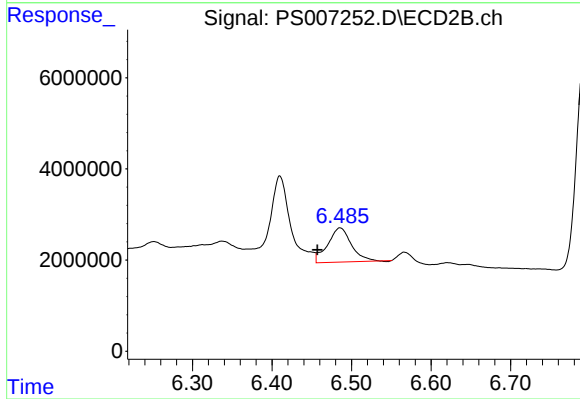


#10 Pentachlorophenol

R.T.: 6.486 min
Delta R.T.: 0.028 min
Response: 15559381
Conc: 1.62 ng/ml

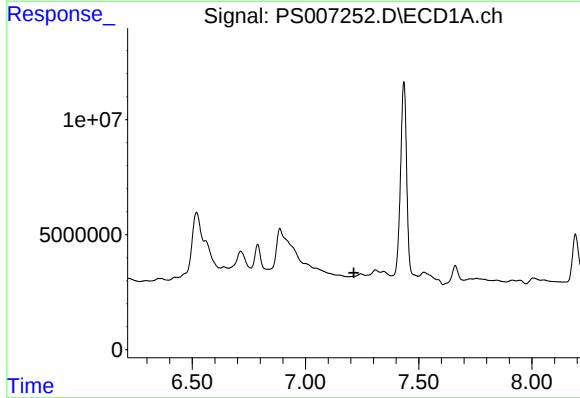


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

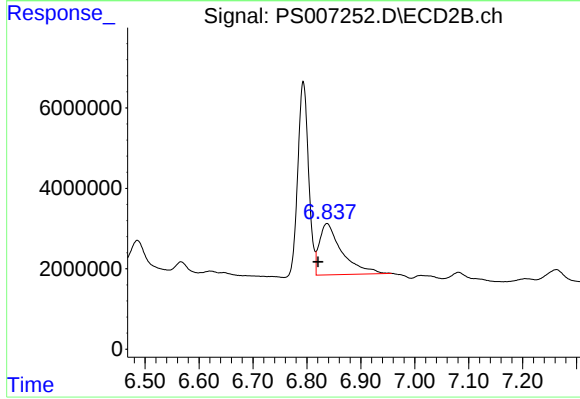

#11 2,4,5-TP (SILVEX)


R.T.: 6.837 min
Delta R.T.: 0.017 min
Response: 36853071
Conc: 9.69 ng/ml

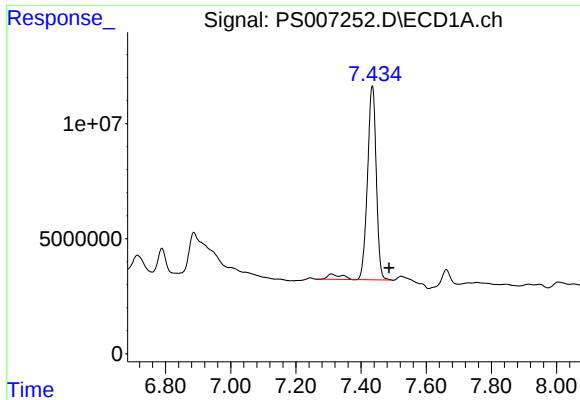

#12 2,4,5-T


R.T.: 7.434 min
Delta R.T.: -0.051 min
Response: 163639898
Conc: 21.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

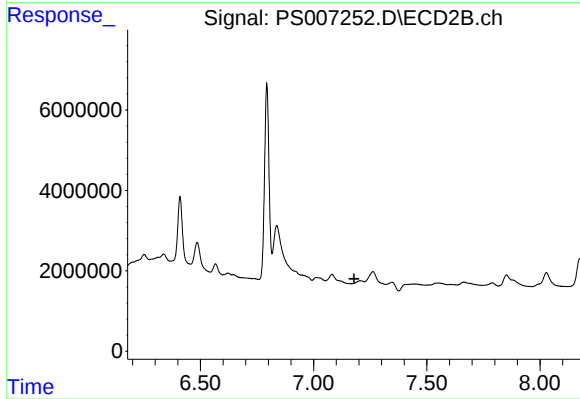


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.178 min
Response: 0
Conc: N.D.

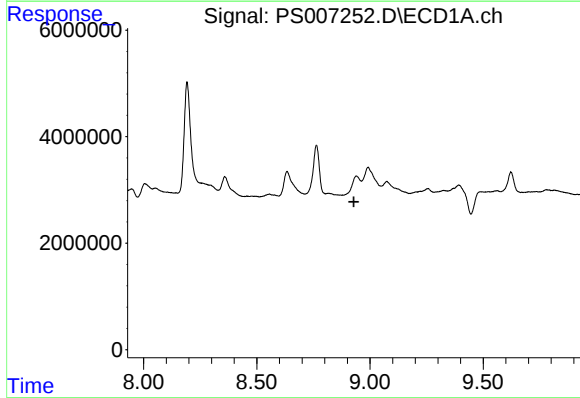

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

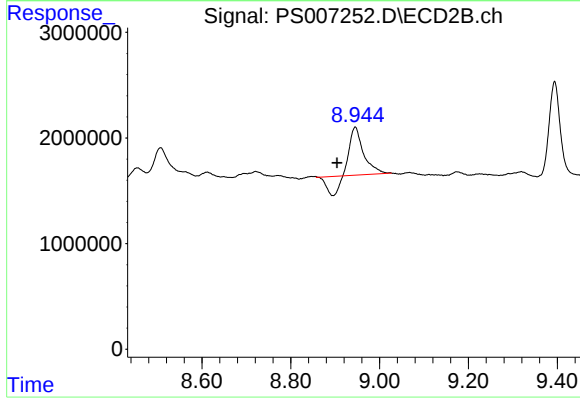

#15 Picloram

R.T.: 8.945 min
Delta R.T.: 0.040 min
Response: 6971973
Conc: 1.14 ng/ml