

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102121\
 Data File : PS017156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2021 09:10
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 16:15:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 19 01:21:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.158	0.000	16768685	0	10.971	N.D.	#
Target Compounds								
3) T	4-Nitroph...	6.944	0.000	3471720	0	3.981	N.D.	#
5) T	DICAMBA	7.345	0.000	6641236	0	1.109	N.D.	#
7) T	MCPA	7.688	0.000	578383	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.038	0.000	2696831	0	1.799	N.D.	#
9) T	2,4-D	8.274	0.000	4046294	0	2.284	N.D.	#
10) T	Pentachlo...	8.570	8.225	15754181	6416969	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.122	0.000	12420040	0	1.527	N.D.	#
12) T	2,4,5-T	9.411	8.968	22185513	7871128	2.762	2.483	
13) T	2,4-DB	9.962	0.000	4995836	0	3.321	N.D.	#
14) T	DINOSEB	11.107	0.000	14509675	0	2.561	N.D.	#
15) T	Picloram	10.937	10.777	242.1E6	72490215	22.664	18.928	
16) T	DCPA	11.376	10.723	20291654	7799495	1.992	1.828	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102121\
Data File : PS017156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2021 09:10
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 16:15:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
Quant Title : 8080.M
QLast Update : Tue Oct 19 01:21:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

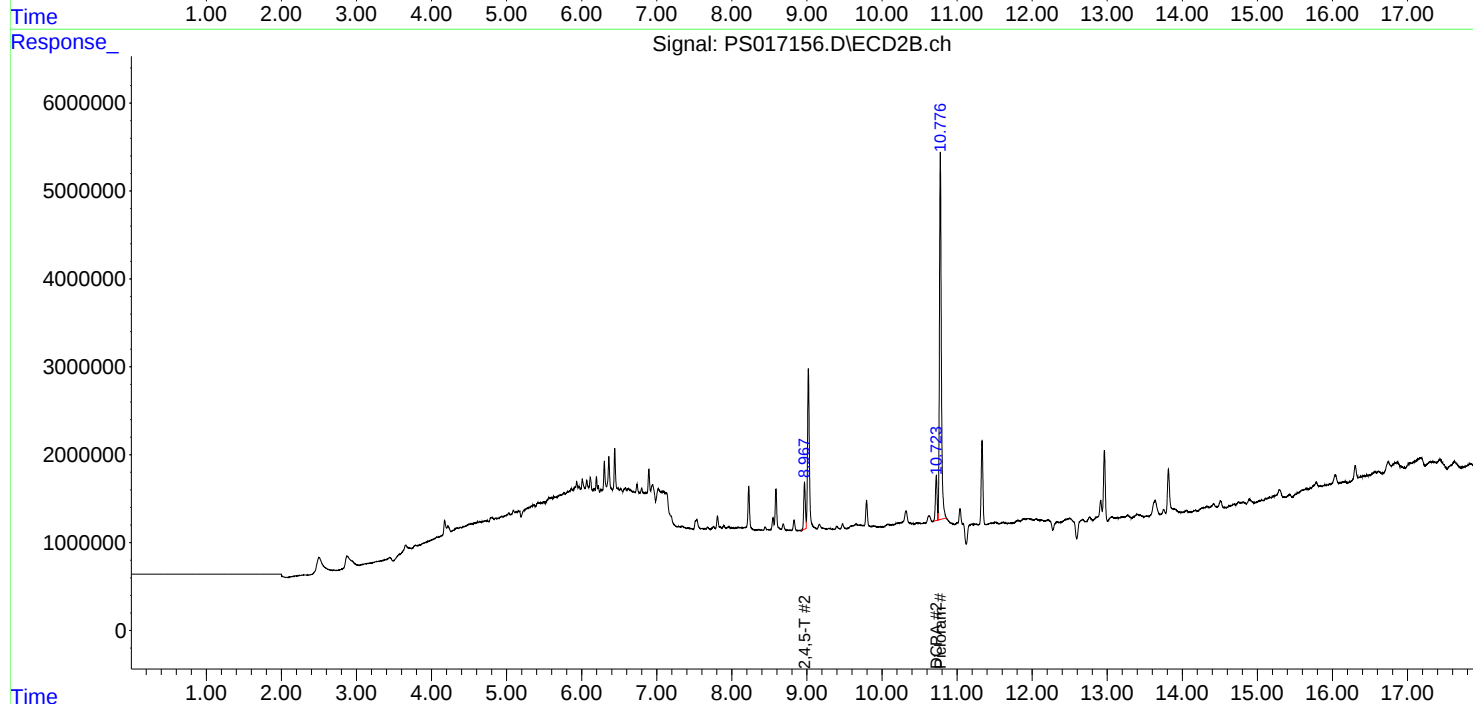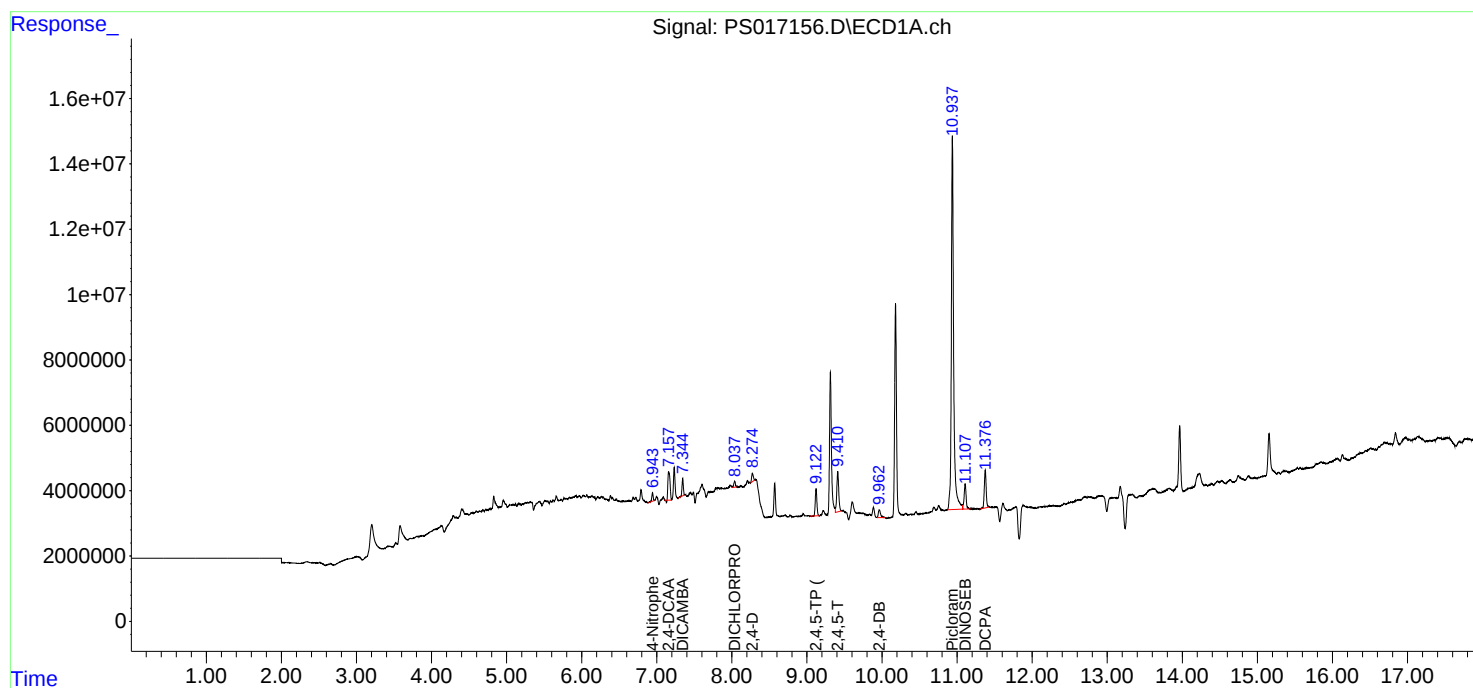


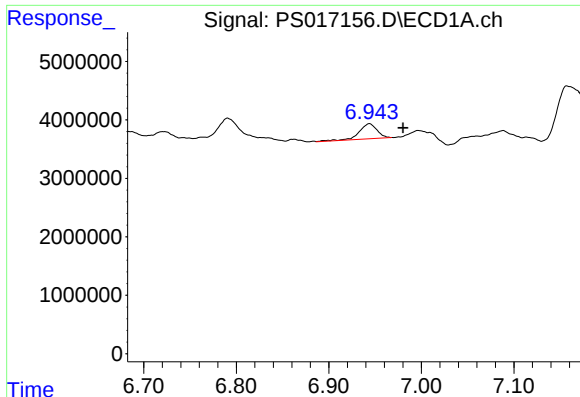

#3 4-Nitrophenol


R.T.: 6.944 min
Delta R.T.: -0.036 min
Response: 3471720
Conc: 3.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

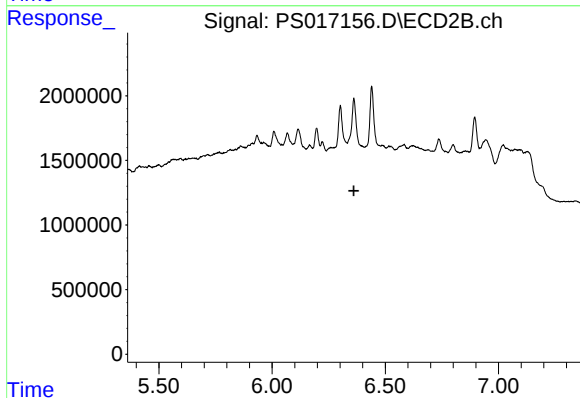


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.361 min
Response: 0
Conc: N.D.

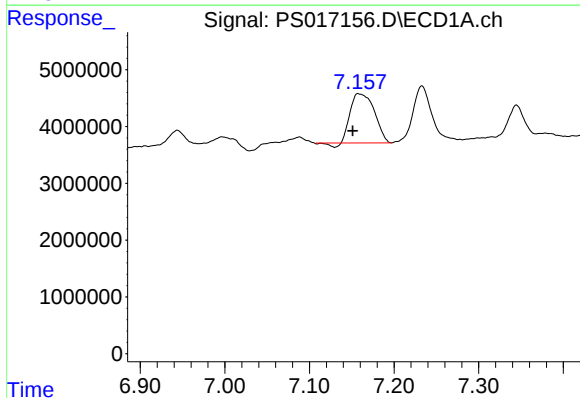


#4 2,4-DCAA

R.T.: 7.158 min
Delta R.T.: 0.007 min
Response: 16768685
Conc: 10.97 ng/ml

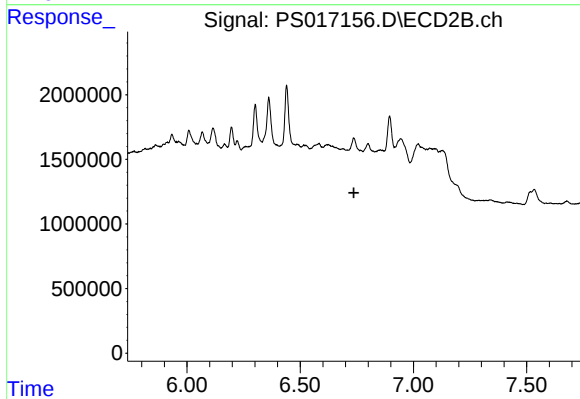

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.737 min
Response: 0
Conc: N.D.

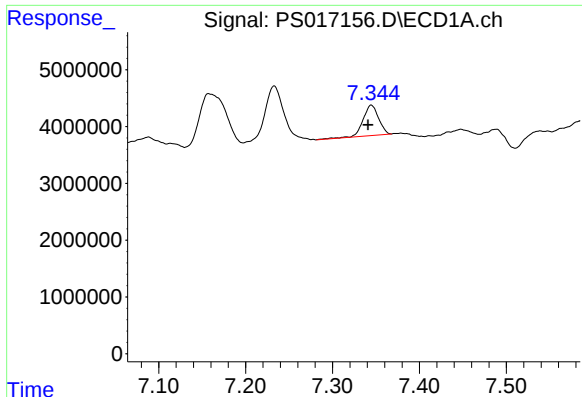

#5 DICAMBA


R.T.: 7.345 min
Delta R.T.: 0.004 min
Response: 6641236
Conc: 1.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

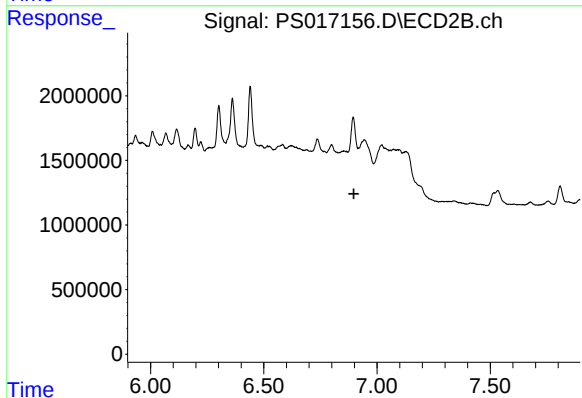


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.898 min
Response: 0
Conc: N.D.

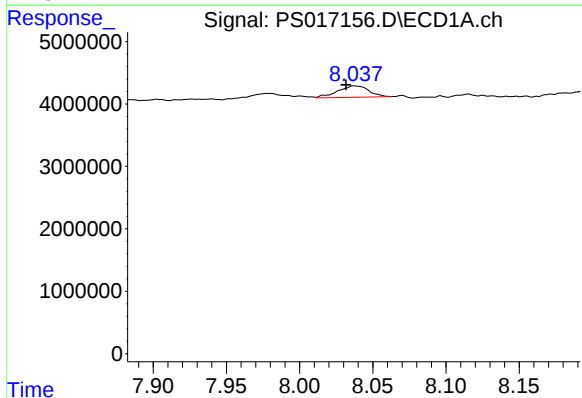


#8 DICHLORPROP

R.T.: 8.038 min
Delta R.T.: 0.006 min
Response: 2696831
Conc: 1.80 ng/ml

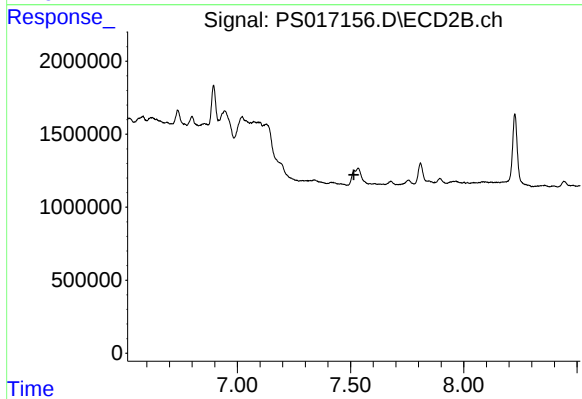

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

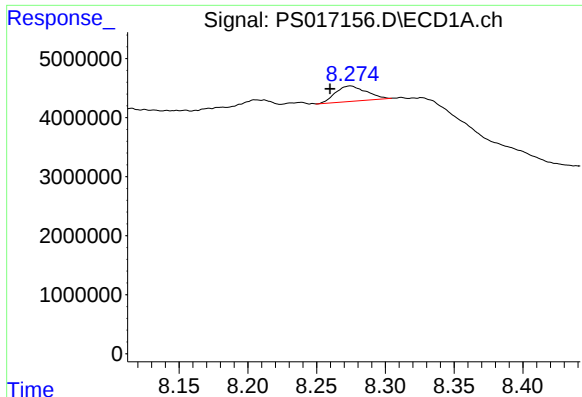

#9 2,4-D


R.T.: 8.274 min
Delta R.T.: 0.015 min
Response: 4046294
Conc: 2.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

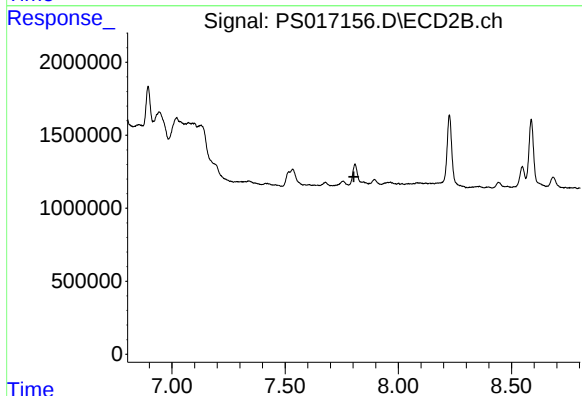


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.804 min
Response: 0
Conc: N.D.

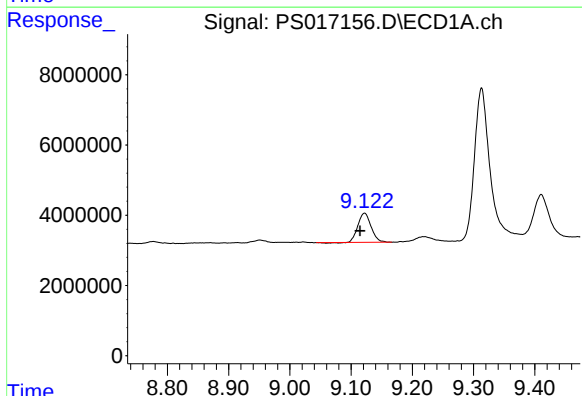


#11 2,4,5-TP (SILVEX)

R.T.: 9.122 min
Delta R.T.: 0.008 min
Response: 12420040
Conc: 1.53 ng/ml

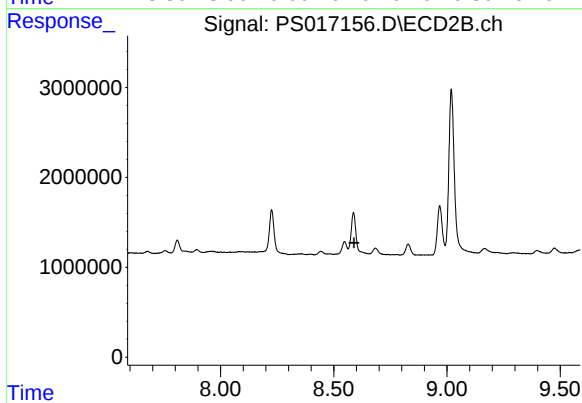

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 8.589 min
Response: 0
Conc: N.D.

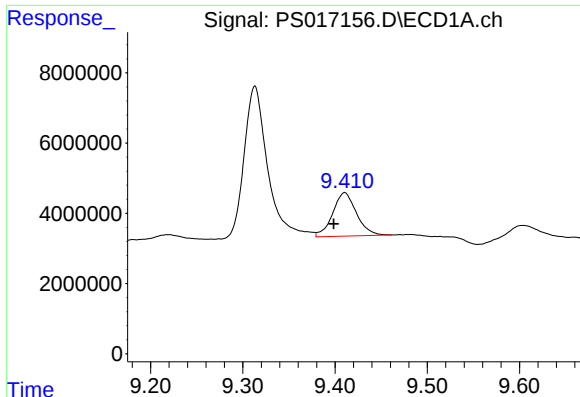

#12 2,4,5-T


R.T.: 9.411 min
Delta R.T.: 0.012 min
Response: 22185513
Conc: 2.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

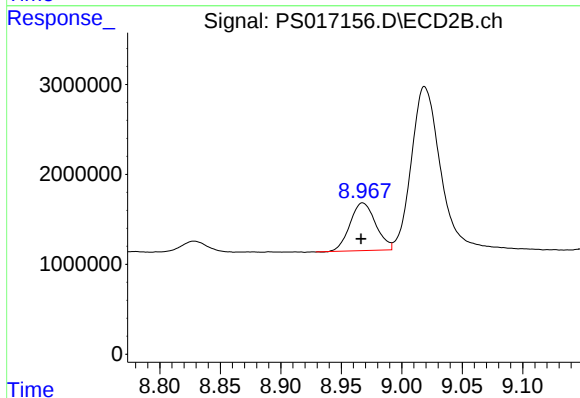


#12 2,4,5-T

R.T.: 8.968 min
Delta R.T.: 0.001 min
Response: 7871128
Conc: 2.48 ng/ml

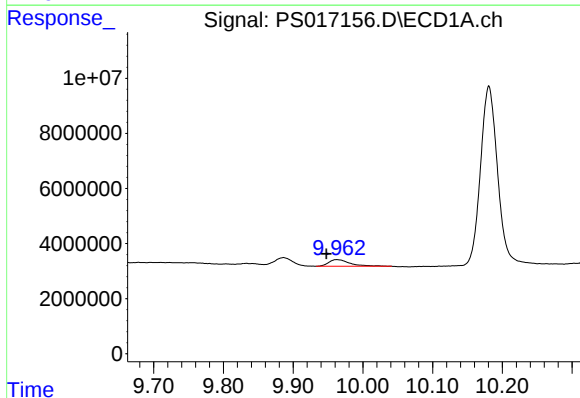


#13 2,4-DB

R.T.: 9.962 min
Delta R.T.: 0.015 min
Response: 4995836
Conc: 3.32 ng/ml

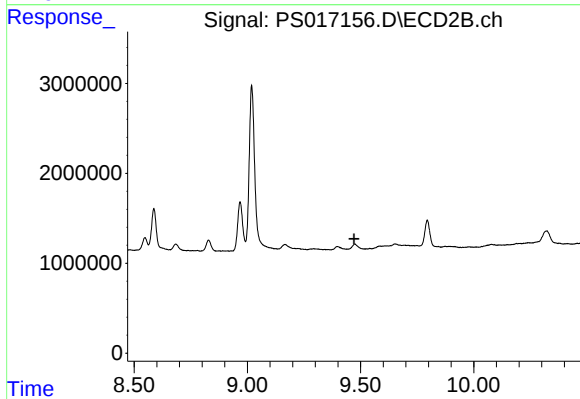

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.471 min
Response: 0
Conc: N.D.

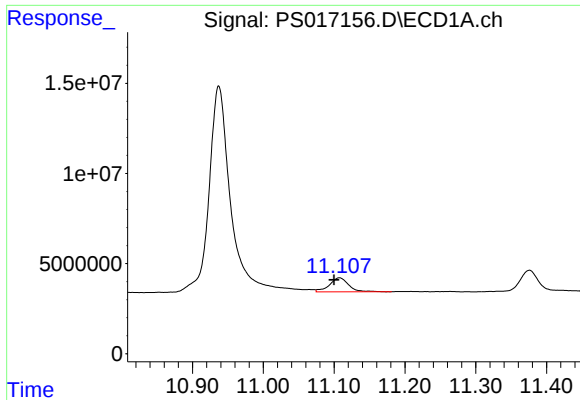

#14 DINOSEB


R.T.: 11.107 min
Delta R.T.: 0.008 min
Response: 14509675
Conc: 2.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

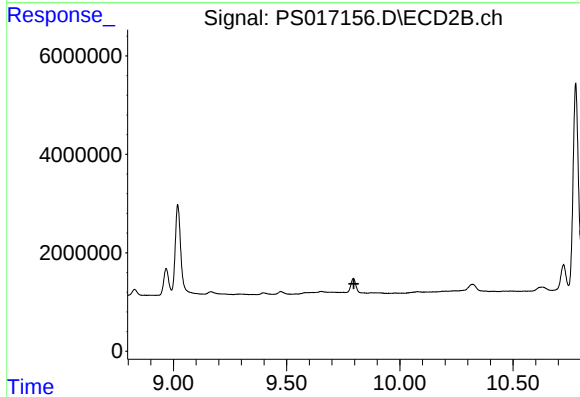


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.797 min
Response: 0
Conc: N.D.

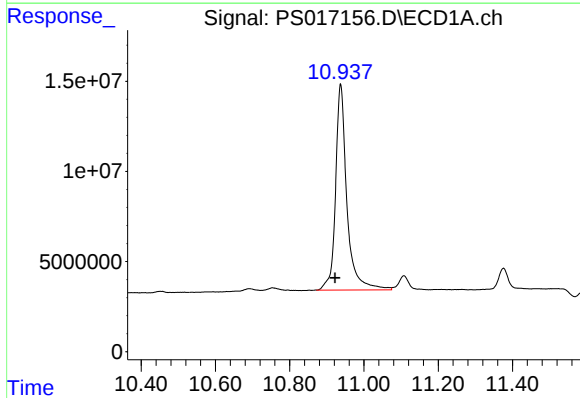


#15 Picloram

R.T.: 10.937 min
Delta R.T.: 0.015 min
Response: 242081284
Conc: 22.66 ng/ml

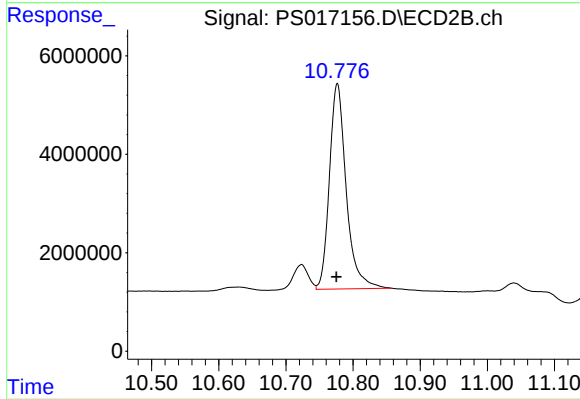

#15 Picloram


R.T.: 10.777 min
Delta R.T.: 0.002 min
Response: 72490215
Conc: 18.93 ng/ml

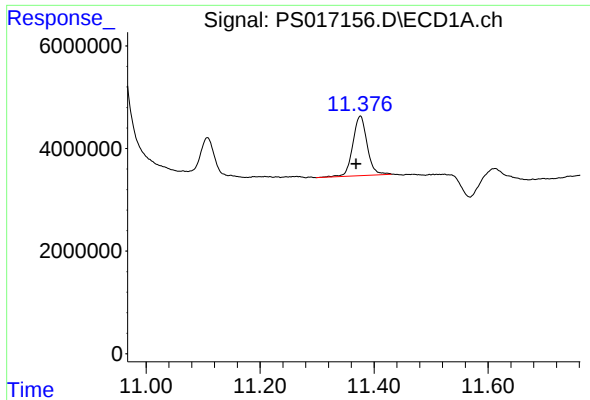

#16 DCPA

R.T.: 11.376 min
Delta R.T.: 0.007 min
Response: 20291654
Conc: 1.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

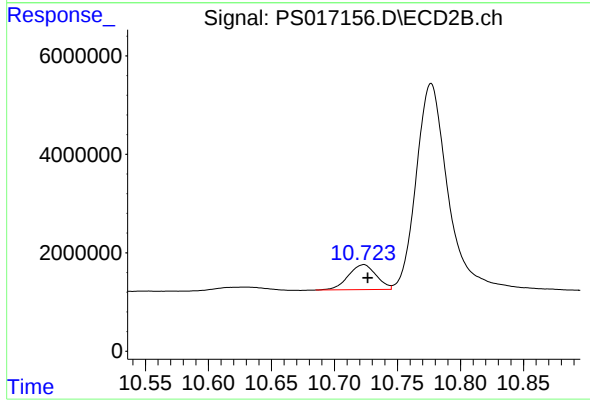

#16 DCPA

R.T.: 10.723 min
Delta R.T.: -0.003 min
Response: 7799495
Conc: 1.83 ng/ml