

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102125\
 Data File : PS032101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2025 12:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 14:23:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.291	7.759	1838.3E6	507.1E6	385.632	460.893
Target Compounds							
2) T	3,5-DICHL...	6.451	0.000	498991	0	<MDL	N.D. #
3) T	4-Nitroph...	7.072	0.000	3347923	0	2.508	N.D. #
7) T	MCPA	0.000	8.247f	0	25738934	N.D.	6.823
8) T	DICHLORPROP	8.180	0.000	1425327	0	<MDL	N.D. #
10) T	Pentachlo...	8.723	0.000	5394876	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.283	0.000	3664824	0	<MDL	N.D. #
12) T	2,4,5-T	9.595	0.000	1170269	0	<MDL	N.D. #
13) T	2,4-DB	10.152	0.000	393221	0	<MDL	N.D. #
14) T	DINOSEB	11.358	0.000	1725698	0	<MDL	N.D. #
15) T	Picloram	11.184	12.378	667055	1032444	<MDL	<MDL #
16) T	DCPA	11.657	12.334f	4341190	4537515	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102125\
Data File : PS032101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2025 12:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 14:23:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

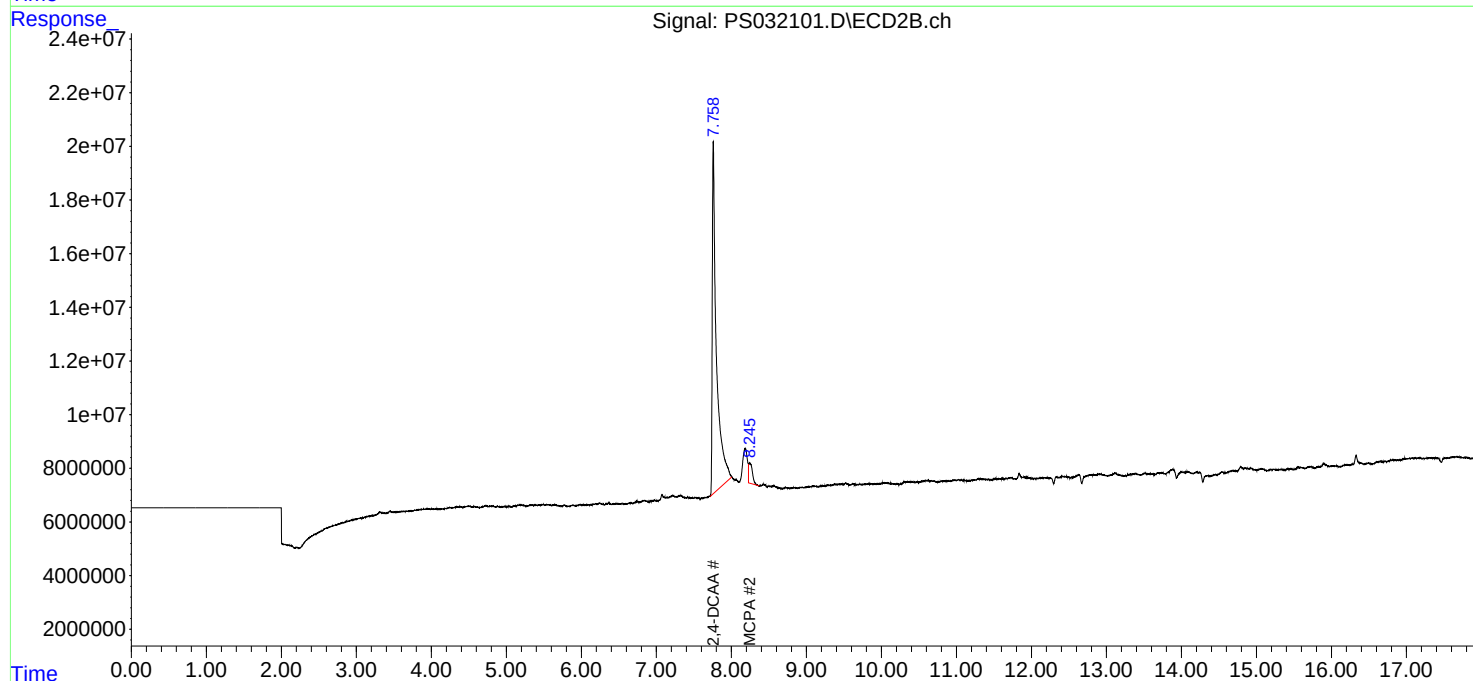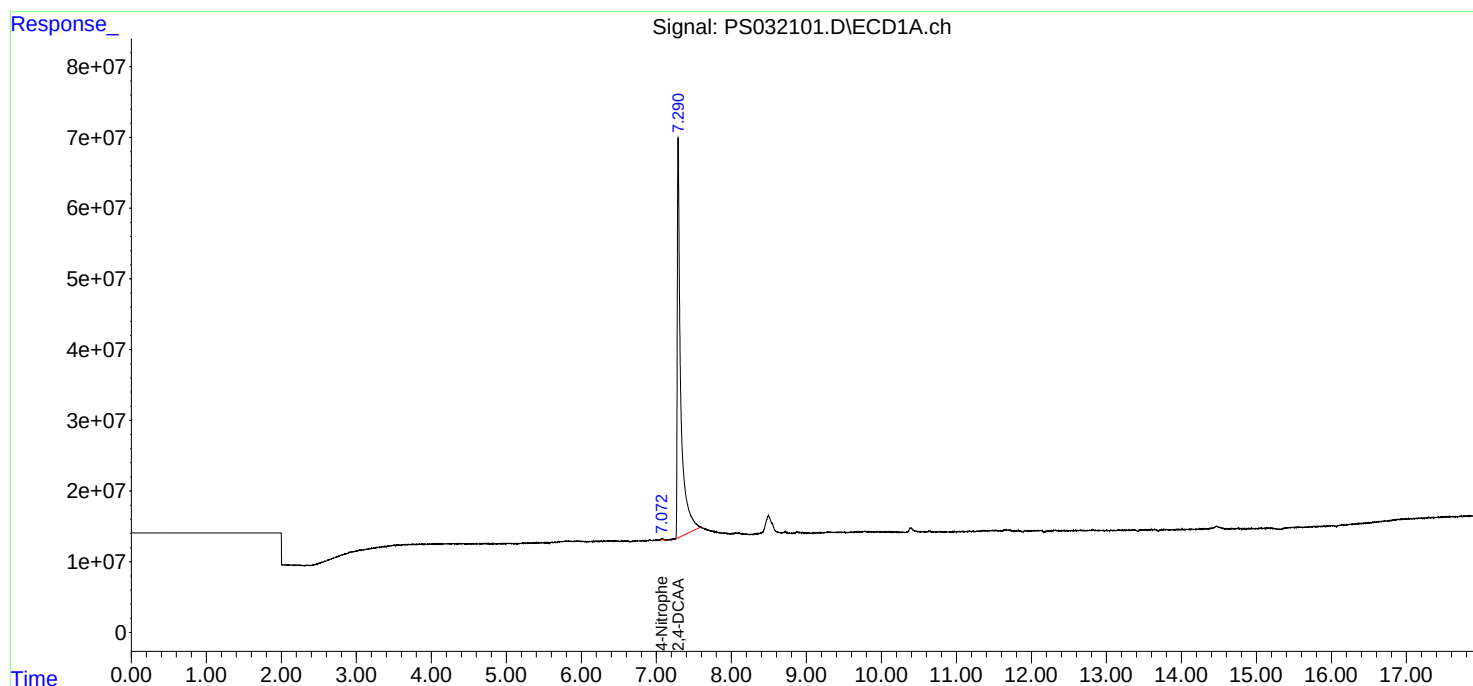


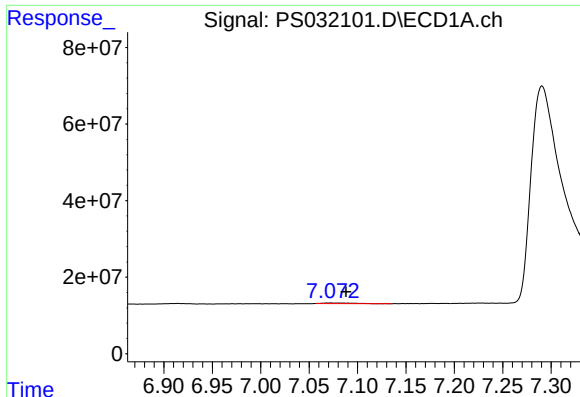

#3 4-Nitrophenol


R.T.: 7.072 min
Delta R.T.: -0.016 min
Response: 3347923
Conc: 2.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

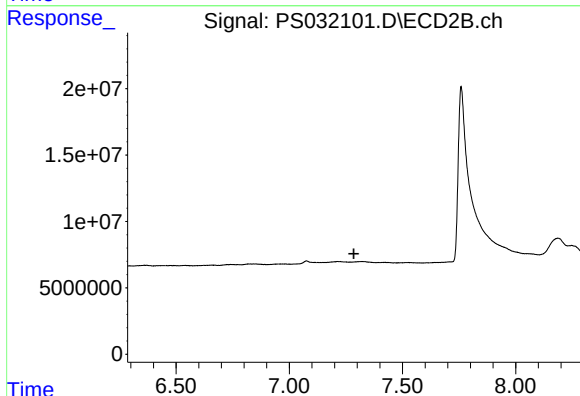


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.285 min
Response: 0
Conc: N.D.

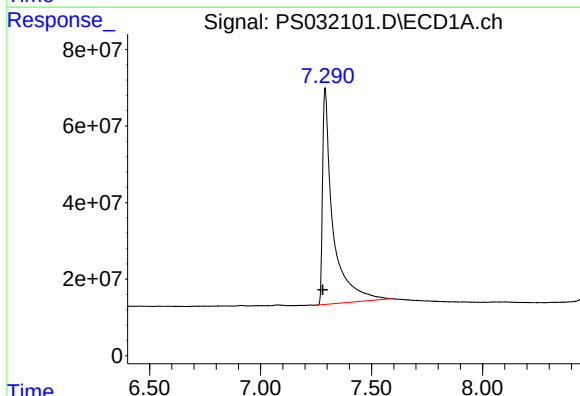


#4 2,4-DCAA

R.T.: 7.291 min
Delta R.T.: 0.011 min
Response: 1838321887
Conc: 385.63 ng/ml

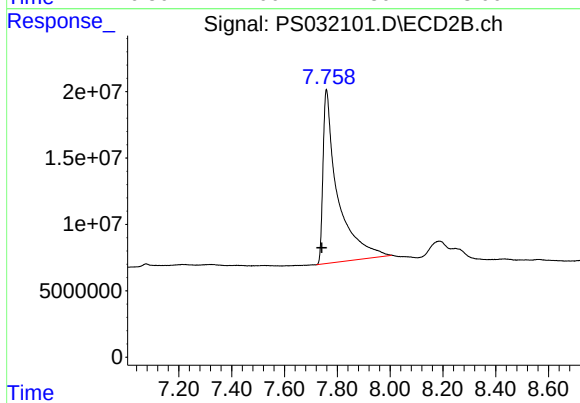

#4 2,4-DCAA


R.T.: 7.759 min
Delta R.T.: 0.018 min
Response: 507138939
Conc: 460.89 ng/ml

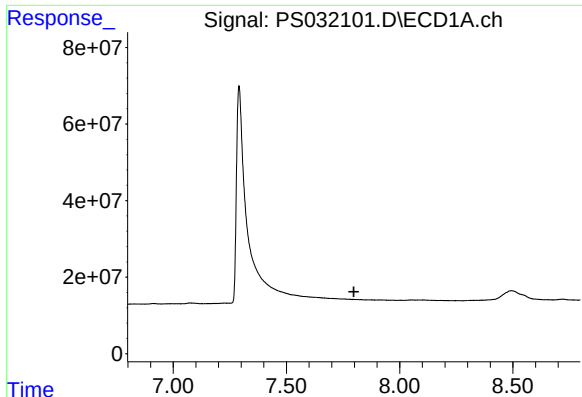

#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.798 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

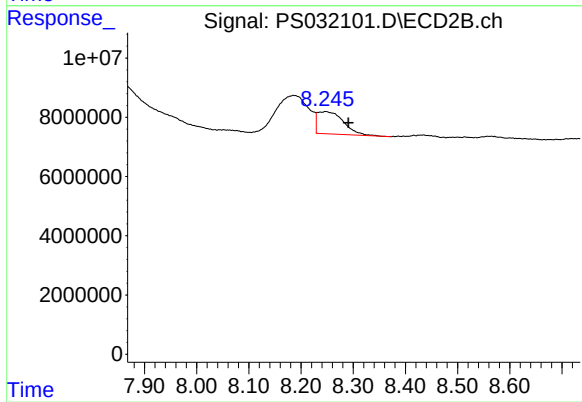

#7 MCPA

R.T.: 8.247 min
Delta R.T.: -0.044 min
Response: 25738934
Conc: 6.82 ug/ml