

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102125\
 Data File : PS032117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2025 23:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 15:30:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.282	7.748	1902.2E6	540.3E6	399.036	490.992
Target Compounds							
2) T	3,5-DICHL...	6.461	0.000	2052105	0	<MDL	N.D. #
3) T	4-Nitroph...	7.066	0.000	368221	0	<MDL	N.D. #
5) T	DICAMBA	7.463	7.941	23913383	8209213	1.142	<MDL #
7) T	MCPA	7.770f	8.254f	6367175	24824284	<MDL	6.581 #
8) T	DICHLORPROP	8.177	0.000	2518812	0	<MDL	N.D. #
10) T	Pentachlo...	8.704	9.514	19653048	33057927	<MDL	<MDL #
11) T	2,4,5-TP ...	9.284	9.908	20435379	20277892	<MDL	1.010 #
12) T	2,4,5-T	9.561	0.000	1088745	0	<MDL	N.D. #
13) T	2,4-DB	10.151	10.919f	4937527	11765404	1.593	9.106 #
14) T	DINOSEB	11.349	0.000	7541613	0	<MDL	N.D. #
15) T	Picloram	11.156	0.000	5838483	0	<MDL	N.D. #
16) T	DCPA	11.650	12.310	50605849	21149383	1.377	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102125\
Data File : PS032117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2025 23:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 15:30:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

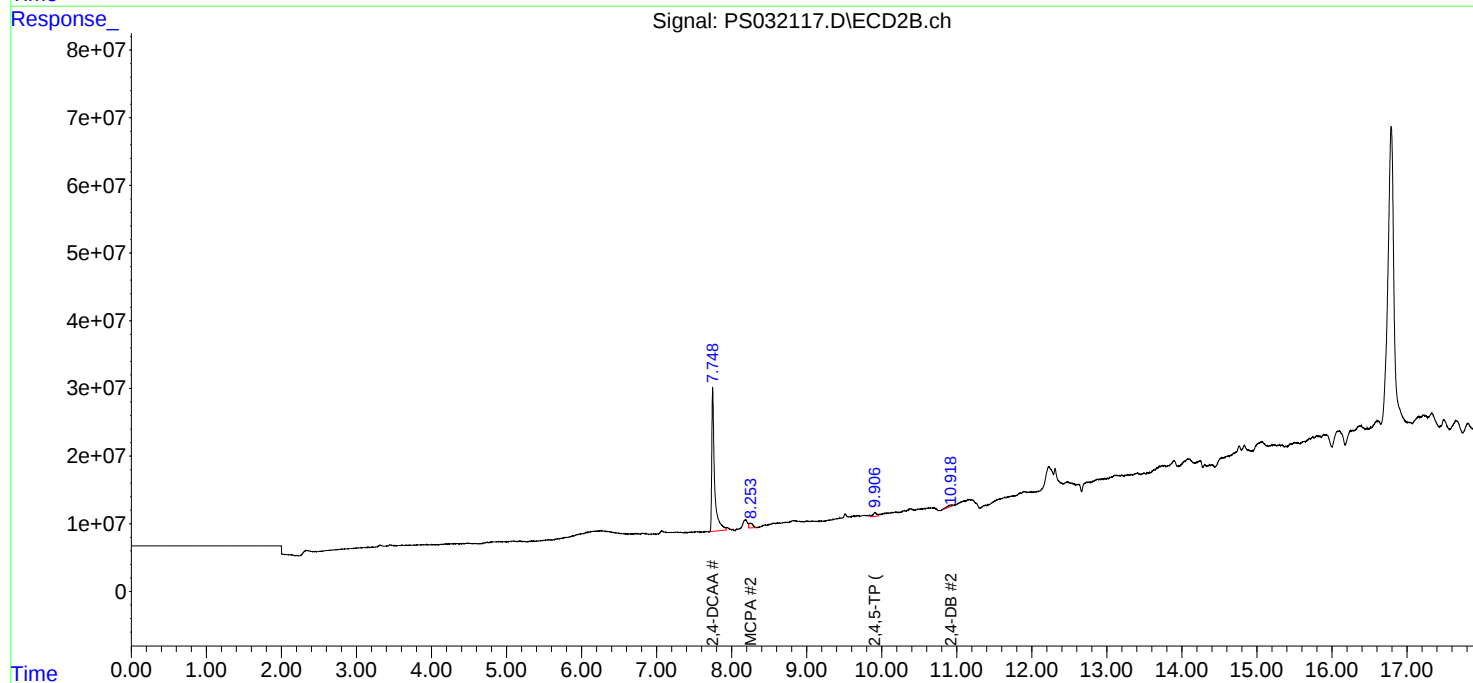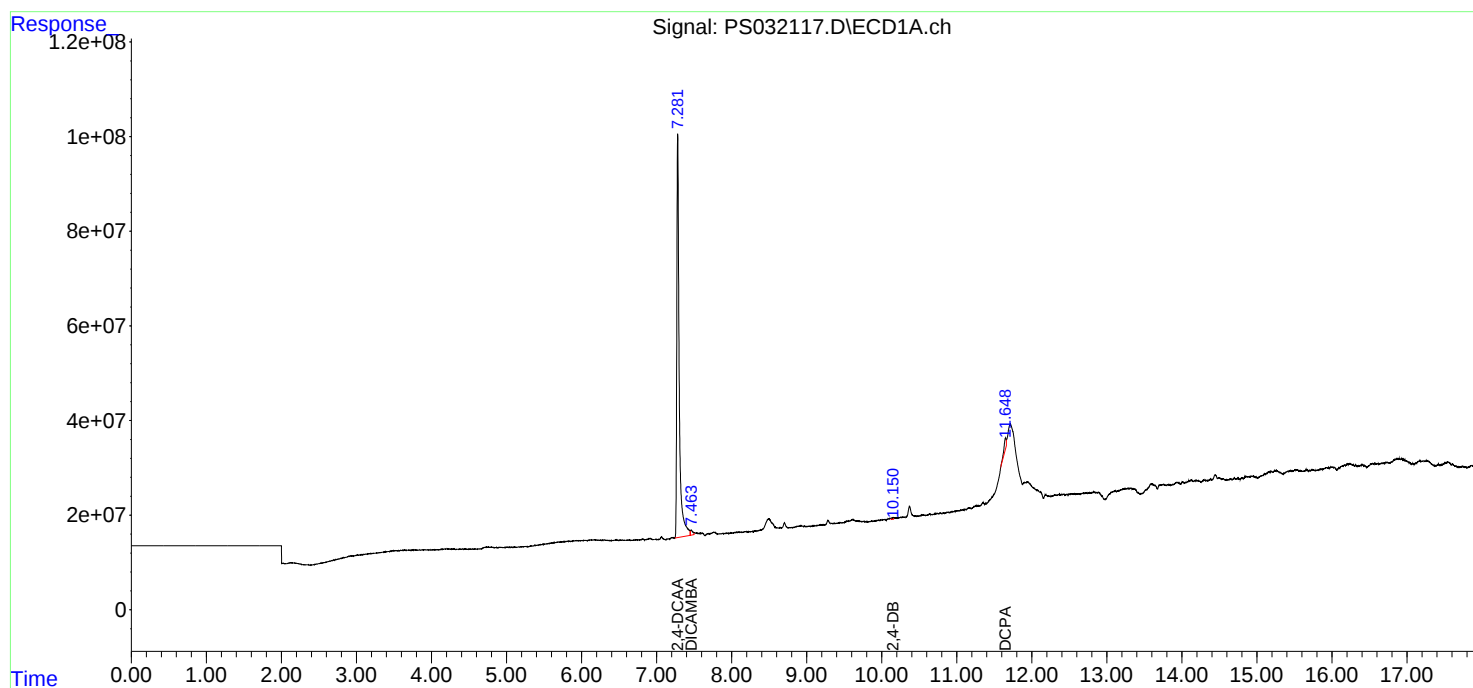


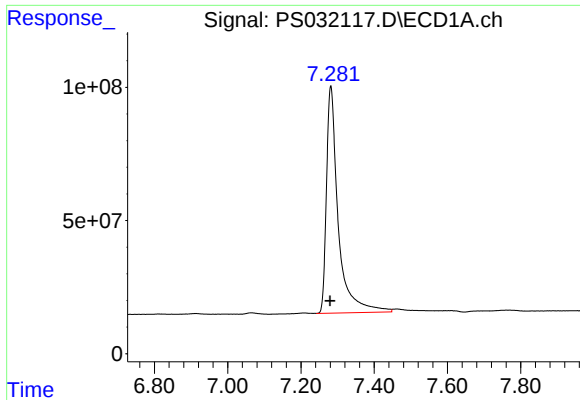

#4 2,4-DCAA


R.T.: 7.282 min
Delta R.T.: 0.002 min
Response: 1902220028
Conc: 399.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

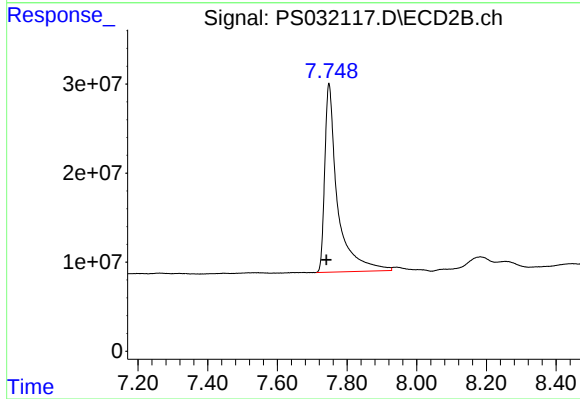


#4 2,4-DCAA

R.T.: 7.748 min
Delta R.T.: 0.007 min
Response: 540258429
Conc: 490.99 ng/ml

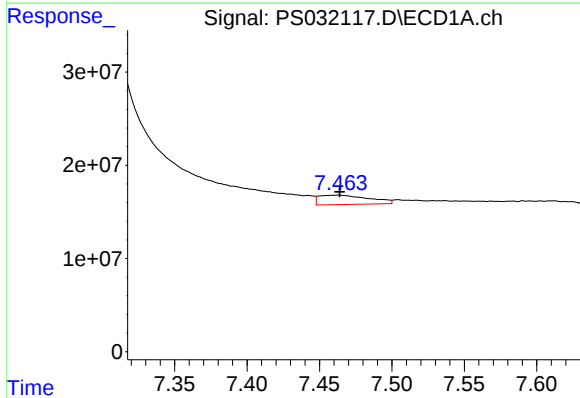


#5 DICAMBA

R.T.: 7.463 min
Delta R.T.: 0.000 min
Response: 23913383
Conc: 1.14 ng/ml

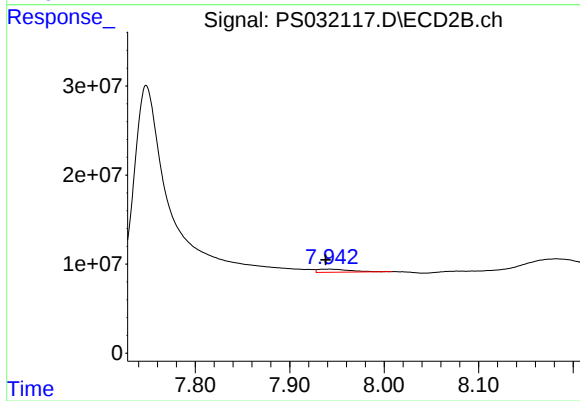

#5 DICAMBA


R.T.: 7.941 min
Delta R.T.: 0.003 min
Response: 8209213
Conc: N.D.

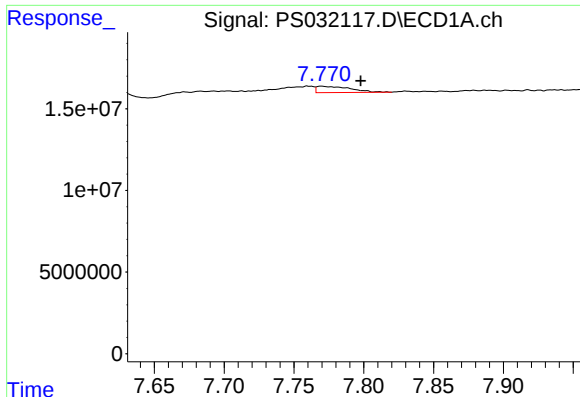

#7 MCPA


R.T.: 7.770 min
Delta R.T.: -0.028 min
Response: 6367175
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

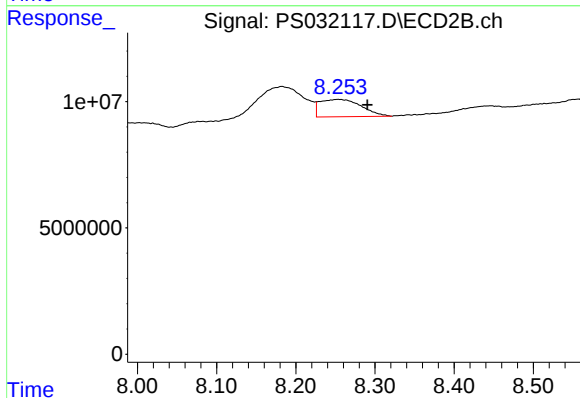


#7 MCPA

R.T.: 8.254 min
Delta R.T.: -0.036 min
Response: 24824284
Conc: 6.58 ug/ml

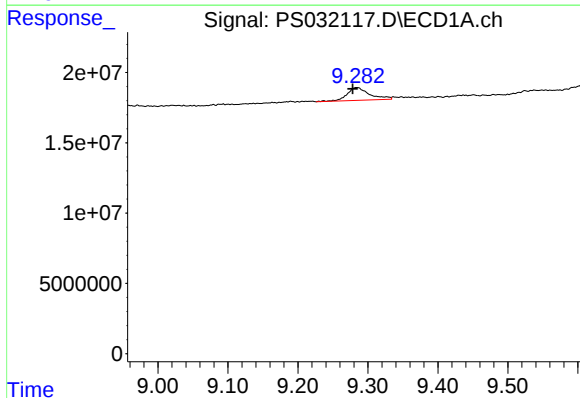


#11 2,4,5-TP (SILVEX)

R.T.: 9.284 min
Delta R.T.: 0.006 min
Response: 20435379
Conc: N.D.

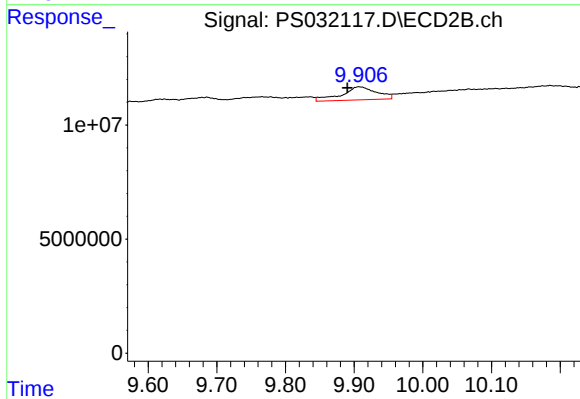

#11 2,4,5-TP (SILVEX)


R.T.: 9.908 min
Delta R.T.: 0.017 min
Response: 20277892
Conc: 1.01 ng/ml

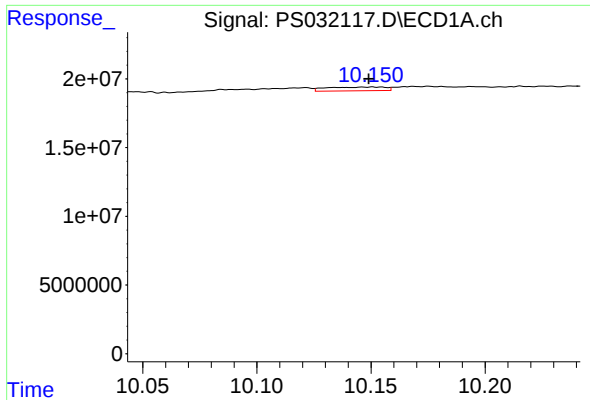

#13 2,4-DB


R.T.: 10.151 min
Delta R.T.: 0.002 min
Response: 4937527
Conc: 1.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

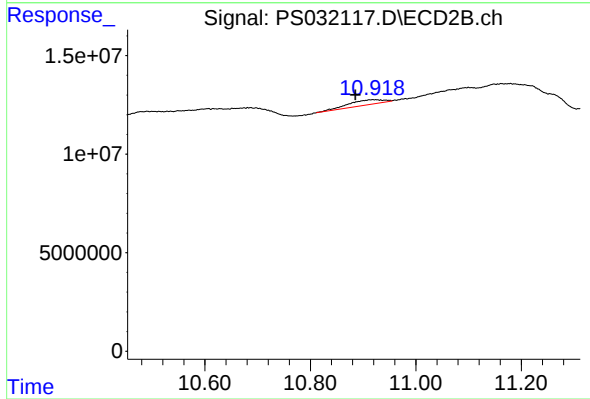


#13 2,4-DB

R.T.: 10.919 min
Delta R.T.: 0.034 min
Response: 11765404
Conc: 9.11 ng/ml

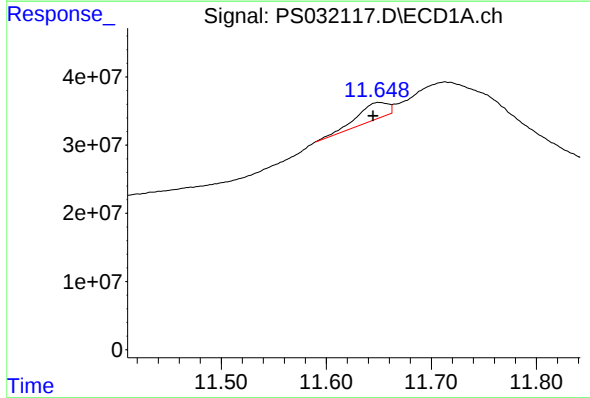

#16 DCPA

R.T.: 11.650 min
Delta R.T.: 0.005 min
Response: 50605849
Conc: 1.38 ng/ml

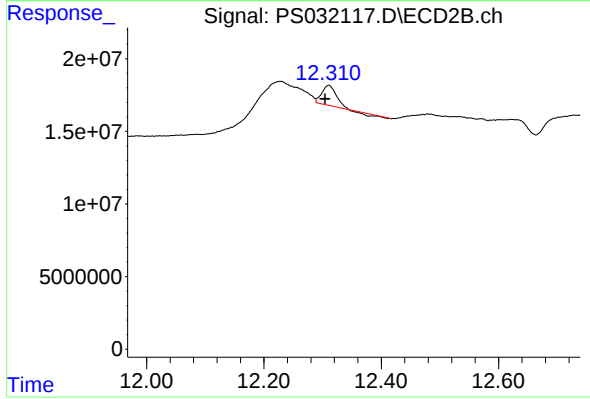

#16 DCPA

R.T.: 12.310 min
Delta R.T.: 0.006 min
Response: 21149383
Conc: N.D.