

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102225\
 Data File : PS032120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2025 09:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 15:50:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.288	7.754	1984.2E6	555.0E6	416.227	504.349
Target Compounds							
2) T	3,5-DICHL...	6.445	0.000	989395	0	<MDL	N.D. #
7) T	MCPA	0.000	8.241f	0	16217905	N.D.	4.299
8) T	DICHLORPROP	8.193	0.000	603694	0	<MDL	N.D. #
10) T	Pentachlo...	8.715	9.519	9504296	5021399	<MDL	<MDL #
11) T	2,4,5-TP ...	9.308f	9.928f	8533360	3714503	<MDL	<MDL #
12) T	2,4,5-T	9.606f	10.305	-498512	2561252	N.D.	<MDL
13) T	2,4-DB	10.111f	0.000	4492945	0	1.449	N.D. #
14) T	DINOSEB	11.354	11.280	17713197	3808728	<MDL	<MDL #
15) T	Picloram	11.172	12.414f	2810500	22083609	<MDL	<MDL #
16) T	DCPA	11.651	12.319	20037453	30708241	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102225\
Data File : PS032120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2025 09:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 15:50:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

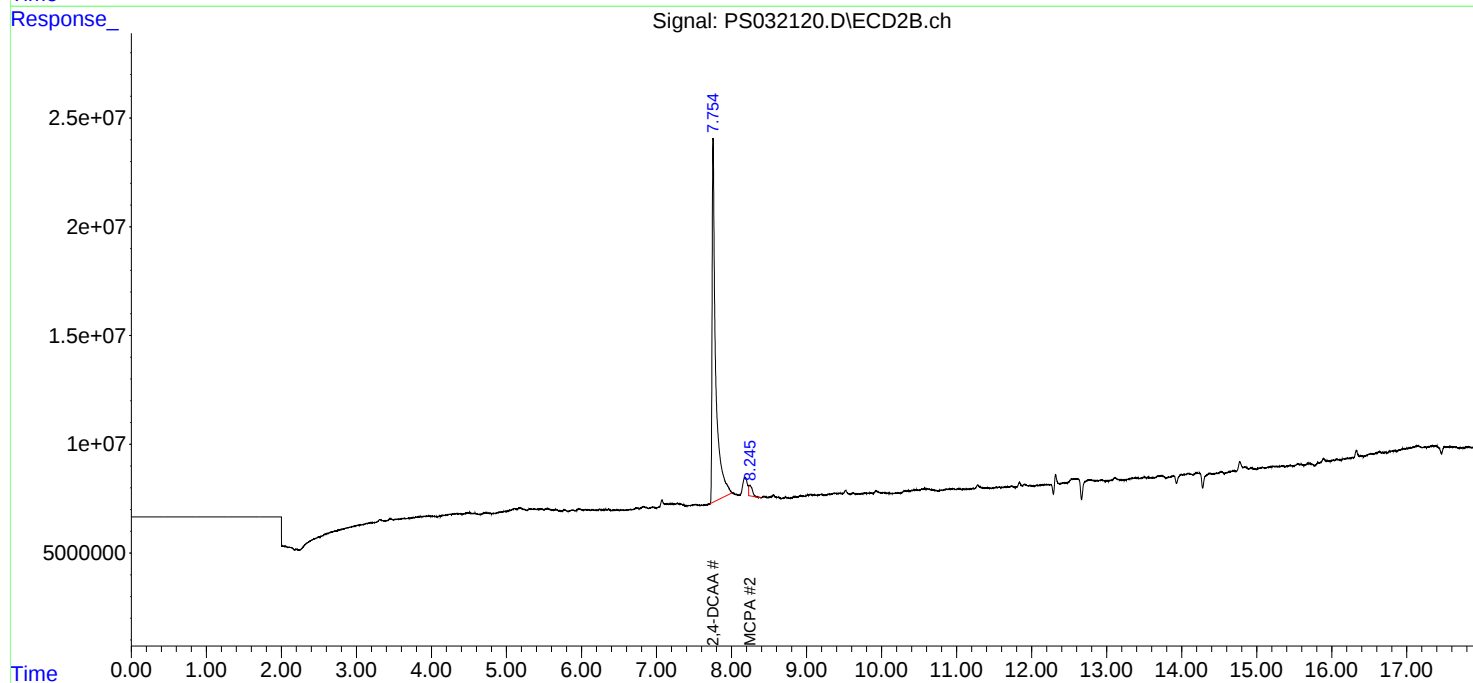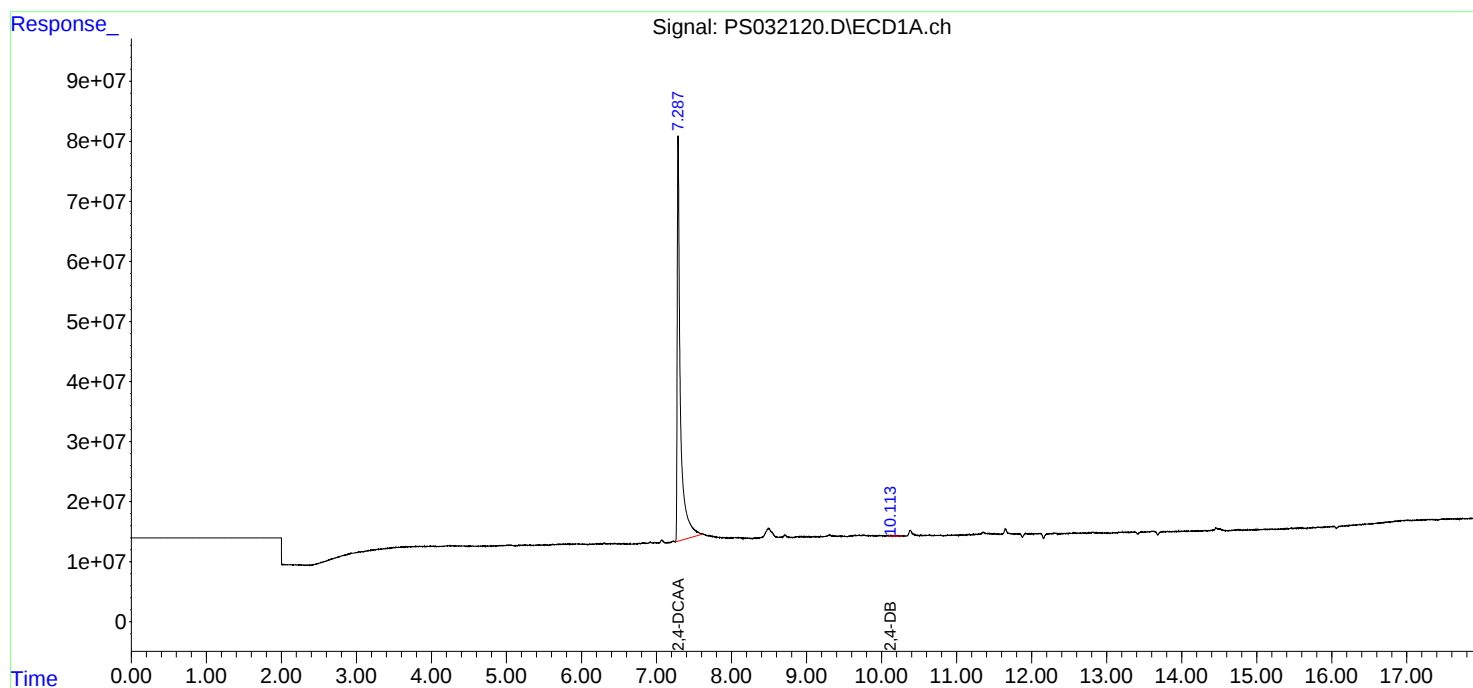


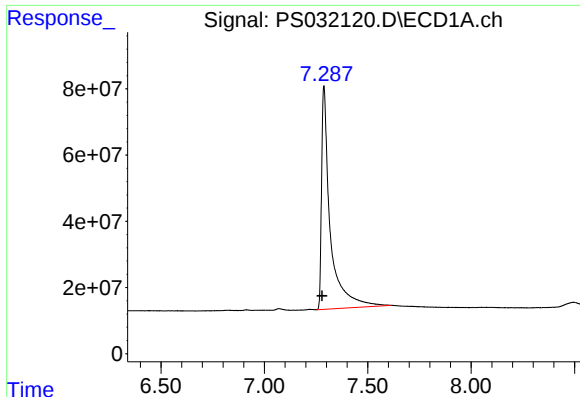

#4 2,4-DCAA


R.T.: 7.288 min
Delta R.T.: 0.008 min
Response: 1984168126
Conc: 416.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

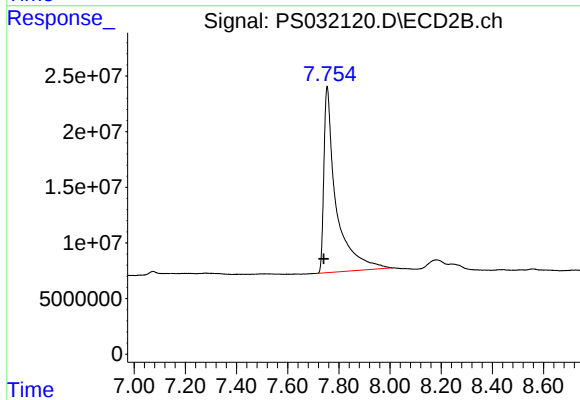


#4 2,4-DCAA

R.T.: 7.754 min
Delta R.T.: 0.013 min
Response: 554956095
Conc: 504.35 ng/ml

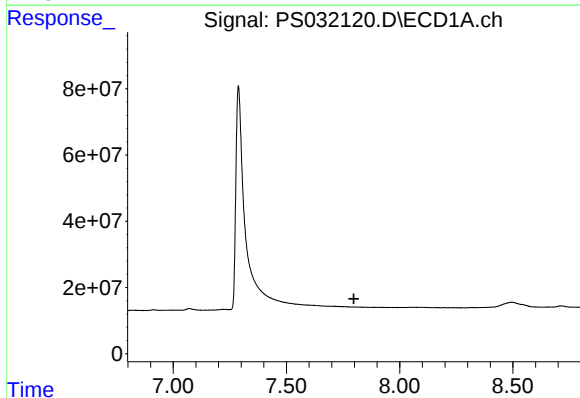


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.798 min
Response: 0
Conc: N.D.

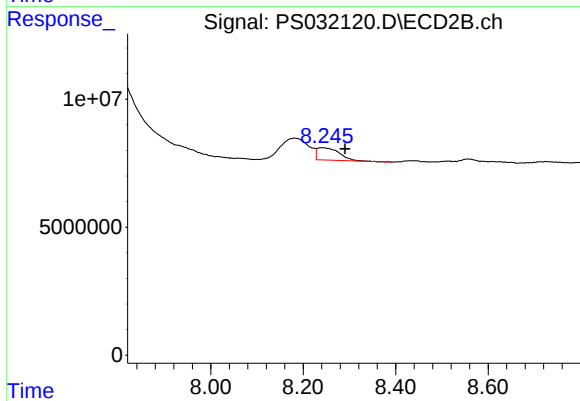

#7 MCPA


R.T.: 8.241 min
Delta R.T.: -0.050 min
Response: 16217905
Conc: 4.30 ug/ml

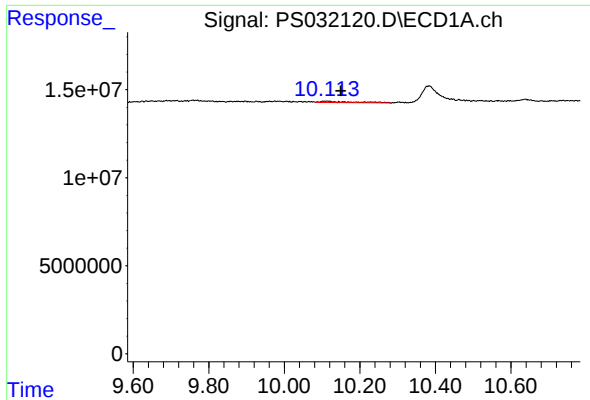

#13 2,4-DB

R.T.: 10.111 min
Delta R.T.: -0.038 min
Response: 4492945
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

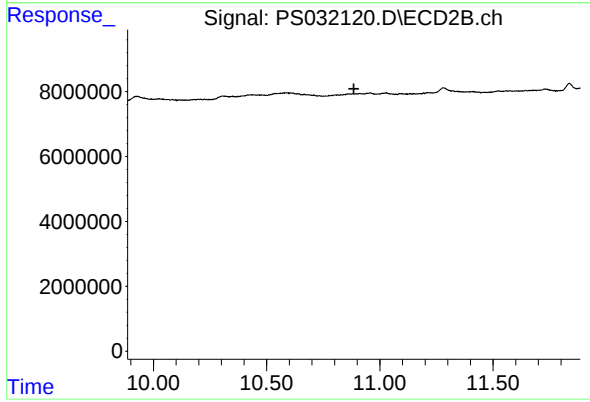

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.885 min
Response: 0
Conc: N.D.