

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
 Data File : PS002083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2018 18:56
 Operator : EI\SJ
 Sample : PB114099TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 01:00:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.468	10.960	102.1E6	96493447	482.730	404.573
Target Compounds							
1) T	Dalapon	2.904	2.387	46306922	70328765	151.748	240.879 #
2) T	3,5-DICHL...	0.000	9.051	0	4955453	N.D.	16.946 #
5) T	DICAMBA	11.706	11.202	5485308	20777461	6.969	25.286 #
6) T	MCP	12.058	0.000	211091	0	0.377	N.D. #
10) T	Pentachlo...	0.000	13.314	0	3480737	N.D.	1.099 #
13) T	2,4-DB	15.710	0.000	4856822	0	30.921	N.D. #
16) T	DCPA	17.473	16.892	17080783	-316433	12.323	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
Data File : PS002083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2018 18:56
Operator : EI\SJ
Sample : PB114099TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 01:00:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

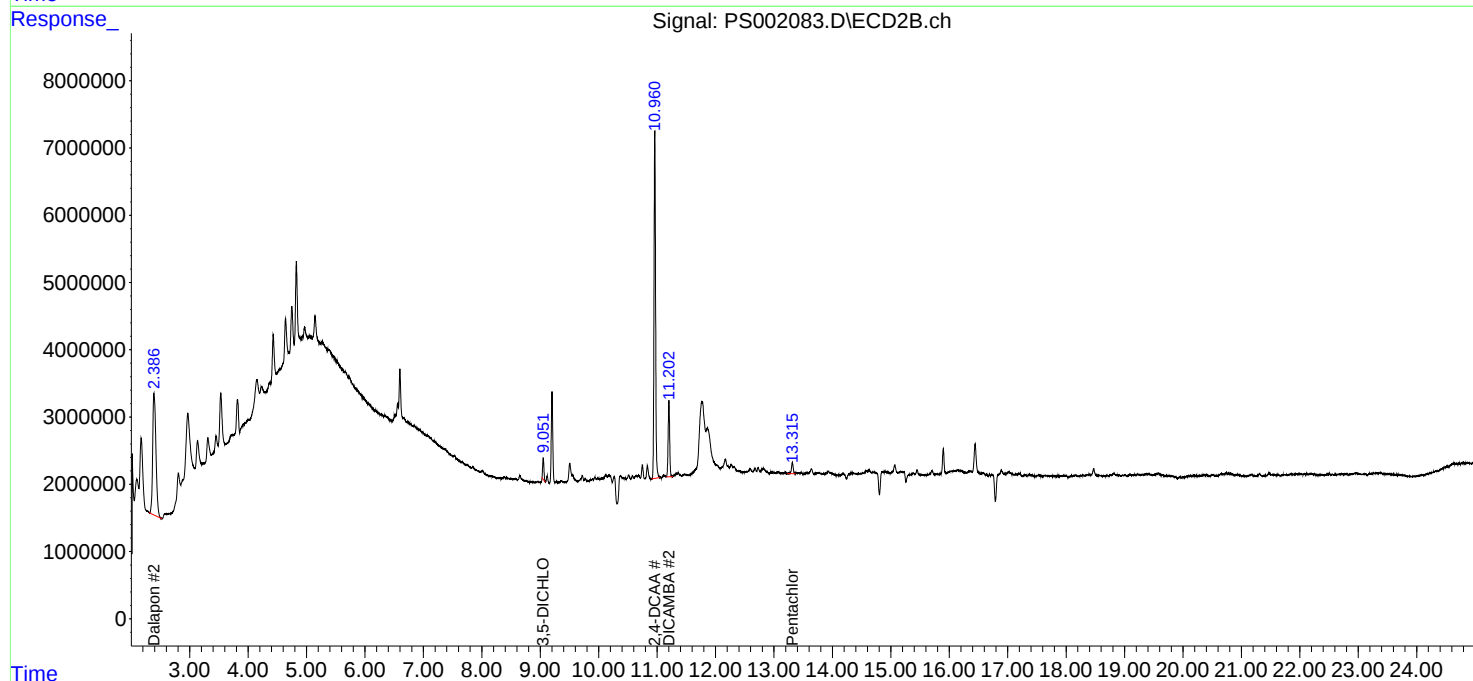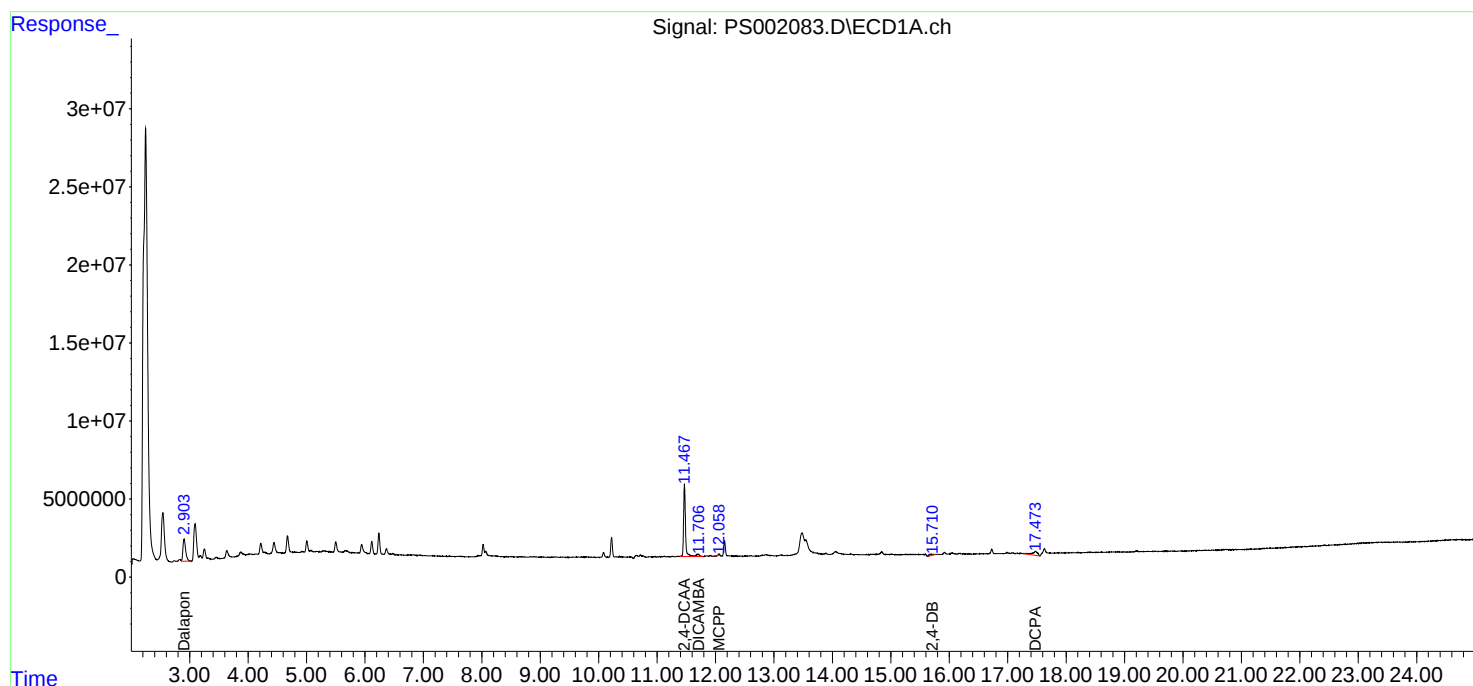


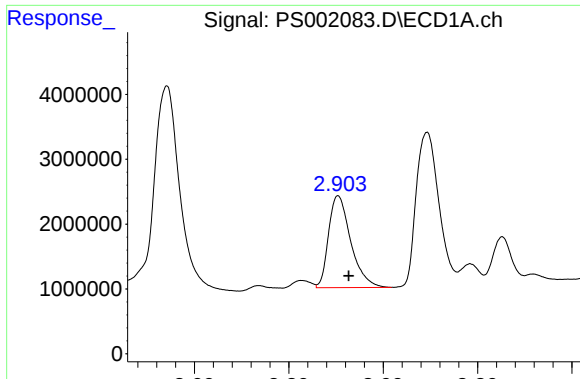

#1 Dalapon


R.T.: 2.904 min
Delta R.T.: -0.023 min
Response: 46306922
Conc: 151.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

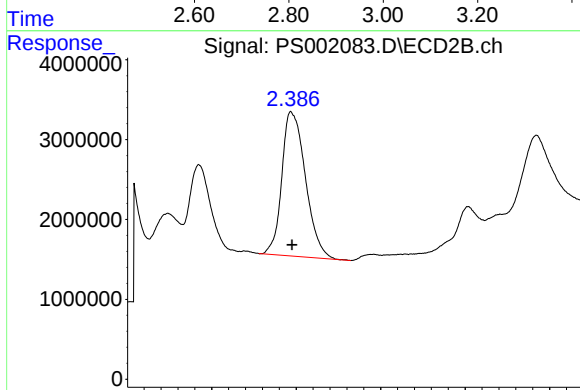


#1 Dalapon

R.T.: 2.387 min
Delta R.T.: -0.003 min
Response: 70328765
Conc: 240.88 ng/ml

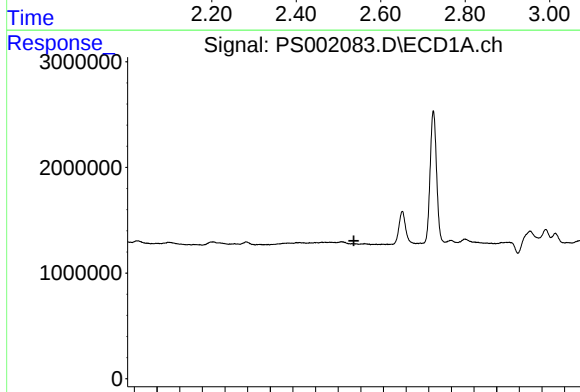


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

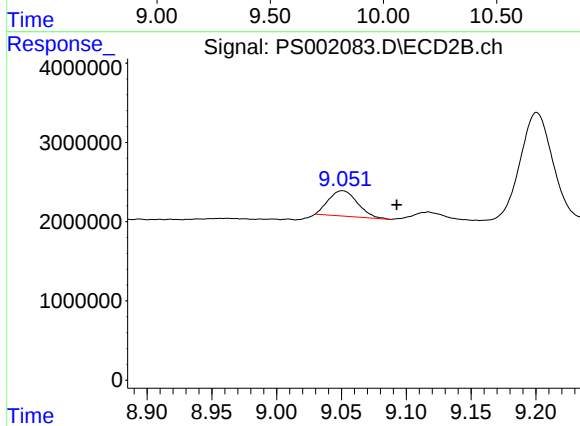

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.051 min
Delta R.T.: -0.042 min
Response: 4955453
Conc: 16.95 ng/ml

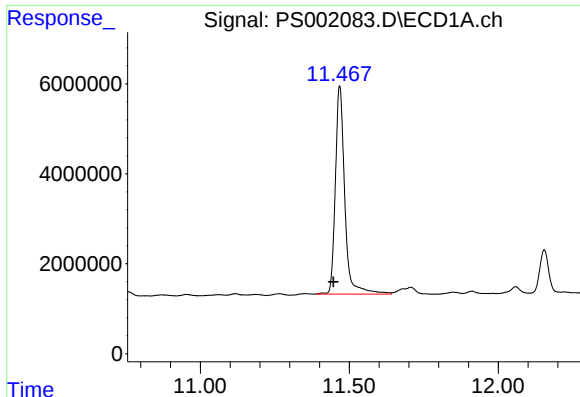

#4 2,4-DCAA


R.T.: 11.468 min
Delta R.T.: 0.021 min
Response: 102050148
Conc: 482.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

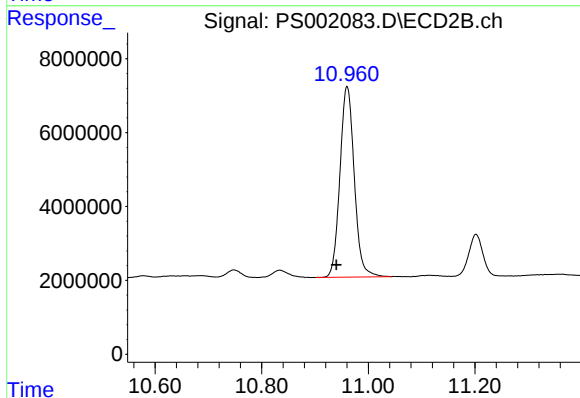


#4 2,4-DCAA

R.T.: 10.960 min
Delta R.T.: 0.020 min
Response: 96493447
Conc: 404.57 ng/ml

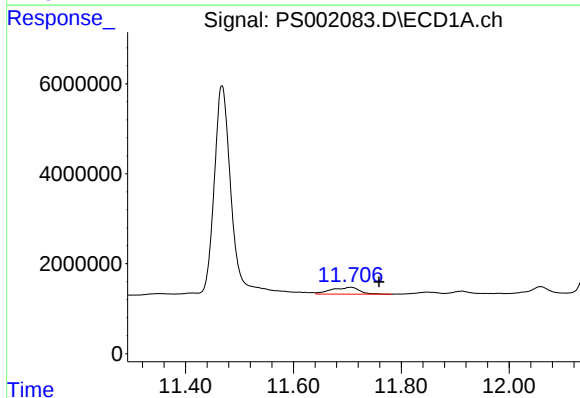


#5 DICAMBA

R.T.: 11.706 min
Delta R.T.: -0.053 min
Response: 5485308
Conc: 6.97 ng/ml

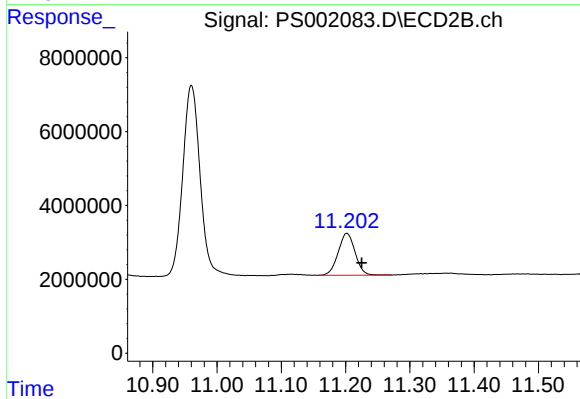

#5 DICAMBA


R.T.: 11.202 min
Delta R.T.: -0.023 min
Response: 20777461
Conc: 25.29 ng/ml

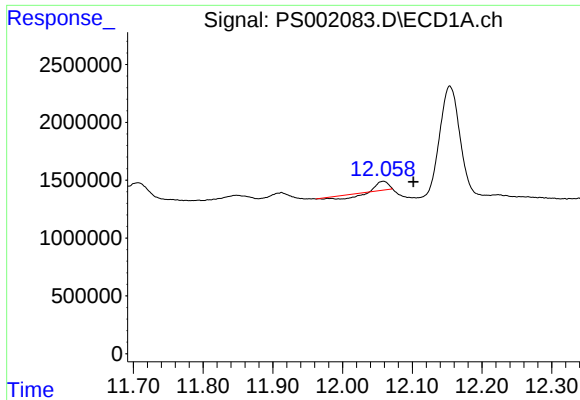

#6 MCP


R.T.: 12.058 min
Delta R.T.: -0.044 min
Response: 211091
Conc: 0.38 ug/ml

Instrument :
ECD_S
ClientSampleId :

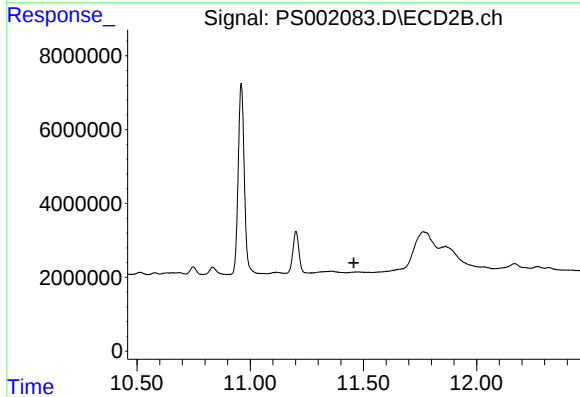


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.458 min
Response: 0
Conc: N.D.

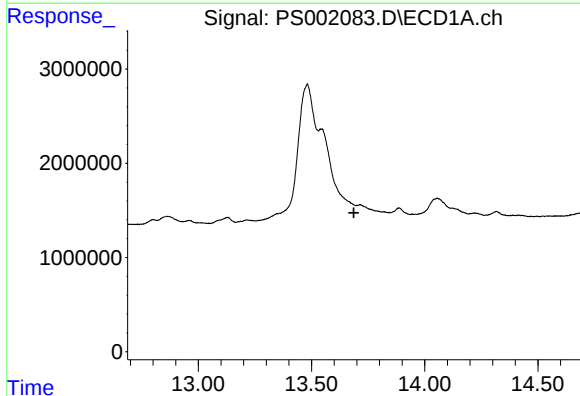


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.687 min
Response: 0
Conc: N.D.

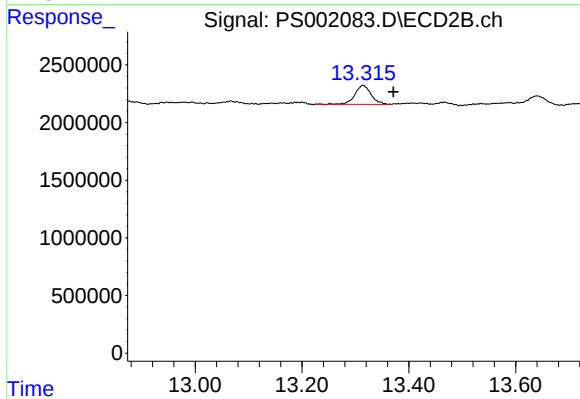

#10 Pentachlorophenol


R.T.: 13.314 min
Delta R.T.: -0.057 min
Response: 3480737
Conc: 1.10 ng/ml

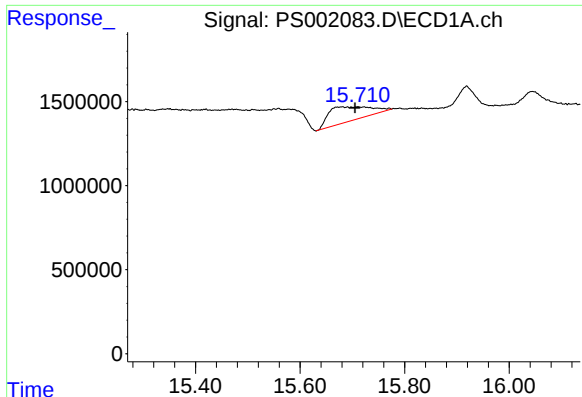

#13 2,4-DB


R.T.: 15.710 min
Delta R.T.: 0.005 min
Response: 4856822
Conc: 30.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

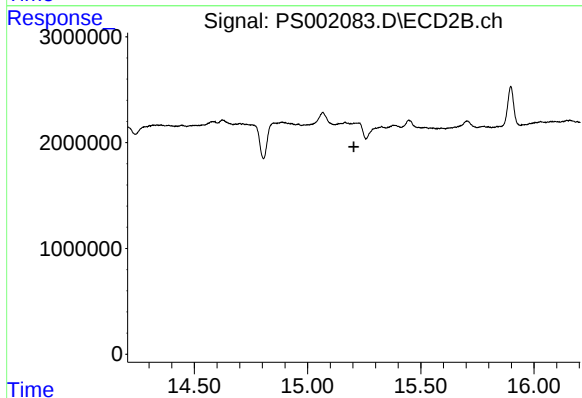


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.205 min
Response: 0
Conc: N.D.

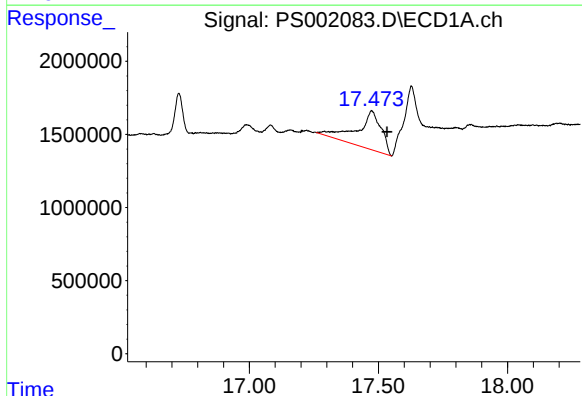

#16 DCPA

R.T.: 17.473 min
Delta R.T.: -0.060 min
Response: 17080783
Conc: 12.32 ng/ml

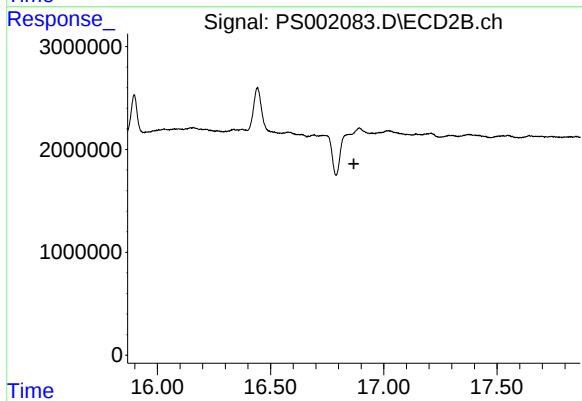

#16 DCPA

R.T.: 16.892 min
Delta R.T.: 0.024 min
Response: -316433
Conc: N.D.