

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
 Data File : PS002085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2018 19:58
 Operator : EI\SJ
 Sample : J5604-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 01:00:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.464	10.957	89955455	89168266	425.518	373.860
Target Compounds							
1) T	Dalapon	2.900	2.388	54965464	95476680	180.122	327.012 #
2) T	3,5-DICHL...	0.000	9.047	0	4011718	N.D.	13.718 #
5) T	DICAMBA	11.702	11.198	3428732	20451925	4.356	24.890 #
6) T	MCP	12.150	0.000	18495611	0	33.031	N.D. #
10) T	Pentachlo...	0.000	13.310	0	4393881	N.D.	1.388 #
11) T	2,4,5-TP ...	14.531	0.000	7846127	0	7.173	N.D. #
14) T	DINOSEB	0.000	15.703	0	3276174	N.D.	3.704 #
16) T	DCPA	17.470	16.934	11953812	17833811	8.624	9.857



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
Data File : PS002085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2018 19:58
Operator : EI\SJ
Sample : J5604-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 01:00:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

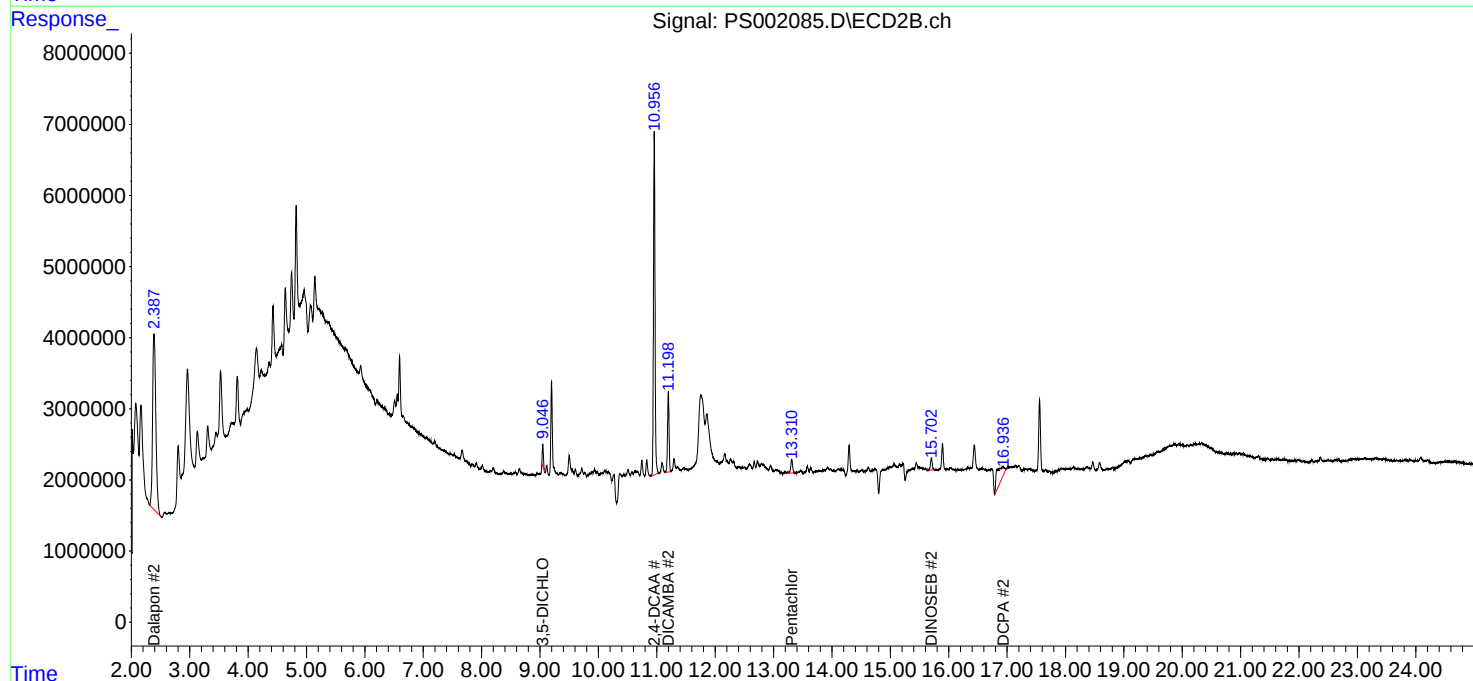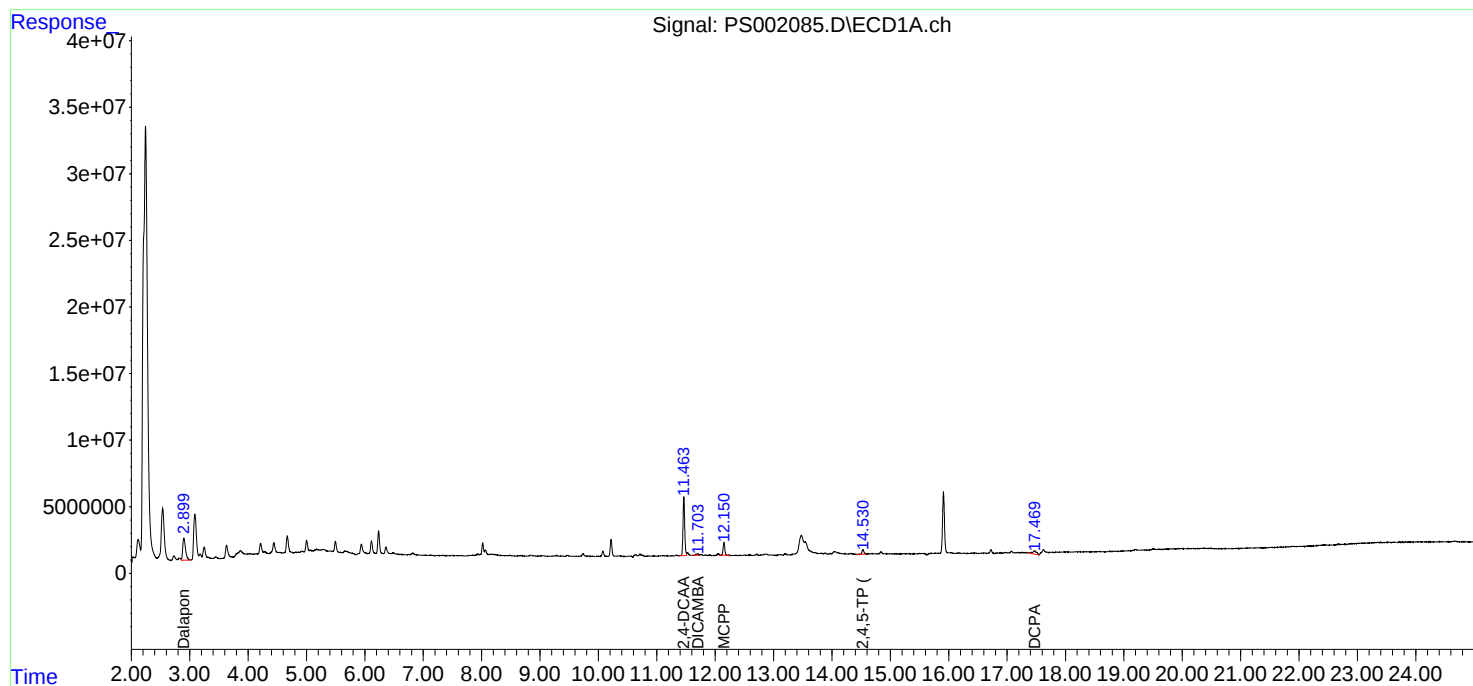


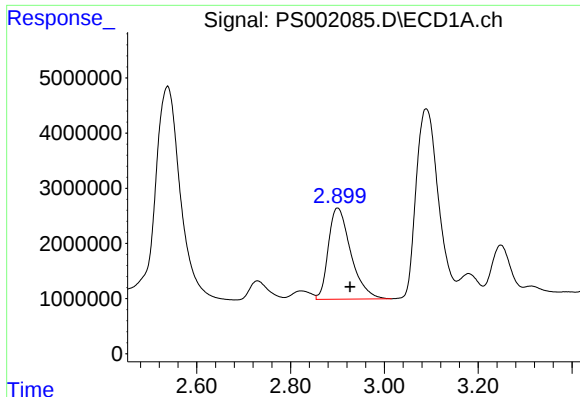

#1 Dalapon


R.T.: 2.900 min
Delta R.T.: -0.027 min
Response: 54965464
Conc: 180.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

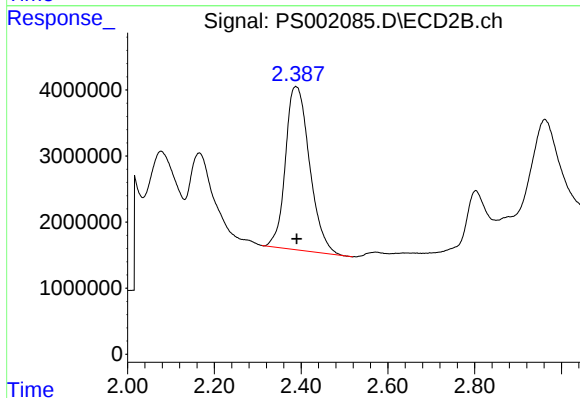


#1 Dalapon

R.T.: 2.388 min
Delta R.T.: -0.002 min
Response: 95476680
Conc: 327.01 ng/ml

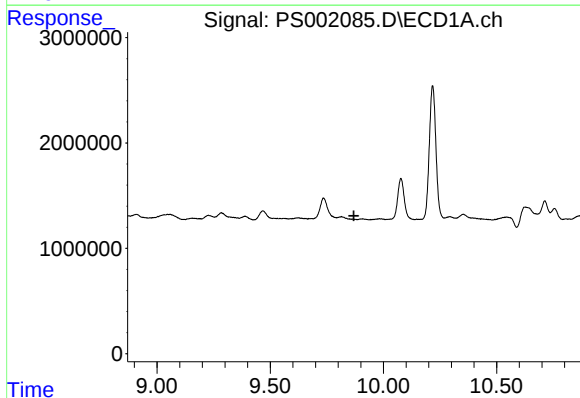


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

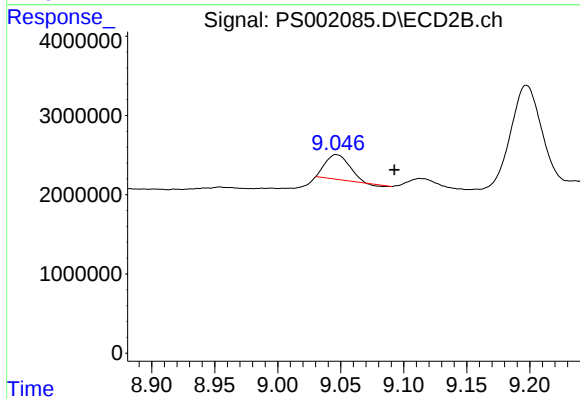

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.047 min
Delta R.T.: -0.046 min
Response: 4011718
Conc: 13.72 ng/ml

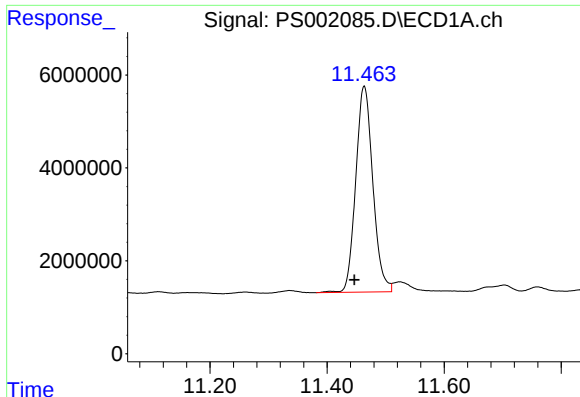

#4 2,4-DCAA


R.T.: 11.464 min
Delta R.T.: 0.017 min
Response: 89955455
Conc: 425.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

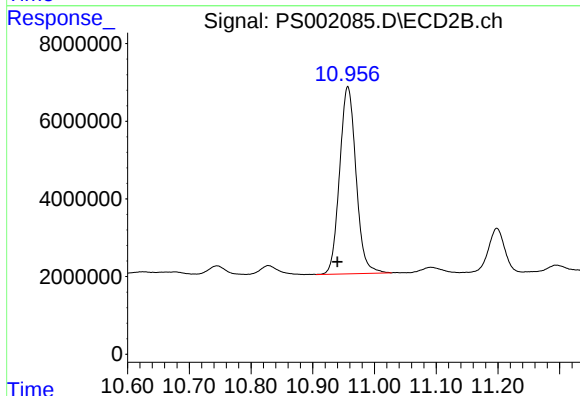


#4 2,4-DCAA

R.T.: 10.957 min
Delta R.T.: 0.017 min
Response: 89168266
Conc: 373.86 ng/ml

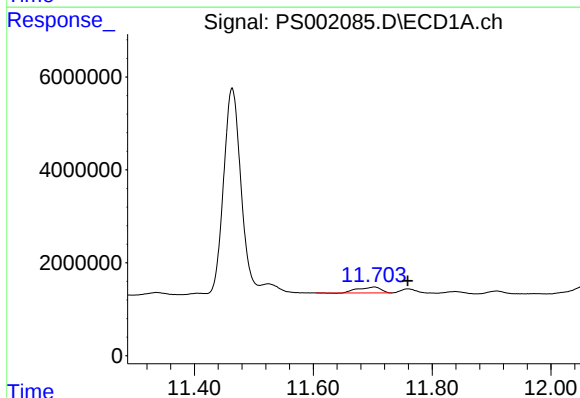


#5 DICAMBA

R.T.: 11.702 min
Delta R.T.: -0.056 min
Response: 3428732
Conc: 4.36 ng/ml

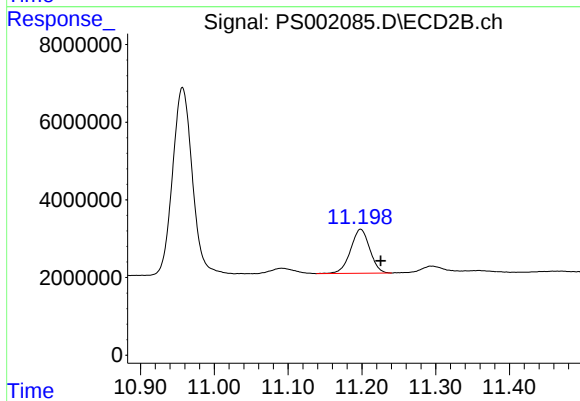

#5 DICAMBA


R.T.: 11.198 min
Delta R.T.: -0.027 min
Response: 20451925
Conc: 24.89 ng/ml

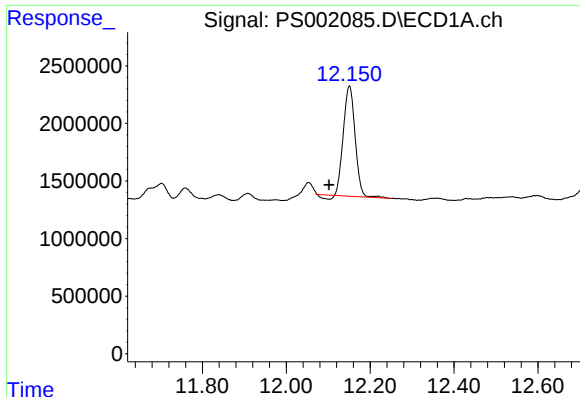

#6 MCP


R.T.: 12.150 min
Delta R.T.: 0.049 min
Response: 18495611
Conc: 33.03 ug/ml

Instrument :
ECD_S
ClientSampleId :

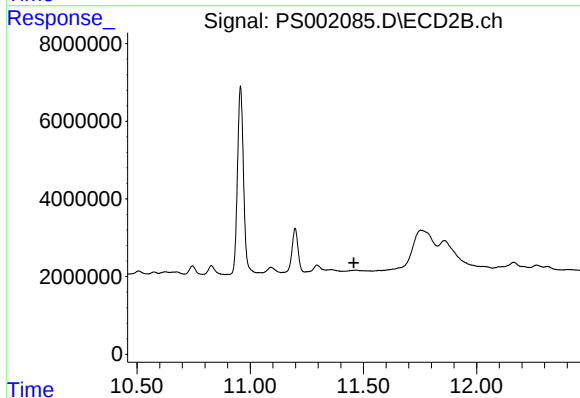


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.458 min
Response: 0
Conc: N.D.

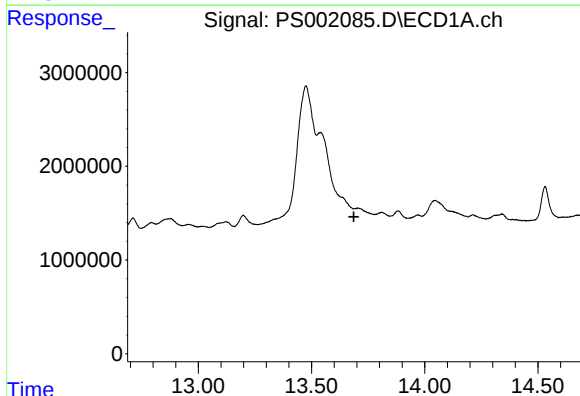


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.687 min
Response: 0
Conc: N.D.

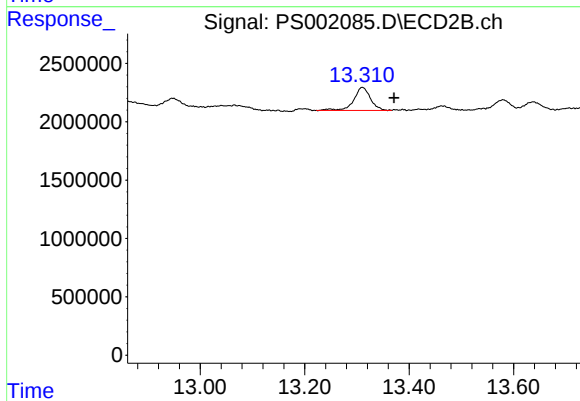

#10 Pentachlorophenol


R.T.: 13.310 min
Delta R.T.: -0.061 min
Response: 4393881
Conc: 1.39 ng/ml

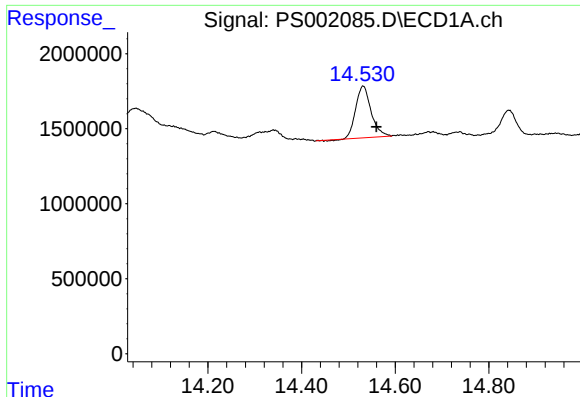

#11 2,4,5-TP (SILVEX)


R.T.: 14.531 min
Delta R.T.: -0.028 min
Response: 7846127
Conc: 7.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

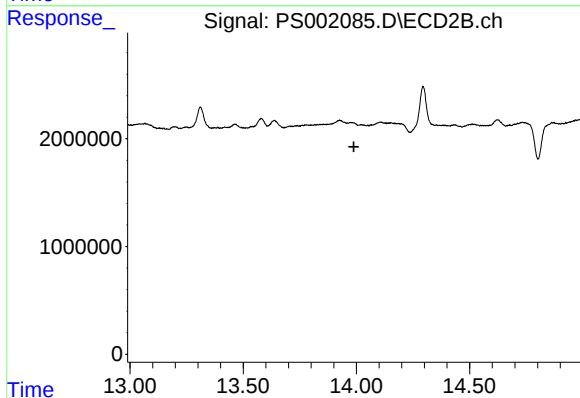


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.988 min
Response: 0
Conc: N.D.

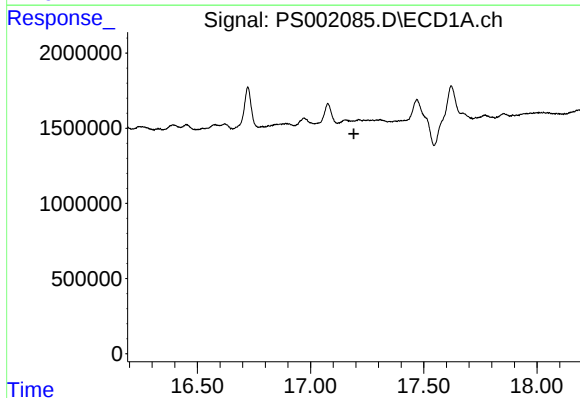


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.192 min
Response: 0
Conc: N.D.

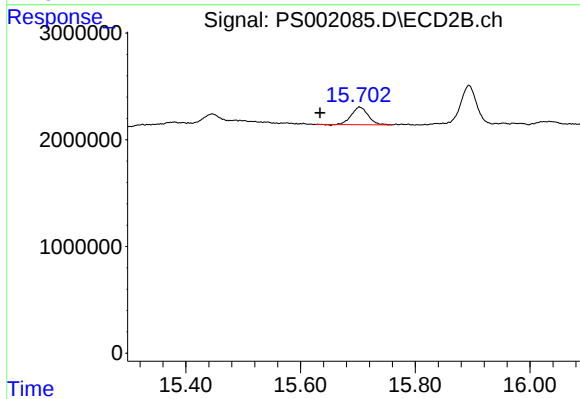

#14 DINOSEB


R.T.: 15.703 min
Delta R.T.: 0.069 min
Response: 3276174
Conc: 3.70 ng/ml

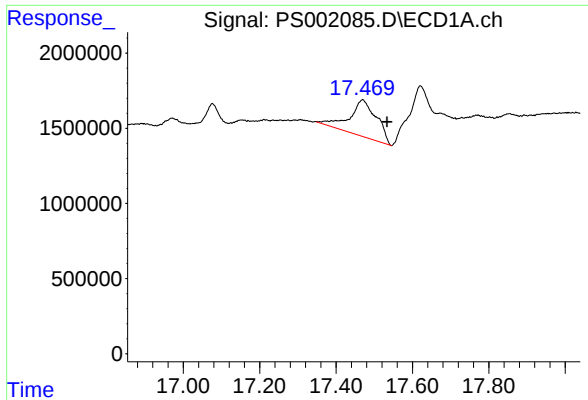

#16 DCPA

R.T.: 17.470 min
Delta R.T.: -0.064 min
Response: 11953812
Conc: 8.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

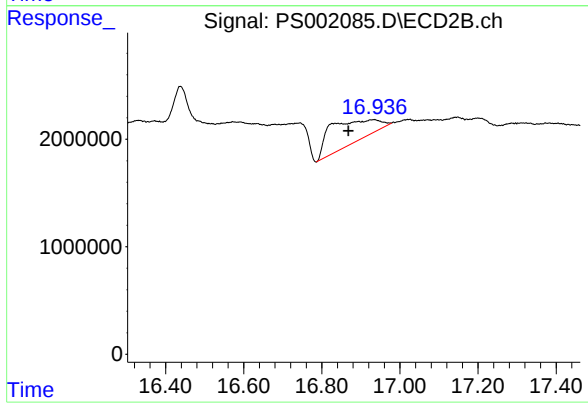

#16 DCPA

R.T.: 16.934 min
Delta R.T.: 0.066 min
Response: 17833811
Conc: 9.86 ng/ml