

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
 Data File : PS002090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2018 22:34
 Operator : EI\SJ
 Sample : J5604-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 01:02:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.445	10.938	98230203	94058447	464.661	394.363
Target Compounds							
1) T	Dalapon	2.882	2.365	49635307	63759200	162.655	218.378 #
5) T	DICAMBA	11.746	11.180	2211143	24348545	2.809	29.632 #
6) T	MCPD	12.132	0.000	23505187	0	41.977	N.D. #
7) T	MCPA	0.000	11.843	0	33314	N.D.	0.040 #
11) T	2,4,5-TP ...	14.516	0.000	6585140	0	6.020	N.D. #
12) T	2,4,5-T	0.000	14.557	0	2631825	N.D.	2.403 #
13) T	2,4-DB	15.761	15.201	30086	64394933	0.192	409.054 #
15) T	Picloram	16.966	16.869	14567425	37080064	8.520	23.376 #
16) T	DCPA	0.000	16.869	0	37080064	N.D.	20.495 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
Data File : PS002090.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2018 22:34
Operator : EI\SJ
Sample : J5604-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 01:02:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

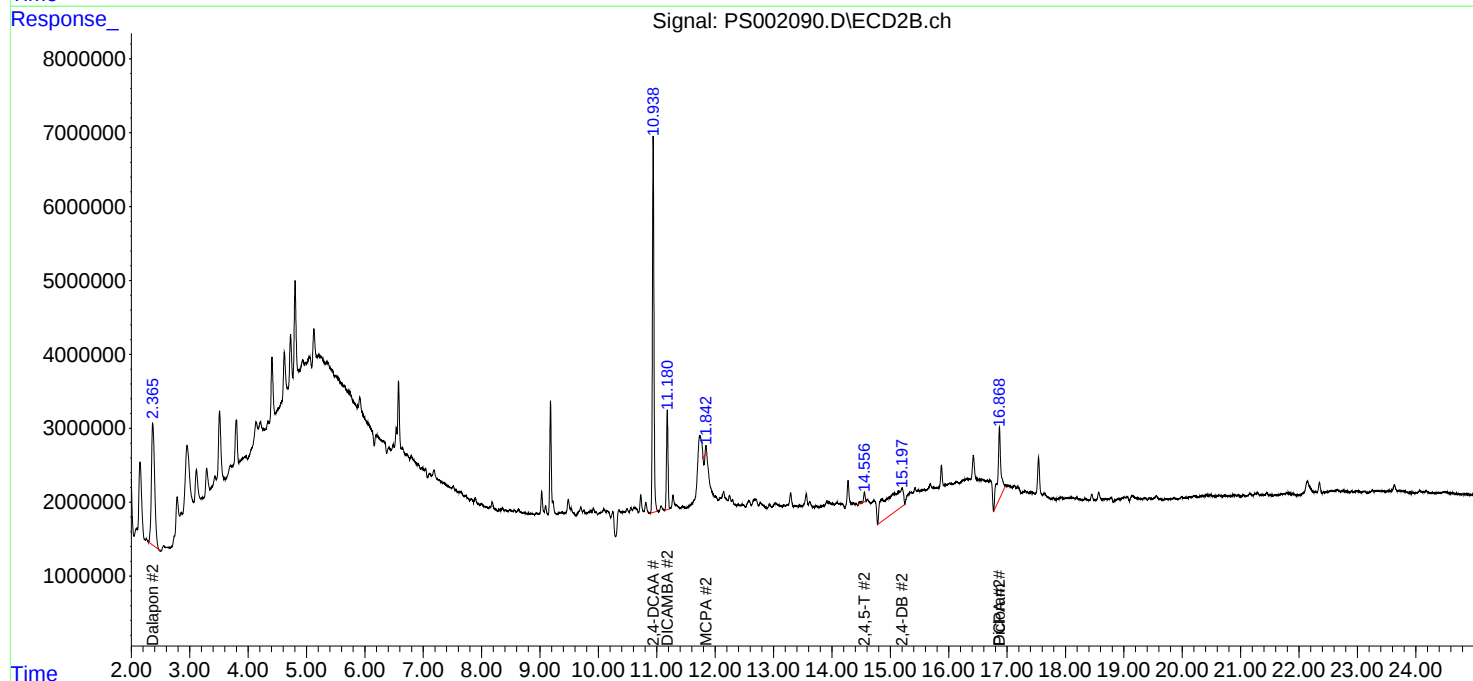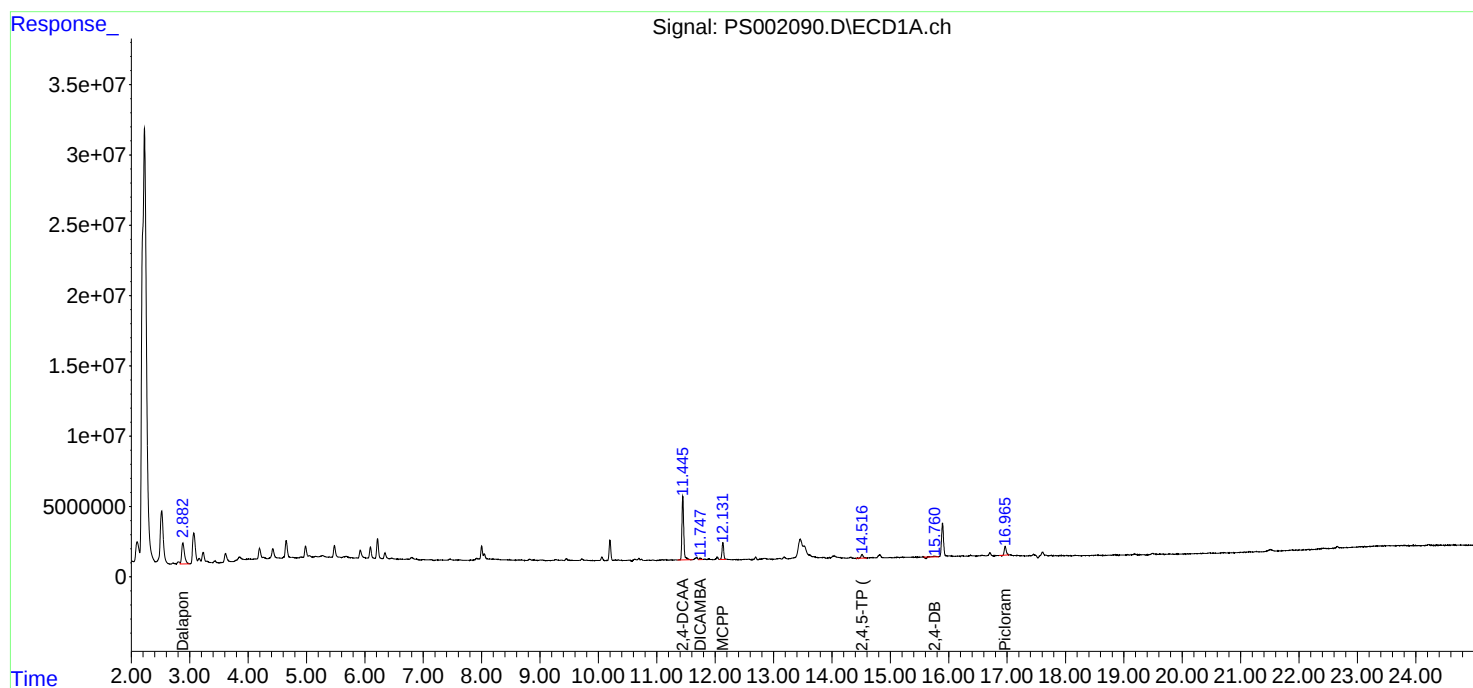


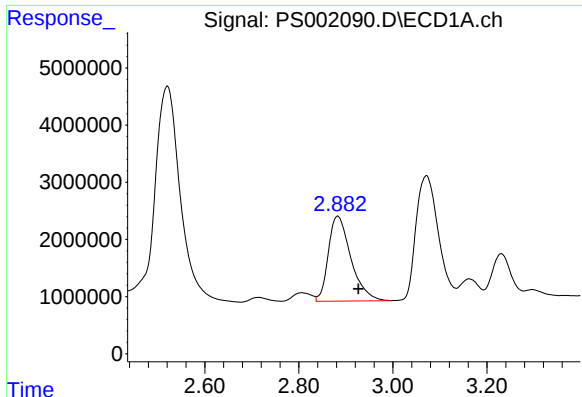

#1 Dalapon


R.T.: 2.882 min
Delta R.T.: -0.045 min
Response: 49635307
Conc: 162.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

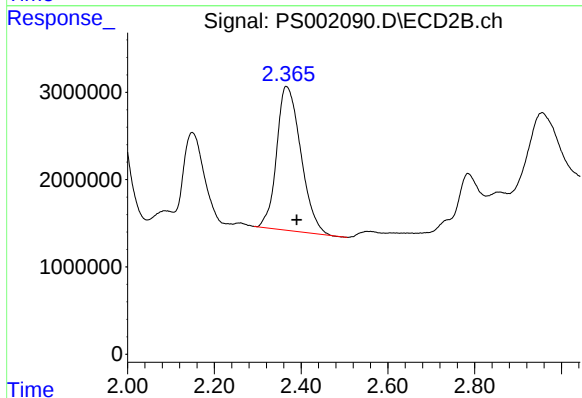


#1 Dalapon

R.T.: 2.365 min
Delta R.T.: -0.025 min
Response: 63759200
Conc: 218.38 ng/ml

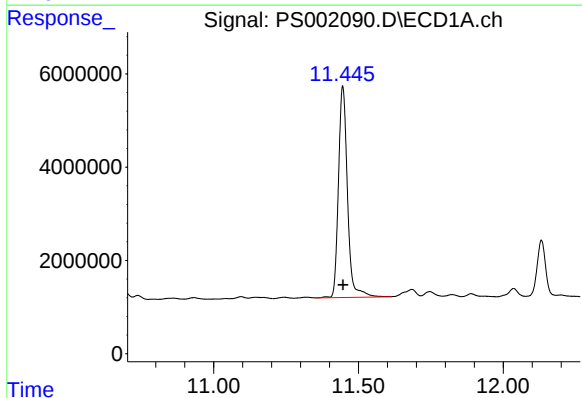


#4 2,4-DCAA

R.T.: 11.445 min
Delta R.T.: -0.001 min
Response: 98230203
Conc: 464.66 ng/ml

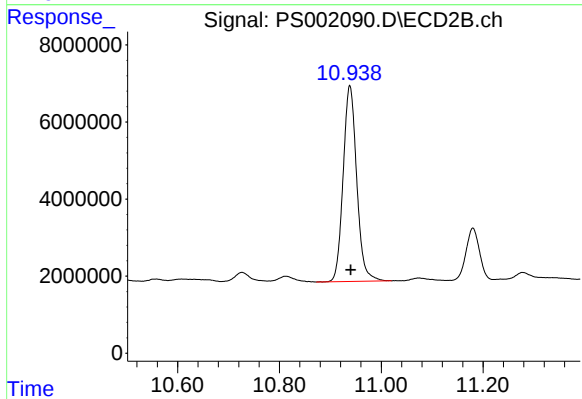

#4 2,4-DCAA


R.T.: 10.938 min
Delta R.T.: -0.002 min
Response: 94058447
Conc: 394.36 ng/ml

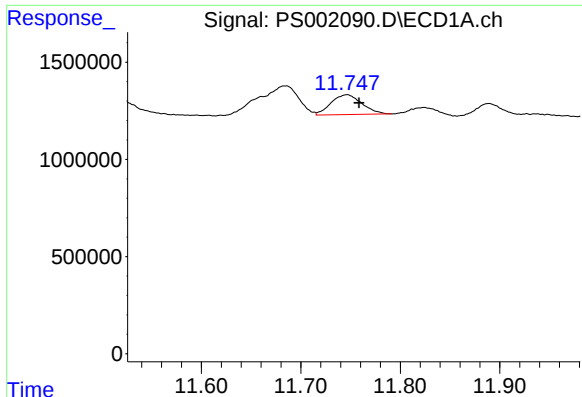

#5 DICAMBA


R.T.: 11.746 min
Delta R.T.: -0.012 min
Response: 2211143
Conc: 2.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

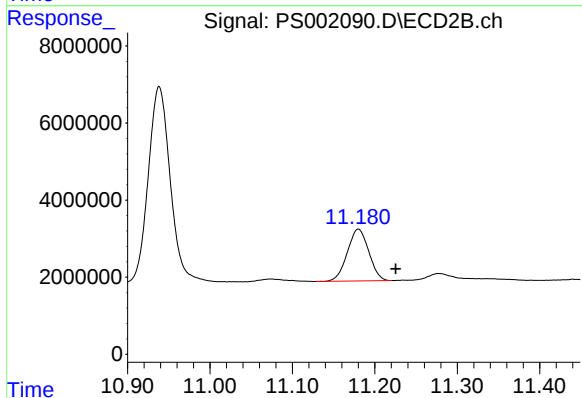


#5 DICAMBA

R.T.: 11.180 min
Delta R.T.: -0.045 min
Response: 24348545
Conc: 29.63 ng/ml

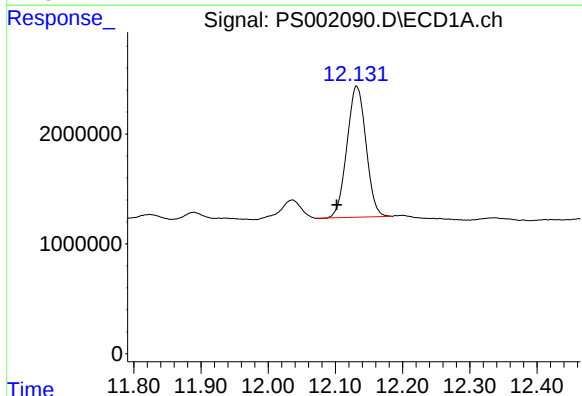


#6 MCP

R.T.: 12.132 min
Delta R.T.: 0.030 min
Response: 23505187
Conc: 41.98 ug/ml

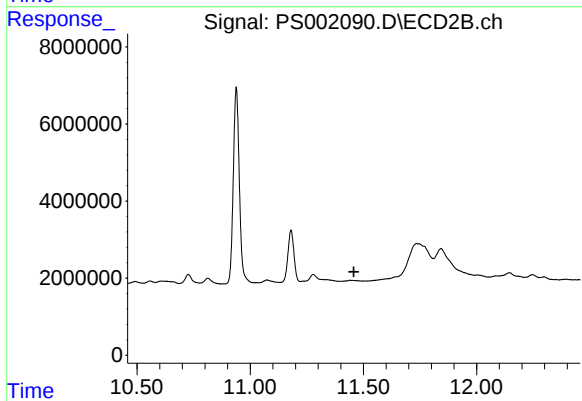

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.458 min
Response: 0
Conc: N.D.

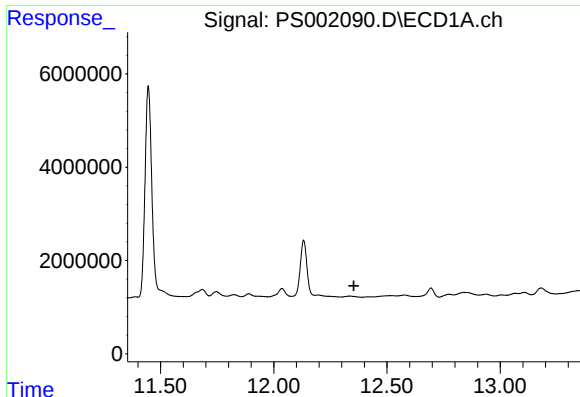

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

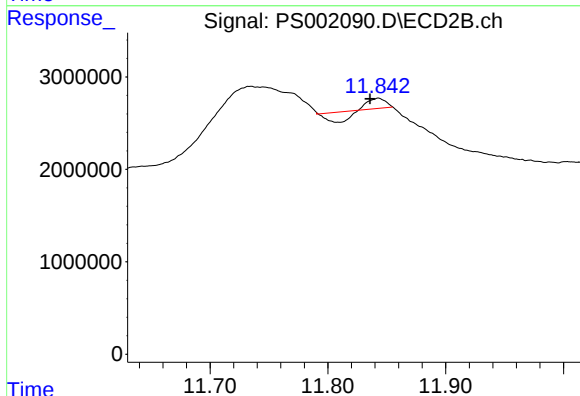


#7 MCPA

R.T.: 11.843 min
Delta R.T.: 0.007 min
Response: 33314
Conc: 0.04 ug/ml

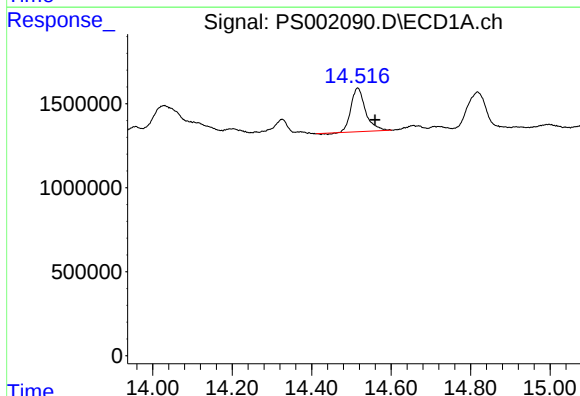


#11 2,4,5-TP (SILVEX)

R.T.: 14.516 min
Delta R.T.: -0.044 min
Response: 6585140
Conc: 6.02 ng/ml

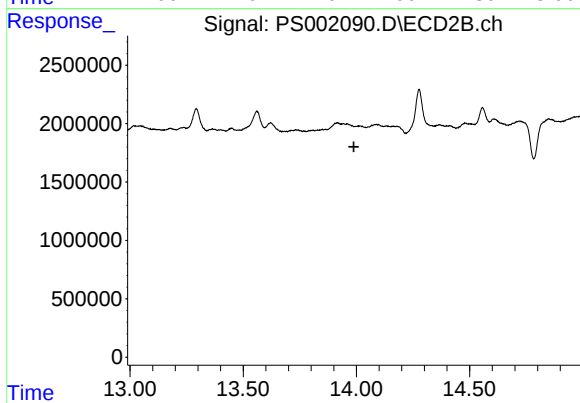

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 13.988 min
Response: 0
Conc: N.D.

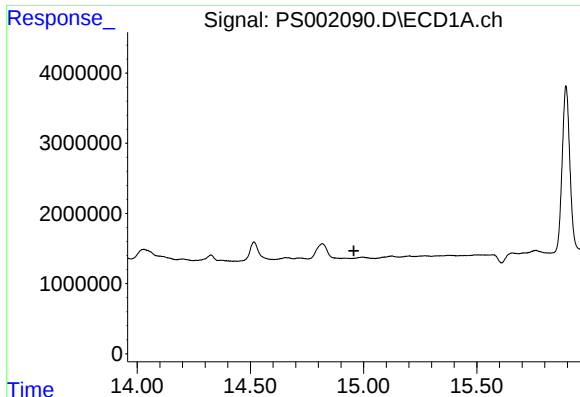

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

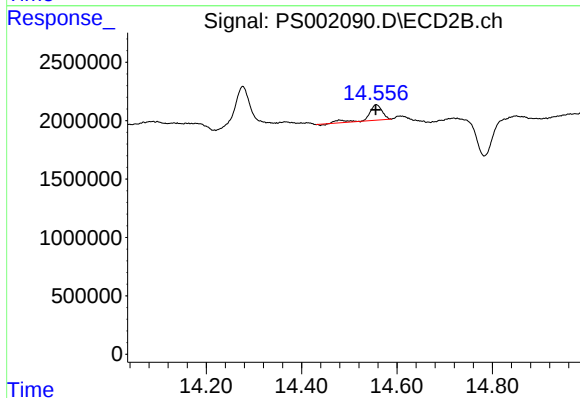


#12 2,4,5-T

R.T.: 14.557 min
Delta R.T.: 0.001 min
Response: 2631825
Conc: 2.40 ng/ml

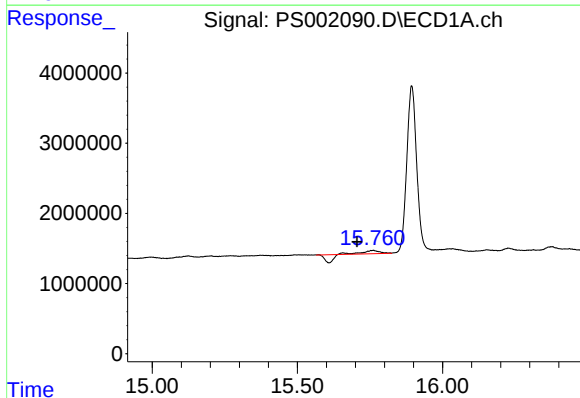


#13 2,4-DB

R.T.: 15.761 min
Delta R.T.: 0.056 min
Response: 30086
Conc: 0.19 ng/ml

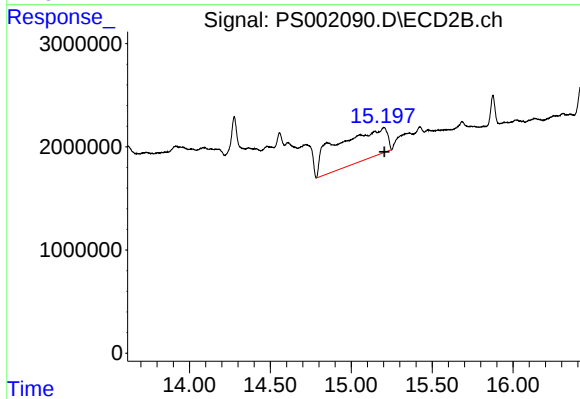

#13 2,4-DB


R.T.: 15.201 min
Delta R.T.: -0.004 min
Response: 64394933
Conc: 409.05 ng/ml

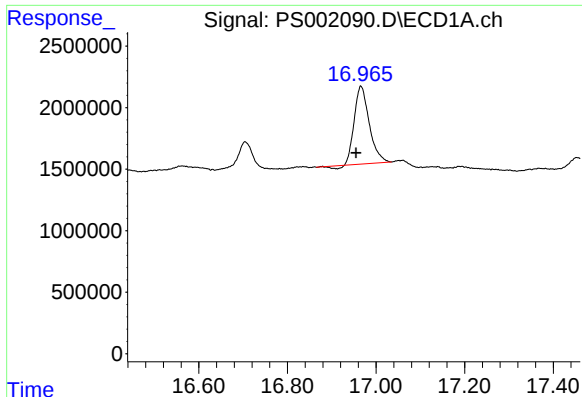

#15 Picloram


R.T.: 16.966 min
Delta R.T.: 0.011 min
Response: 14567425
Conc: 8.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

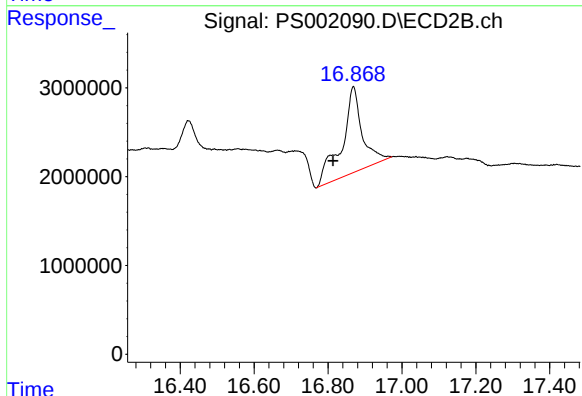


#15 Picloram

R.T.: 16.869 min
Delta R.T.: 0.055 min
Response: 37080064
Conc: 23.38 ng/ml

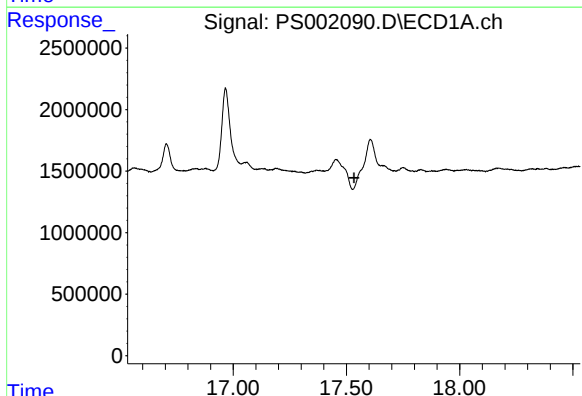

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.533 min
Response: 0
Conc: N.D.

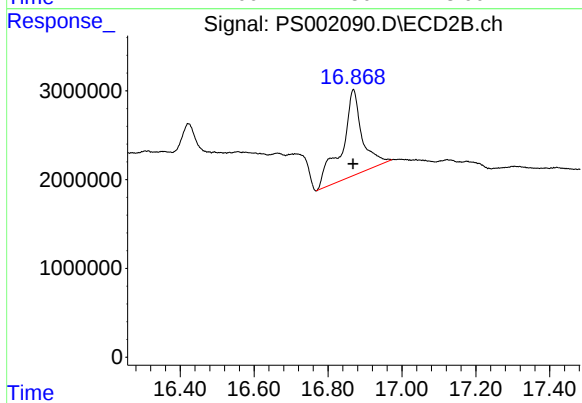

#16 DCPA

R.T.: 16.869 min
Delta R.T.: 0.000 min
Response: 37080064
Conc: 20.50 ng/ml