

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
 Data File : PS002091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2018 23:05
 Operator : EI\SJ
 Sample : J5605-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 01:02:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.447	10.938	111.5E6	104.9E6	527.597	439.863
Target Compounds							
1) T	Dalapon	2.883	2.365	52852163	77389724	173.197	265.063 #
5) T	DICAMBA	0.000	11.181	0	21712223	N.D.	26.424 #
6) T	MCPD	12.132	0.000	20091522	0	35.881	N.D. #
12) T	2,4,5-T	0.000	14.601	0	6218796	N.D.	5.678 #
15) T	Picloram	0.000	16.811	0	4408395	N.D.	2.779 #
16) T	DCPA	0.000	16.878	0	6675690	N.D.	3.690 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
Data File : PS002091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2018 23:05
Operator : EI\SJ
Sample : J5605-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 01:02:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

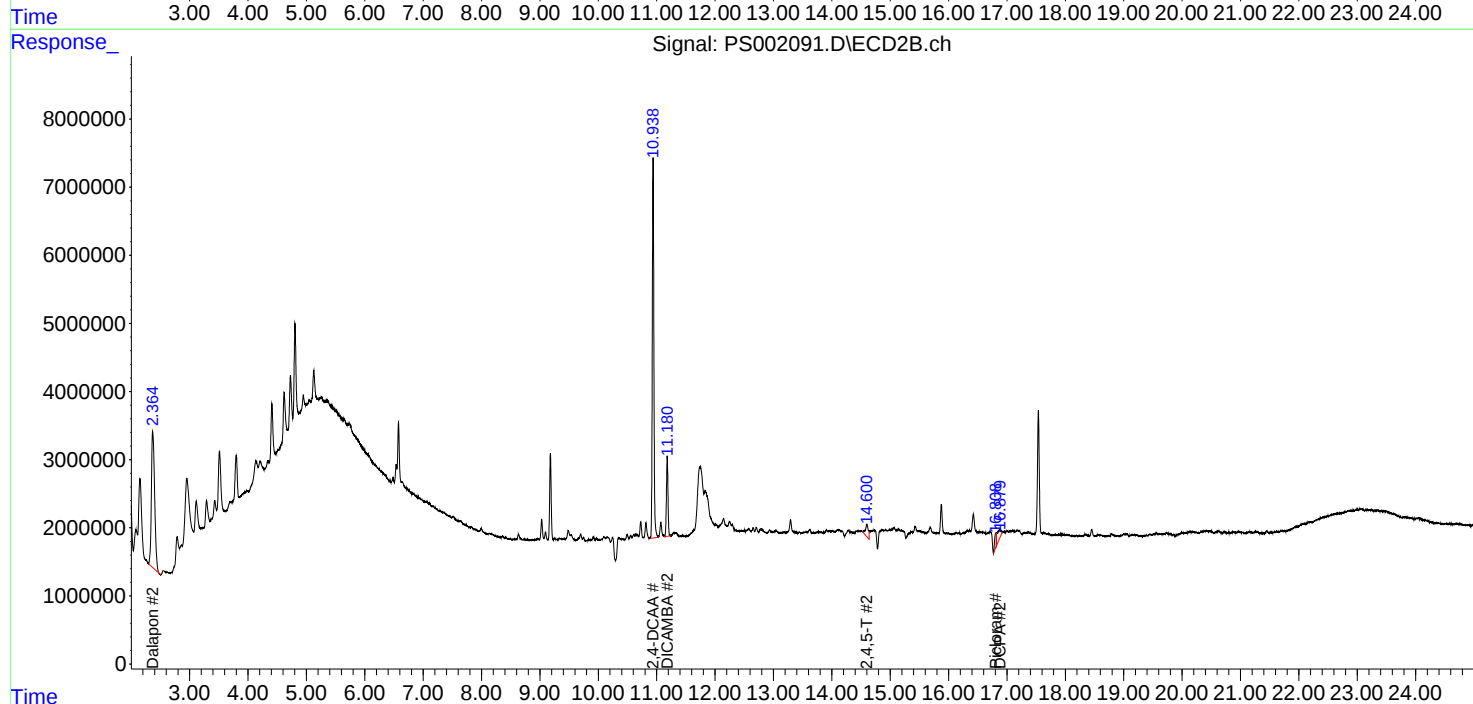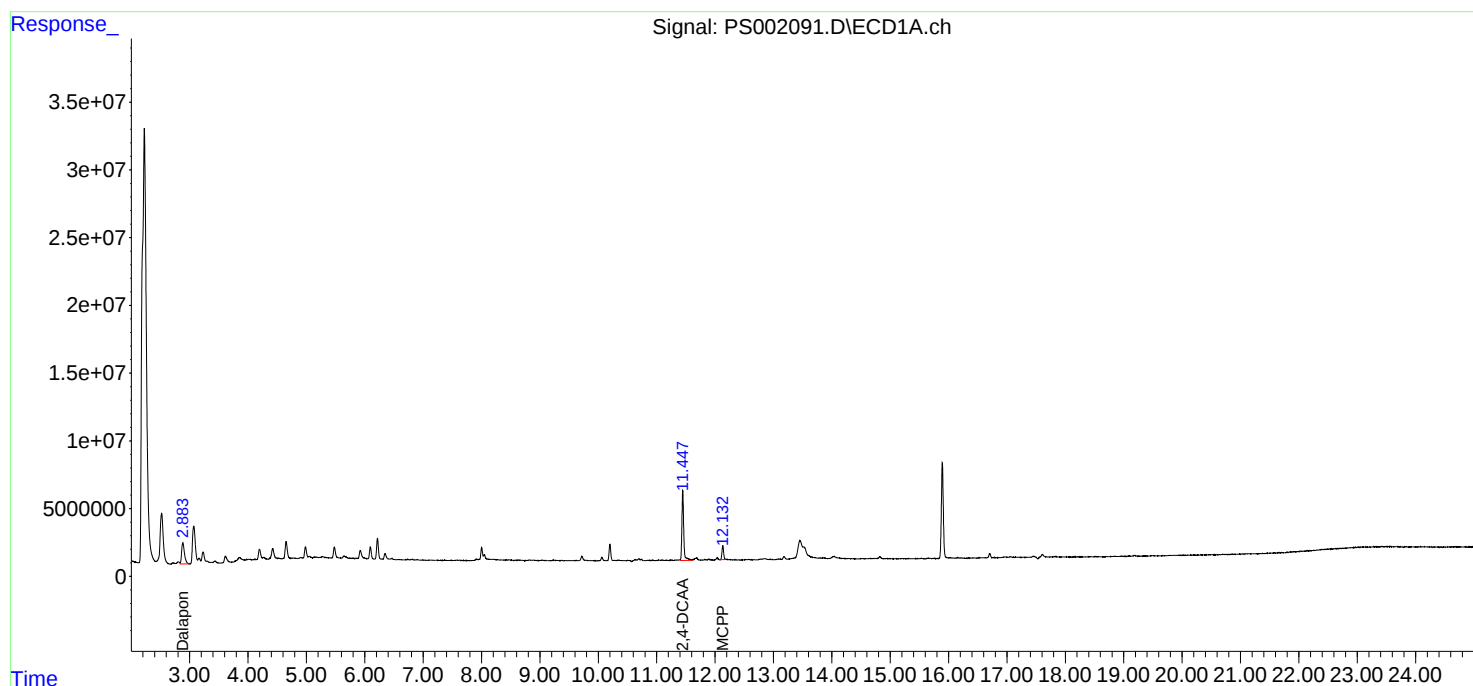


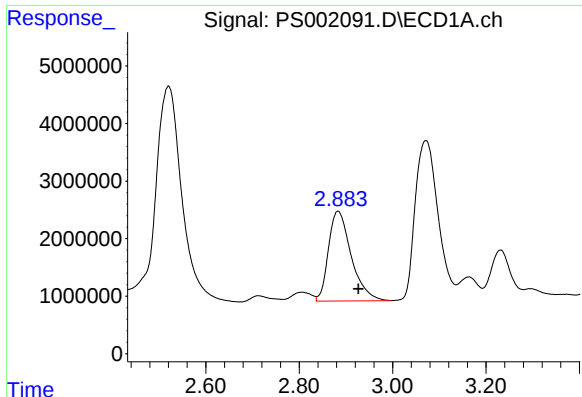

#1 Dalapon


R.T.: 2.883 min
Delta R.T.: -0.044 min
Response: 52852163
Conc: 173.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

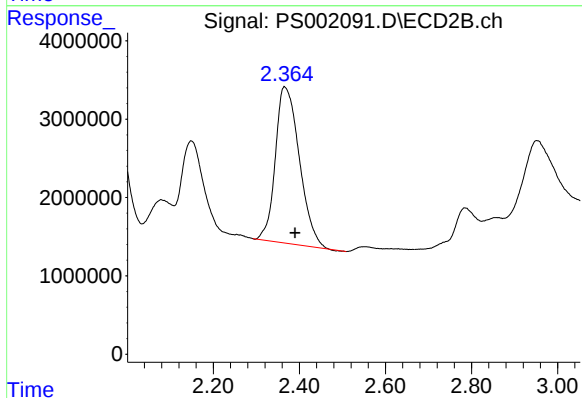


#1 Dalapon

R.T.: 2.365 min
Delta R.T.: -0.025 min
Response: 77389724
Conc: 265.06 ng/ml

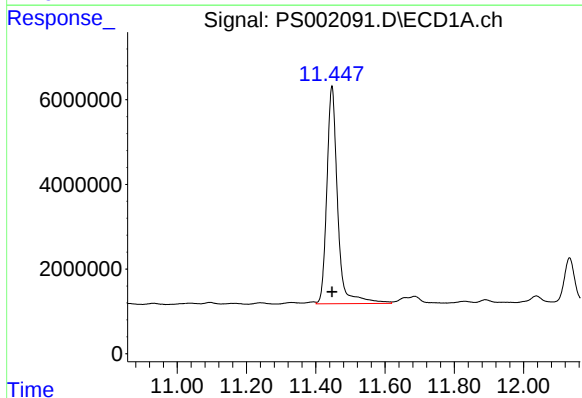


#4 2,4-DCAA

R.T.: 11.447 min
Delta R.T.: 0.000 min
Response: 111535194
Conc: 527.60 ng/ml

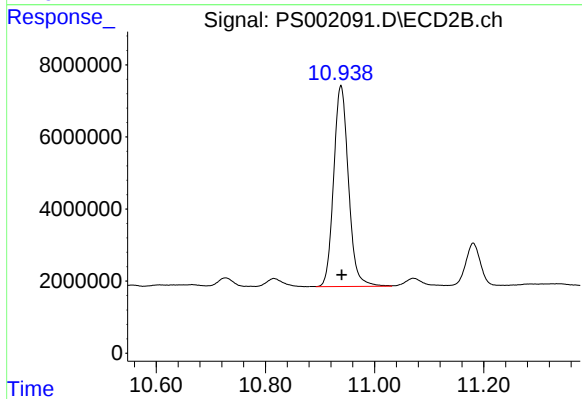

#4 2,4-DCAA


R.T.: 10.938 min
Delta R.T.: -0.002 min
Response: 104910491
Conc: 439.86 ng/ml

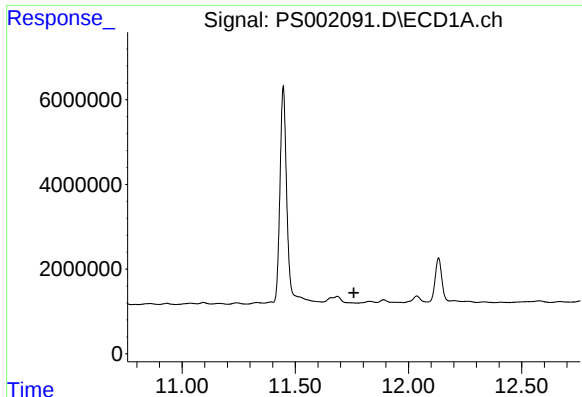

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.759 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

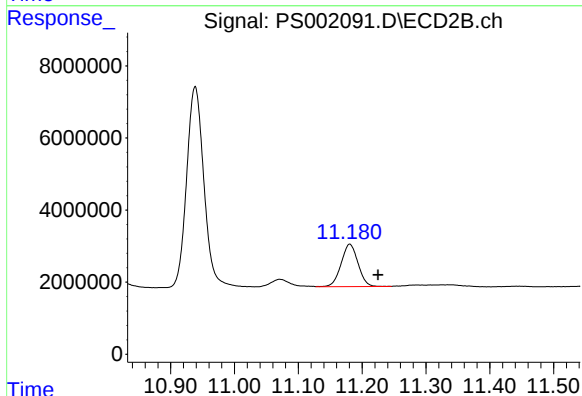


#5 DICAMBA

R.T.: 11.181 min
Delta R.T.: -0.045 min
Response: 21712223
Conc: 26.42 ng/ml

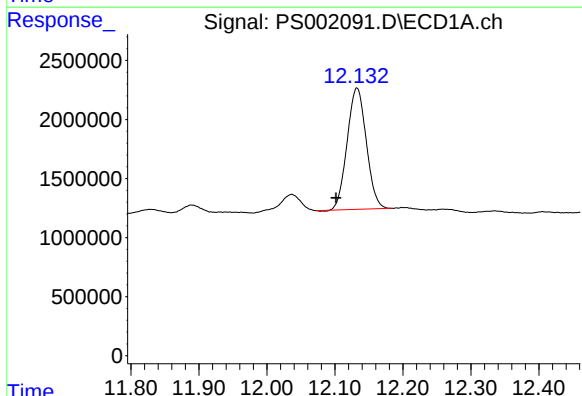


#6 MCP

R.T.: 12.132 min
Delta R.T.: 0.031 min
Response: 20091522
Conc: 35.88 ug/ml

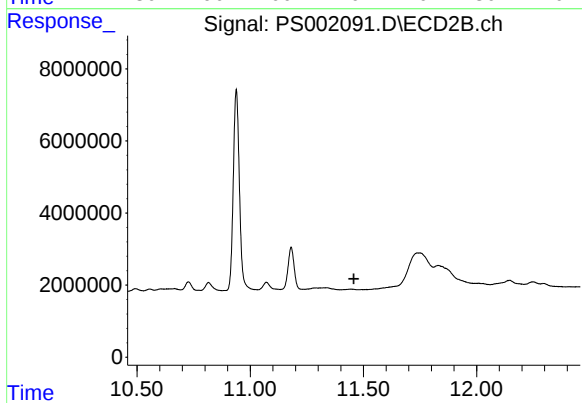

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.458 min
Response: 0
Conc: N.D.

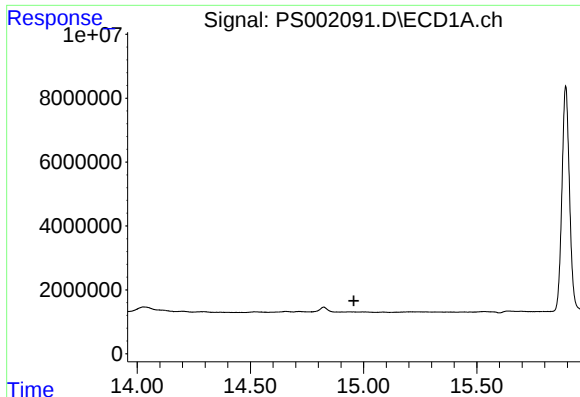

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

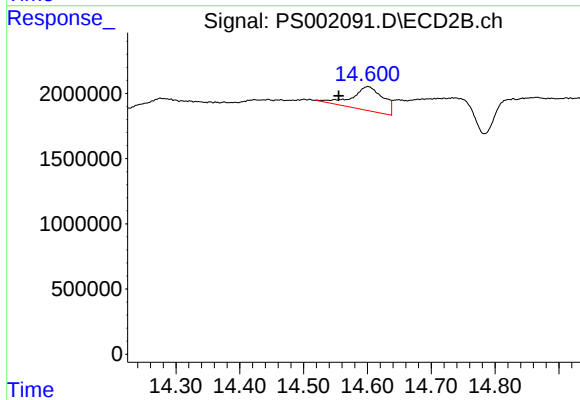


#12 2,4,5-T

R.T.: 14.601 min
Delta R.T.: 0.046 min
Response: 6218796
Conc: 5.68 ng/ml

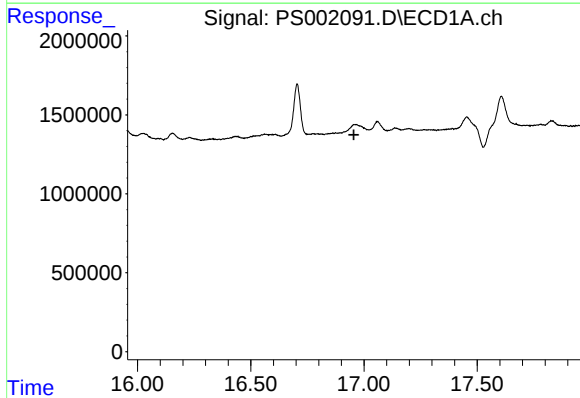


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.955 min
Response: 0
Conc: N.D.

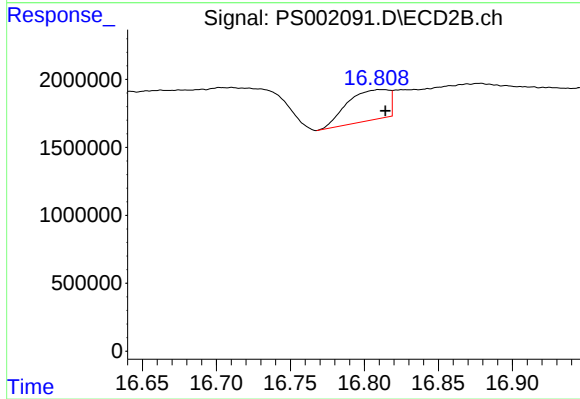

#15 Picloram


R.T.: 16.811 min
Delta R.T.: -0.003 min
Response: 4408395
Conc: 2.78 ng/ml

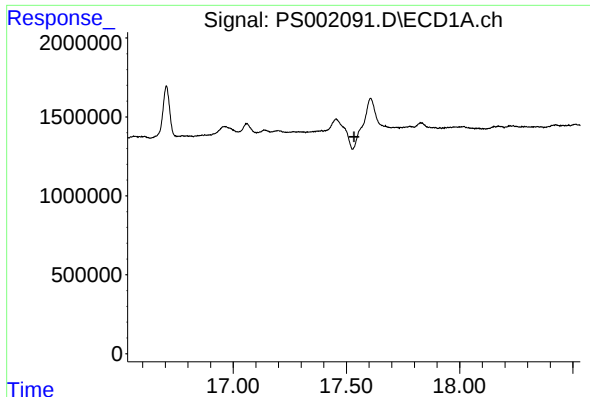

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.533 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

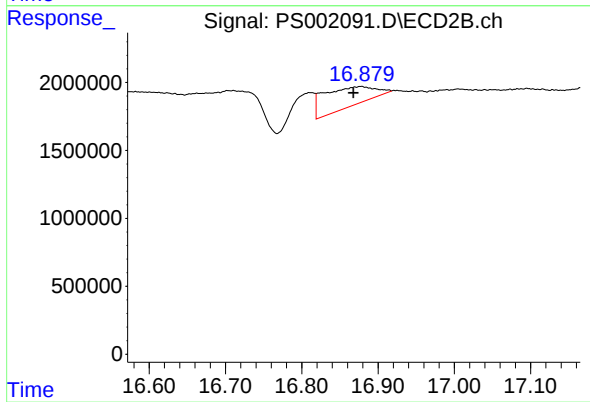

#16 DCPA

R.T.: 16.878 min
Delta R.T.: 0.010 min
Response: 6675690
Conc: 3.69 ng/ml