

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
 Data File : PS002094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2018 00:38
 Operator : EI\SJ
 Sample : J5622-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:34:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.447	10.939	71977489	71012486	340.477	297.737
Target Compounds							
1) T	Dalapon	2.882	2.366	49998737	74641161	163.846	255.649 #
2) T	3,5-DICHL...	0.000	9.095	0	773277	N.D.	2.644 #
5) T	DICAMBA	0.000	11.180	0	15192627	N.D.	18.489 #
6) T	MCP	12.132	0.000	15094699	0	26.957	N.D. #
11) T	2,4,5-TP ...	14.521	0.000	3192186	0	2.918	N.D. #
12) T	2,4,5-T	0.000	14.599	0	2719618	N.D.	2.483 #
13) T	2,4-DB	0.000	15.145	0	2200174	N.D.	13.976 #
14) T	DINOSEB	0.000	15.690	0	4290011	N.D.	4.851 #
15) T	Picloram	16.950	16.804	3004768	6241707	1.757	3.935 #
16) T	DCPA	0.000	16.804	0	6241707	N.D.	3.450 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
Data File : PS002094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2018 00:38
Operator : EI\SJ
Sample : J5622-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:34:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

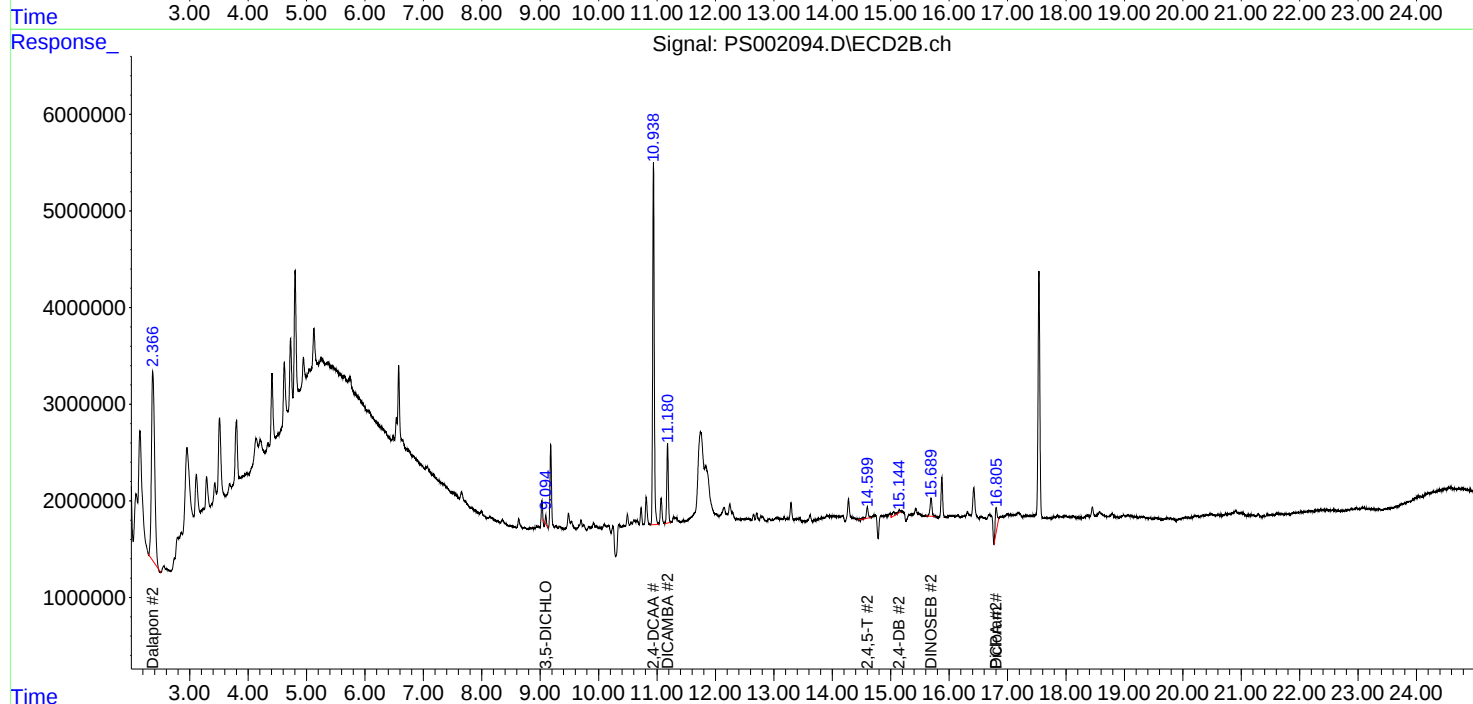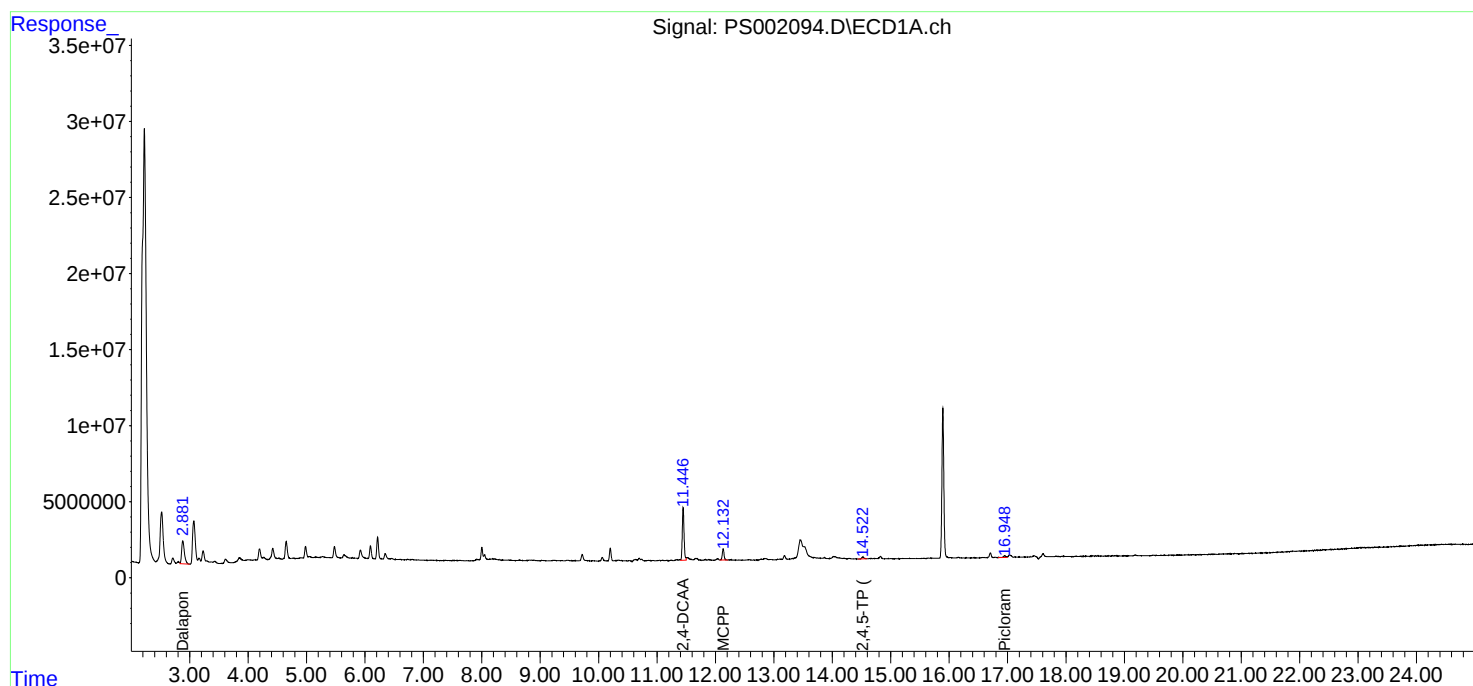


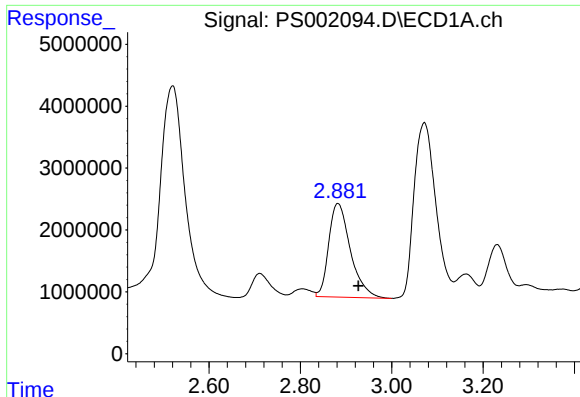

#1 Dalapon


R.T.: 2.882 min
Delta R.T.: -0.045 min
Response: 49998737
Conc: 163.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

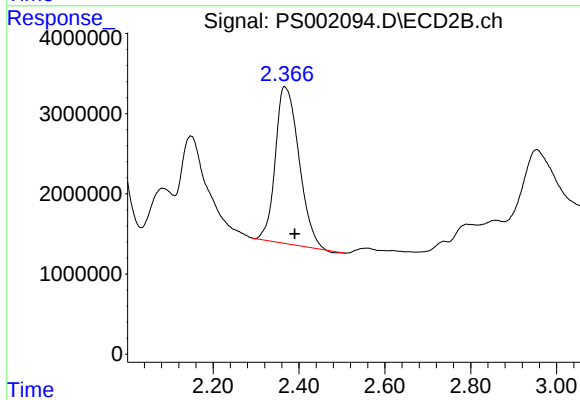


#1 Dalapon

R.T.: 2.366 min
Delta R.T.: -0.024 min
Response: 74641161
Conc: 255.65 ng/ml

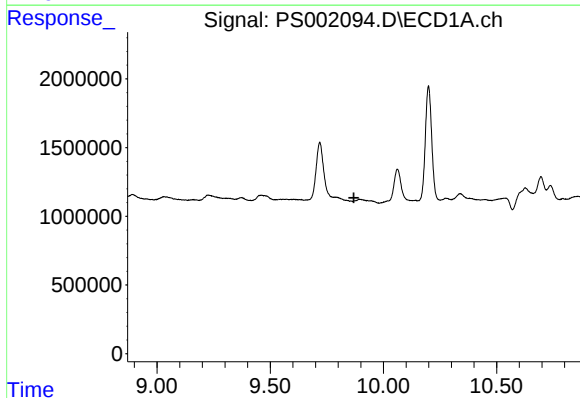


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

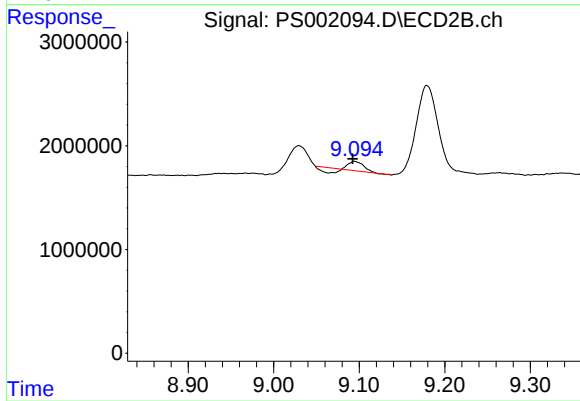

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.095 min
Delta R.T.: 0.002 min
Response: 773277
Conc: 2.64 ng/ml

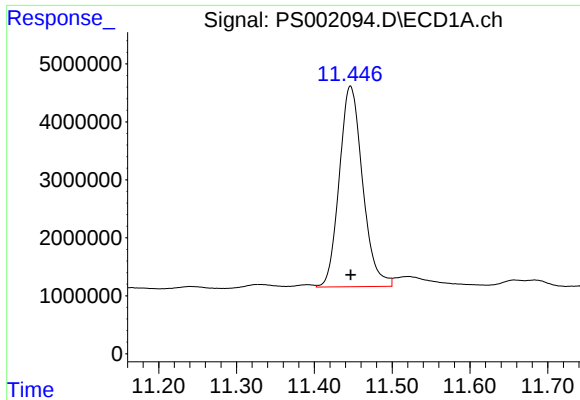

#4 2,4-DCAA


R.T.: 11.447 min
Delta R.T.: 0.000 min
Response: 71977489
Conc: 340.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

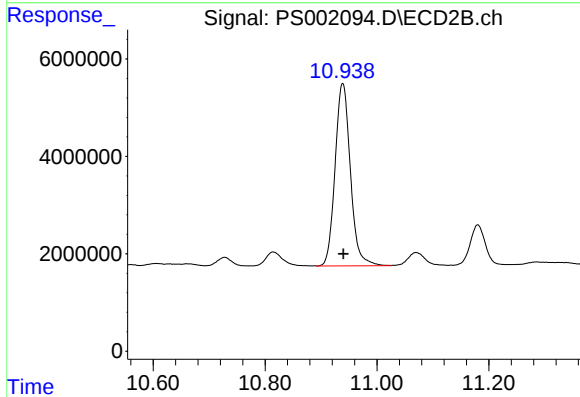


#4 2,4-DCAA

R.T.: 10.939 min
Delta R.T.: -0.001 min
Response: 71012486
Conc: 297.74 ng/ml

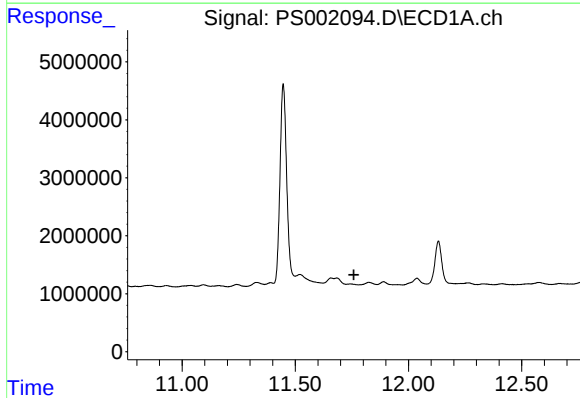


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.759 min
Response: 0
Conc: N.D.

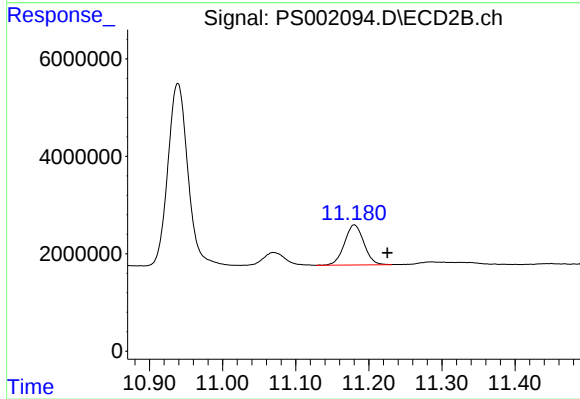

#5 DICAMBA


R.T.: 11.180 min
Delta R.T.: -0.045 min
Response: 15192627
Conc: 18.49 ng/ml

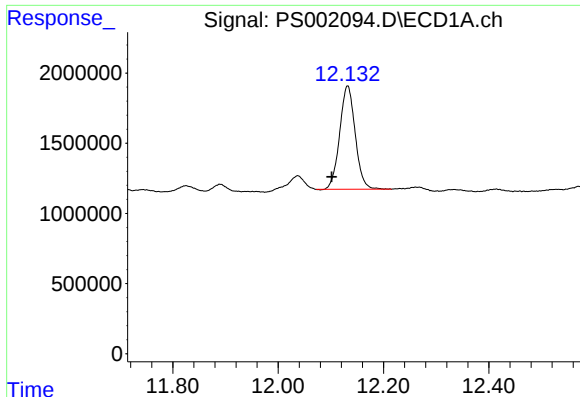

#6 MCP


R.T.: 12.132 min
Delta R.T.: 0.030 min
Response: 15094699
Conc: 26.96 ug/ml

Instrument :
ECD_S
ClientSampleId :

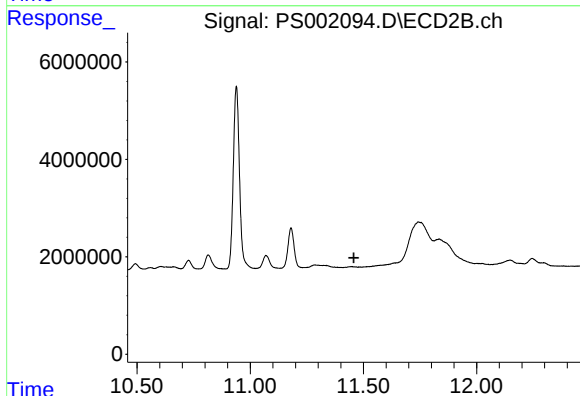


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.458 min
Response: 0
Conc: N.D.

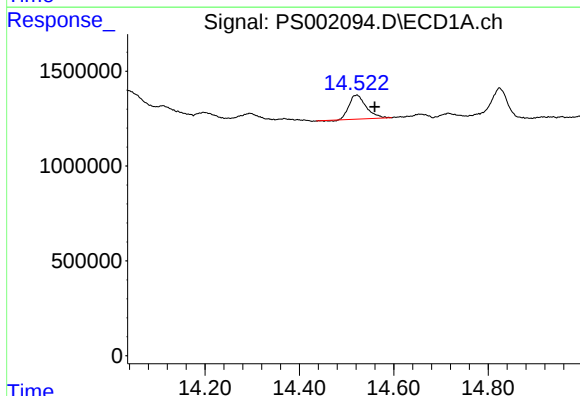


#11 2,4,5-TP (SILVEX)

R.T.: 14.521 min
Delta R.T.: -0.039 min
Response: 3192186
Conc: 2.92 ng/ml

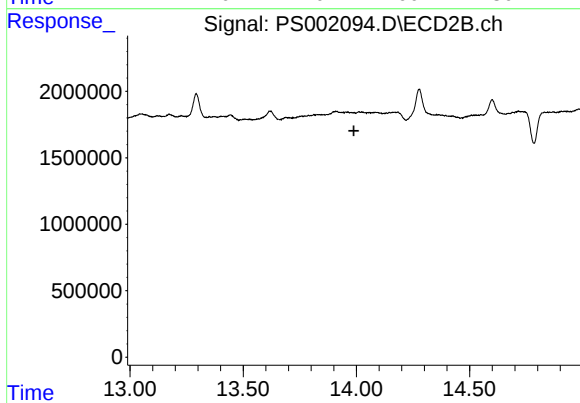

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 13.988 min
Response: 0
Conc: N.D.

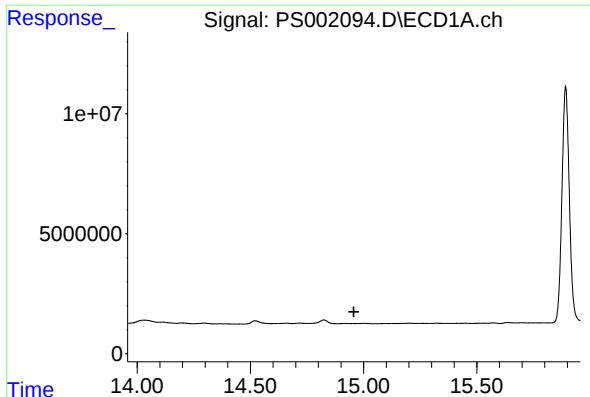

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

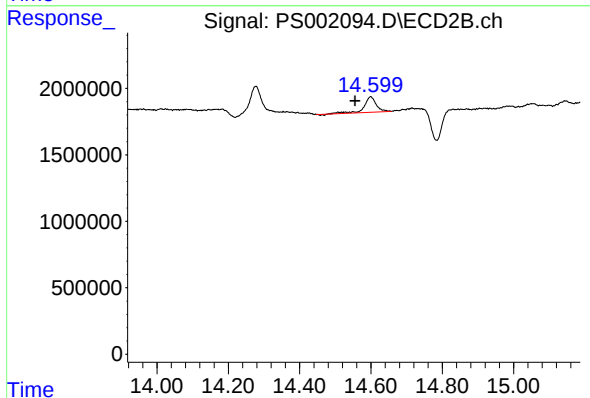


#12 2,4,5-T

R.T.: 14.599 min
Delta R.T.: 0.044 min
Response: 2719618
Conc: 2.48 ng/ml

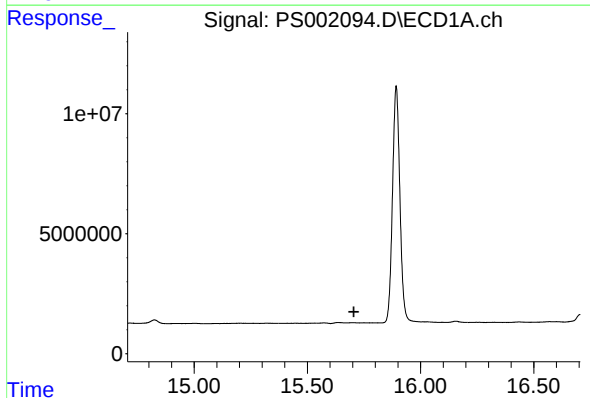


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.705 min
Response: 0
Conc: N.D.

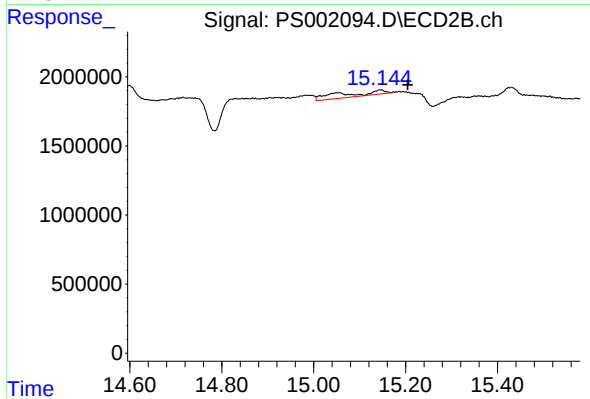

#13 2,4-DB


R.T.: 15.145 min
Delta R.T.: -0.060 min
Response: 2200174
Conc: 13.98 ng/ml

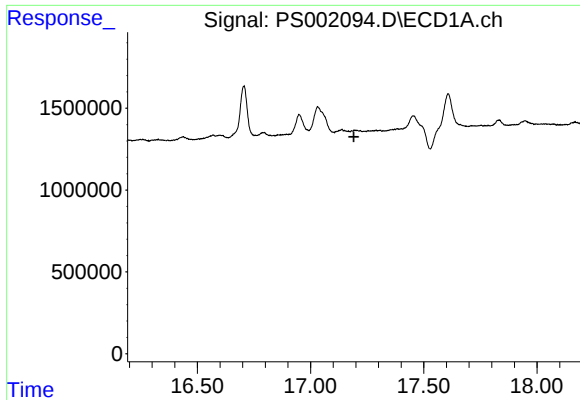

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.192 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

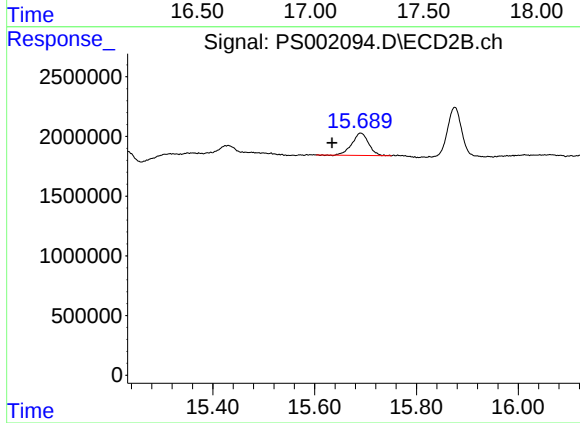


#14 DINOSEB

R.T.: 15.690 min
Delta R.T.: 0.056 min
Response: 4290011
Conc: 4.85 ng/ml

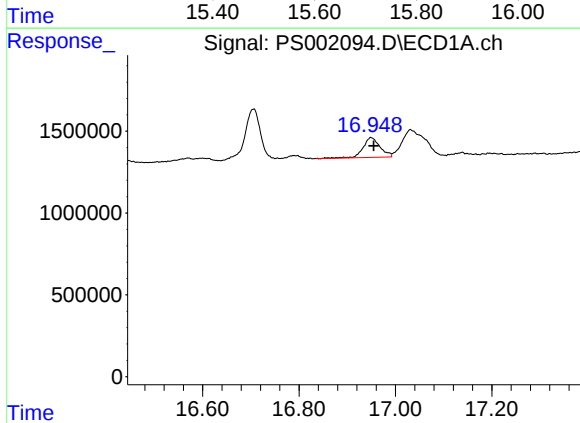


#15 Picloram

R.T.: 16.950 min
Delta R.T.: -0.005 min
Response: 3004768
Conc: 1.76 ng/ml

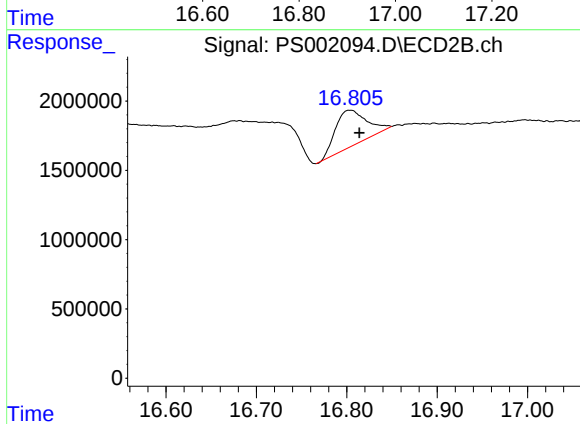

#15 Picloram


R.T.: 16.804 min
Delta R.T.: -0.010 min
Response: 6241707
Conc: 3.93 ng/ml

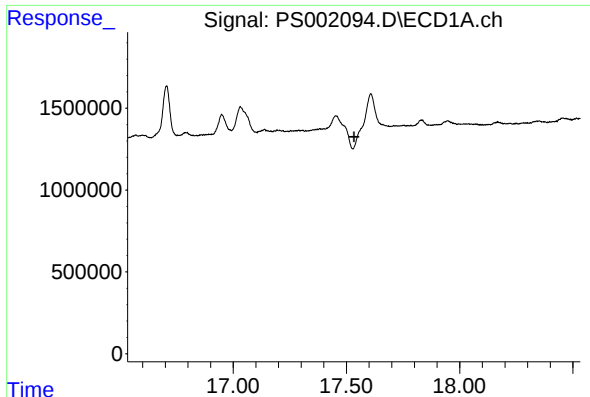

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.533 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

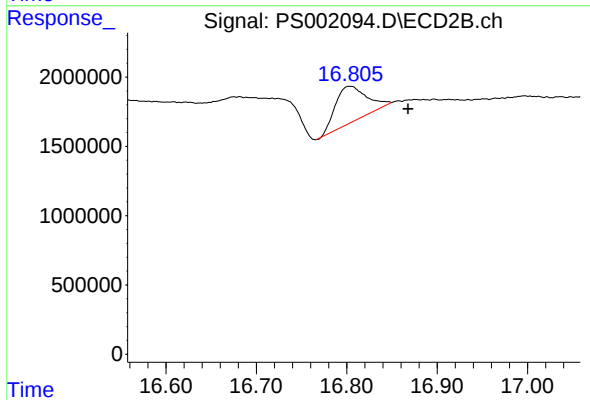

#16 DCPA

R.T.: 16.804 min
Delta R.T.: -0.064 min
Response: 6241707
Conc: 3.45 ng/ml