

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
 Data File : PS002095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2018 01:09
 Operator : EI\SJ
 Sample : J5622-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:34:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.459	10.951	80850518	74303772	382.449	311.537
Target Compounds							
1) T	Dalapon	2.896	2.378	41498149	48149697	135.989	164.915
2) T	3,5-DICHL...	0.000	9.042	0	3028815	N.D.	10.357 #
5) T	DICAMBA	11.762	11.193	1405957	20630376	1.786	25.107 #
6) T	MCP	12.145	0.000	19145780	0	34.192	N.D. #
10) T	Pentachlo...	0.000	13.306	0	3494246	N.D.	1.104 #
11) T	2,4,5-TP ...	14.531	0.000	21961259	0	20.077	N.D. #
13) T	2,4-DB	15.665	15.156	1044492	-991325	6.650	N.D. #
14) T	DINOSEB	0.000	15.698	0	3053965	N.D.	3.453 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102318\
Data File : PS002095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2018 01:09
Operator : EI\SJ
Sample : J5622-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:34:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

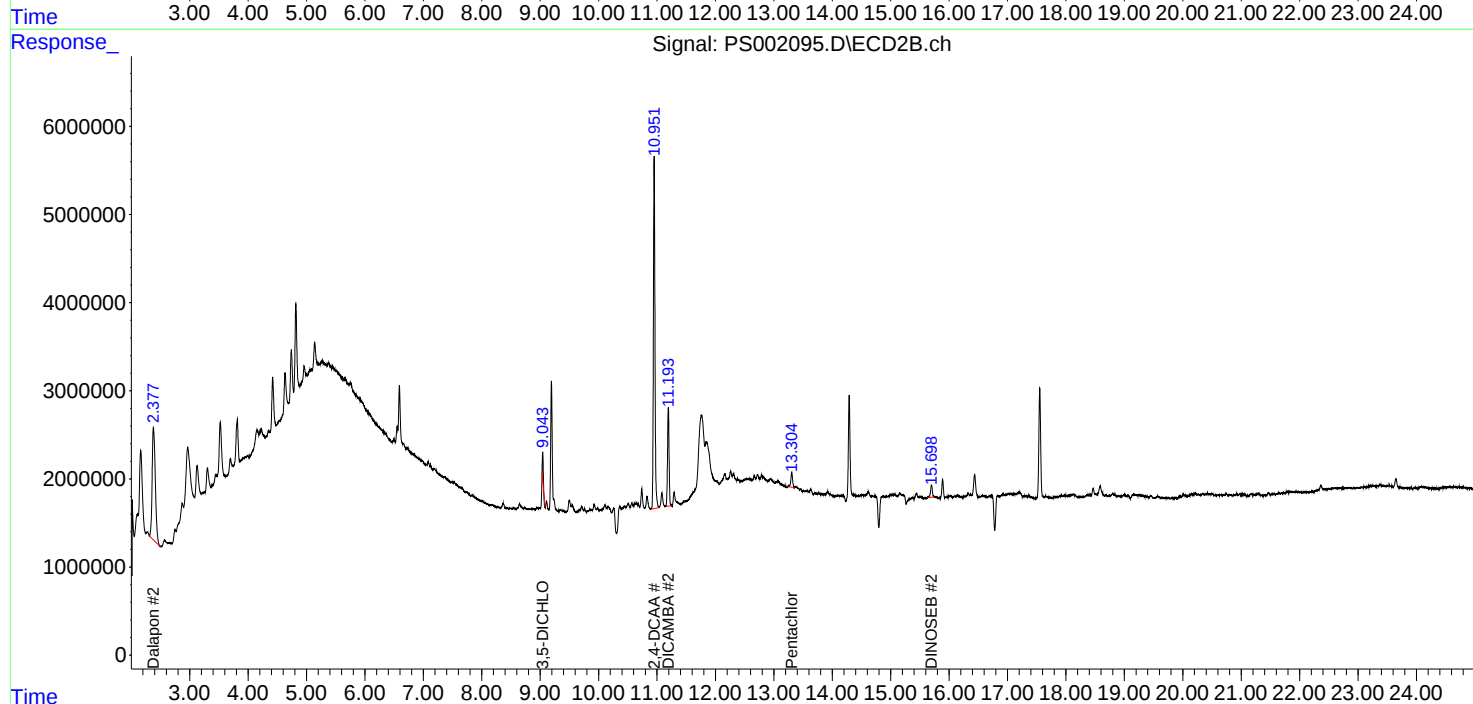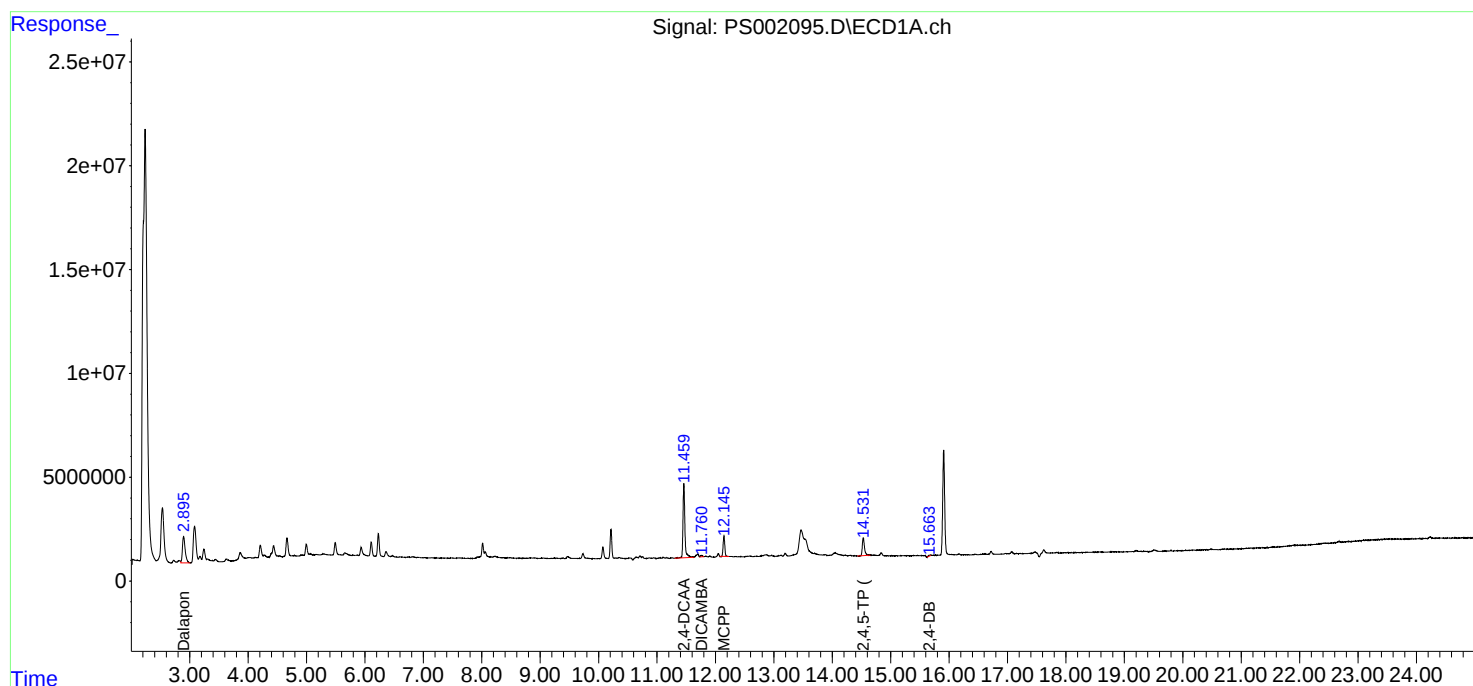


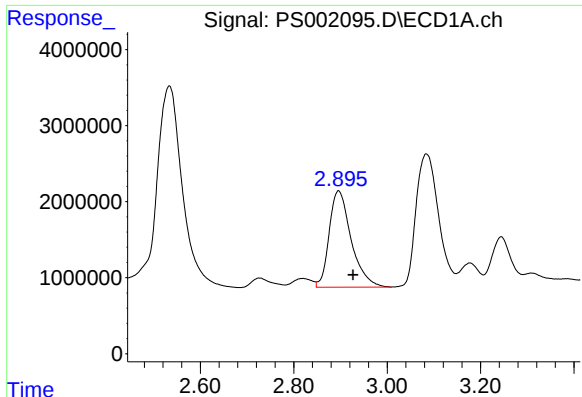

#1 Dalapon


R.T.: 2.896 min
Delta R.T.: -0.031 min
Response: 41498149
Conc: 135.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

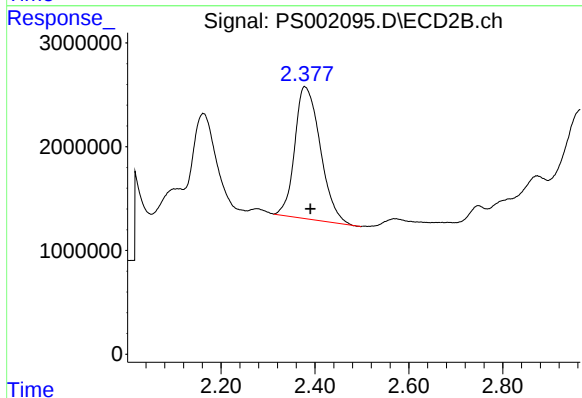


#1 Dalapon

R.T.: 2.378 min
Delta R.T.: -0.013 min
Response: 48149697
Conc: 164.91 ng/ml

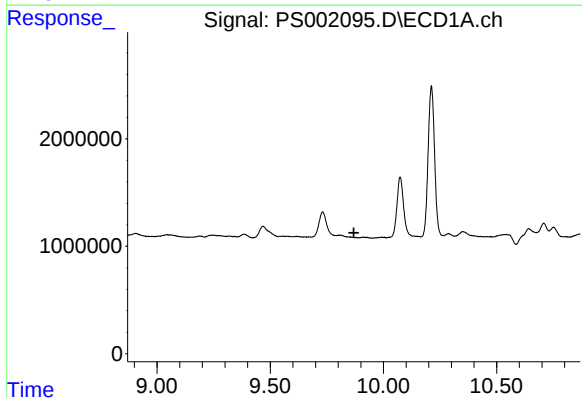


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

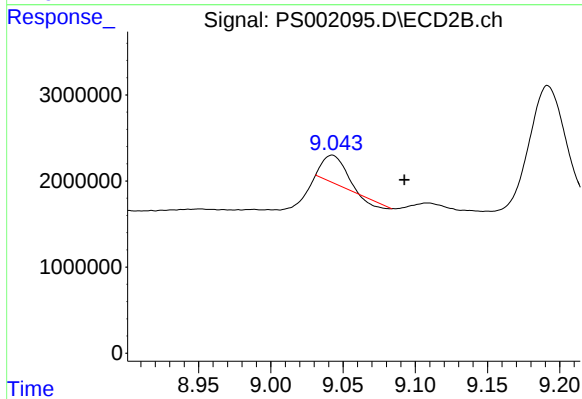

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.042 min
Delta R.T.: -0.050 min
Response: 3028815
Conc: 10.36 ng/ml

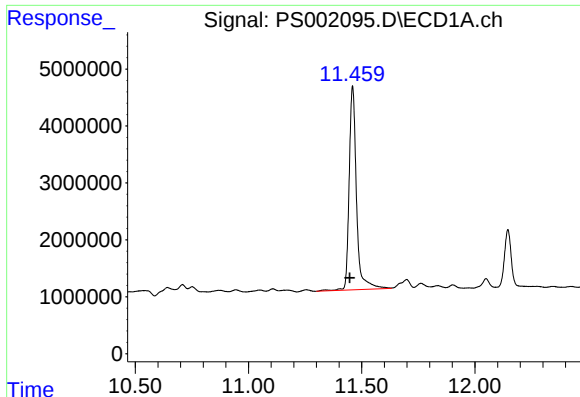

#4 2,4-DCAA


R.T.: 11.459 min
Delta R.T.: 0.013 min
Response: 80850518
Conc: 382.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

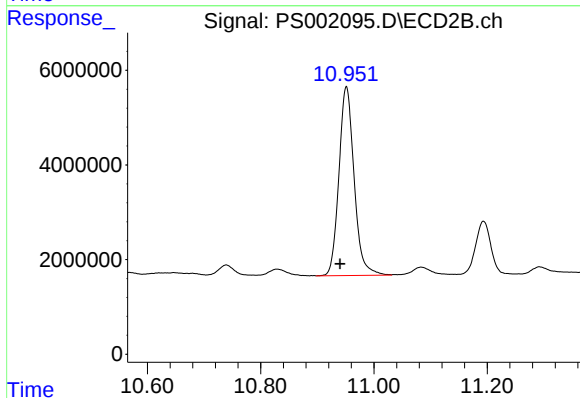


#4 2,4-DCAA

R.T.: 10.951 min
Delta R.T.: 0.011 min
Response: 74303772
Conc: 311.54 ng/ml

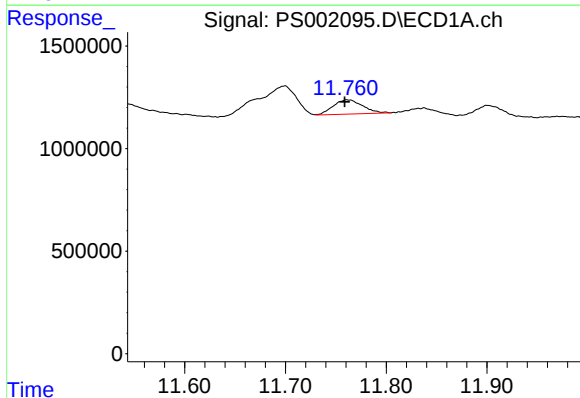


#5 DICAMBA

R.T.: 11.762 min
Delta R.T.: 0.003 min
Response: 1405957
Conc: 1.79 ng/ml

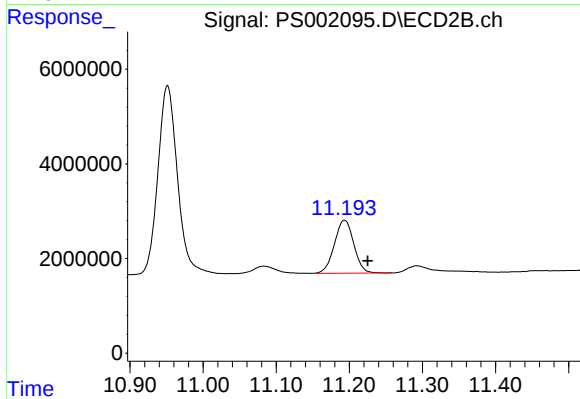

#5 DICAMBA


R.T.: 11.193 min
Delta R.T.: -0.032 min
Response: 20630376
Conc: 25.11 ng/ml

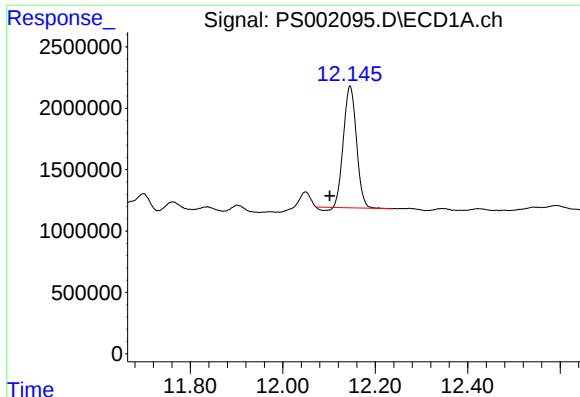

#6 MCP


R.T.: 12.145 min
Delta R.T.: 0.044 min
Response: 19145780
Conc: 34.19 ug/ml

Instrument :
ECD_S
ClientSampleId :

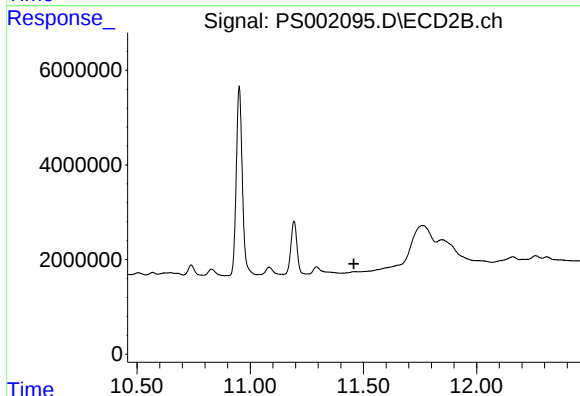


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.458 min
Response: 0
Conc: N.D.

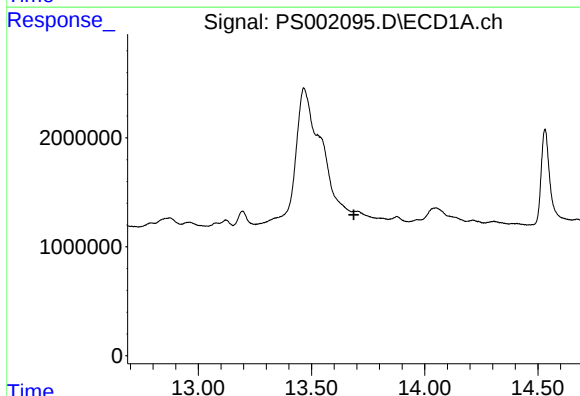


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.687 min
Response: 0
Conc: N.D.

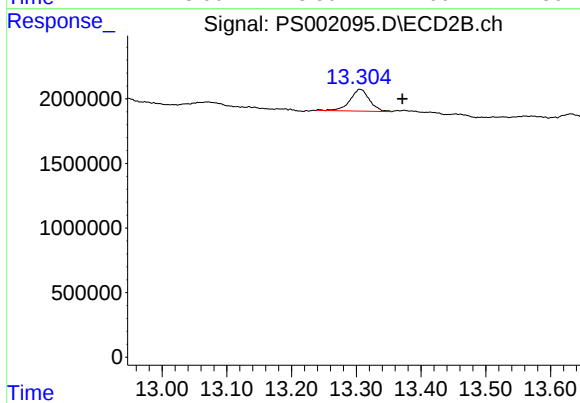

#10 Pentachlorophenol


R.T.: 13.306 min
Delta R.T.: -0.065 min
Response: 3494246
Conc: 1.10 ng/ml

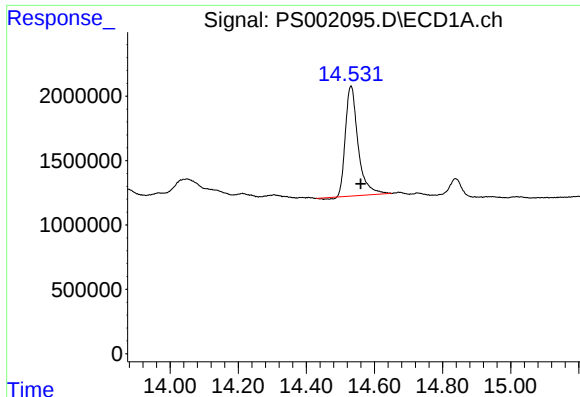

#11 2,4,5-TP (SILVEX)


R.T.: 14.531 min
Delta R.T.: -0.029 min
Response: 21961259
Conc: 20.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

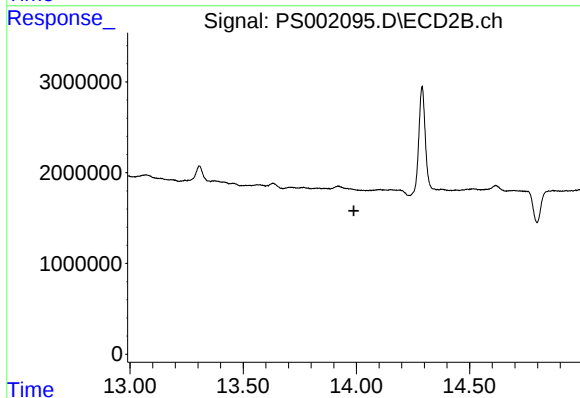


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.988 min
Response: 0
Conc: N.D.

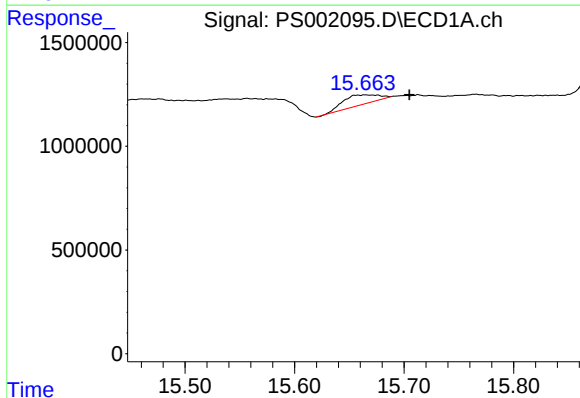


#13 2,4-DB

R.T.: 15.665 min
Delta R.T.: -0.040 min
Response: 1044492
Conc: 6.65 ng/ml

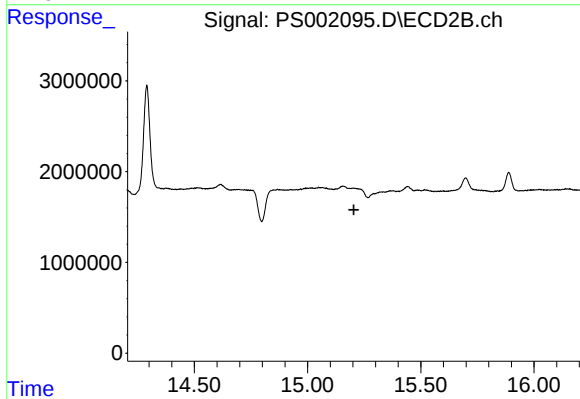

#13 2,4-DB


R.T.: 15.156 min
Delta R.T.: -0.049 min
Response: -991325
Conc: N.D.

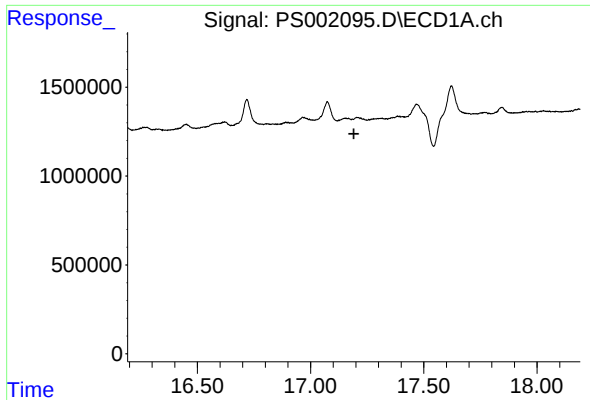

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.192 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

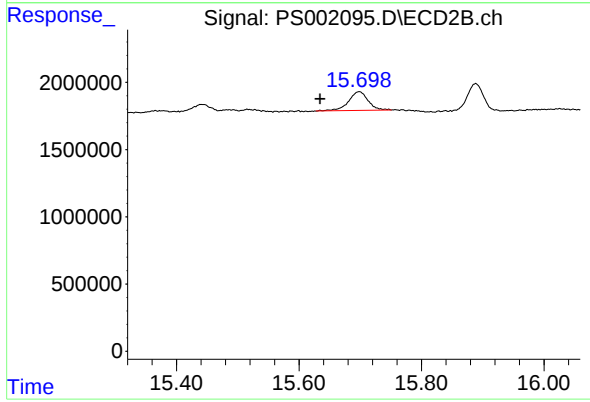

#14 DINOSEB

R.T.: 15.698 min
Delta R.T.: 0.064 min
Response: 3053965
Conc: 3.45 ng/ml