

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102319\
 Data File : PS007270.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 17:31
 Operator : SM\AJ
 Sample : K5139-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 22:52:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.465	5.194	512.1E6	289.7E6	374.130	411.875
Target Compounds							
1) T	Dalapon	2.020	1.733	100.9E6	167.9E6	60.300	184.479 #
2) T	3,5-DICHL...	0.000	4.482	0	8707267	N.D.	10.120
5) T	DICAMBA	5.557	5.331	51167180	8388140	10.414	3.224 #
6) T	MCP	0.000	5.331	0	8388140	N.D.	4.422
7) T	MCPA	0.000	5.513	0	45100975	N.D.	15.514
9) T	2,4-D	0.000	6.038	0	21767497	N.D.	27.285
10) T	Pentachlo...	0.000	6.409	0	22633326	N.D.	2.354
11) T	2,4,5-TP ...	0.000	6.793	0	44048888	N.D.	11.581
12) T	2,4,5-T	7.434	0.000	104.2E6	0	13.625	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102319\
Data File : PS007270.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 17:31
Operator : SM\AJ
Sample : K5139-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 22:52:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

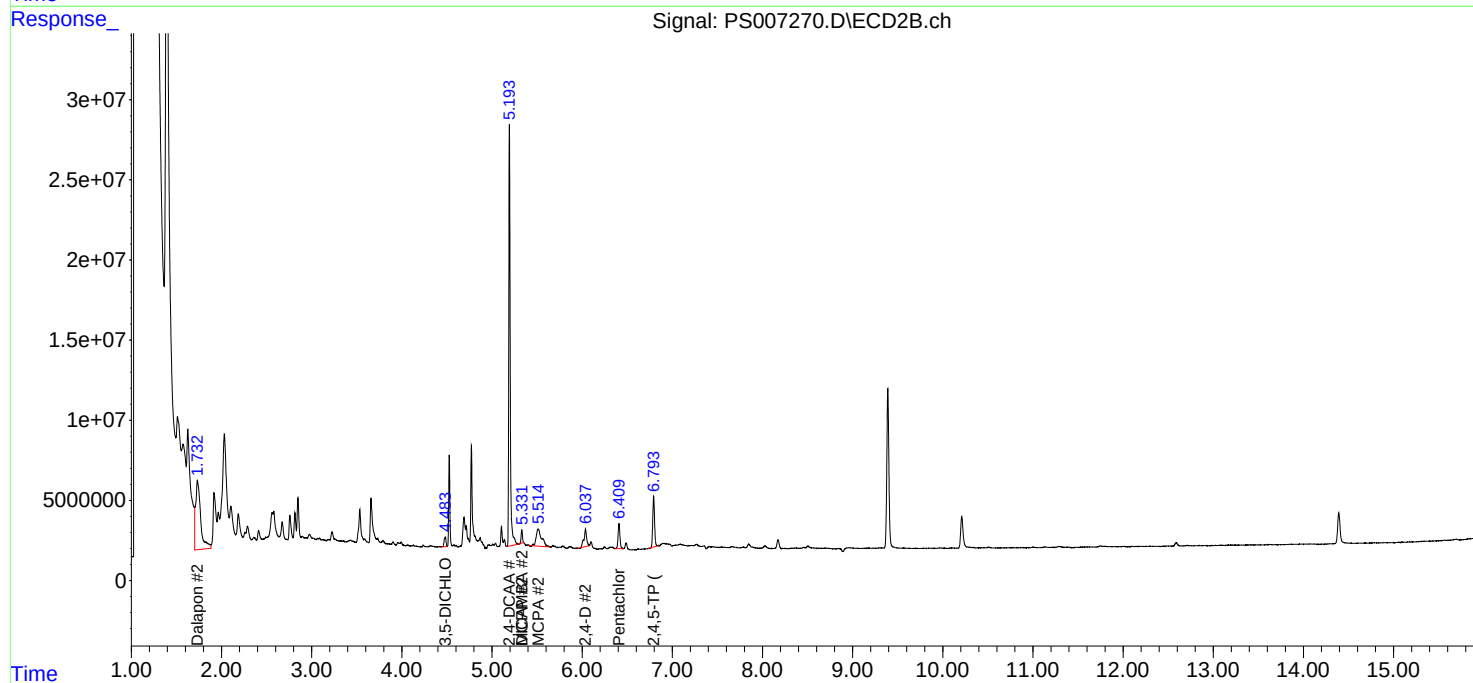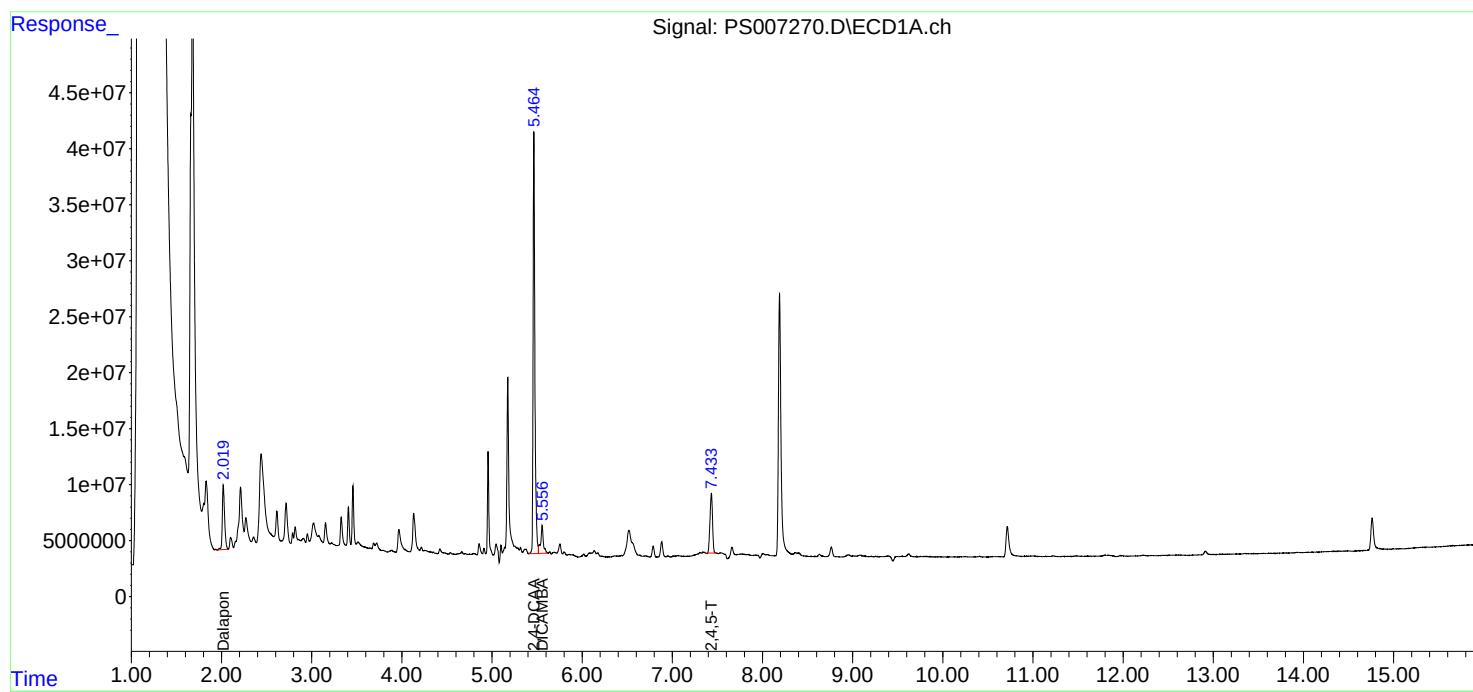


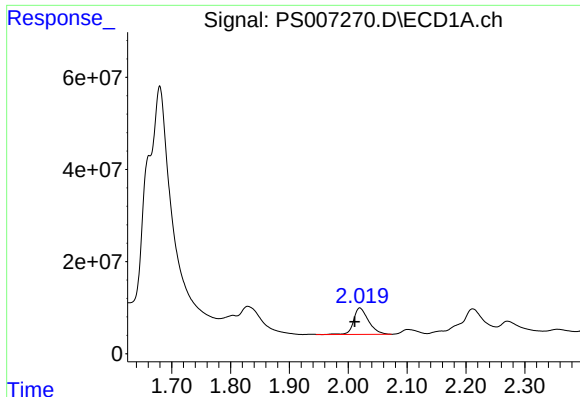

#1 Dalapon


R.T.: 2.020 min
Delta R.T.: 0.009 min
Response: 100899420
Conc: 60.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

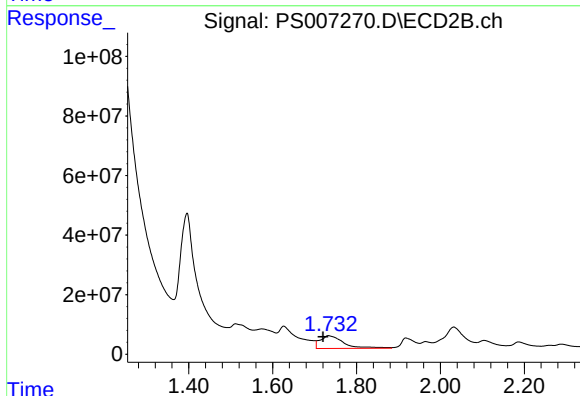


#1 Dalapon

R.T.: 1.733 min
Delta R.T.: 0.013 min
Response: 167876284
Conc: 184.48 ng/ml

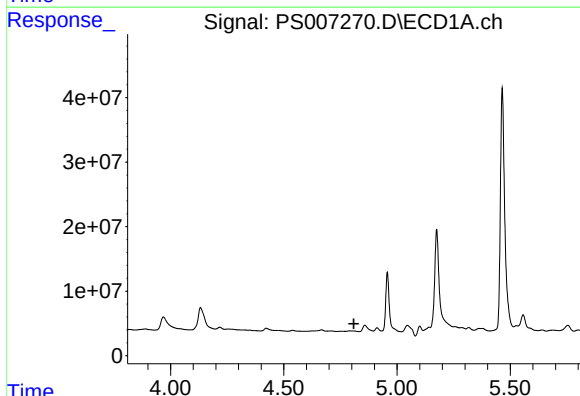


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

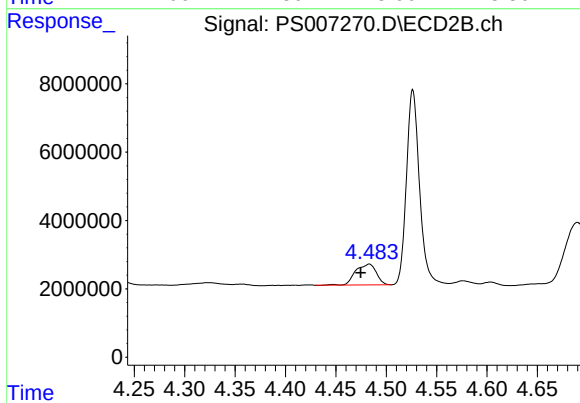

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.482 min
Delta R.T.: 0.008 min
Response: 8707267
Conc: 10.12 ng/ml

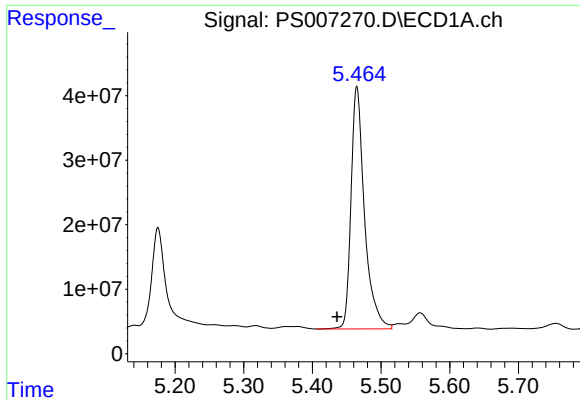

#4 2,4-DCAA


R.T.: 5.465 min
Delta R.T.: 0.029 min
Response: 512060170
Conc: 374.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

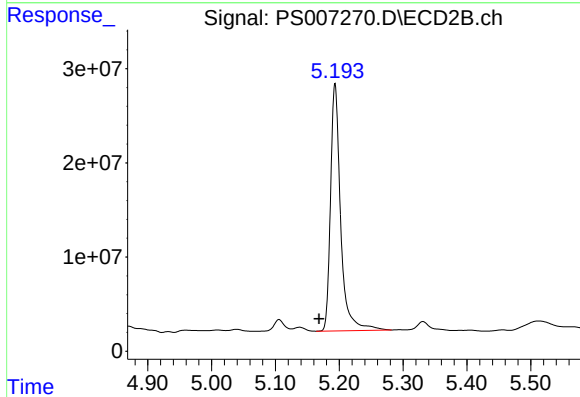


#4 2,4-DCAA

R.T.: 5.194 min
Delta R.T.: 0.025 min
Response: 289674098
Conc: 411.87 ng/ml

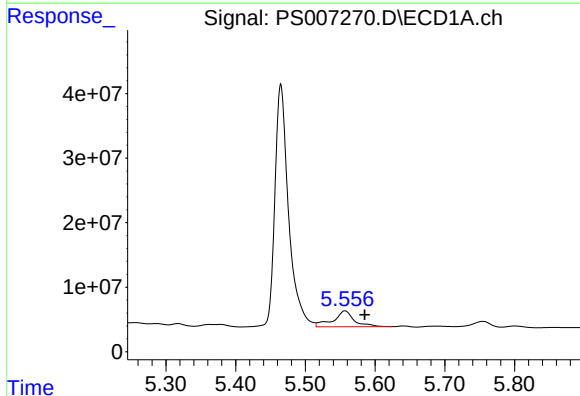


#5 DICAMBA

R.T.: 5.557 min
Delta R.T.: -0.028 min
Response: 51167180
Conc: 10.41 ng/ml

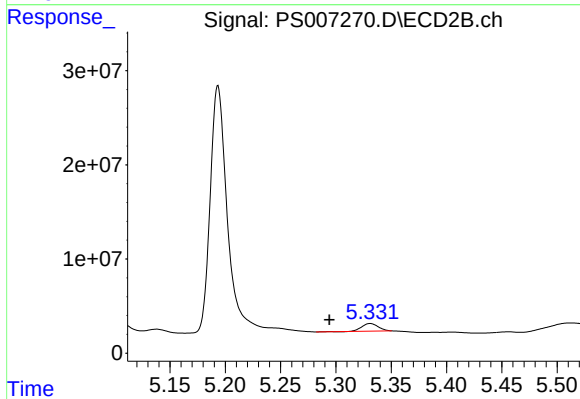

#5 DICAMBA


R.T.: 5.331 min
Delta R.T.: 0.037 min
Response: 8388140
Conc: 3.22 ng/ml

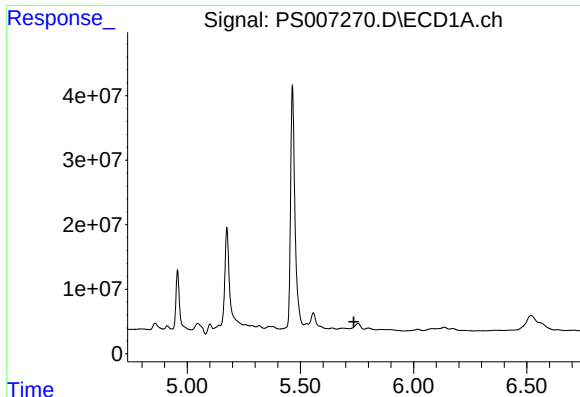

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.736 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

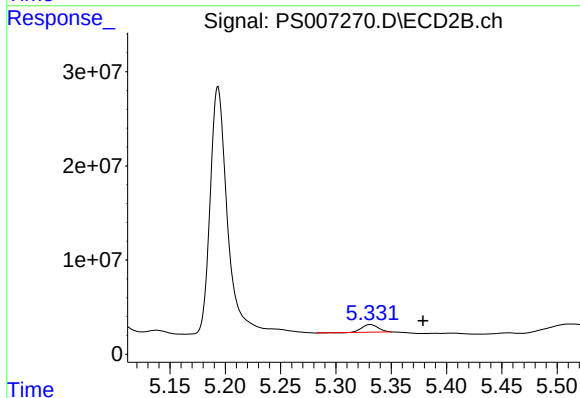


#6 MCPP

R.T.: 5.331 min
Delta R.T.: -0.048 min
Response: 8388140
Conc: 4.42 ug/ml

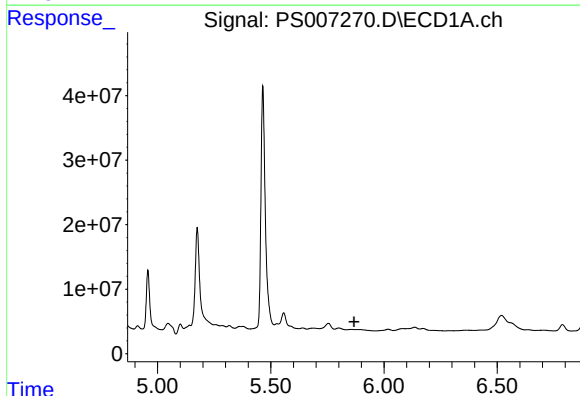


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

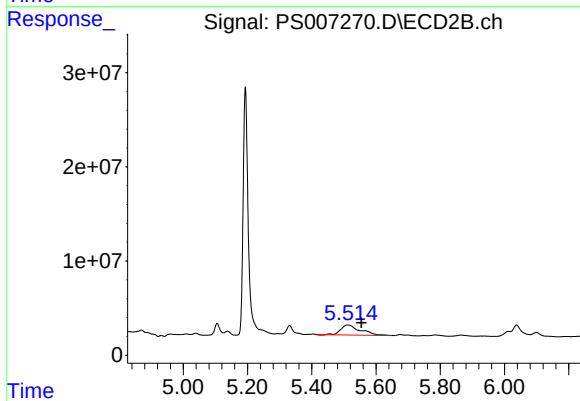

#7 MCPA


R.T.: 5.513 min
Delta R.T.: -0.042 min
Response: 45100975
Conc: 15.51 ug/ml

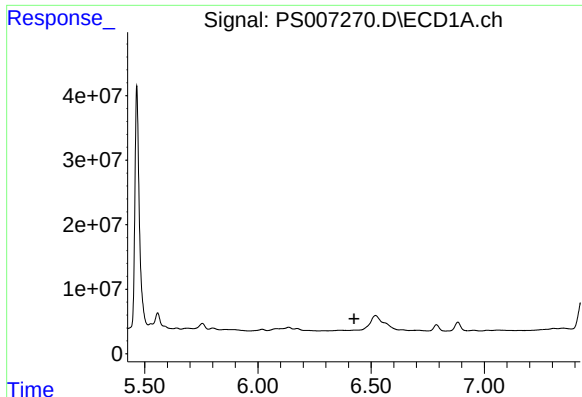

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

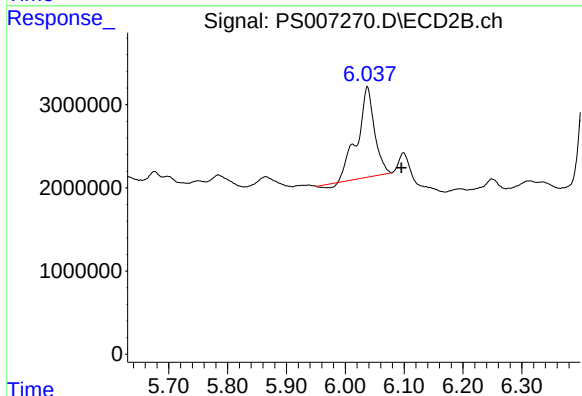


#9 2,4-D

R.T.: 6.038 min
Delta R.T.: -0.058 min
Response: 21767497
Conc: 27.28 ng/ml

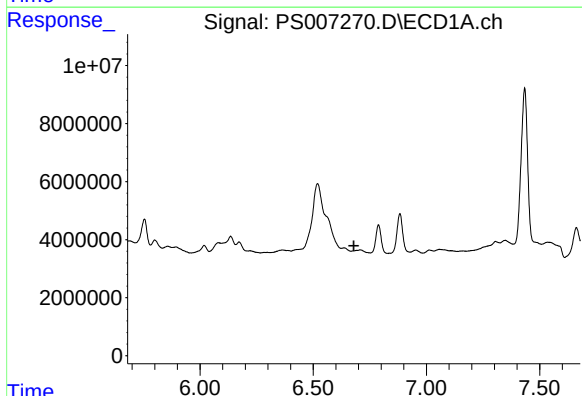


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

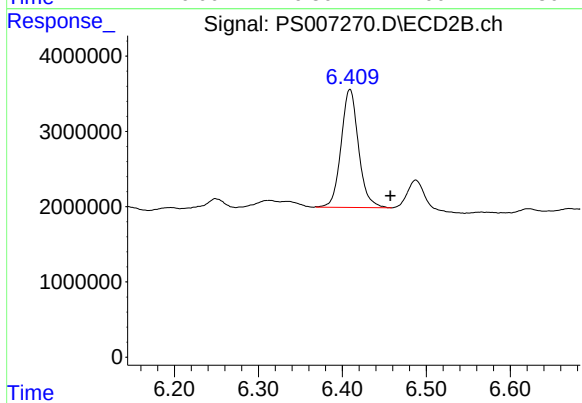

#10 Pentachlorophenol


R.T.: 6.409 min
Delta R.T.: -0.048 min
Response: 22633326
Conc: 2.35 ng/ml

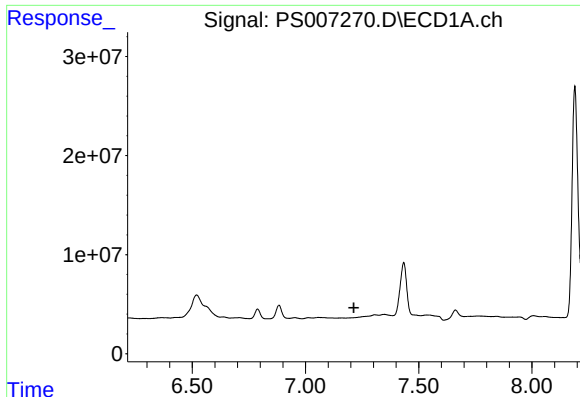

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

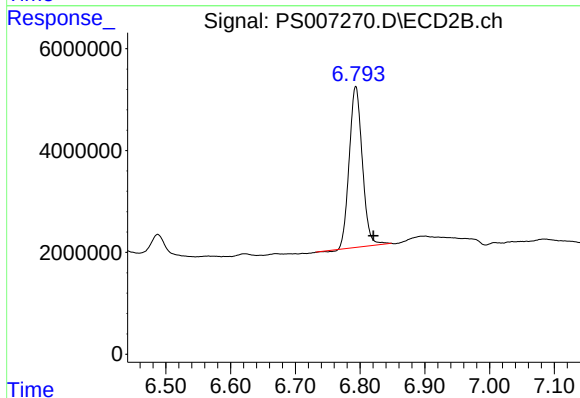


#11 2,4,5-TP (SILVEX)

R.T.: 6.793 min
Delta R.T.: -0.027 min
Response: 44048888
Conc: 11.58 ng/ml

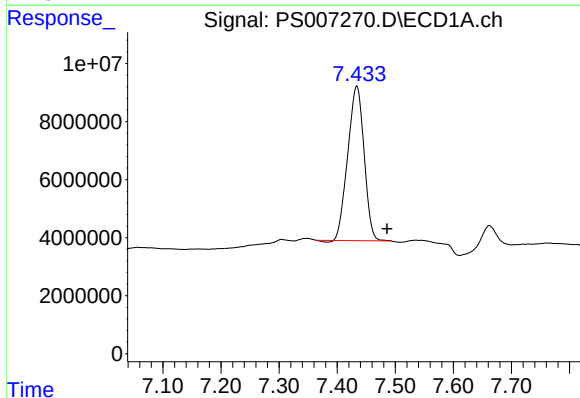

#12 2,4,5-T

R.T.: 7.434 min
Delta R.T.: -0.052 min
Response: 104163024
Conc: 13.63 ng/ml

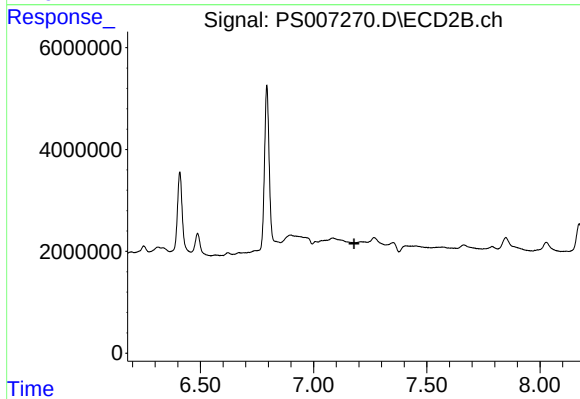

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.178 min
Response: 0
Conc: N.D.