

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102319\
 Data File : PS007275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2019 19:21
 Operator : SM\AJ
 Sample : K5152-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 22:53:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.455	5.170	319.8E6	187.3E6	233.656	266.320
Target Compounds							
1) T	Dalapon	2.009	1.709	67184388	184.4E6	40.151	202.627 #
2) T	3,5-DICHL...	0.000	4.460	0	9012852	N.D.	10.475
5) T	DICAMBA	5.545	0.000	47498676	0	9.667	N.D. #
9) T	2,4-D	0.000	6.075	0	8090751	N.D.	10.141
10) T	Pentachlo...	0.000	6.465	0	6389978	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.821	0	76504330	N.D.	20.114
12) T	2,4,5-T	7.420	0.000	101.1E6	0	13.227	N.D. #
15) T	Picloram	0.000	8.925	0	12173255	N.D.	1.983
16) T	DCPA	0.000	8.925	0	12173255	N.D.	2.428



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102319\
Data File : PS007275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2019 19:21
Operator : SM\AJ
Sample : K5152-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 22:53:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

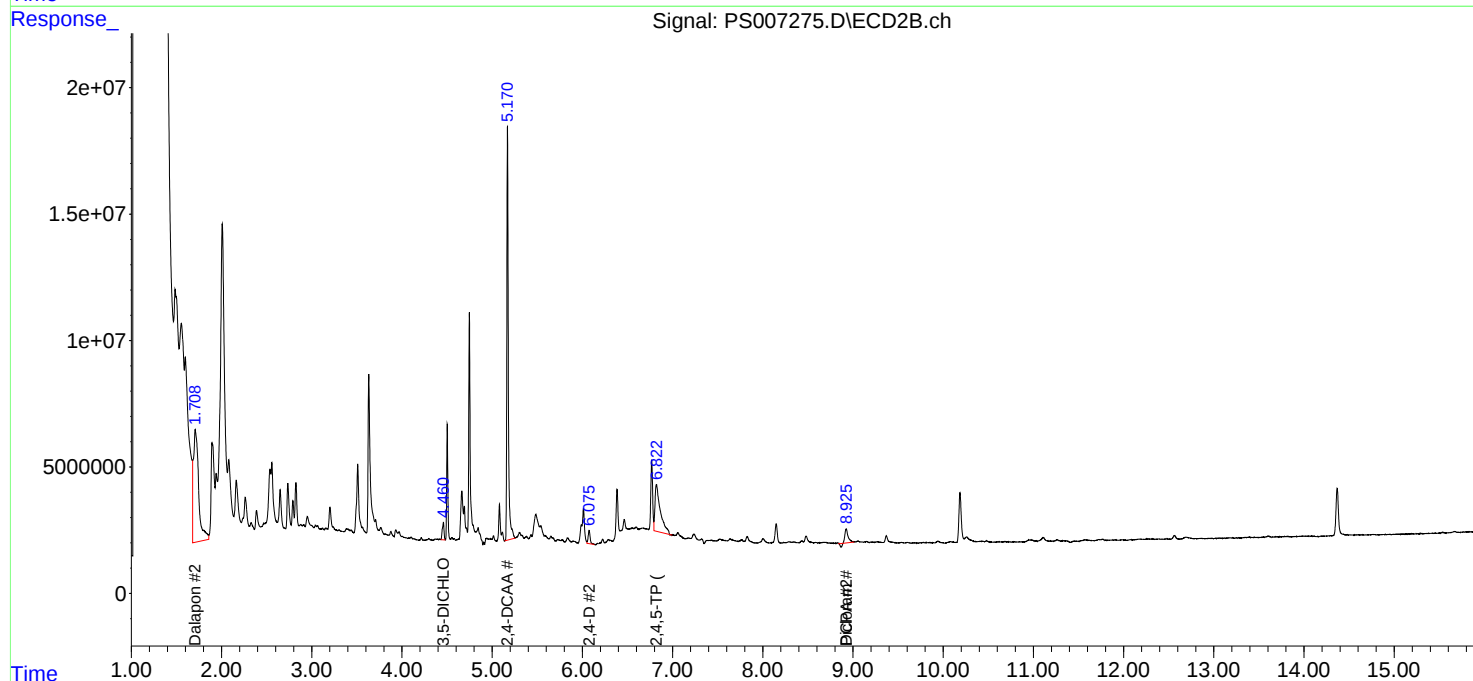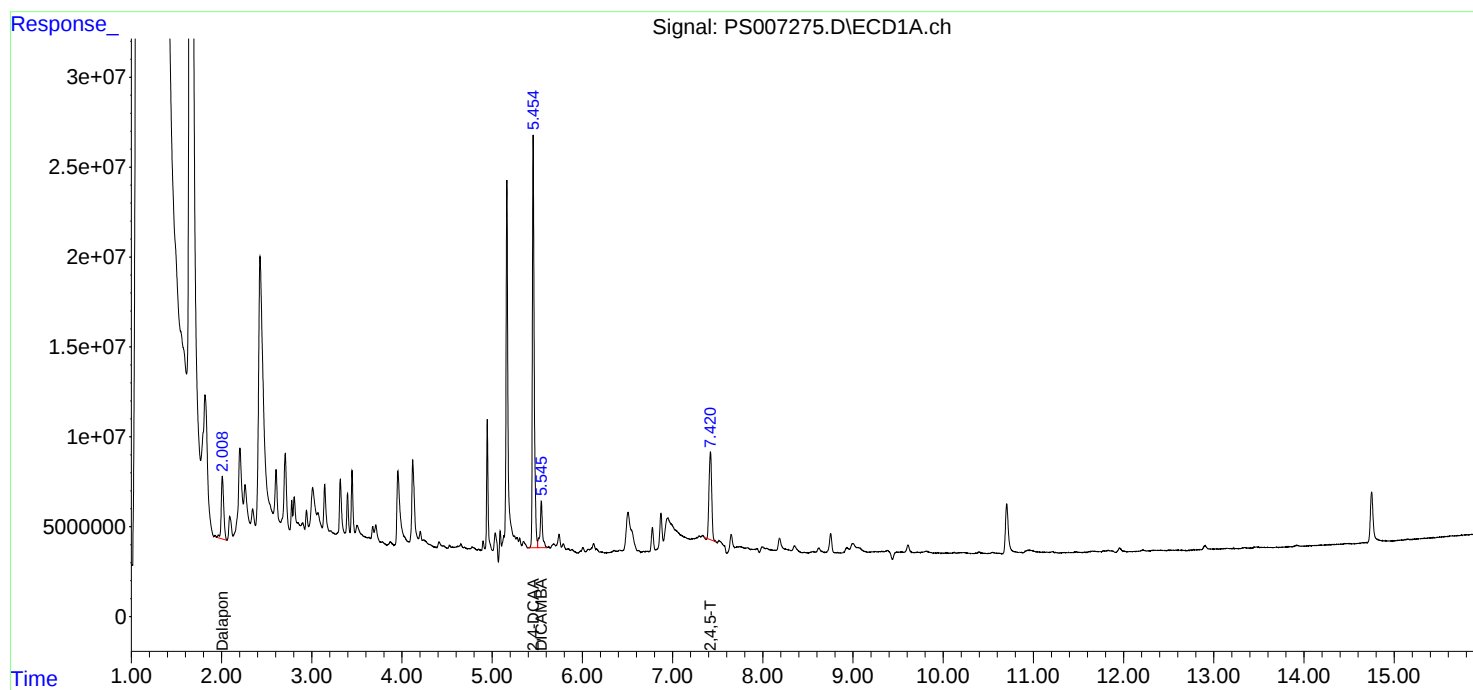


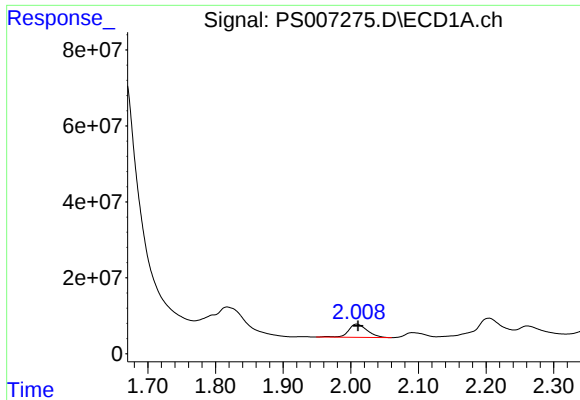

#1 Dalapon


R.T.: 2.009 min
Delta R.T.: -0.002 min
Response: 67184388
Conc: 40.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

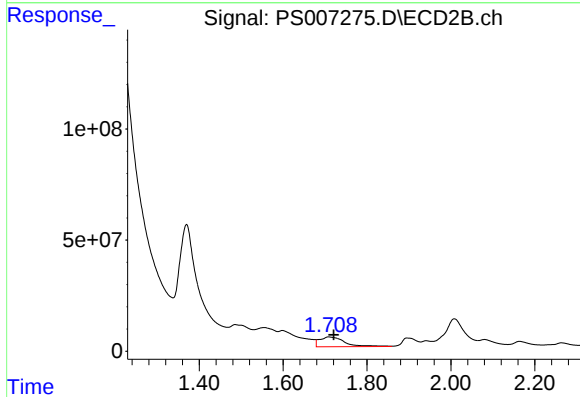


#1 Dalapon

R.T.: 1.709 min
Delta R.T.: -0.012 min
Response: 184391495
Conc: 202.63 ng/ml

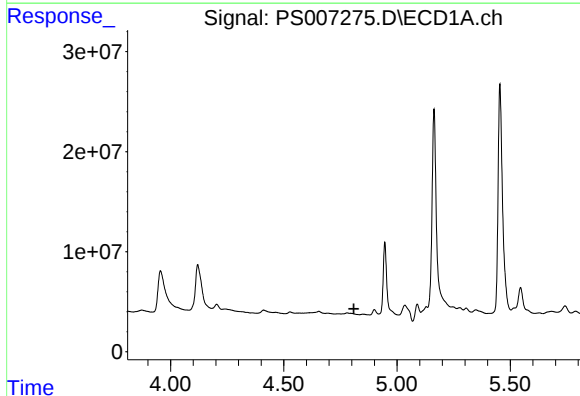


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

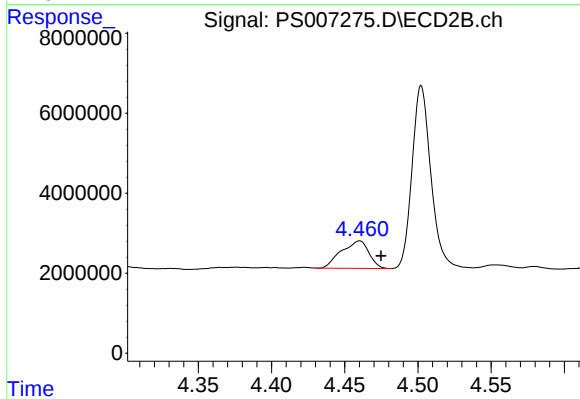

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.460 min
Delta R.T.: -0.015 min
Response: 9012852
Conc: 10.47 ng/ml

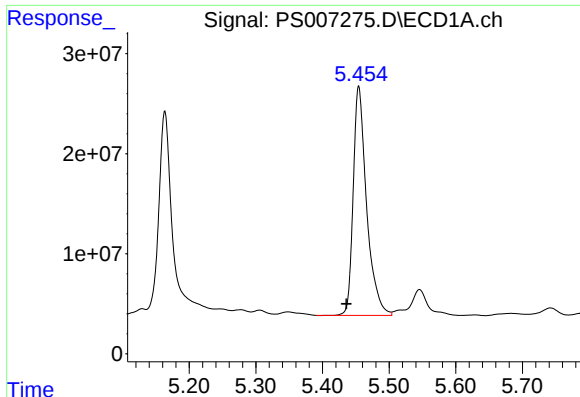

#4 2,4-DCAA


R.T.: 5.455 min
Delta R.T.: 0.019 min
Response: 319797668
Conc: 233.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

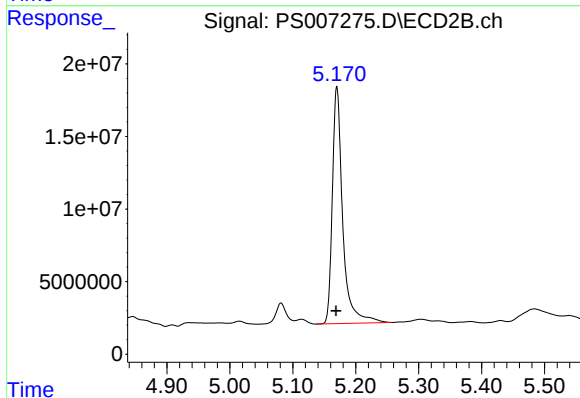


#4 2,4-DCAA

R.T.: 5.170 min
Delta R.T.: 0.002 min
Response: 187304525
Conc: 266.32 ng/ml

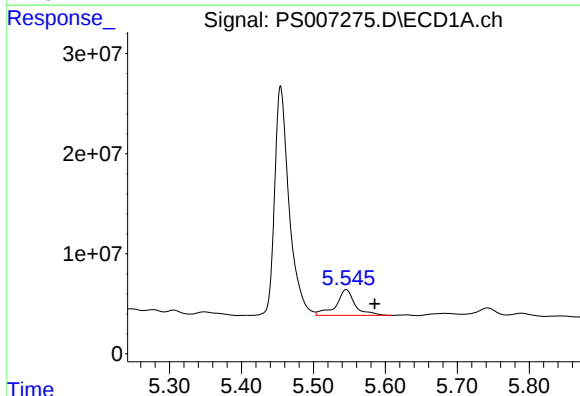


#5 DICAMBA

R.T.: 5.545 min
Delta R.T.: -0.040 min
Response: 47498676
Conc: 9.67 ng/ml

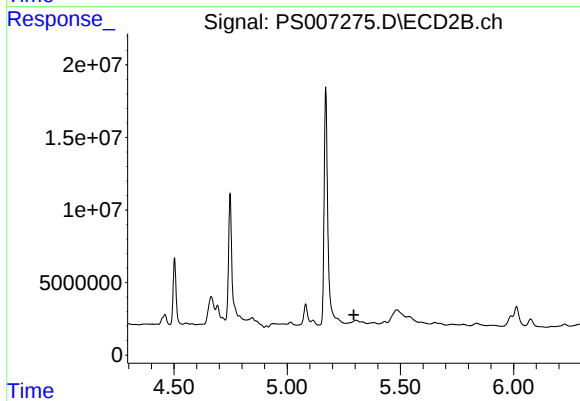

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

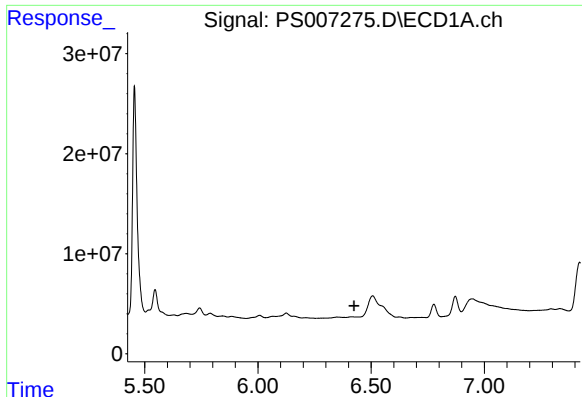

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

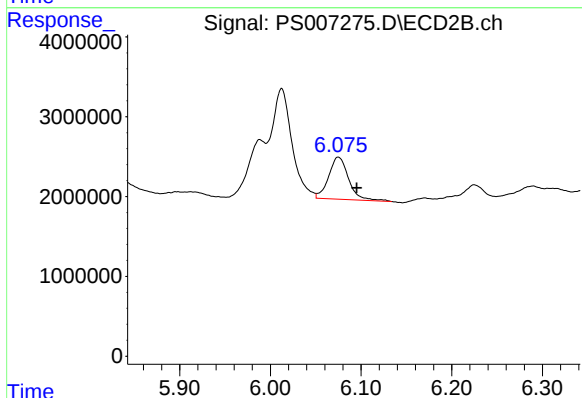


#9 2,4-D

R.T.: 6.075 min
Delta R.T.: -0.020 min
Response: 8090751
Conc: 10.14 ng/ml

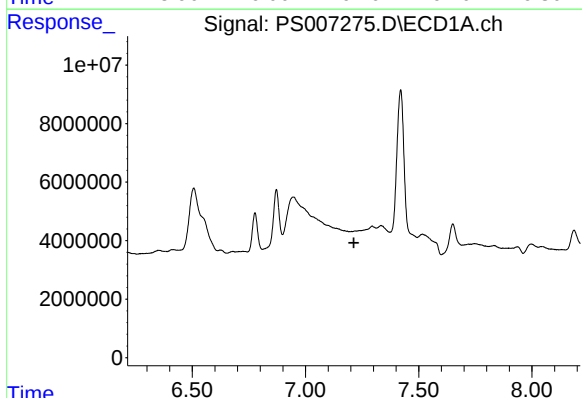


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

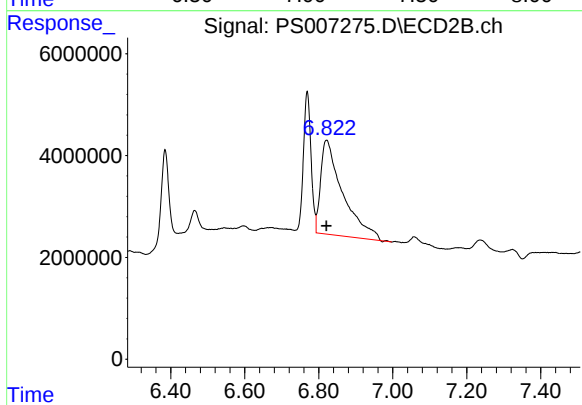

#11 2,4,5-TP (SILVEX)


R.T.: 6.821 min
Delta R.T.: 0.000 min
Response: 76504330
Conc: 20.11 ng/ml

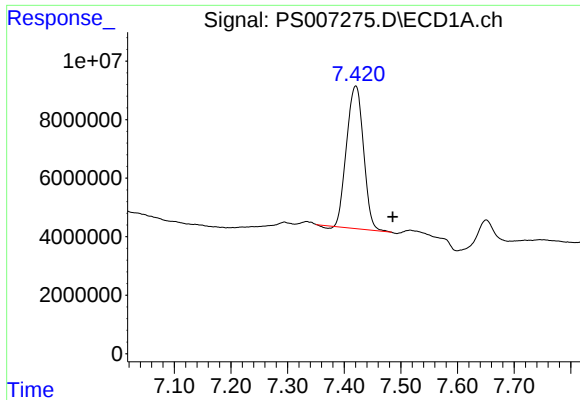

#12 2,4,5-T


R.T.: 7.420 min
Delta R.T.: -0.066 min
Response: 101117522
Conc: 13.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

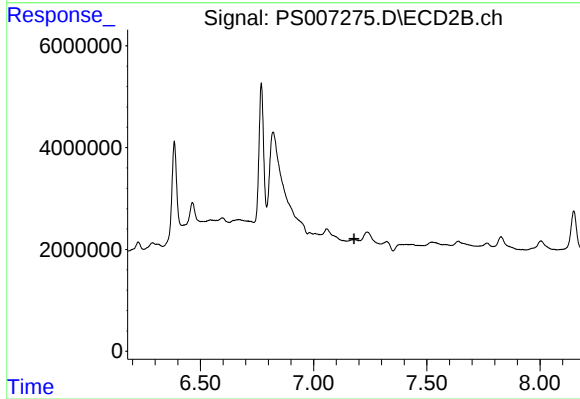


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.178 min
Response: 0
Conc: N.D.

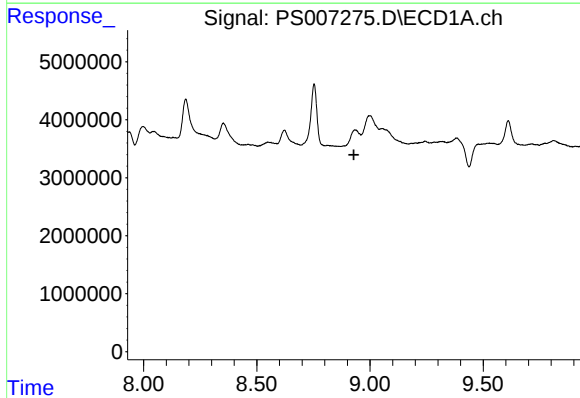


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

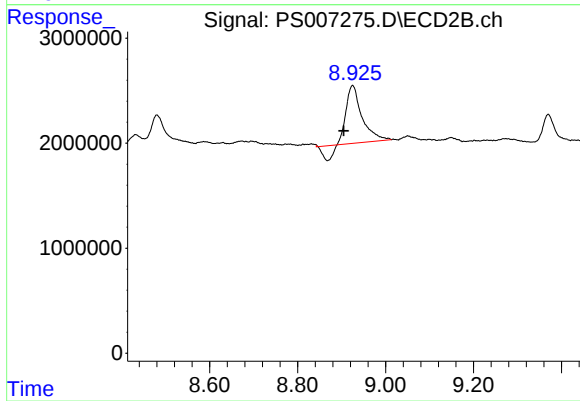

#15 Picloram


R.T.: 8.925 min
Delta R.T.: 0.020 min
Response: 12173255
Conc: 1.98 ng/ml

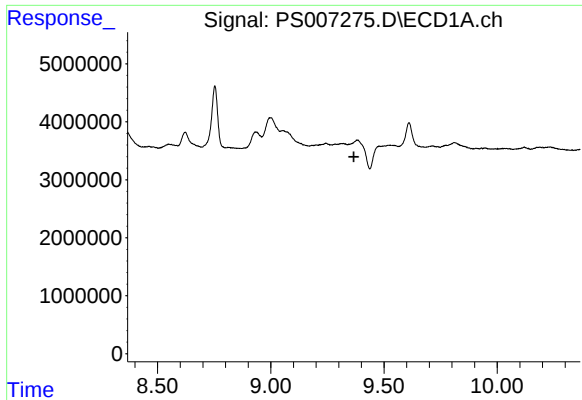

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

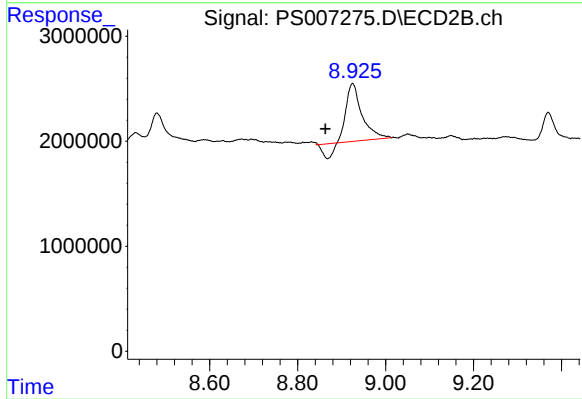

#16 DCPA

R.T.: 8.925 min
Delta R.T.: 0.062 min
Response: 12173255
Conc: 2.43 ng/ml