

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102324\
 Data File : PS028014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2024 14:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 15:08:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 23 13:25:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.094	7.611	1328.8E6	438.1E6	492.711	461.754
Target Compounds							
1) T	Dalapon	2.539	0.000	10536189	0	2.312	N.D. #
2) T	3,5-DICHL...	6.312f	0.000	278833	0	<MDL	N.D. #
3) T	4-Nitroph...	6.894	0.000	9917467	0	5.360	N.D. #
6) T	MCP	0.000	7.939f	0	8560010	N.D.	3.311
7) T	MCPA	7.637f	0.000	1607157	0	<MDL	N.D. #
9) T	2,4-D	8.189	0.000	10940298	0	3.229	N.D. #
11) T	2,4,5-TP ...	9.032	0.000	1804647	0	<MDL	N.D. #
12) T	2,4,5-T	9.330	0.000	5320395	0	<MDL	N.D. #
13) T	2,4-DB	9.901	0.000	4022319	0	1.528	N.D. #
14) T	DINOSEB	11.058	0.000	8394340	0	<MDL	N.D. #
15) T	Picloram	10.881	12.160	59696588	4786261	2.681	1.050 #
16) T	DCPA	11.349	12.077f	5325052	4046052	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102324\
Data File : PS028014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2024 14:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 15:08:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
Quant Title : 8080.M
QLast Update : Wed Oct 23 13:25:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

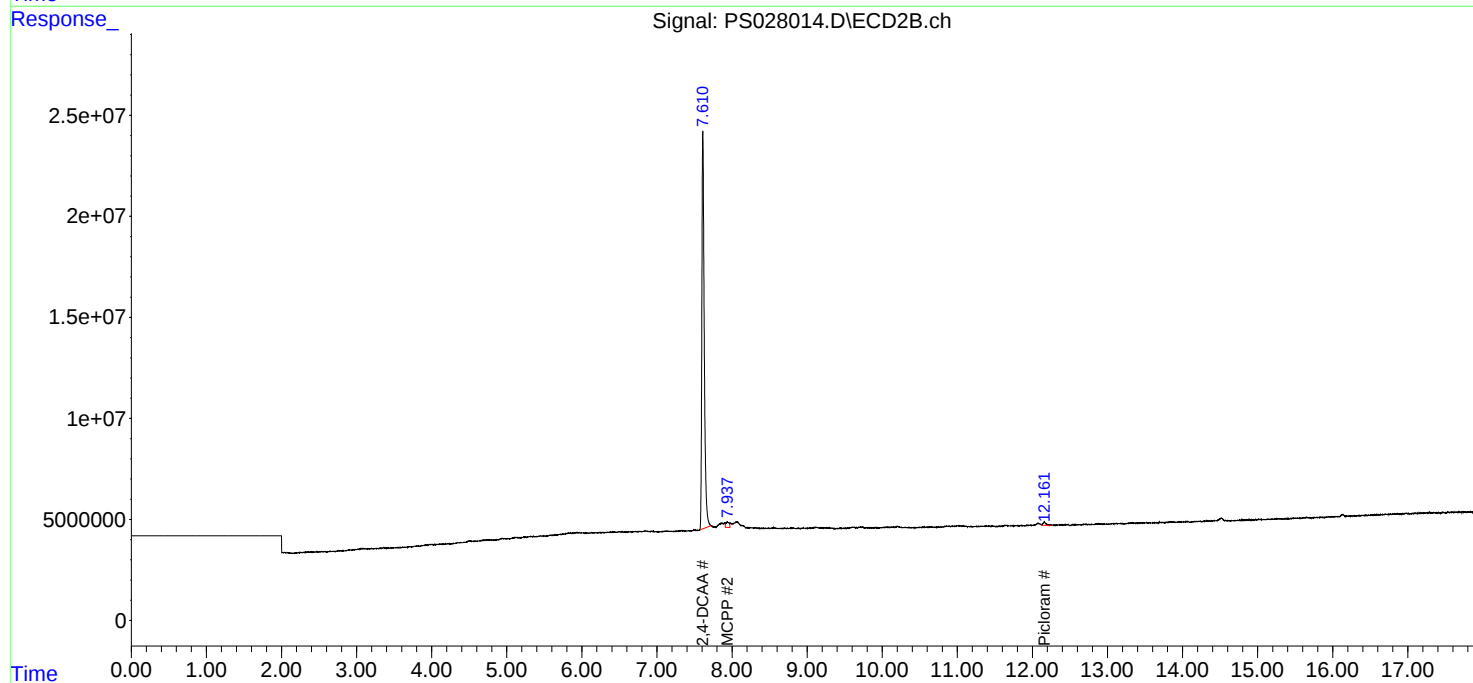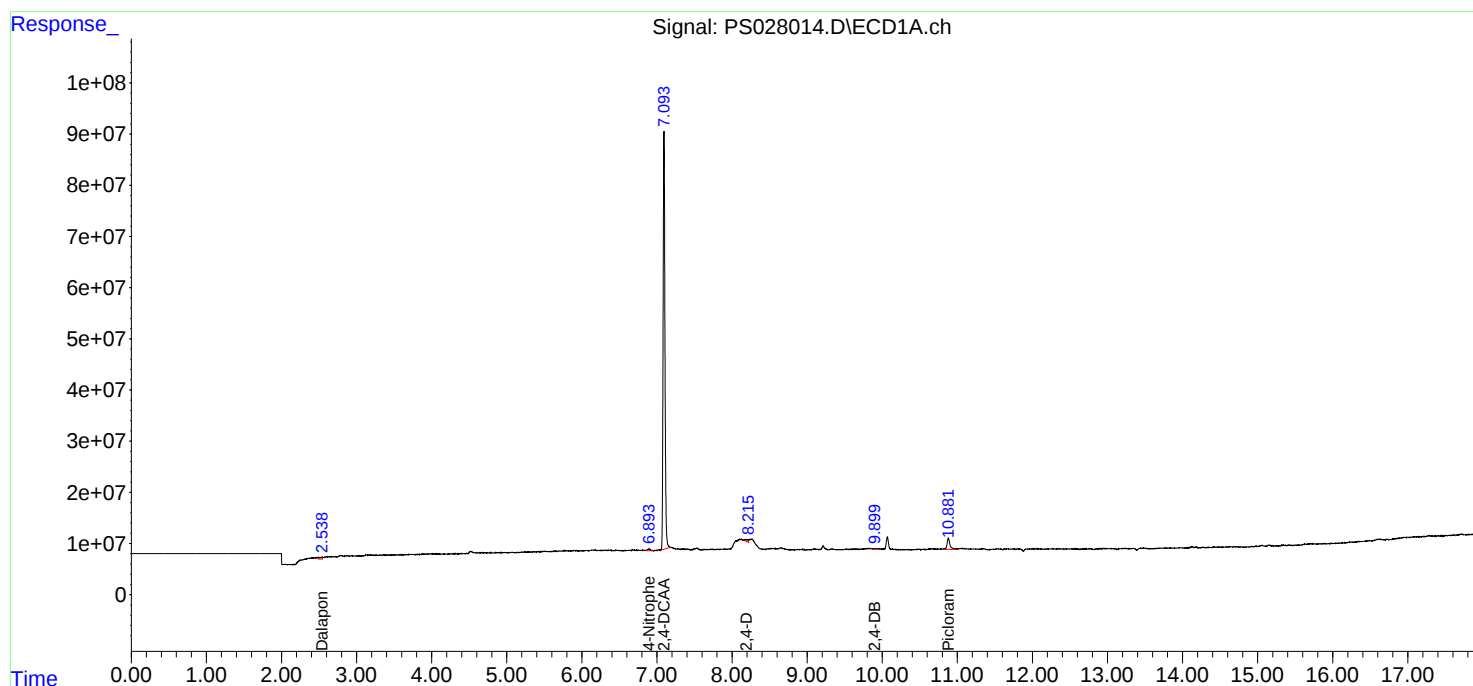


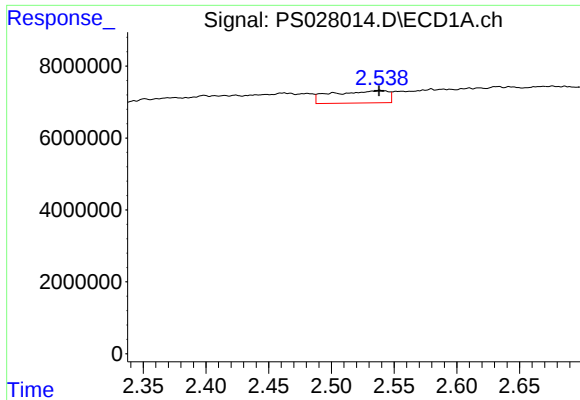

#1 Dalapon


R.T.: 2.539 min
Delta R.T.: 0.000 min
Response: 10536189
Conc: 2.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

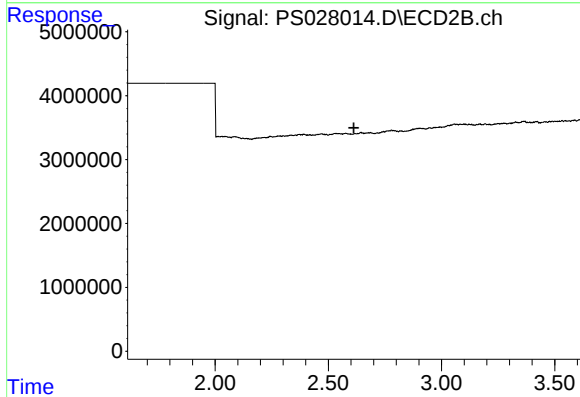


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.613 min
Response: 0
Conc: N.D.

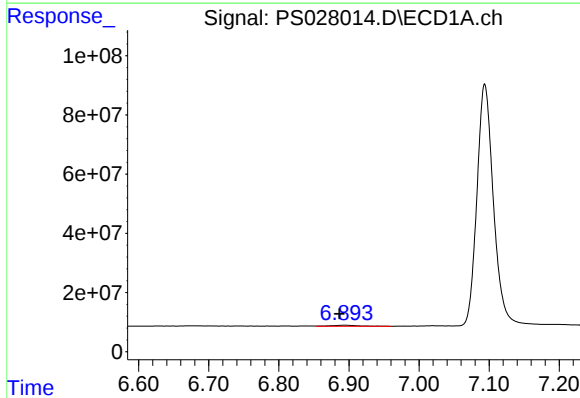


#3 4-Nitrophenol

R.T.: 6.894 min
Delta R.T.: 0.008 min
Response: 9917467
Conc: 5.36 ng/ml

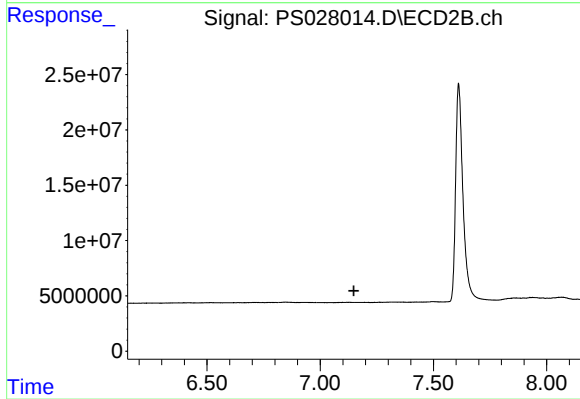

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

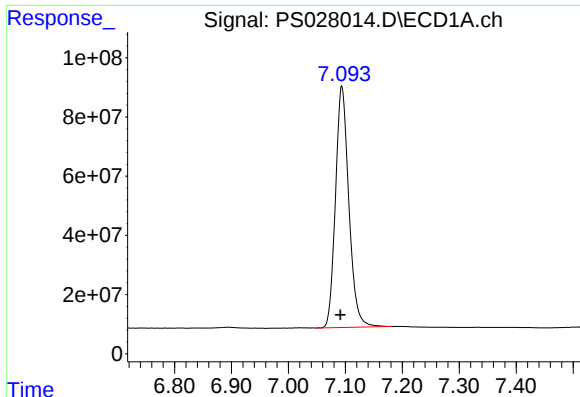

#4 2,4-DCAA


R.T.: 7.094 min
Delta R.T.: 0.003 min
Response: 1328824955
Conc: 492.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

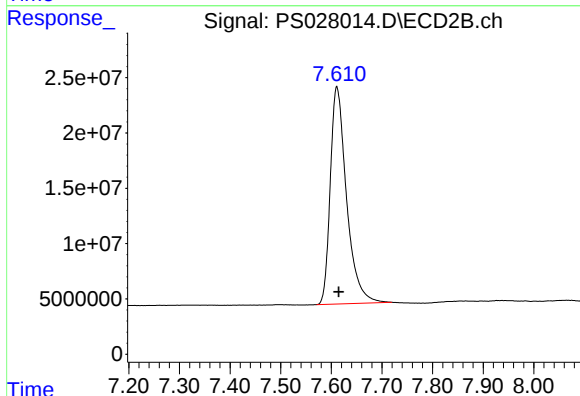


#4 2,4-DCAA

R.T.: 7.611 min
Delta R.T.: -0.003 min
Response: 438055764
Conc: 461.75 ng/ml

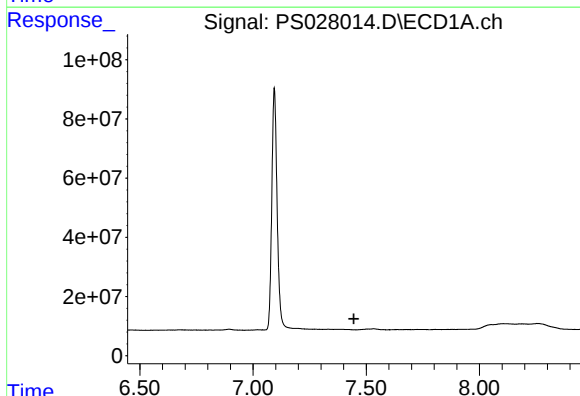


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

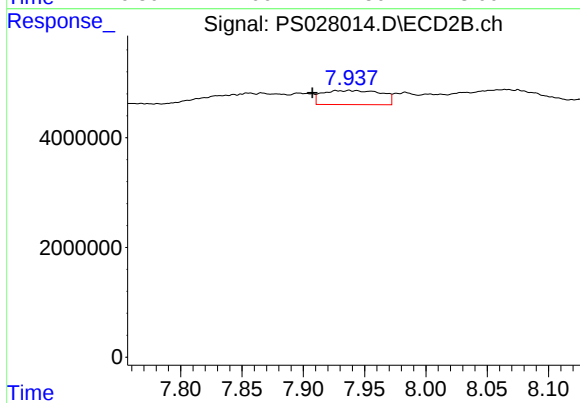

#6 MCP


R.T.: 7.939 min
Delta R.T.: 0.031 min
Response: 8560010
Conc: 3.31 ug/ml

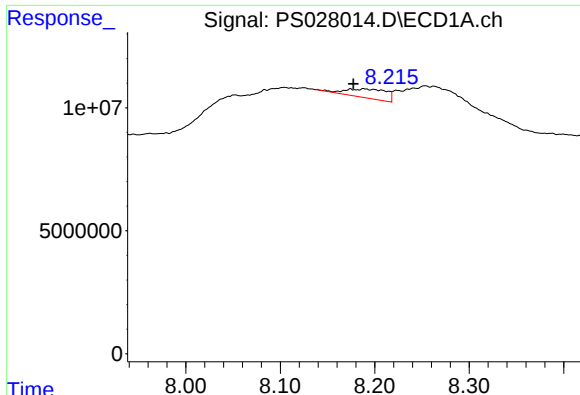

#9 2,4-D


R.T.: 8.189 min
Delta R.T.: 0.011 min
Response: 10940298
Conc: 3.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

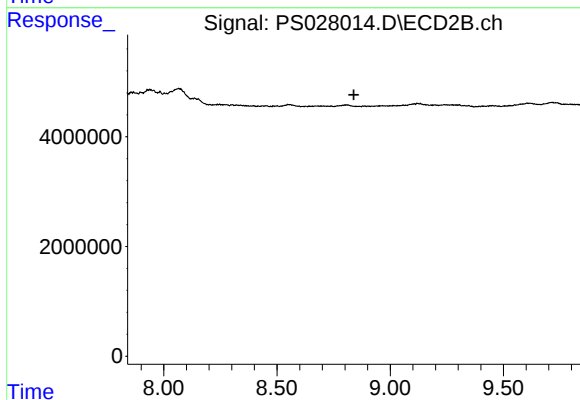


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.840 min
Response: 0
Conc: N.D.

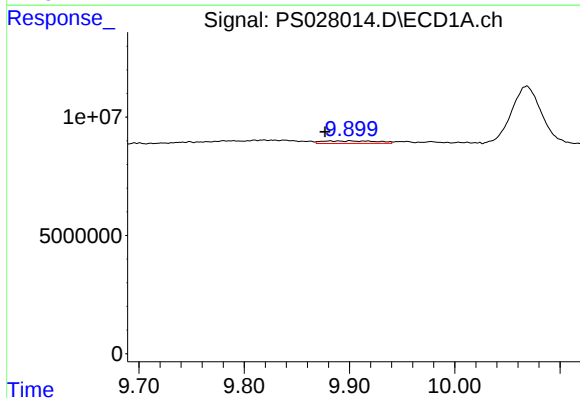


#13 2,4-DB

R.T.: 9.901 min
Delta R.T.: 0.024 min
Response: 4022319
Conc: 1.53 ng/ml

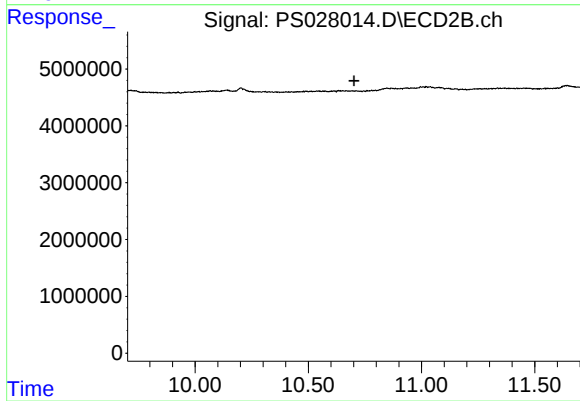

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.702 min
Response: 0
Conc: N.D.

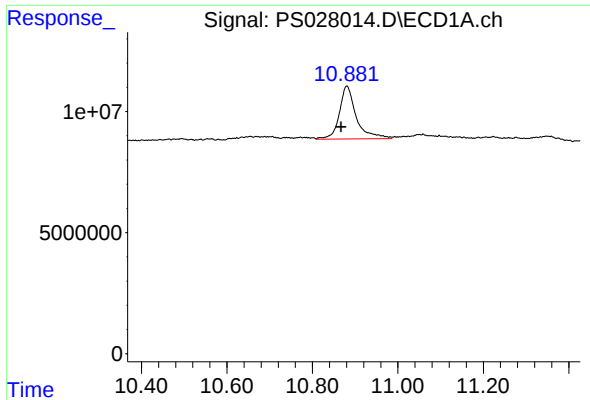

#15 Picloram

R.T.: 10.881 min
Delta R.T.: 0.014 min
Response: 59696588
Conc: 2.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

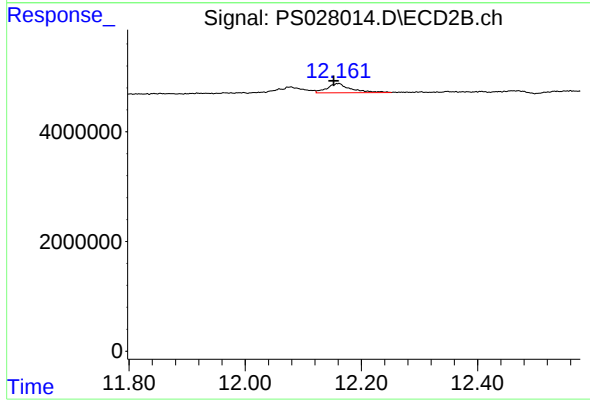

#15 Picloram

R.T.: 12.160 min
Delta R.T.: 0.008 min
Response: 4786261
Conc: 1.05 ng/ml