

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102324\
 Data File : PS028028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 01:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 03:57:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 23 13:25:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.094	7.611	1316.7E6	491.1E6	488.214	517.711
Target Compounds							
3) T	4-Nitroph...	6.885	0.000	8877431	0	4.798	N.D. #
7) T	MCPA	7.632f	0.000	15388171	0	1.451	N.D. #
8) T	DICHLORPROP	7.967	0.000	2470186	0	<MDL	N.D. #
9) T	2,4-D	8.192	0.000	14430231	0	4.259	N.D. #
10) T	Pentachlo...	8.471	0.000	1266960	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.007	0.000	3052931	0	<MDL	N.D. #
12) T	2,4,5-T	9.322	0.000	2683979	0	<MDL	N.D. #
13) T	2,4-DB	9.831f	0.000	2495030	0	<MDL	N.D. #
14) T	DINOSEB	11.094f	0.000	5472610	0	<MDL	N.D. #
15) T	Picloram	10.866	0.000	17784114	0	<MDL	N.D. #
16) T	DCPA	11.357	0.000	1358565	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102324\
Data File : PS028028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 01:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 03:57:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
Quant Title : 8080.M
QLast Update : Wed Oct 23 13:25:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

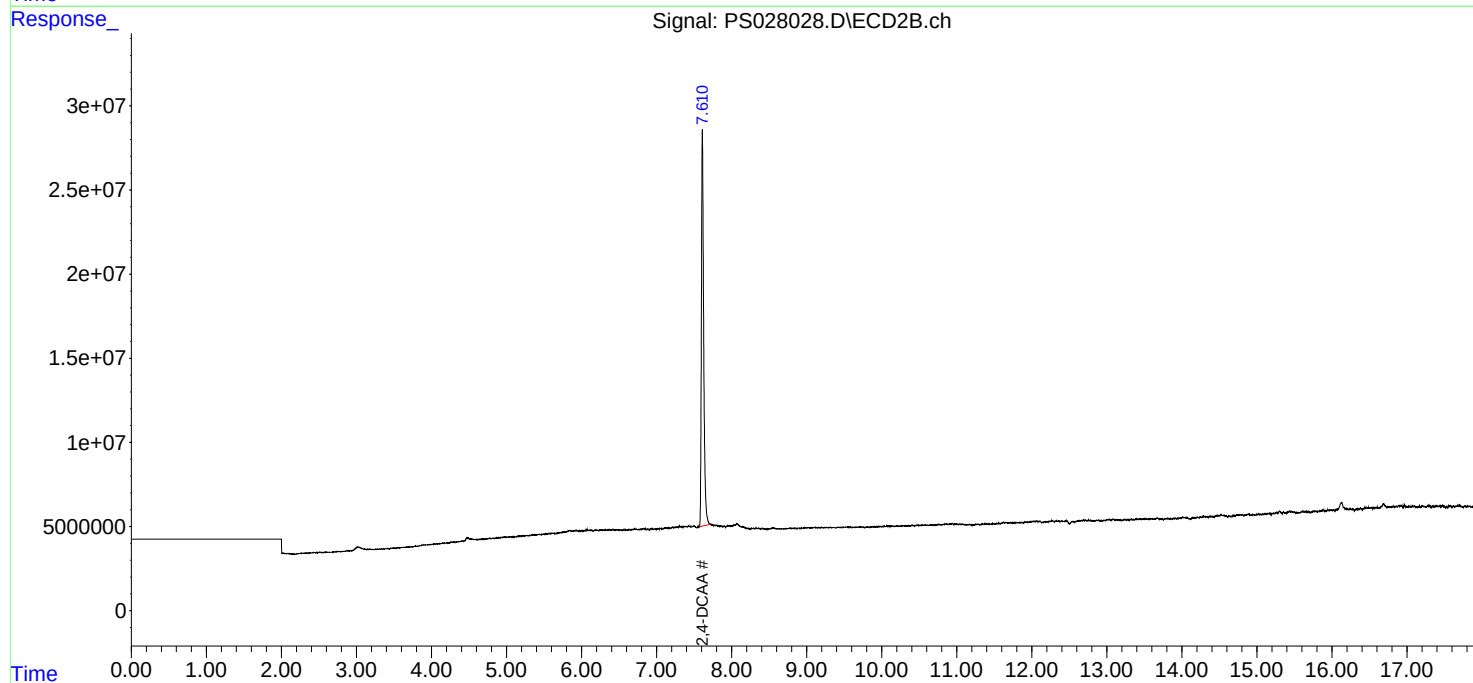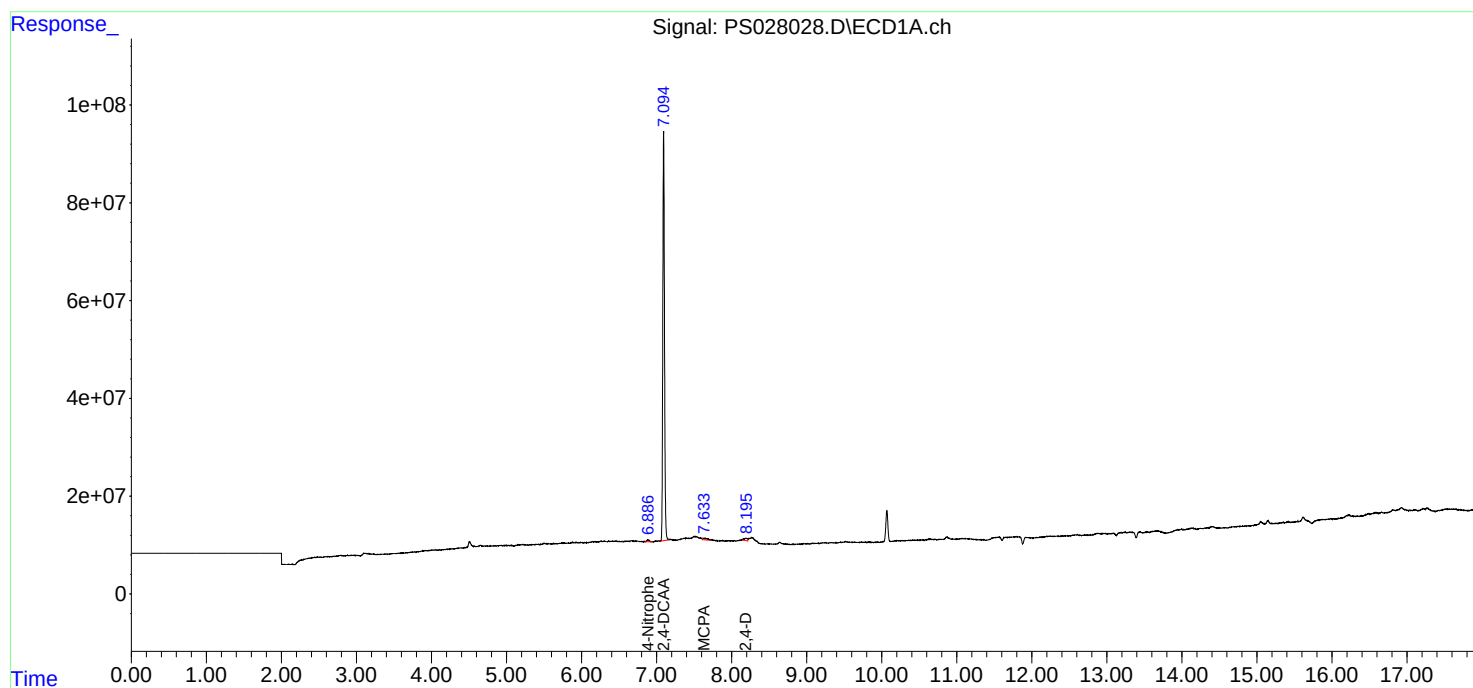


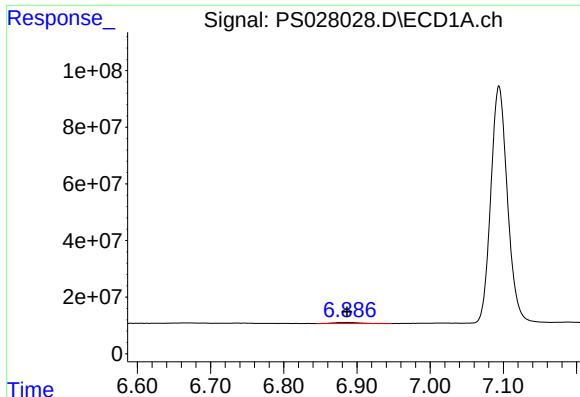

#3 4-Nitrophenol


R.T.: 6.885 min
Delta R.T.: -0.001 min
Response: 8877431
Conc: 4.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

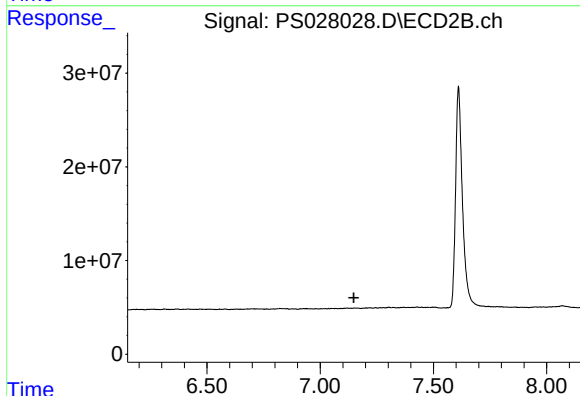


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

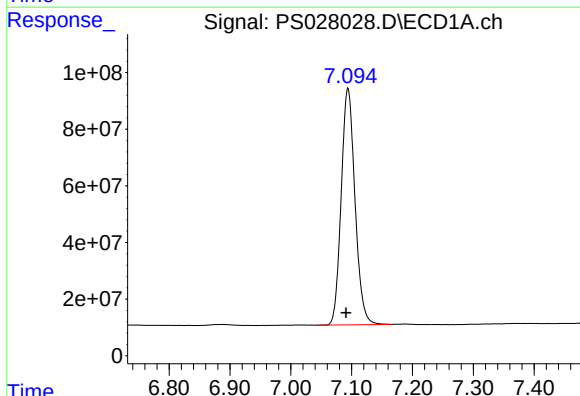


#4 2,4-DCAA

R.T.: 7.094 min
Delta R.T.: 0.003 min
Response: 1316695267
Conc: 488.21 ng/ml

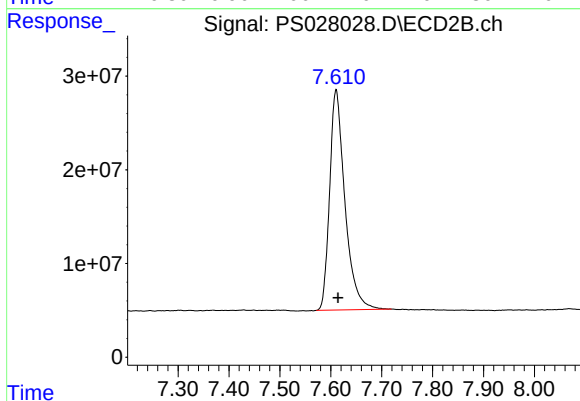

#4 2,4-DCAA


R.T.: 7.611 min
Delta R.T.: -0.004 min
Response: 491140979
Conc: 517.71 ng/ml

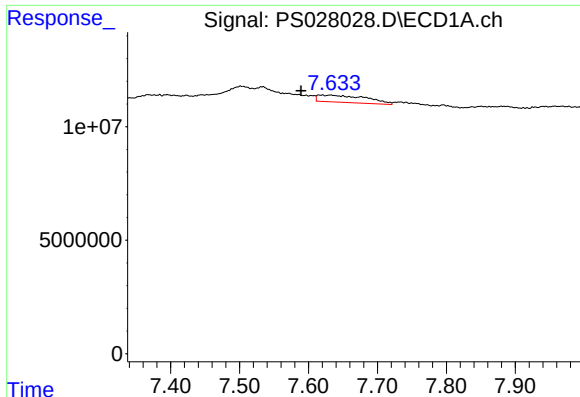

#7 MCPA


R.T.: 7.632 min
Delta R.T.: 0.043 min
Response: 15388171
Conc: 1.45 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

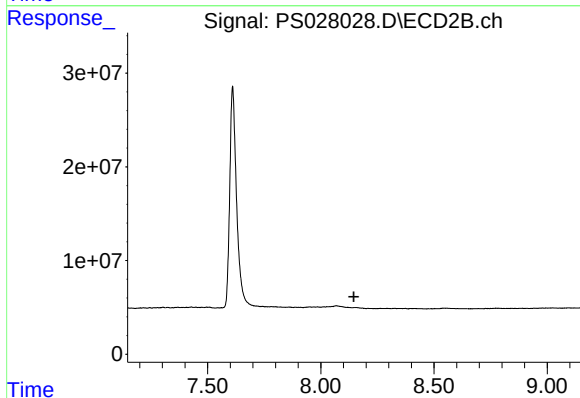


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 8.146 min
Response: 0
Conc: N.D.

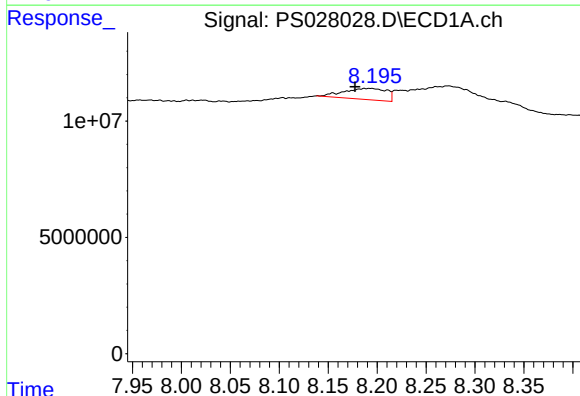

#9 2,4-D

R.T.: 8.192 min
Delta R.T.: 0.014 min
Response: 14430231
Conc: 4.26 ng/ml

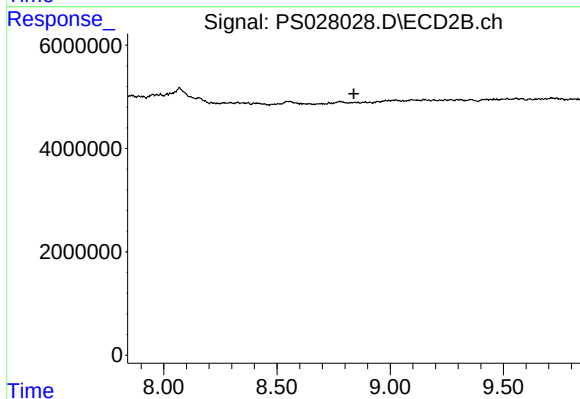

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.840 min
Response: 0
Conc: N.D.