

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS102324\  
 Data File : PS028021.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Oct 2024 17:01  
 Operator : AR\AJ  
 Sample : PB174307BL  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 PB174307BL

Manual Integrations  
 APPROVED

Reviewed By :Abdul  
 Mirza  
 10/24/2024

Supervised By :Ankita  
 Jodhani  
 10/24/2024

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 24 02:28:52 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS102324.M  
 Quant Title : 8080.M  
 QLast Update : Wed Oct 23 13:25:49 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

|      |          |       |       |          |         |          |         |
|------|----------|-------|-------|----------|---------|----------|---------|
| 4) S | 2,4-DCAA | 7.090 | 7.613 | 1457.1E6 | 491.5E6 | 540.276m | 518.079 |
|------|----------|-------|-------|----------|---------|----------|---------|

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS102324\  
Data File : PS028021.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 23 Oct 2024 17:01  
Operator : AR\AJ  
Sample : PB174307BL  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
PB174307BL



Manual Integrations  
APPROVED


Reviewed By : Abdul  
Mirza  
10/24/2024

Supervised By : Ankita  
Jodhani  
10/24/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 24 02:28:52 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS102324.M  
Quant Title : 8080.M  
QLast Update : Wed Oct 23 13:25:49 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

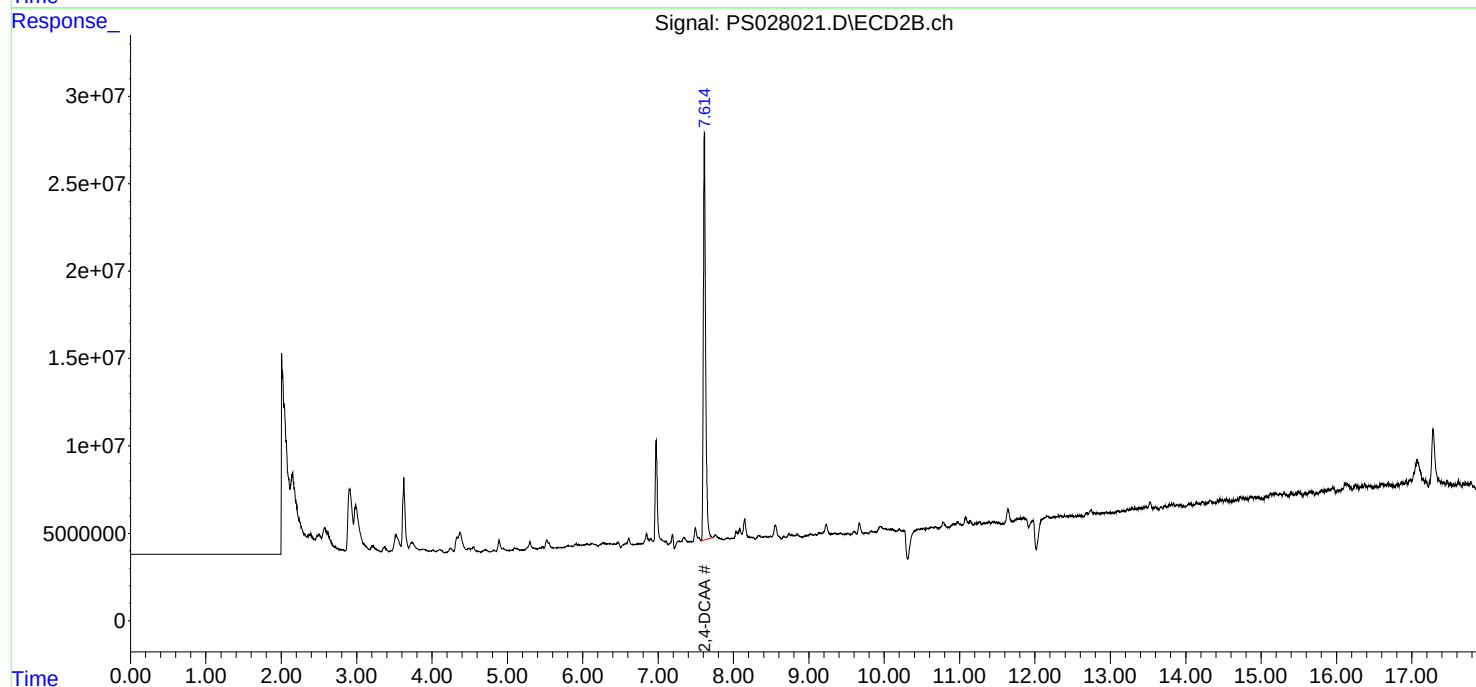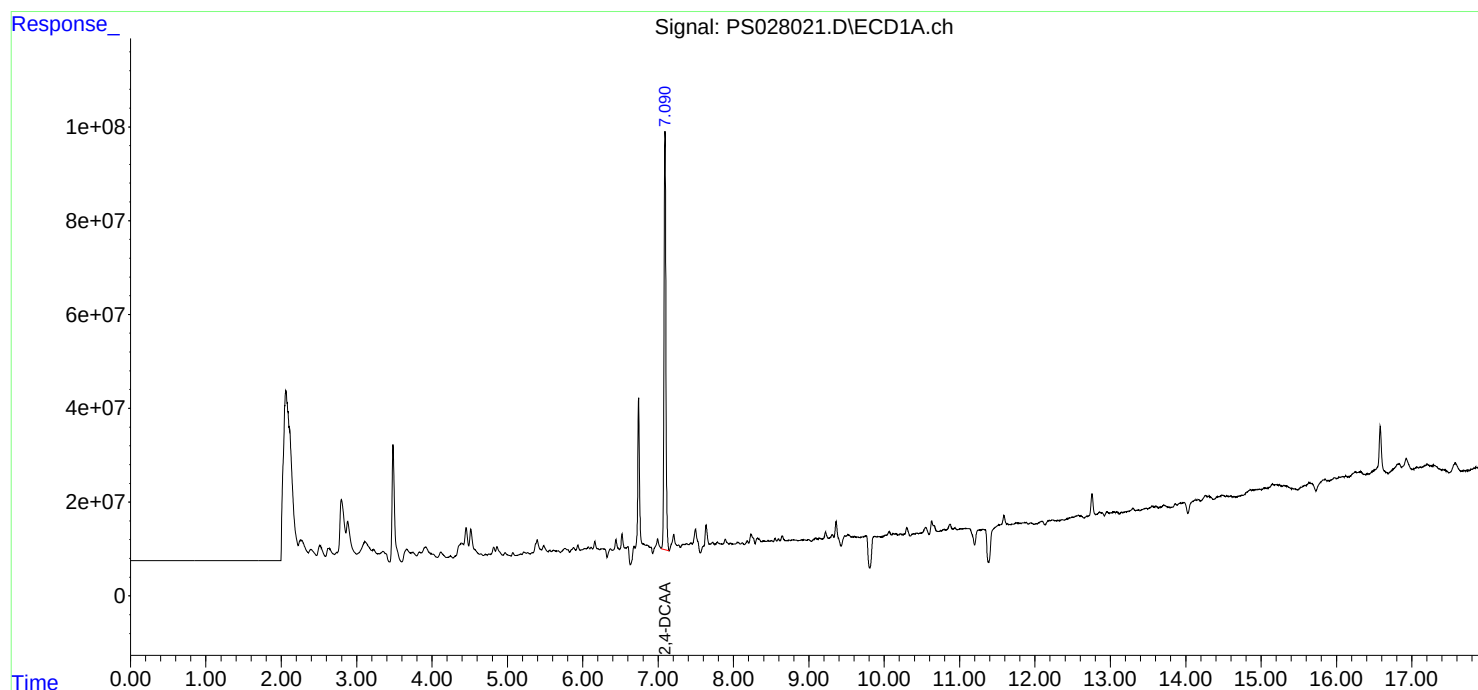

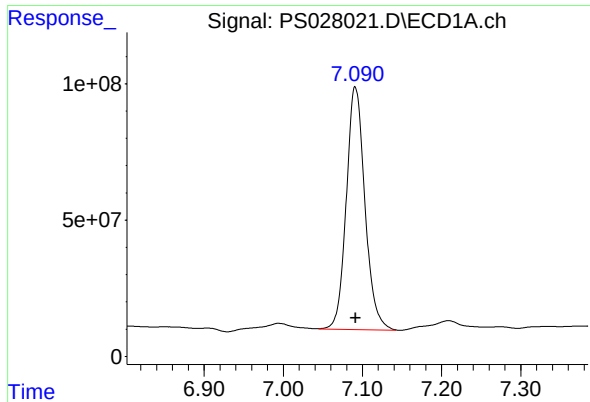

#4 2,4-DCAA


R.T.: 7.090 min  
Delta R.T.: 0.000 min  
Response: 1457105034  
Conc: 540.28 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
PB174307BL

Manual Integrations  
APPROVED

Reviewed By :Abdul  
Mirza  
10/24/2024

Supervised By :Ankita  
Jodhani  
10/24/2024

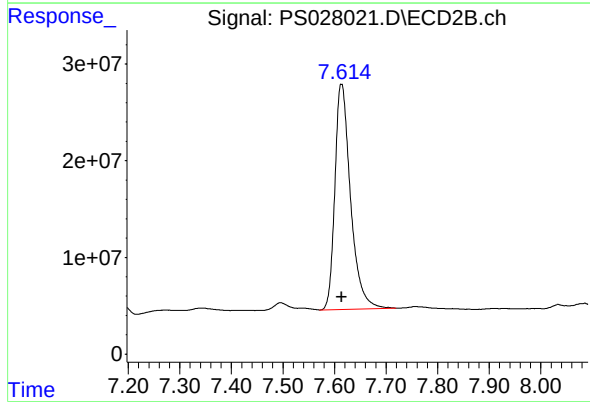

#4 2,4-DCAA

R.T.: 7.613 min  
Delta R.T.: 0.000 min  
Response: 491490441  
Conc: 518.08 ng/ml