

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102325\
 Data File : PS032130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2025 09:16
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 17:30:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.281	0.000	1254776	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.448	0.000	784687	0	<MDL	N.D. #
5) T	DICAMBA	7.470	7.951	1528995	1122432	<MDL	<MDL #
7) T	MCPA	7.793	0.000	983414	0	<MDL	N.D. #
8) T	DICHLORPROP	8.185	0.000	5258811	0	1.106	N.D. #
9) T	2,4-D	8.410	0.000	3749036	0	<MDL	N.D. #
10) T	Pentachlo...	8.707	9.508	17322589	11520444	<MDL	<MDL #
11) T	2,4,5-TP ...	9.295	9.905	5318449	16575640	<MDL	<MDL #
12) T	2,4,5-T	9.570	10.365f	2979590	12566304	<MDL	<MDL #
13) T	2,4-DB	10.157	0.000	975053	0	<MDL	N.D. #
14) T	DINOSEB	11.349	0.000	10035299	0	<MDL	N.D. #
15) T	Picloram	11.193	0.000	14072454	0	<MDL	N.D. #
16) T	DCPA	11.651	12.317	17787476	31308693	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102325\
Data File : PS032130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2025 09:16
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 17:30:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

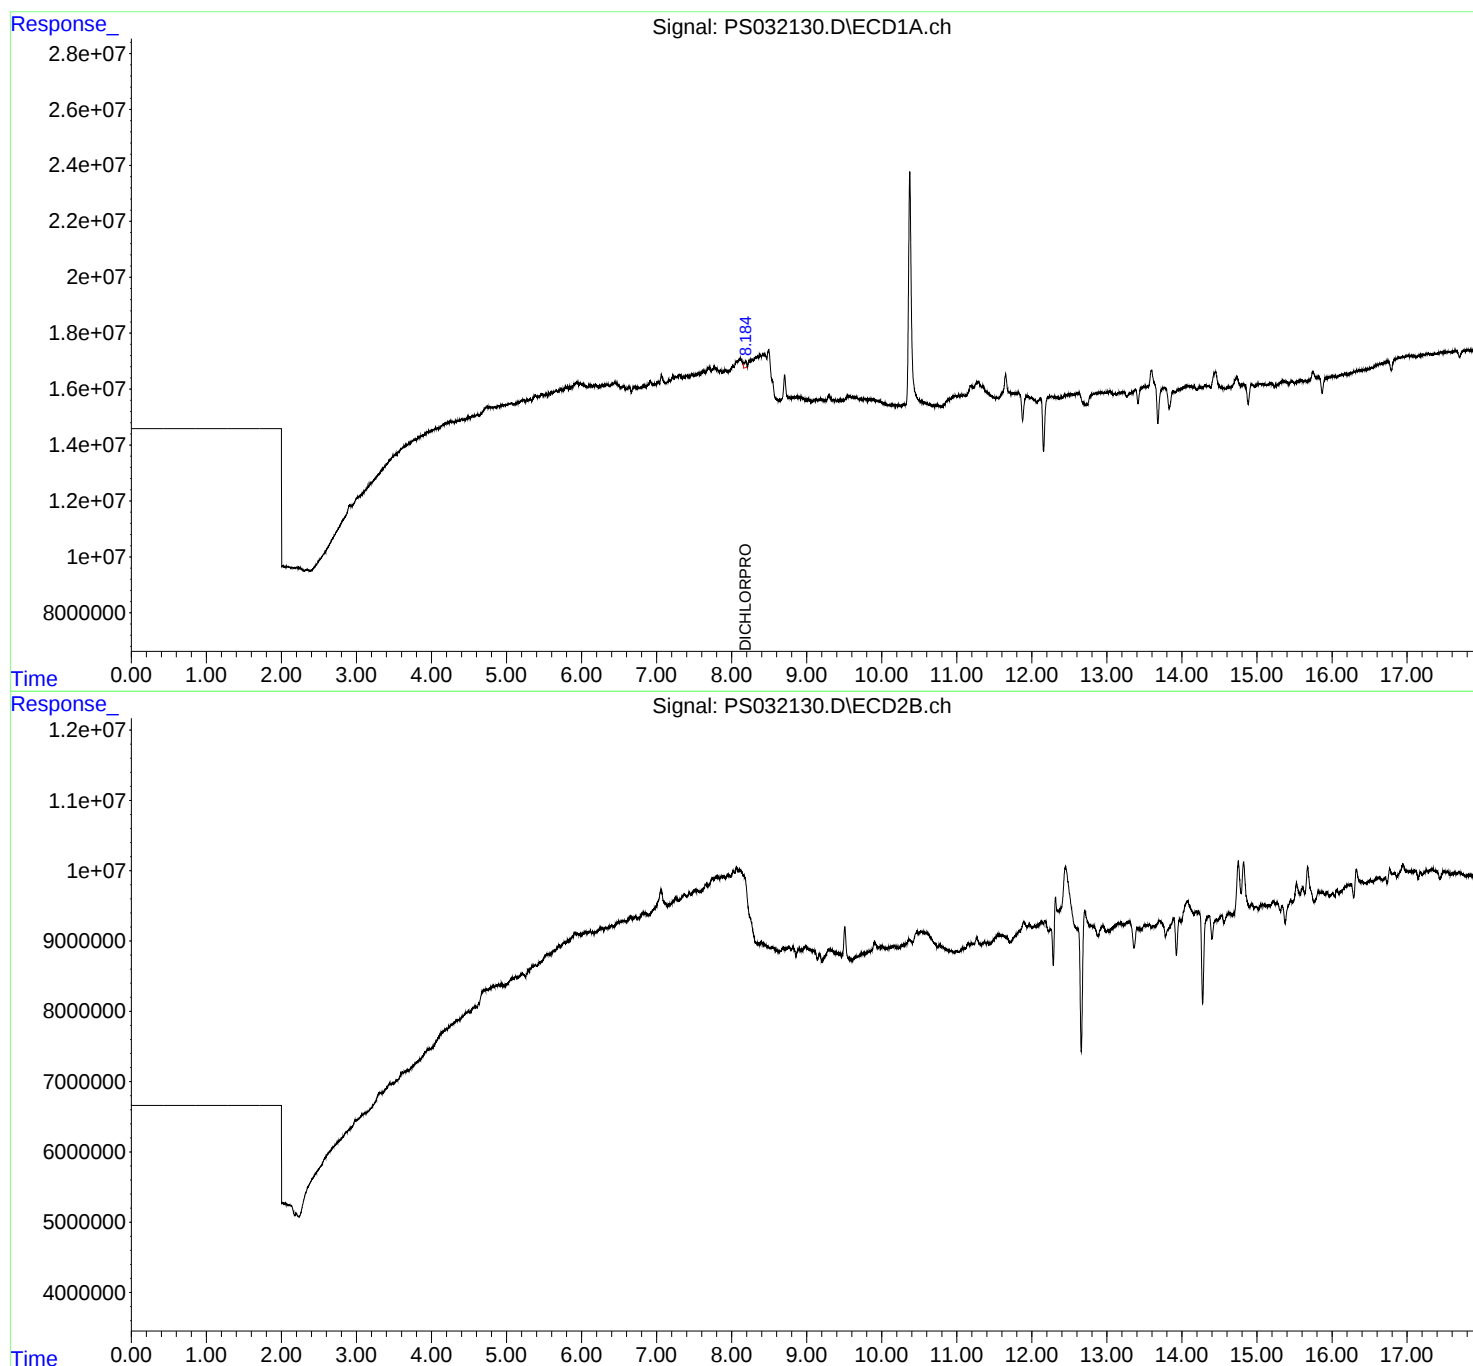


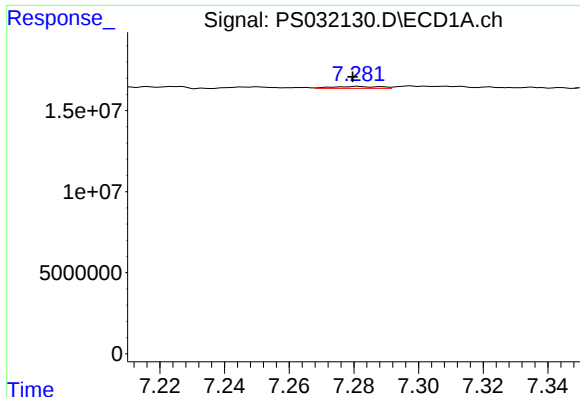

#4 2,4-DCAA


R.T.: 7.281 min
Delta R.T.: 0.002 min
Response: 1254776
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

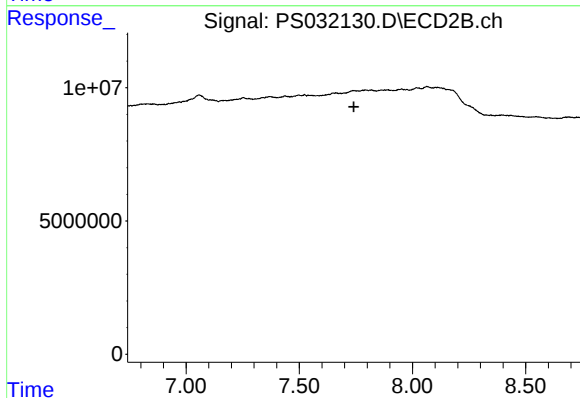


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.741 min
Response: 0
Conc: N.D.

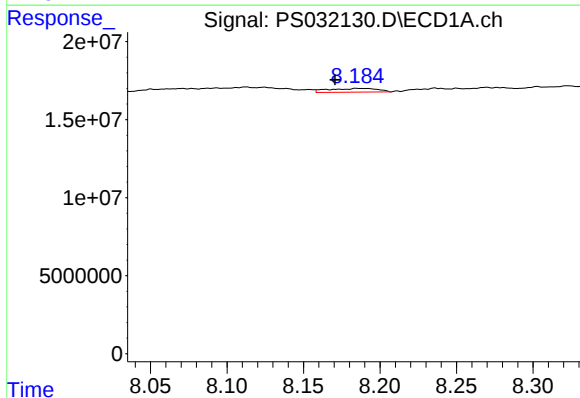

#8 DICHLORPROP

R.T.: 8.185 min
Delta R.T.: 0.015 min
Response: 5258811
Conc: 1.11 ng/ml

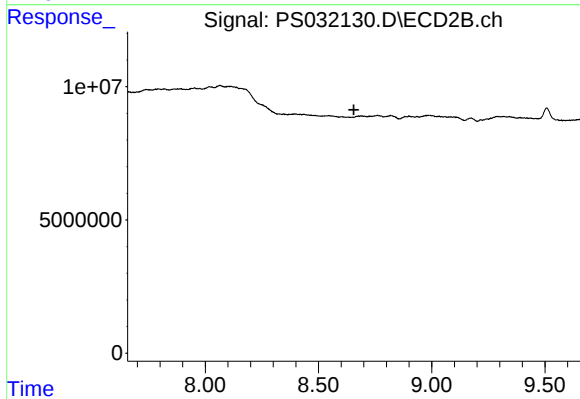

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.656 min
Response: 0
Conc: N.D.