

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102325\
 Data File : PS032131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2025 09:40
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 17:30:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.751	1941.5E6	554.4E6	407.269	503.869
Target Compounds							
1) T	Dalapon	2.680	2.738f	6528218	76526707	<MDL	20.362 #
2) T	3,5-DICHL...	6.445	0.000	213827	0	<MDL	N.D. #
7) T	MCPA	0.000	8.246f	0	19145436	N.D.	5.075
8) T	DICHLORPROP	8.185	0.000	1748466	0	<MDL	N.D. #
9) T	2,4-D	0.000	9.013	0	4232262	N.D.	2.036
10) T	Pentachlo...	8.707	9.515	19895653	10596233	<MDL	<MDL #
11) T	2,4,5-TP ...	9.299	9.916f	27184962	13315591	<MDL	<MDL #
12) T	2,4,5-T	9.609f	10.304	5855273	2603056	<MDL	<MDL #
13) T	2,4-DB	10.163	0.000	843229	0	<MDL	N.D. #
14) T	DINOSEB	11.351	11.275	32546893	11247852	1.459	<MDL #
15) T	Picloram	11.165	0.000	2407907	0	<MDL	N.D. #
16) T	DCPA	11.647	12.313	50629630	32292315	1.378	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102325\
Data File : PS032131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2025 09:40
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 17:30:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

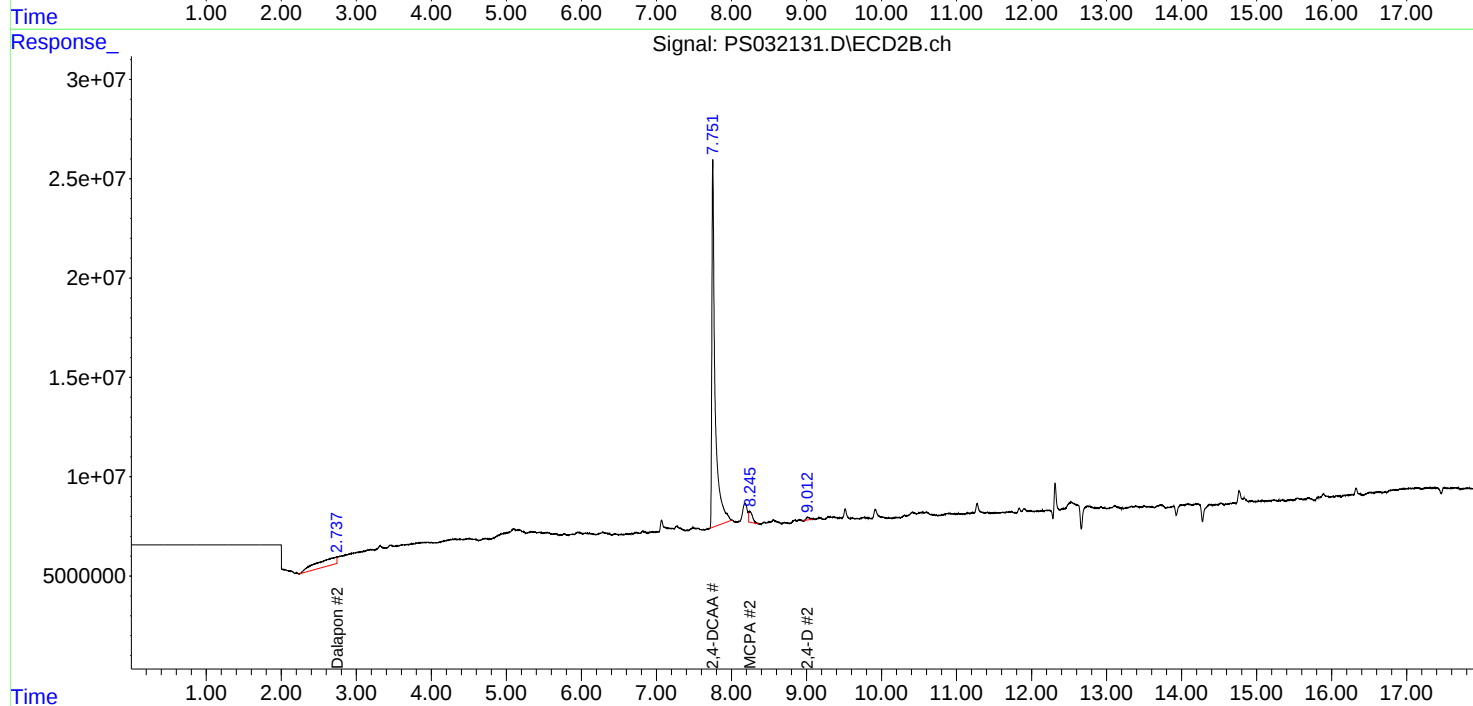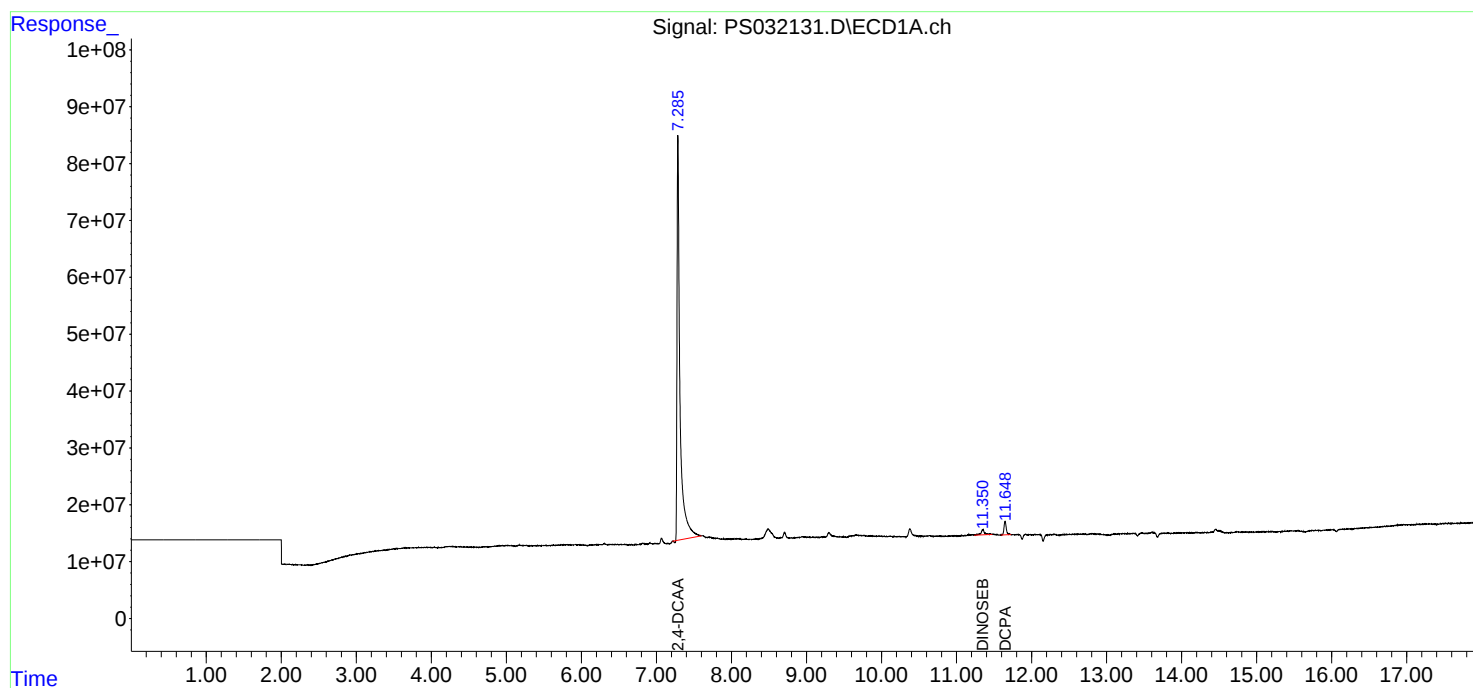


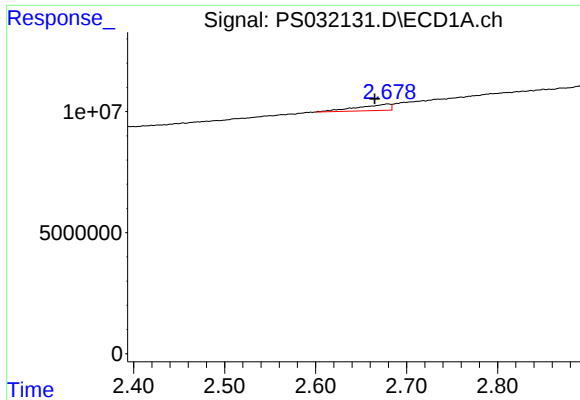

#1 Dalapon


R.T.: 2.680 min
Delta R.T.: 0.015 min
Response: 6528218
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

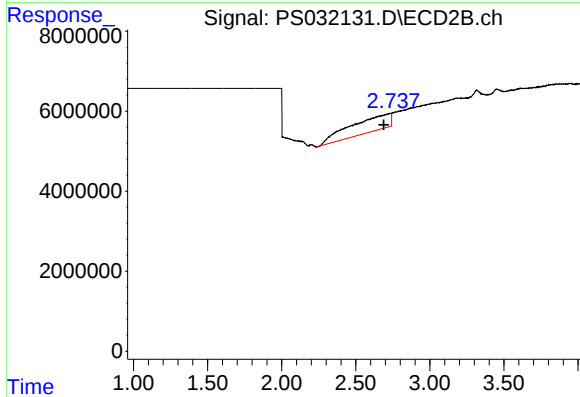


#1 Dalapon

R.T.: 2.738 min
Delta R.T.: 0.049 min
Response: 76526707
Conc: 20.36 ng/ml

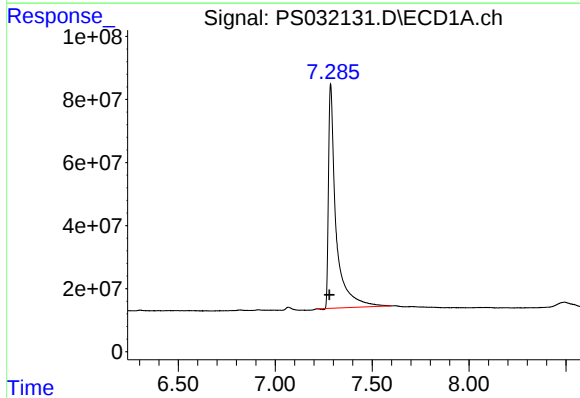


#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: 0.006 min
Response: 1941464997
Conc: 407.27 ng/ml

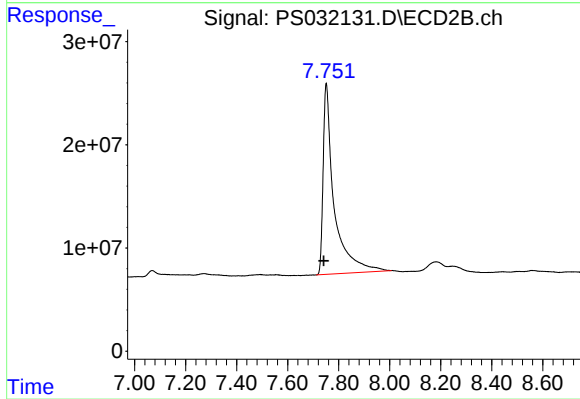

#4 2,4-DCAA


R.T.: 7.751 min
Delta R.T.: 0.010 min
Response: 554427605
Conc: 503.87 ng/ml

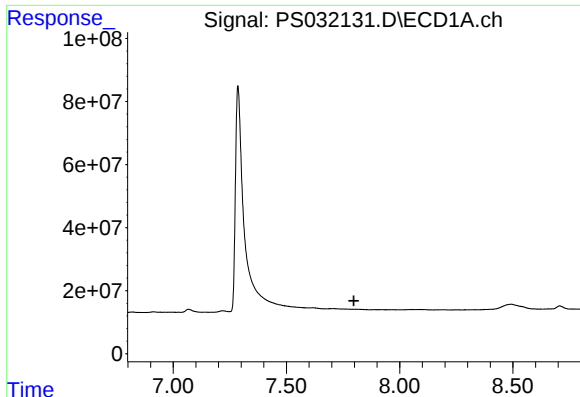

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.798 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

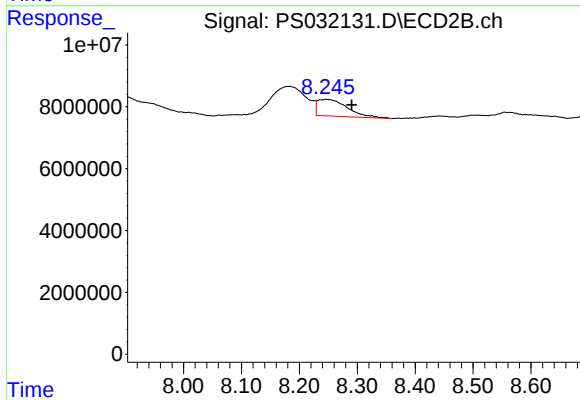


#7 MCPA

R.T.: 8.246 min
Delta R.T.: -0.045 min
Response: 19145436
Conc: 5.08 ug/ml

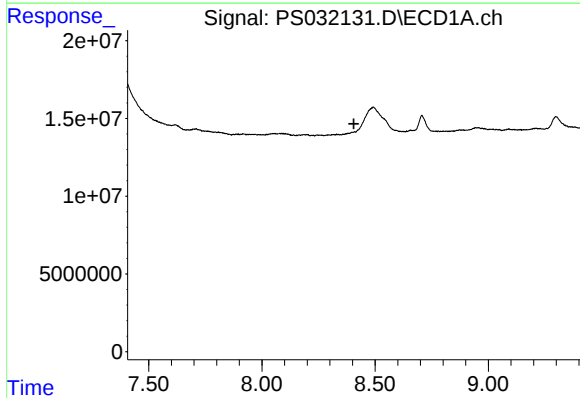


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.406 min
Response: 0
Conc: N.D.

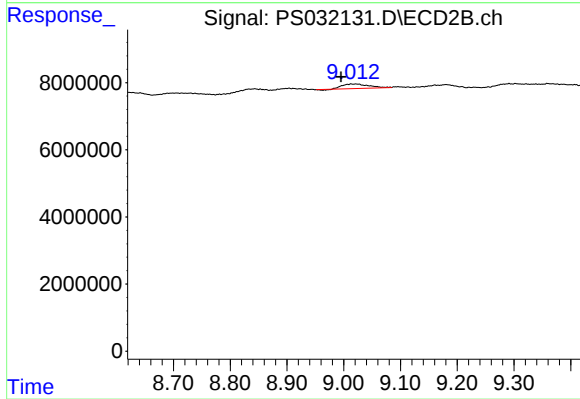

#9 2,4-D


R.T.: 9.013 min
Delta R.T.: 0.018 min
Response: 4232262
Conc: 2.04 ng/ml

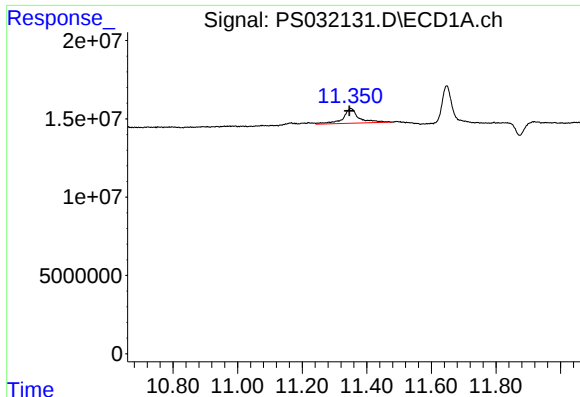

#14 DINOSEB


R.T.: 11.351 min
Delta R.T.: 0.005 min
Response: 32546893
Conc: 1.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

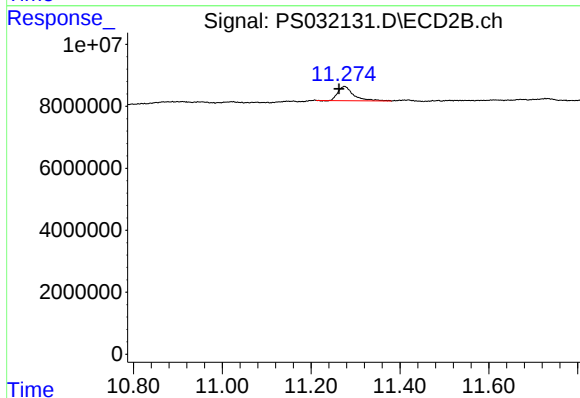


#14 DINOSEB

R.T.: 11.275 min
Delta R.T.: 0.012 min
Response: 11247852
Conc: N.D.

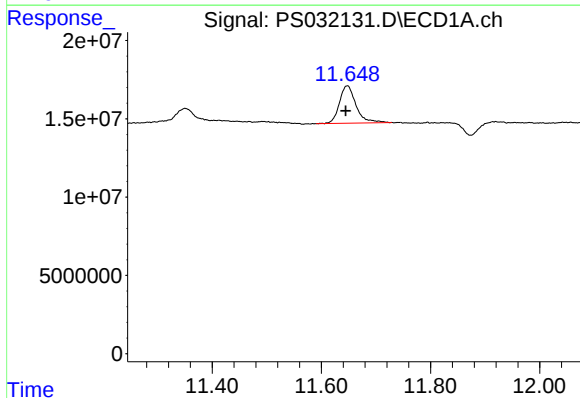

#16 DCPA

R.T.: 11.647 min
Delta R.T.: 0.003 min
Response: 50629630
Conc: 1.38 ng/ml

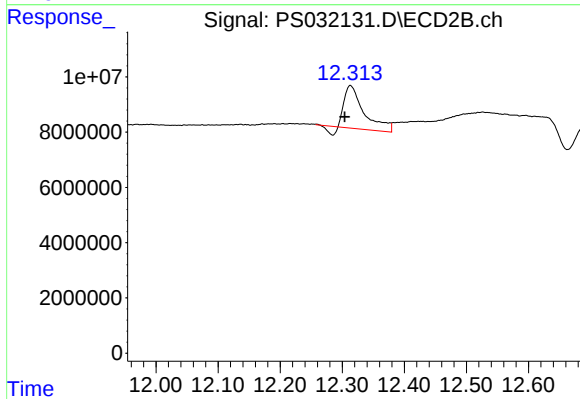

#16 DCPA

R.T.: 12.313 min
Delta R.T.: 0.009 min
Response: 32292315
Conc: N.D.