

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102325\
 Data File : PS032136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2025 11:44
 Operator : AR\AJ
 Sample : Q3399-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-ROLLOFF

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 17:31:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.279	7.744	1988.8E6	485.6E6	417.197	441.325
Target Compounds							
1) T	Dalapon	2.646	2.683	1285.1E6	1212.6E6	166.299	322.652 #
2) T	3,5-DICHL...	6.458	6.723f	94825853	20003058	13.472	9.590 #
3) T	4-Nitroph...	7.138f	7.309	124.6E6	281154	93.382	<MDL #
5) T	DICAMBA	7.484	7.917	19947647	39014755	<MDL	4.505 #
6) T	MCP	7.632	7.997f	1434567	8068685	<MDL	3.251 #
8) T	DICHLORPROP	8.176	8.662	9975608	10612709	2.098	5.419 #
9) T	2,4-D	8.394	9.008	1934000	6139384	<MDL	2.954 #
10) T	Pentachlo...	8.705	9.510	23072876	41524448	<MDL	<MDL #
11) T	2,4,5-TP ...	9.324f	9.878	957.1E6	1450.3E6	33.888	72.242 #
12) T	2,4,5-T	0.000	10.350f	0	71990609	N.D.	4.199
13) T	2,4-DB	10.180f	10.851f	84519055	45045807	27.261	34.863 #
14) T	DINOSEB	11.309f	11.278	631.9E6	1145.3E6	28.333	75.336 #
15) T	Picloram	11.149	0.000	9061977	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102325\
Data File : PS032136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2025 11:44
Operator : AR\AJ
Sample : Q3399-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-ROLLOFF

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 17:31:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

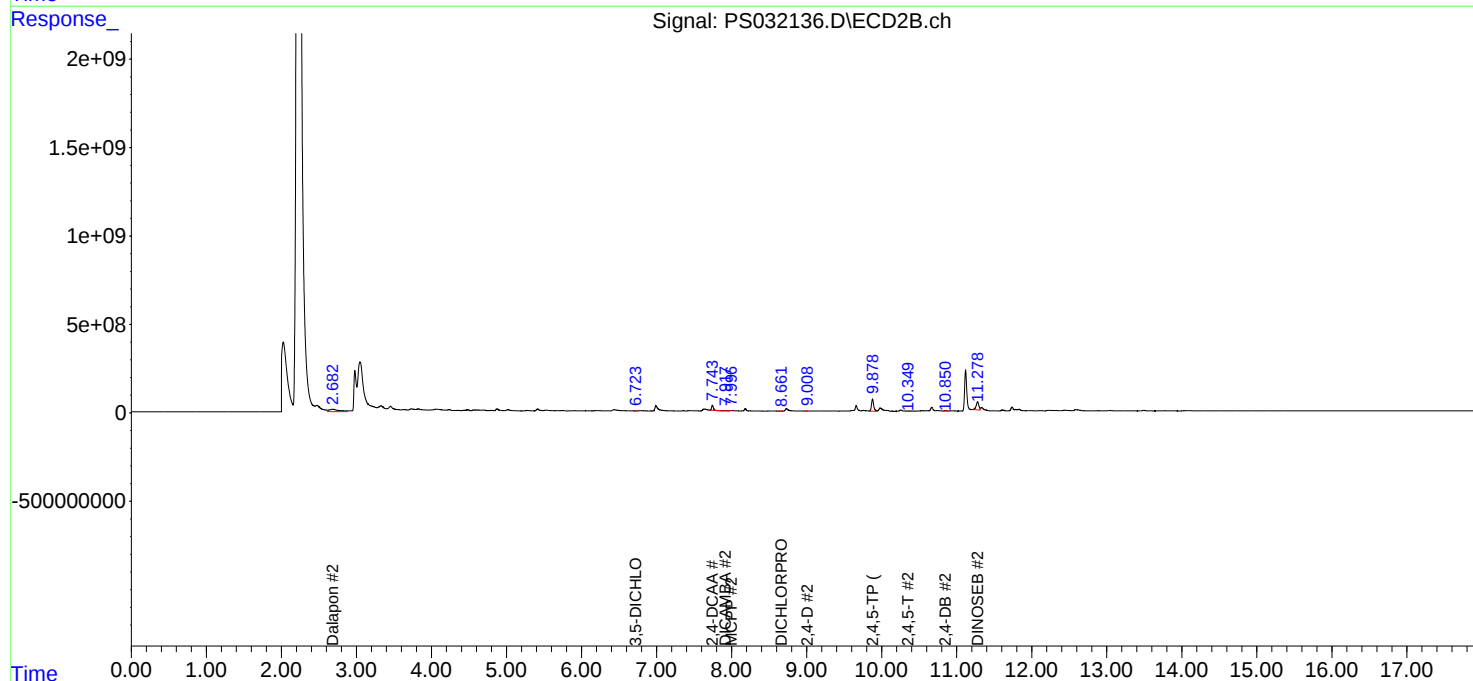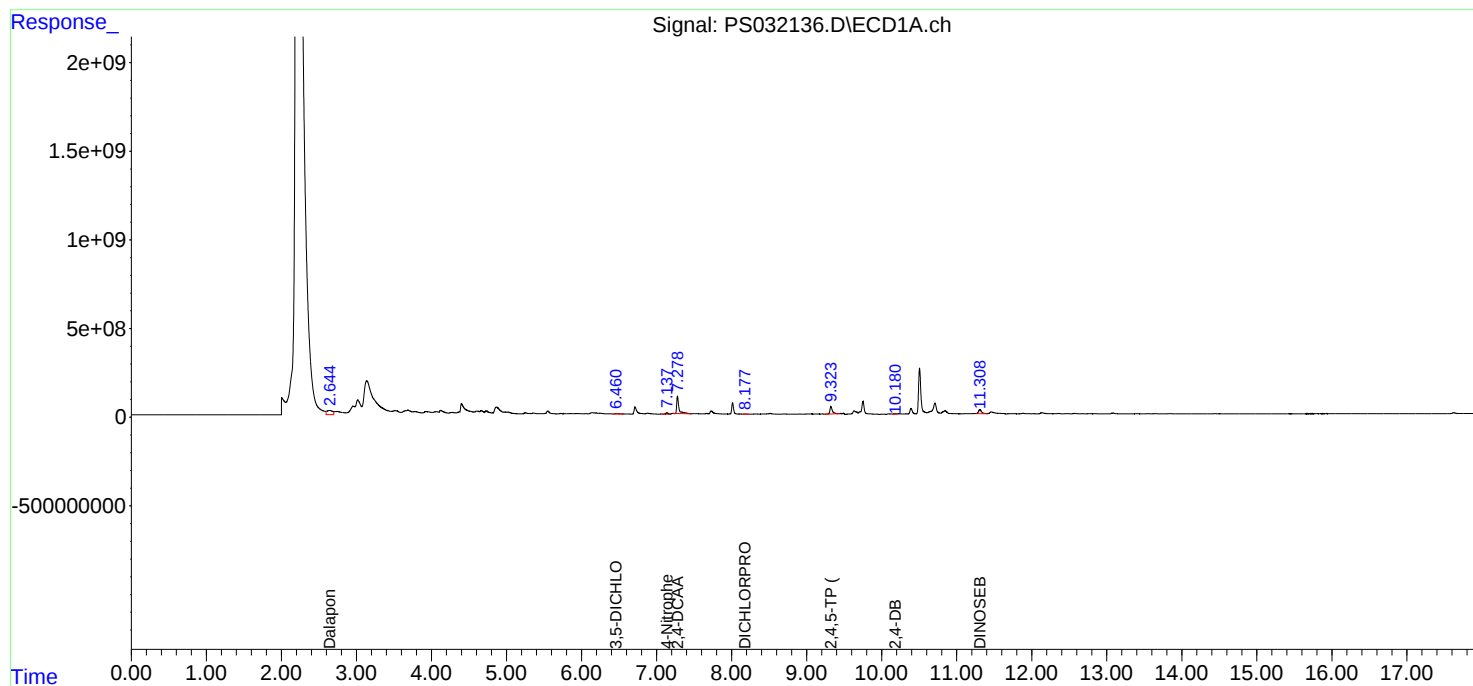


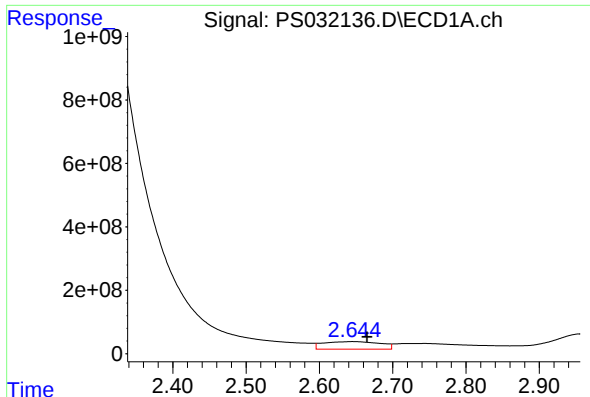

#1 Dalapon


R.T.: 2.646 min
Delta R.T.: -0.019 min
Response: 1285082564
Conc: 166.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-ROLLOFF

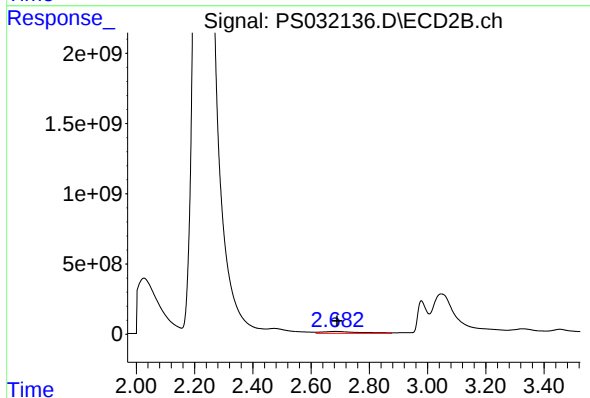


#1 Dalapon

R.T.: 2.683 min
Delta R.T.: -0.006 min
Response: 1212611816
Conc: 322.65 ng/ml

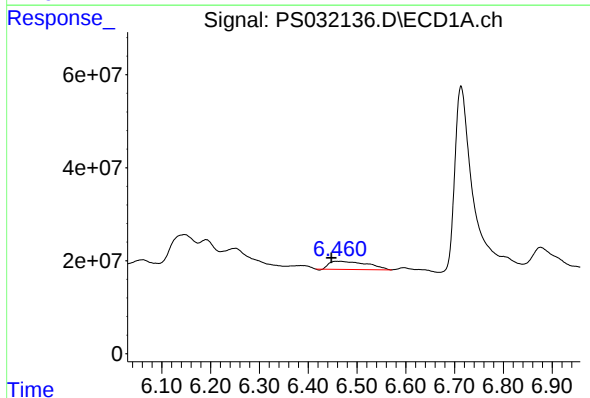


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.458 min
Delta R.T.: 0.010 min
Response: 94825853
Conc: 13.47 ng/ml

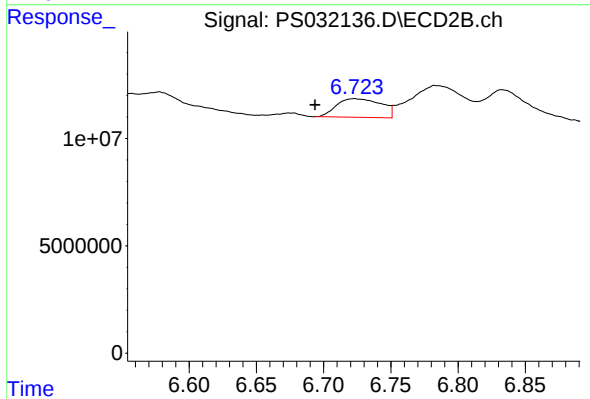

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.723 min
Delta R.T.: 0.029 min
Response: 20003058
Conc: 9.59 ng/ml

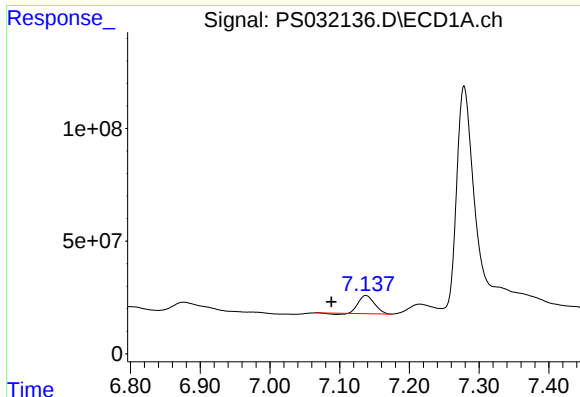

#3 4-Nitrophenol


R.T.: 7.138 min
Delta R.T.: 0.049 min
Response: 124634860
Conc: 93.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-ROLLOFF

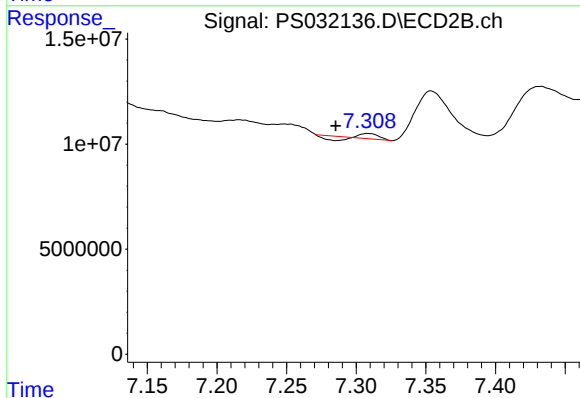


#3 4-Nitrophenol

R.T.: 7.309 min
Delta R.T.: 0.023 min
Response: 281154
Conc: N.D.

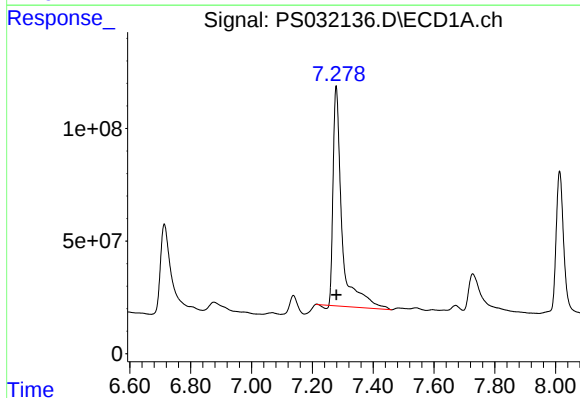


#4 2,4-DCAA

R.T.: 7.279 min
Delta R.T.: 0.000 min
Response: 1988794602
Conc: 417.20 ng/ml

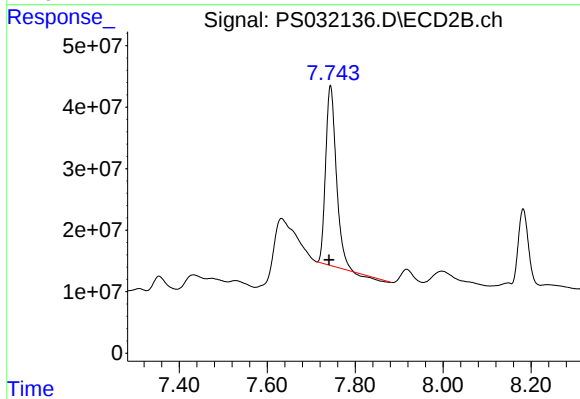

#4 2,4-DCAA


R.T.: 7.744 min
Delta R.T.: 0.003 min
Response: 485607345
Conc: 441.32 ng/ml

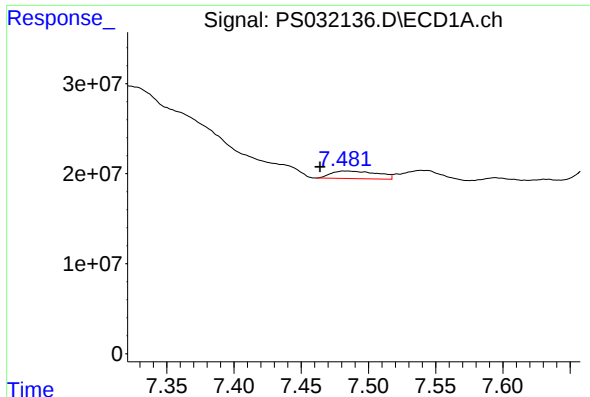

#5 DICAMBA


R.T.: 7.484 min
Delta R.T.: 0.020 min
Response: 19947647
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-ROLLOFF

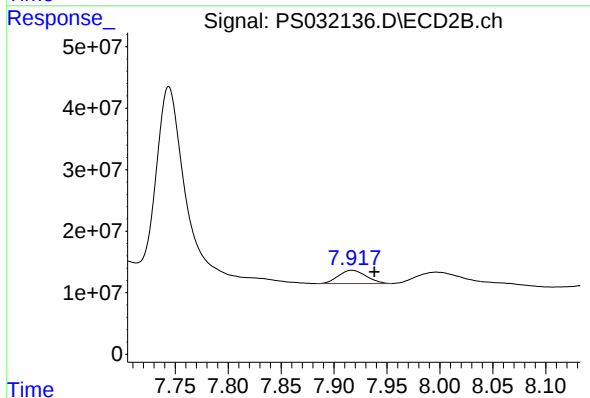


#5 DICAMBA

R.T.: 7.917 min
Delta R.T.: -0.021 min
Response: 39014755
Conc: 4.50 ng/ml

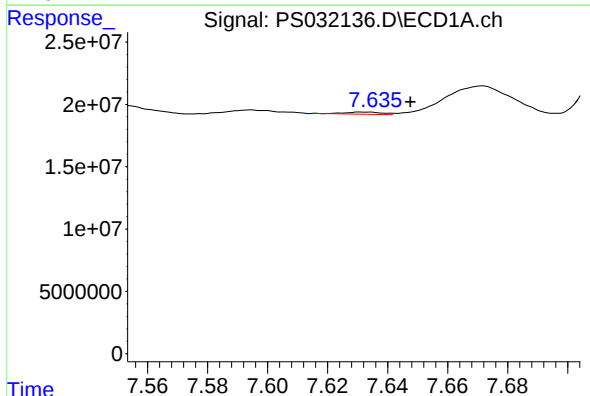


#6 MCP

R.T.: 7.632 min
Delta R.T.: -0.015 min
Response: 1434567
Conc: N.D.

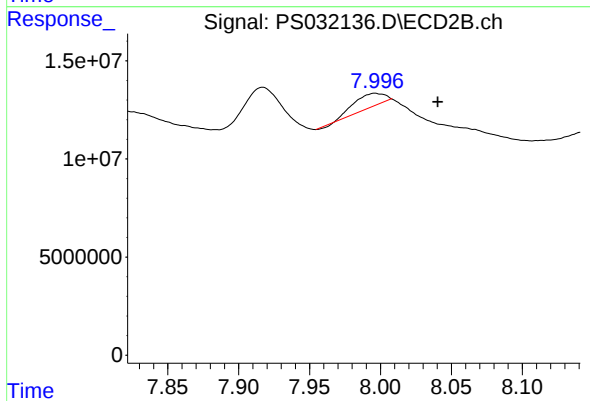

#6 MCP


R.T.: 7.997 min
Delta R.T.: -0.044 min
Response: 8068685
Conc: 3.25 ug/ml

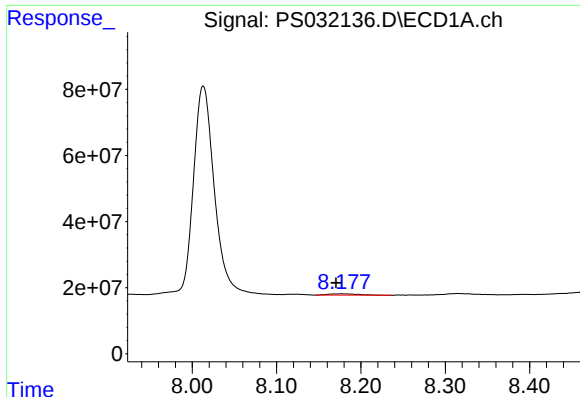

#8 DICHLORPROP


R.T.: 8.176 min
Delta R.T.: 0.005 min
Response: 9975608
Conc: 2.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-ROLLOFF

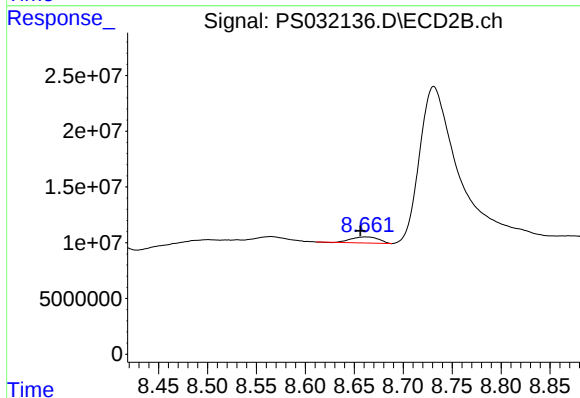


#8 DICHLORPROP

R.T.: 8.662 min
Delta R.T.: 0.006 min
Response: 10612709
Conc: 5.42 ng/ml

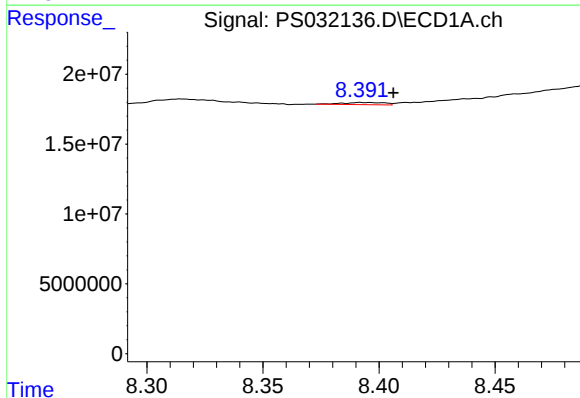


#9 2,4-D

R.T.: 8.394 min
Delta R.T.: -0.012 min
Response: 1934000
Conc: N.D.

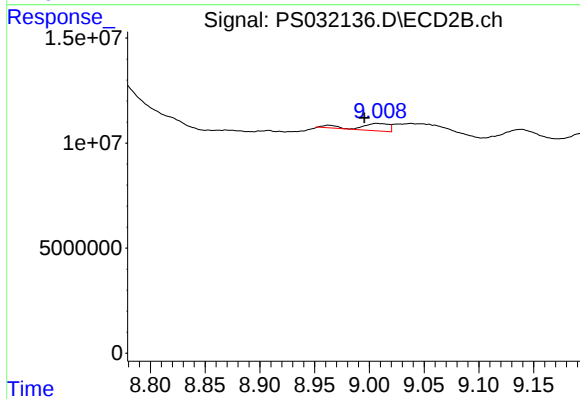

#9 2,4-D


R.T.: 9.008 min
Delta R.T.: 0.012 min
Response: 6139384
Conc: 2.95 ng/ml

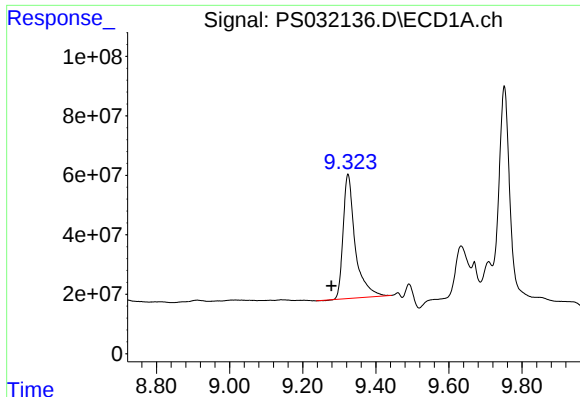

#11 2,4,5-TP (SILVEX)


R.T.: 9.324 min
Delta R.T.: 0.046 min
Response: 957072815
Conc: 33.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-ROLLOFF

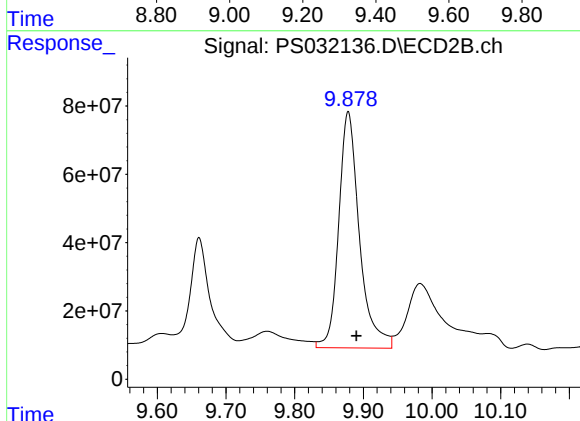


#11 2,4,5-TP (SILVEX)

R.T.: 9.878 min
Delta R.T.: -0.012 min
Response: 1450251499
Conc: 72.24 ng/ml

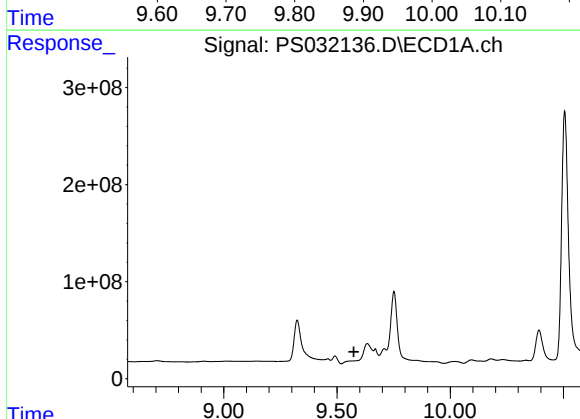


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.574 min
Response: 0
Conc: N.D.

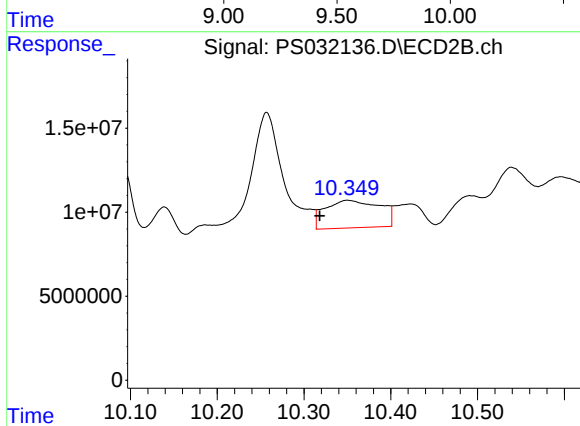

#12 2,4,5-T


R.T.: 10.350 min
Delta R.T.: 0.032 min
Response: 71990609
Conc: 4.20 ng/ml

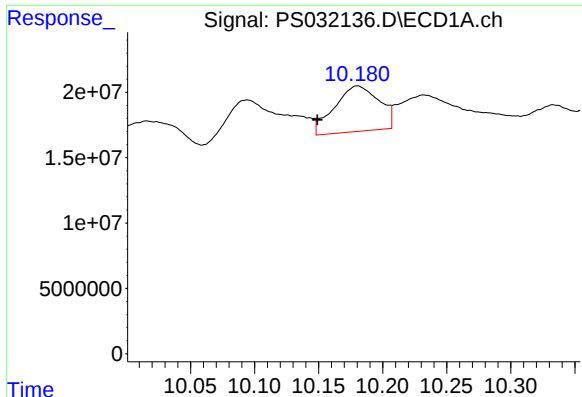

#13 2,4-DB


R.T.: 10.180 min
Delta R.T.: 0.031 min
Response: 84519055
Conc: 27.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-ROLLOFF

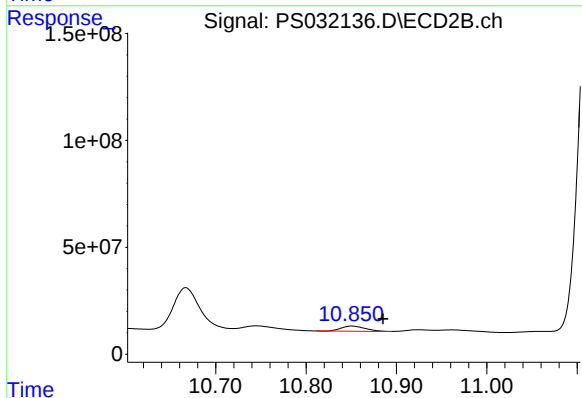


#13 2,4-DB

R.T.: 10.851 min
Delta R.T.: -0.034 min
Response: 45045807
Conc: 34.86 ng/ml

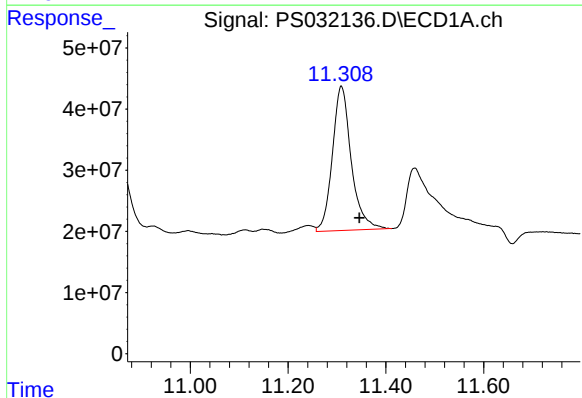

#14 DINOSEB

R.T.: 11.309 min
Delta R.T.: -0.037 min
Response: 631859113
Conc: 28.33 ng/ml

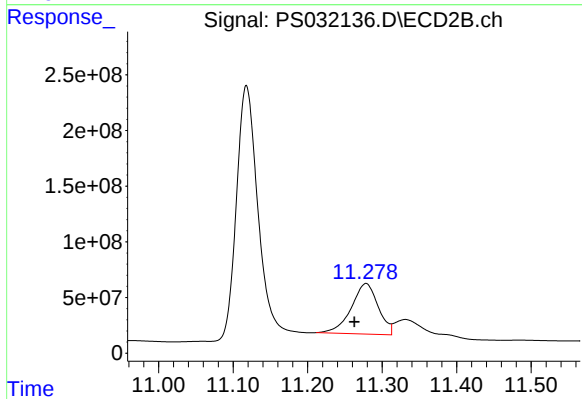

#14 DINOSEB

R.T.: 11.278 min
Delta R.T.: 0.015 min
Response: 1145341032
Conc: 75.34 ng/ml