

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102325\
 Data File : PS032143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2025 14:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 04:41:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.281	7.748	1982.9E6	556.5E6	415.955	505.763
Target Compounds							
2) T	3,5-DICHL...	6.452	0.000	2055815	0	<MDL	N.D. #
6) T	MCP	7.646	0.000	56344	0	<MDL	N.D. #
7) T	MCPA	7.819	8.255f	735369	19073058	<MDL	5.056 #
8) T	DICHLORPROP	8.187	0.000	1007250	0	<MDL	N.D. #
10) T	Pentachlo...	8.710	9.510	5188093	2506703	<MDL	<MDL #
11) T	2,4,5-TP ...	9.280	9.868	8766205	376523	<MDL	<MDL #
12) T	2,4,5-T	9.576	10.303	1680924	1567374	<MDL	<MDL #
13) T	2,4-DB	10.176f	0.000	4077286	0	1.315	N.D. #
14) T	DINOSEB	11.348	0.000	3009232	0	<MDL	N.D. #
15) T	Picloram	11.178	0.000	4623778	0	<MDL	N.D. #
16) T	DCPA	0.000	12.315	0	3557276	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102325\
Data File : PS032143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2025 14:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 04:41:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

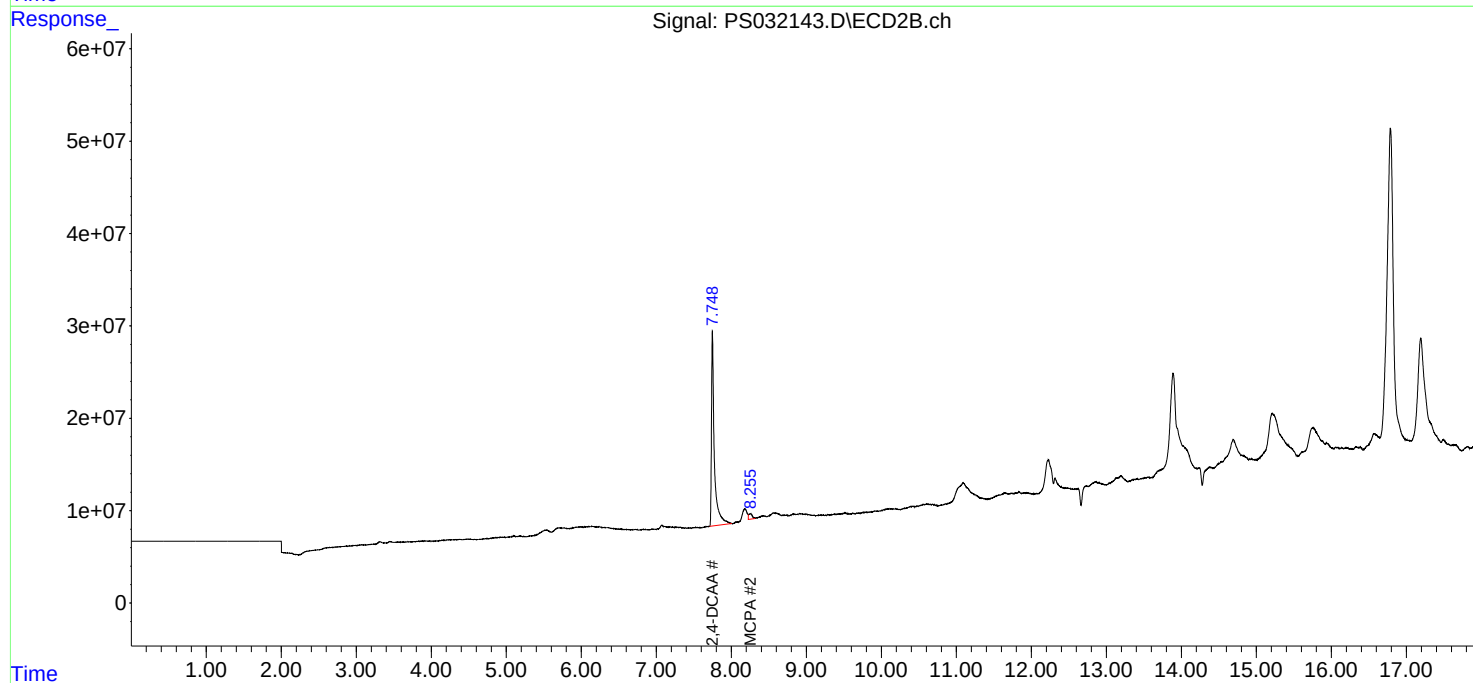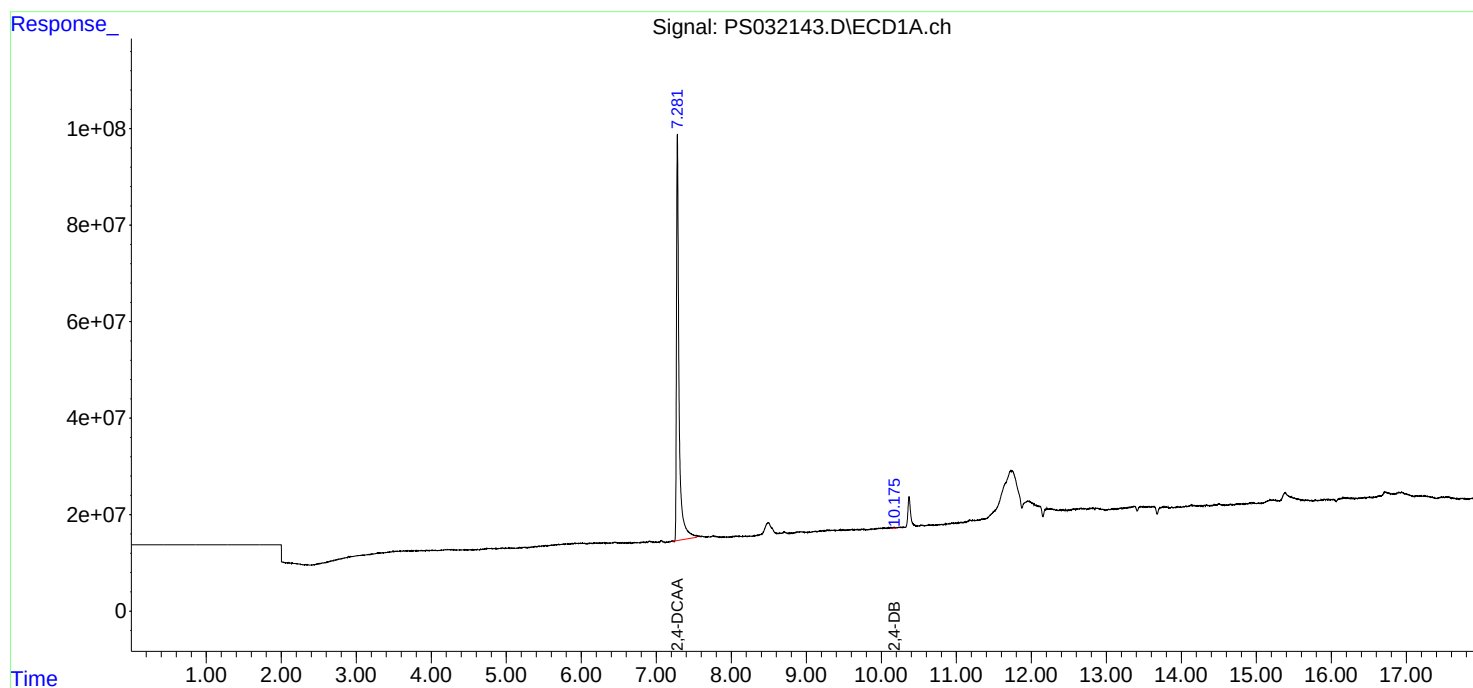


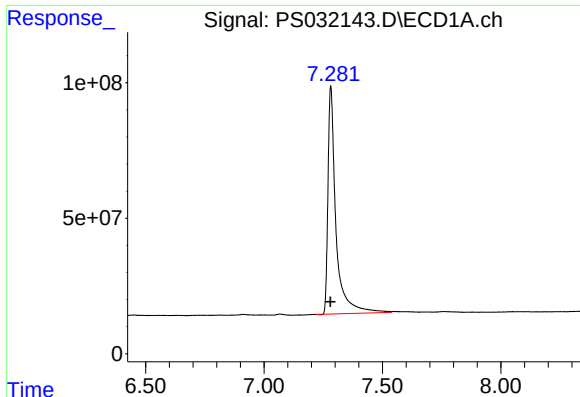

#4 2,4-DCAA


R.T.: 7.281 min
Delta R.T.: 0.002 min
Response: 1982873183
Conc: 415.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

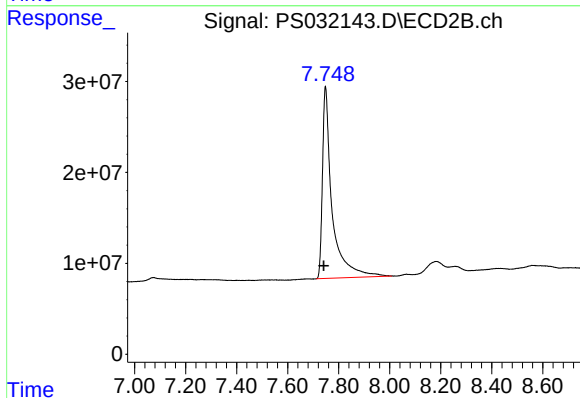


#4 2,4-DCAA

R.T.: 7.748 min
Delta R.T.: 0.007 min
Response: 556511907
Conc: 505.76 ng/ml

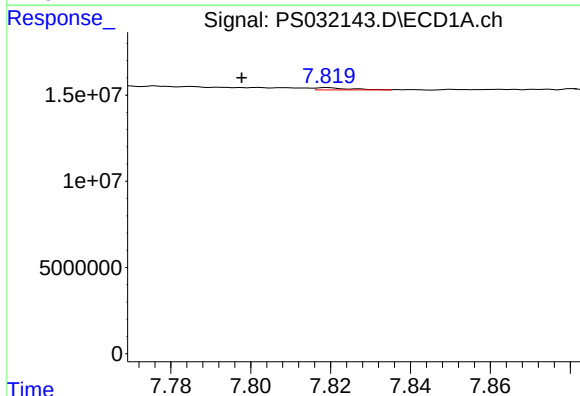


#7 MCPA

R.T.: 7.819 min
Delta R.T.: 0.021 min
Response: 735369
Conc: N.D.

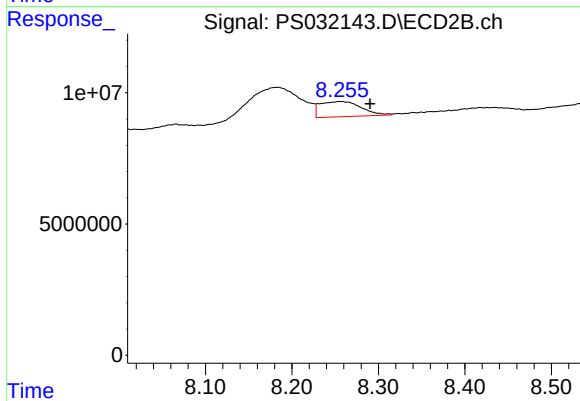

#7 MCPA


R.T.: 8.255 min
Delta R.T.: -0.035 min
Response: 19073058
Conc: 5.06 ug/ml

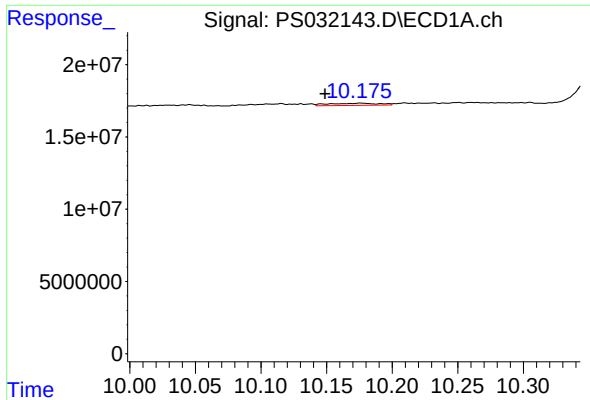

#13 2,4-DB

R.T.: 10.176 min
Delta R.T.: 0.027 min
Response: 4077286
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

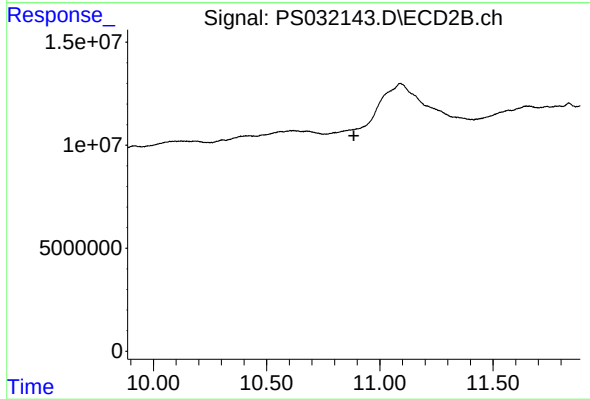

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.885 min
Response: 0
Conc: N.D.