

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102418\
 Data File : PS002107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2018 15:28
 Operator : EI\SJ
 Sample : J5610-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:25:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.442	10.934	18375575	21751604	86.922	91.199
Target Compounds							
1) T	Dalapon	2.878	2.360	48230441	69603504	158.051	238.395 #
5) T	DICAMBA	11.736	11.176	2731725	27687917	3.471	33.696 #
6) T	MCPD	12.126	11.401	30218726	3717575	53.967	6.812 #
8) T	DICHLORPROP	0.000	12.355	0	1617430	N.D.	7.384 #
10) T	Pentachlo...	13.683	13.364	10421690	4922998	3.683	1.555 #
11) T	2,4,5-TP ...	0.000	13.960	0	3803688	N.D.	2.994 #
13) T	2,4-DB	15.690	15.190	18863357	17275532	120.095	109.739
14) T	DINOSEB	17.124	15.672	1508299	18585414	1.802	21.014 #
15) T	Picloram	17.005	0.000	3091999	0	1.808	N.D. #
16) T	DCPA	17.468	0.000	19974361	0	14.410	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102418\
Data File : PS002107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2018 15:28
Operator : EI\SJ
Sample : J5610-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:25:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

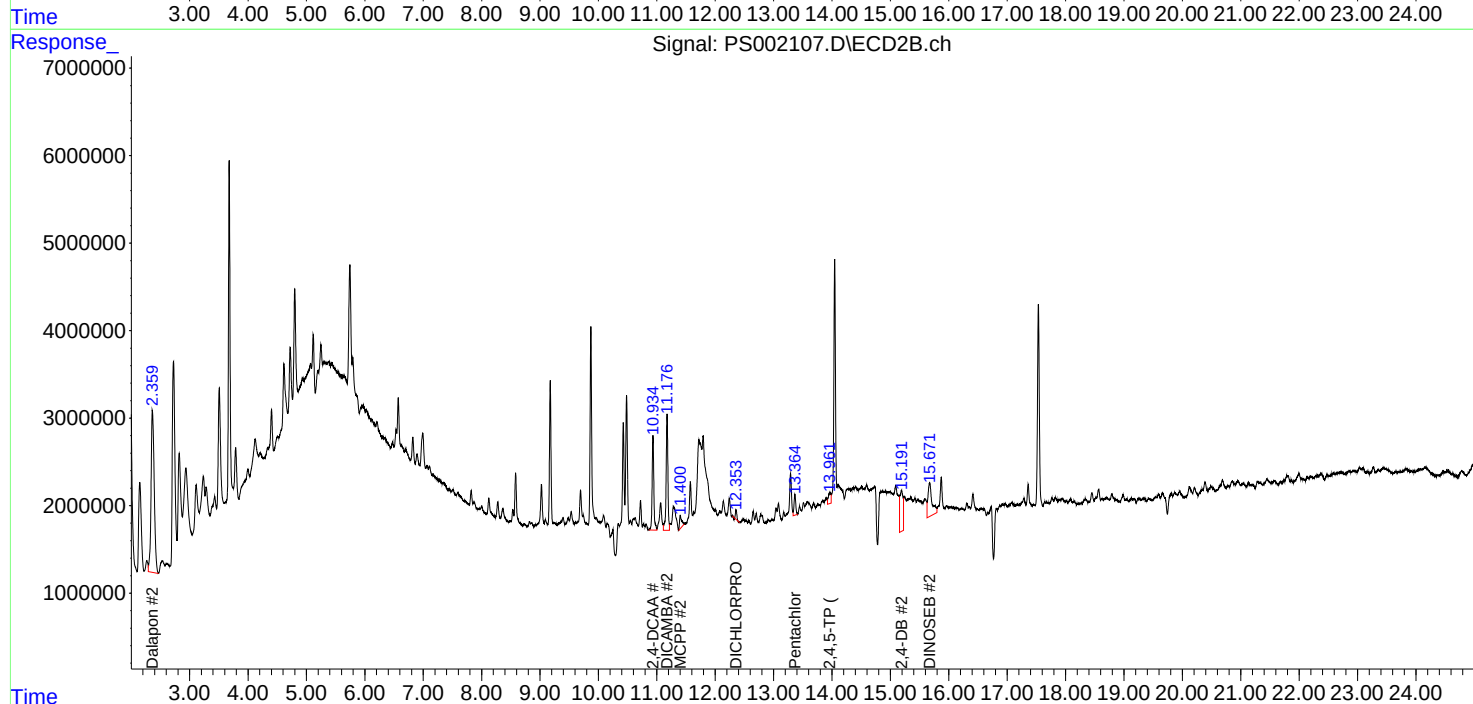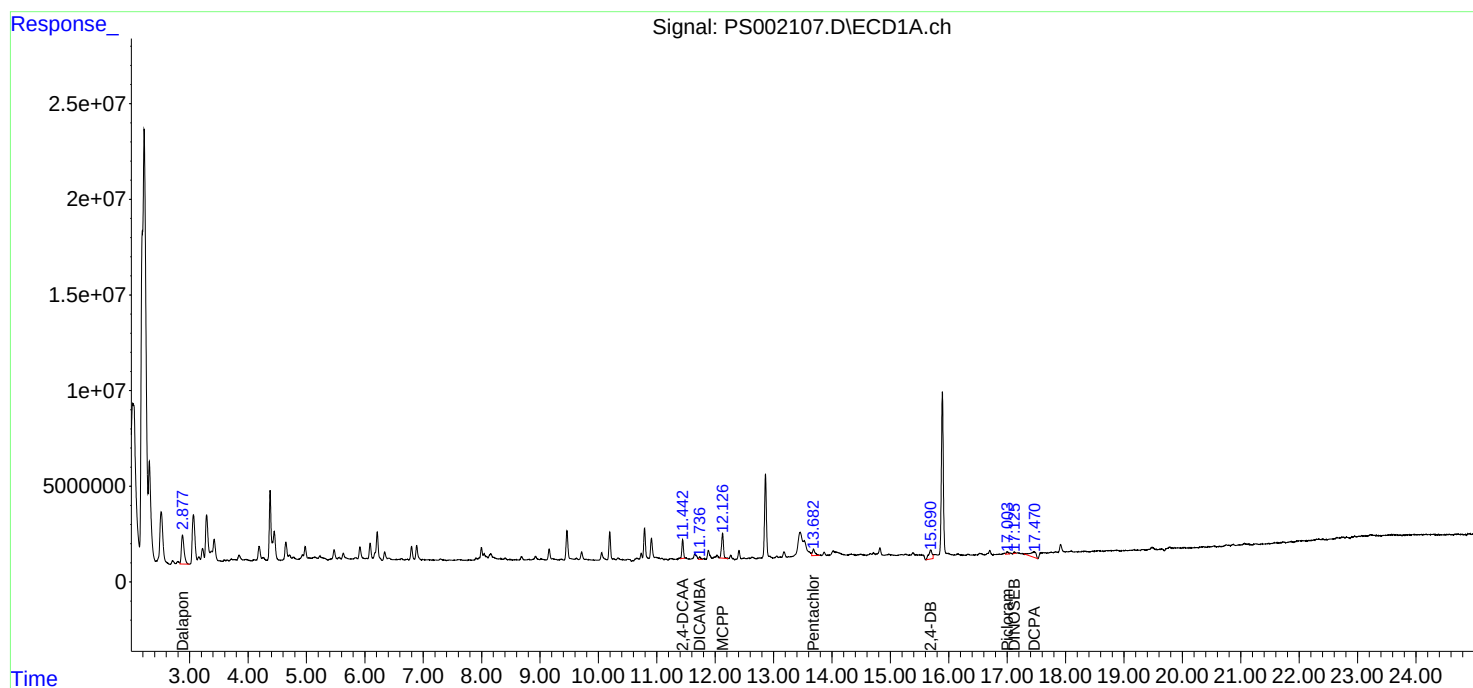


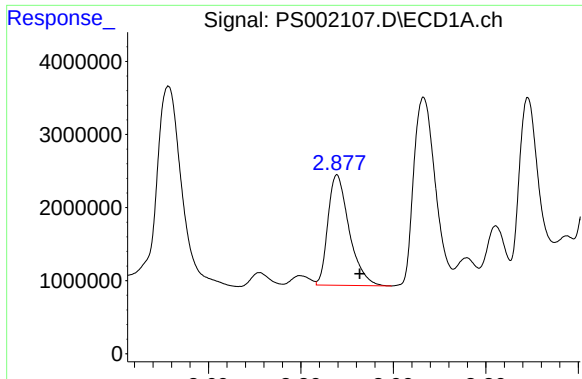

#1 Dalapon


R.T.: 2.878 min
Delta R.T.: -0.049 min
Response: 48230441
Conc: 158.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

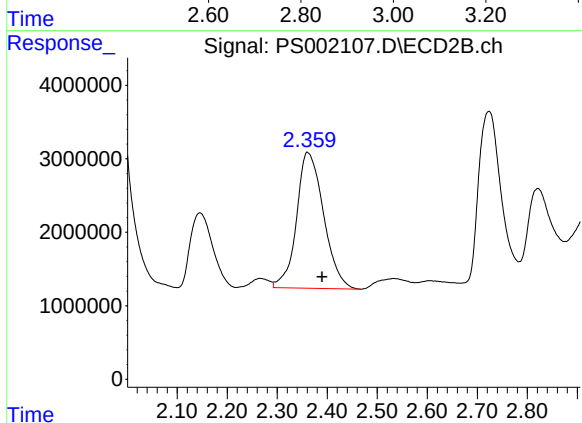


#1 Dalapon

R.T.: 2.360 min
Delta R.T.: -0.030 min
Response: 69603504
Conc: 238.40 ng/ml

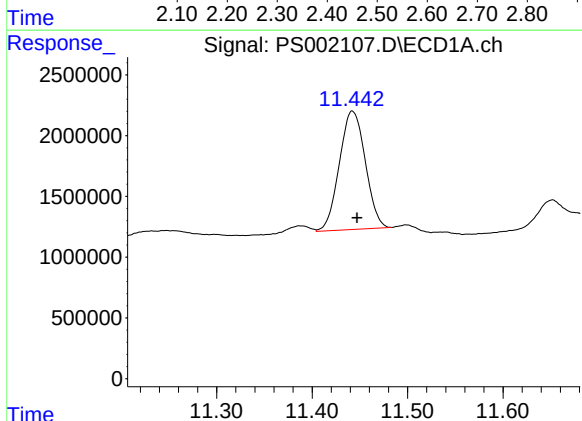


#4 2,4-DCAA

R.T.: 11.442 min
Delta R.T.: -0.004 min
Response: 18375575
Conc: 86.92 ng/ml

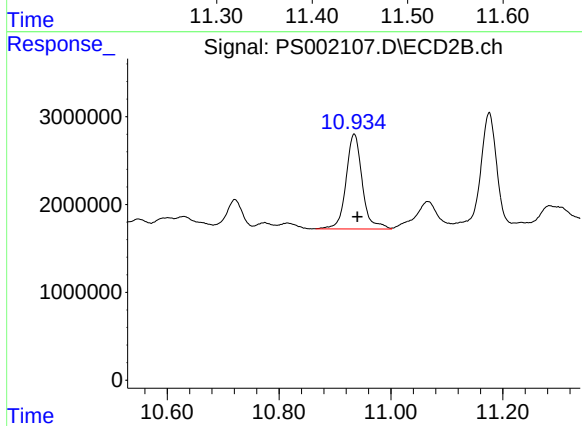

#4 2,4-DCAA


R.T.: 10.934 min
Delta R.T.: -0.006 min
Response: 21751604
Conc: 91.20 ng/ml

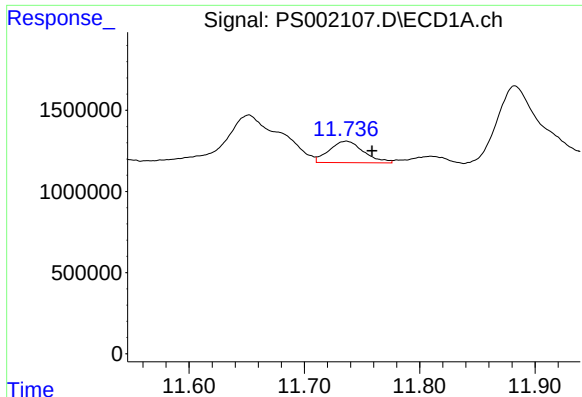

#5 DICAMBA


R.T.: 11.736 min
Delta R.T.: -0.023 min
Response: 2731725
Conc: 3.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

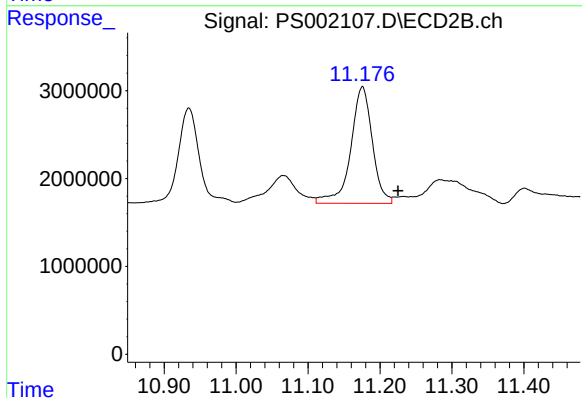


#5 DICAMBA

R.T.: 11.176 min
Delta R.T.: -0.050 min
Response: 27687917
Conc: 33.70 ng/ml

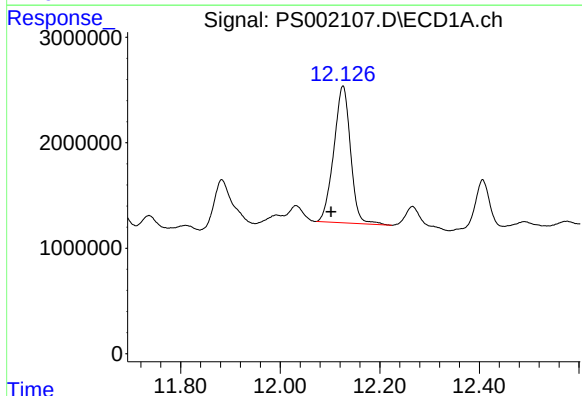


#6 MCP

R.T.: 12.126 min
Delta R.T.: 0.024 min
Response: 30218726
Conc: 53.97 ug/ml

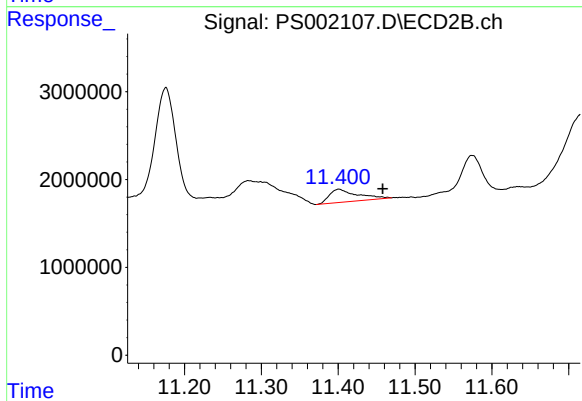

#6 MCP


R.T.: 11.401 min
Delta R.T.: -0.057 min
Response: 3717575
Conc: 6.81 ug/ml

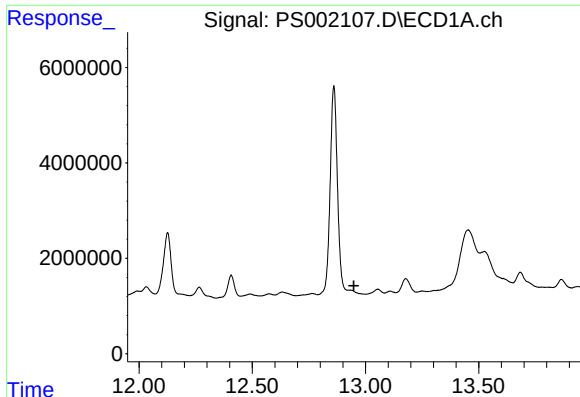

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

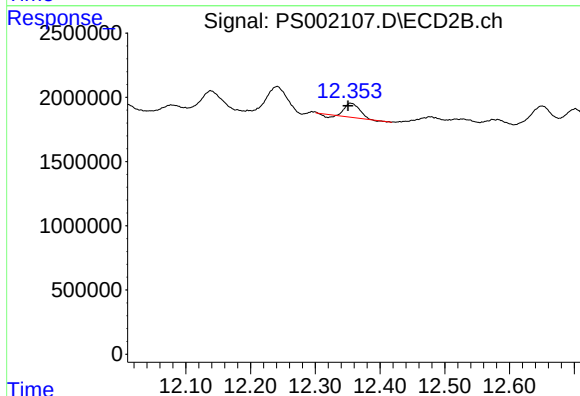


#8 DICHLORPROP

R.T.: 12.355 min
Delta R.T.: 0.004 min
Response: 1617430
Conc: 7.38 ng/ml

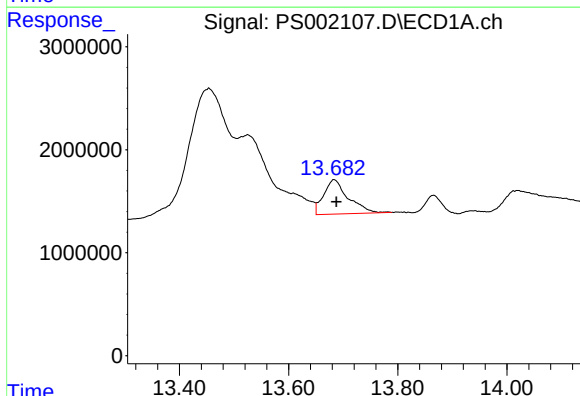


#10 Pentachlorophenol

R.T.: 13.683 min
Delta R.T.: -0.004 min
Response: 10421690
Conc: 3.68 ng/ml

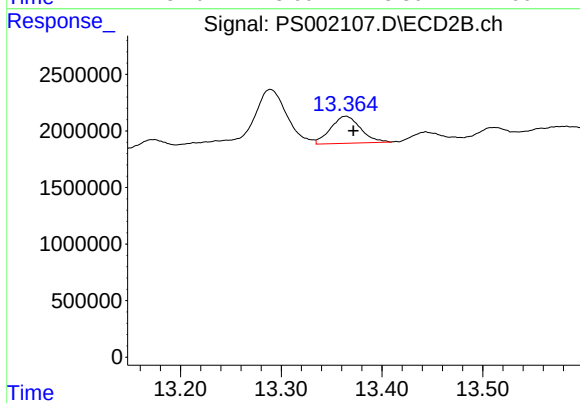

#10 Pentachlorophenol


R.T.: 13.364 min
Delta R.T.: -0.007 min
Response: 4922998
Conc: 1.55 ng/ml

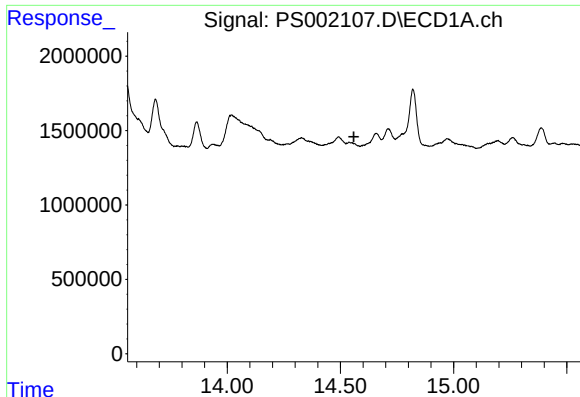

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.560 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

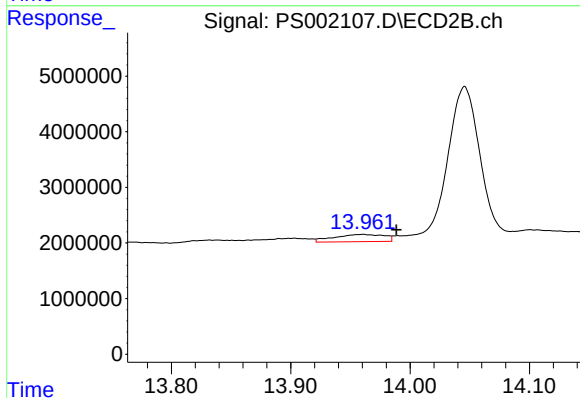


#11 2,4,5-TP (SILVEX)

R.T.: 13.960 min
Delta R.T.: -0.029 min
Response: 3803688
Conc: 2.99 ng/ml

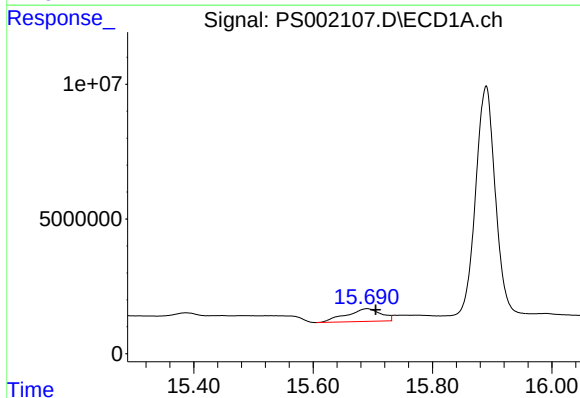


#13 2,4-DB

R.T.: 15.690 min
Delta R.T.: -0.015 min
Response: 18863357
Conc: 120.09 ng/ml

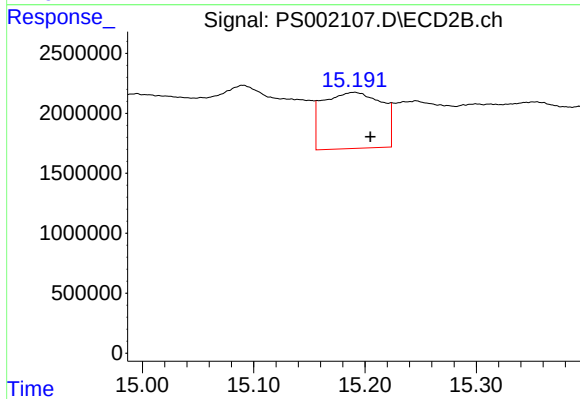

#13 2,4-DB


R.T.: 15.190 min
Delta R.T.: -0.015 min
Response: 17275532
Conc: 109.74 ng/ml

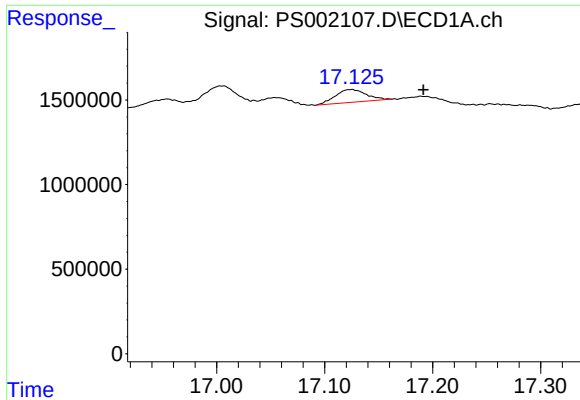

#14 DINOSEB


R.T.: 17.124 min
Delta R.T.: -0.067 min
Response: 1508299
Conc: 1.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

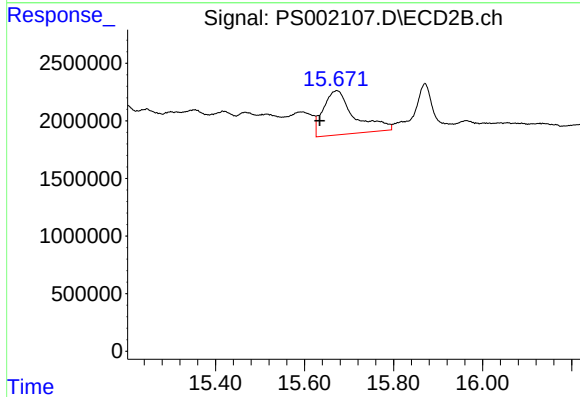


#14 DINOSEB

R.T.: 15.672 min
Delta R.T.: 0.038 min
Response: 18585414
Conc: 21.01 ng/ml

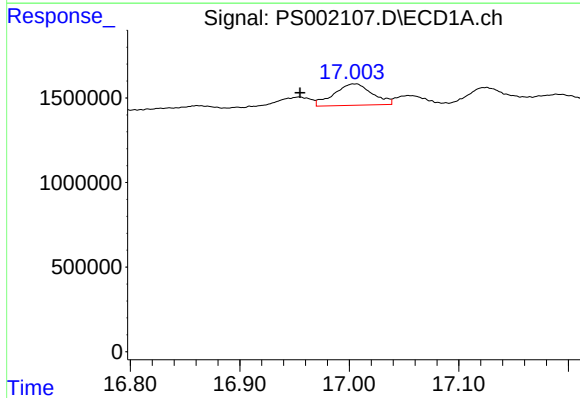


#15 Picloram

R.T.: 17.005 min
Delta R.T.: 0.050 min
Response: 3091999
Conc: 1.81 ng/ml

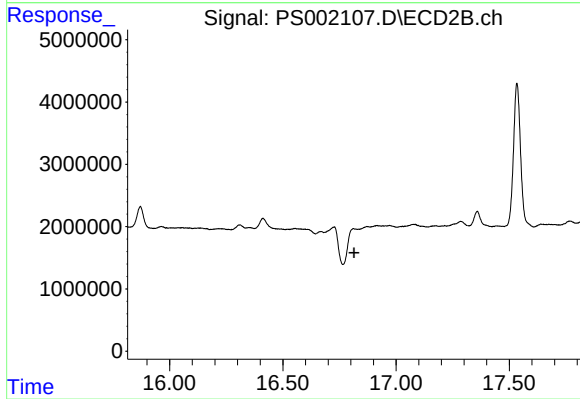

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.814 min
Response: 0
Conc: N.D.

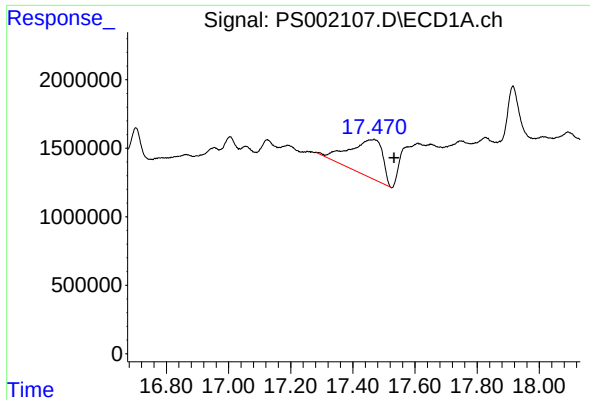

#16 DCPA

R.T.: 17.468 min
Delta R.T.: -0.065 min
Response: 19974361
Conc: 14.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

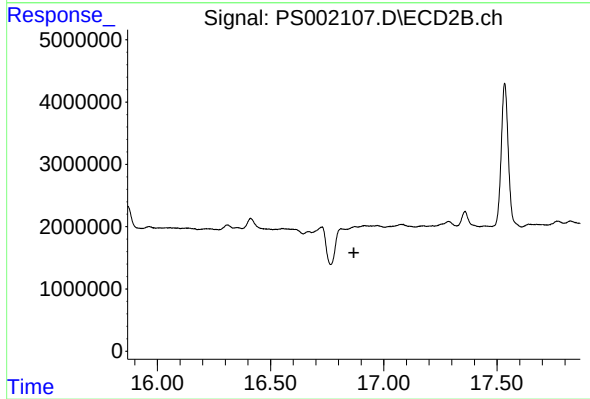

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.868 min
Response: 0
Conc: N.D.