

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102418\
 Data File : PS002115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2018 19:37
 Operator : EI\SJ
 Sample : J5610-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:26:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.458	10.950	23632266	20926058	111.788	87.738
Target Compounds							
1) T	Dalapon	2.894	2.379	49545201	71065289	162.360	243.402 #
2) T	3,5-DICHL...	0.000	9.040	0	1799728	N.D.	6.154 #
5) T	DICAMBA	11.694	11.191	3677102	29523908	4.672	35.930 #
6) T	MCP	12.143	11.448	26313769	2039669	46.993	3.737 #
10) T	Pentachlo...	0.000	13.305	0	10607906	N.D.	3.350 #
13) T	2,4-DB	15.714	15.203	10661672	4043469	67.878	25.685 #
14) T	DINOSEB	0.000	15.695	0	3732439	N.D.	4.220 #
15) T	Picloram	0.000	16.881	0	27604663	N.D.	17.403 #
16) T	DCPA	0.000	16.881	0	27604663	N.D.	15.258 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102418\
Data File : PS002115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2018 19:37
Operator : EI\SJ
Sample : J5610-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:26:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

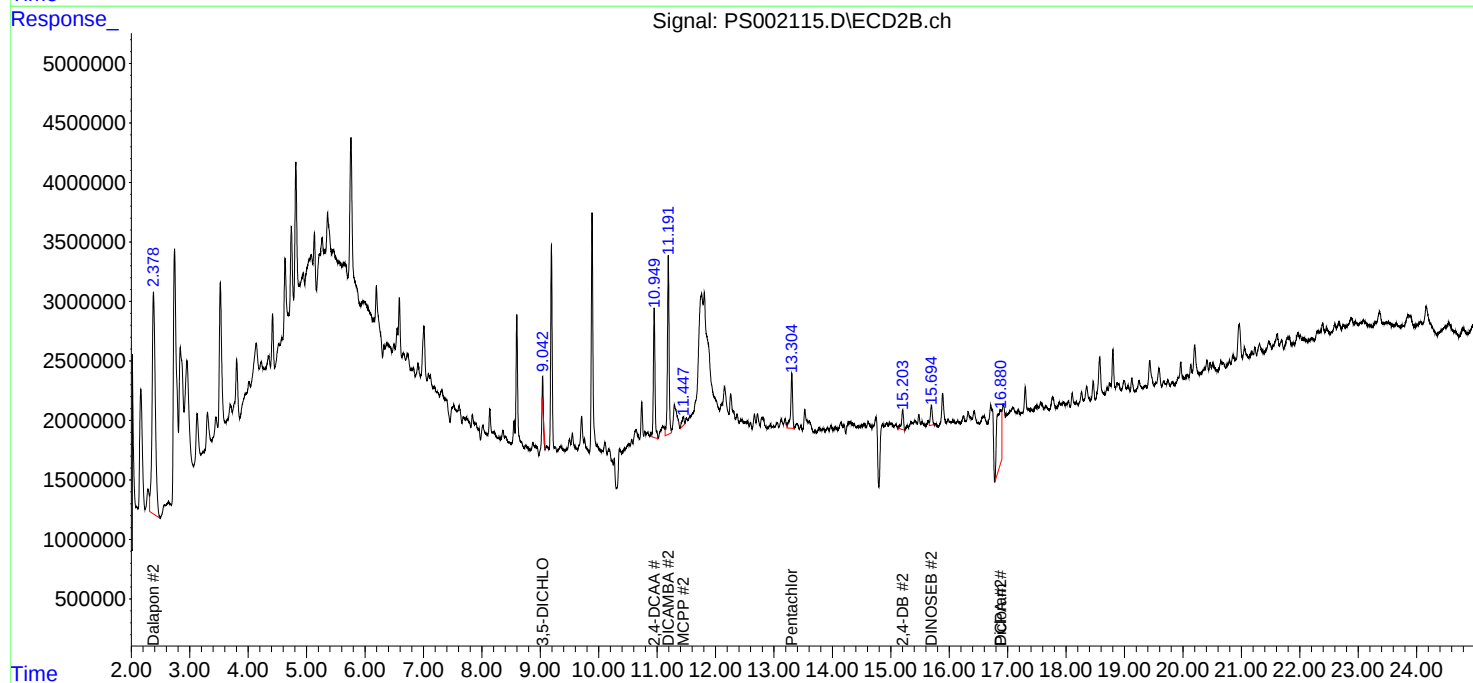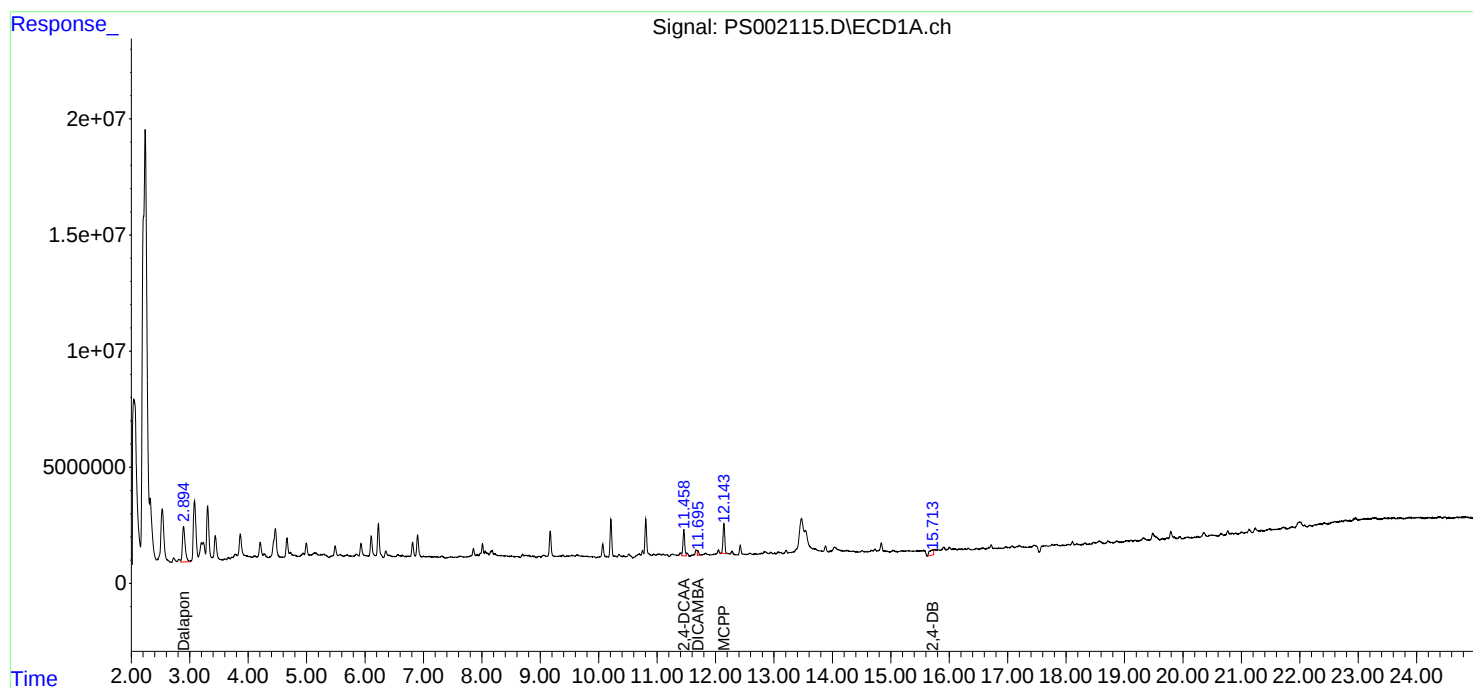


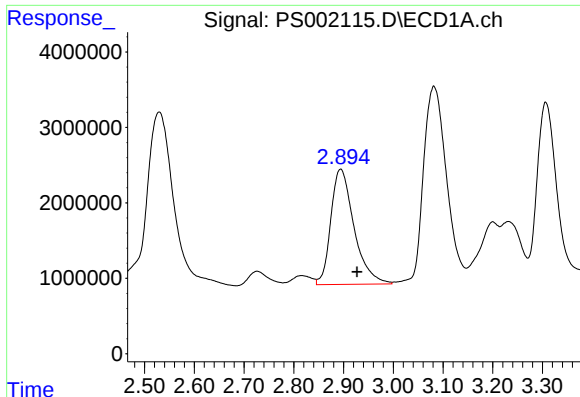

#1 Dalapon


R.T.: 2.894 min
Delta R.T.: -0.033 min
Response: 49545201
Conc: 162.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

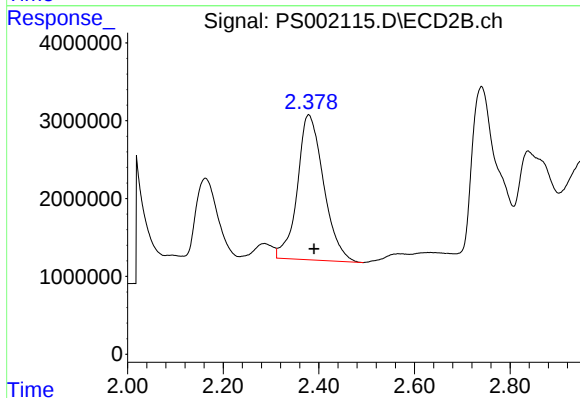


#1 Dalapon

R.T.: 2.379 min
Delta R.T.: -0.011 min
Response: 71065289
Conc: 243.40 ng/ml

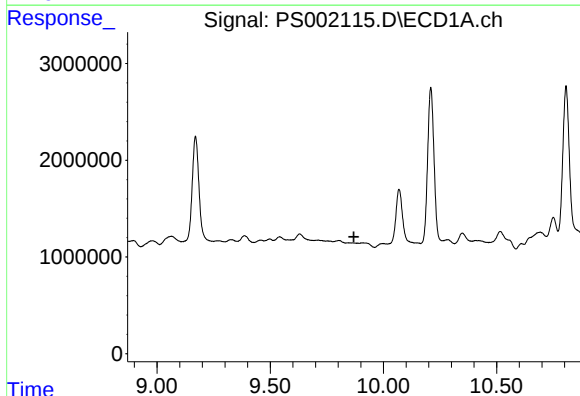


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

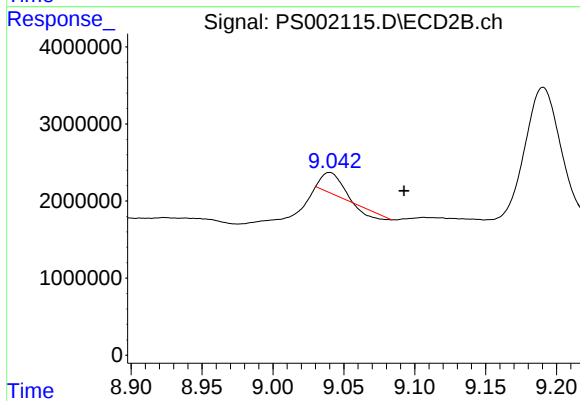

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.040 min
Delta R.T.: -0.053 min
Response: 1799728
Conc: 6.15 ng/ml

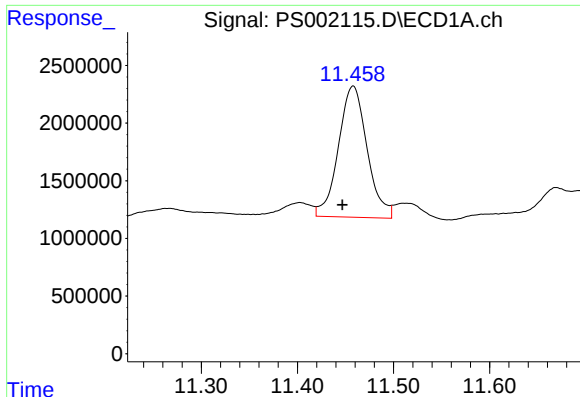

#4 2,4-DCAA


R.T.: 11.458 min
Delta R.T.: 0.011 min
Response: 23632266
Conc: 111.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

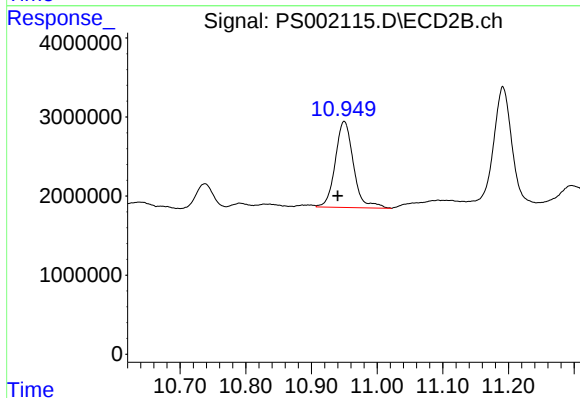


#4 2,4-DCAA

R.T.: 10.950 min
Delta R.T.: 0.010 min
Response: 20926058
Conc: 87.74 ng/ml

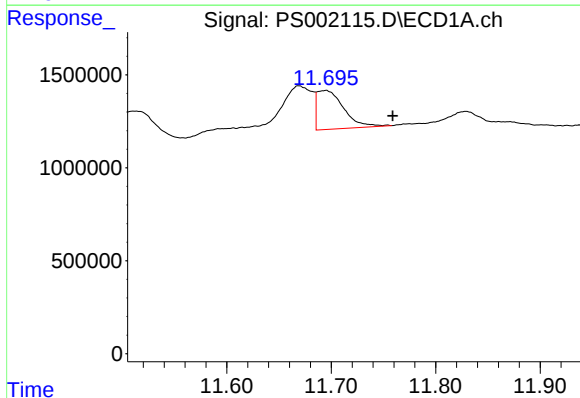


#5 DICAMBA

R.T.: 11.694 min
Delta R.T.: -0.065 min
Response: 3677102
Conc: 4.67 ng/ml

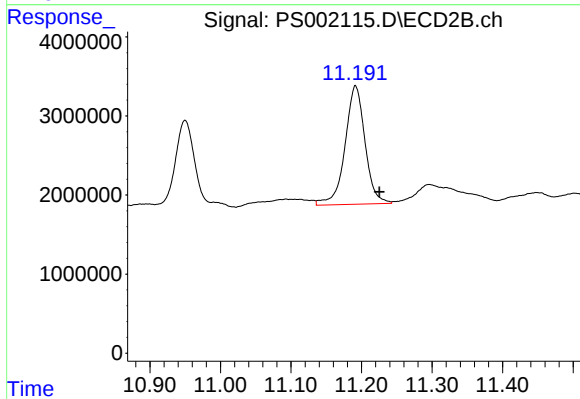

#5 DICAMBA


R.T.: 11.191 min
Delta R.T.: -0.034 min
Response: 29523908
Conc: 35.93 ng/ml

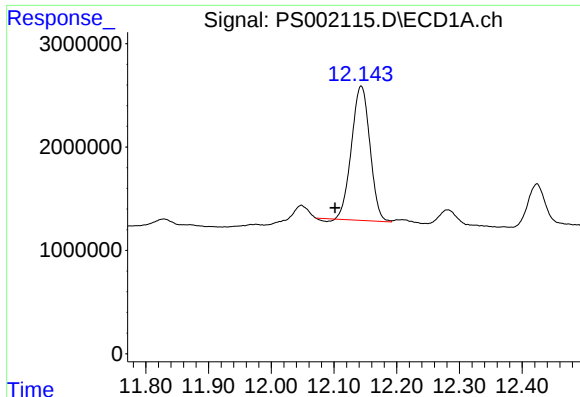

#6 MCP


R.T.: 12.143 min
Delta R.T.: 0.041 min
Response: 26313769
Conc: 46.99 ug/ml

Instrument :
ECD_S
ClientSampleId :

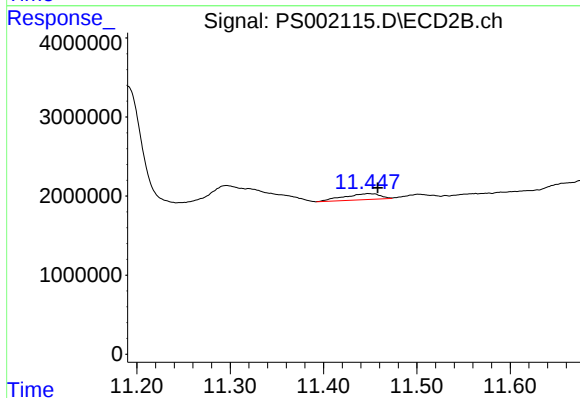


#6 MCP

R.T.: 11.448 min
Delta R.T.: -0.010 min
Response: 2039669
Conc: 3.74 ug/ml

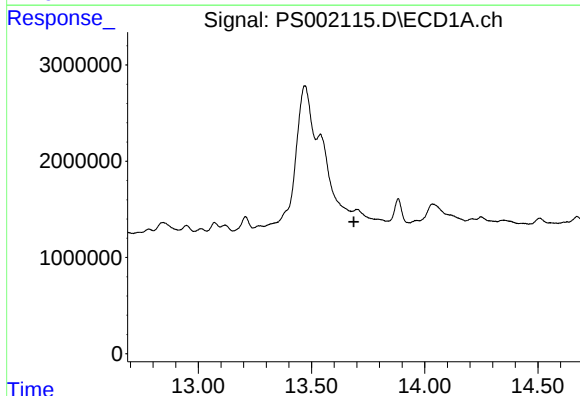


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.687 min
Response: 0
Conc: N.D.

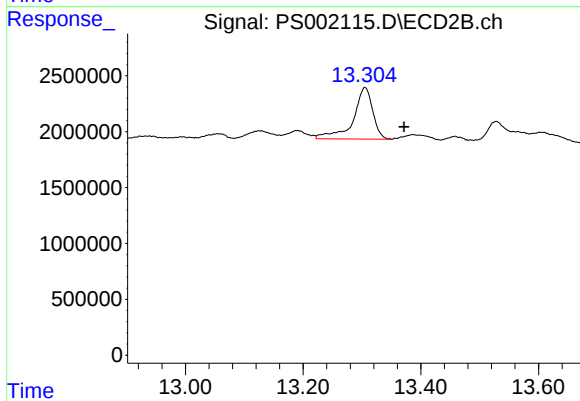

#10 Pentachlorophenol


R.T.: 13.305 min
Delta R.T.: -0.066 min
Response: 10607906
Conc: 3.35 ng/ml

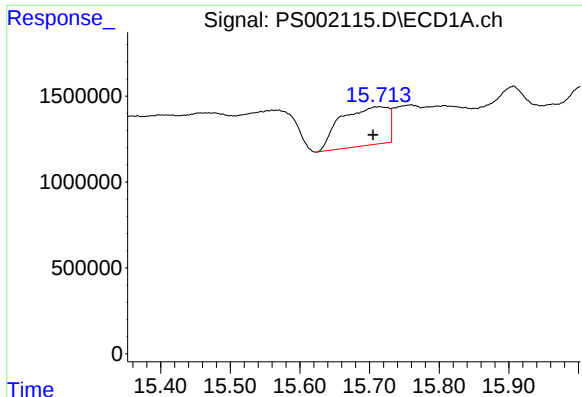

#13 2,4-DB


R.T.: 15.714 min
Delta R.T.: 0.009 min
Response: 10661672
Conc: 67.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

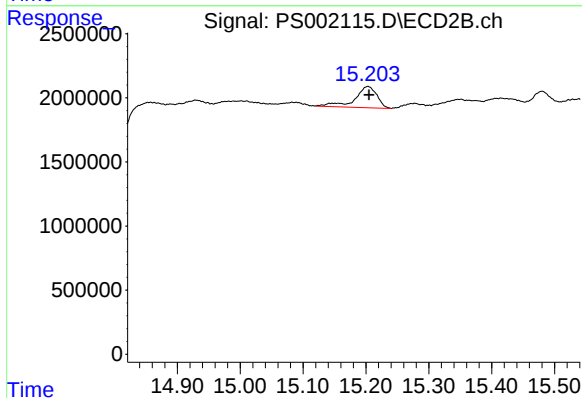


#13 2,4-DB

R.T.: 15.203 min
Delta R.T.: -0.002 min
Response: 4043469
Conc: 25.69 ng/ml

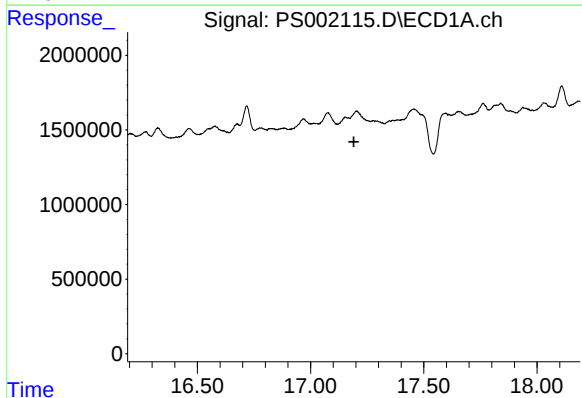


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.192 min
Response: 0
Conc: N.D.

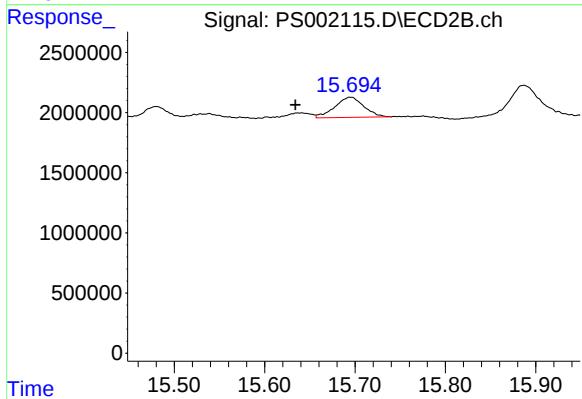

#14 DINOSEB


R.T.: 15.695 min
Delta R.T.: 0.061 min
Response: 3732439
Conc: 4.22 ng/ml

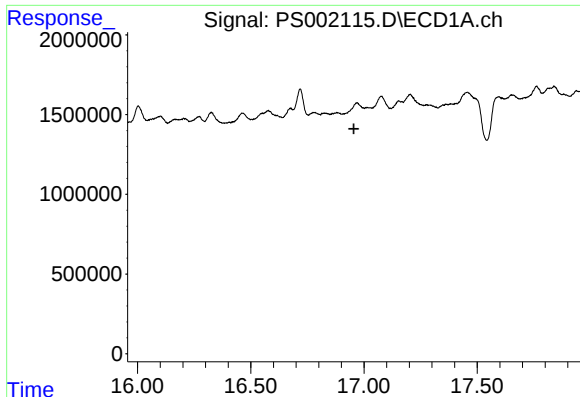

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.955 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

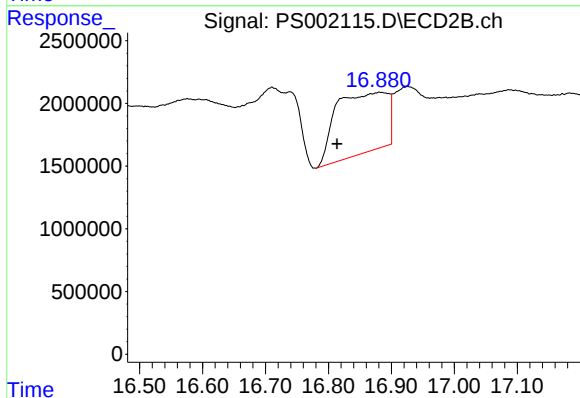


#15 Picloram

R.T.: 16.881 min
Delta R.T.: 0.067 min
Response: 27604663
Conc: 17.40 ng/ml

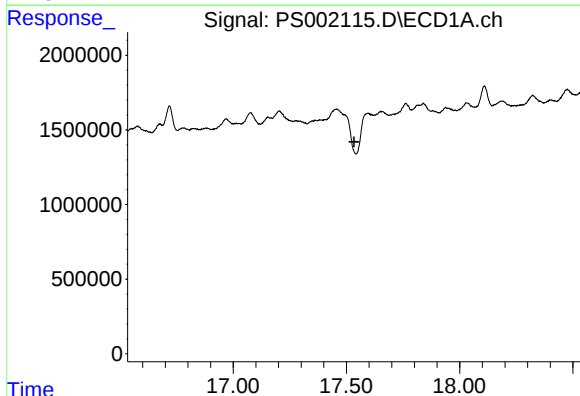

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.533 min
Response: 0
Conc: N.D.

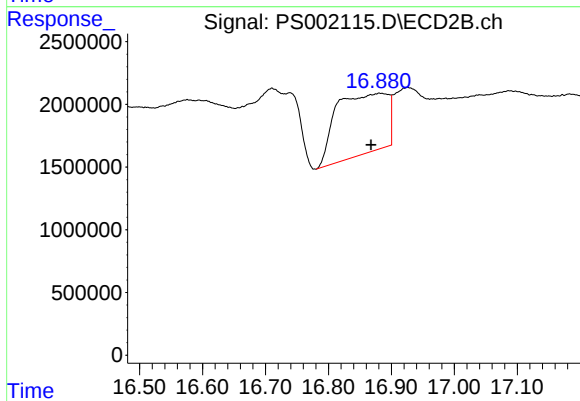

#16 DCPA

R.T.: 16.881 min
Delta R.T.: 0.013 min
Response: 27604663
Conc: 15.26 ng/ml