

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102418\
 Data File : PS002123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2018 23:46
 Operator : EI\SJ
 Sample : J5624-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:28:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.445	10.937	53329659	54035155	252.267	226.556
Target Compounds							
1) T	Dalapon	2.882	2.366	32176926	42665149	105.444	146.130 #
5) T	DICAMBA	0.000	11.179	0	26792143	N.D.	32.606 #
6) T	MCPD	12.130	11.469	21270377	5755785	37.986	10.546 #
9) T	2,4-D	0.000	12.785	0	6726644	N.D.	22.511 #
12) T	2,4,5-T	0.000	14.554	0	49820337	N.D.	45.485 #
13) T	2,4-DB	15.724	15.178	21371963	18321359	136.066	116.382
14) T	DINOSEB	0.000	15.681	0	16032213	N.D.	18.127 #
15) T	Picloram	16.959	16.865	51422424	94987863	30.077	59.882 #
16) T	DCPA	0.000	16.865	0	94987863	N.D.	52.502 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102418\
Data File : PS002123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2018 23:46
Operator : EI\SJ
Sample : J5624-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:28:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

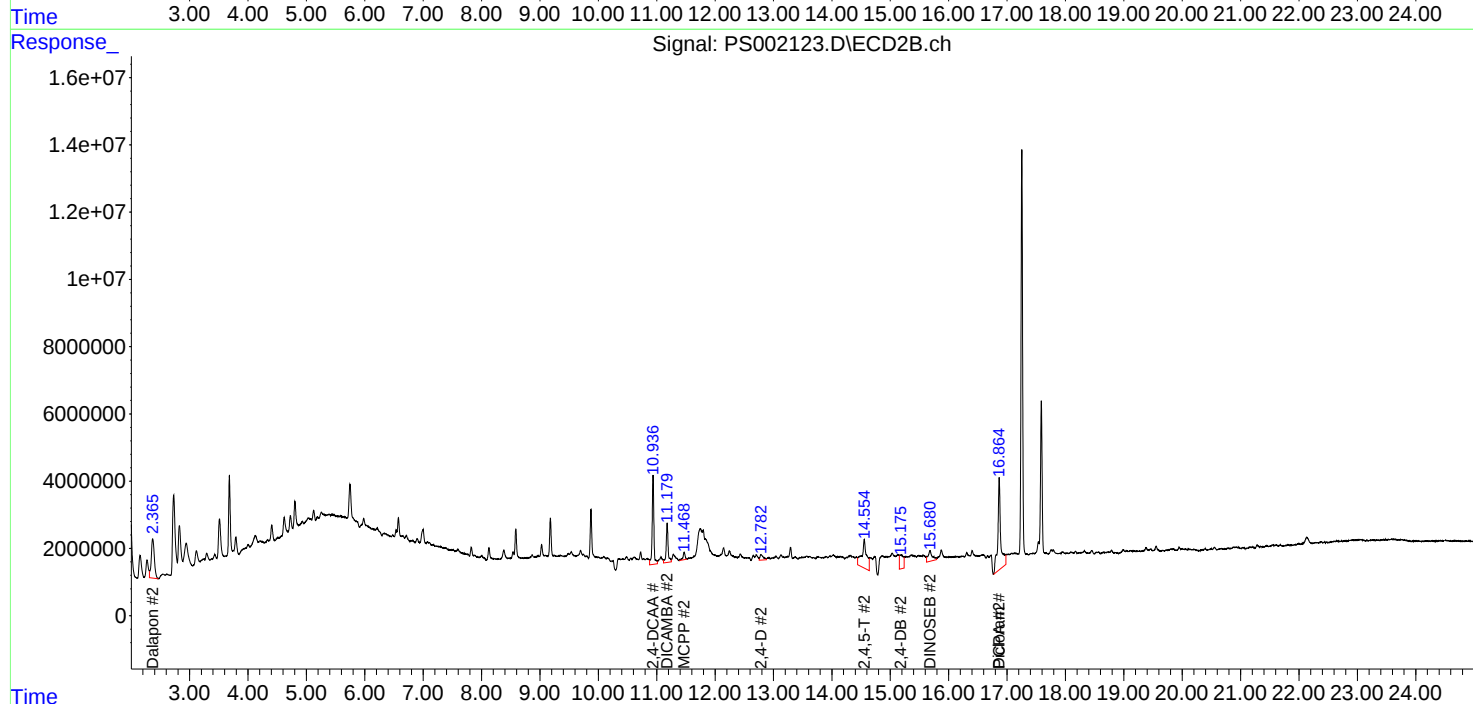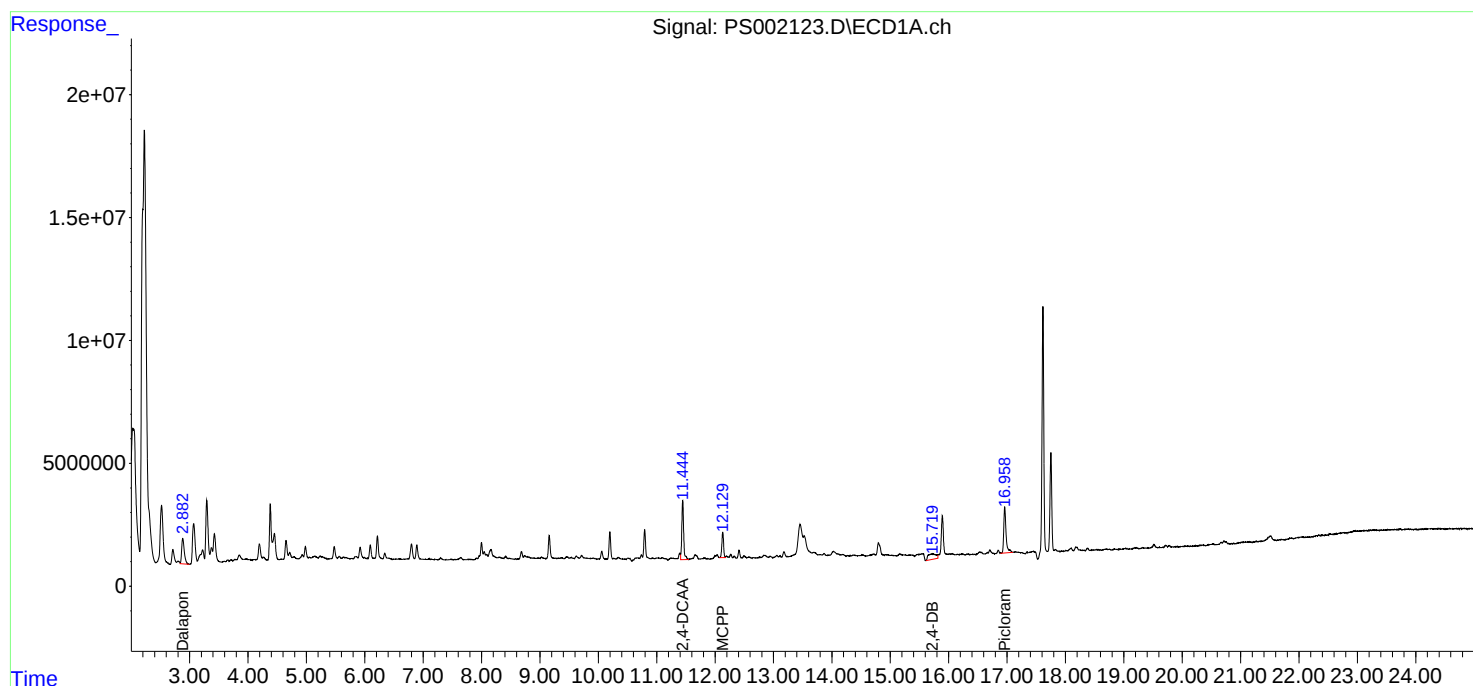


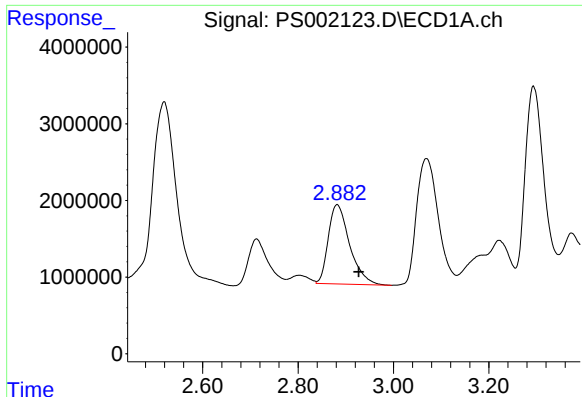

#1 Dalapon


R.T.: 2.882 min
Delta R.T.: -0.045 min
Response: 32176926
Conc: 105.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

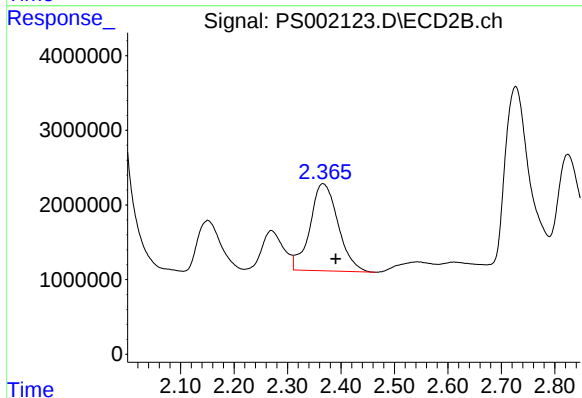


#1 Dalapon

R.T.: 2.366 min
Delta R.T.: -0.024 min
Response: 42665149
Conc: 146.13 ng/ml

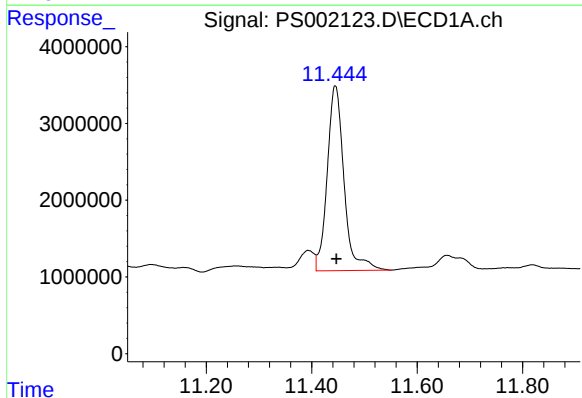


#4 2,4-DCAA

R.T.: 11.445 min
Delta R.T.: -0.002 min
Response: 53329659
Conc: 252.27 ng/ml

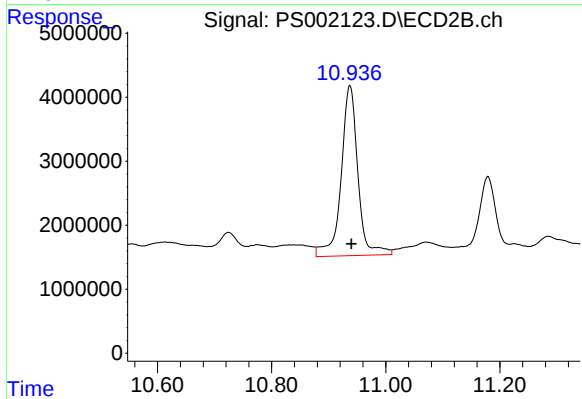

#4 2,4-DCAA


R.T.: 10.937 min
Delta R.T.: -0.003 min
Response: 54035155
Conc: 226.56 ng/ml

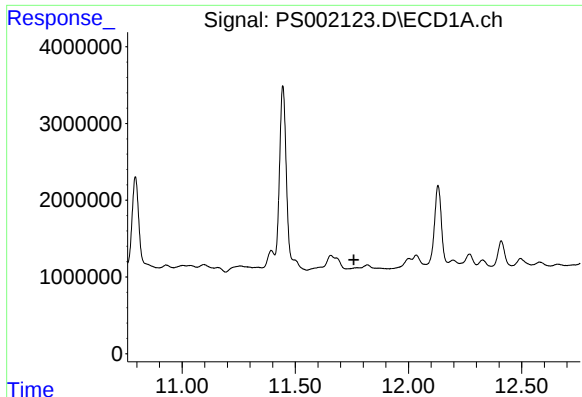

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.759 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

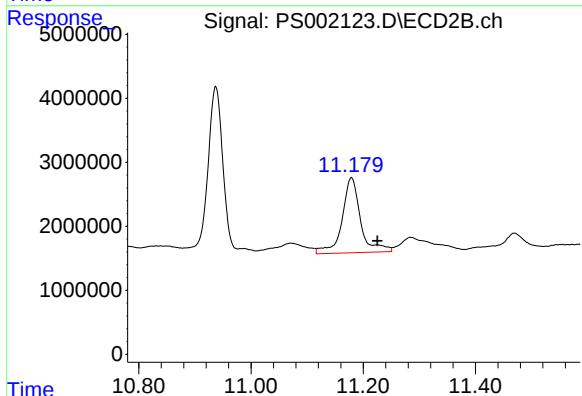


#5 DICAMBA

R.T.: 11.179 min
Delta R.T.: -0.046 min
Response: 26792143
Conc: 32.61 ng/ml

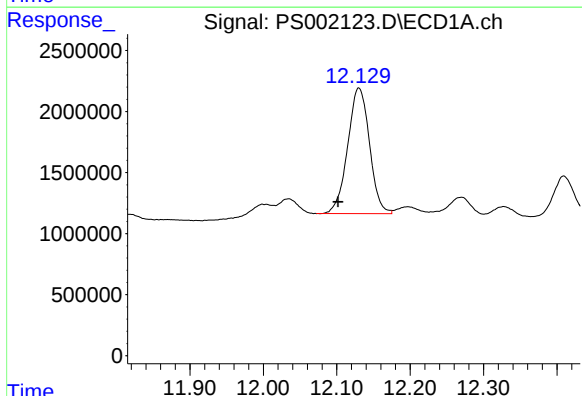


#6 MCP

R.T.: 12.130 min
Delta R.T.: 0.028 min
Response: 21270377
Conc: 37.99 ug/ml

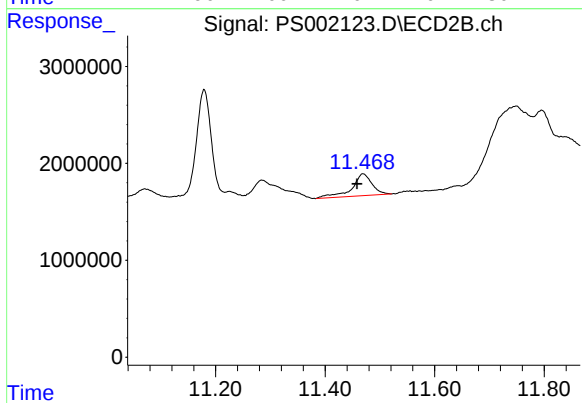

#6 MCP


R.T.: 11.469 min
Delta R.T.: 0.011 min
Response: 5755785
Conc: 10.55 ug/ml

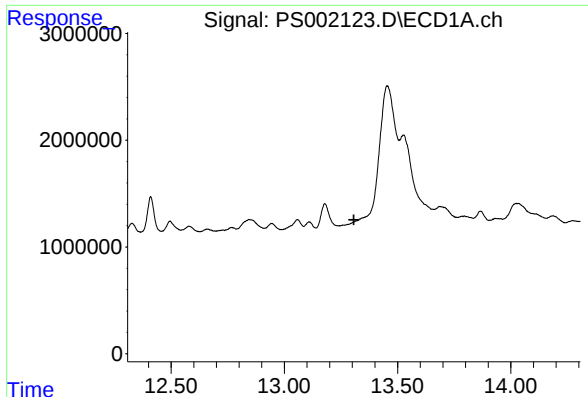

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.307 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

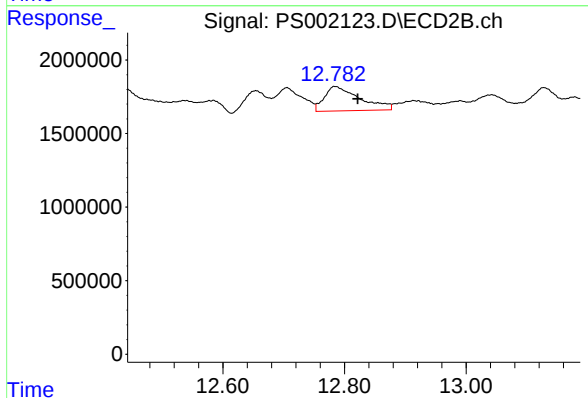


#9 2,4-D

R.T.: 12.785 min
Delta R.T.: -0.037 min
Response: 6726644
Conc: 22.51 ng/ml

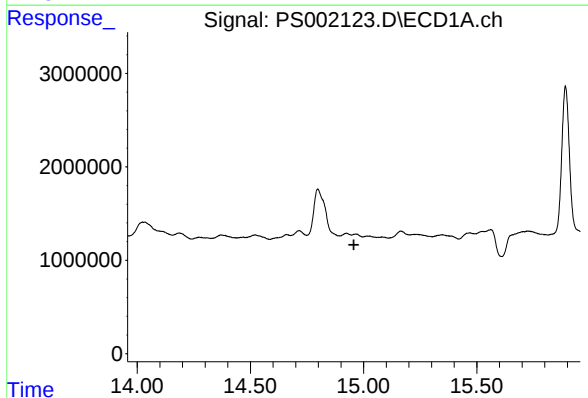


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.957 min
Response: 0
Conc: N.D.

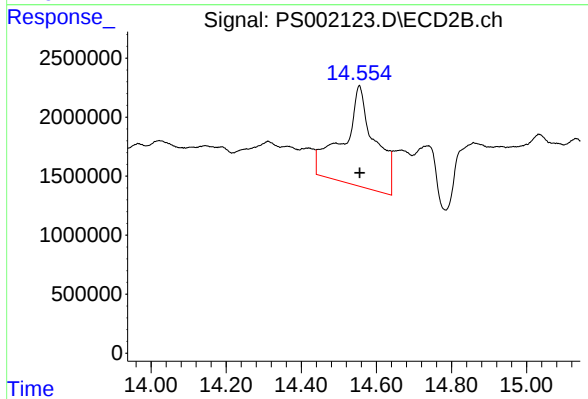

#12 2,4,5-T


R.T.: 14.554 min
Delta R.T.: 0.000 min
Response: 49820337
Conc: 45.48 ng/ml

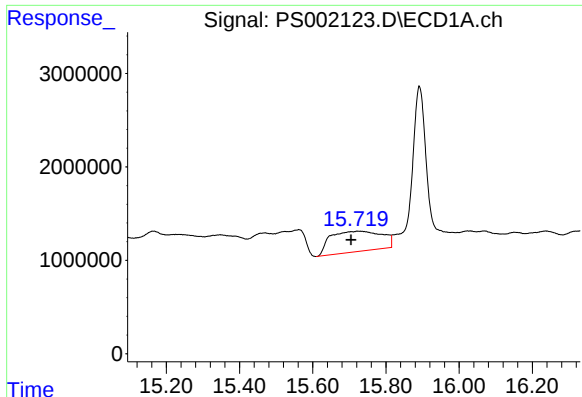

#13 2,4-DB


R.T.: 15.724 min
Delta R.T.: 0.019 min
Response: 21371963
Conc: 136.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

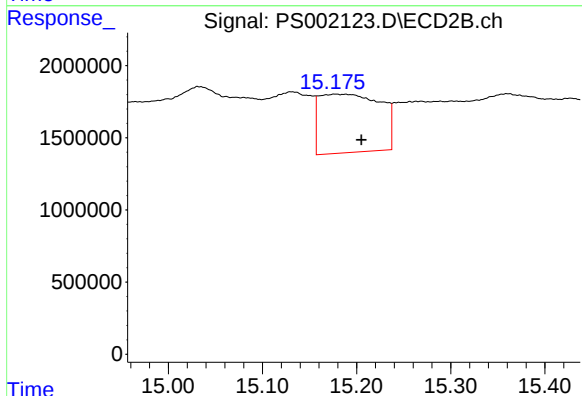


#13 2,4-DB

R.T.: 15.178 min
Delta R.T.: -0.027 min
Response: 18321359
Conc: 116.38 ng/ml

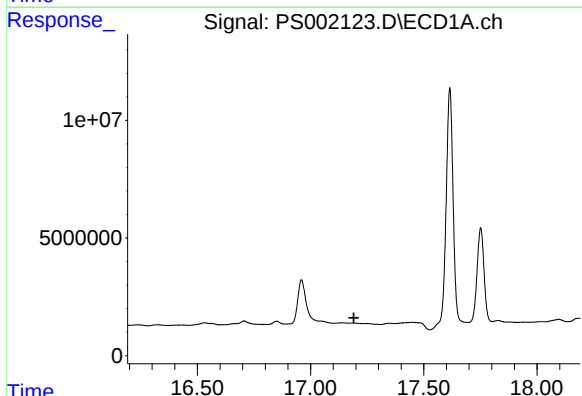


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.192 min
Response: 0
Conc: N.D.

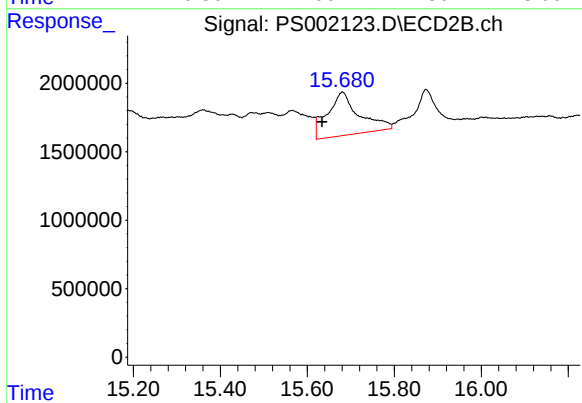

#14 DINOSEB


R.T.: 15.681 min
Delta R.T.: 0.046 min
Response: 16032213
Conc: 18.13 ng/ml

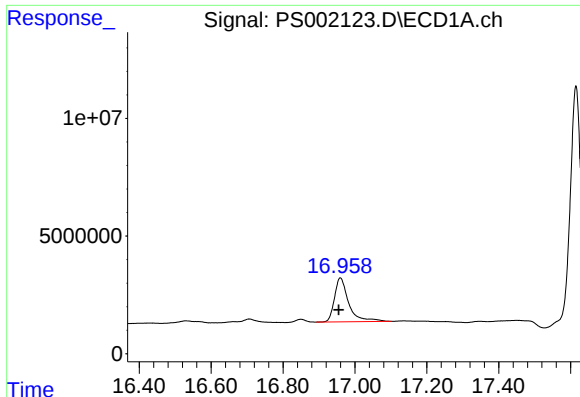

#15 Picloram


R.T.: 16.959 min
Delta R.T.: 0.004 min
Response: 51422424
Conc: 30.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

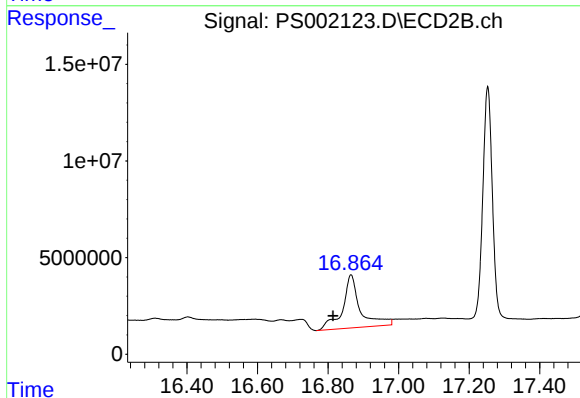


#15 Picloram

R.T.: 16.865 min
Delta R.T.: 0.051 min
Response: 94987863
Conc: 59.88 ng/ml

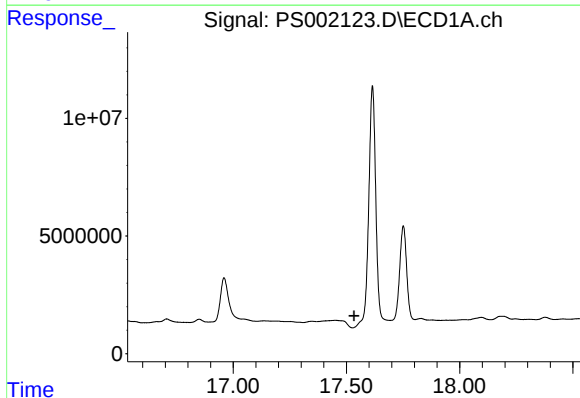

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.533 min
Response: 0
Conc: N.D.

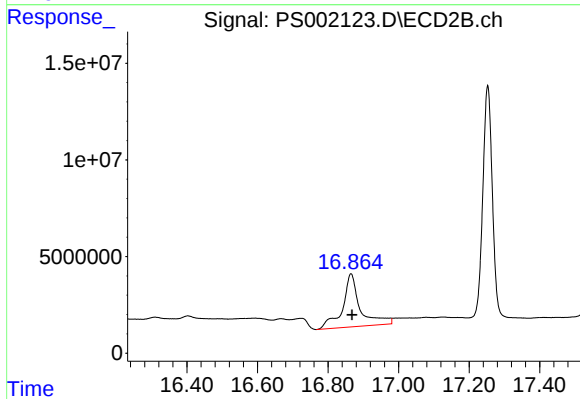

#16 DCPA

R.T.: 16.865 min
Delta R.T.: -0.003 min
Response: 94987863
Conc: 52.50 ng/ml