

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102418\
 Data File : PS002128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 02:21
 Operator : EI\SJ
 Sample : J5624-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 04:23:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.455	10.948	28582290	26591641	135.203	111.492
Target Compounds							
1) T	Dalapon	2.893	2.377	46049132	69065794	150.903	236.554 #
5) T	DICAMBA	0.000	11.190	0	29594177	N.D.	36.016 #
6) T	MCPD	12.141	11.481	25502748	6898928	45.545	12.641 #
9) T	2,4-D	0.000	12.816	0	4598604	N.D.	15.389 #
10) T	Pentachlo...	13.696	13.377	10332300	8503764	3.651	2.686 #
13) T	2,4-DB	15.759	0.000	28531770	0	181.650	N.D. #
14) T	DINOSEB	17.192	15.693	16411136	7982328	19.602	9.025 #
15) T	Picloram	0.000	16.822	0	14276593	N.D.	9.000 #
16) T	DCPA	0.000	16.878	0	15668120	N.D.	8.660 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102418\
Data File : PS002128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 02:21
Operator : EI\SJ
Sample : J5624-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 04:23:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

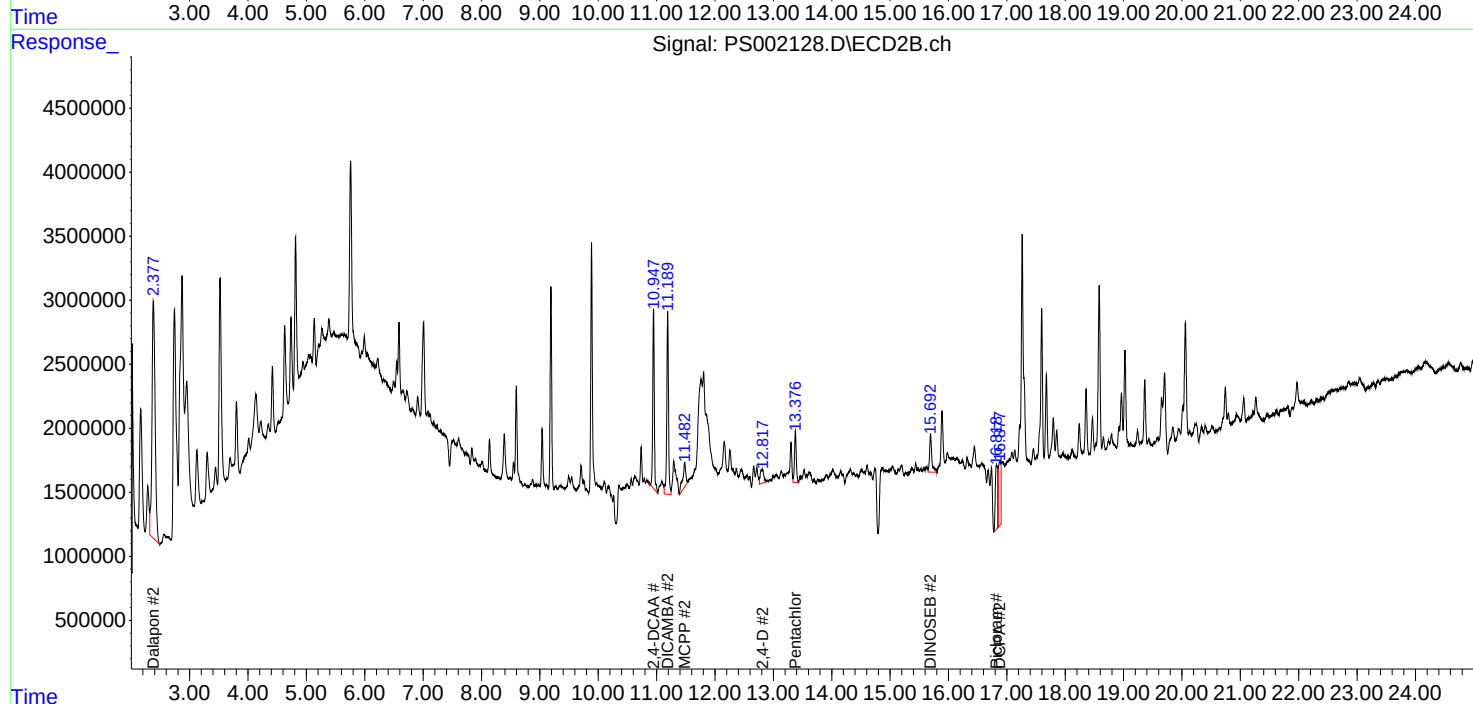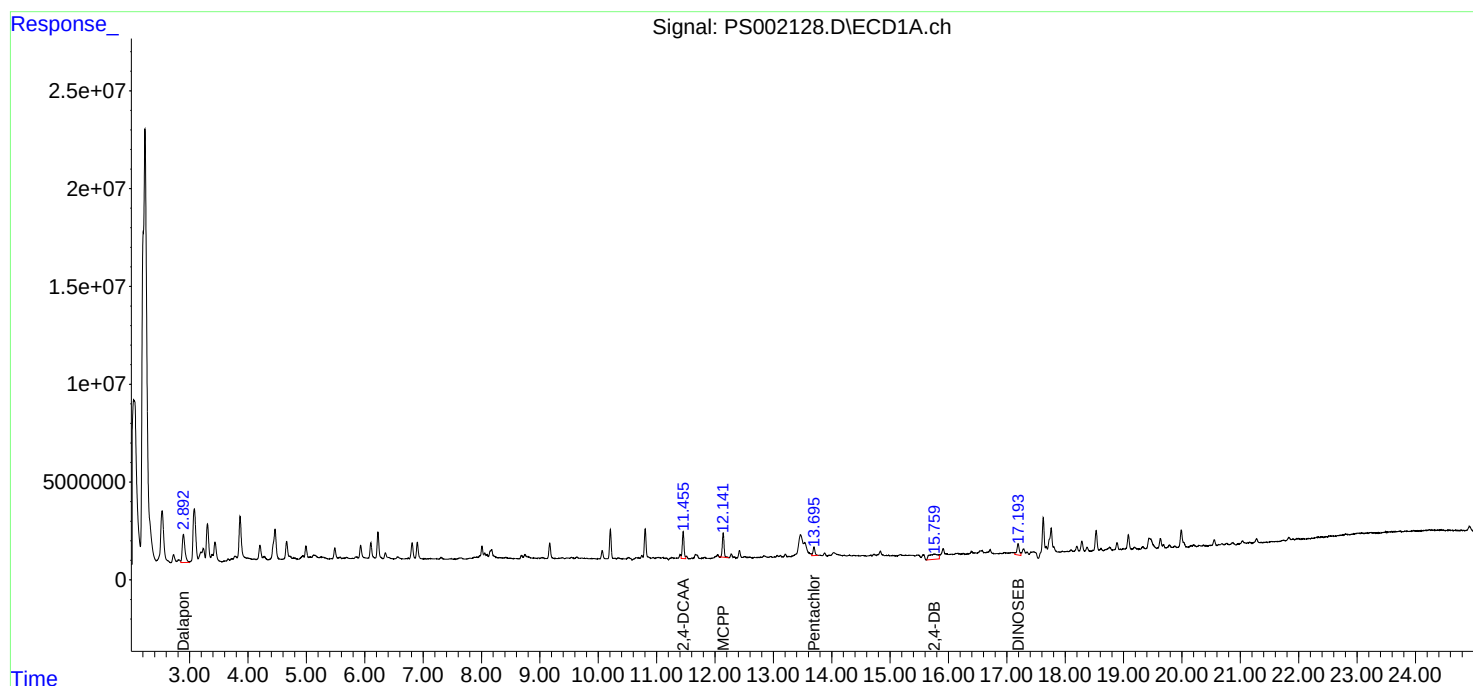


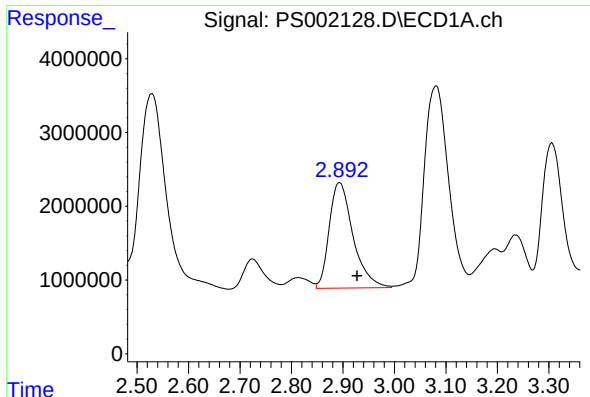

#1 Dalapon


R.T.: 2.893 min
Delta R.T.: -0.034 min
Response: 46049132
Conc: 150.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

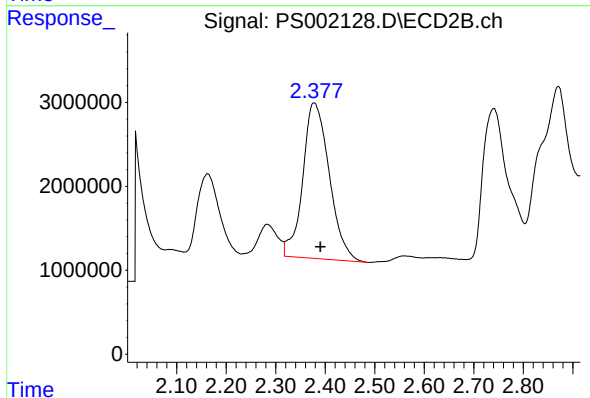


#1 Dalapon

R.T.: 2.377 min
Delta R.T.: -0.013 min
Response: 69065794
Conc: 236.55 ng/ml

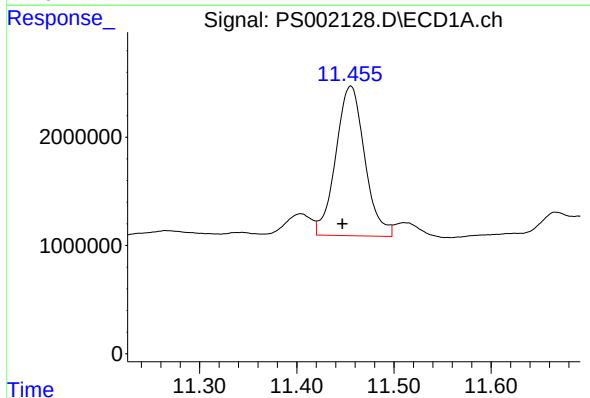


#4 2,4-DCAA

R.T.: 11.455 min
Delta R.T.: 0.008 min
Response: 28582290
Conc: 135.20 ng/ml

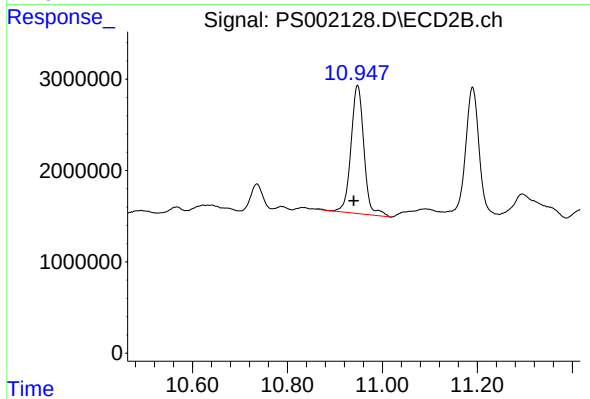

#4 2,4-DCAA


R.T.: 10.948 min
Delta R.T.: 0.008 min
Response: 26591641
Conc: 111.49 ng/ml

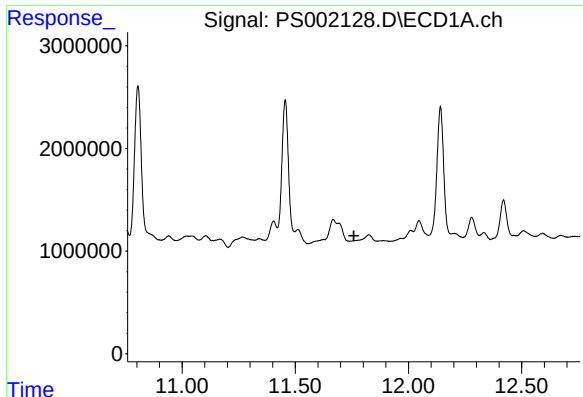

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.759 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

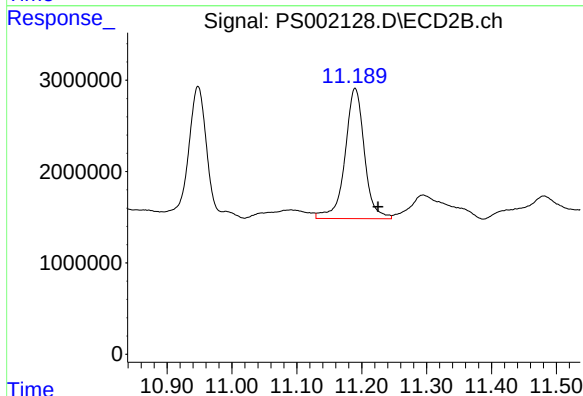


#5 DICAMBA

R.T.: 11.190 min
Delta R.T.: -0.035 min
Response: 29594177
Conc: 36.02 ng/ml

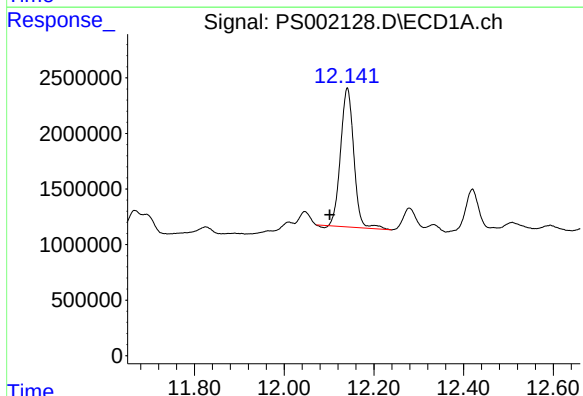


#6 MCP

R.T.: 12.141 min
Delta R.T.: 0.039 min
Response: 25502748
Conc: 45.54 ug/ml

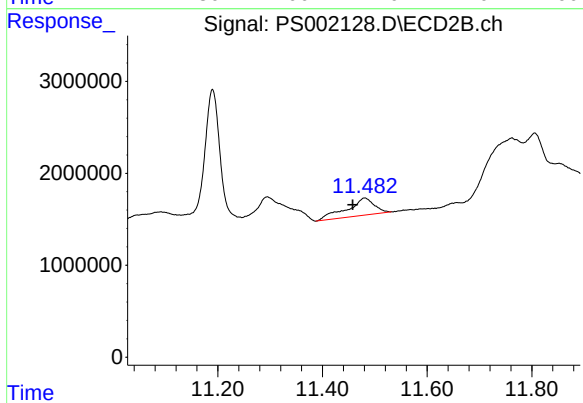

#6 MCP


R.T.: 11.481 min
Delta R.T.: 0.023 min
Response: 6898928
Conc: 12.64 ug/ml

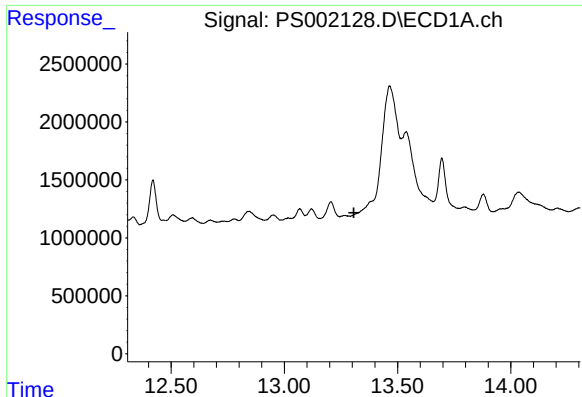

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.307 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

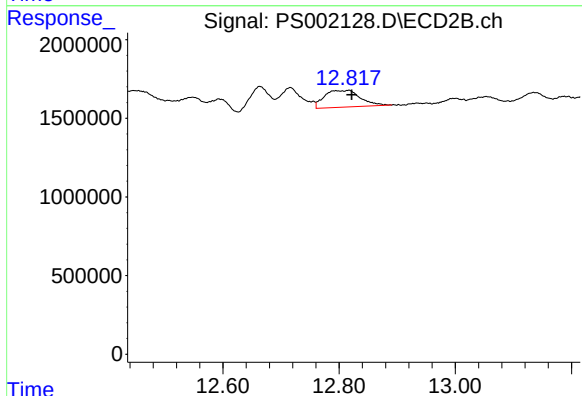


#9 2,4-D

R.T.: 12.816 min
Delta R.T.: -0.006 min
Response: 4598604
Conc: 15.39 ng/ml

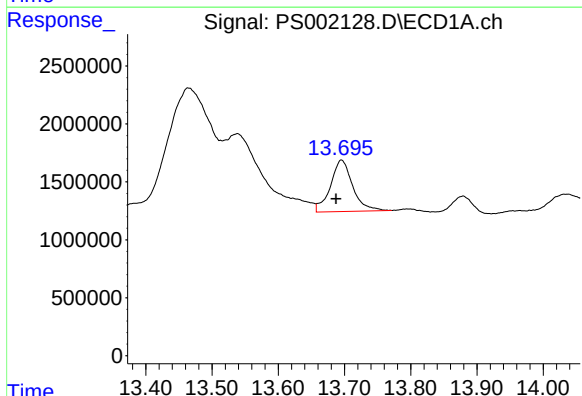


#10 Pentachlorophenol

R.T.: 13.696 min
Delta R.T.: 0.008 min
Response: 10332300
Conc: 3.65 ng/ml

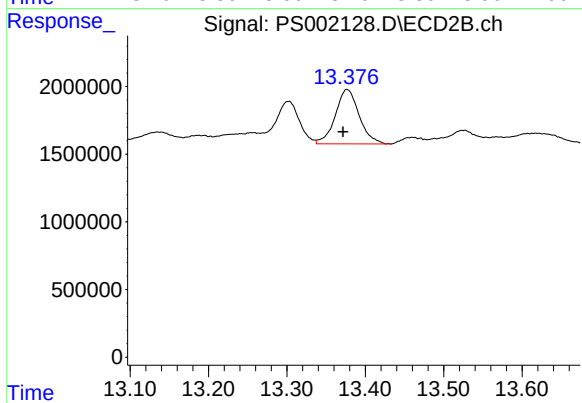

#10 Pentachlorophenol


R.T.: 13.377 min
Delta R.T.: 0.005 min
Response: 8503764
Conc: 2.69 ng/ml

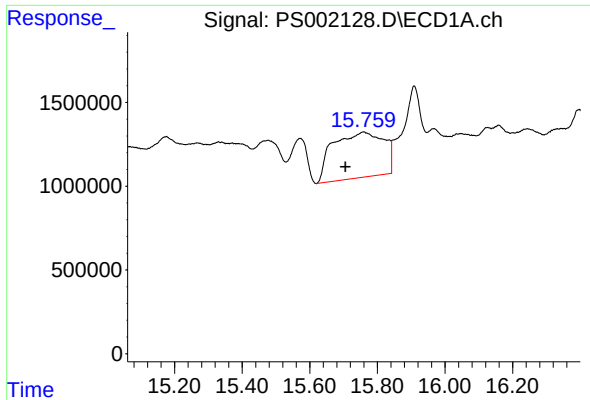

#13 2,4-DB


R.T.: 15.759 min
Delta R.T.: 0.054 min
Response: 28531770
Conc: 181.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

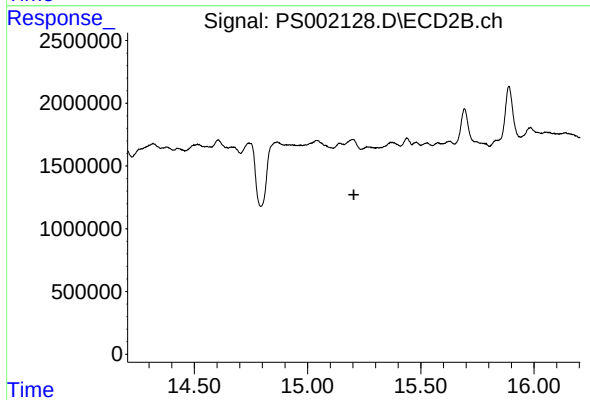


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.205 min
Response: 0
Conc: N.D.

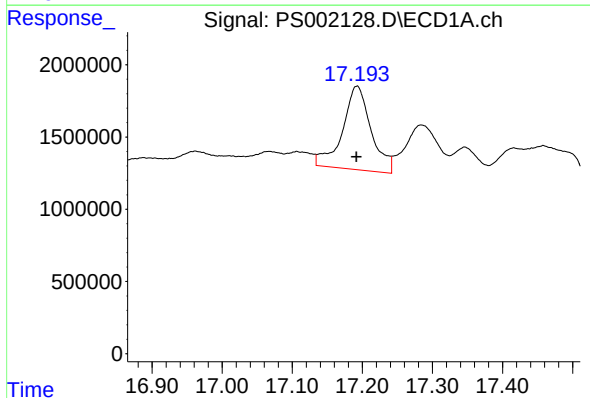


#14 DINOSEB

R.T.: 17.192 min
Delta R.T.: 0.000 min
Response: 16411136
Conc: 19.60 ng/ml

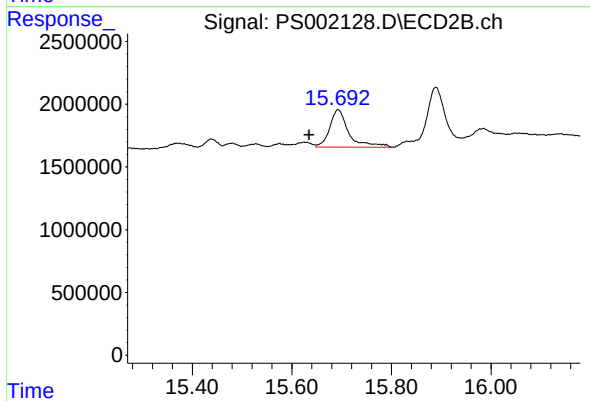

#14 DINOSEB


R.T.: 15.693 min
Delta R.T.: 0.059 min
Response: 7982328
Conc: 9.03 ng/ml

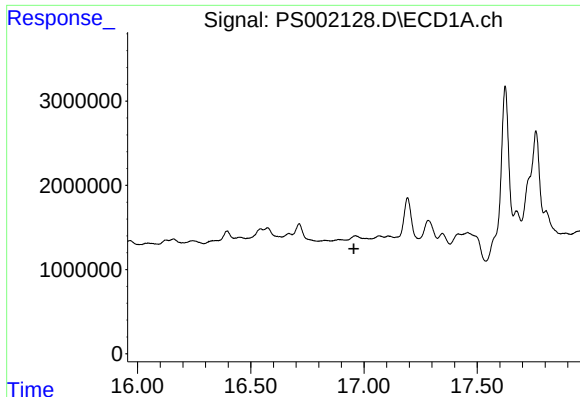

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.955 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

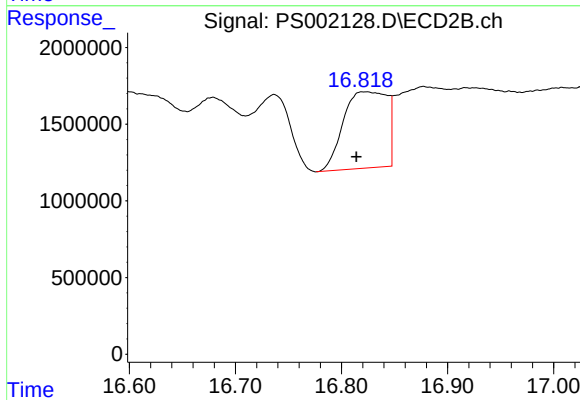


#15 Picloram

R.T.: 16.822 min
Delta R.T.: 0.008 min
Response: 14276593
Conc: 9.00 ng/ml

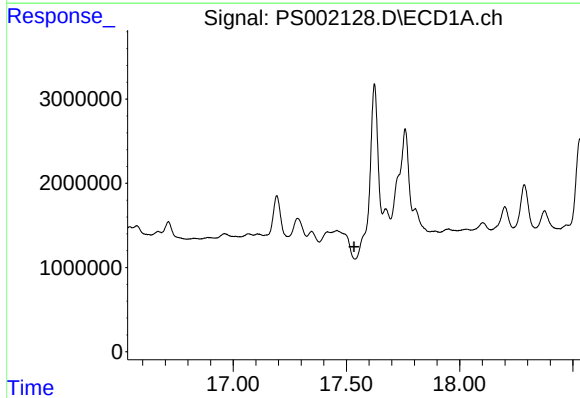

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.533 min
Response: 0
Conc: N.D.

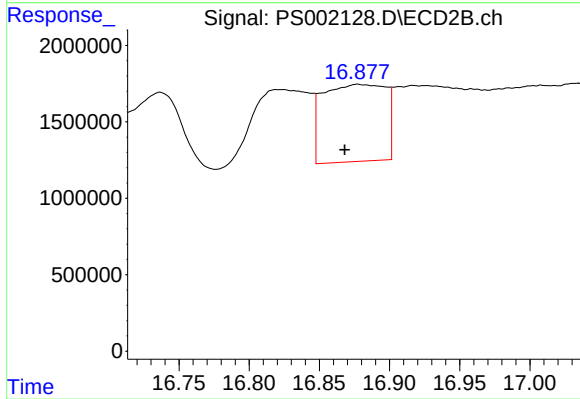

#16 DCPA

R.T.: 16.878 min
Delta R.T.: 0.010 min
Response: 15668120
Conc: 8.66 ng/ml