

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102418\
 Data File : PS002129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 02:53
 Operator : EI\SJ
 Sample : J5674-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 04:23:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.442	10.935	75329484	68762864	356.333	288.305
Target Compounds							
1) T	Dalapon	2.881	2.360	32537960	38084809	106.627	130.442
2) T	3,5-DICHL...	0.000	9.025	0	3310191	N.D.	11.319 #
5) T	DICAMBA	0.000	11.176	0	37814224	N.D.	46.020 #
6) T	MCP	12.128	0.000	36167141	0	64.590	N.D. #
9) T	2,4-D	0.000	12.780	0	5950817	N.D.	19.915 #
13) T	2,4-DB	15.741	15.180	20580589	21322921	131.028	135.449
14) T	DINOSEB	0.000	15.677	0	10205218	N.D.	11.539 #
15) T	Picloram	0.000	16.812	0	12045915	N.D.	7.594 #
16) T	DCPA	0.000	16.865	0	12287247	N.D.	6.791 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102418\
Data File : PS002129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 02:53
Operator : EI\SJ
Sample : J5674-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 04:23:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

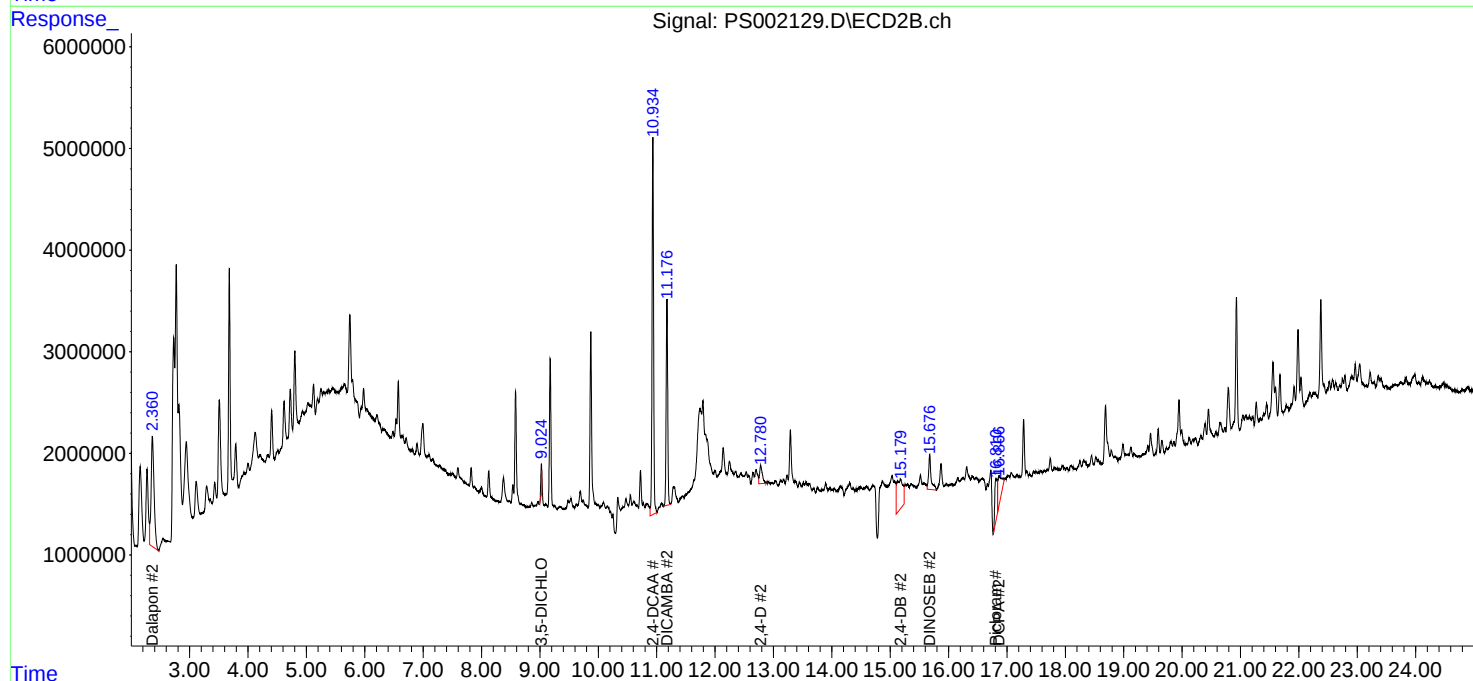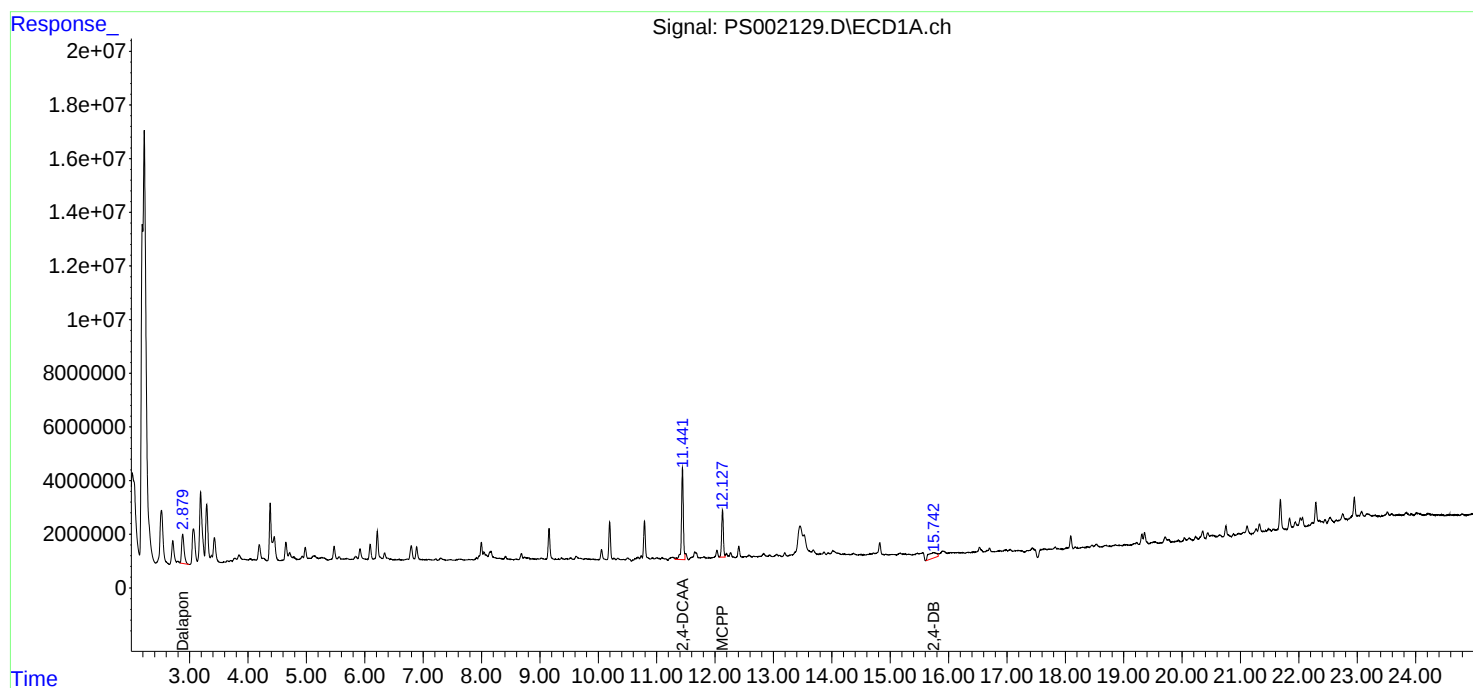


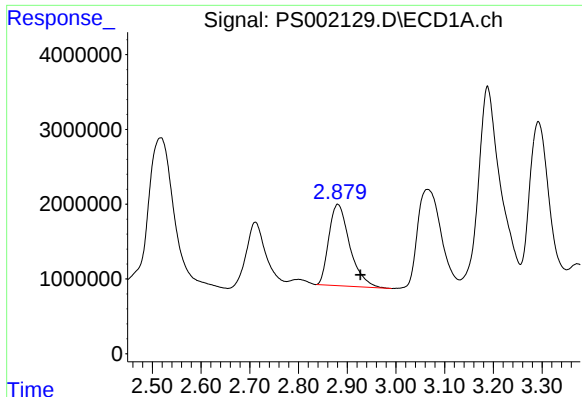

#1 Dalapon


R.T.: 2.881 min
Delta R.T.: -0.046 min
Response: 32537960
Conc: 106.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

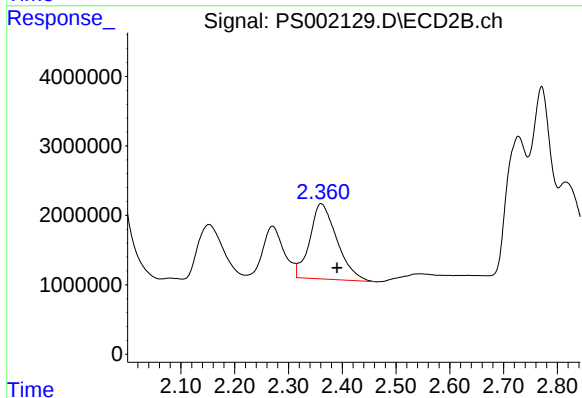


#1 Dalapon

R.T.: 2.360 min
Delta R.T.: -0.030 min
Response: 38084809
Conc: 130.44 ng/ml

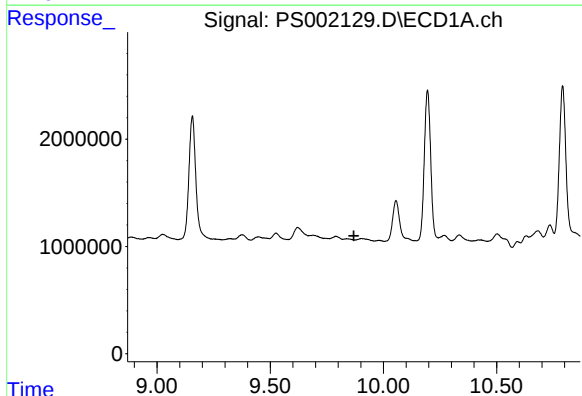


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

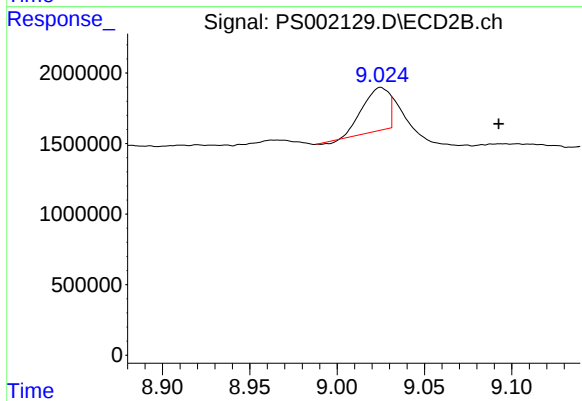

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.025 min
Delta R.T.: -0.067 min
Response: 3310191
Conc: 11.32 ng/ml

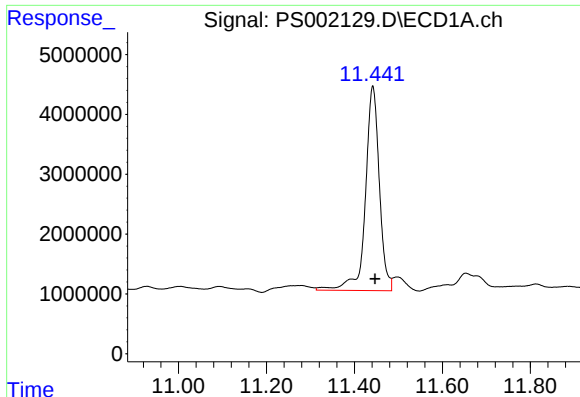

#4 2,4-DCAA


R.T.: 11.442 min
Delta R.T.: -0.005 min
Response: 75329484
Conc: 356.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

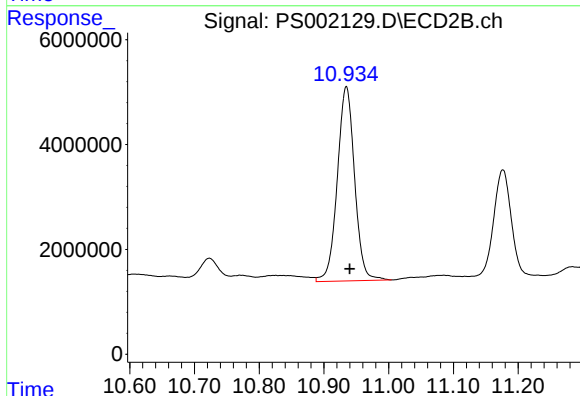


#4 2,4-DCAA

R.T.: 10.935 min
Delta R.T.: -0.005 min
Response: 68762864
Conc: 288.31 ng/ml

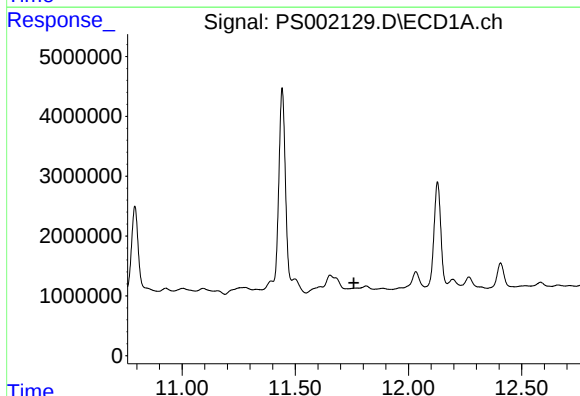


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.759 min
Response: 0
Conc: N.D.

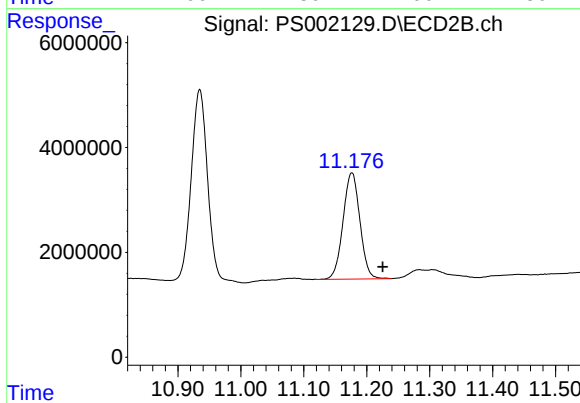

#5 DICAMBA


R.T.: 11.176 min
Delta R.T.: -0.049 min
Response: 37814224
Conc: 46.02 ng/ml

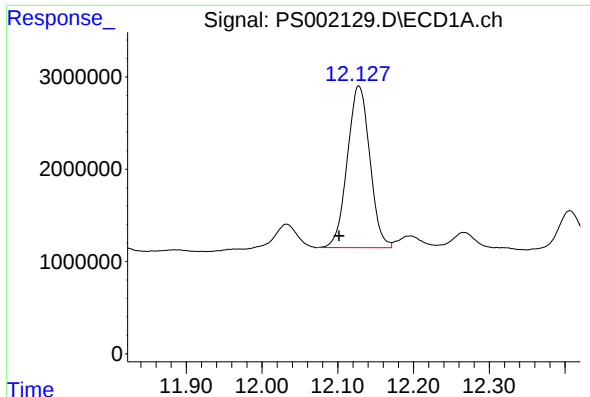

#6 MCP


R.T.: 12.128 min
Delta R.T.: 0.026 min
Response: 36167141
Conc: 64.59 ug/ml

Instrument :
ECD_S
ClientSampleId :

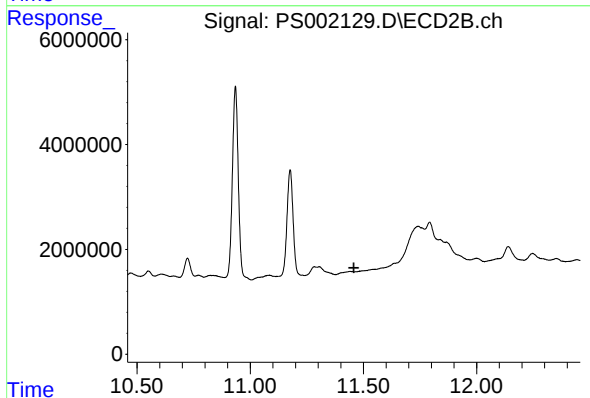


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.458 min
Response: 0
Conc: N.D.

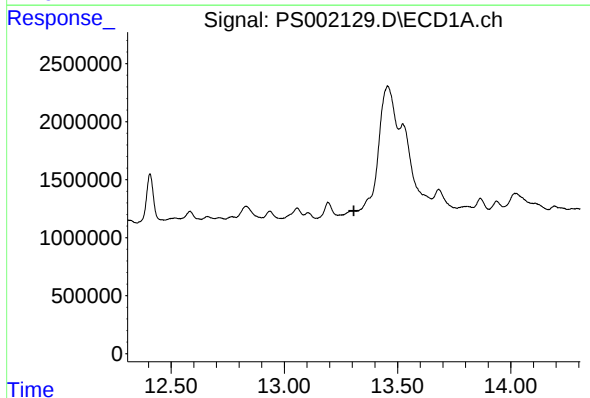


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.307 min
Response: 0
Conc: N.D.

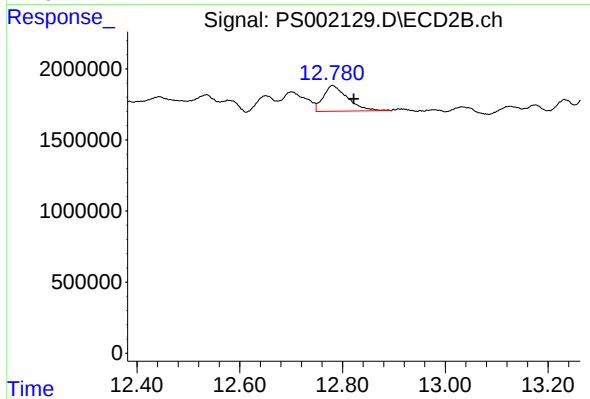

#9 2,4-D


R.T.: 12.780 min
Delta R.T.: -0.041 min
Response: 5950817
Conc: 19.91 ng/ml

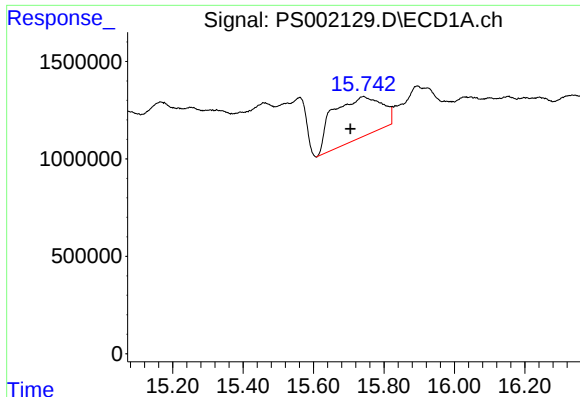

#13 2,4-DB


R.T.: 15.741 min
Delta R.T.: 0.036 min
Response: 20580589
Conc: 131.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

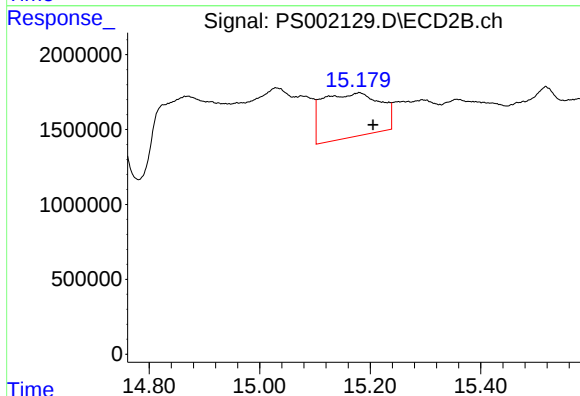


#13 2,4-DB

R.T.: 15.180 min
Delta R.T.: -0.025 min
Response: 21322921
Conc: 135.45 ng/ml

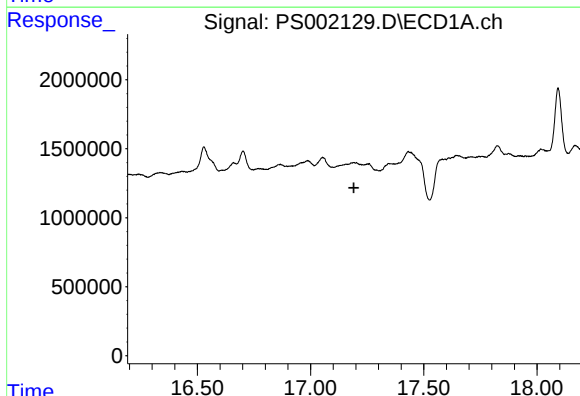


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.192 min
Response: 0
Conc: N.D.

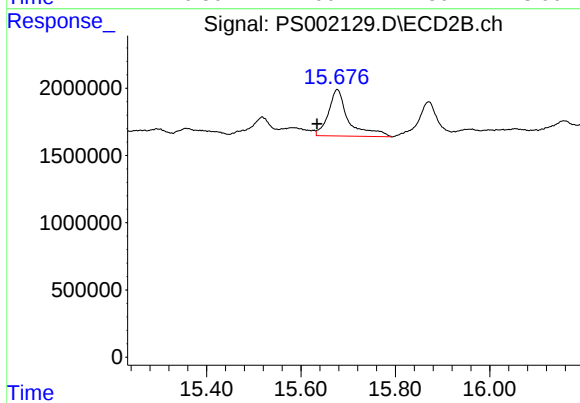

#14 DINOSEB


R.T.: 15.677 min
Delta R.T.: 0.043 min
Response: 10205218
Conc: 11.54 ng/ml

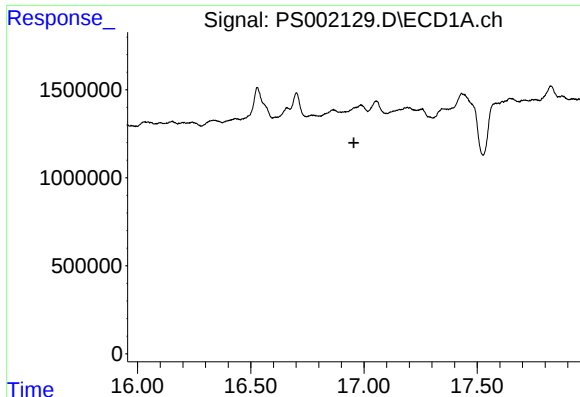

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.955 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

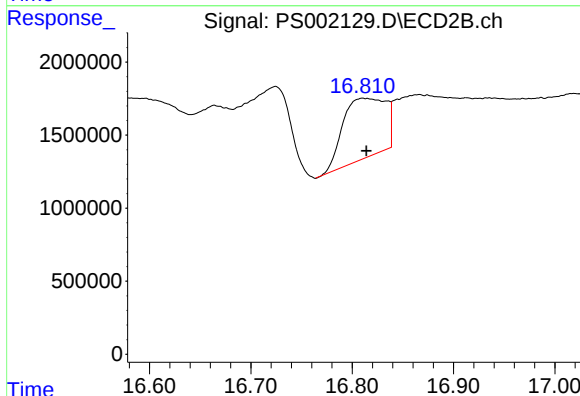


#15 Picloram

R.T.: 16.812 min
Delta R.T.: -0.002 min
Response: 12045915
Conc: 7.59 ng/ml

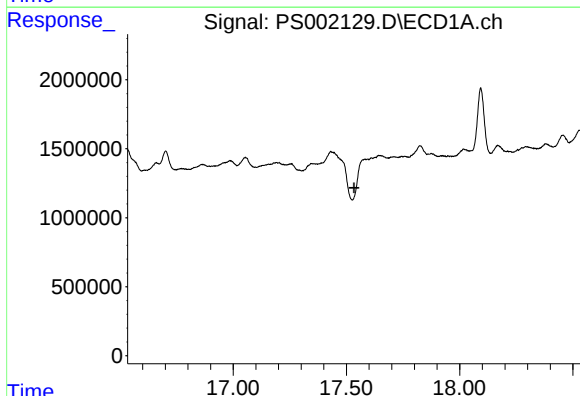

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.533 min
Response: 0
Conc: N.D.

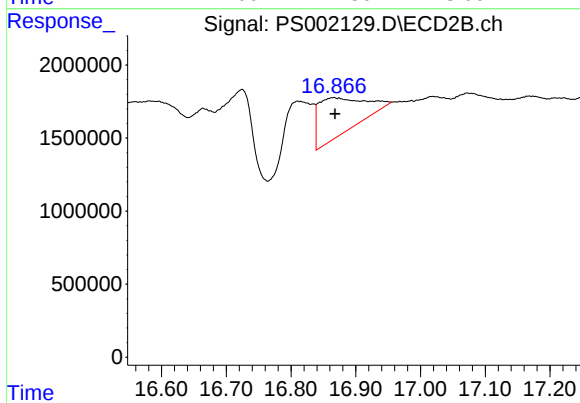

#16 DCPA

R.T.: 16.865 min
Delta R.T.: -0.003 min
Response: 12287247
Conc: 6.79 ng/ml