

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102419\
 Data File : PS007293.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2019 14:01
 Operator : SM\AJ
 Sample : K5494-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 17:51:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.453	5.181	331.2E6	178.4E6	242.014	253.612
Target Compounds							
1) T	Dalapon	2.008	1.677	160.1E6	1698.1E6	95.700	1866.007 #
2) T	3,5-DICHL...	0.000	4.460	0	15654891	N.D.	18.194
5) T	DICAMBA	5.546	0.000	52681656	0	10.722	N.D. #
6) T	MCP	0.000	5.396	0	1088171	N.D.	<MDL
7) T	MCPA	0.000	5.552	0	11799710	N.D.	4.059
8) T	DICHLORPROP	0.000	5.770	0	11366575	N.D.	17.454
9) T	2,4-D	0.000	6.086	0	12885578	N.D.	16.151
10) T	Pentachlo...	0.000	6.475	0	10411744	N.D.	1.083
11) T	2,4,5-TP ...	0.000	6.780	0	67348096	N.D.	17.706
12) T	2,4,5-T	7.422	0.000	163.9E6	0	21.437	N.D. #
13) T	2,4-DB	0.000	7.614	0	6258273	N.D.	13.353
14) T	DINOSEB	0.000	7.971	0	5395438	N.D.	1.922
15) T	Picloram	0.000	8.950	0	18374048	N.D.	2.992



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102419\
Data File : PS007293.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2019 14:01
Operator : SM\AJ
Sample : K5494-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 17:51:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

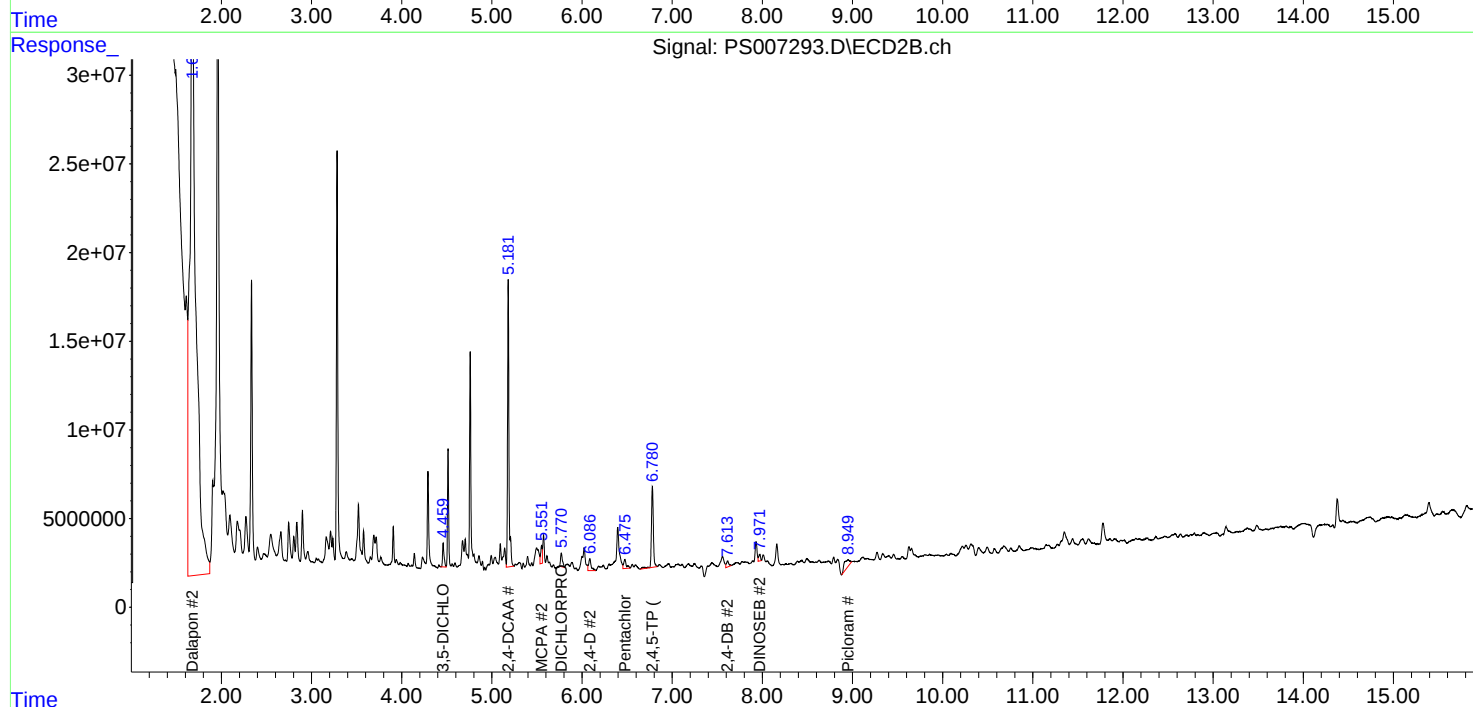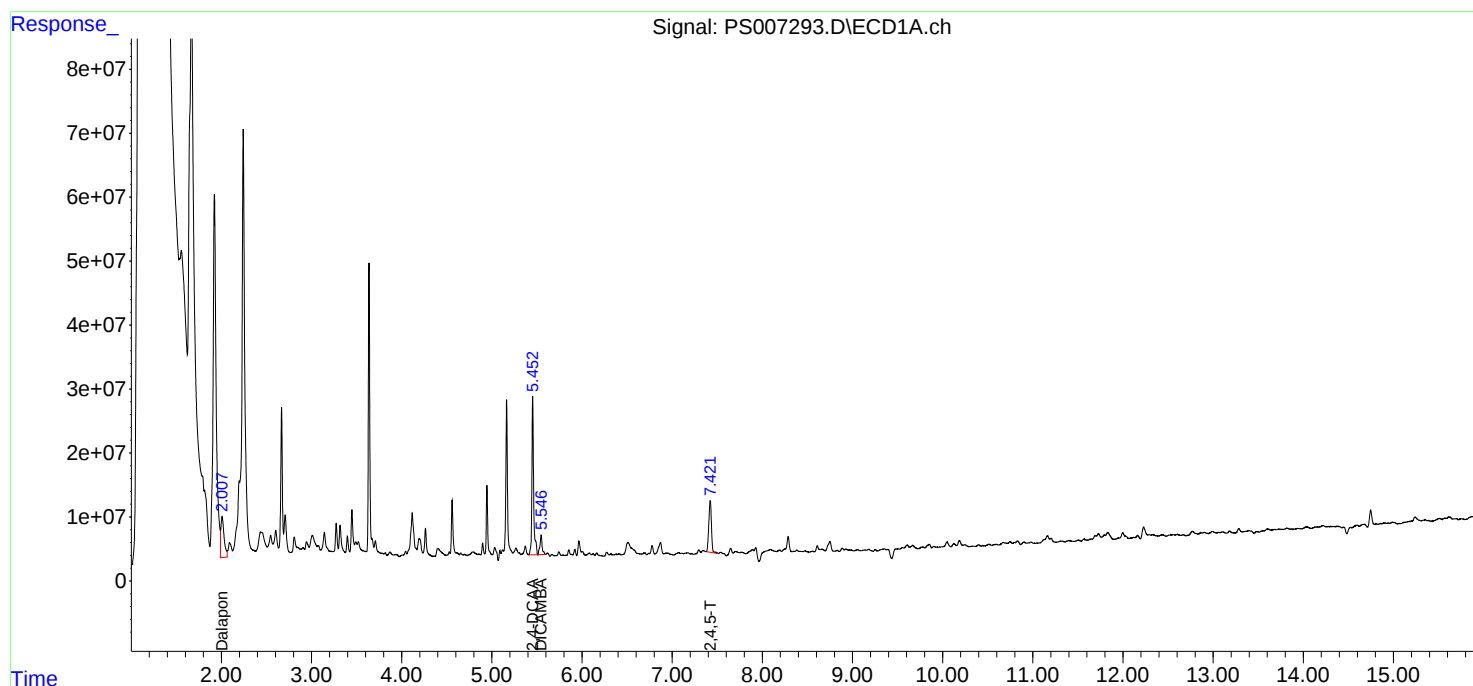


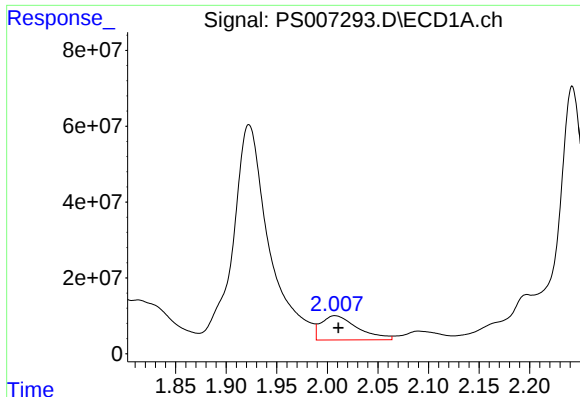

#1 Dalapon


R.T.: 2.008 min
Delta R.T.: -0.003 min
Response: 160133518
Conc: 95.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

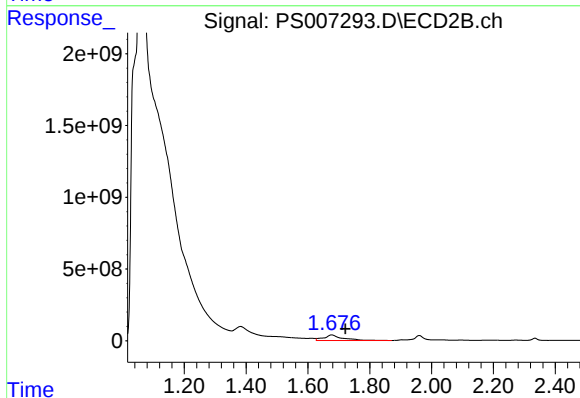


#1 Dalapon

R.T.: 1.677 min
Delta R.T.: -0.044 min
Response: 1698073089
Conc: 1866.01 ng/ml

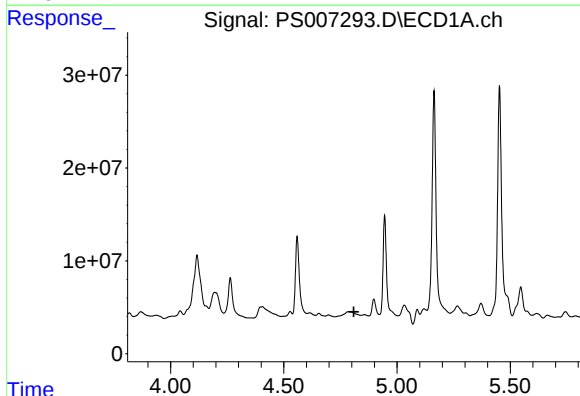


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

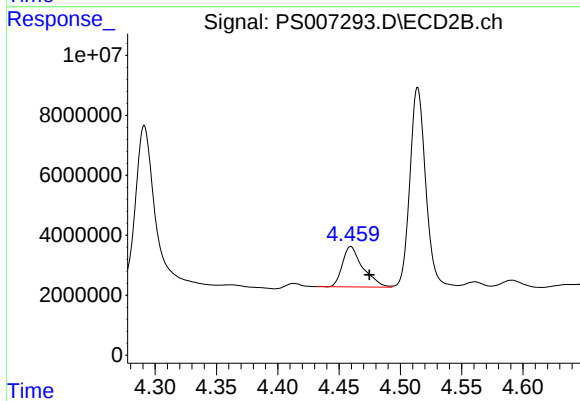

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.460 min
Delta R.T.: -0.015 min
Response: 15654891
Conc: 18.19 ng/ml

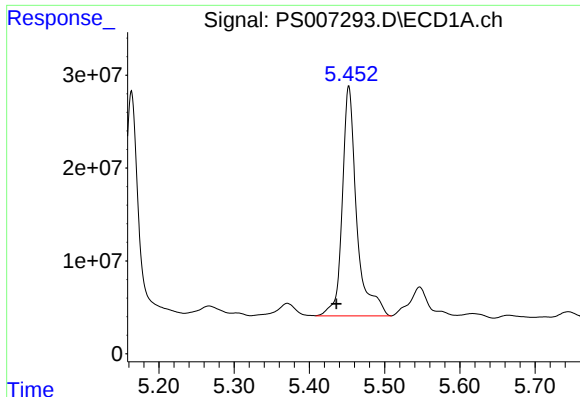

#4 2,4-DCAA


R.T.: 5.453 min
Delta R.T.: 0.017 min
Response: 331237413
Conc: 242.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

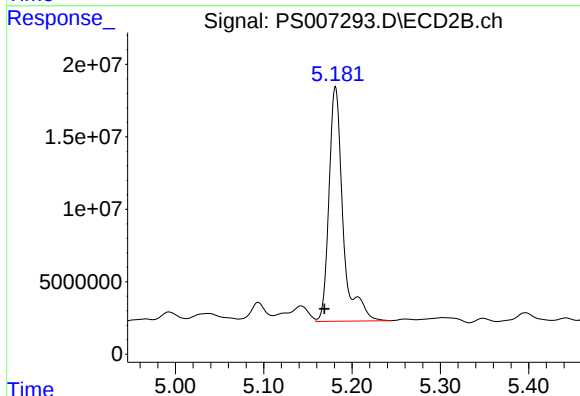


#4 2,4-DCAA

R.T.: 5.181 min
Delta R.T.: 0.013 min
Response: 178367042
Conc: 253.61 ng/ml

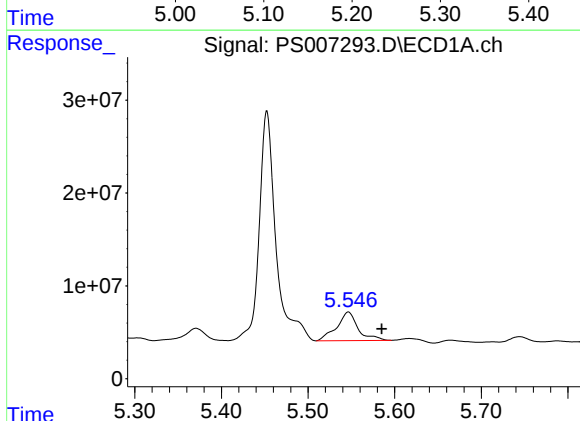


#5 DICAMBA

R.T.: 5.546 min
Delta R.T.: -0.039 min
Response: 52681656
Conc: 10.72 ng/ml

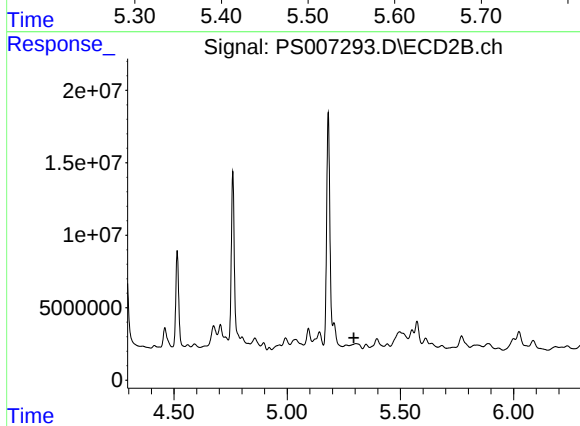

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

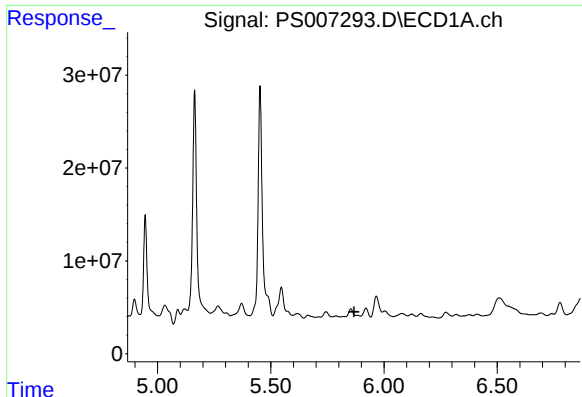

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

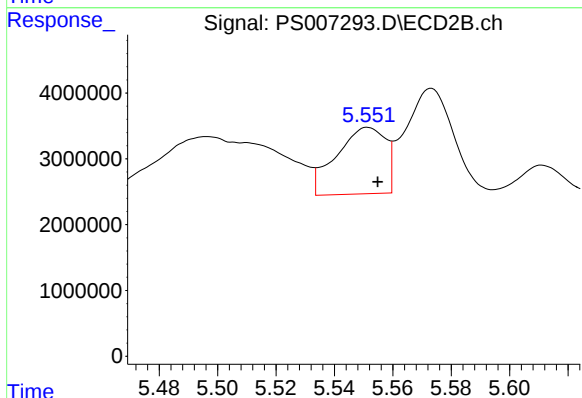


#7 MCPA

R.T.: 5.552 min
Delta R.T.: -0.003 min
Response: 11799710
Conc: 4.06 ug/ml

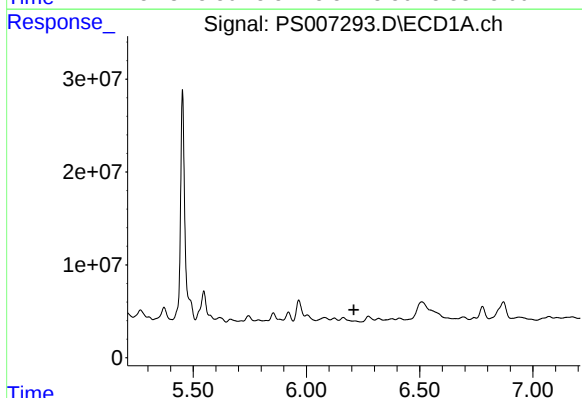


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.209 min
Response: 0
Conc: N.D.

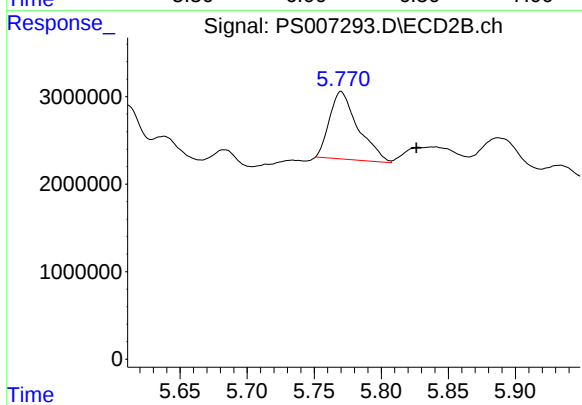

#8 DICHLORPROP


R.T.: 5.770 min
Delta R.T.: -0.056 min
Response: 11366575
Conc: 17.45 ng/ml

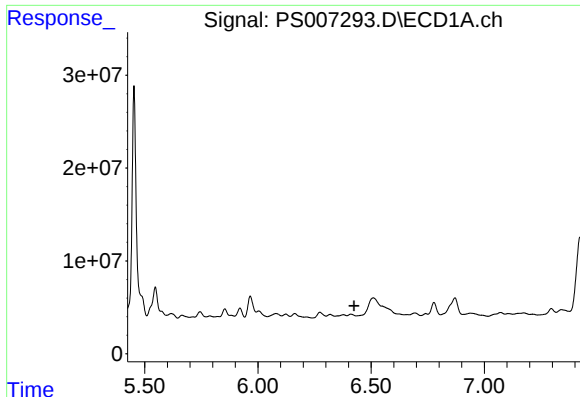

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

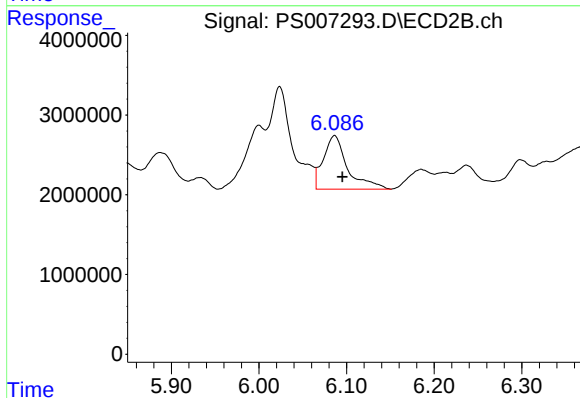


#9 2,4-D

R.T.: 6.086 min
Delta R.T.: -0.009 min
Response: 12885578
Conc: 16.15 ng/ml

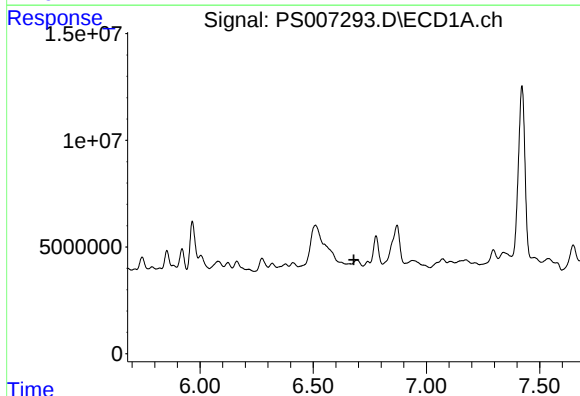


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

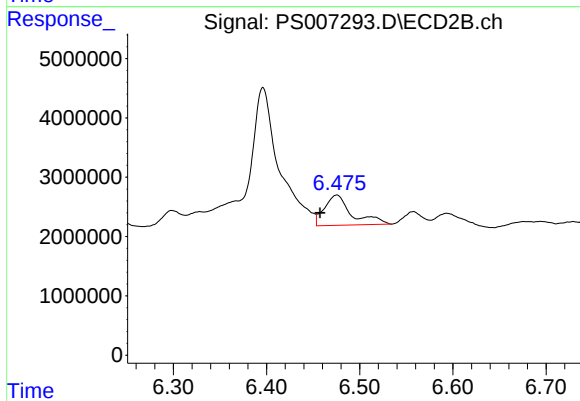

#10 Pentachlorophenol


R.T.: 6.475 min
Delta R.T.: 0.018 min
Response: 10411744
Conc: 1.08 ng/ml

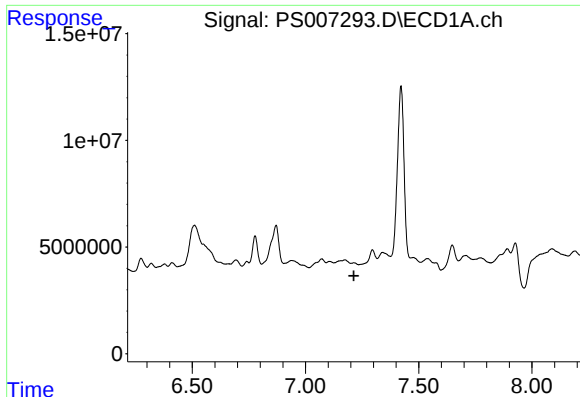

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

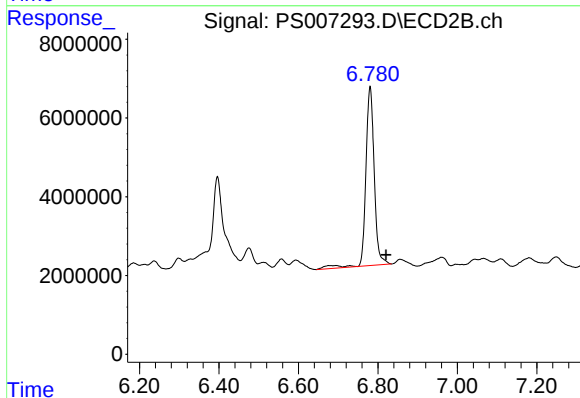


#11 2,4,5-TP (SILVEX)

R.T.: 6.780 min
Delta R.T.: -0.040 min
Response: 67348096
Conc: 17.71 ng/ml

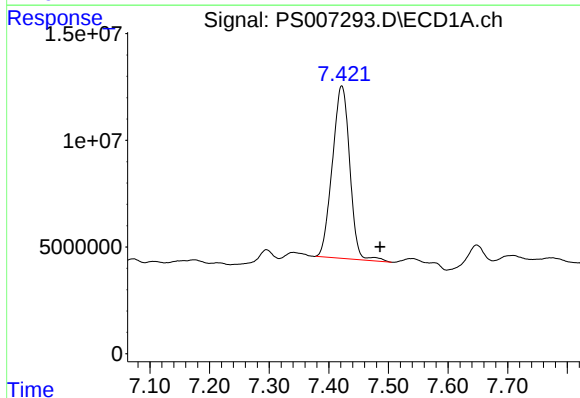


#12 2,4,5-T

R.T.: 7.422 min
Delta R.T.: -0.064 min
Response: 163880309
Conc: 21.44 ng/ml

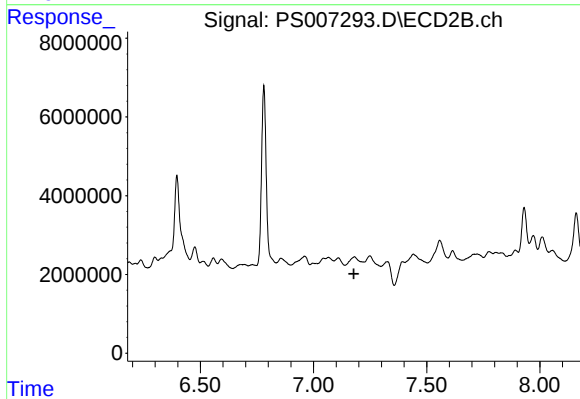

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.178 min
Response: 0
Conc: N.D.

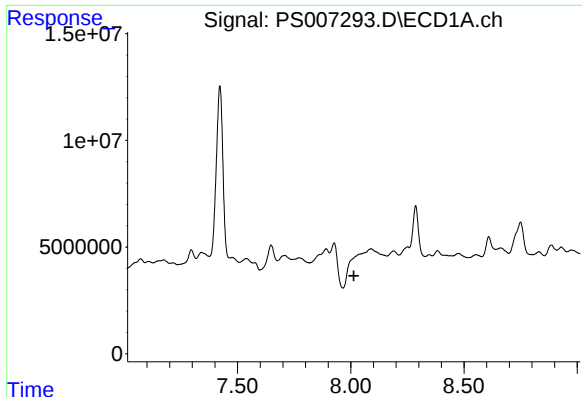

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.014 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

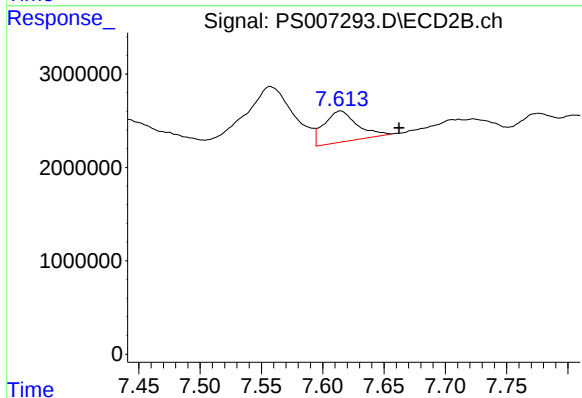


#13 2,4-DB

R.T.: 7.614 min
Delta R.T.: -0.048 min
Response: 6258273
Conc: 13.35 ng/ml

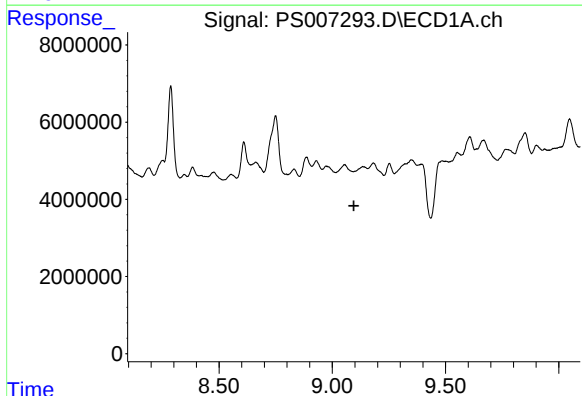


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

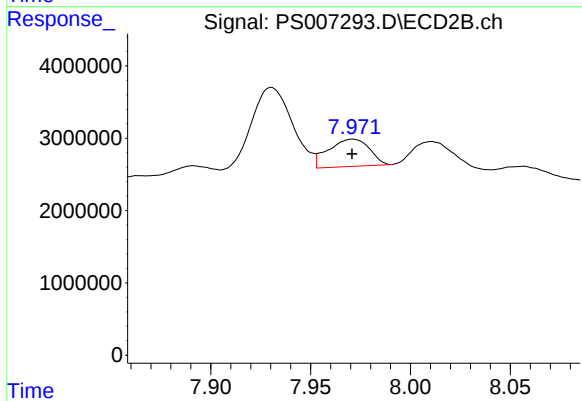

#14 DINOSEB


R.T.: 7.971 min
Delta R.T.: 0.000 min
Response: 5395438
Conc: 1.92 ng/ml

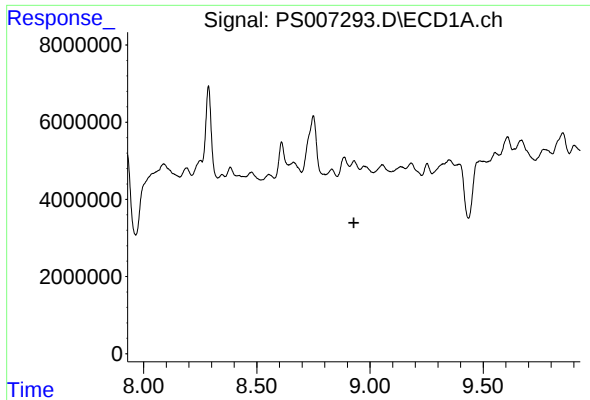

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

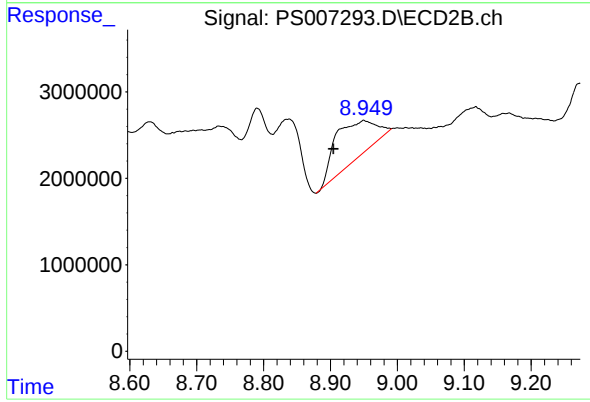

#15 Picloram

R.T.: 8.950 min
Delta R.T.: 0.046 min
Response: 18374048
Conc: 2.99 ng/ml