

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102419\
 Data File : PS007305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2019 18:53
 Operator : SM\AJ
 Sample : K5497-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 01:51:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.436	5.164	335.5E6	176.5E6	245.122	250.892
Target Compounds							
1) T	Dalapon	1.993	1.660	84530867	399.5E6	50.518	438.989 #
2) T	3,5-DICHL...	0.000	4.498	0	31441680	N.D.	36.542
5) T	DICAMBA	5.530	0.000	38771262	0	7.891	N.D. #
7) T	MCPA	0.000	5.555	0	9480429	N.D.	3.261
9) T	2,4-D	6.488	6.069	90371808	9984205	73.333	12.515 #
10) T	Pentachlo...	0.000	6.458	0	7463817	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.763	0	47024764	N.D.	12.363
14) T	DINOSEB	0.000	7.914	0	9707933	N.D.	3.458
15) T	Picloram	0.000	8.939	0	18329806	N.D.	2.985
16) T	DCPA	0.000	8.812	0	21947699	N.D.	4.377



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102419\
Data File : PS007305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2019 18:53
Operator : SM\AJ
Sample : K5497-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 01:51:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

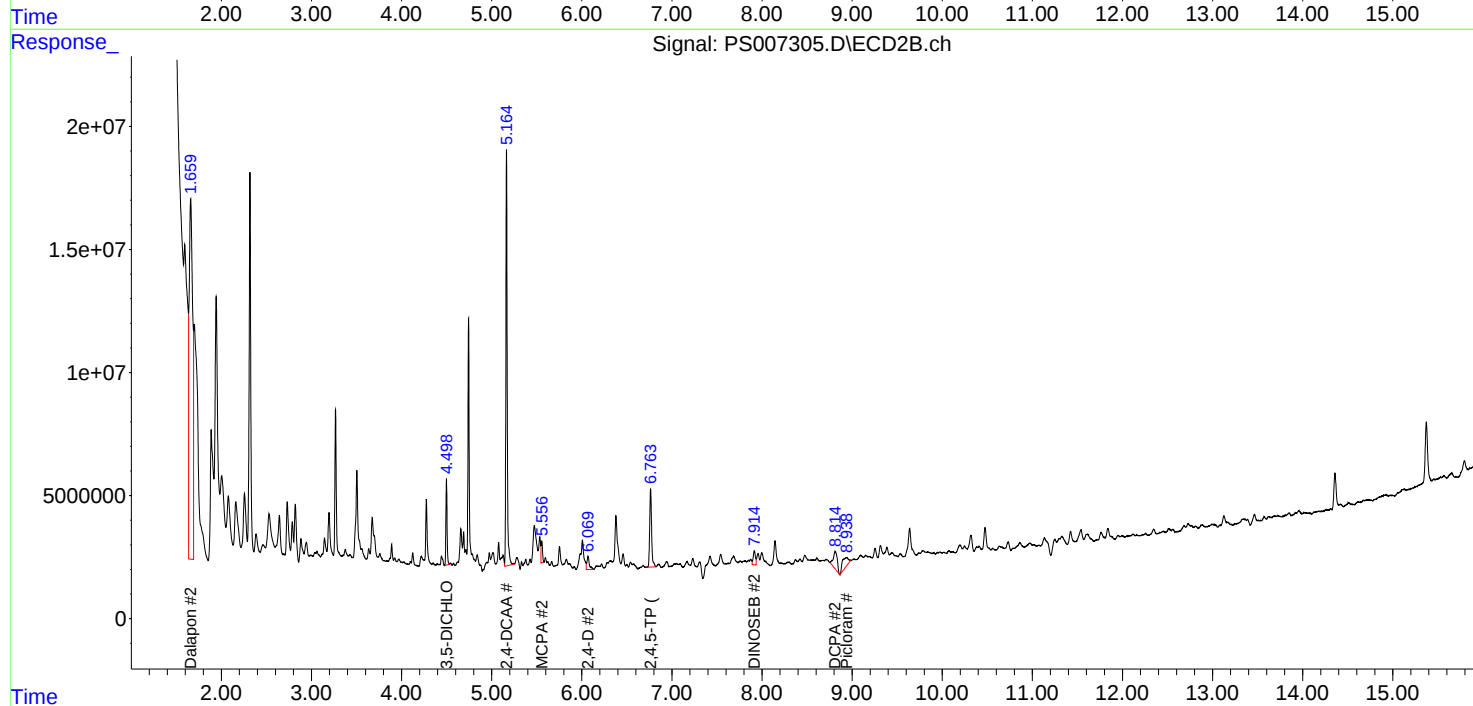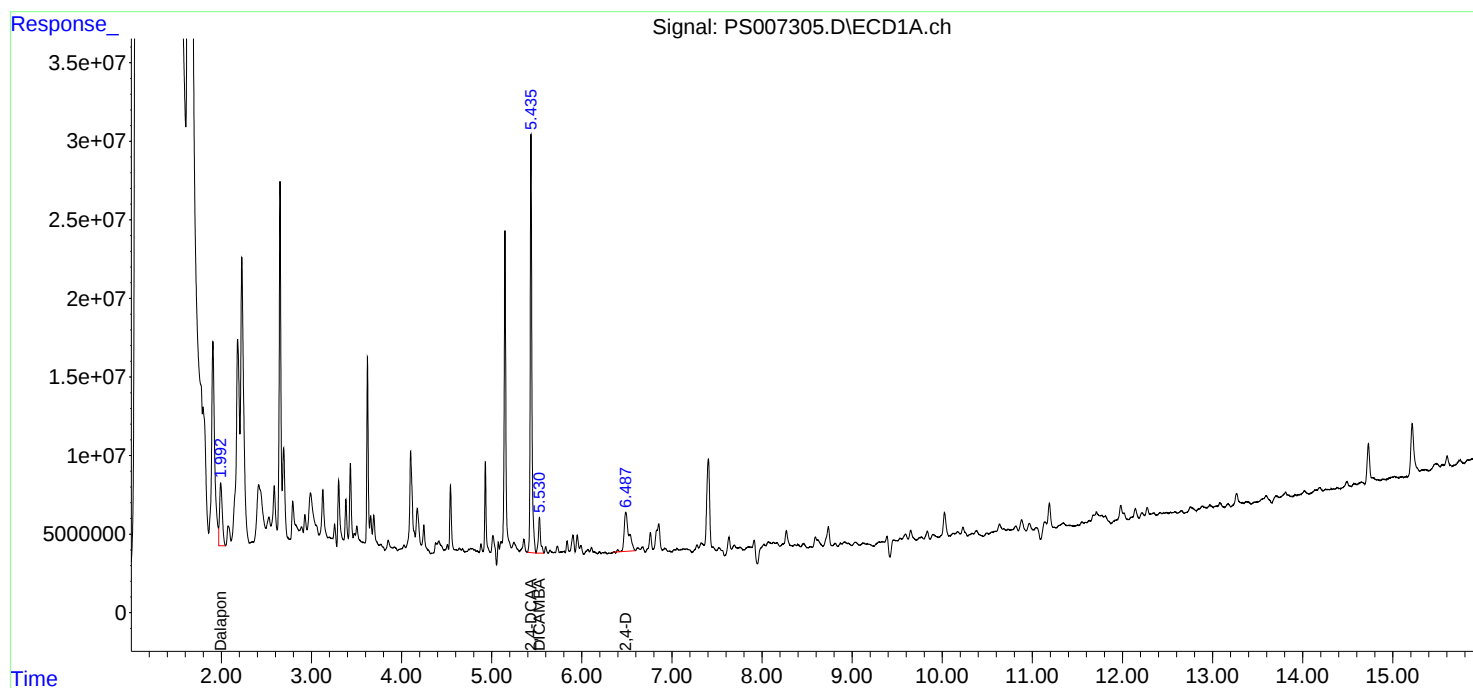


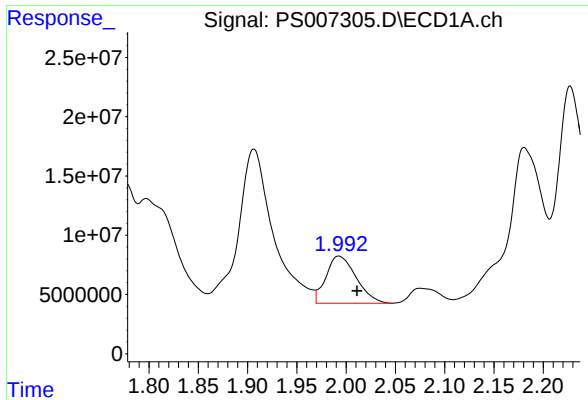

#1 Dalapon


R.T.: 1.993 min
Delta R.T.: -0.018 min
Response: 84530867
Conc: 50.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

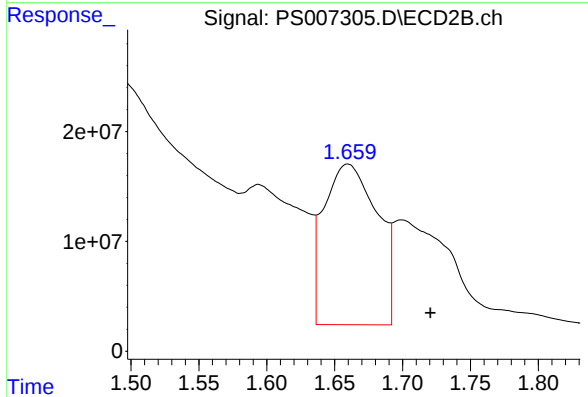


#1 Dalapon

R.T.: 1.660 min
Delta R.T.: -0.061 min
Response: 399481636
Conc: 438.99 ng/ml

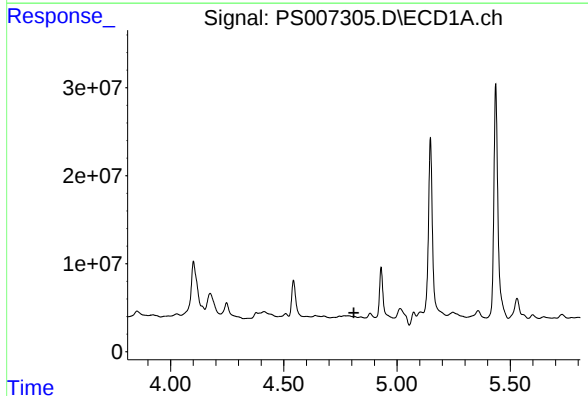


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

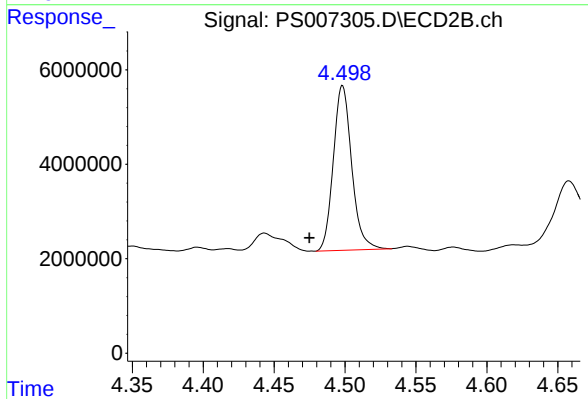

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.498 min
Delta R.T.: 0.024 min
Response: 31441680
Conc: 36.54 ng/ml

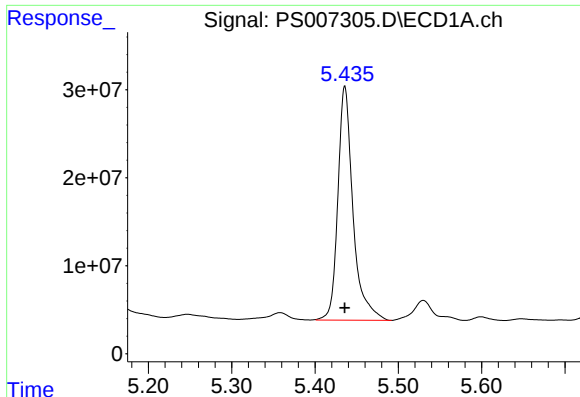

#4 2,4-DCAA


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 335490288
Conc: 245.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

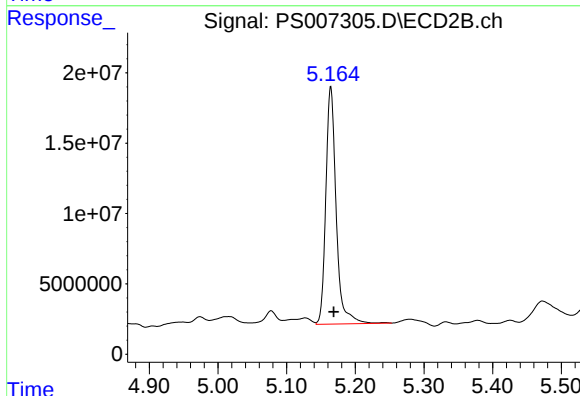


#4 2,4-DCAA

R.T.: 5.164 min
Delta R.T.: -0.004 min
Response: 176453727
Conc: 250.89 ng/ml

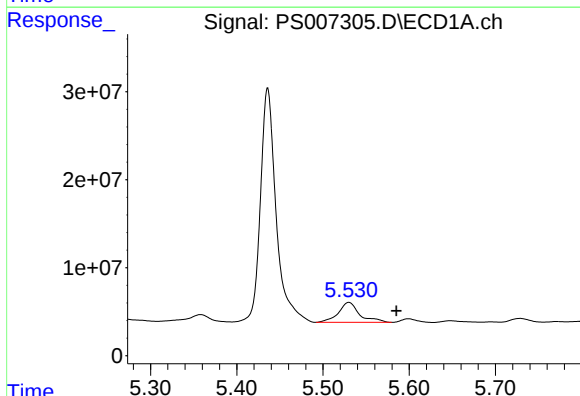


#5 DICAMBA

R.T.: 5.530 min
Delta R.T.: -0.055 min
Response: 38771262
Conc: 7.89 ng/ml

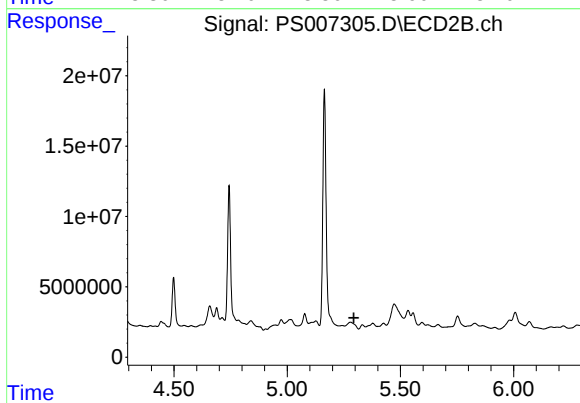

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

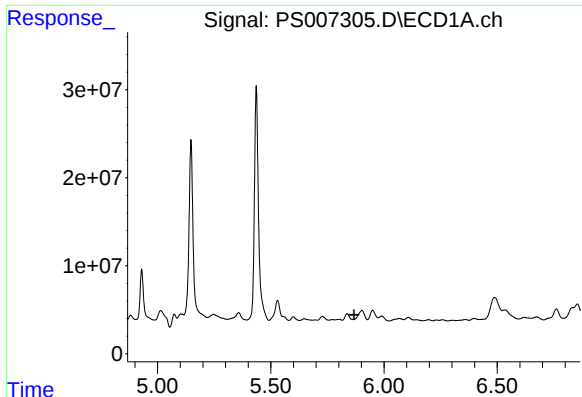

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

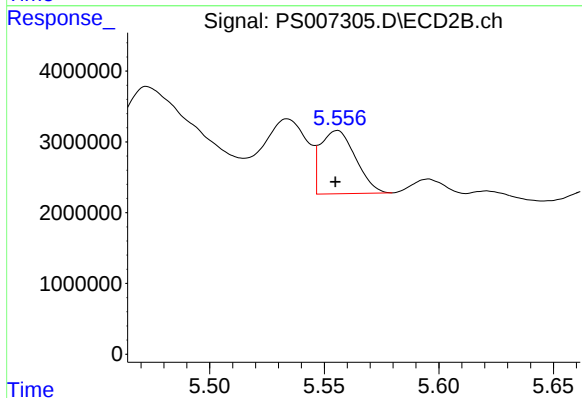


#7 MCPA

R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 9480429
Conc: 3.26 ug/ml

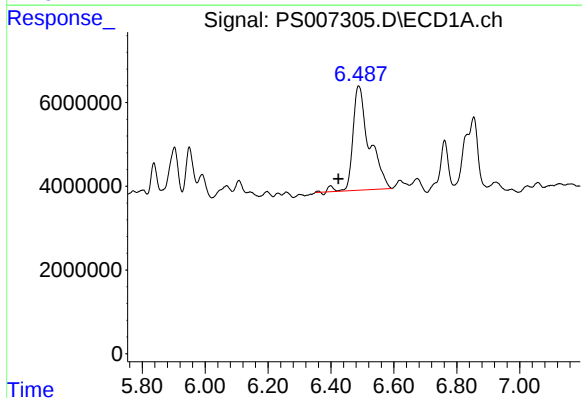


#9 2,4-D

R.T.: 6.488 min
Delta R.T.: 0.064 min
Response: 90371808
Conc: 73.33 ng/ml

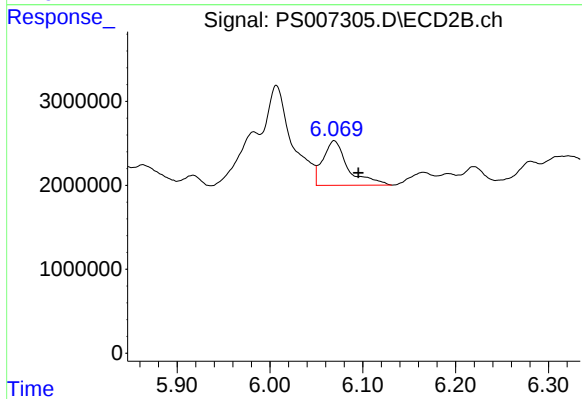

#9 2,4-D


R.T.: 6.069 min
Delta R.T.: -0.026 min
Response: 9984205
Conc: 12.51 ng/ml

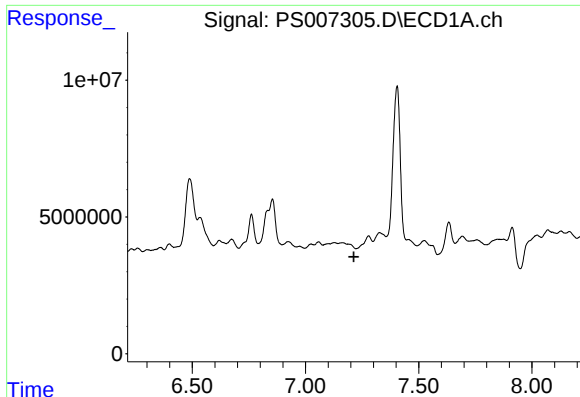

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

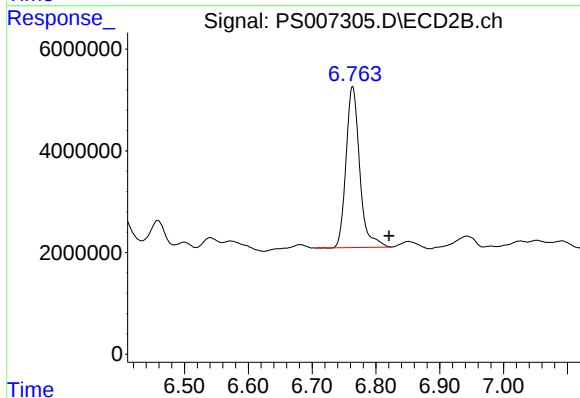


#11 2,4,5-TP (SILVEX)

R.T.: 6.763 min
Delta R.T.: -0.057 min
Response: 47024764
Conc: 12.36 ng/ml

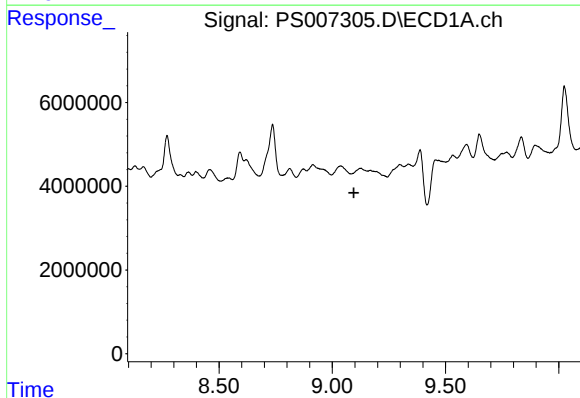


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

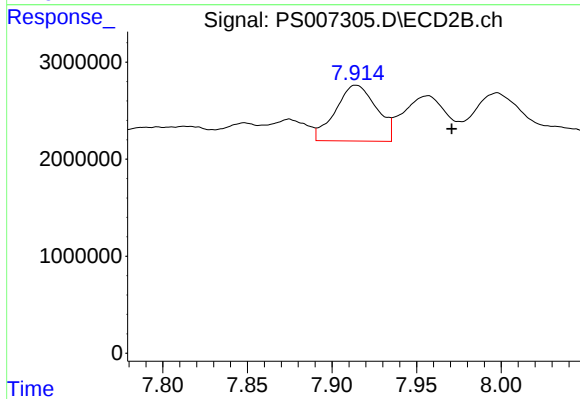

#14 DINOSEB


R.T.: 7.914 min
Delta R.T.: -0.056 min
Response: 9707933
Conc: 3.46 ng/ml

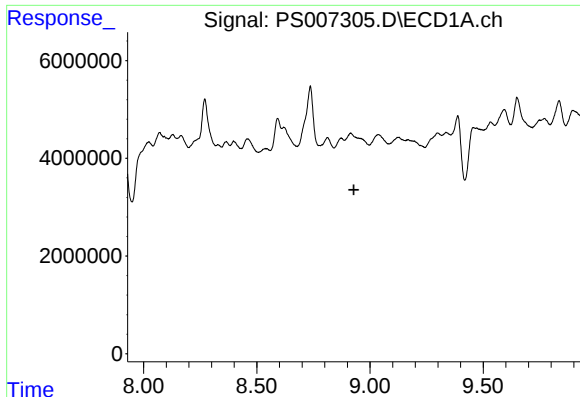

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

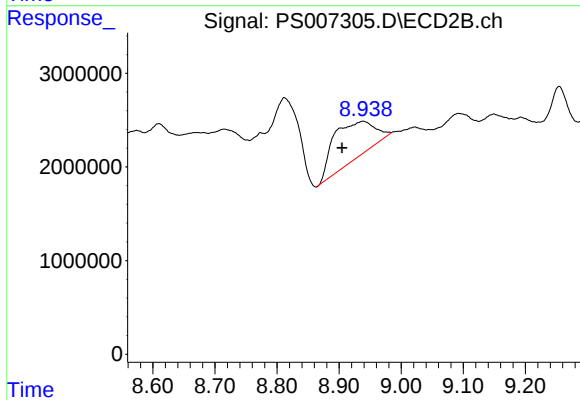


#15 Picloram

R.T.: 8.939 min
Delta R.T.: 0.034 min
Response: 18329806
Conc: 2.99 ng/ml

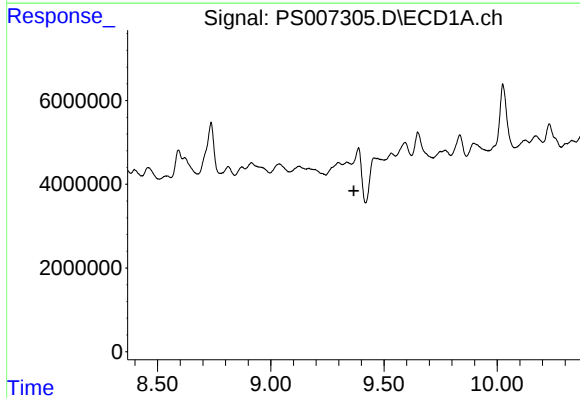

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

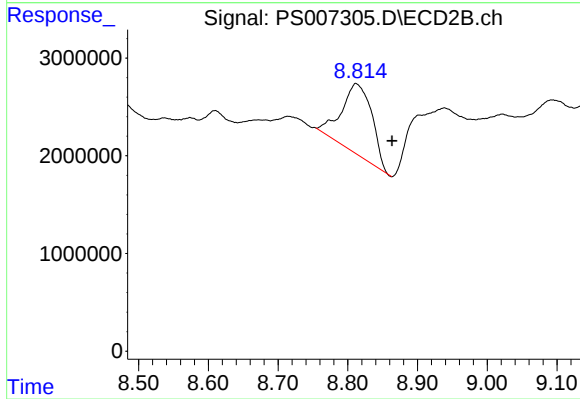

#16 DCPA

R.T.: 8.812 min
Delta R.T.: -0.051 min
Response: 21947699
Conc: 4.38 ng/ml