

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102419\
 Data File : PS007313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2019 21:49
 Operator : SM\AJ
 Sample : K5498-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 01:54:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.436	5.165	358.9E6	184.0E6	262.200	261.605
Target Compounds							
1) T	Dalapon	1.995	1.705	79363252	228.2E6	47.430	250.738 #
2) T	3,5-DICHL...	0.000	4.498	0	46378853	N.D.	53.902
5) T	DICAMBA	5.530	0.000	44981070	0	9.155	N.D. #
7) T	MCPA	0.000	5.535	0	19242660	N.D.	6.619
9) T	2,4-D	6.489	6.070	78255695	9207501	63.502	11.541 #
10) T	Pentachlo...	0.000	6.459	0	8348929	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.763	0	41127246	N.D.	10.813
14) T	DINOSEB	0.000	7.958	0	10489634	N.D.	3.736
15) T	Picloram	0.000	8.948	0	24324635	N.D.	3.962



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102419\
Data File : PS007313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2019 21:49
Operator : SM\AJ
Sample : K5498-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 01:54:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

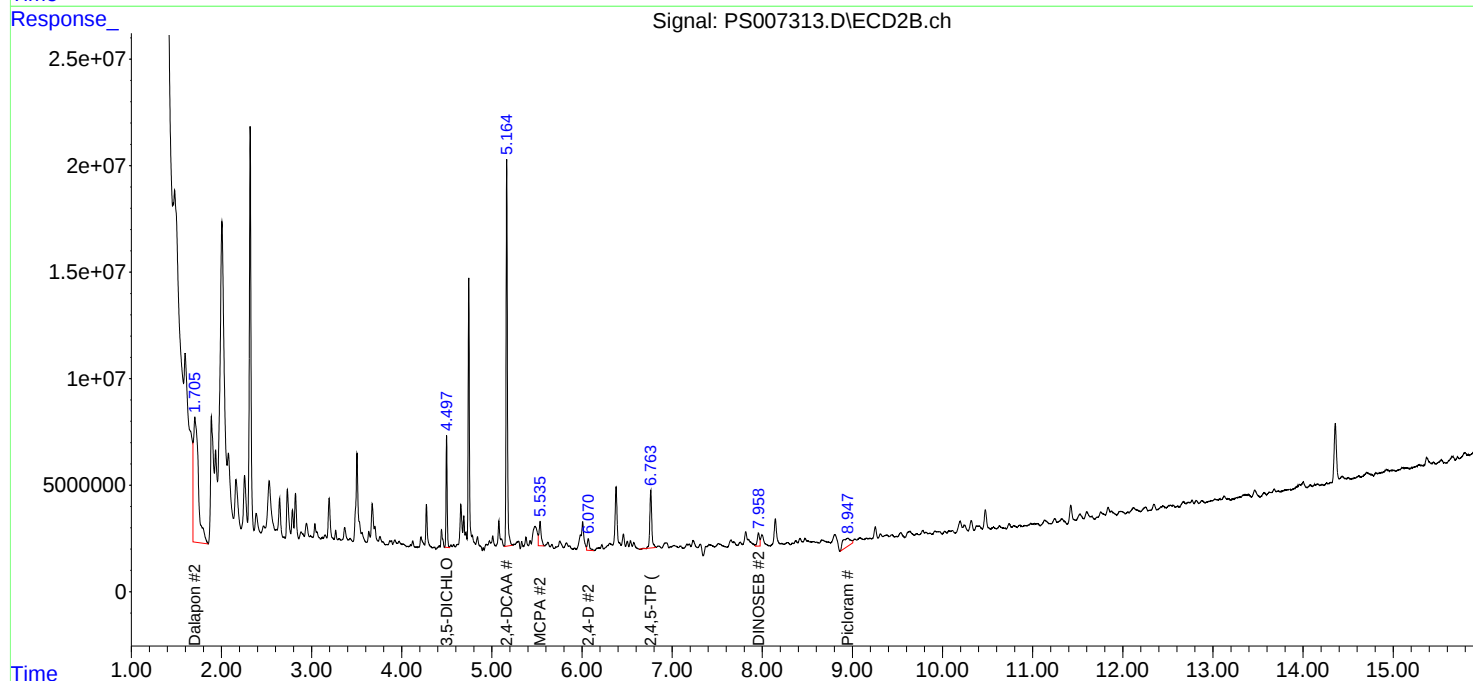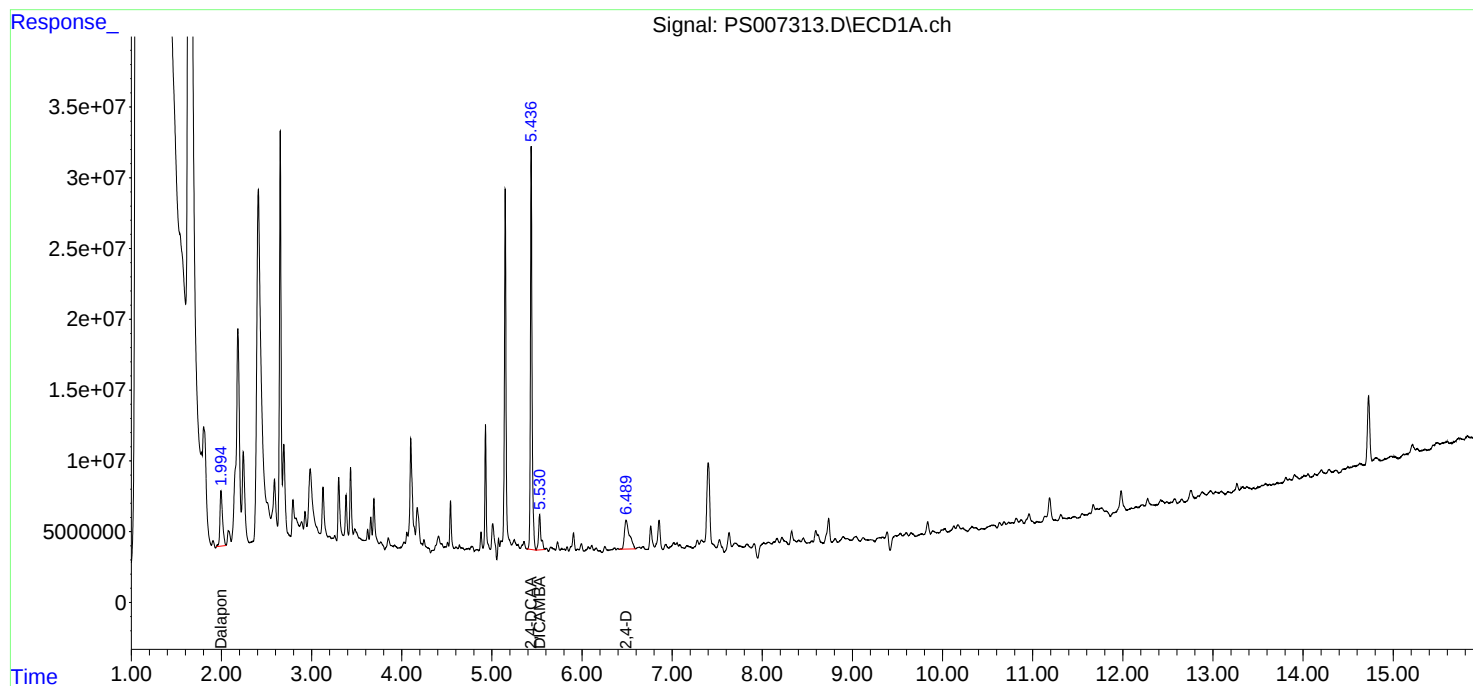


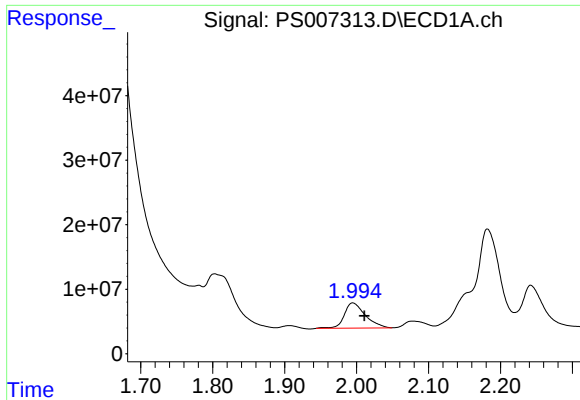

#1 Dalapon


R.T.: 1.995 min
Delta R.T.: -0.016 min
Response: 79363252
Conc: 47.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

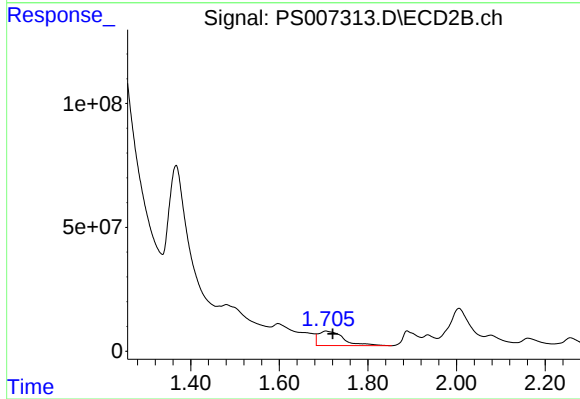


#1 Dalapon

R.T.: 1.705 min
Delta R.T.: -0.015 min
Response: 228172907
Conc: 250.74 ng/ml

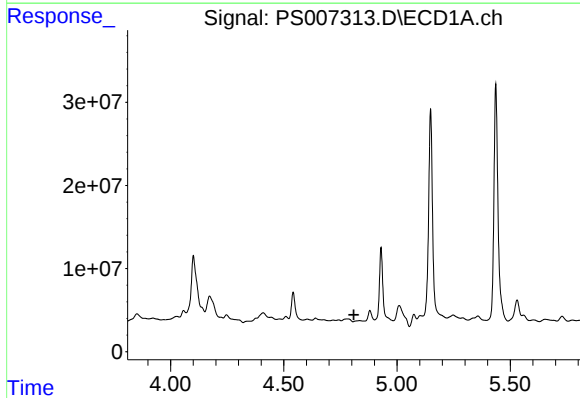


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

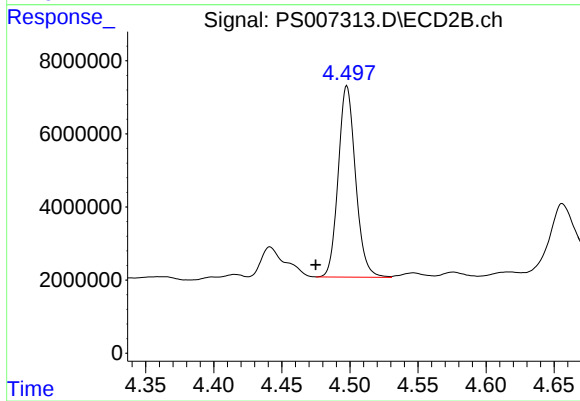

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.498 min
Delta R.T.: 0.023 min
Response: 46378853
Conc: 53.90 ng/ml

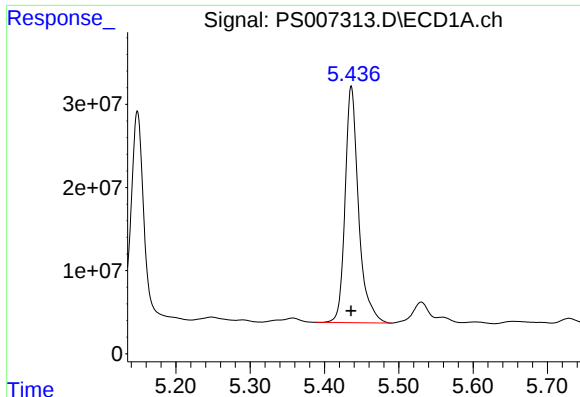

#4 2,4-DCAA


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 358865065
Conc: 262.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

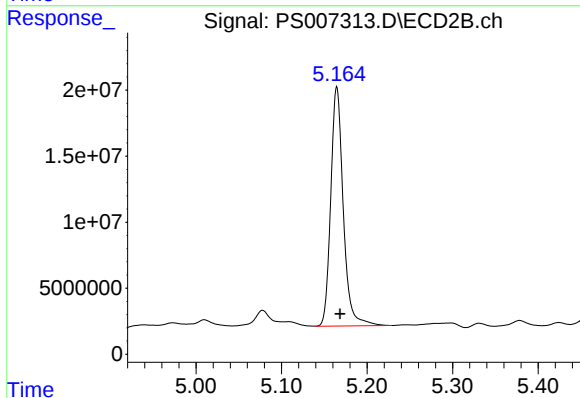


#4 2,4-DCAA

R.T.: 5.165 min
Delta R.T.: -0.004 min
Response: 183988235
Conc: 261.60 ng/ml

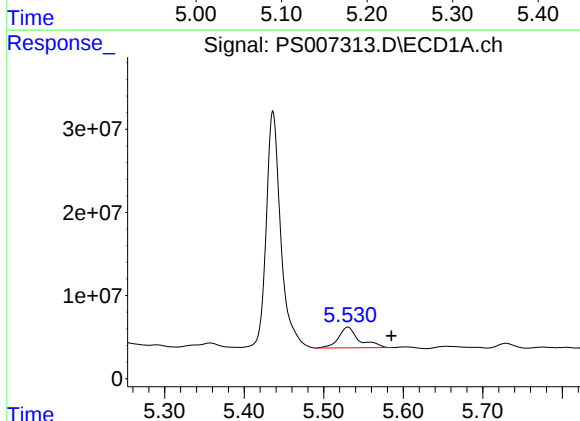


#5 DICAMBA

R.T.: 5.530 min
Delta R.T.: -0.055 min
Response: 44981070
Conc: 9.15 ng/ml

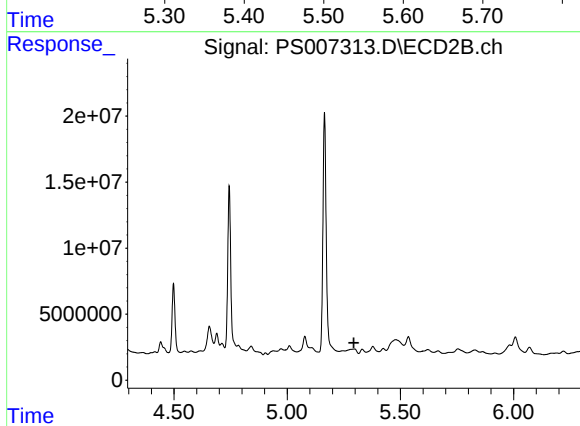

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

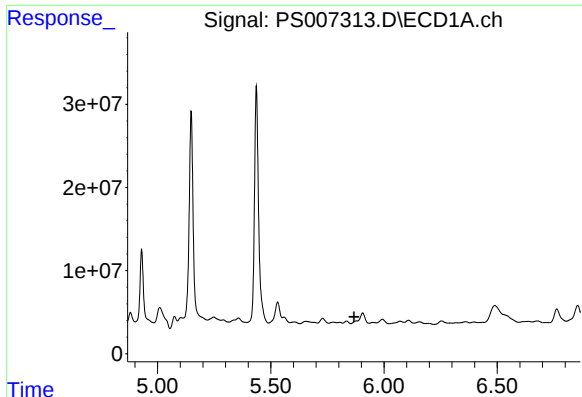

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

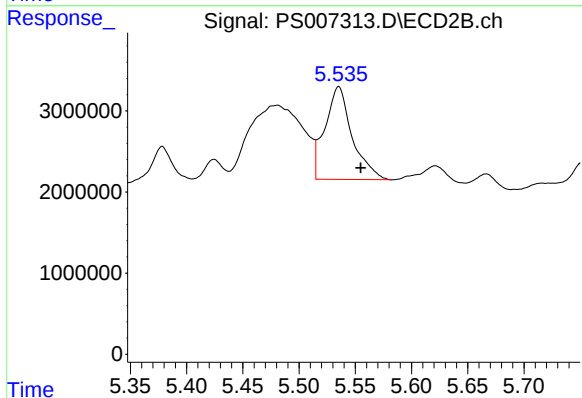


#7 MCPA

R.T.: 5.535 min
Delta R.T.: -0.020 min
Response: 19242660
Conc: 6.62 ug/ml

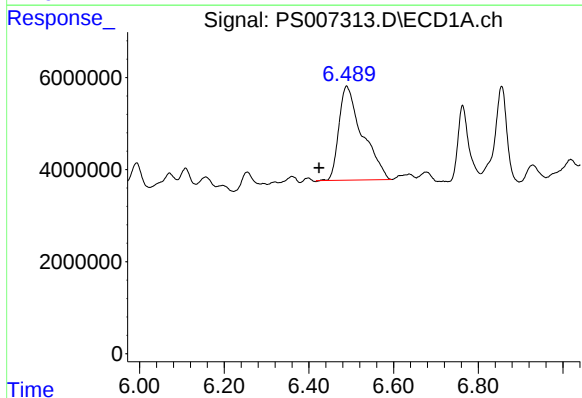


#9 2,4-D

R.T.: 6.489 min
Delta R.T.: 0.065 min
Response: 78255695
Conc: 63.50 ng/ml

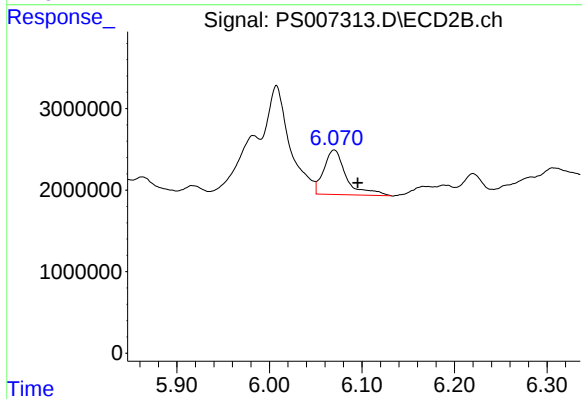

#9 2,4-D


R.T.: 6.070 min
Delta R.T.: -0.025 min
Response: 9207501
Conc: 11.54 ng/ml

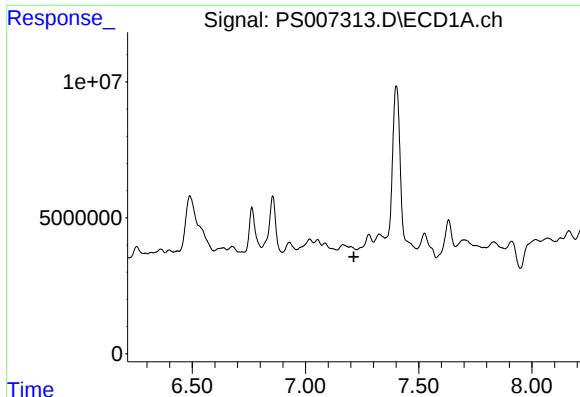

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

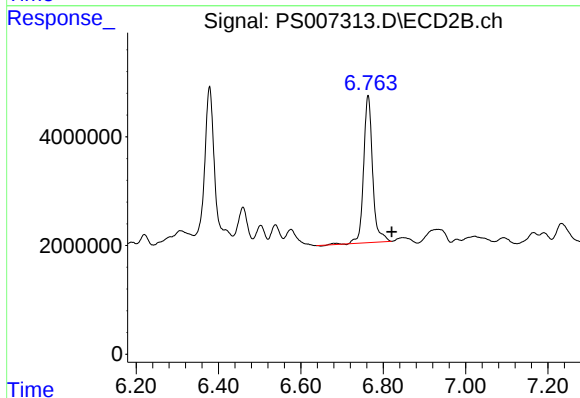


#11 2,4,5-TP (SILVEX)

R.T.: 6.763 min
Delta R.T.: -0.057 min
Response: 41127246
Conc: 10.81 ng/ml

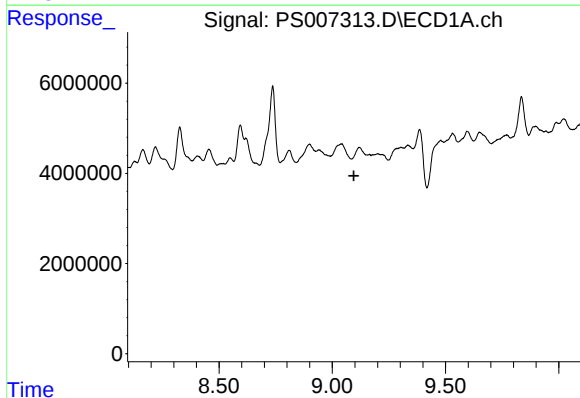


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

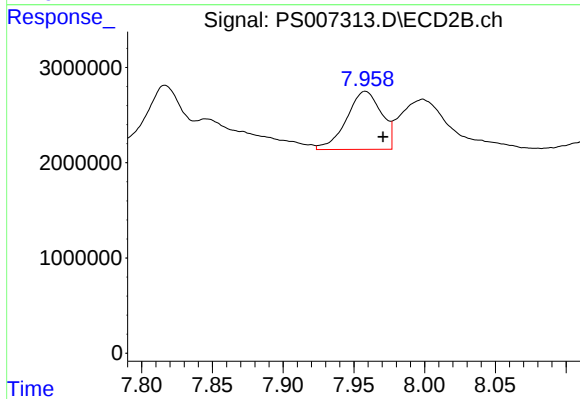

#14 DINOSEB


R.T.: 7.958 min
Delta R.T.: -0.013 min
Response: 10489634
Conc: 3.74 ng/ml

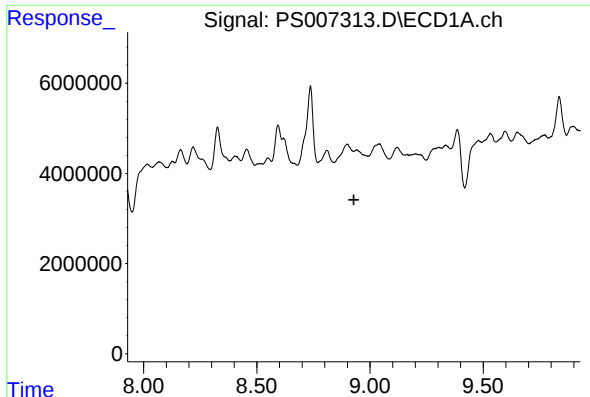

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

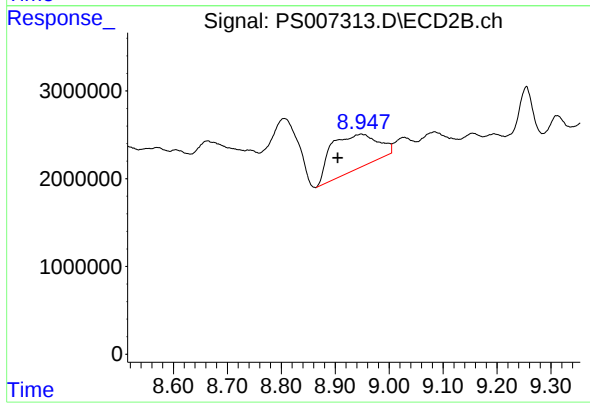

#15 Picloram

R.T.: 8.948 min
Delta R.T.: 0.044 min
Response: 24324635
Conc: 3.96 ng/ml