

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102419\
Data File : PS007328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2019 03:17
Operator : SM\AJ
Sample : K5497-19 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
189-04-(0-1.2)

Manual Integrations
APPROVED

Ankita
10/25/2019 10:56:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 04:03:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	5.435	5.161	33097117	15520337	24.182	22.068m
------	----------	-------	-------	----------	----------	--------	---------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102419\
Data File : PS007328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2019 03:17
Operator : SM\AJ
Sample : K5497-19 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
189-04-(0-1.2)


Manual Integrations
APPROVED

Ankita
10/25/2019 10:56:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 04:03:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

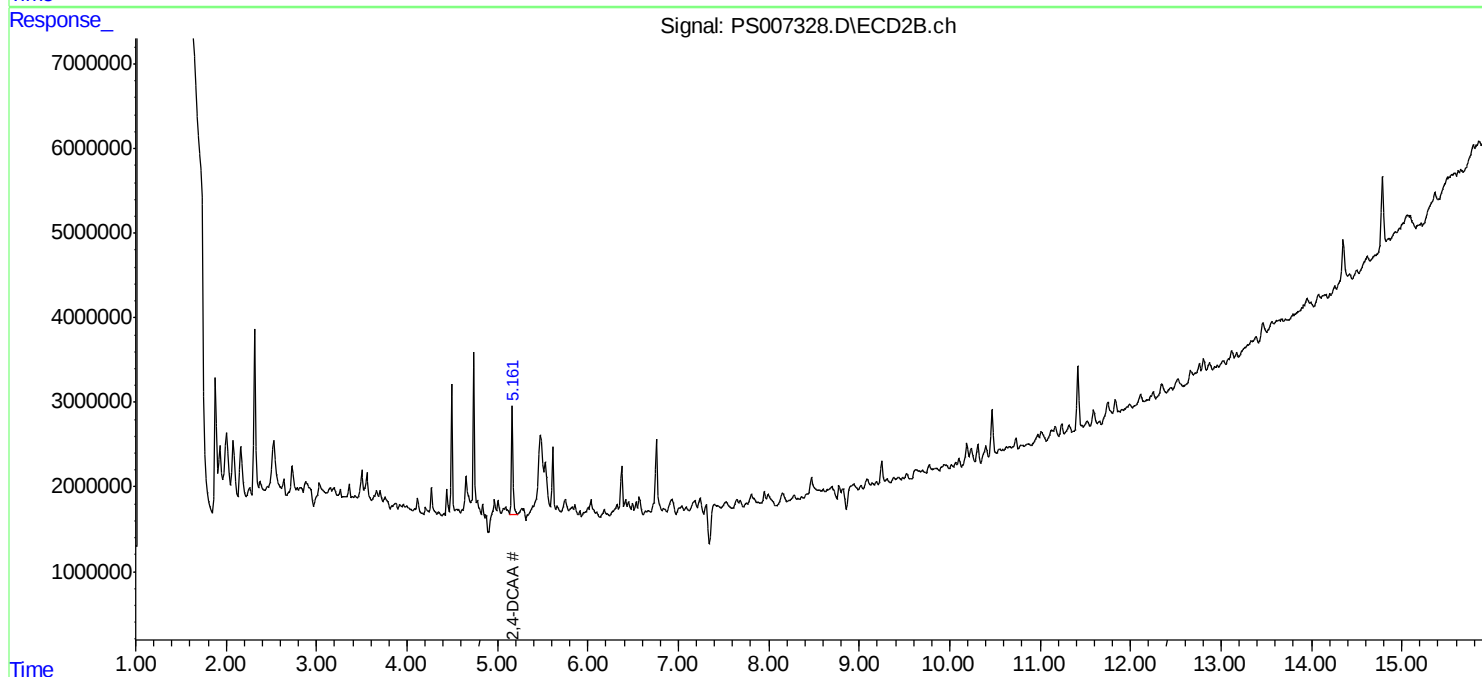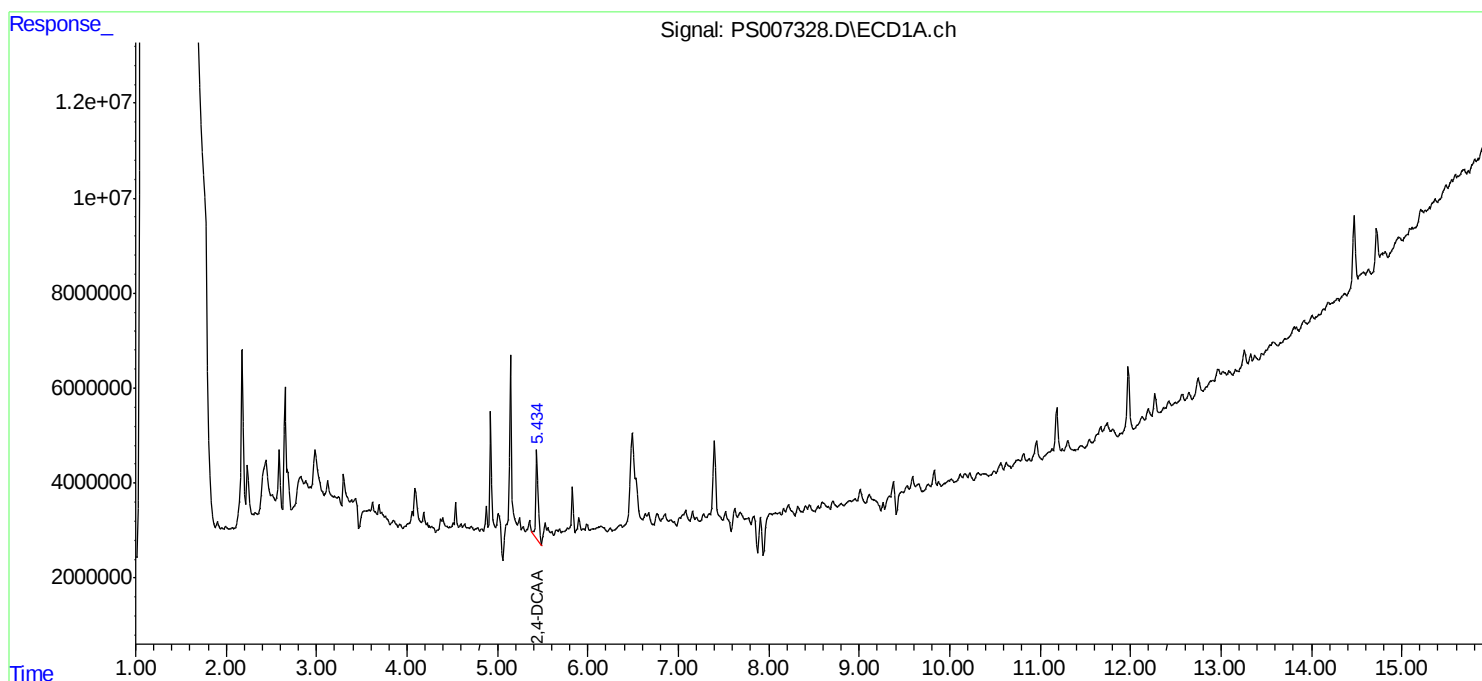

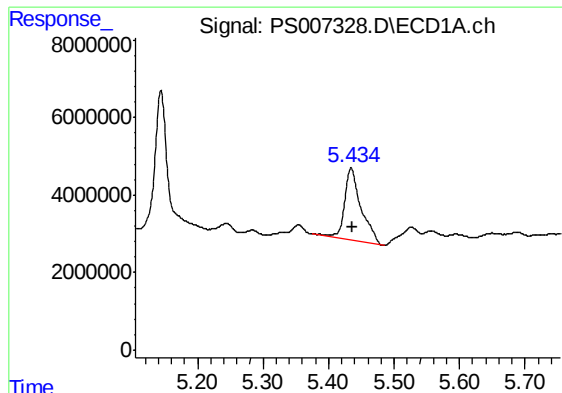


#4 2,4-DCAA

R.T.: 5.435 min
Delta R.T.: -0.001 min
Response: 33097117
Conc: 24.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
189-04-(0-1.2)

Manual Integrations
APPROVED

Ankita
10/25/2019 10:56:47 AM

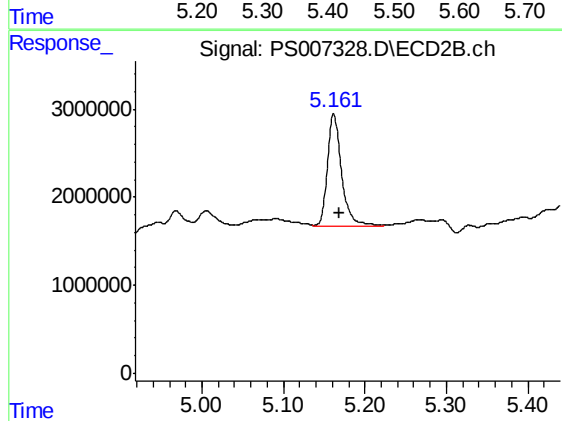

#4 2,4-DCAA

R.T.: 5.161 min
Delta R.T.: -0.007 min
Response: 15520337
Conc: 22.07 ng/ml m