

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102422\
 Data File : PS020855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 15:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 18:37:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.415	6.857	982.0E6	658.0E6	520.574	491.414
Target Compounds							
1) T	Dalapon	2.515	0.000	316091	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.796	6.105f	2165489	-3006	<MDL	N.D. #
5) T	DICAMBA	6.562	0.000	1260816	0	<MDL	N.D. #
6) T	MCP	6.742	0.000	3921534	0	<MDL	N.D. #
7) T	MCPA	6.914f	0.000	222492	0	<MDL	N.D. #
8) T	DICHLORPROP	7.209	7.672	664399	1390792	<MDL	<MDL #
10) T	Pentachlo...	7.595	8.379	304650	2357242	<MDL	<MDL #
11) T	2,4,5-TP ...	8.123	8.760	10684215	3998252	<MDL	<MDL #
12) T	2,4,5-T	8.397	9.115	14836808	2950055	1.335	<MDL #
13) T	2,4-DB	8.879	0.000	713332	0	<MDL	N.D. #
14) T	DINOSEB	9.961	0.000	2942840	0	<MDL	N.D. #
15) T	Picloram	9.777	10.924	12711828	7288543	<MDL	<MDL #
16) T	DCPA	10.220	10.924	2316069	7288543	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102422\
Data File : PS020855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2022 15:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 18:37:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

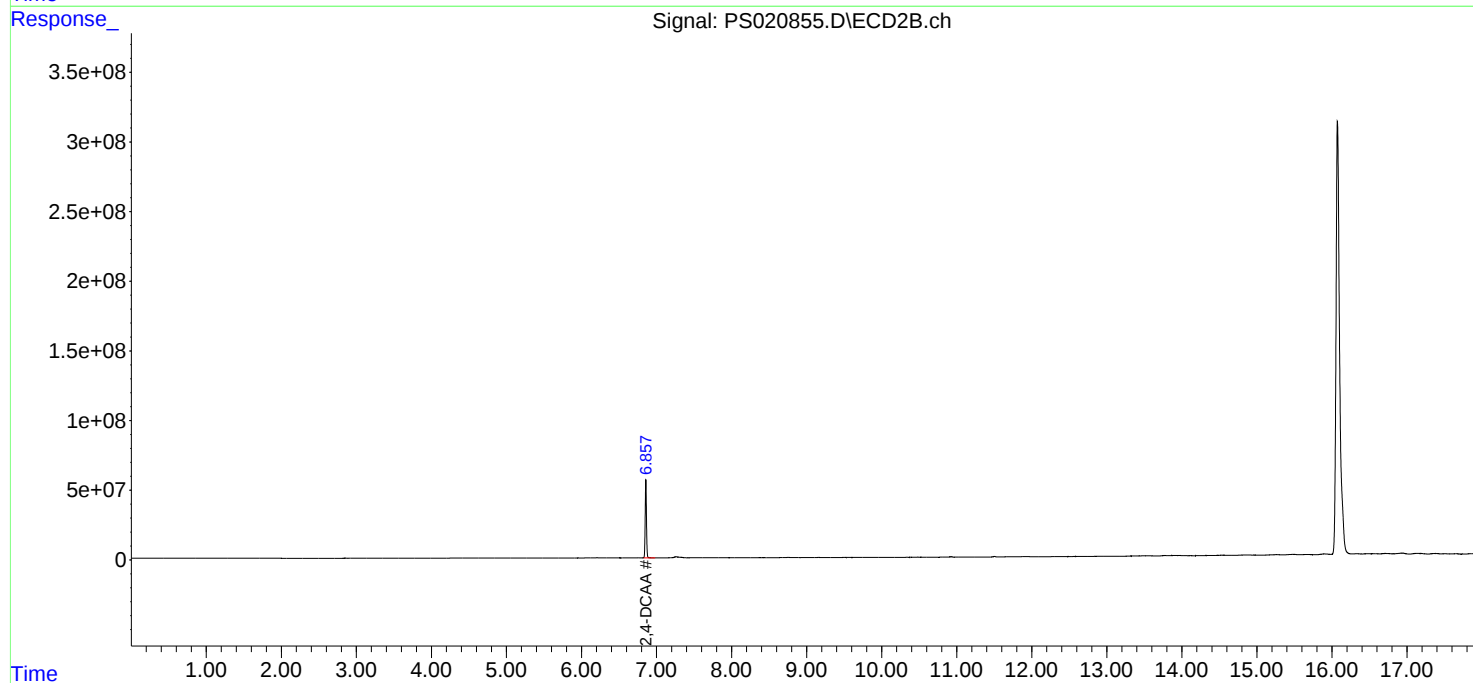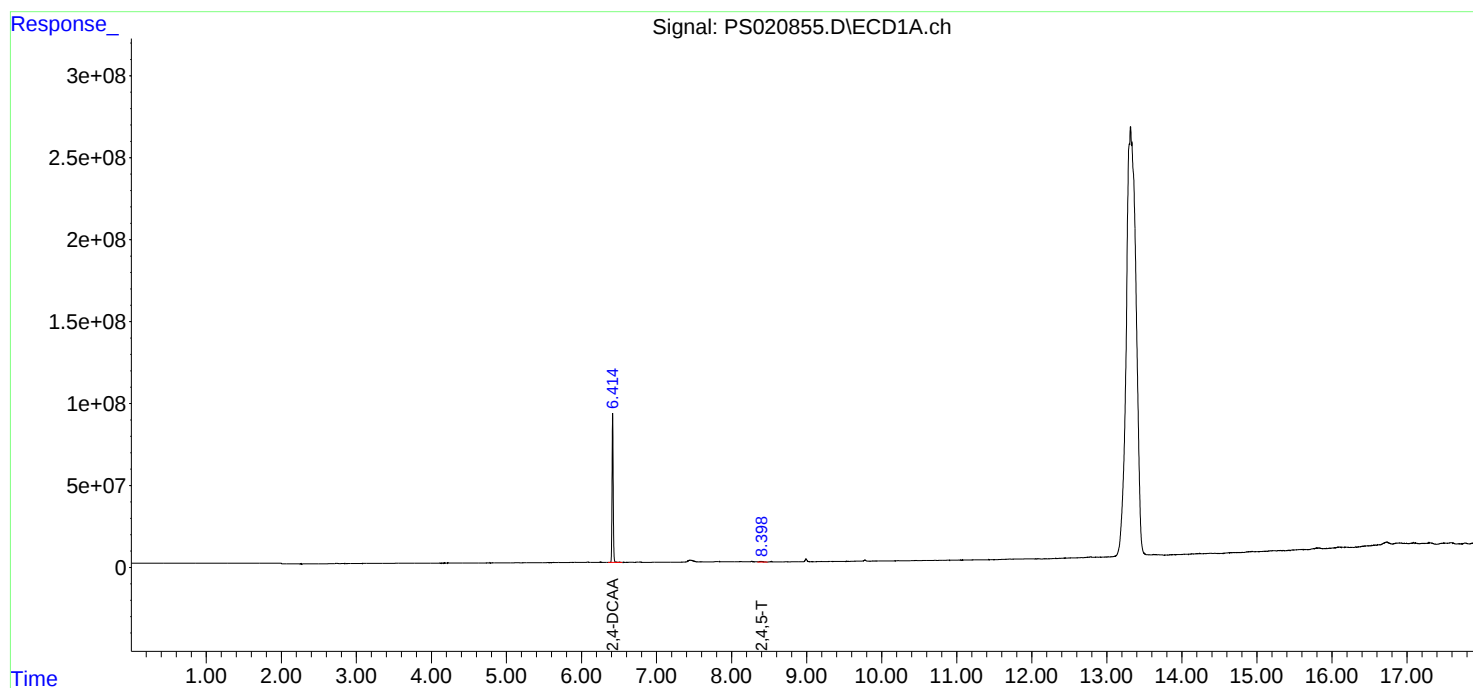


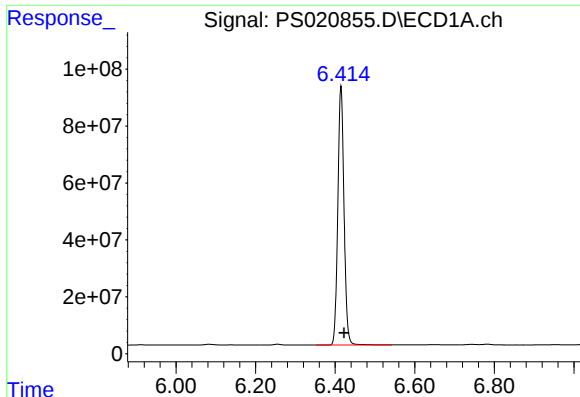

#4 2,4-DCAA


R.T.: 6.415 min
Delta R.T.: -0.007 min
Response: 982037268
Conc: 520.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

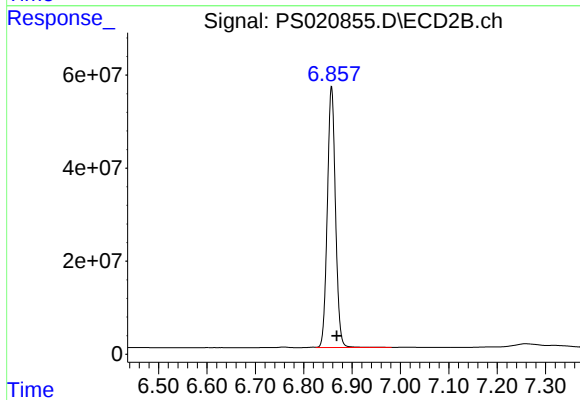


#4 2,4-DCAA

R.T.: 6.857 min
Delta R.T.: -0.011 min
Response: 657993903
Conc: 491.41 ng/ml

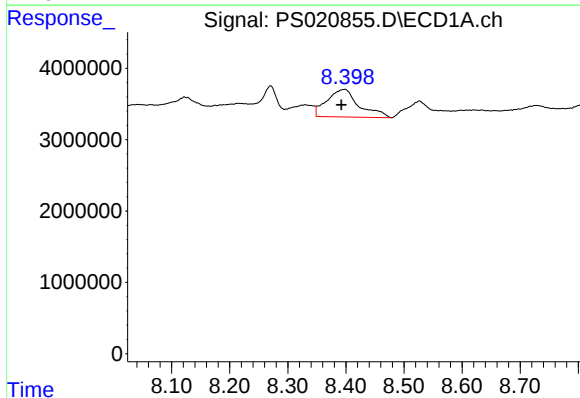

#12 2,4,5-T

R.T.: 8.397 min
Delta R.T.: 0.005 min
Response: 14836808
Conc: 1.33 ng/ml

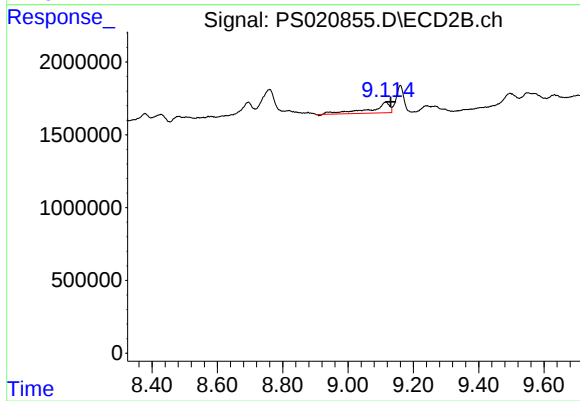

#12 2,4,5-T

R.T.: 9.115 min
Delta R.T.: -0.016 min
Response: 2950055
Conc: N.D.