

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102423\
 Data File : PS024678.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 08:35
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 11:45:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	0.000	2.569	0	2657325	N.D. 2.374
5) T	DICAMBA	0.000	6.982	0	12153286	N.D. 4.104
6) T	MCP	0.000	6.982f	0	12153286	N.D. 6.167
7) T	MCPA	0.000	7.239	0	4889828	N.D. 1.526
8) T	DICHLORPROP	0.000	7.570	0	1069752	N.D. 1.422
9) T	2,4-D	7.249	7.786f	129.7E6	595424	46.933 <MDL #
11) T	2,4,5-TP ...	0.000	8.621	0	431145	N.D. <MDL
12) T	2,4,5-T	0.000	9.035	0	3668689	N.D. <MDL
15) T	Picloram	9.657	10.777	15452113	21111447	<MDL 3.397 #
16) T	DCPA	0.000	10.777	0	21111447	N.D. 4.046



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102423\
Data File : PS024678.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 08:35
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 11:45:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

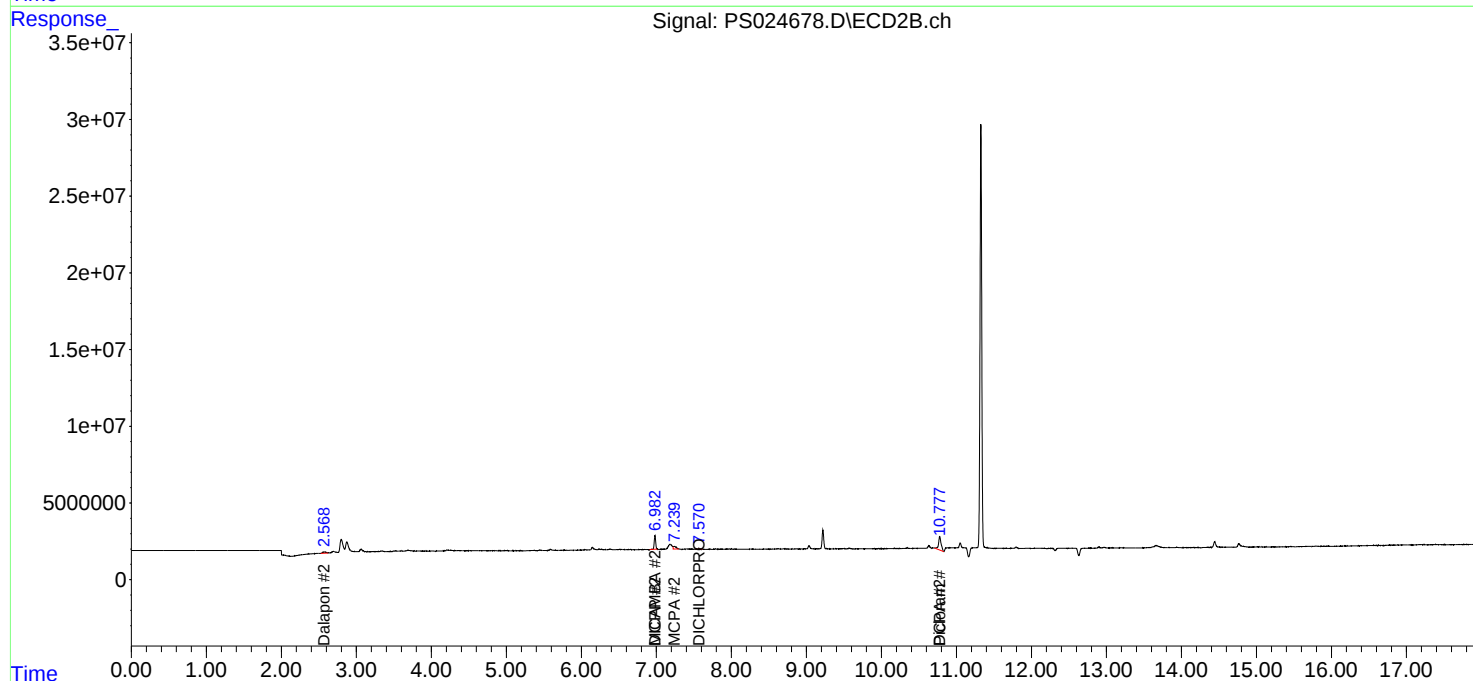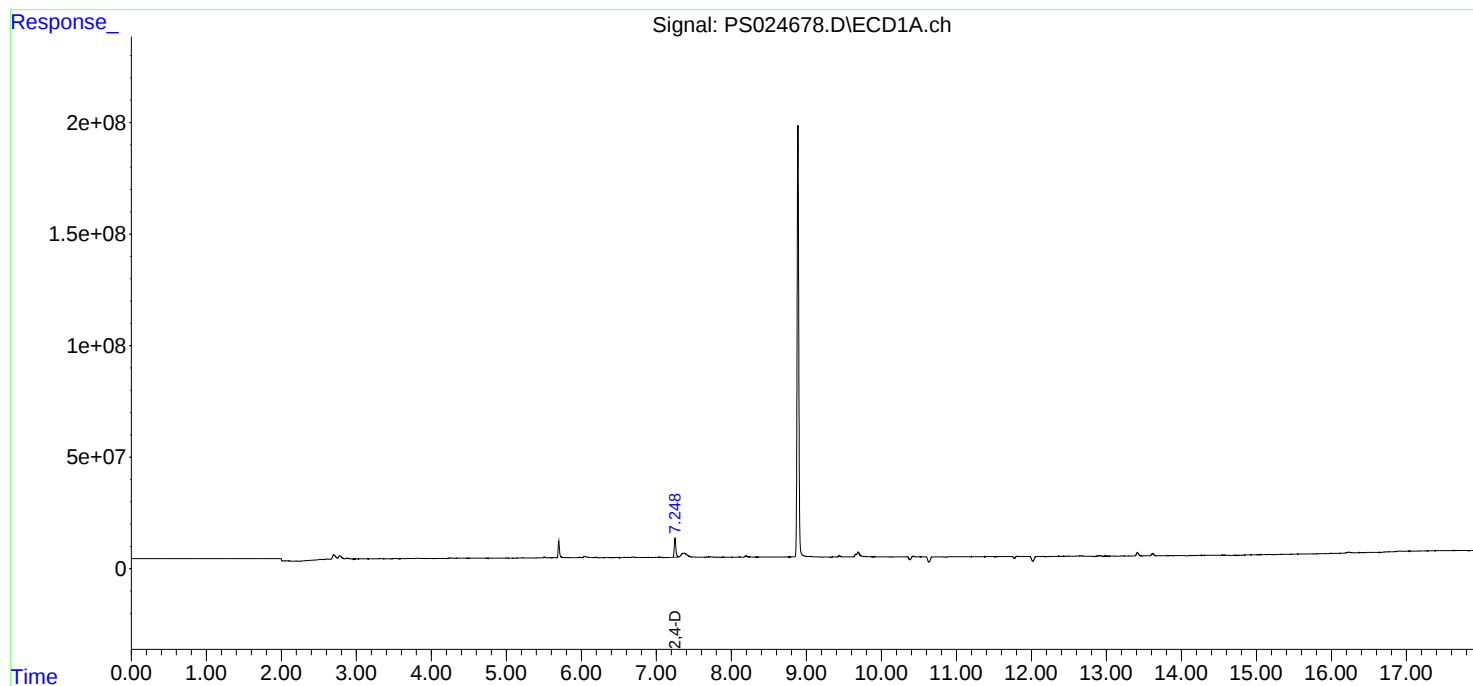


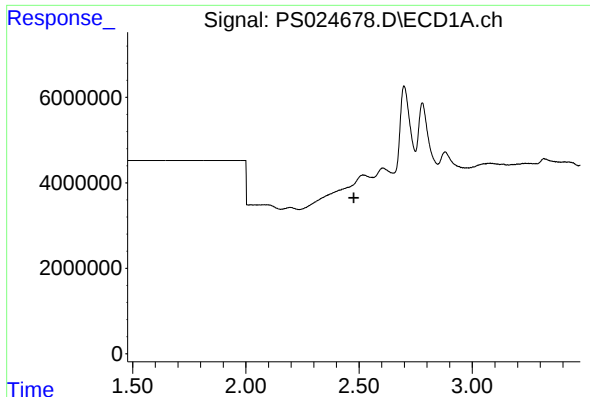

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

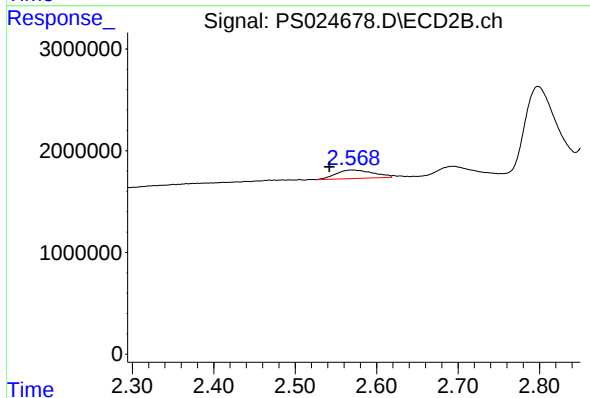


#1 Dalapon

R.T.: 2.569 min
Delta R.T.: 0.027 min
Response: 2657325
Conc: 2.37 ng/ml

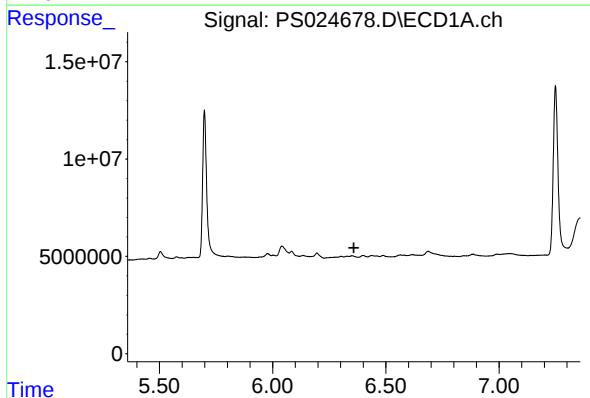


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.359 min
Response: 0
Conc: N.D.

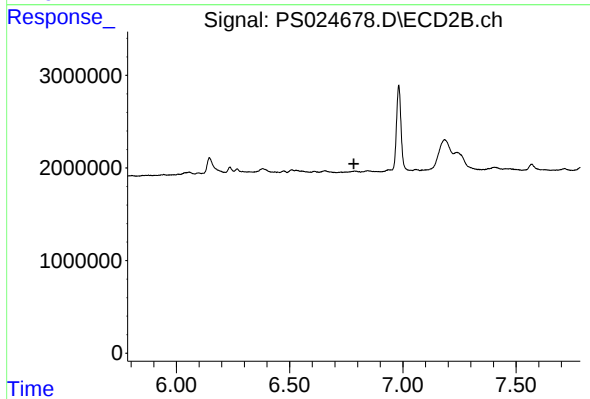

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.784 min
Response: 0
Conc: N.D.

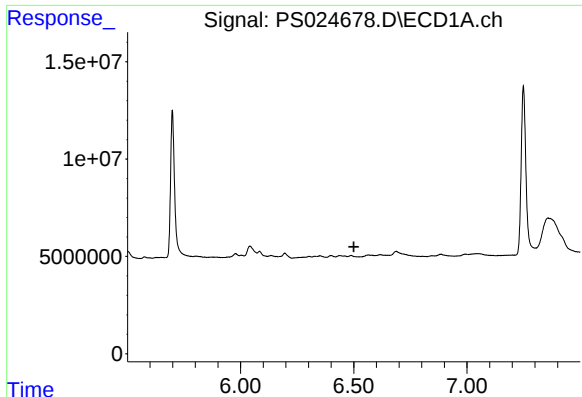

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

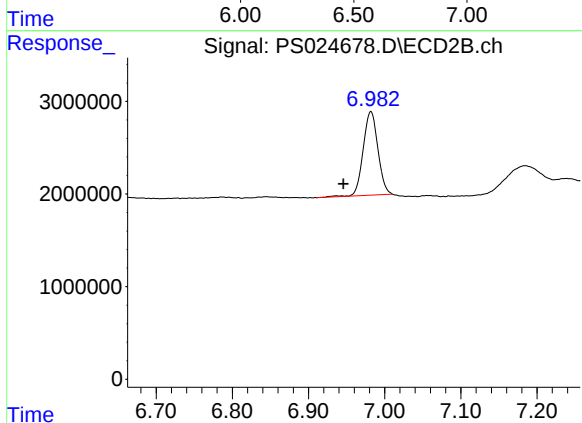


#5 DICAMBA

R.T.: 6.982 min
Delta R.T.: 0.036 min
Response: 12153286
Conc: 4.10 ng/ml

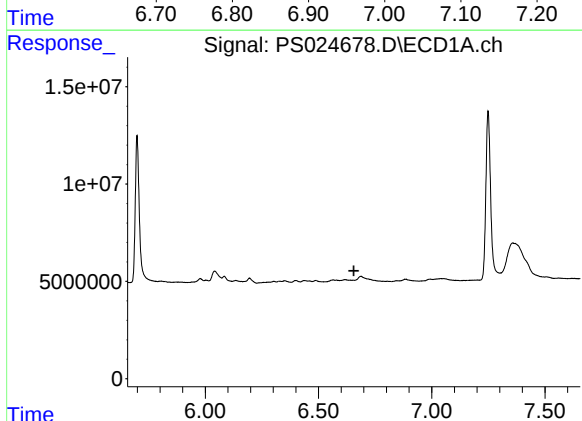


#6 MCP

R.T.: 0.000 min
Exp R.T.: 6.656 min
Response: 0
Conc: N.D.

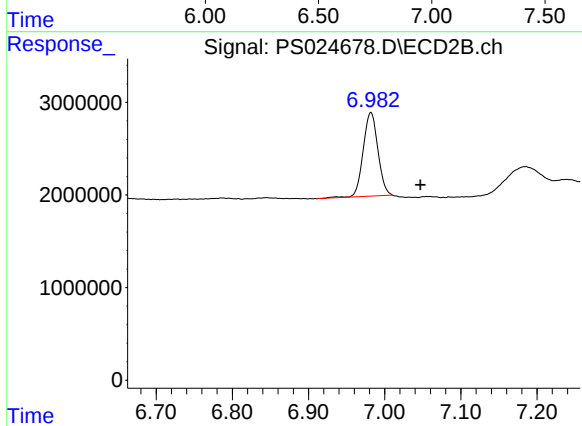

#6 MCP


R.T.: 6.982 min
Delta R.T.: -0.065 min
Response: 12153286
Conc: 6.17 ug/ml

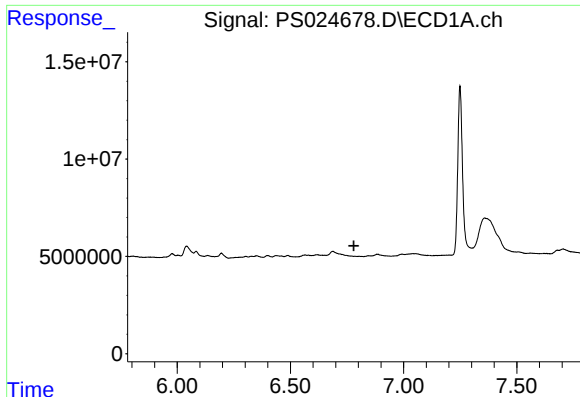

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

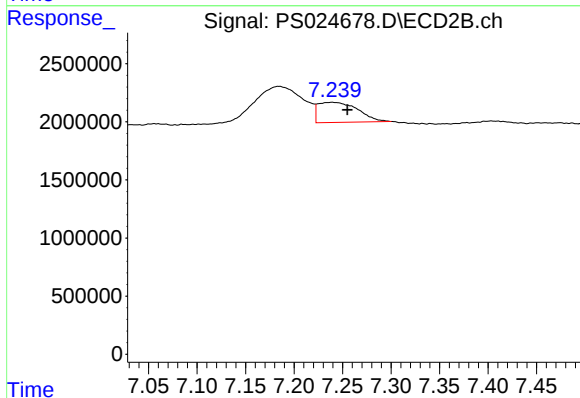


#7 MCPA

R.T.: 7.239 min
Delta R.T.: -0.016 min
Response: 4889828
Conc: 1.53 ug/ml

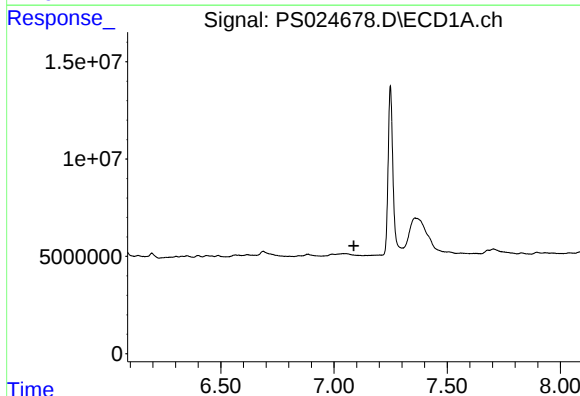


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

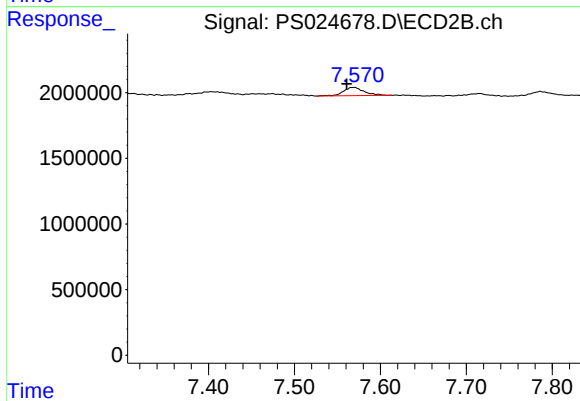

#8 DICHLORPROP


R.T.: 7.570 min
Delta R.T.: 0.009 min
Response: 1069752
Conc: 1.42 ng/ml

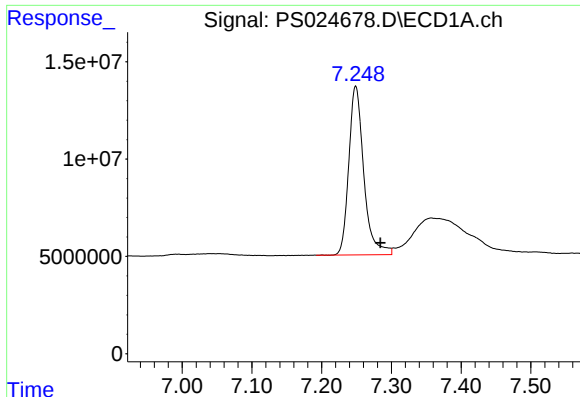

#9 2,4-D


R.T.: 7.249 min
Delta R.T.: -0.035 min
Response: 129675003
Conc: 46.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

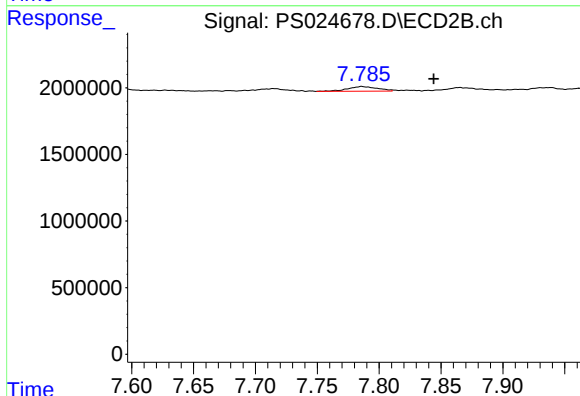


#9 2,4-D

R.T.: 7.786 min
Delta R.T.: -0.058 min
Response: 595424
Conc: N.D.

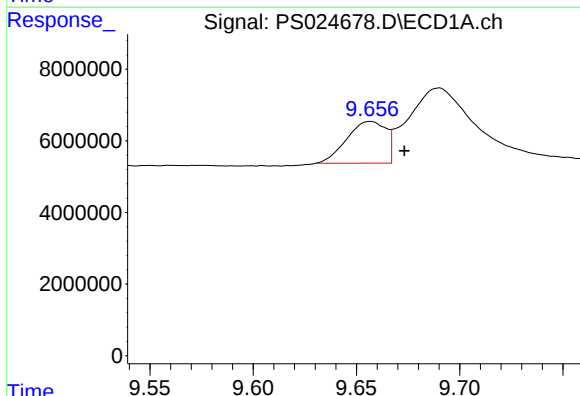


#15 Picloram

R.T.: 9.657 min
Delta R.T.: -0.016 min
Response: 15452113
Conc: N.D.

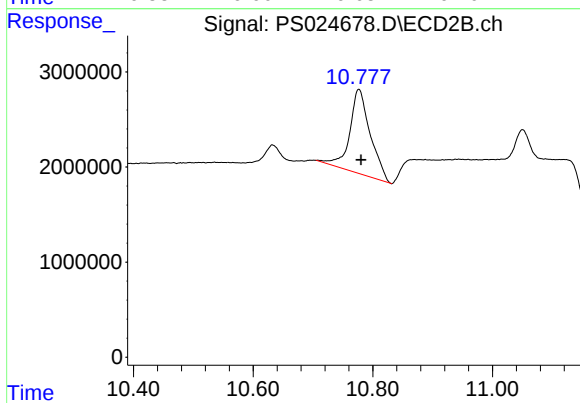

#15 Picloram


R.T.: 10.777 min
Delta R.T.: -0.003 min
Response: 21111447
Conc: 3.40 ng/ml

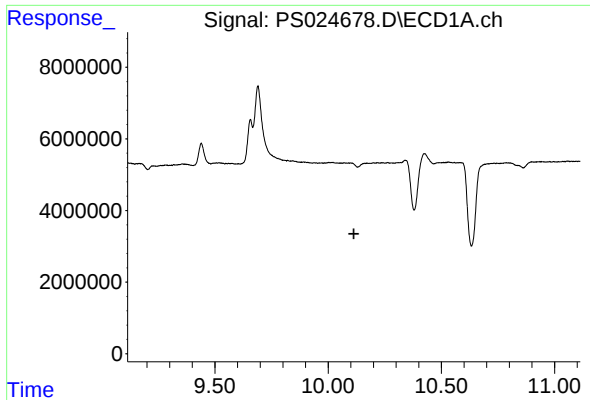

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

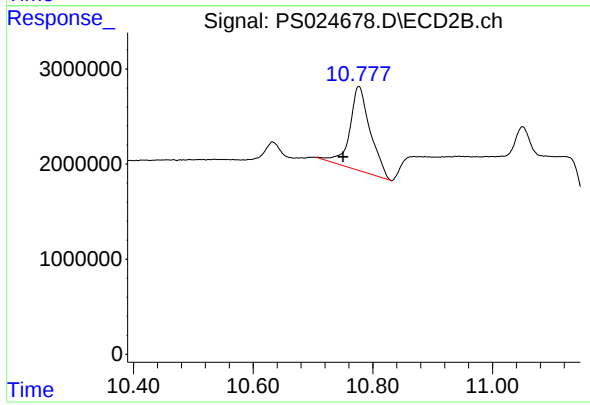

#16 DCPA

R.T.: 10.777 min
Delta R.T.: 0.027 min
Response: 21111447
Conc: 4.05 ng/ml