

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102423\
 Data File : PS024691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 14:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 14:59:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.358	6.778	930.4E6	305.3E6	452.251	441.706
Target Compounds							
1) T	Dalapon	0.000	2.568	0	1520354	N.D.	1.359
7) T	MCPA	0.000	7.241	0	9115424	N.D.	2.845
8) T	DICHLORPROP	0.000	7.569	0	2529670	N.D.	3.364
9) T	2,4-D	0.000	7.784 ^f	0	937993	N.D.	1.019
11) T	2,4,5-TP ...	0.000	8.616	0	515783	N.D.	<MDL
12) T	2,4,5-T	0.000	9.035	0	692552	N.D.	<MDL
13) T	2,4-DB	0.000	9.487	0	762189	N.D.	1.496
15) T	Picloram	0.000	10.778	0	2529776	N.D.	<MDL
16) T	DCPA	0.000	10.778	0	2529776	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102423\
Data File : PS024691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 14:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 14:59:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

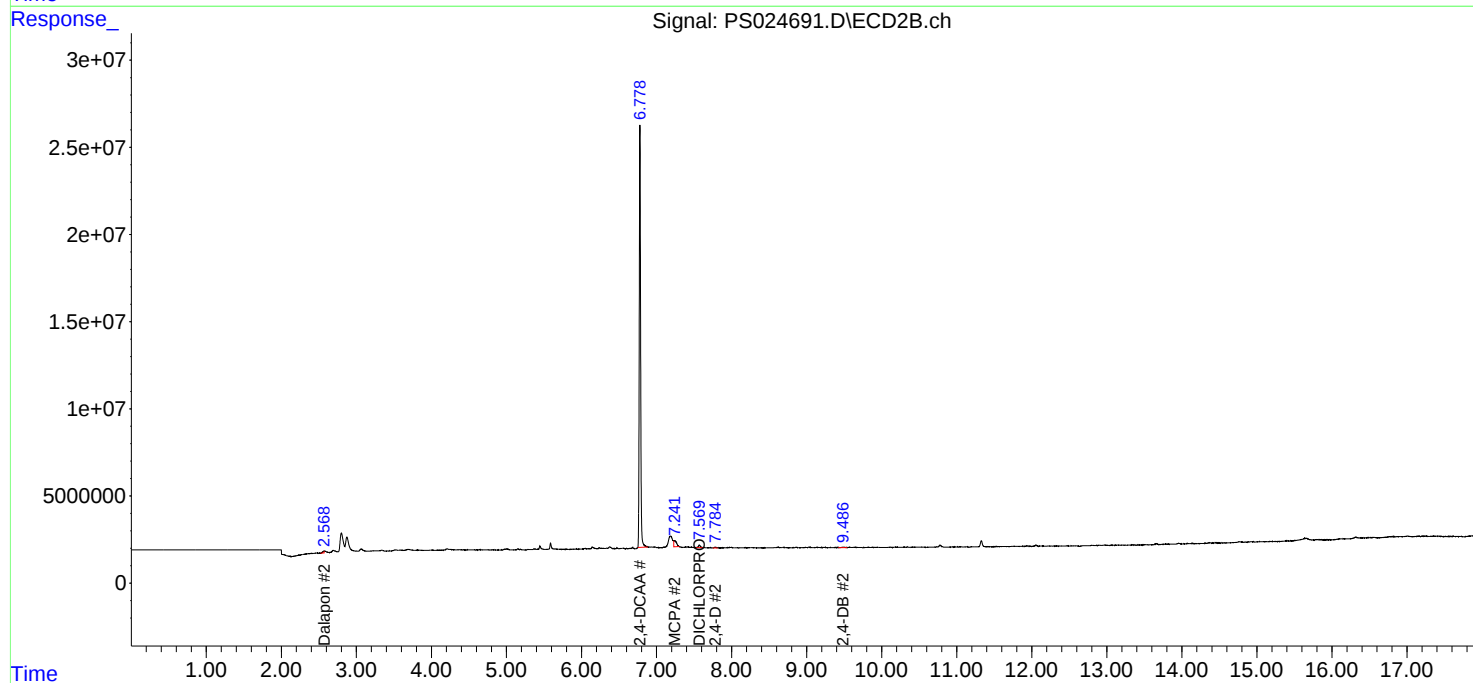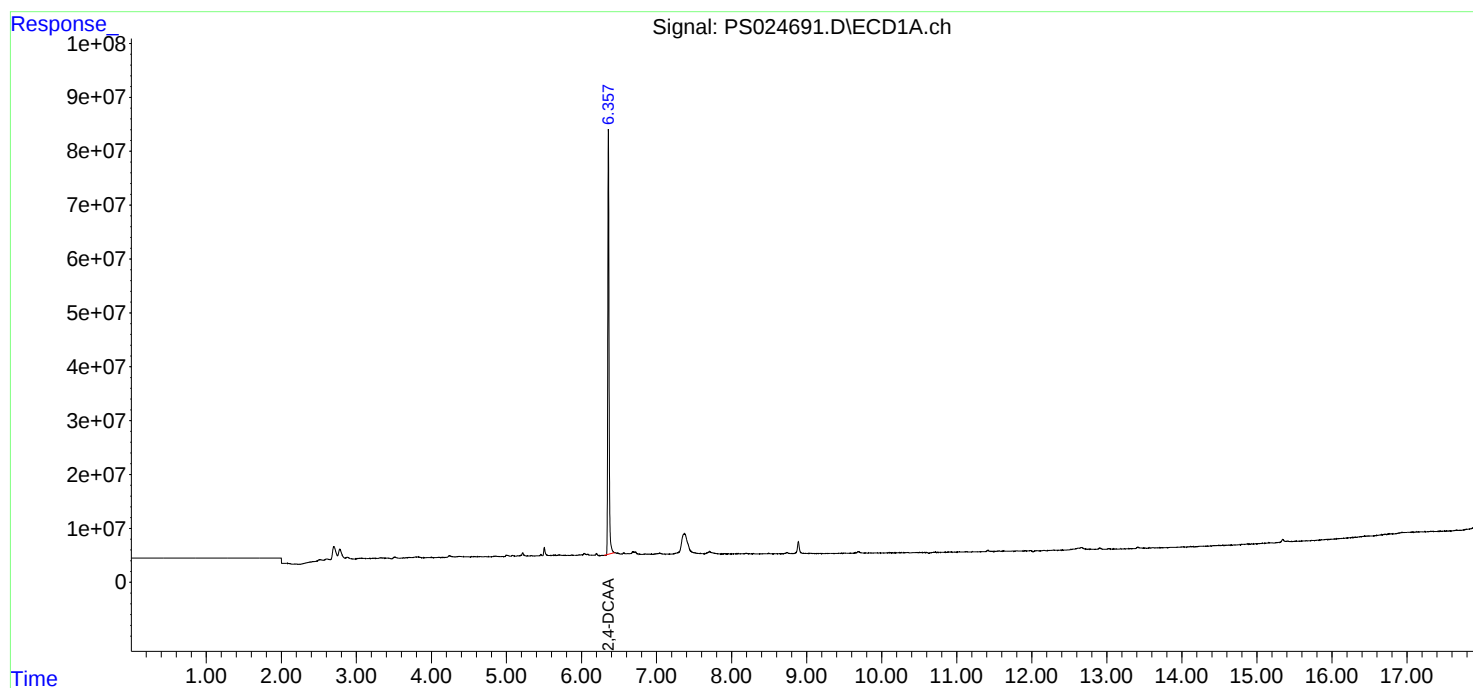


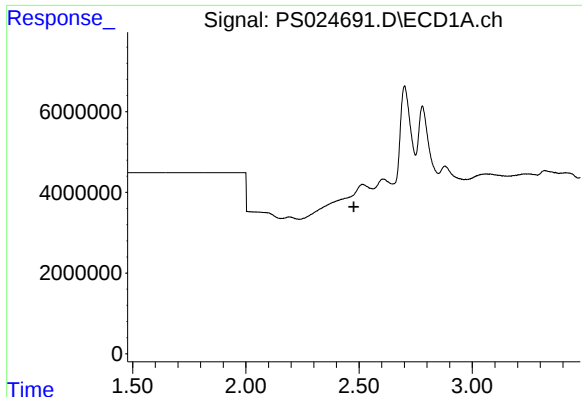

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

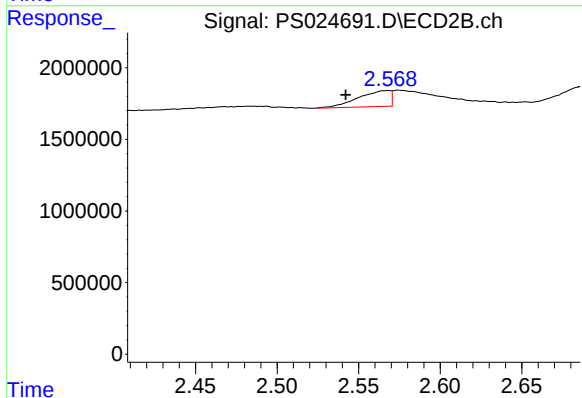


#1 Dalapon

R.T.: 2.568 min
Delta R.T.: 0.026 min
Response: 1520354
Conc: 1.36 ng/ml

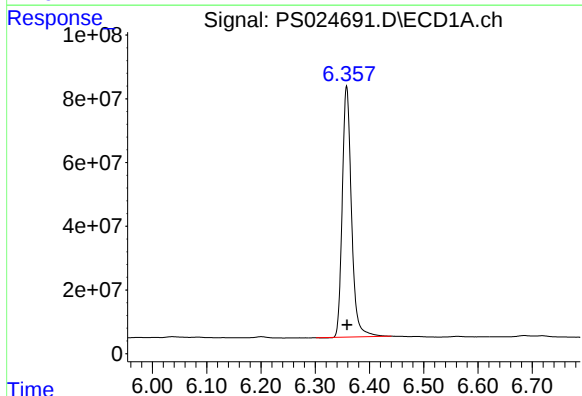


#4 2,4-DCAA

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 930429127
Conc: 452.25 ng/ml

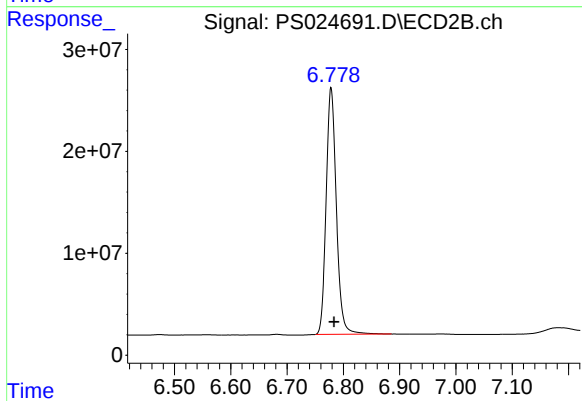

#4 2,4-DCAA


R.T.: 6.778 min
Delta R.T.: -0.005 min
Response: 305346908
Conc: 441.71 ng/ml

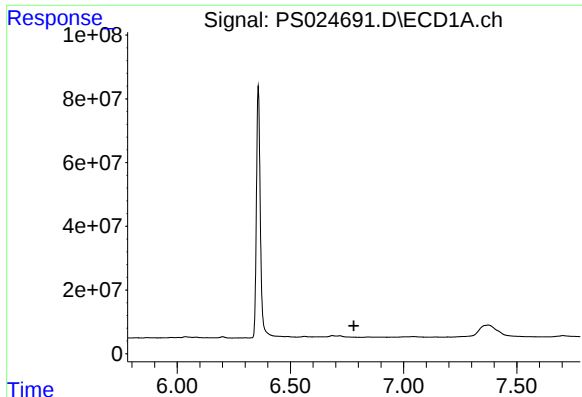

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

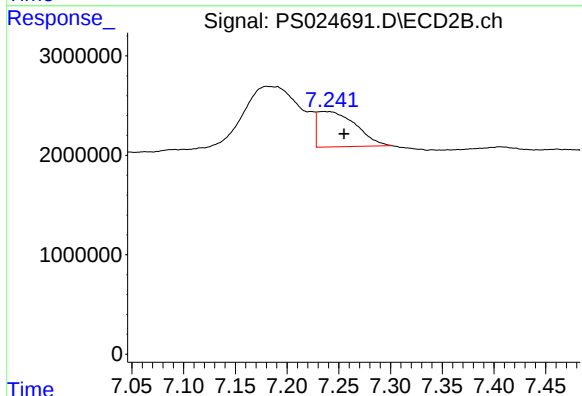


#7 MCPA

R.T.: 7.241 min
Delta R.T.: -0.014 min
Response: 9115424
Conc: 2.84 ug/ml

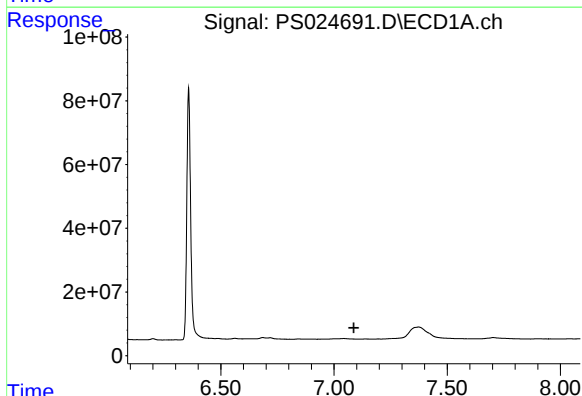


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

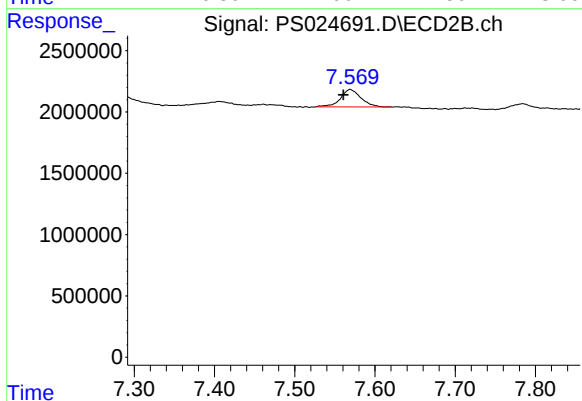

#8 DICHLORPROP


R.T.: 7.569 min
Delta R.T.: 0.008 min
Response: 2529670
Conc: 3.36 ng/ml

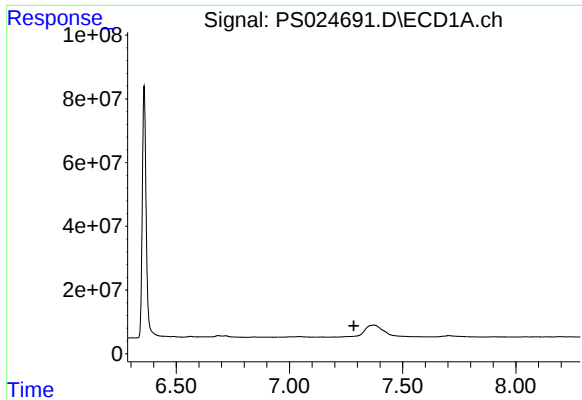

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

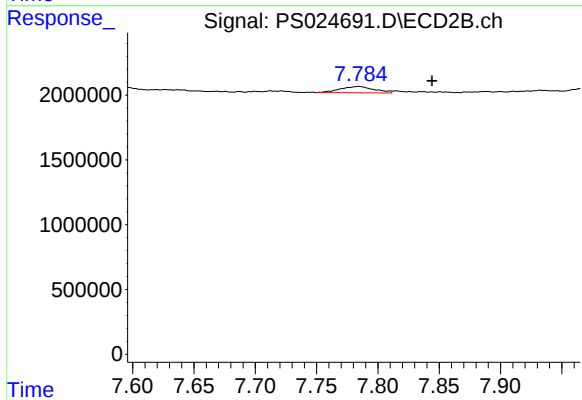


#9 2,4-D

R.T.: 7.784 min
Delta R.T.: -0.060 min
Response: 937993
Conc: 1.02 ng/ml

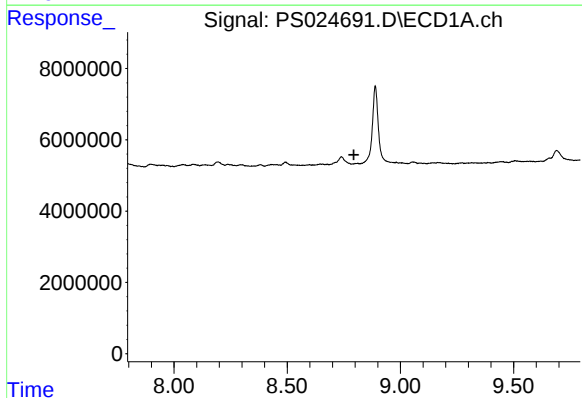

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

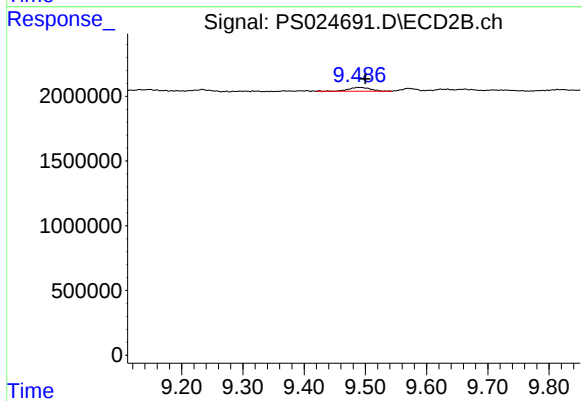

#13 2,4-DB

R.T.: 9.487 min
Delta R.T.: -0.013 min
Response: 762189
Conc: 1.50 ng/ml