

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102423\
 Data File : PS024702.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 19:02
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 01:05:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.358	6.778	930.5E6	305.1E6	452.286	441.350
Target Compounds							
1) T	Dalapon	0.000	2.569	0	3463938	N.D.	3.095
5) T	DICAMBA	0.000	6.977	0	1162833	N.D.	<MDL
6) T	MCPD	0.000	6.977f	0	1162833	N.D.	<MDL
7) T	MCPA	0.000	7.248	0	5699354	N.D.	1.779
8) T	DICHLORPROP	0.000	7.568	0	2474461	N.D.	3.290
9) T	2,4-D	0.000	7.784f	0	643773	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.619	0	439197	N.D.	<MDL
12) T	2,4,5-T	0.000	9.033	0	610693	N.D.	<MDL
13) T	2,4-DB	0.000	9.492	0	738623	N.D.	1.449
15) T	Picloram	0.000	10.778	0	2103649	N.D.	<MDL
16) T	DCPA	0.000	10.778	0	2103649	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102423\
Data File : PS024702.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 19:02
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 01:05:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

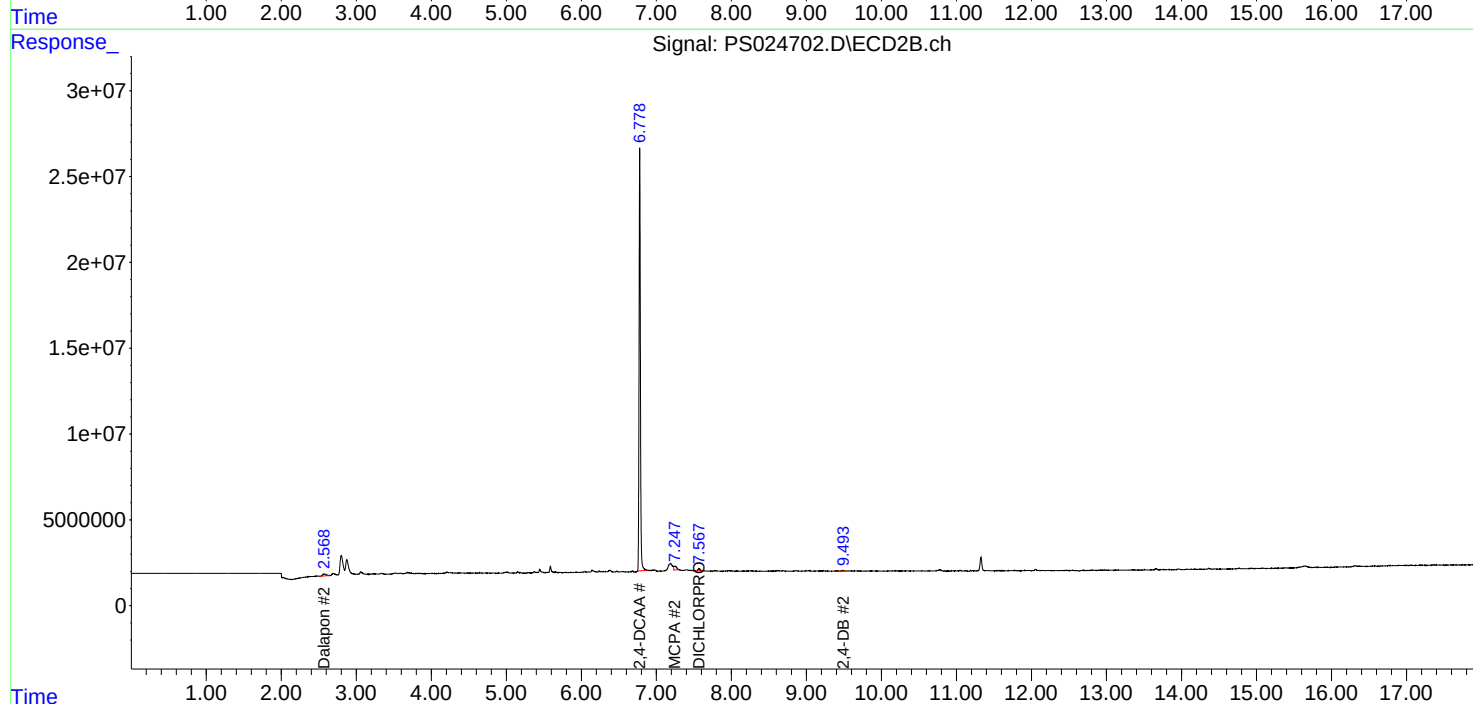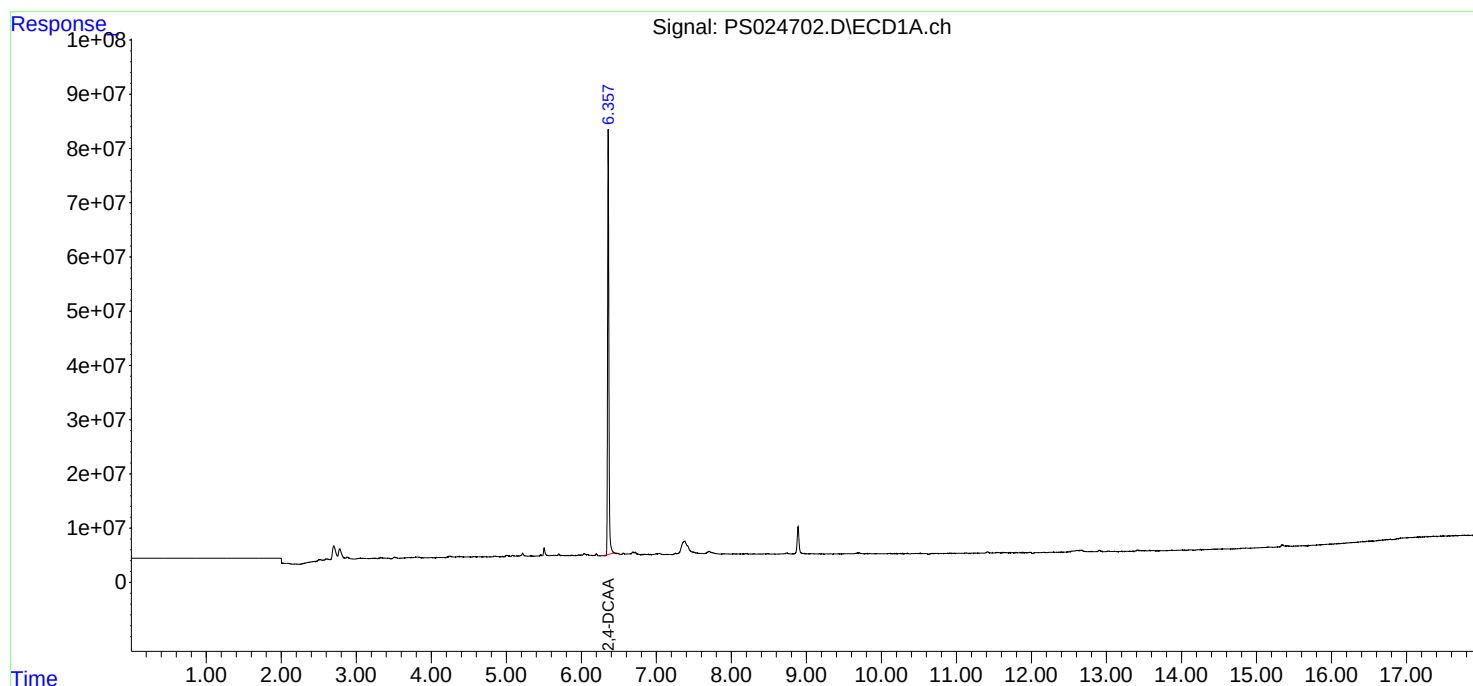


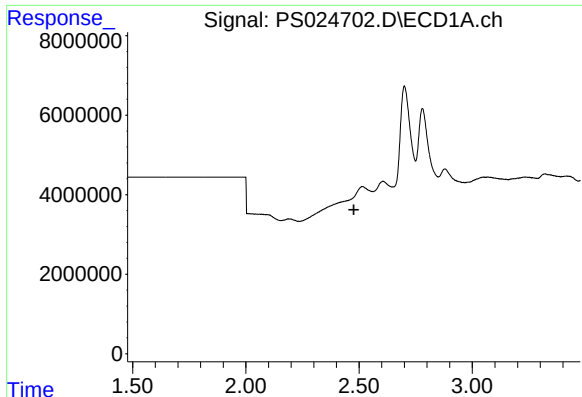

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

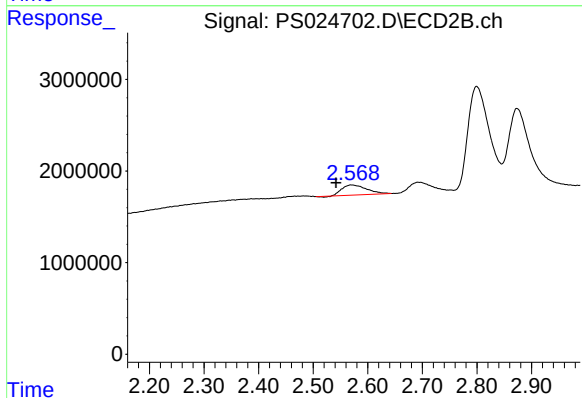


#1 Dalapon

R.T.: 2.569 min
Delta R.T.: 0.027 min
Response: 3463938
Conc: 3.10 ng/ml

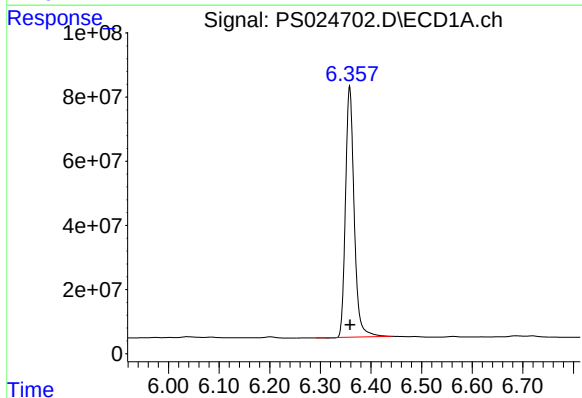


#4 2,4-DCAA

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 930501088
Conc: 452.29 ng/ml

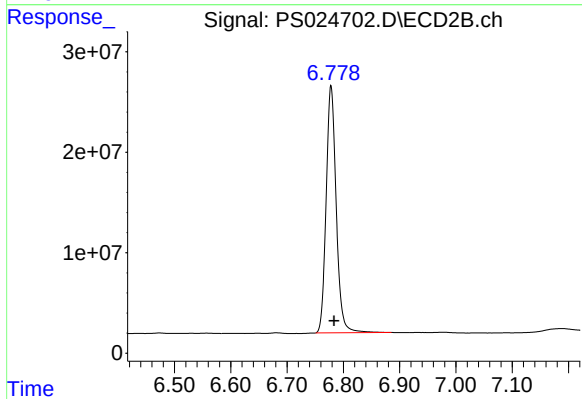

#4 2,4-DCAA


R.T.: 6.778 min
Delta R.T.: -0.005 min
Response: 305100935
Conc: 441.35 ng/ml

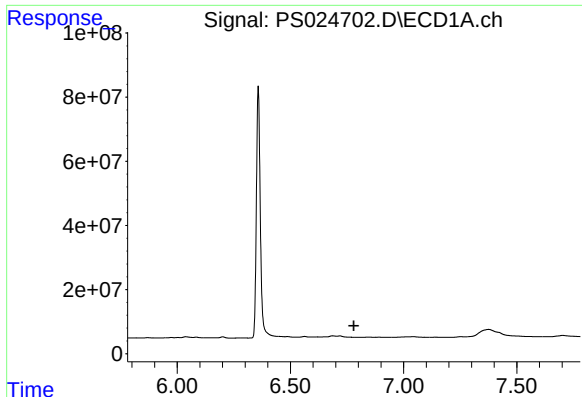

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

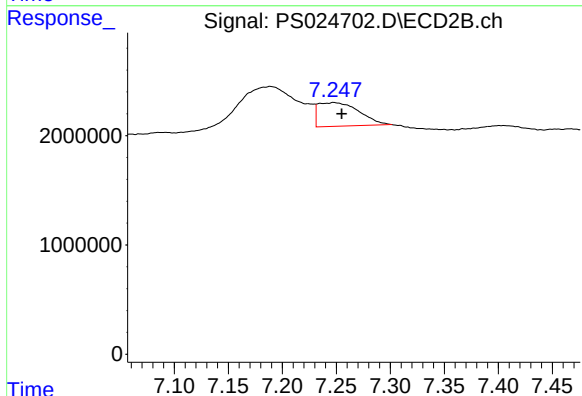


#7 MCPA

R.T.: 7.248 min
Delta R.T.: -0.007 min
Response: 5699354
Conc: 1.78 ug/ml

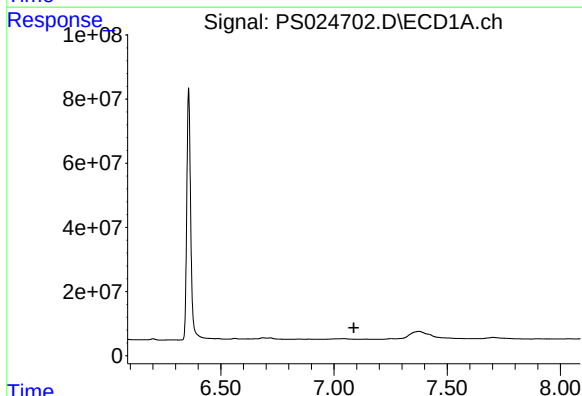


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

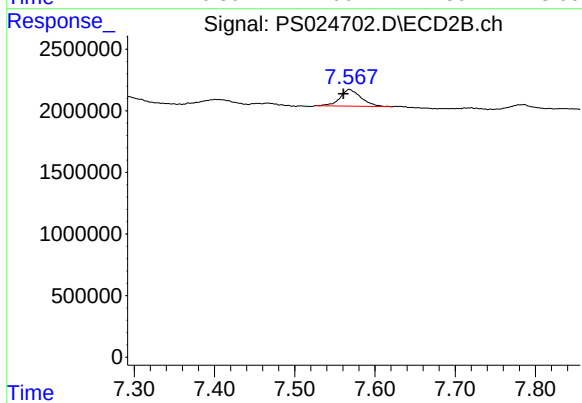

#8 DICHLORPROP


R.T.: 7.568 min
Delta R.T.: 0.008 min
Response: 2474461
Conc: 3.29 ng/ml

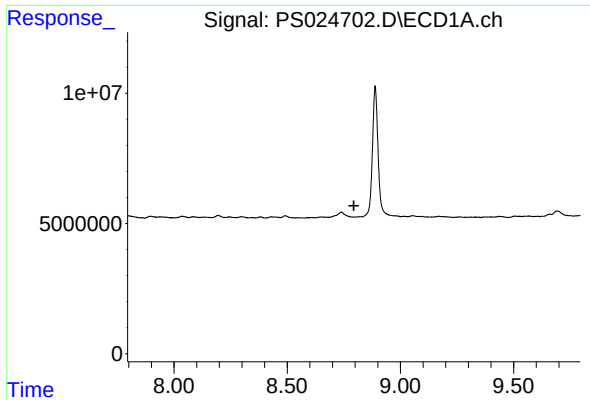

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

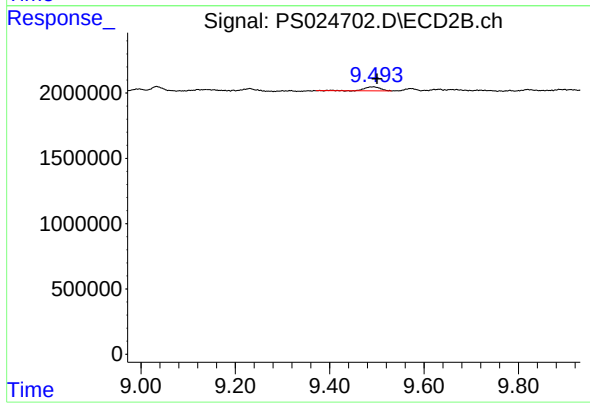

#13 2,4-DB

R.T.: 9.492 min
Delta R.T.: -0.008 min
Response: 738623
Conc: 1.45 ng/ml