

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102424\
 Data File : PS028030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 09:02
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:36:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 23 13:25:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.103	0.000	1839418	0	<MDL	N.D.	#
Target Compounds								
1) T	Dalapon	2.539	0.000	15003269	0	3.293	N.D.	#
3) T	4-Nitroph...	6.878	0.000	6896212	0	3.727	N.D.	#
7) T	MCPA	7.633f	0.000	1896745	0	<MDL	N.D.	#
8) T	DICHLORPROP	7.965	0.000	1398763	0	<MDL	N.D.	#
9) T	2,4-D	8.186	0.000	16707712	0	4.931	N.D.	#
10) T	Pentachlo...	8.467	0.000	2913586	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.035	0.000	5904139	0	<MDL	N.D.	#
12) T	2,4,5-T	9.322	0.000	9424985	0	<MDL	N.D.	#
13) T	2,4-DB	9.881	0.000	2097427	0	<MDL	N.D.	#
14) T	DINOSEB	11.056	0.000	3382172	0	<MDL	N.D.	#
15) T	Picloram	10.874	12.149	95027861	6404172	4.268	1.405	#
16) T	DCPA	11.350	12.149f	3499647	6404172	<MDL	1.380	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102424\
Data File : PS028030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 09:02
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:36:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
Quant Title : 8080.M
QLast Update : Wed Oct 23 13:25:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

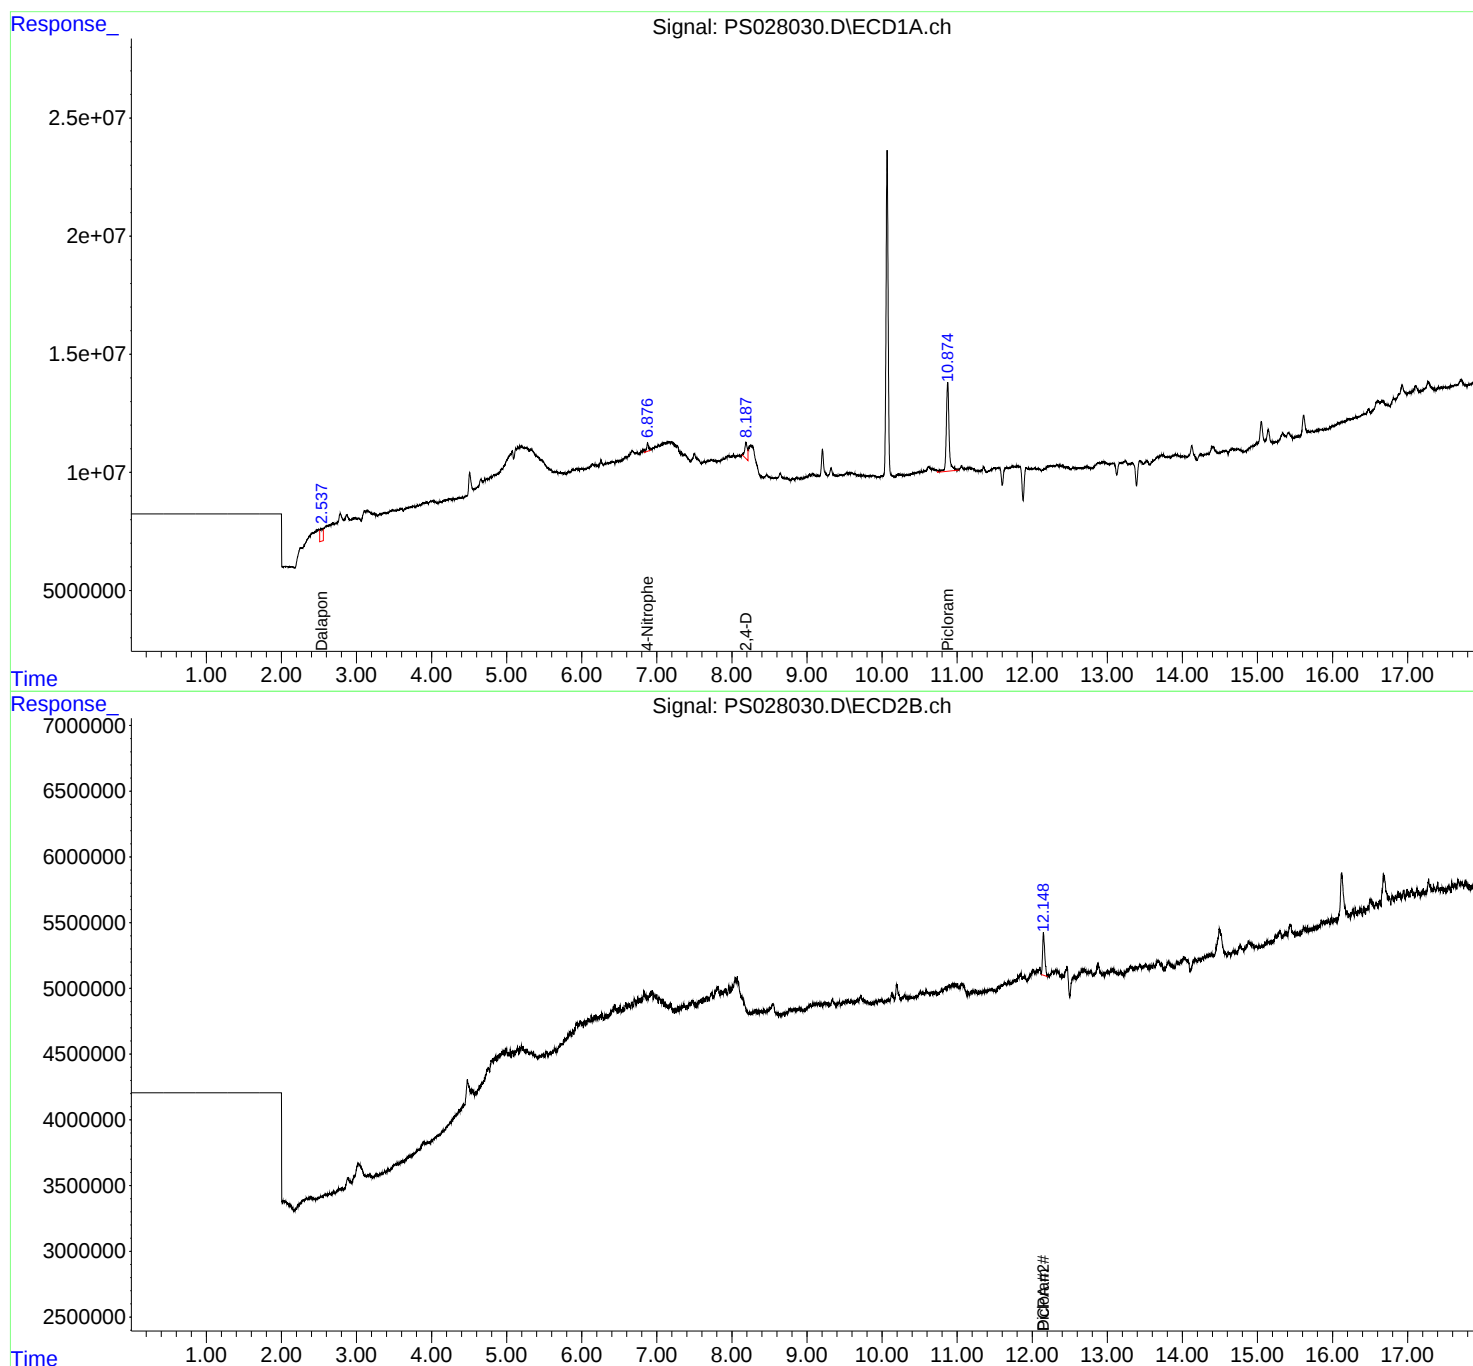


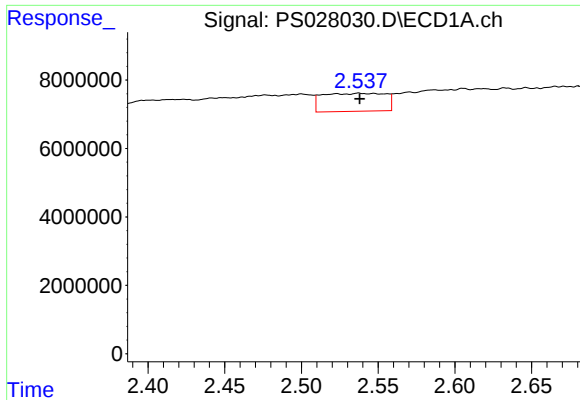

#1 Dalapon


R.T.: 2.539 min
Delta R.T.: 0.000 min
Response: 15003269
Conc: 3.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

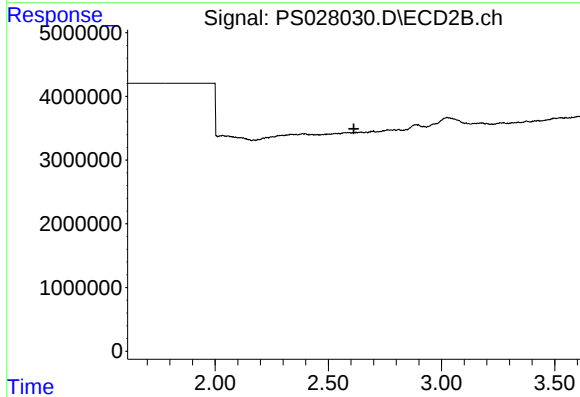


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.613 min
Response: 0
Conc: N.D.

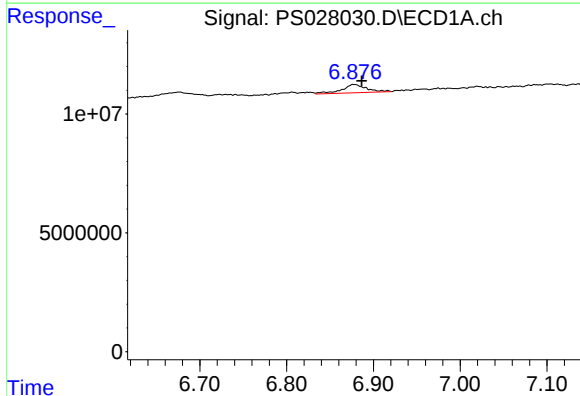


#3 4-Nitrophenol

R.T.: 6.878 min
Delta R.T.: -0.009 min
Response: 6896212
Conc: 3.73 ng/ml

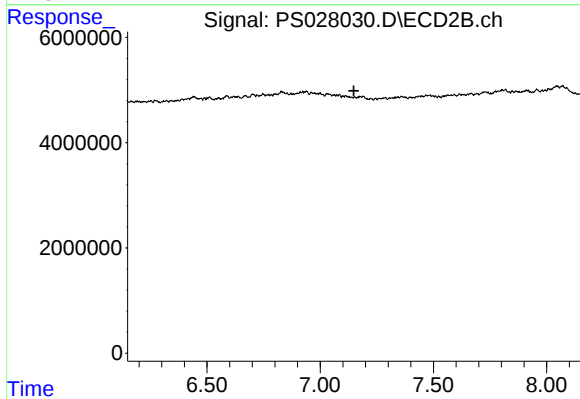

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

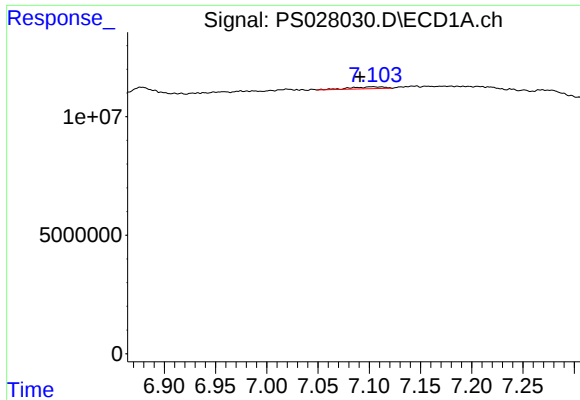

#4 2,4-DCAA


R.T.: 7.103 min
Delta R.T.: 0.012 min
Response: 1839418
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

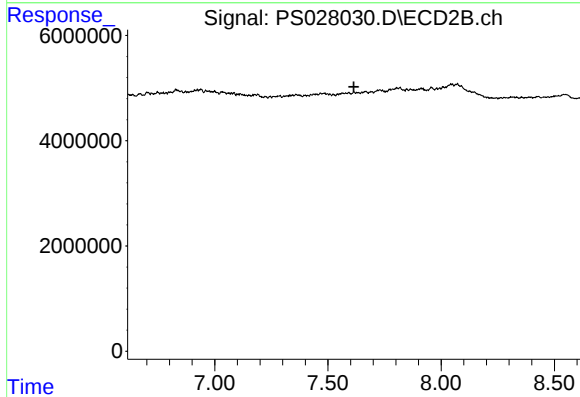


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.614 min
Response: 0
Conc: N.D.

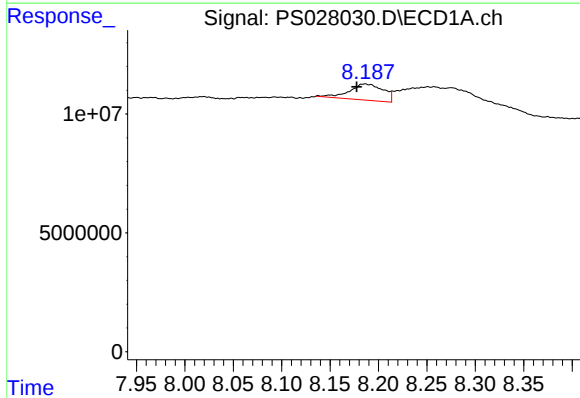


#9 2,4-D

R.T.: 8.186 min
Delta R.T.: 0.009 min
Response: 16707712
Conc: 4.93 ng/ml

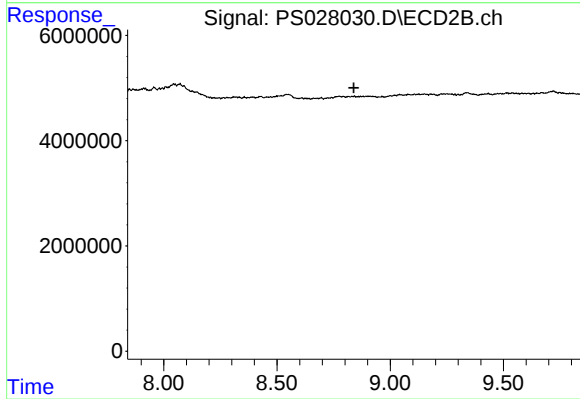

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.840 min
Response: 0
Conc: N.D.

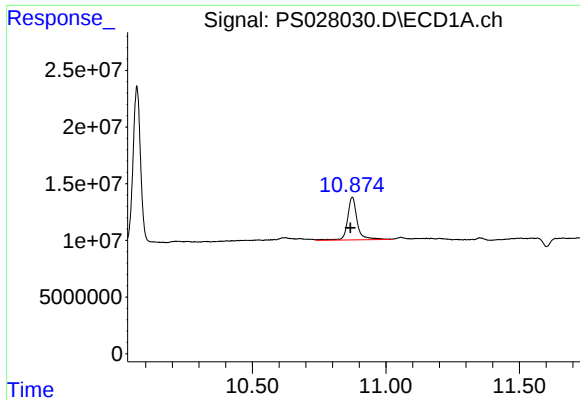

#15 Picloram


R.T.: 10.874 min
Delta R.T.: 0.007 min
Response: 95027861
Conc: 4.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

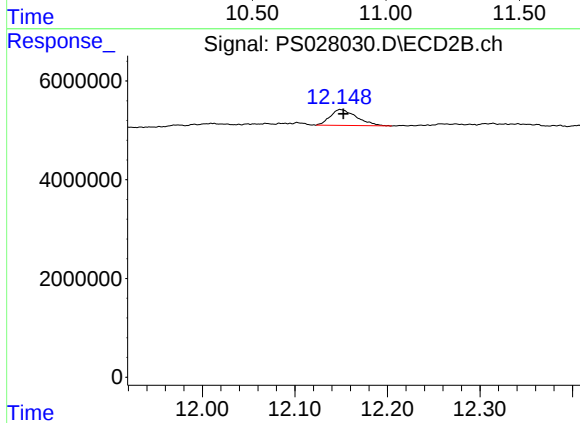


#15 Picloram

R.T.: 12.149 min
Delta R.T.: -0.003 min
Response: 6404172
Conc: 1.41 ng/ml

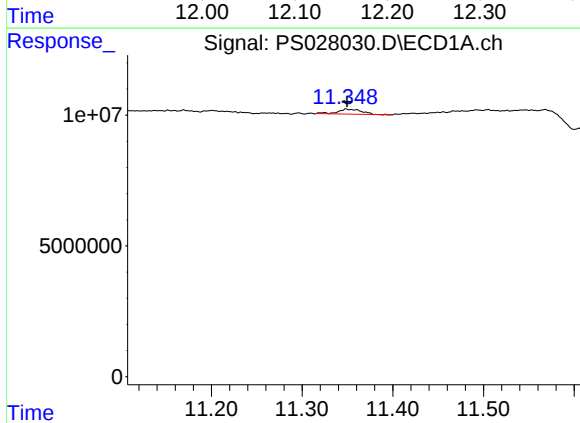

#16 DCPA

R.T.: 11.350 min
Delta R.T.: 0.000 min
Response: 3499647
Conc: N.D.

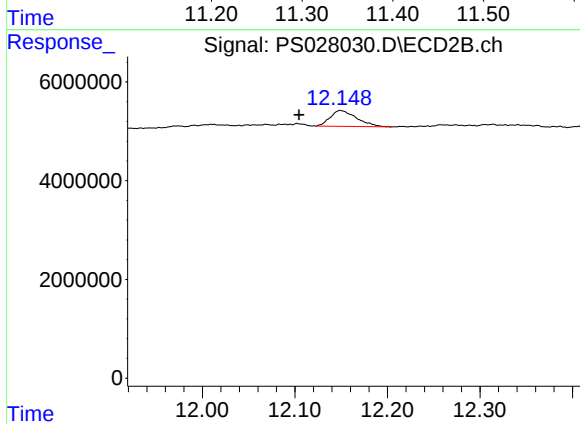

#16 DCPA

R.T.: 12.149 min
Delta R.T.: 0.045 min
Response: 6404172
Conc: 1.38 ng/ml