

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102424\
 Data File : PS028031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 09:26
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:37:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 23 13:25:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.092	7.613	1368.0E6	496.6E6	507.224	523.493
Target Compounds							
1) T	Dalapon	2.527	0.000	4181612	0	<MDL	N.D. #
3) T	4-Nitroph...	6.882	0.000	16482023	0	8.907	N.D. #
7) T	MCPA	7.628f	0.000	858551	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	8.557f	0	2511438	N.D.	2.680
10) T	Pentachlo...	8.469	0.000	1795527	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.015	0.000	1778854	0	<MDL	N.D. #
12) T	2,4,5-T	9.320	0.000	4427762	0	<MDL	N.D. #
13) T	2,4-DB	9.879	0.000	2284342	0	<MDL	N.D. #
14) T	DINOSEB	11.056	0.000	3468159	0	<MDL	N.D. #
15) T	Picloram	10.873	12.163	65195416	4482526	2.928	<MDL #
16) T	DCPA	11.350	0.000	3252375	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102424\
Data File : PS028031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 09:26
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:37:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
Quant Title : 8080.M
QLast Update : Wed Oct 23 13:25:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

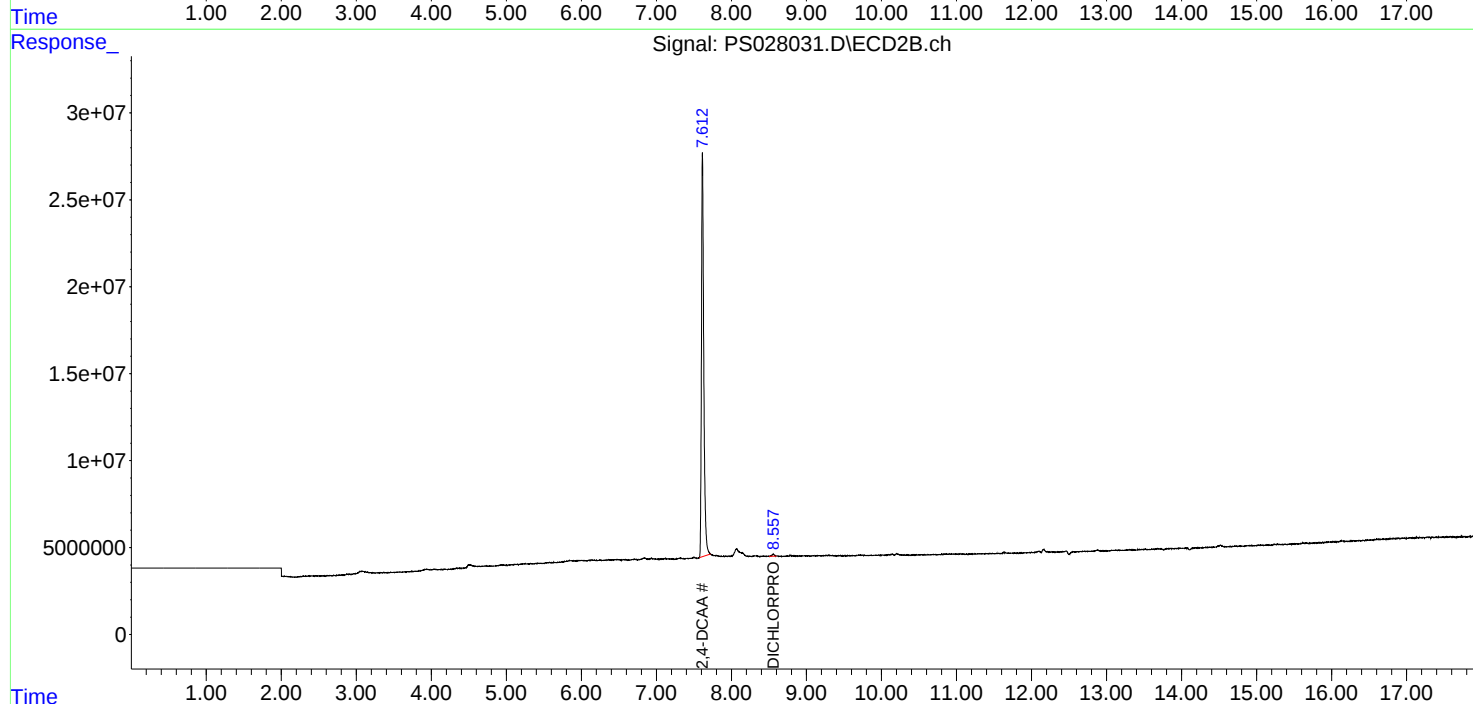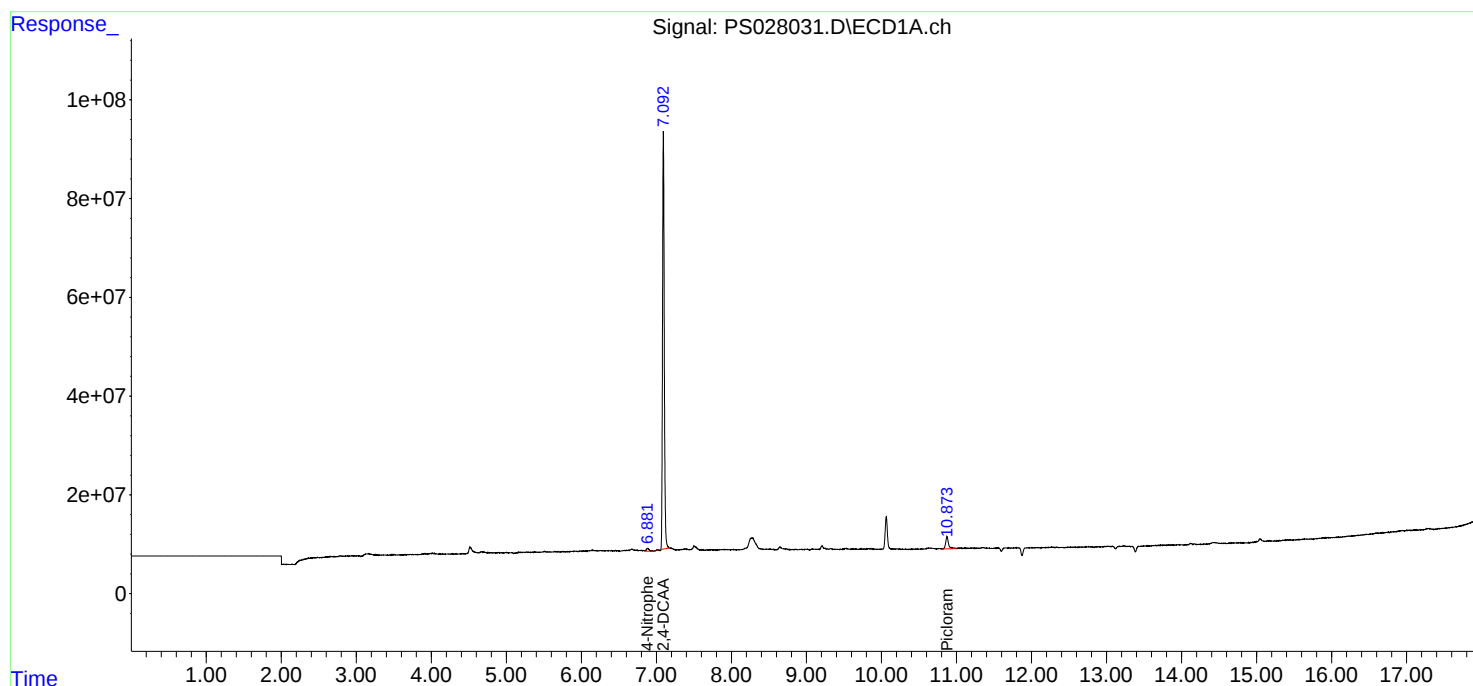


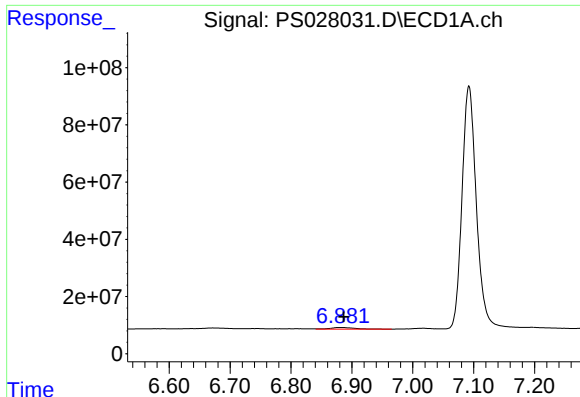

#3 4-Nitrophenol


R.T.: 6.882 min
Delta R.T.: -0.004 min
Response: 16482023
Conc: 8.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

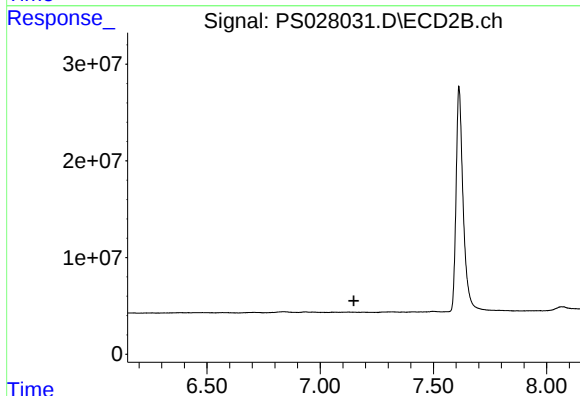


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

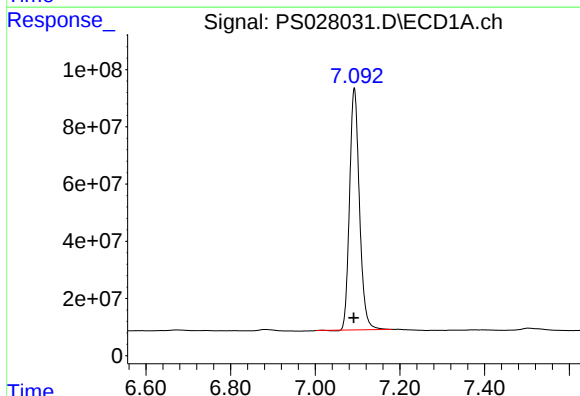


#4 2,4-DCAA

R.T.: 7.092 min
Delta R.T.: 0.001 min
Response: 1367964816
Conc: 507.22 ng/ml

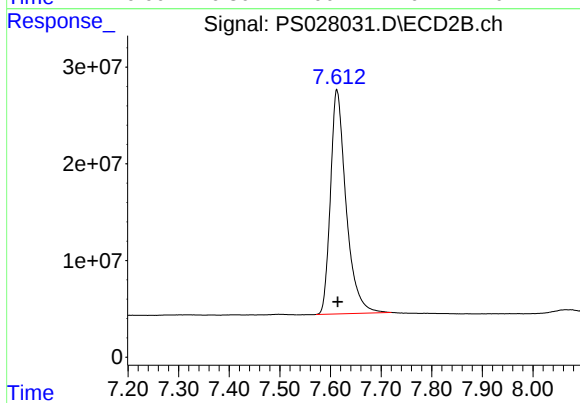

#4 2,4-DCAA


R.T.: 7.613 min
Delta R.T.: -0.002 min
Response: 496626255
Conc: 523.49 ng/ml

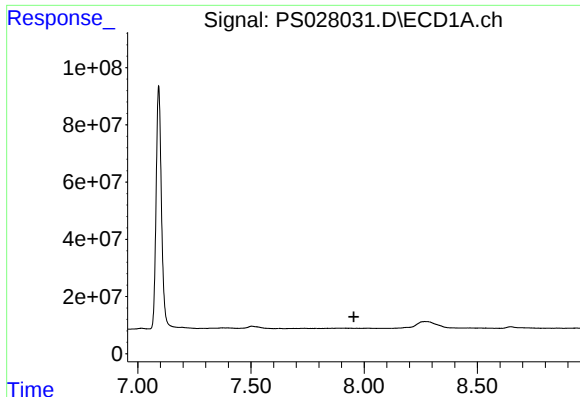

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.955 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

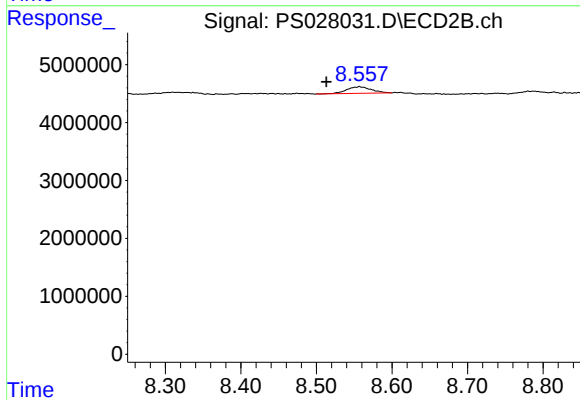


#8 DICHLORPROP

R.T.: 8.557 min
Delta R.T.: 0.044 min
Response: 2511438
Conc: 2.68 ng/ml

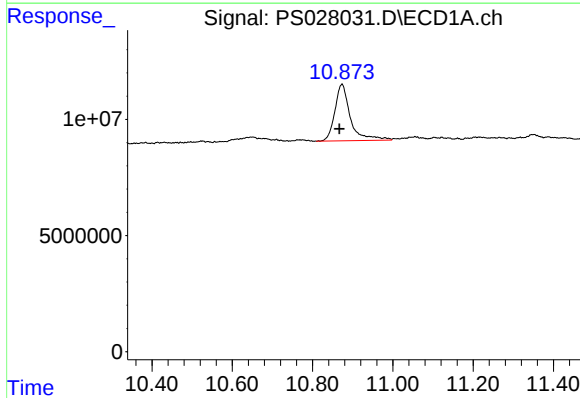

#15 Picloram

R.T.: 10.873 min
Delta R.T.: 0.006 min
Response: 65195416
Conc: 2.93 ng/ml

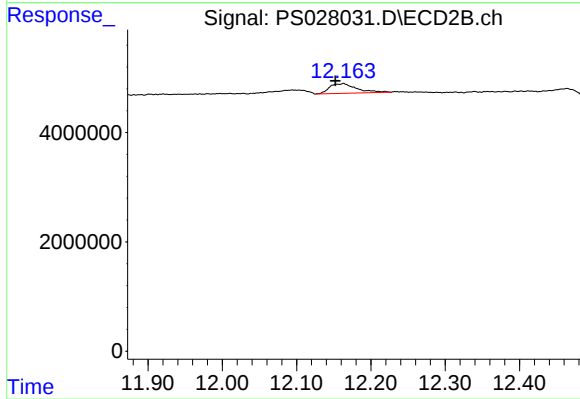

#15 Picloram

R.T.: 12.163 min
Delta R.T.: 0.011 min
Response: 4482526
Conc: N.D.