

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102424\
 Data File : PS028044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 19:56
 Operator : AR\AJ
 Sample : P4460-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WB-303-BOT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:48:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 23 13:25:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.091	7.612	389.3E6	125.0E6	144.360	131.730
Target Compounds							
1) T	Dalapon	2.511f	2.586f	69438034	140.1E6	15.240	82.144 #
2) T	3,5-DICHL...	0.000	6.607	0	4379739	N.D.	3.275
3) T	4-Nitroph...	6.872	7.191f	37570724	9191259	20.304	13.296 #
7) T	MCPA	0.000	8.148	0	6545690	N.D.	1.422
8) T	DICHLORPROP	7.972	8.551f	-2384643	25292940	N.D.	26.995
9) T	2,4-D	8.182	0.000	18197001	0	5.370	N.D. #
10) T	Pentachlo...	8.461	9.343	36467864	2672348	<MDL	<MDL #
11) T	2,4,5-TP ...	8.990f	0.000	30905268	0	1.914	N.D. #
12) T	2,4,5-T	9.312	0.000	36793586	0	2.202	N.D. #
13) T	2,4-DB	9.846f	0.000	91787048	0	34.861	N.D. #
14) T	DINOSEB	11.034	11.093	9254993	2916461	<MDL	<MDL #
15) T	Picloram	10.866	12.153	38928690	5662696	1.748	1.243 #
16) T	DCPA	11.344	12.097	43785750	13697888	2.368	2.951



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102424\
Data File : PS028044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 19:56
Operator : AR\AJ
Sample : P4460-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
WB-303-BOT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:48:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
Quant Title : 8080.M
QLast Update : Wed Oct 23 13:25:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

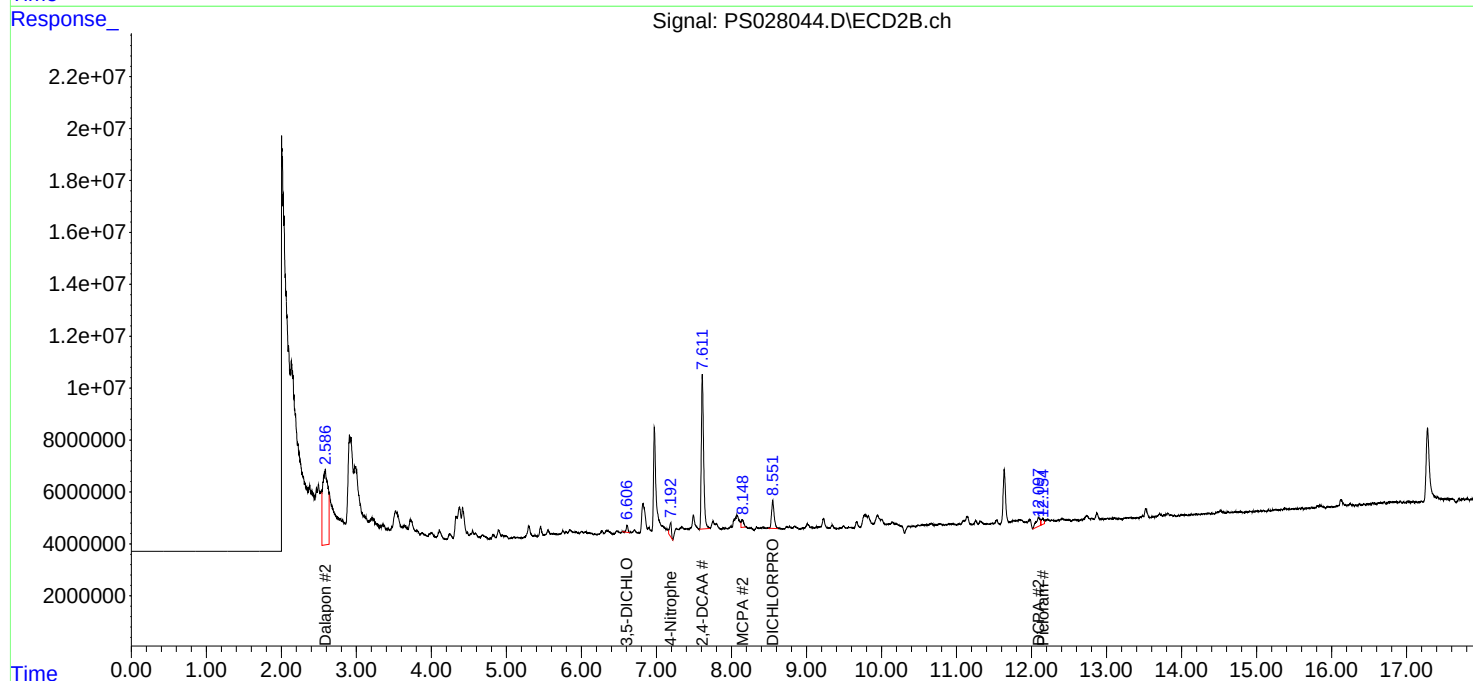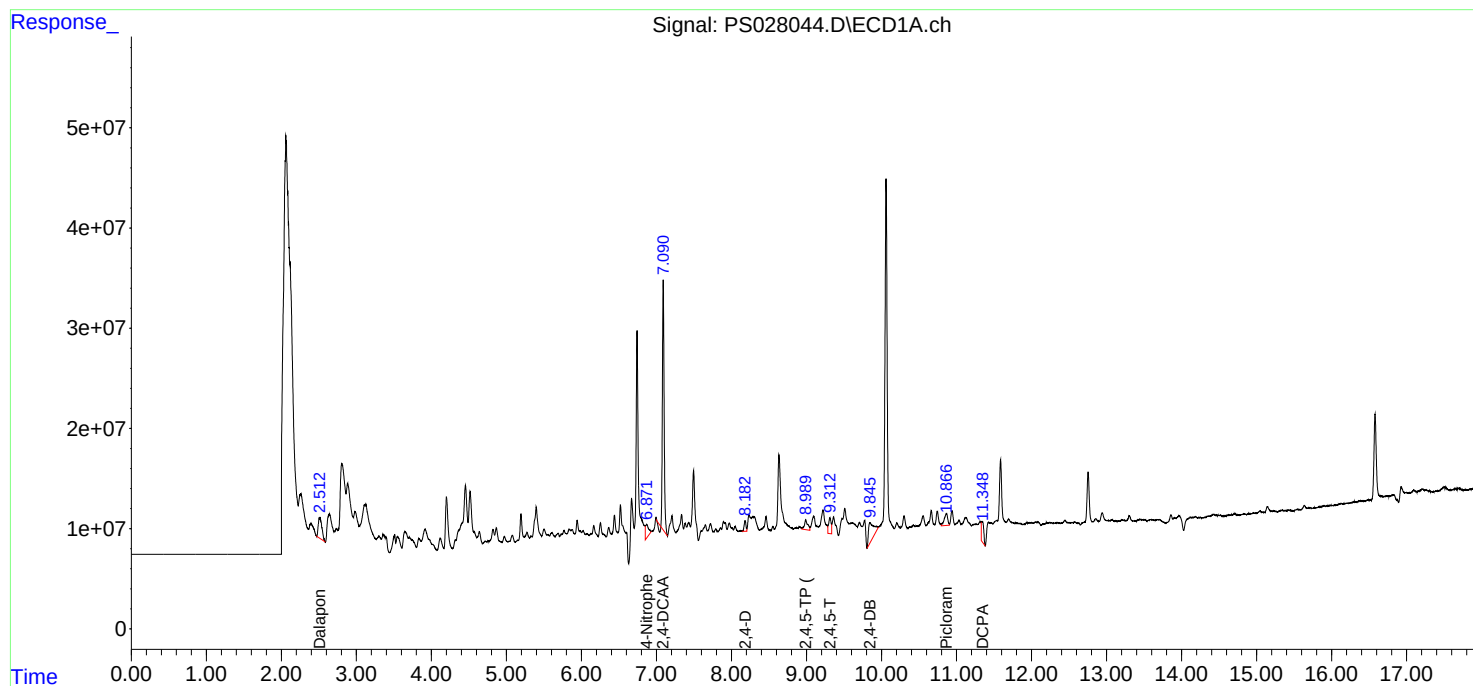


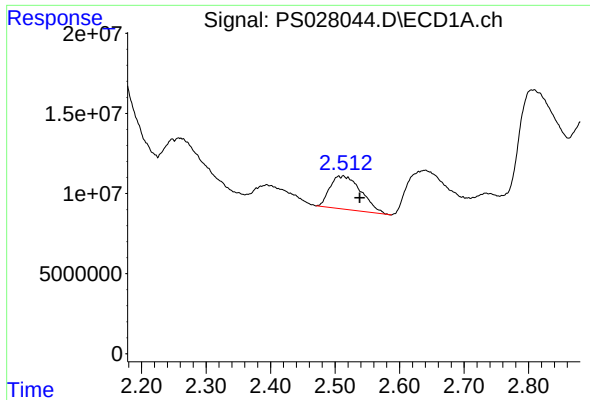

#1 Dalapon


R.T.: 2.511 min
Delta R.T.: -0.027 min
Response: 69438034
Conc: 15.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
WB-303-BOT

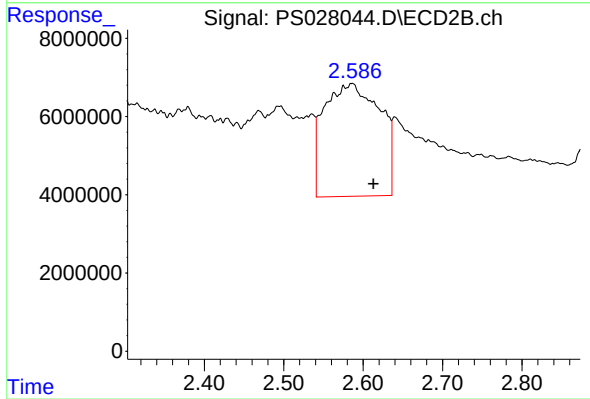


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.026 min
Response: 140089353
Conc: 82.14 ng/ml

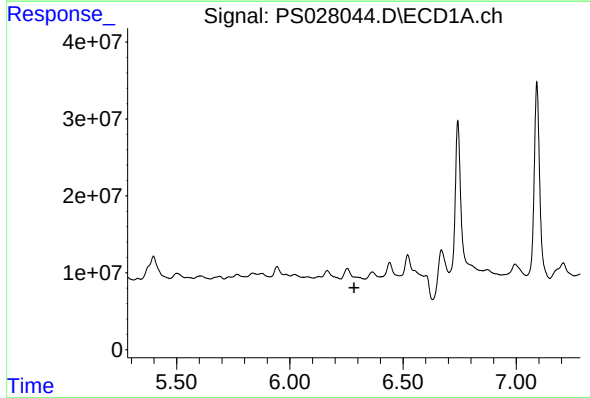


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.283 min
Response: 0
Conc: N.D.

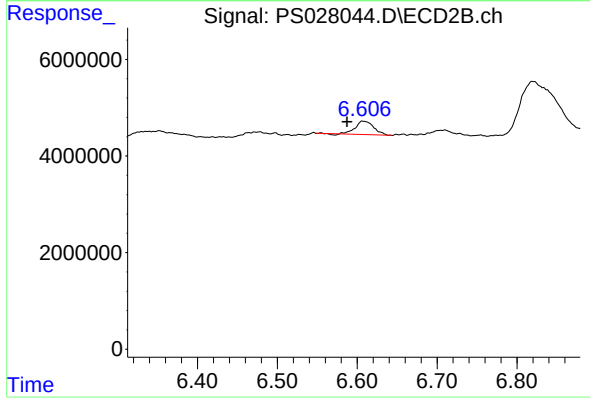

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.607 min
Delta R.T.: 0.020 min
Response: 4379739
Conc: 3.27 ng/ml

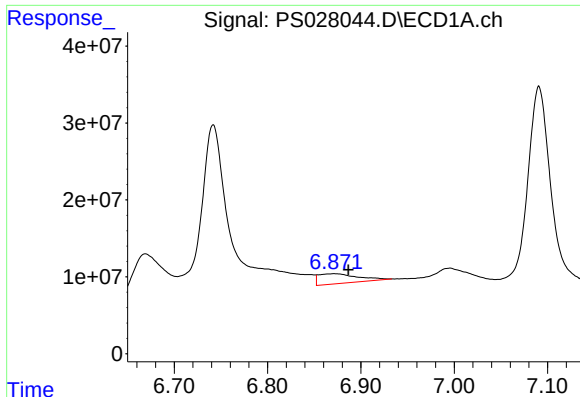

#3 4-Nitrophenol


R.T.: 6.872 min
Delta R.T.: -0.015 min
Response: 37570724
Conc: 20.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
WB-303-BOT

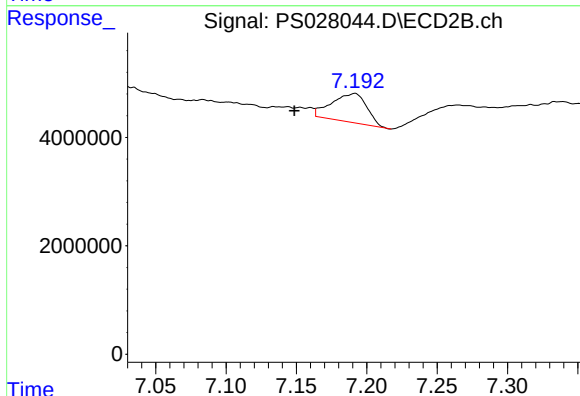


#3 4-Nitrophenol

R.T.: 7.191 min
Delta R.T.: 0.043 min
Response: 9191259
Conc: 13.30 ng/ml

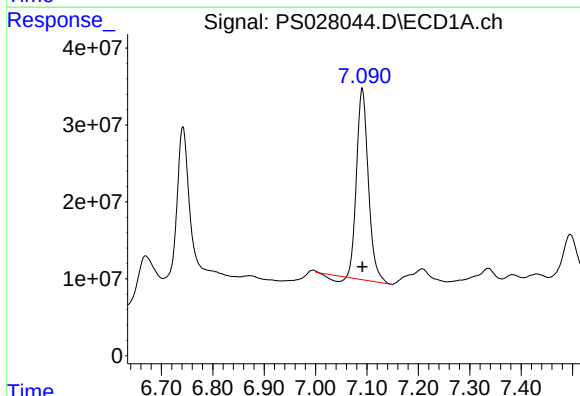


#4 2,4-DCAA

R.T.: 7.091 min
Delta R.T.: 0.000 min
Response: 389333458
Conc: 144.36 ng/ml

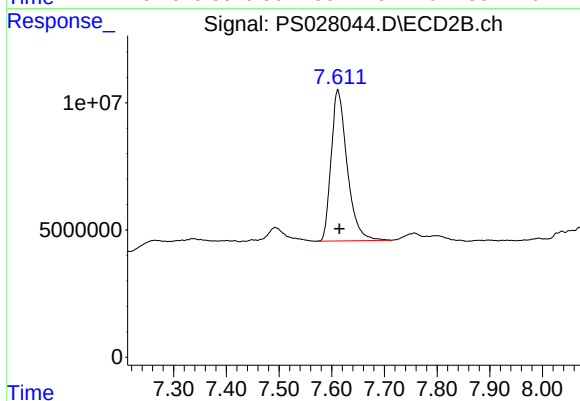

#4 2,4-DCAA


R.T.: 7.612 min
Delta R.T.: -0.003 min
Response: 124969409
Conc: 131.73 ng/ml

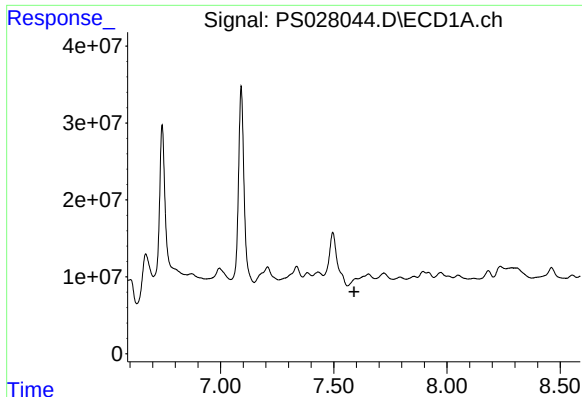

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.589 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WB-303-BOT

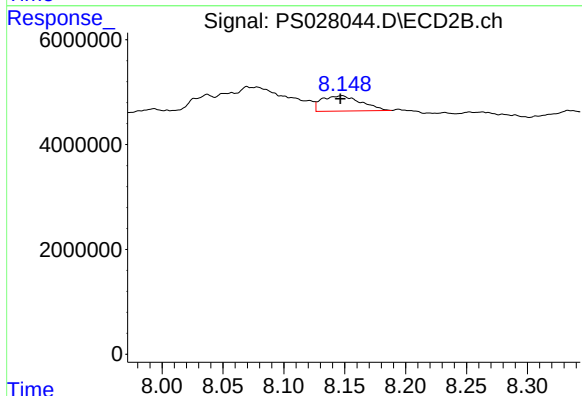


#7 MCPA

R.T.: 8.148 min
Delta R.T.: 0.001 min
Response: 6545690
Conc: 1.42 ug/ml

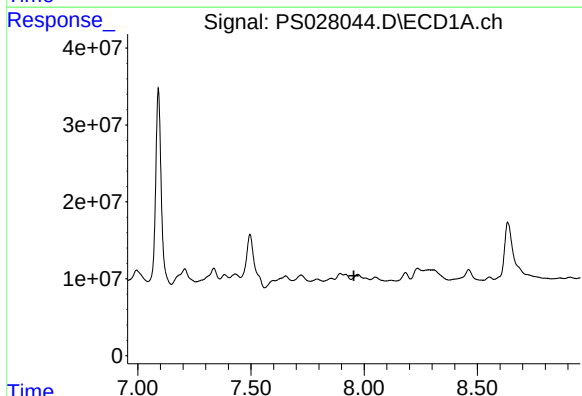


#8 DICHLORPROP

R.T.: 7.972 min
Delta R.T.: 0.017 min
Response: -2384643
Conc: N.D.

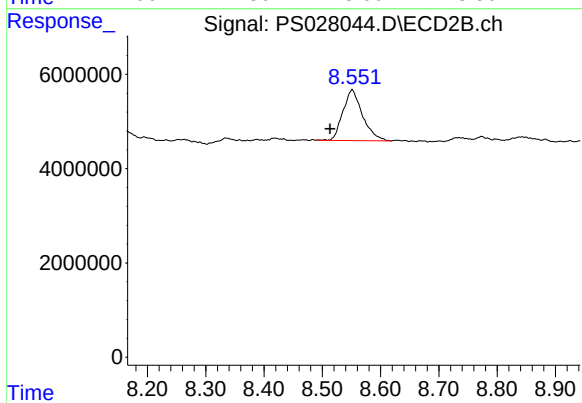

#8 DICHLORPROP


R.T.: 8.551 min
Delta R.T.: 0.038 min
Response: 25292940
Conc: 26.99 ng/ml

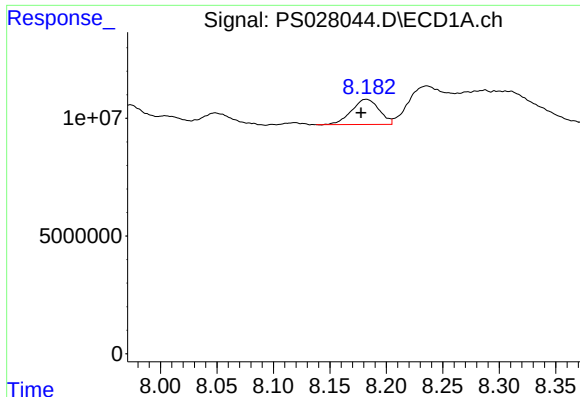

#9 2,4-D


R.T.: 8.182 min
Delta R.T.: 0.005 min
Response: 18197001
Conc: 5.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
WB-303-BOT

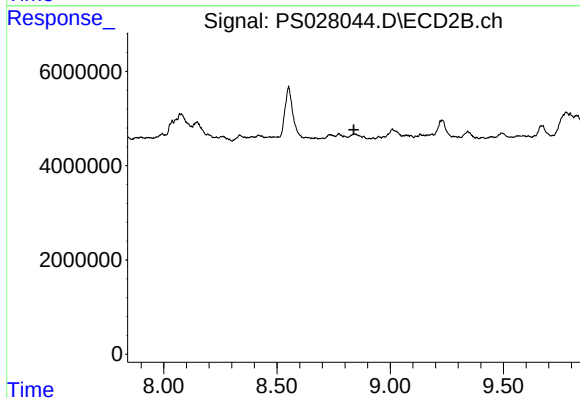


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.840 min
Response: 0
Conc: N.D.

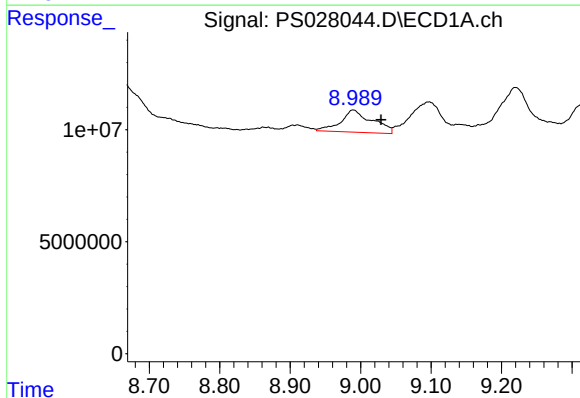


#11 2,4,5-TP (SILVEX)

R.T.: 8.990 min
Delta R.T.: -0.039 min
Response: 30905268
Conc: 1.91 ng/ml

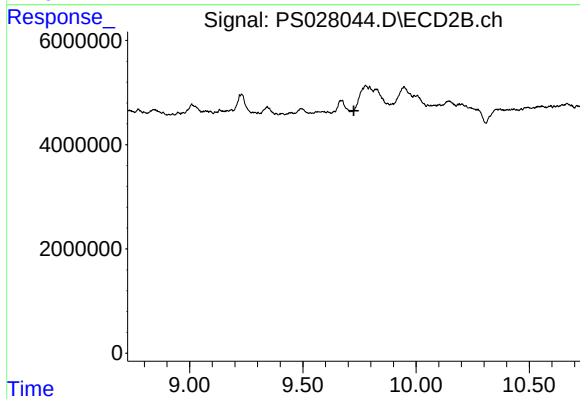

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.725 min
Response: 0
Conc: N.D.

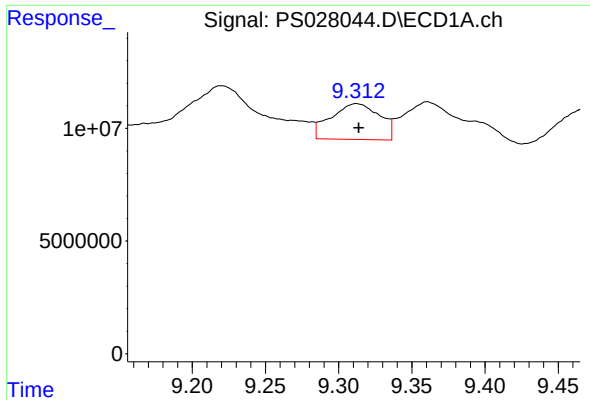

#12 2,4,5-T


R.T.: 9.312 min
Delta R.T.: -0.001 min
Response: 36793586
Conc: 2.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
WB-303-BOT

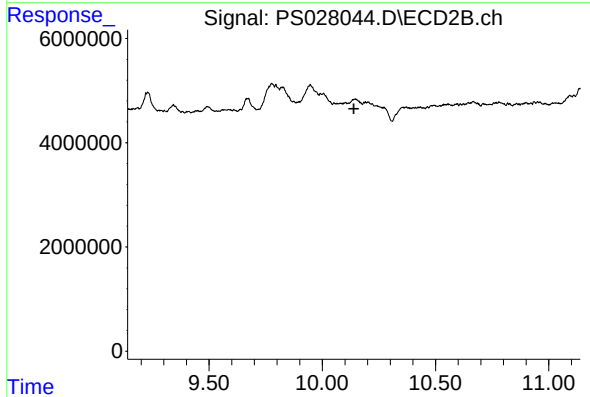


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 10.139 min
Response: 0
Conc: N.D.

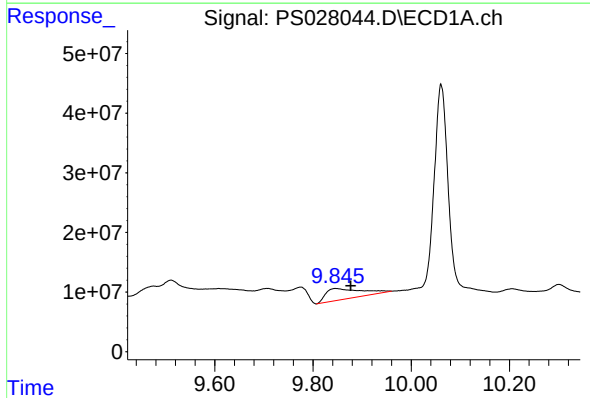


#13 2,4-DB

R.T.: 9.846 min
Delta R.T.: -0.031 min
Response: 91787048
Conc: 34.86 ng/ml

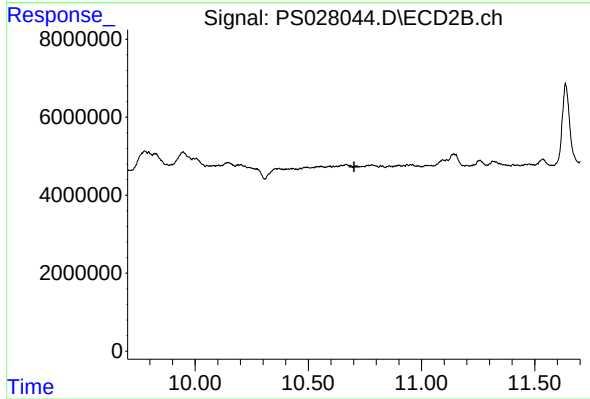

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.702 min
Response: 0
Conc: N.D.

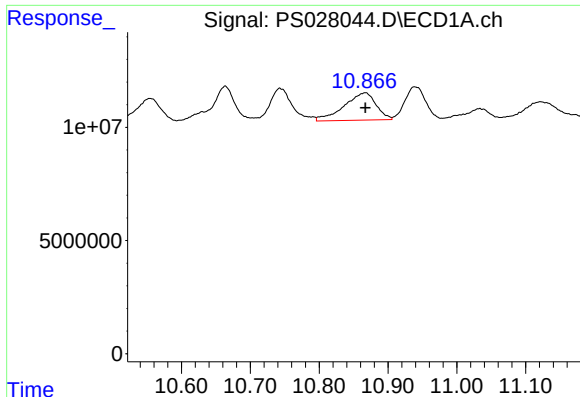

#15 Picloram


R.T.: 10.866 min
Delta R.T.: 0.000 min
Response: 38928690
Conc: 1.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
WB-303-BOT

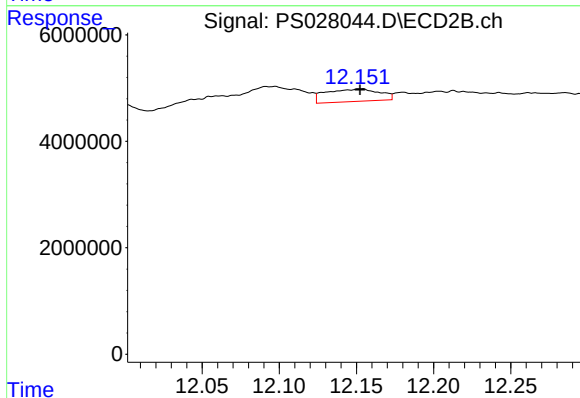


#15 Picloram

R.T.: 12.153 min
Delta R.T.: 0.000 min
Response: 5662696
Conc: 1.24 ng/ml

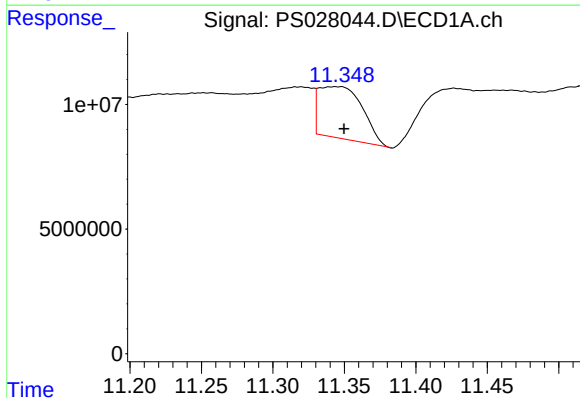

#16 DCPA

R.T.: 11.344 min
Delta R.T.: -0.005 min
Response: 43785750
Conc: 2.37 ng/ml

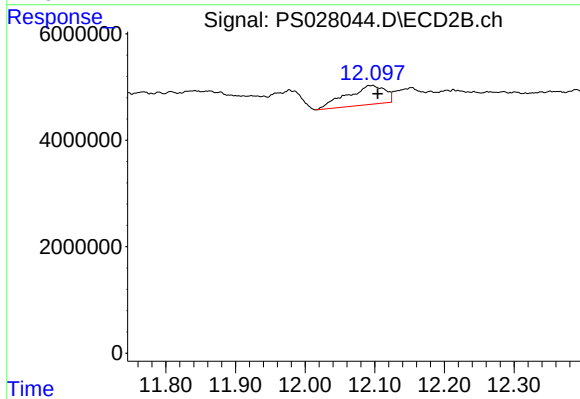

#16 DCPA

R.T.: 12.097 min
Delta R.T.: -0.008 min
Response: 13697888
Conc: 2.95 ng/ml