

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102425\
 Data File : PS032149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2025 09:46
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 06:21:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.266	0.000	1167683	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.444	0.000	8212860	0	1.167	N.D. #
5) T	DICAMBA	7.474	7.959	931201	4212581	<MDL	<MDL #
6) T	MCP	7.631	8.051	343584	467366	<MDL	<MDL #
7) T	MCPA	7.793	0.000	5272685	0	<MDL	N.D. #
8) T	DICHLORPROP	8.181	0.000	1844100	0	<MDL	N.D. #
9) T	2,4-D	8.414	0.000	3538836	0	<MDL	N.D. #
10) T	Pentachlo...	8.706	9.507	16666941	11219240	<MDL	<MDL #
11) T	2,4,5-TP ...	9.300	9.904	10280307	13833053	<MDL	<MDL #
12) T	2,4,5-T	9.578	0.000	2634779	0	<MDL	N.D. #
13) T	2,4-DB	10.154	0.000	668888	0	<MDL	N.D. #
14) T	DINOSEB	11.345	11.269	10922733	3029652	<MDL	<MDL #
15) T	Picloram	11.190	0.000	23418452	0	<MDL	N.D. #
16) T	DCPA	11.649	12.319	15291414	35876516	<MDL	1.080 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102425\
Data File : PS032149.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2025 09:46
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 06:21:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

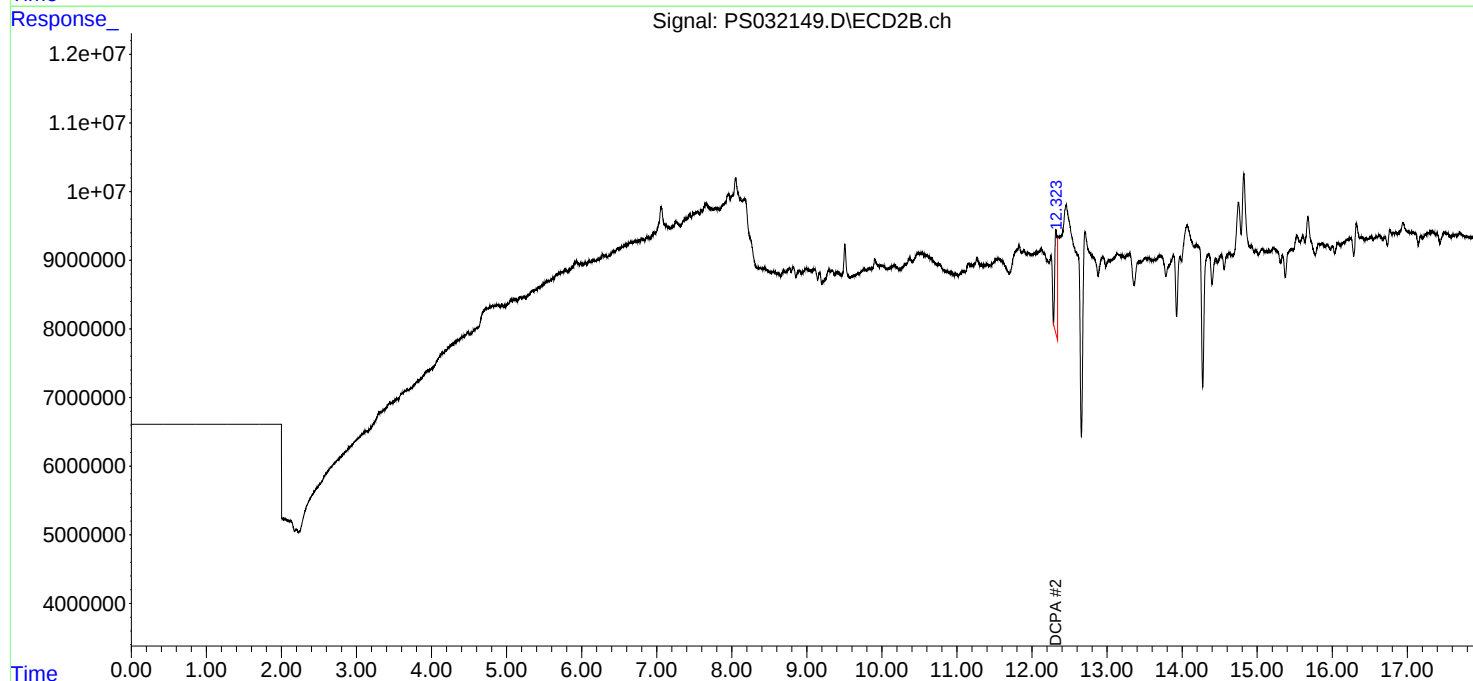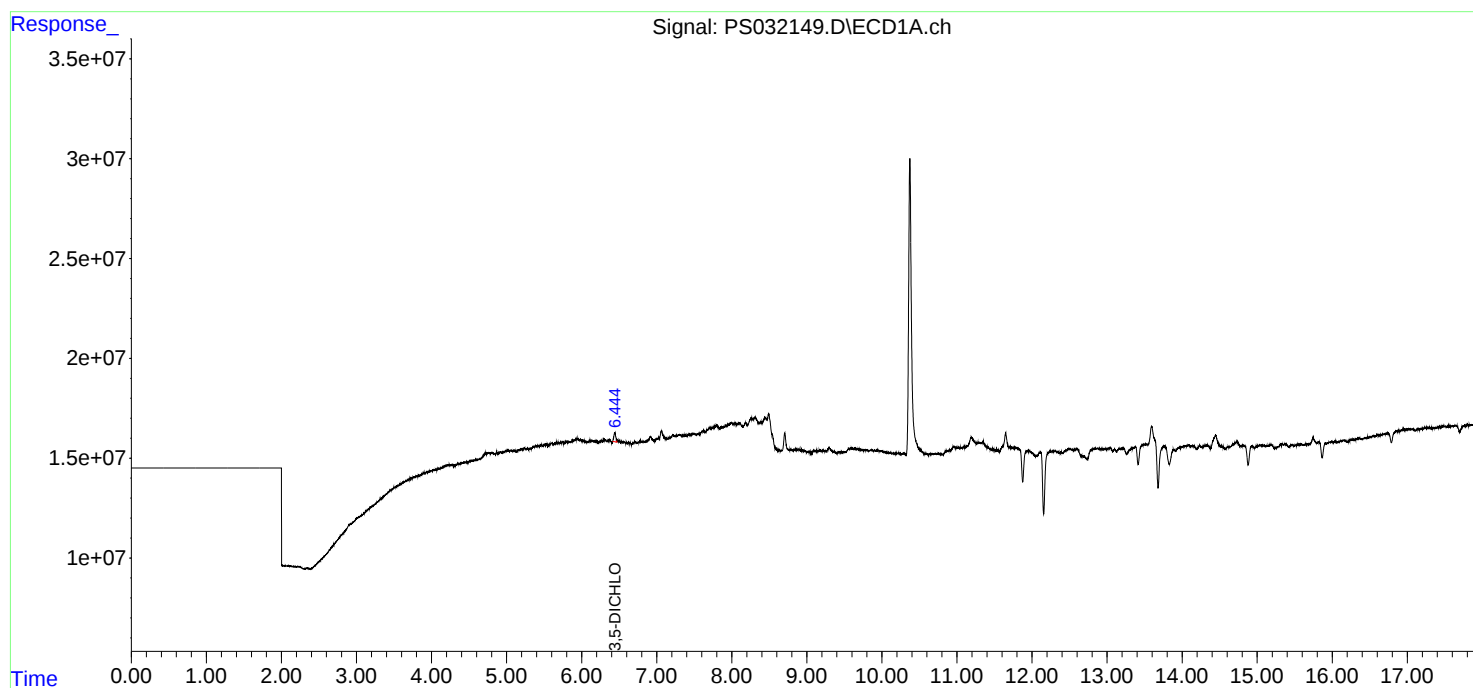


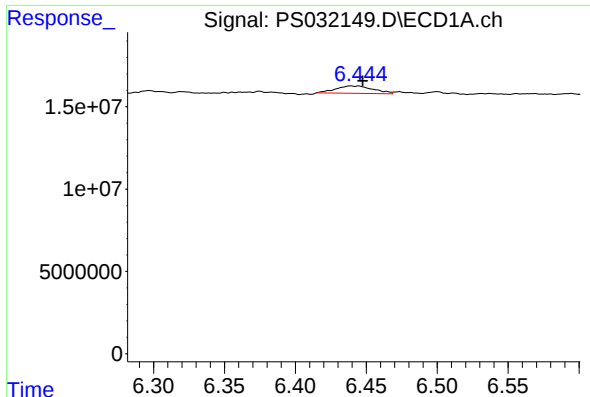

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.444 min
Delta R.T.: -0.003 min
Response: 8212860
Conc: 1.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

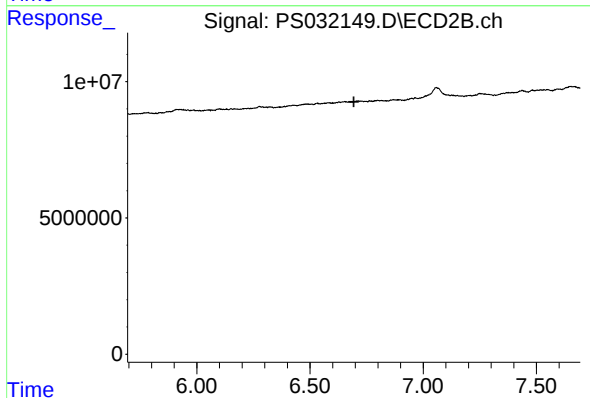


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.694 min
Response: 0
Conc: N.D.

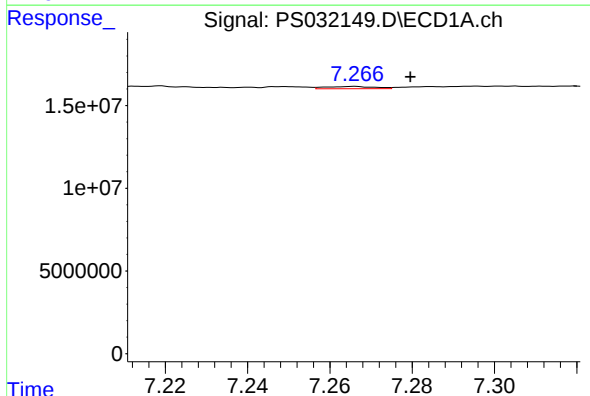


#4 2,4-DCAA

R.T.: 7.266 min
Delta R.T.: -0.014 min
Response: 1167683
Conc: N.D.

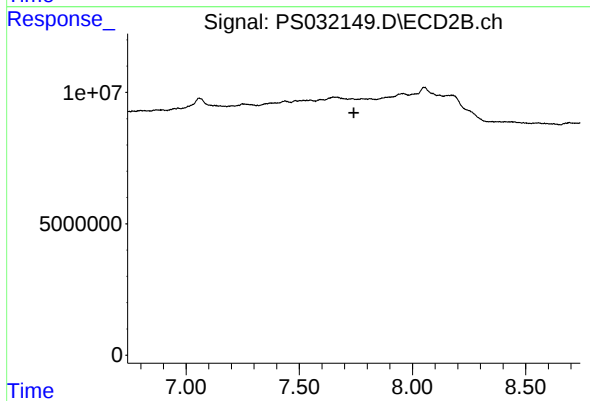

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.741 min
Response: 0
Conc: N.D.

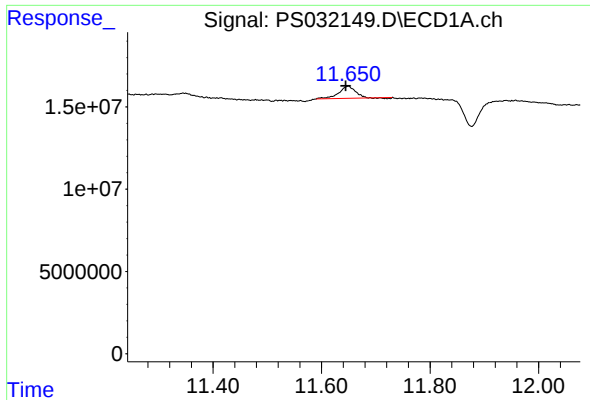

#16 DCPA

R.T.: 11.649 min
Delta R.T.: 0.005 min
Response: 15291414
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

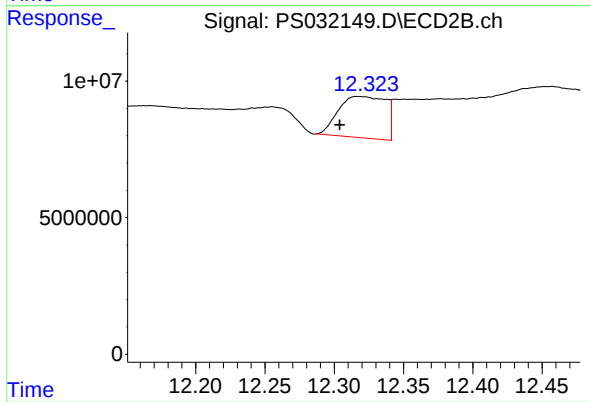

#16 DCPA

R.T.: 12.319 min
Delta R.T.: 0.015 min
Response: 35876516
Conc: 1.08 ng/ml