

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102425\
 Data File : PS032150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2025 10:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 06:21:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.285	7.753	1717.6E6	564.8E6	360.304	513.280 #
Target Compounds							
1) T	Dalapon	0.000	2.668	0	64817785	N.D.	17.247
2) T	3,5-DICHL...	6.458	0.000	241338	0	<MDL	N.D. #
3) T	4-Nitroph...	7.074	0.000	1819414	0	1.363	N.D. #
7) T	MCPA	7.844f	8.245f	189291	13912724	<MDL	3.688 #
8) T	DICHLORPROP	8.188	0.000	602945	0	<MDL	N.D. #
10) T	Pentachlo...	8.717	9.517	5985018	2854798	<MDL	<MDL #
11) T	2,4,5-TP ...	9.278	0.000	3004614	0	<MDL	N.D. #
12) T	2,4,5-T	0.000	10.305	0	3429323	N.D.	<MDL
13) T	2,4-DB	10.179f	0.000	4024012	0	1.298	N.D. #
14) T	DINOSEB	11.356	0.000	7778477	0	<MDL	N.D. #
15) T	Picloram	11.159	0.000	601785	0	<MDL	N.D. #
16) T	DCPA	11.645	0.000	5214646	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102425\
Data File : PS032150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2025 10:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 06:21:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

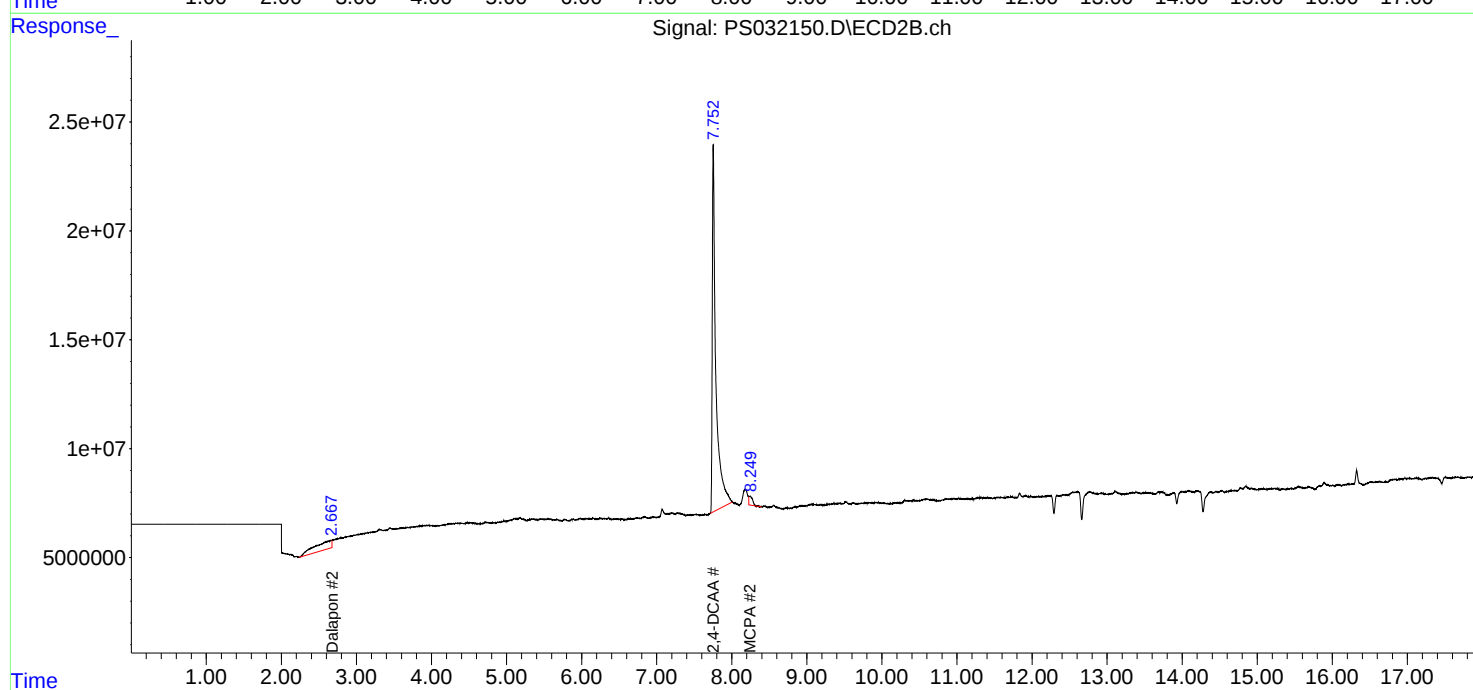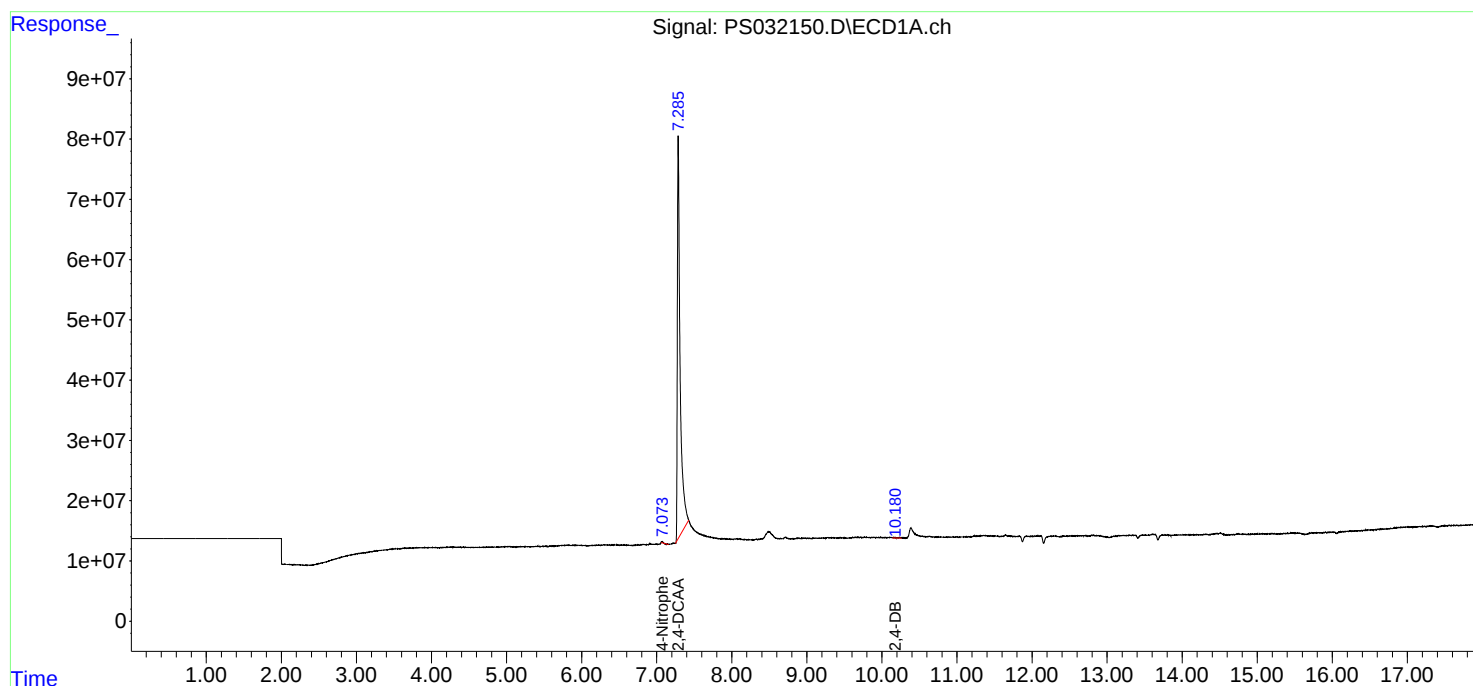


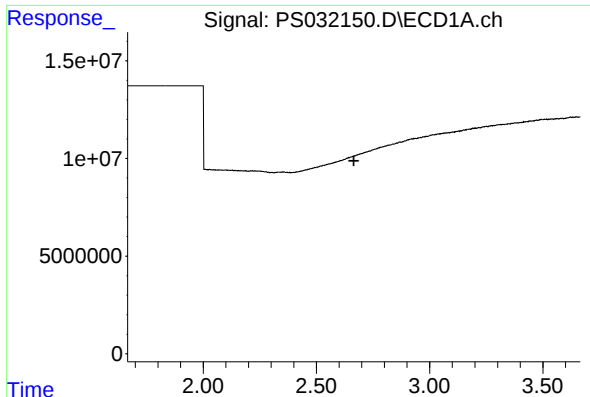

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.665 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

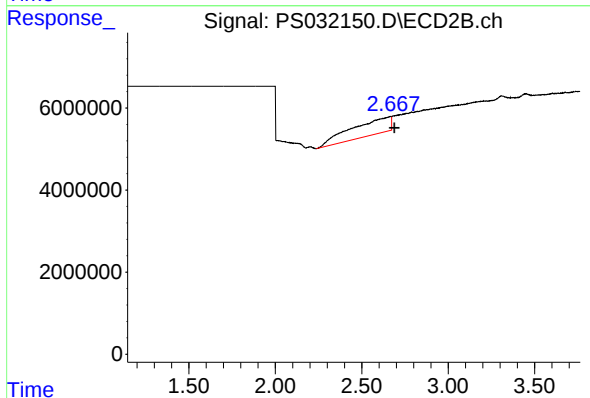


#1 Dalapon

R.T.: 2.668 min
Delta R.T.: -0.021 min
Response: 64817785
Conc: 17.25 ng/ml

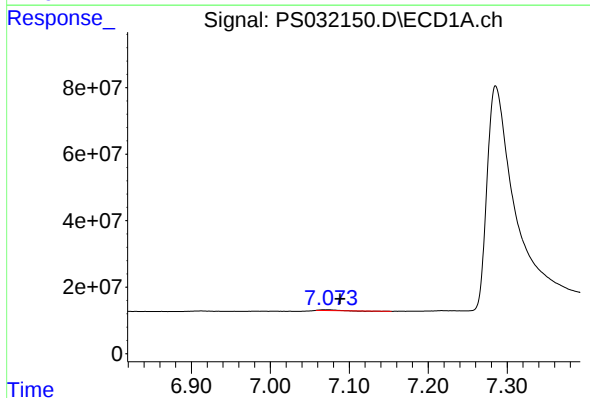


#3 4-Nitrophenol

R.T.: 7.074 min
Delta R.T.: -0.015 min
Response: 1819414
Conc: 1.36 ng/ml

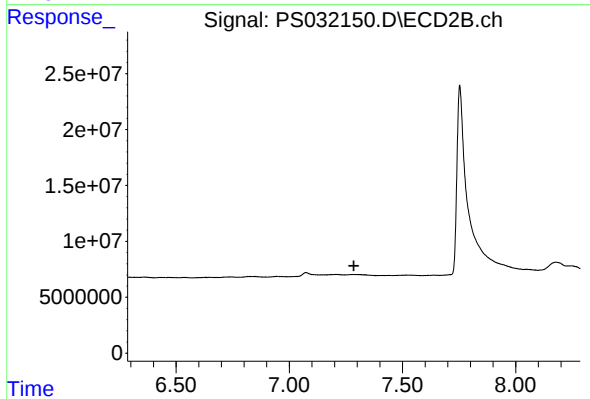

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.285 min
Response: 0
Conc: N.D.

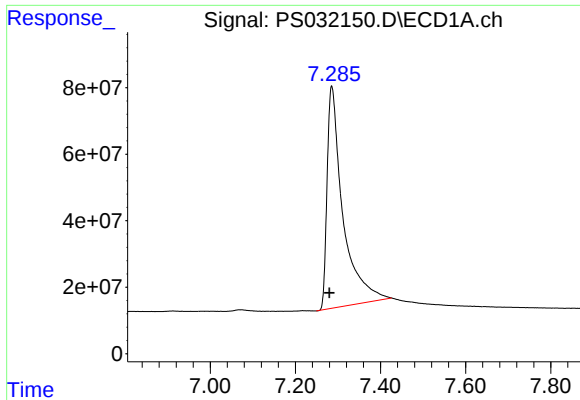

#4 2,4-DCAA


R.T.: 7.285 min
Delta R.T.: 0.006 min
Response: 1717582562
Conc: 360.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

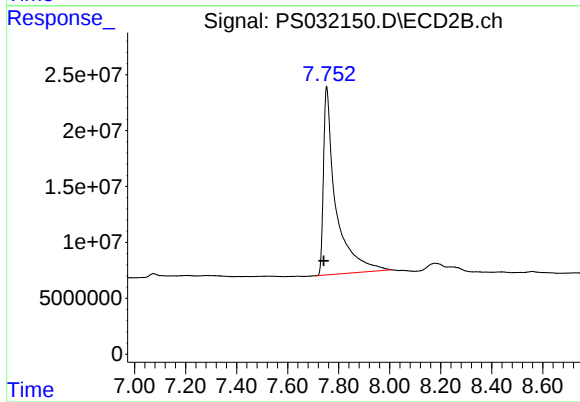


#4 2,4-DCAA

R.T.: 7.753 min
Delta R.T.: 0.012 min
Response: 564782908
Conc: 513.28 ng/ml

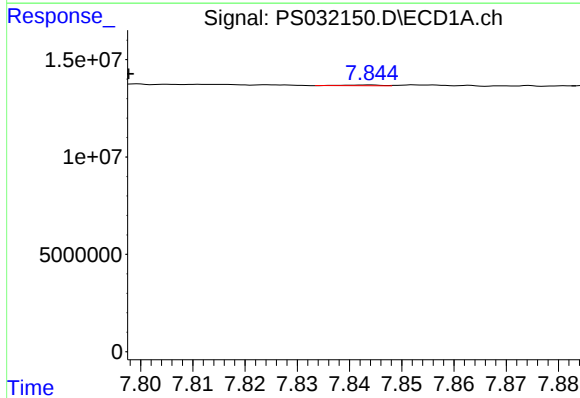


#7 MCPA

R.T.: 7.844 min
Delta R.T.: 0.046 min
Response: 189291
Conc: N.D.

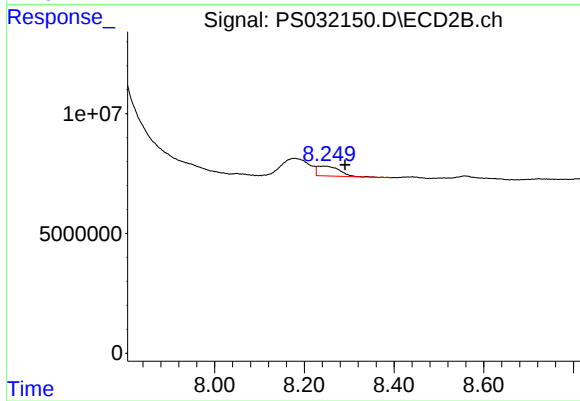

#7 MCPA


R.T.: 8.245 min
Delta R.T.: -0.045 min
Response: 13912724
Conc: 3.69 ug/ml

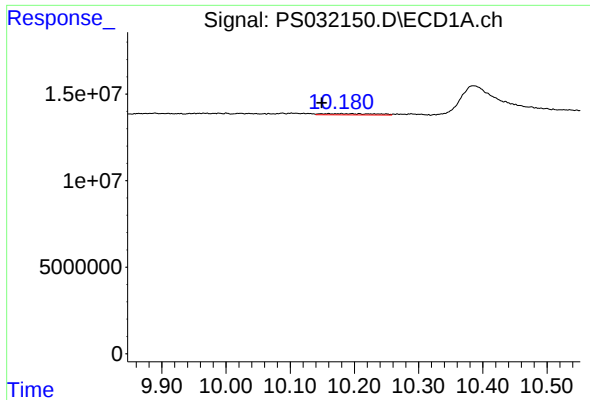

#13 2,4-DB

R.T.: 10.179 min
Delta R.T.: 0.030 min
Response: 4024012
Conc: 1.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

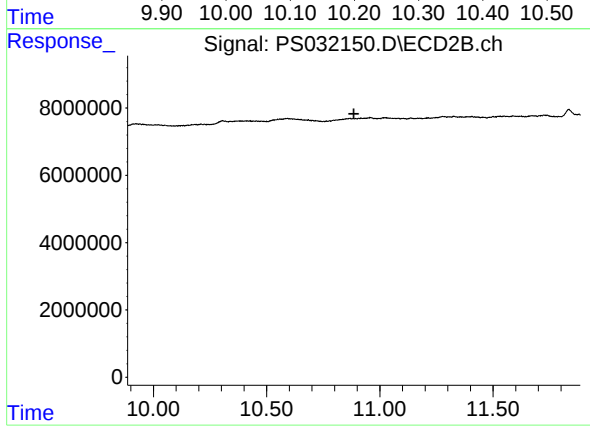

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.885 min
Response: 0
Conc: N.D.