

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102425\
 Data File : PS032152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2025 12:28
 Operator : AR\AJ
 Sample : PB170172TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 06:22:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.284	7.752	1635.6E6	511.4E6	343.113	464.745 #
Target Compounds							
1) T	Dalapon	2.694f	0.000	9595687	0	1.242	N.D. #
2) T	3,5-DICHL...	6.453	0.000	1628764	0	<MDL	N.D. #
3) T	4-Nitroph...	7.069	0.000	1678342	0	1.257	N.D. #
7) T	MCPA	7.798	0.000	991928	0	<MDL	N.D. #
8) T	DICHLORPROP	8.162	0.000	508961	0	<MDL	N.D. #
10) T	Pentachlo...	8.704	9.515	37477109	24054780	<MDL	<MDL #
11) T	2,4,5-TP ...	9.291	9.919f	9813523	6149957	<MDL	<MDL #
12) T	2,4,5-T	9.568	0.000	3906335	0	<MDL	N.D. #
13) T	2,4-DB	10.152	0.000	217088	0	<MDL	N.D. #
14) T	DINOSEB	11.347	11.274	15859222	8313540	<MDL	<MDL #
15) T	Picloram	11.161	0.000	3650025	0	<MDL	N.D. #
16) T	DCPA	11.646	12.311	26753500	49252123	<MDL	1.483 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102425\
Data File : PS032152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2025 12:28
Operator : AR\AJ
Sample : PB170172TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 06:22:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

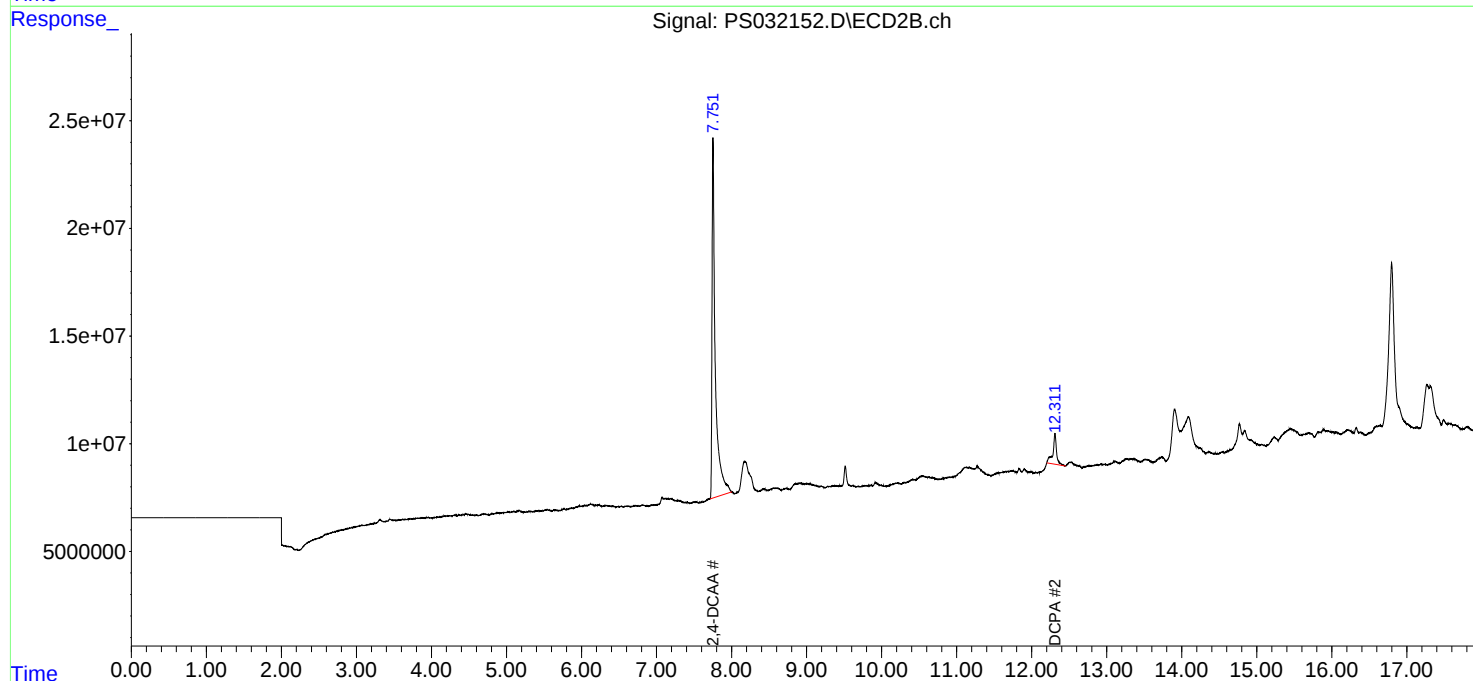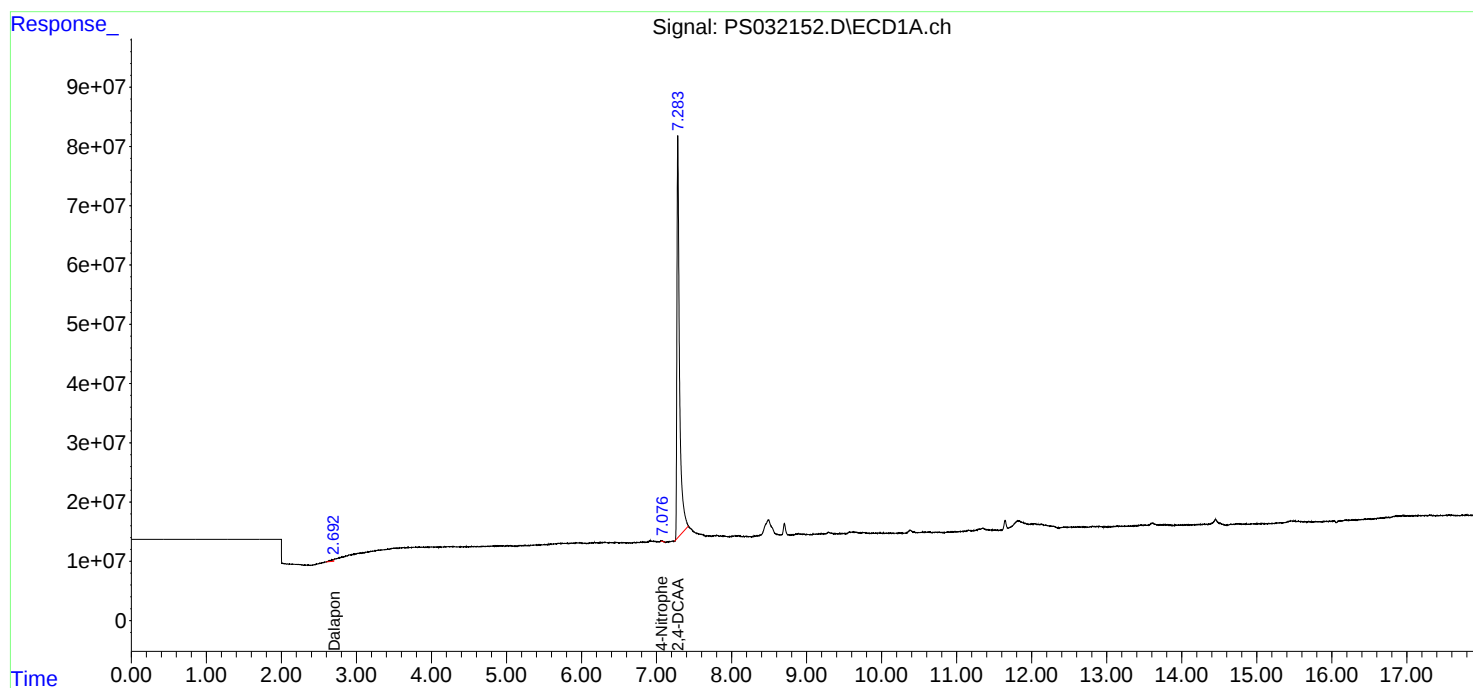


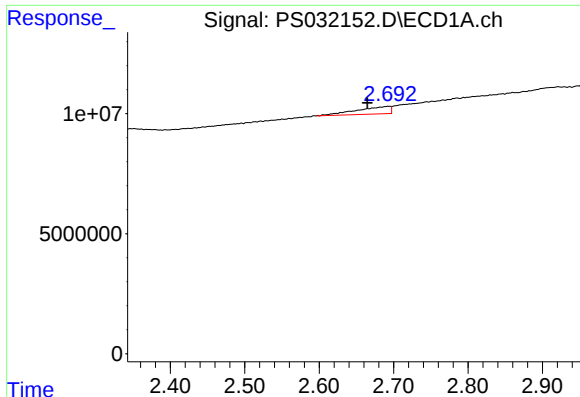

#1 Dalapon


R.T.: 2.694 min
Delta R.T.: 0.029 min
Response: 9595687
Conc: 1.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

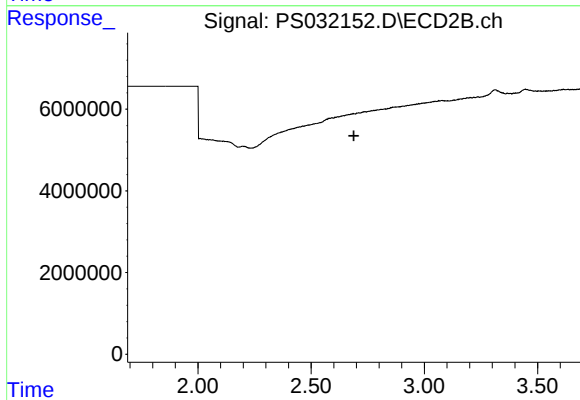


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.689 min
Response: 0
Conc: N.D.

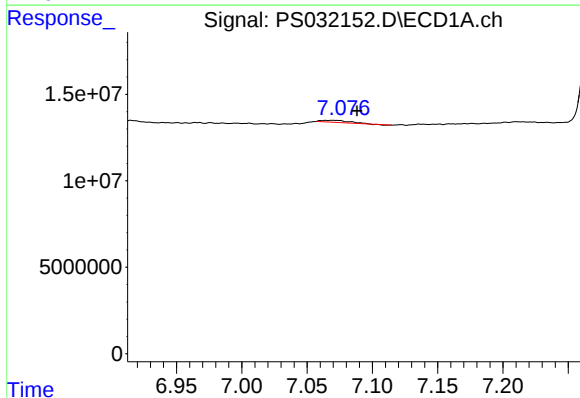


#3 4-Nitrophenol

R.T.: 7.069 min
Delta R.T.: -0.019 min
Response: 1678342
Conc: 1.26 ng/ml

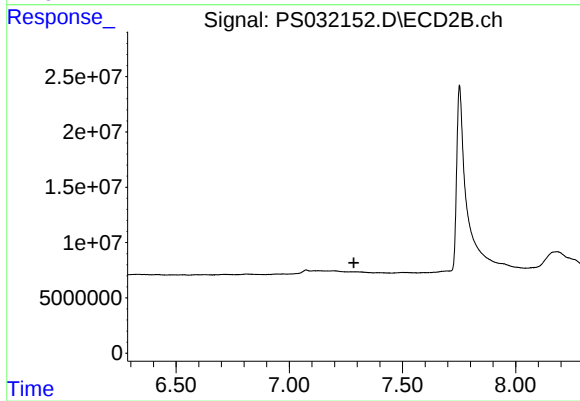

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.285 min
Response: 0
Conc: N.D.

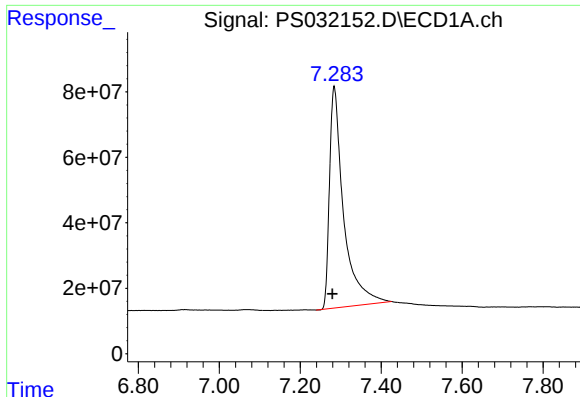

#4 2,4-DCAA


R.T.: 7.284 min
Delta R.T.: 0.004 min
Response: 1635630044
Conc: 343.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

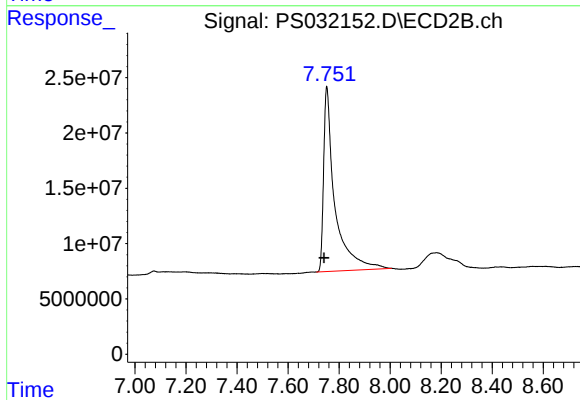


#4 2,4-DCAA

R.T.: 7.752 min
Delta R.T.: 0.011 min
Response: 511377993
Conc: 464.75 ng/ml

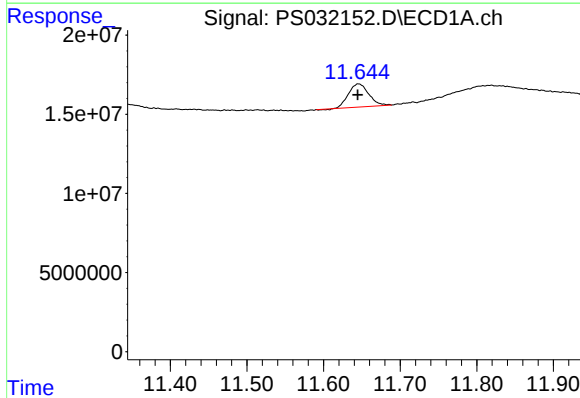

#16 DCPA

R.T.: 11.646 min
Delta R.T.: 0.001 min
Response: 26753500
Conc: N.D.

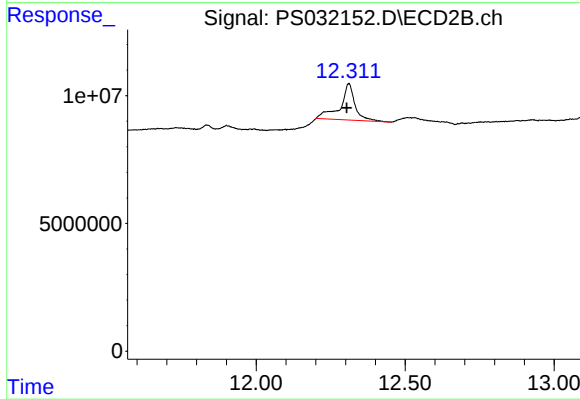

#16 DCPA

R.T.: 12.311 min
Delta R.T.: 0.007 min
Response: 49252123
Conc: 1.48 ng/ml