

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102425\
 Data File : PS032153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2025 14:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 06:22:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.282	7.750	1864.4E6	583.5E6	391.106	530.301 #
Target Compounds							
1) T	Dalapon	2.693f	0.000	7957819	0	1.030	N.D. #
2) T	3,5-DICHL...	6.444	0.000	2944889	0	<MDL	N.D. #
3) T	4-Nitroph...	7.067	0.000	655831	0	<MDL	N.D. #
7) T	MCPA	7.800	8.243f	6806521	20221547	<MDL	5.360 #
8) T	DICHLORPROP	8.154	0.000	463314	0	<MDL	N.D. #
10) T	Pentachlo...	8.706	9.514	8485616	6152155	<MDL	<MDL #
11) T	2,4,5-TP ...	9.288	9.915f	9717830	6097198	<MDL	<MDL #
12) T	2,4,5-T	9.582	10.305	7776912	4333102	<MDL	<MDL #
13) T	2,4-DB	10.139	0.000	667368	0	<MDL	N.D. #
14) T	DINOSEB	11.346	11.275	32060954	5614742	1.438	<MDL #
15) T	Picloram	11.198f	12.406f	11575551	12718618	<MDL	<MDL #
16) T	DCPA	11.645	12.319	9353111	46933734	<MDL	1.413 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102425\
Data File : PS032153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2025 14:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 06:22:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

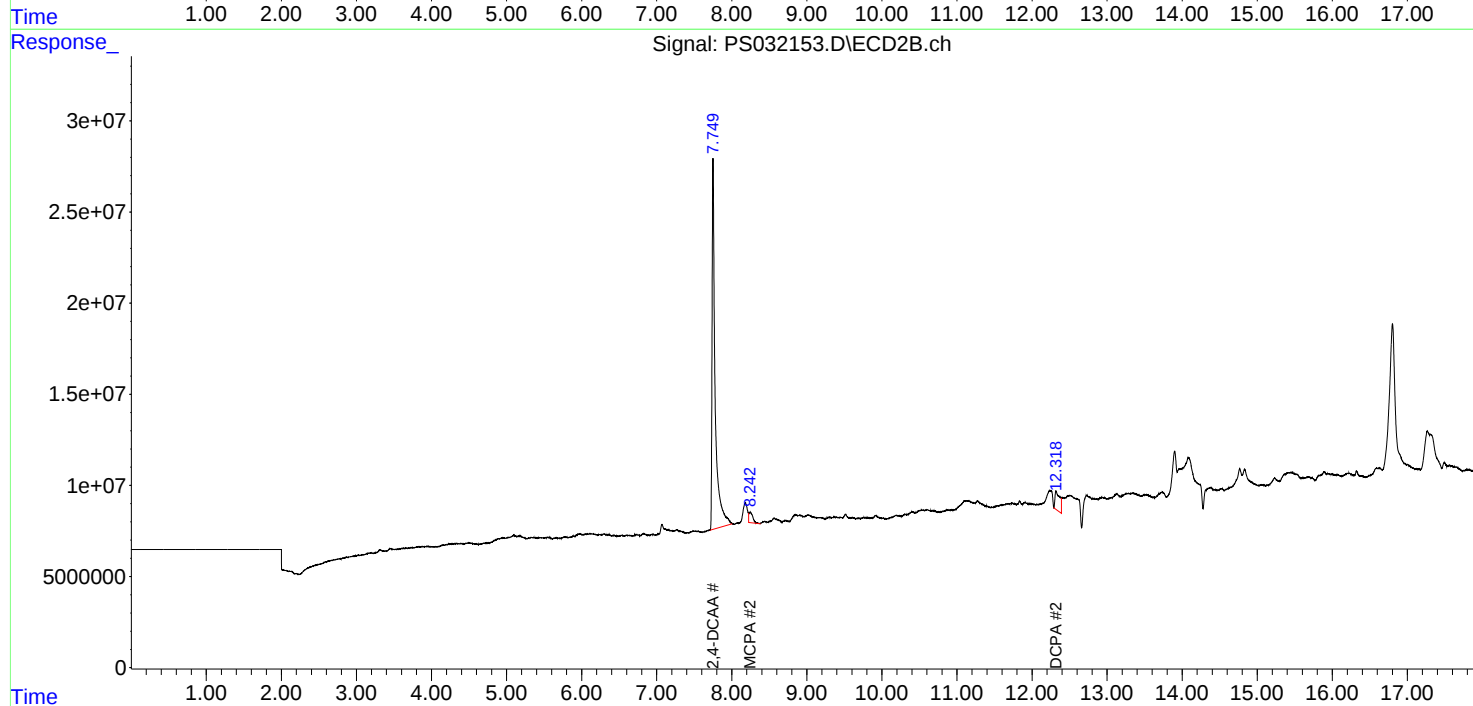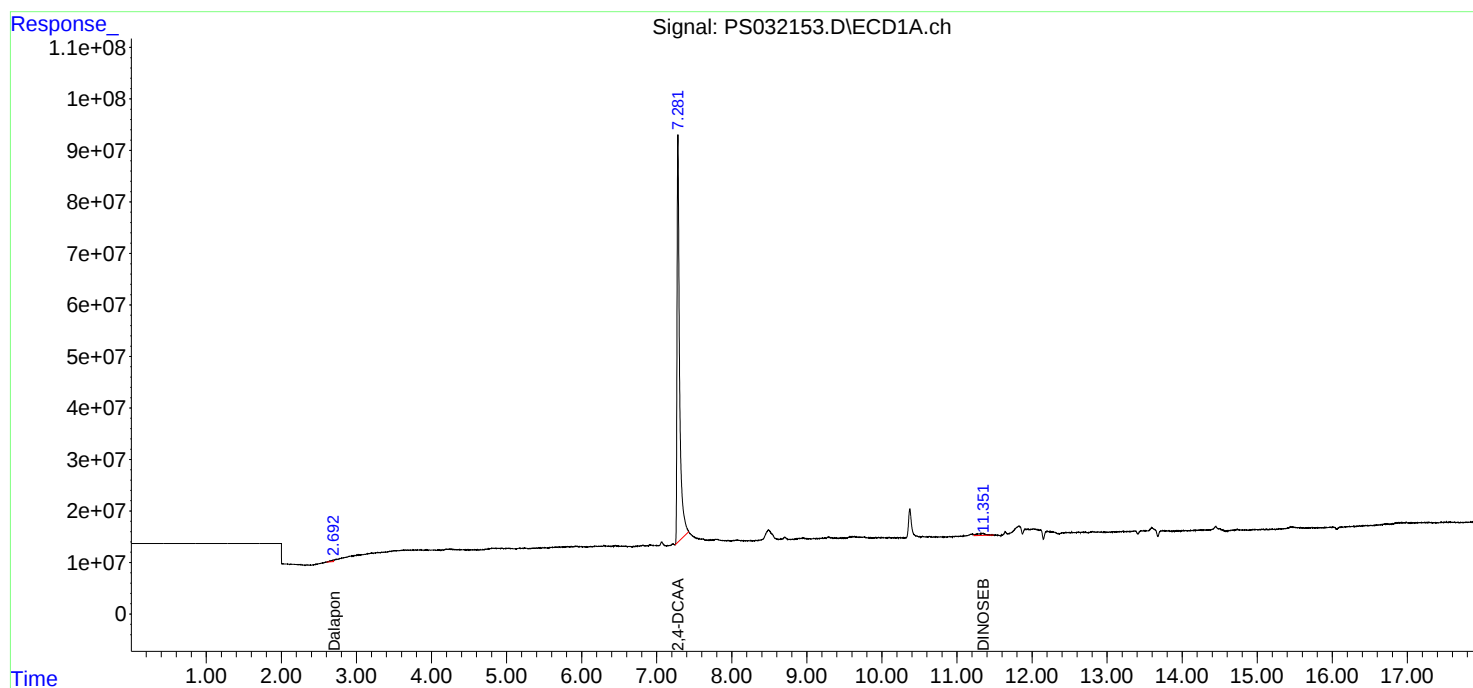


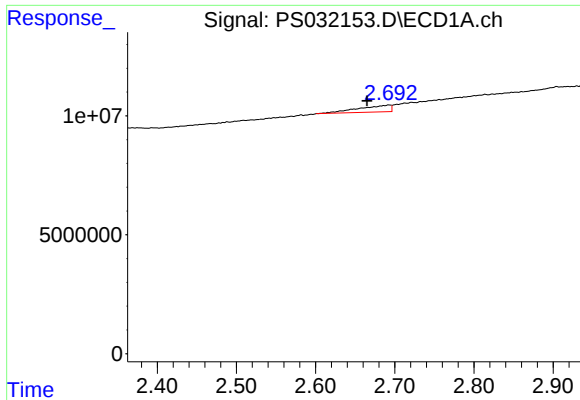

#1 Dalapon


R.T.: 2.693 min
Delta R.T.: 0.028 min
Response: 7957819
Conc: 1.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

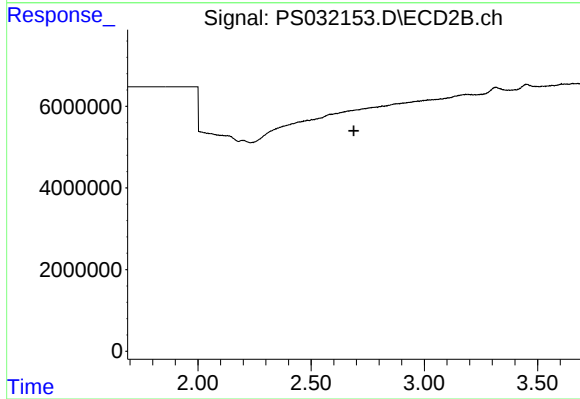


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.689 min
Response: 0
Conc: N.D.

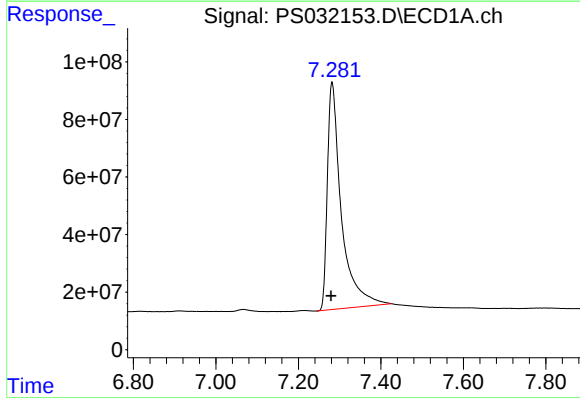


#4 2,4-DCAA

R.T.: 7.282 min
Delta R.T.: 0.002 min
Response: 1864417405
Conc: 391.11 ng/ml

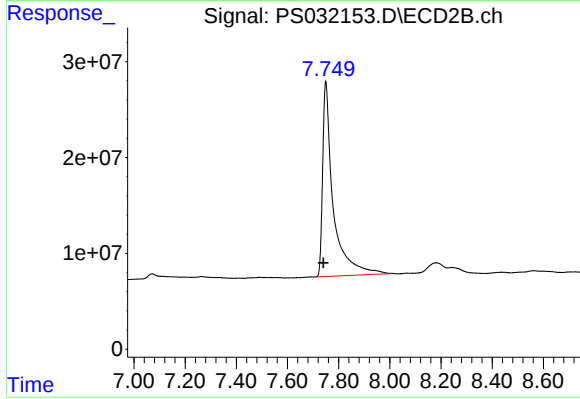

#4 2,4-DCAA


R.T.: 7.750 min
Delta R.T.: 0.009 min
Response: 583512144
Conc: 530.30 ng/ml

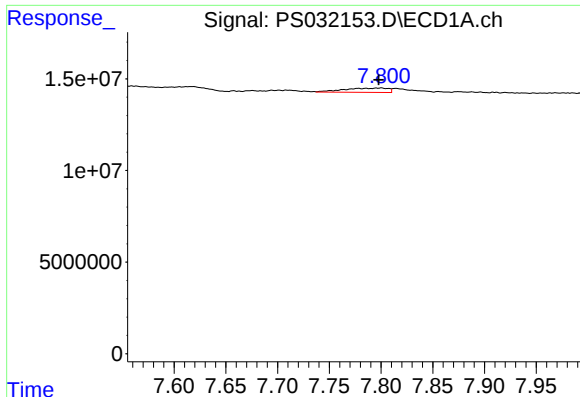

#7 MCPA


R.T.: 7.800 min
Delta R.T.: 0.002 min
Response: 6806521
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

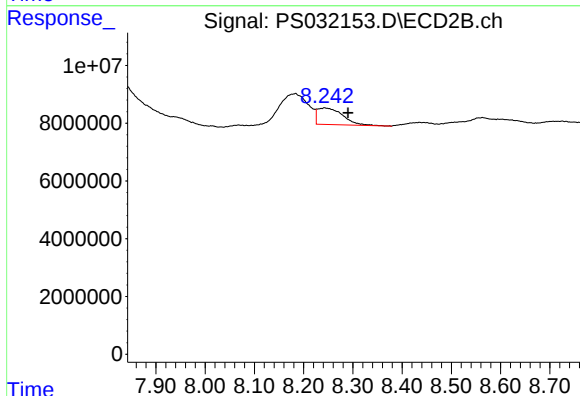


#7 MCPA

R.T.: 8.243 min
Delta R.T.: -0.048 min
Response: 20221547
Conc: 5.36 ug/ml

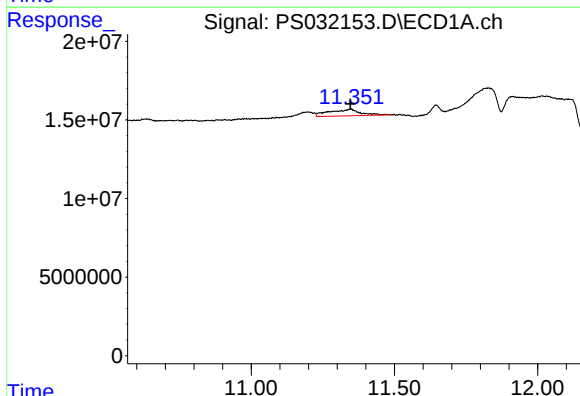


#14 DINOSEB

R.T.: 11.346 min
Delta R.T.: 0.000 min
Response: 32060954
Conc: 1.44 ng/ml

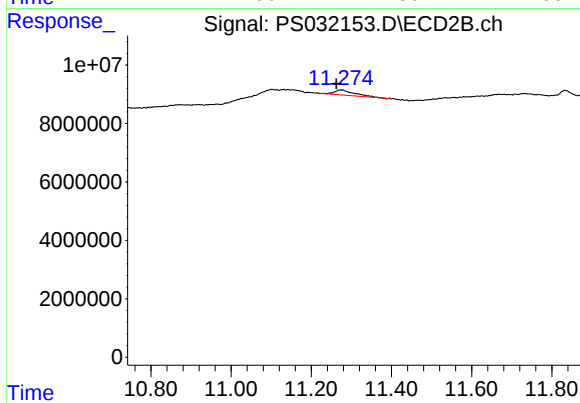

#14 DINOSEB


R.T.: 11.275 min
Delta R.T.: 0.012 min
Response: 5614742
Conc: N.D.

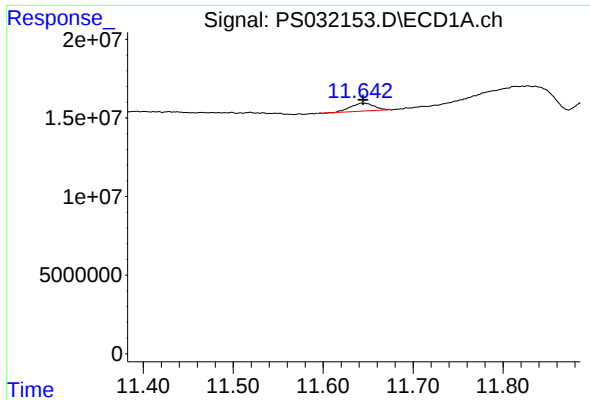

#16 DCPA

R.T.: 11.645 min
Delta R.T.: 0.000 min
Response: 9353111
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

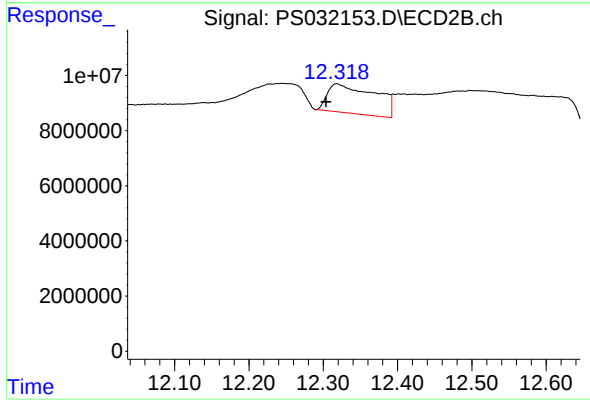

#16 DCPA

R.T.: 12.319 min
Delta R.T.: 0.015 min
Response: 46933734
Conc: 1.41 ng/ml