

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102425\
 Data File : PS032159.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2025 17:28
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 06:23:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.279	7.748	1887.0E6	573.0E6	395.833	520.782 #
Target Compounds							
1) T	Dalapon	2.703f	2.685	52751977	33526099	6.827	8.921 #
2) T	3,5-DICHL...	6.444	0.000	6325371	0	<MDL	N.D. #
6) T	MCP	7.670	0.000	10354	0	<MDL	N.D. #
7) T	MCPA	7.770f	8.247f	15237695	19397968	1.035	5.142 #
8) T	DICHLORPROP	8.175	0.000	1646487	0	<MDL	N.D. #
10) T	Pentachlo...	8.699	9.513	8977449	14921885	<MDL	<MDL #
11) T	2,4,5-TP ...	9.281	9.914	6795351	5943124	<MDL	<MDL #
12) T	2,4,5-T	9.569	0.000	1183663	0	<MDL	N.D. #
13) T	2,4-DB	10.189f	0.000	7682788	0	2.478	N.D. #
15) T	Picloram	11.183	0.000	9075823	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102425\
Data File : PS032159.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2025 17:28
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 06:23:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

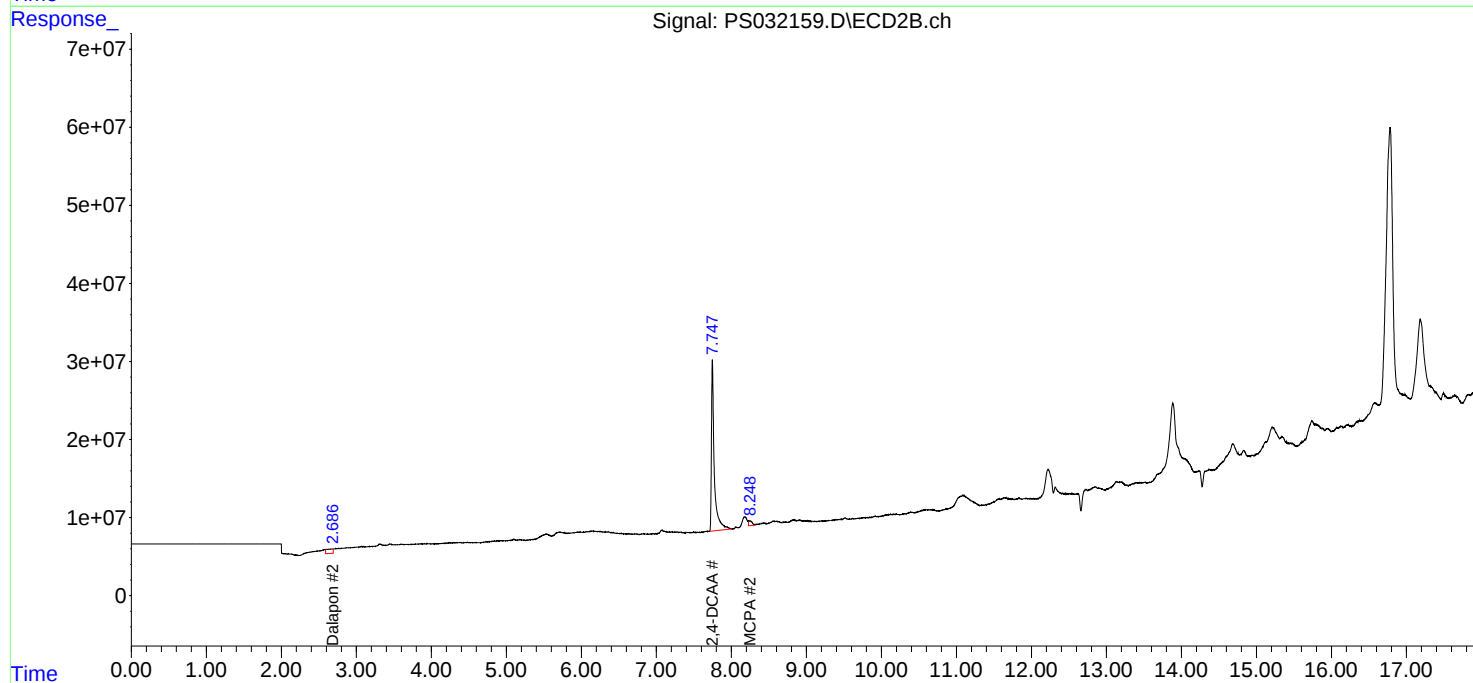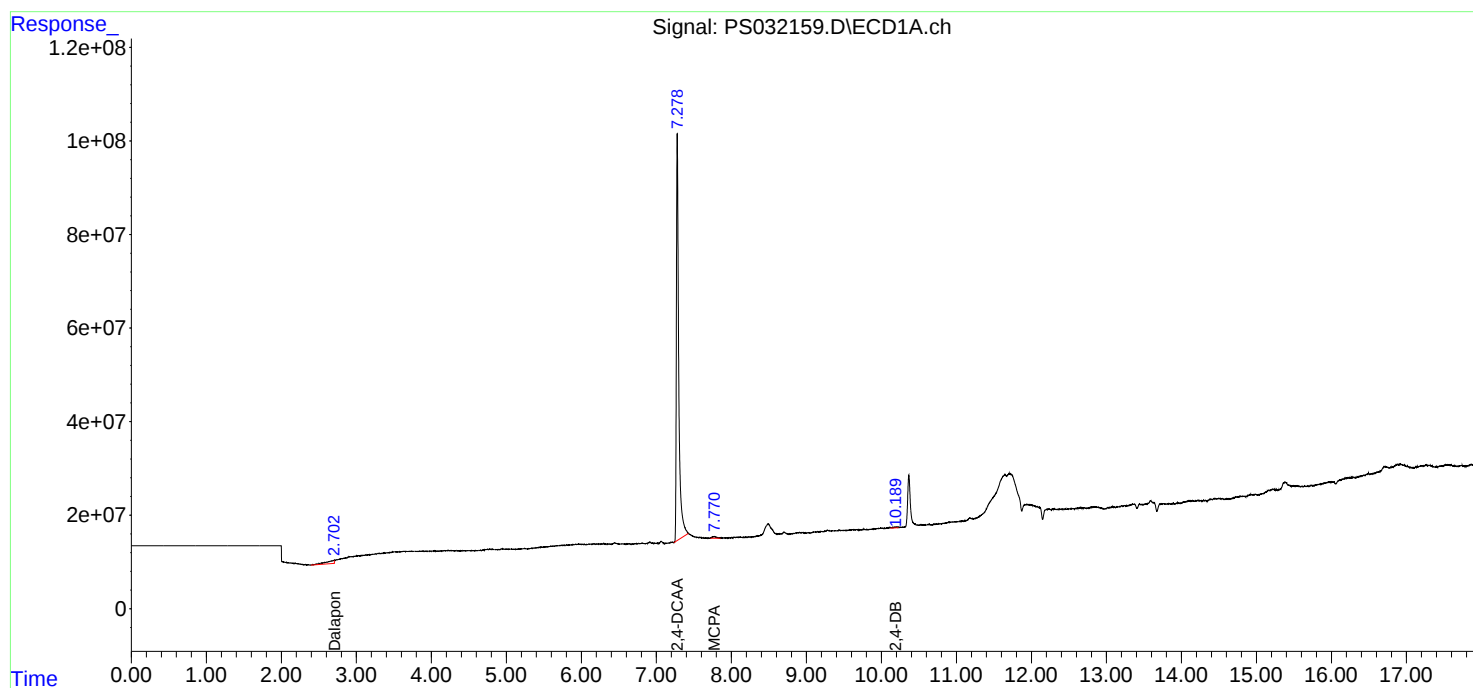


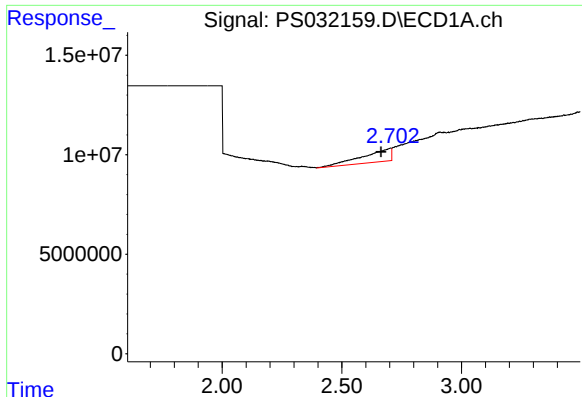

#1 Dalapon


R.T.: 2.703 min
Delta R.T.: 0.038 min
Response: 52751977
Conc: 6.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

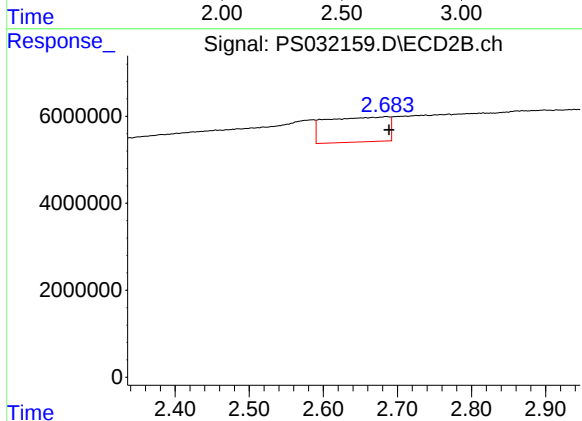


#1 Dalapon

R.T.: 2.685 min
Delta R.T.: -0.004 min
Response: 33526099
Conc: 8.92 ng/ml

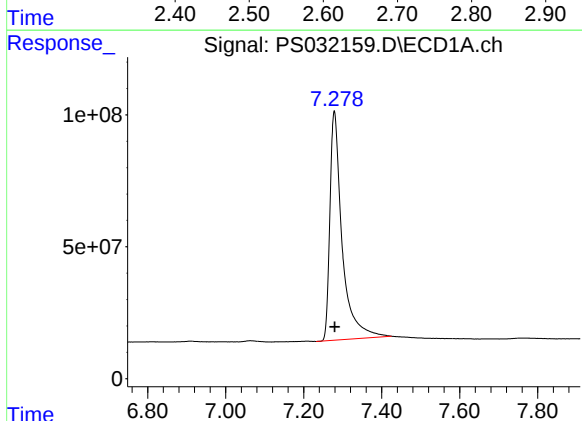


#4 2,4-DCAA

R.T.: 7.279 min
Delta R.T.: -0.001 min
Response: 1886950673
Conc: 395.83 ng/ml

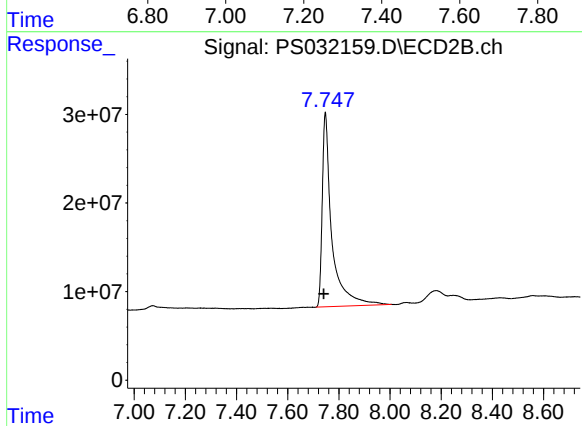

#4 2,4-DCAA


R.T.: 7.748 min
Delta R.T.: 0.007 min
Response: 573037230
Conc: 520.78 ng/ml

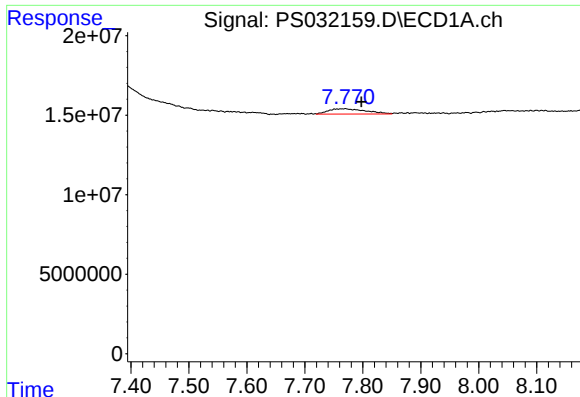

#7 MCPA


R.T.: 7.770 min
Delta R.T.: -0.028 min
Response: 15237695
Conc: 1.04 ug/ml

Instrument :
ECD_S
ClientSampleId :

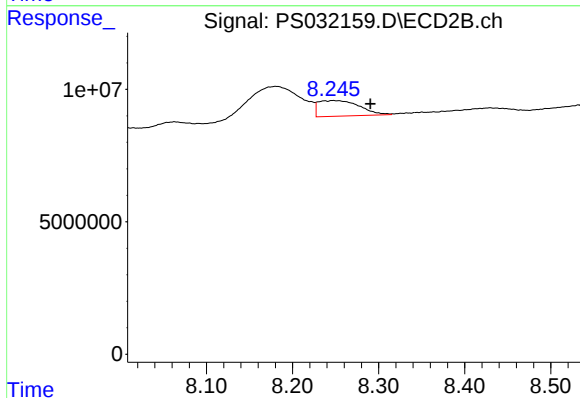


#7 MCPA

R.T.: 8.247 min
Delta R.T.: -0.043 min
Response: 19397968
Conc: 5.14 ug/ml

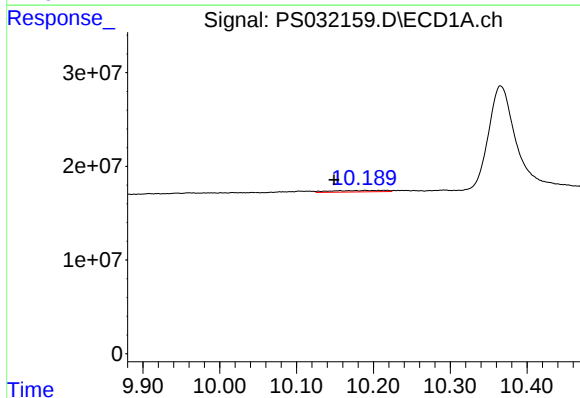

#13 2,4-DB

R.T.: 10.189 min
Delta R.T.: 0.040 min
Response: 7682788
Conc: 2.48 ng/ml

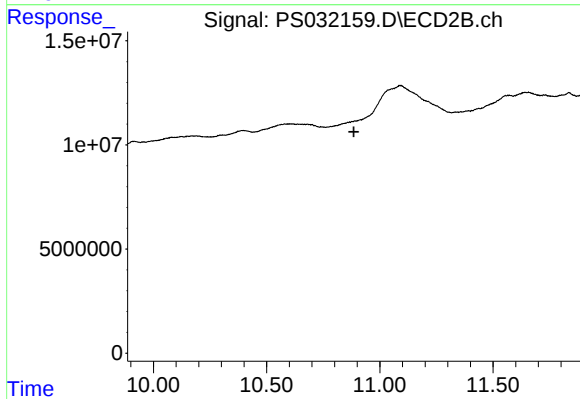

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.885 min
Response: 0
Conc: N.D.