

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
 Data File : PS007337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2019 11:45 am
 Operator : SM\AJ
 Sample : PB124255BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 14:50:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.434	5.162	816.6E6	444.4E6	596.669	631.905
Target Compounds							
1) T	Dalapon	1.994	0.000	37225065	0	22.247	N.D. #
2) T	3,5-DICHL...	0.000	4.497	0	34555058	N.D.	40.160
5) T	DICAMBA	5.528	0.000	49297947	0	10.033	N.D. #
7) T	MCPA	5.838	5.534	37684503	24273309	7.306	8.350
10) T	Pentachlo...	0.000	6.455	0	8086247	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.761	0	21601684	N.D.	5.679
14) T	DINOSEB	0.000	7.955	0	11156734	N.D.	3.974
15) T	Picloram	0.000	8.915	0	22730032	N.D.	3.702
16) T	DCPA	0.000	8.915	0	22730032	N.D.	4.533



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
Data File : PS007337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2019 11:45 am
Operator : SM\AJ
Sample : PB124255BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 14:50:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

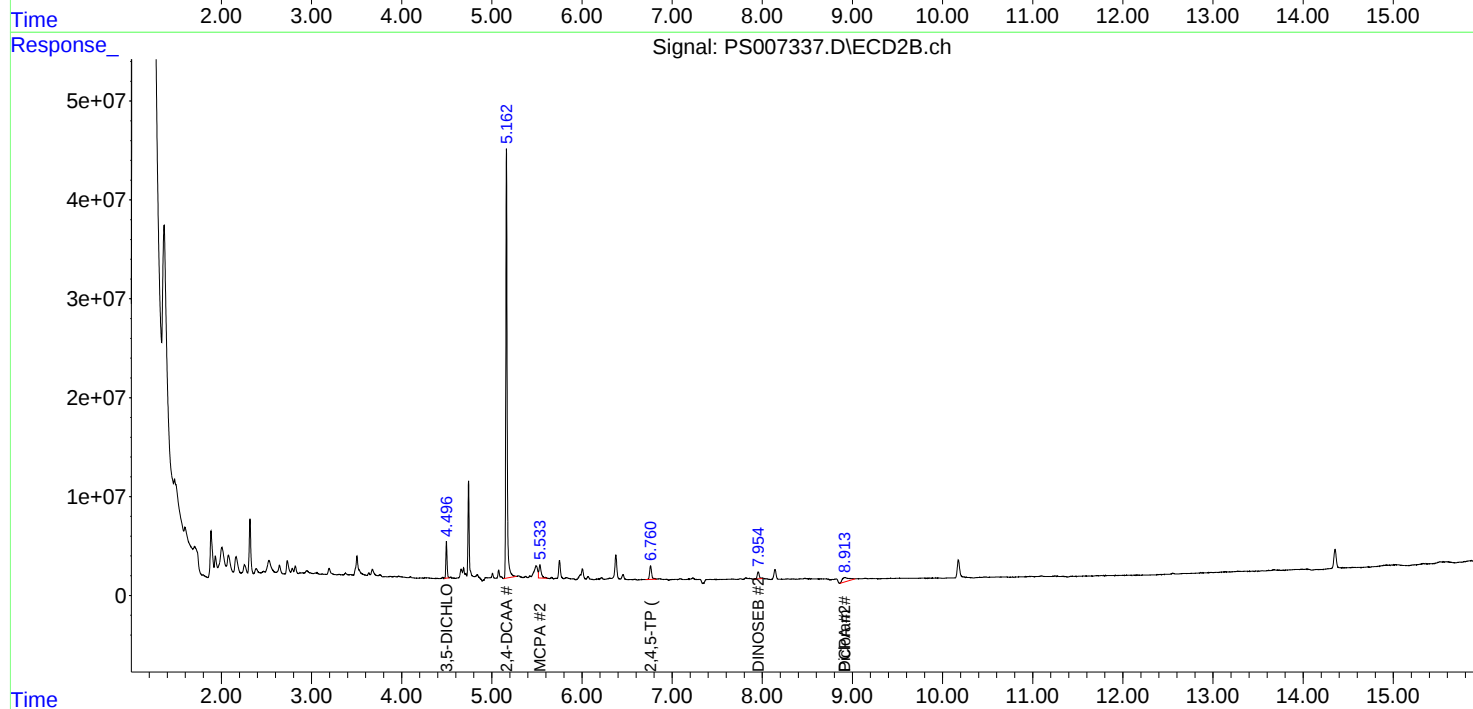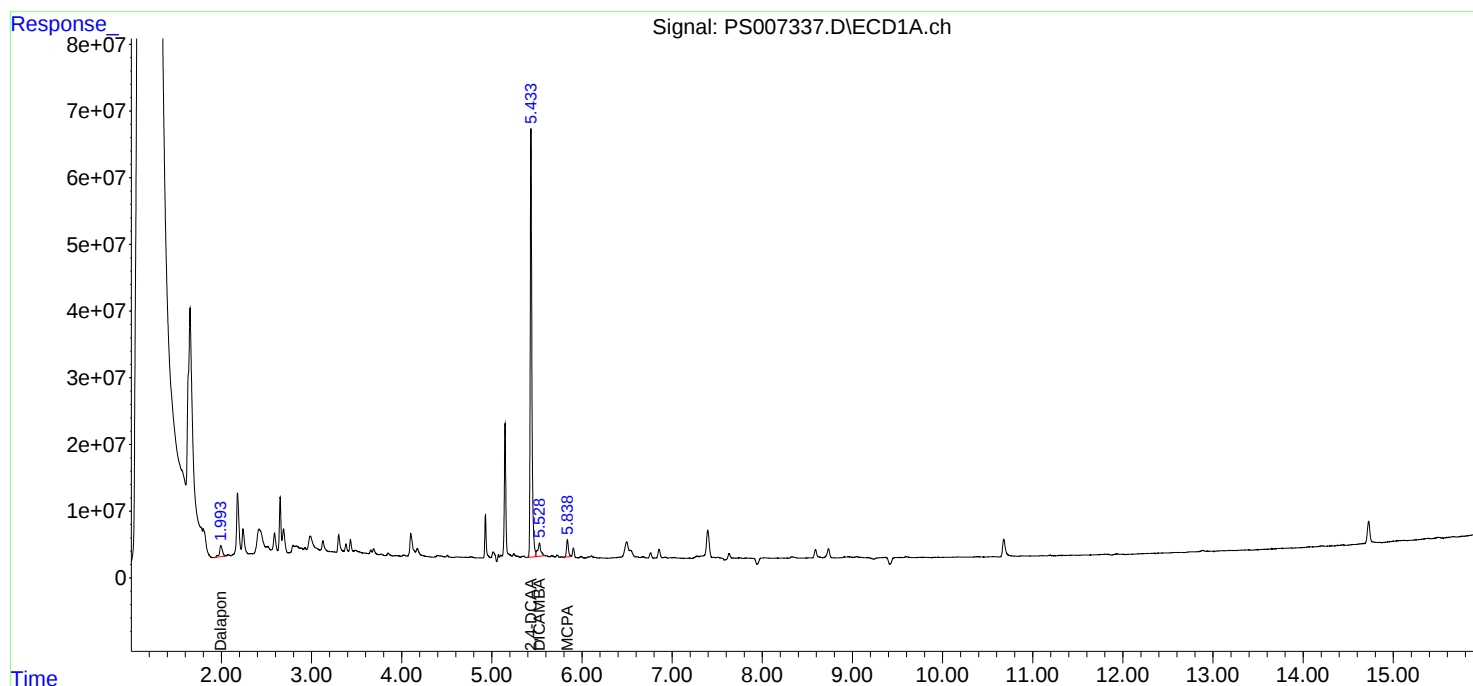


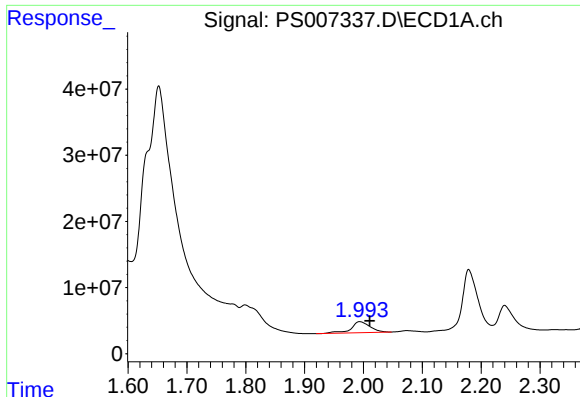

#1 Dalapon


R.T.: 1.994 min
Delta R.T.: -0.017 min
Response: 37225065
Conc: 22.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

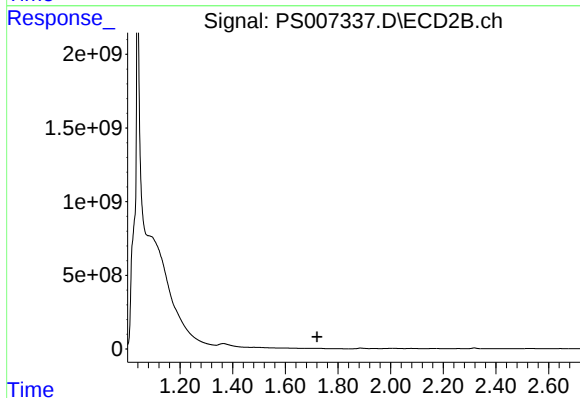


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.721 min
Response: 0
Conc: N.D.

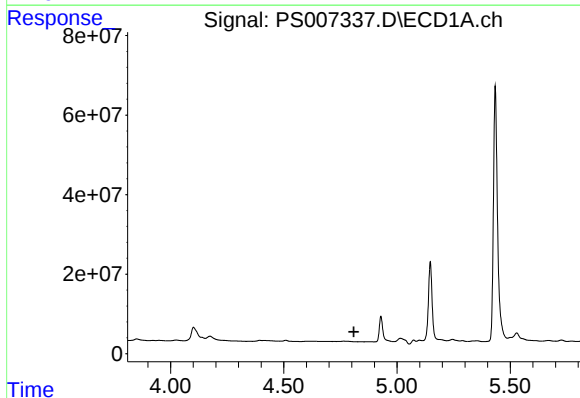


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

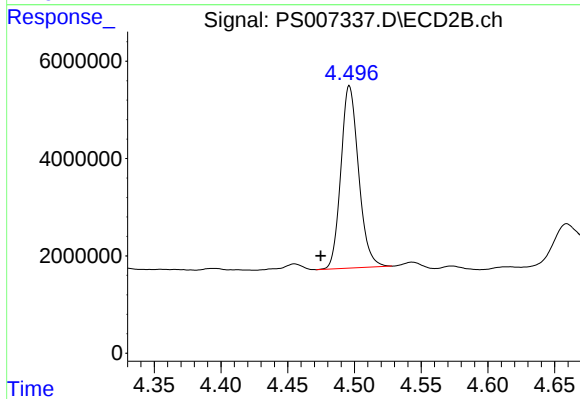

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.497 min
Delta R.T.: 0.022 min
Response: 34555058
Conc: 40.16 ng/ml

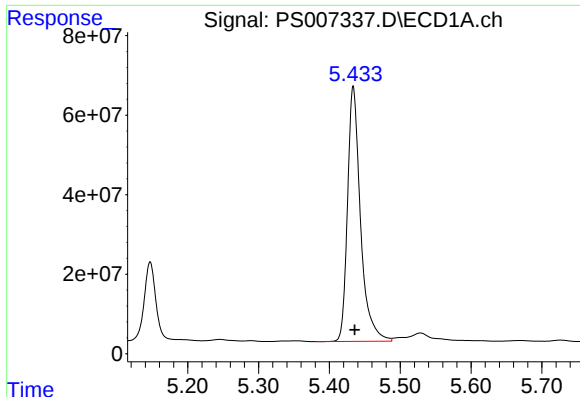

#4 2,4-DCAA


R.T.: 5.434 min
Delta R.T.: -0.002 min
Response: 816641628
Conc: 596.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

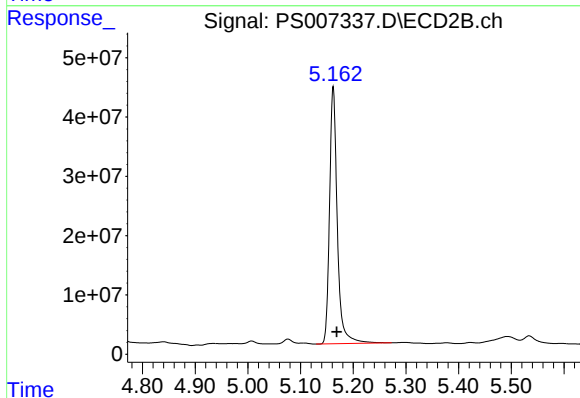


#4 2,4-DCAA

R.T.: 5.162 min
Delta R.T.: -0.006 min
Response: 444422657
Conc: 631.90 ng/ml

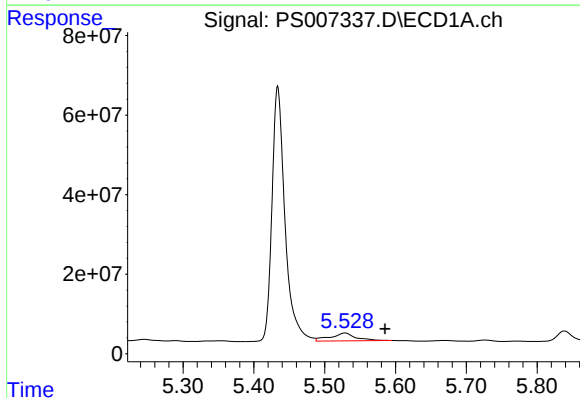


#5 DICAMBA

R.T.: 5.528 min
Delta R.T.: -0.057 min
Response: 49297947
Conc: 10.03 ng/ml

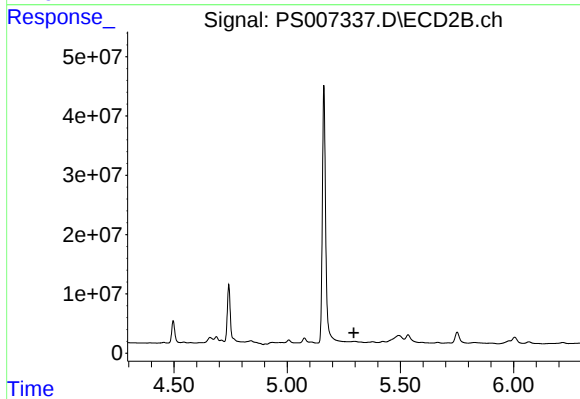

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

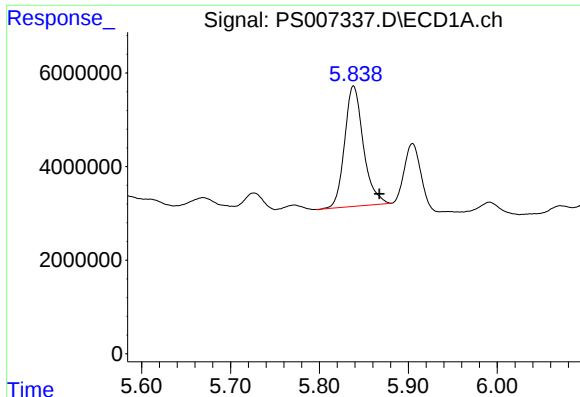

#7 MCPA


R.T.: 5.838 min
Delta R.T.: -0.029 min
Response: 37684503
Conc: 7.31 ug/ml

Instrument :
ECD_S
ClientSampleId :

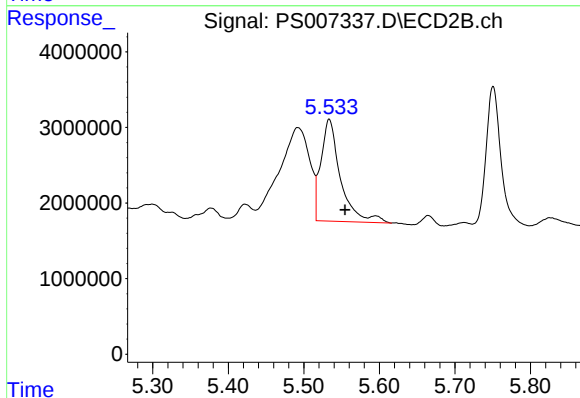


#7 MCPA

R.T.: 5.534 min
Delta R.T.: -0.021 min
Response: 24273309
Conc: 8.35 ug/ml

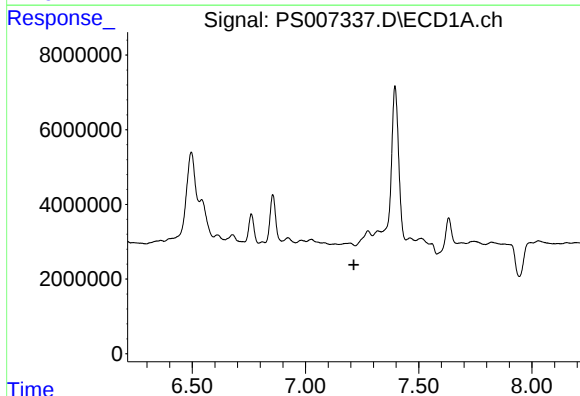


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.214 min
Response: 0
Conc: N.D.

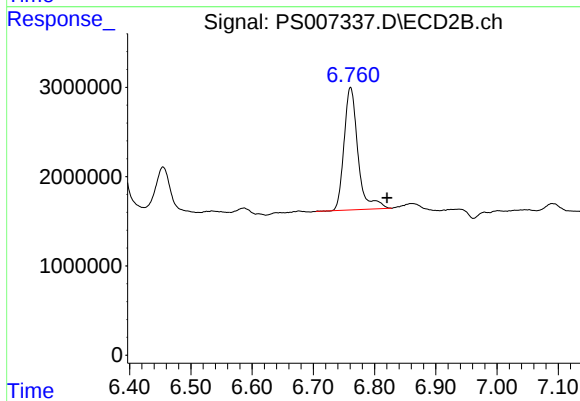

#11 2,4,5-TP (SILVEX)


R.T.: 6.761 min
Delta R.T.: -0.060 min
Response: 21601684
Conc: 5.68 ng/ml

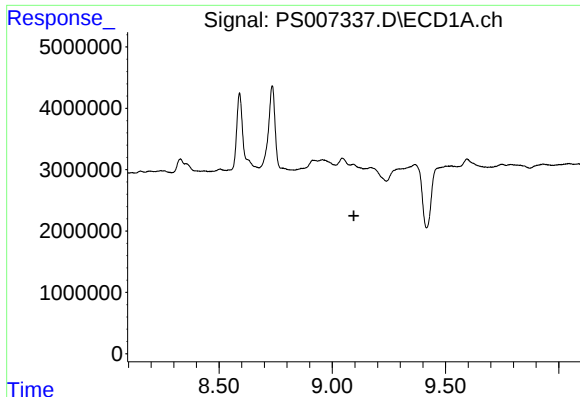

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

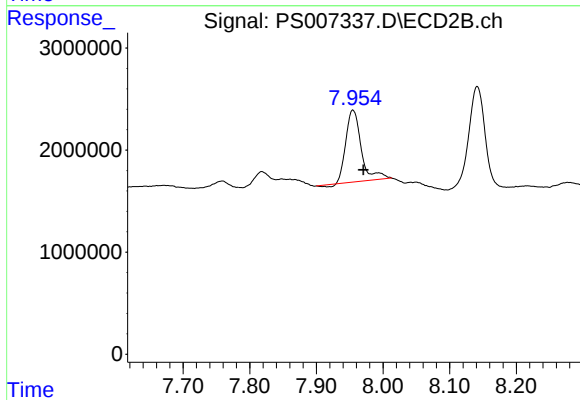


#14 DINOSEB

R.T.: 7.955 min
Delta R.T.: -0.016 min
Response: 11156734
Conc: 3.97 ng/ml

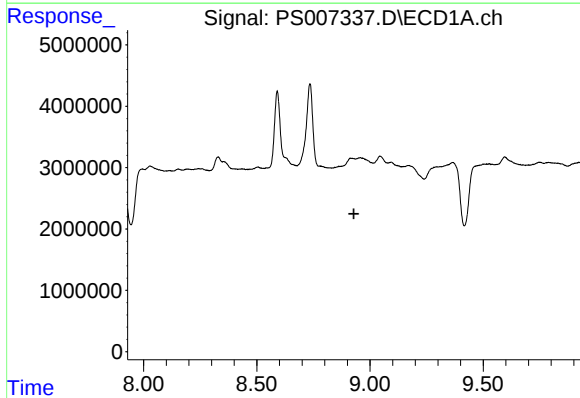


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

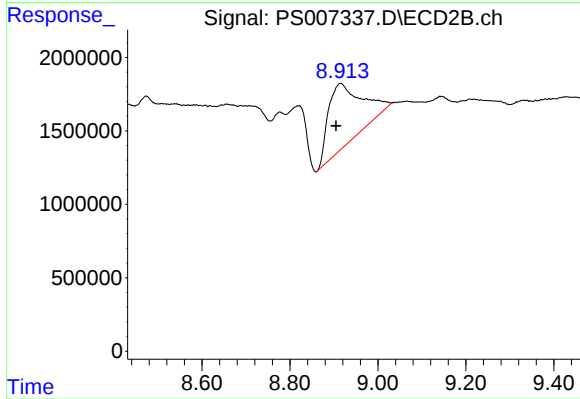

#15 Picloram


R.T.: 8.915 min
Delta R.T.: 0.010 min
Response: 22730032
Conc: 3.70 ng/ml

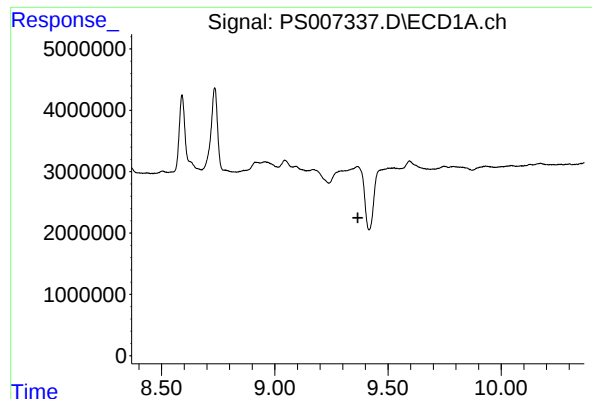

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

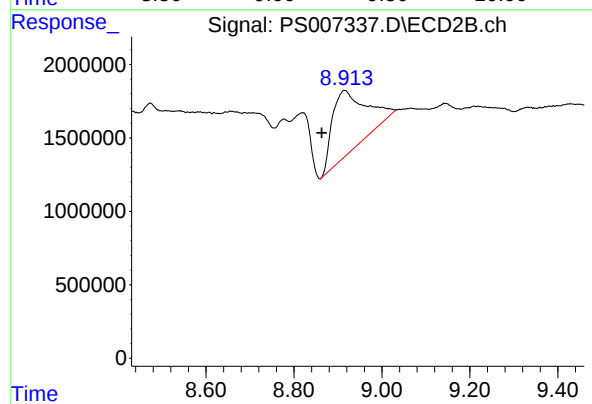

#16 DCPA

R.T.: 8.915 min
Delta R.T.: 0.052 min
Response: 22730032
Conc: 4.53 ng/ml