

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
 Data File : PS007363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2019 21:16
 Operator : SM\AJ
 Sample : K5501-17
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 22:51:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.433	5.160	421.9E6	208.0E6	308.240	295.677
Target Compounds							
1) T	Dalapon	1.992	1.657	60008542	196.1E6	35.863	215.440 #
2) T	3,5-DICHL...	0.000	4.494	0	26139156	N.D.	30.379
5) T	DICAMBA	5.528	5.297	50626151	13291977	10.304	5.108 #
7) T	MCPA	5.904	5.531	26920397	27359076	5.219	9.411 #
9) T	2,4-D	6.486	6.065	15528006	8993838	12.600	11.273
10) T	Pentachlo...	0.000	6.453	0	13234642	N.D.	1.376
11) T	2,4,5-TP ...	0.000	6.759	0	14766110	N.D.	3.882
14) T	DINOSEB	0.000	7.953	0	27748972	N.D.	9.884
15) T	Picloram	0.000	8.923	0	28903724	N.D.	4.707
16) T	DCPA	0.000	8.923	0	28903724	N.D.	5.764



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
Data File : PS007363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2019 21:16
Operator : SM\AJ
Sample : K5501-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 22:51:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

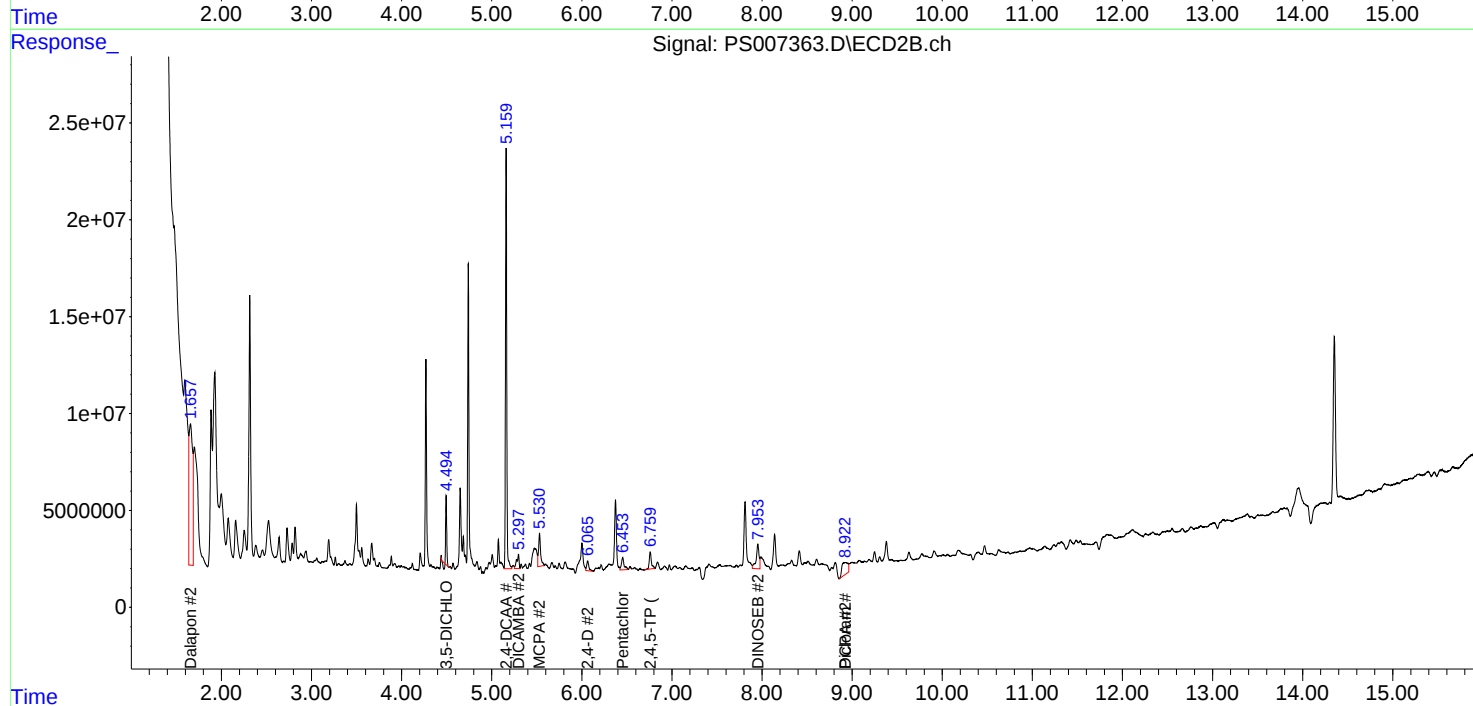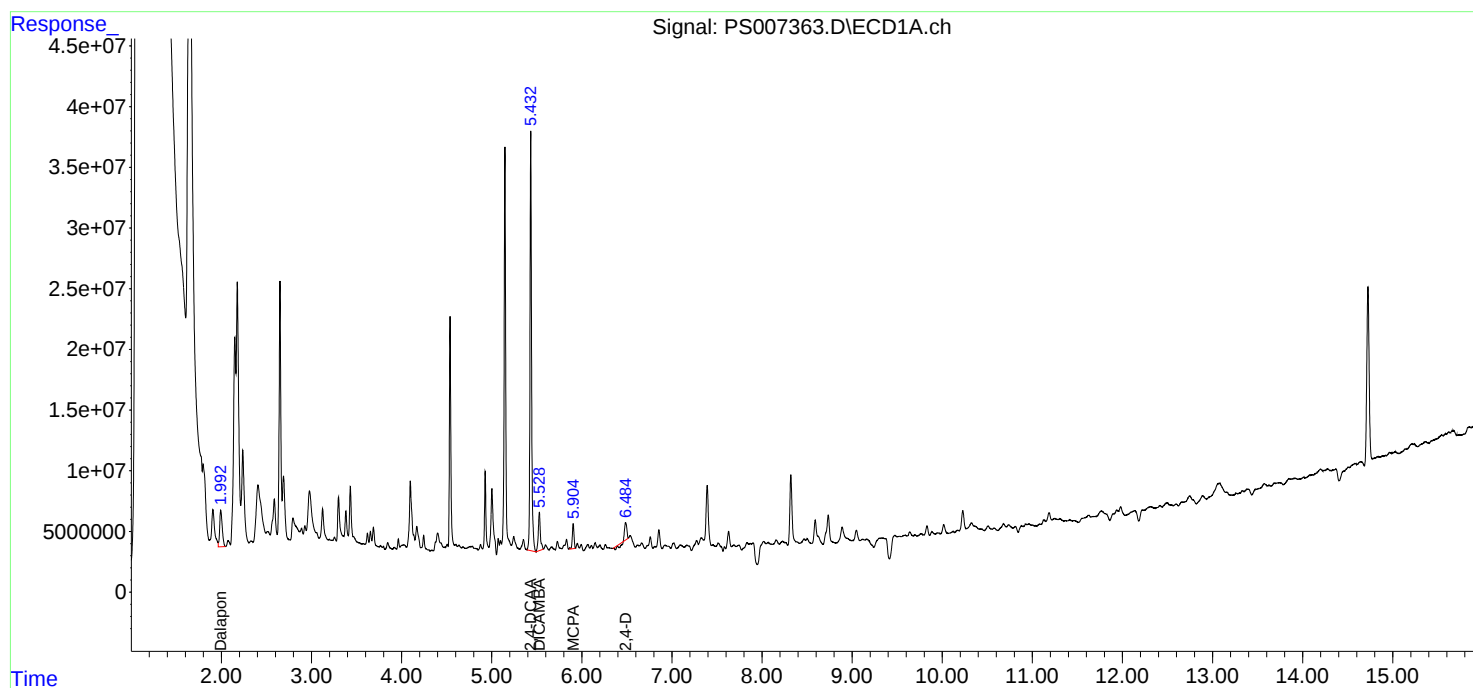


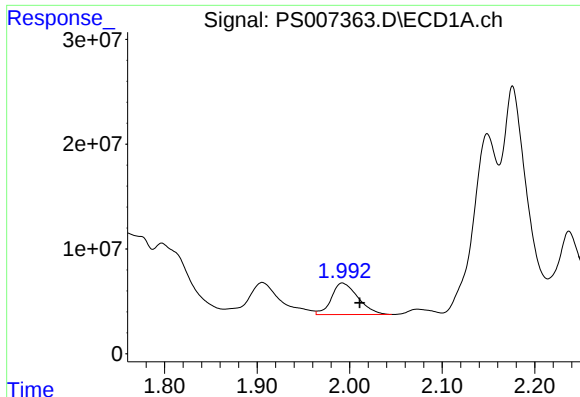

#1 Dalapon


R.T.: 1.992 min
Delta R.T.: -0.019 min
Response: 60008542
Conc: 35.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

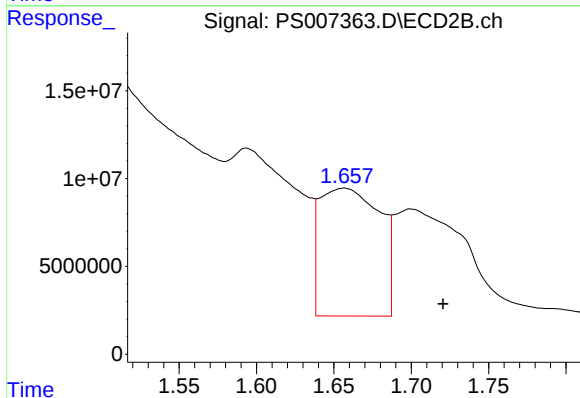


#1 Dalapon

R.T.: 1.657 min
Delta R.T.: -0.064 min
Response: 196050987
Conc: 215.44 ng/ml

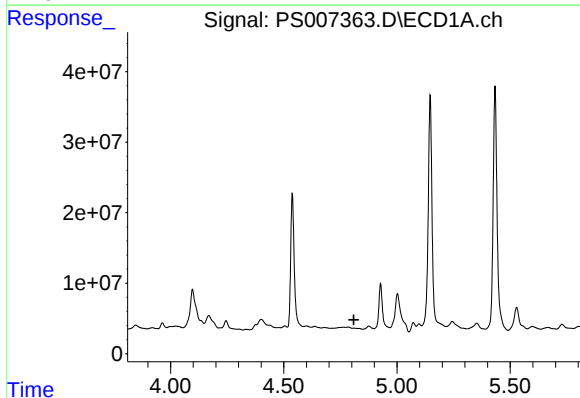


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

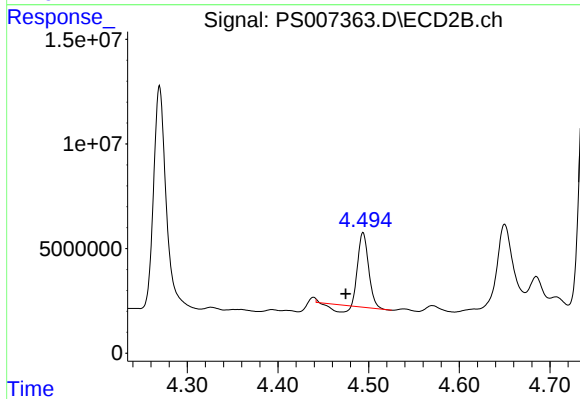

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.494 min
Delta R.T.: 0.019 min
Response: 26139156
Conc: 30.38 ng/ml

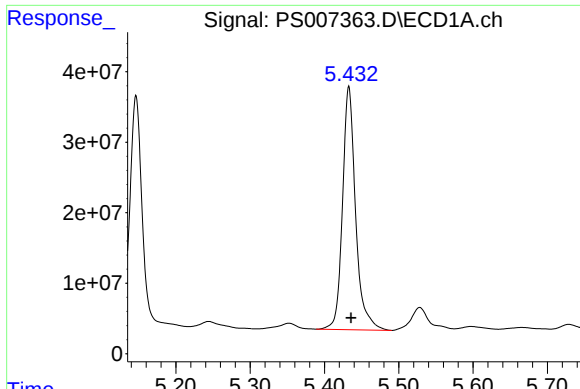

#4 2,4-DCAA


R.T.: 5.433 min
Delta R.T.: -0.003 min
Response: 421878880
Conc: 308.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

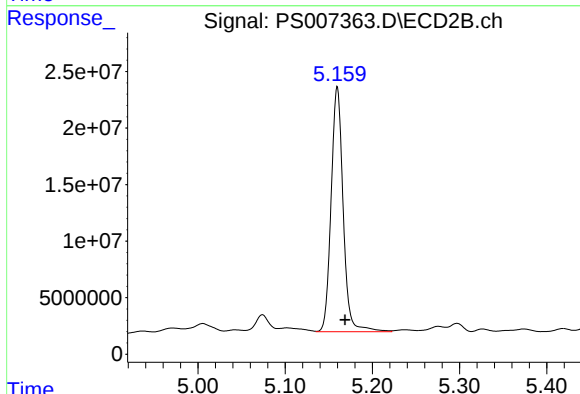


#4 2,4-DCAA

R.T.: 5.160 min
Delta R.T.: -0.009 min
Response: 207951915
Conc: 295.68 ng/ml

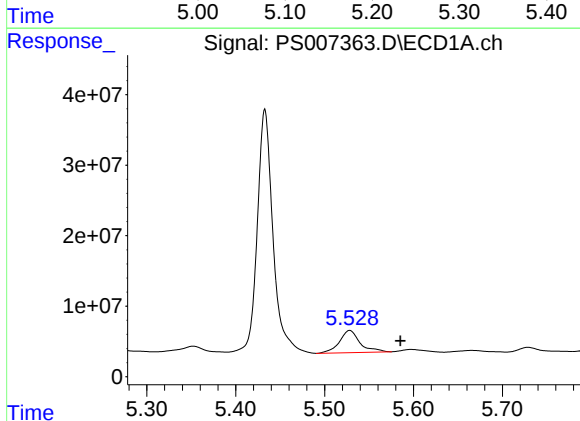


#5 DICAMBA

R.T.: 5.528 min
Delta R.T.: -0.057 min
Response: 50626151
Conc: 10.30 ng/ml

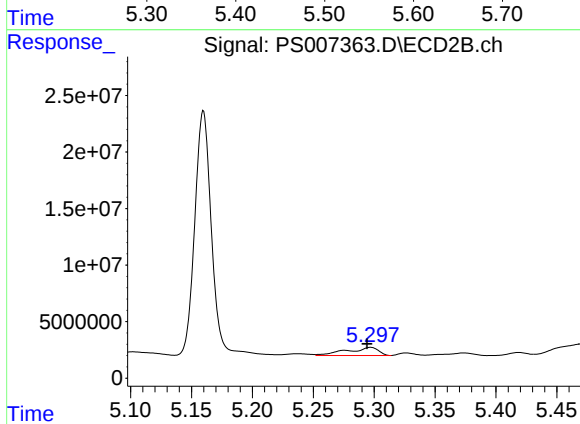

#5 DICAMBA


R.T.: 5.297 min
Delta R.T.: 0.003 min
Response: 13291977
Conc: 5.11 ng/ml

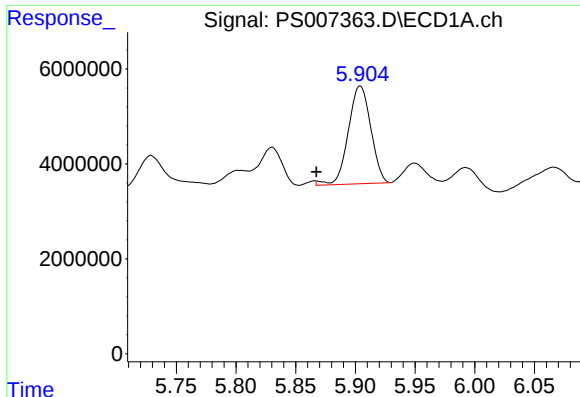

#7 MCPA


R.T.: 5.904 min
Delta R.T.: 0.037 min
Response: 26920397
Conc: 5.22 ug/ml

Instrument :
ECD_S
ClientSampleId :

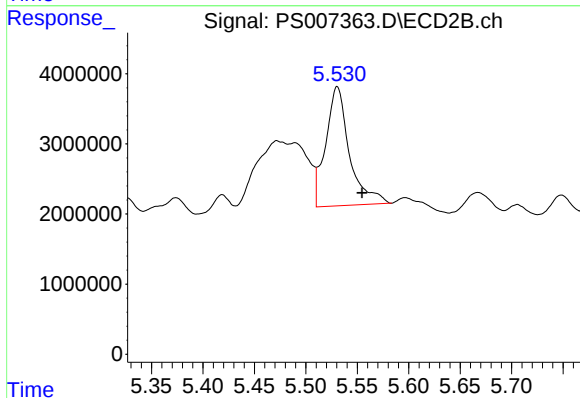


#7 MCPA

R.T.: 5.531 min
Delta R.T.: -0.024 min
Response: 27359076
Conc: 9.41 ug/ml

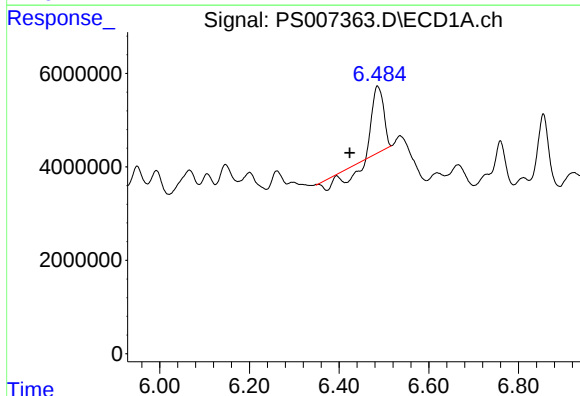


#9 2,4-D

R.T.: 6.486 min
Delta R.T.: 0.062 min
Response: 15528006
Conc: 12.60 ng/ml

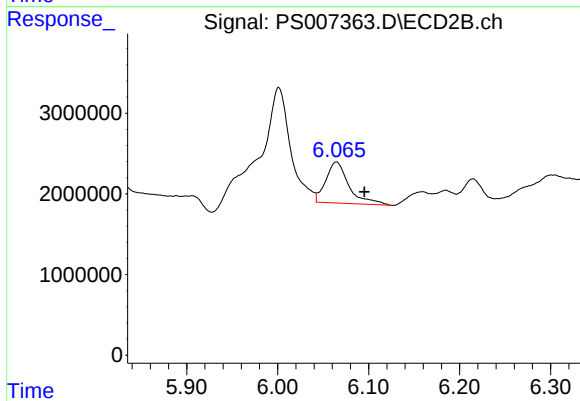

#9 2,4-D


R.T.: 6.065 min
Delta R.T.: -0.031 min
Response: 8993838
Conc: 11.27 ng/ml

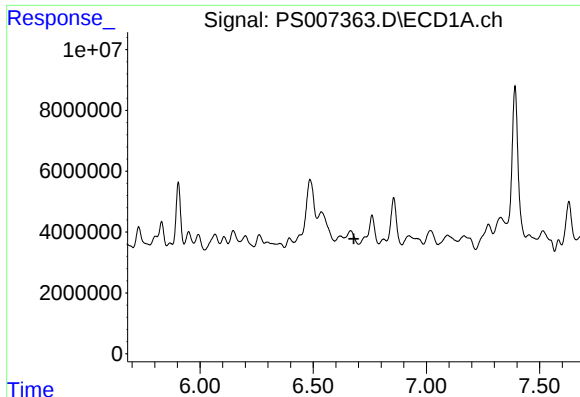

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

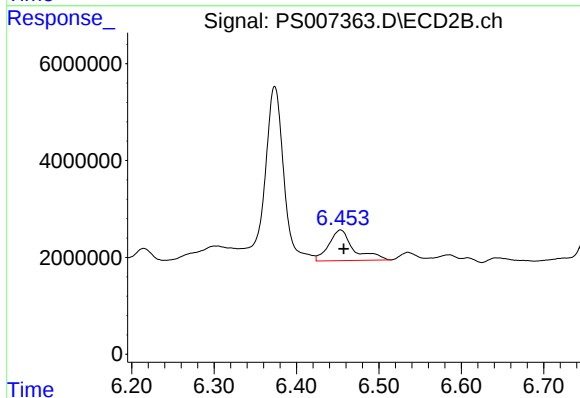


#10 Pentachlorophenol

R.T.: 6.453 min
Delta R.T.: -0.004 min
Response: 13234642
Conc: 1.38 ng/ml

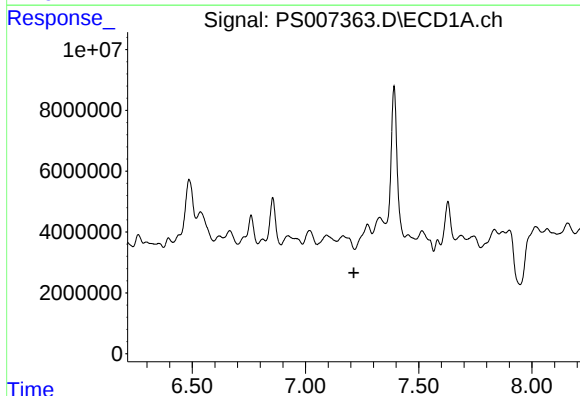


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

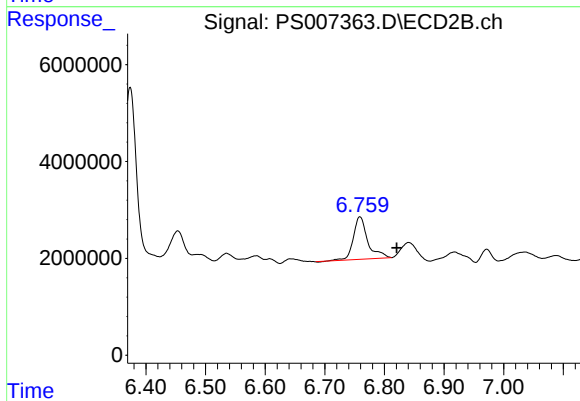

#11 2,4,5-TP (SILVEX)


R.T.: 6.759 min
Delta R.T.: -0.062 min
Response: 14766110
Conc: 3.88 ng/ml

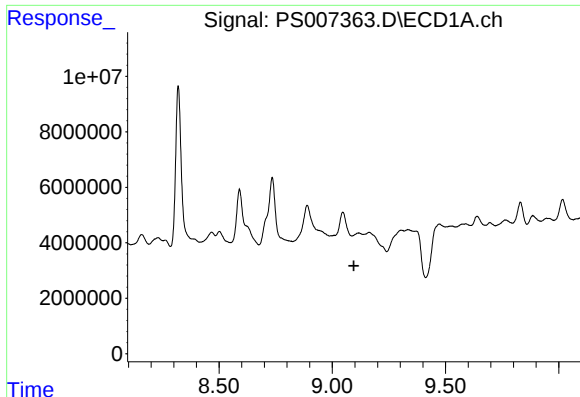

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

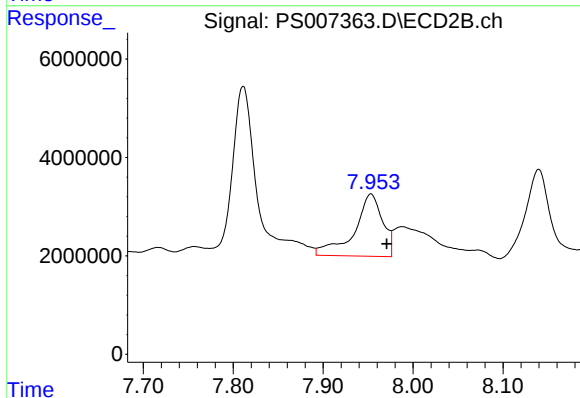


#14 DINOSEB

R.T.: 7.953 min
Delta R.T.: -0.018 min
Response: 27748972
Conc: 9.88 ng/ml

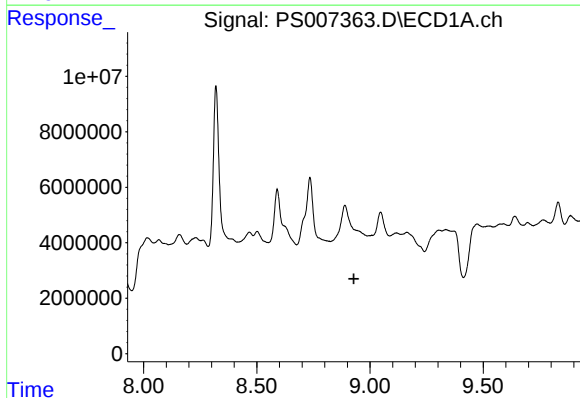


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

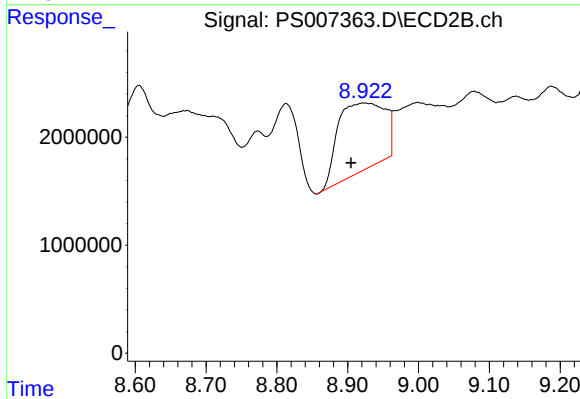

#15 Picloram


R.T.: 8.923 min
Delta R.T.: 0.018 min
Response: 28903724
Conc: 4.71 ng/ml

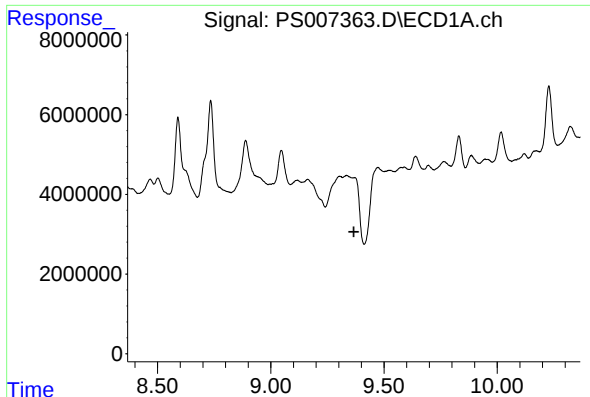

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

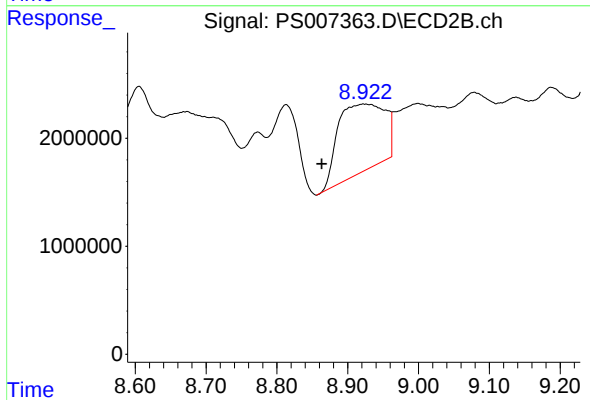

#16 DCPA

R.T.: 8.923 min
Delta R.T.: 0.060 min
Response: 28903724
Conc: 5.76 ng/ml