

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
 Data File : PS007367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2019 22:44
 Operator : SM\AJ
 Sample : PB124311BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 01:15:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.449	5.177	1005.0E6	562.4E6	734.258	799.680
Target Compounds							
1) T	Dalapon	2.010	1.720	85488335	94748096	51.090	104.118 #
2) T	3,5-DICHL...	0.000	4.455	0	7159007	N.D.	8.320
3) T	4-Nitroph...	0.000	4.855	0	21539374	N.D.	54.545
5) T	DICAMBA	5.544	0.000	44065510	0	8.968	N.D. #
7) T	MCPA	0.000	5.495	0	49222060	N.D.	16.932
10) T	Pentachlo...	0.000	6.472	0	7691589	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.776	0	50242945	N.D.	13.209
12) T	2,4,5-T	7.417	0.000	138.0E6	0	18.054	N.D. #
14) T	DINOSEB	0.000	7.971	0	6507621	N.D.	2.318
15) T	Picloram	0.000	8.925	0	13075376	N.D.	2.129
16) T	DCPA	0.000	8.925	0	13075376	N.D.	2.607



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
Data File : PS007367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2019 22:44
Operator : SM\AJ
Sample : PB124311BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 01:15:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

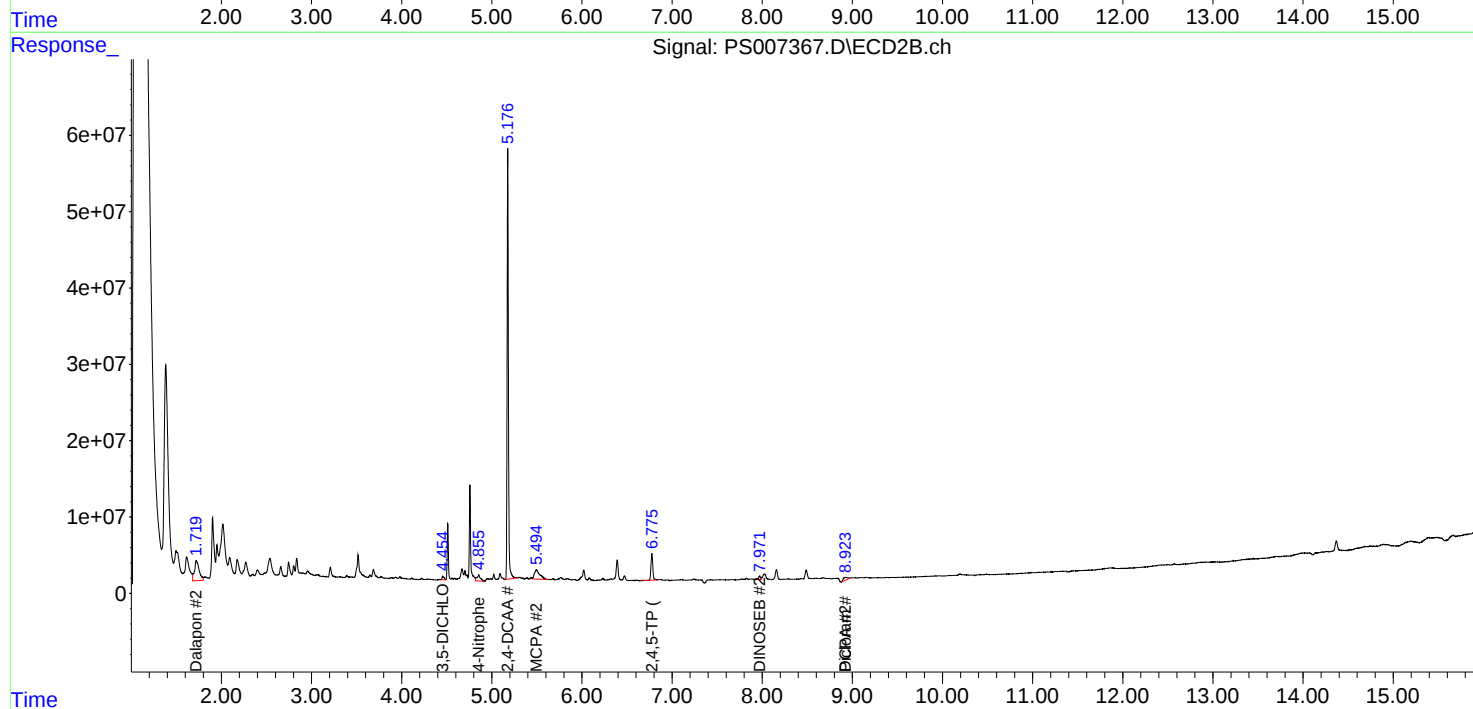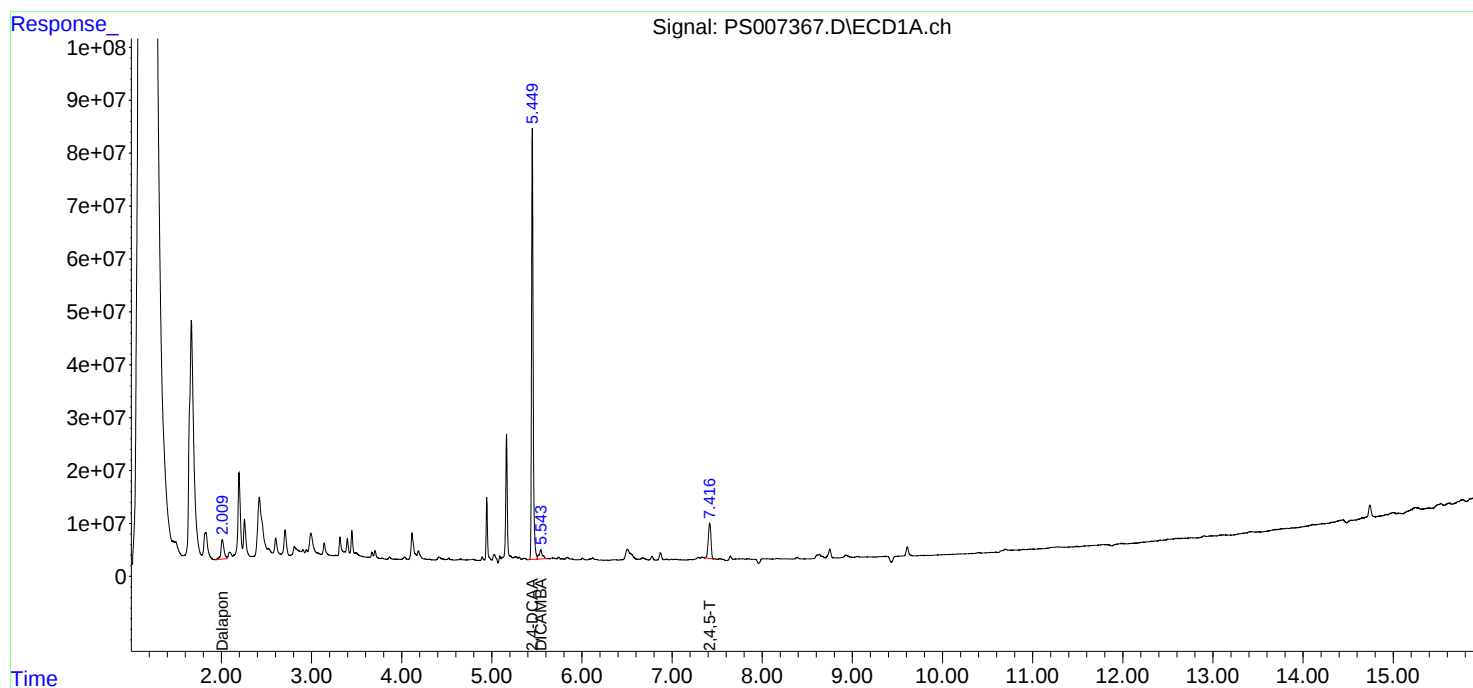


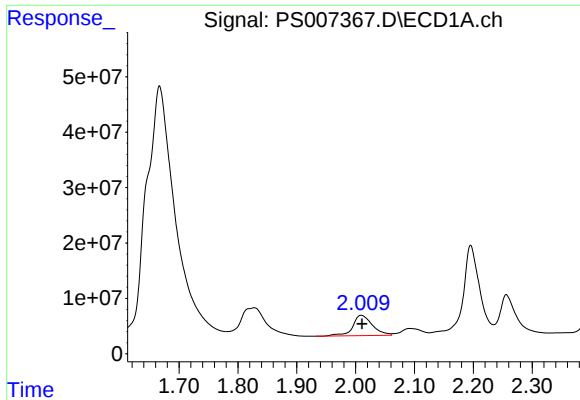

#1 Dalapon


R.T.: 2.010 min
Delta R.T.: -0.001 min
Response: 85488335
Conc: 51.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

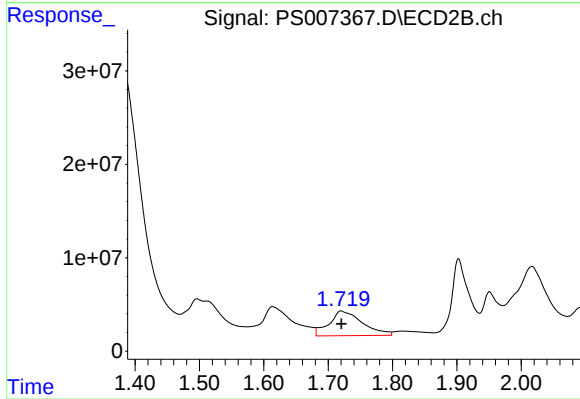


#1 Dalapon

R.T.: 1.720 min
Delta R.T.: 0.000 min
Response: 94748096
Conc: 104.12 ng/ml

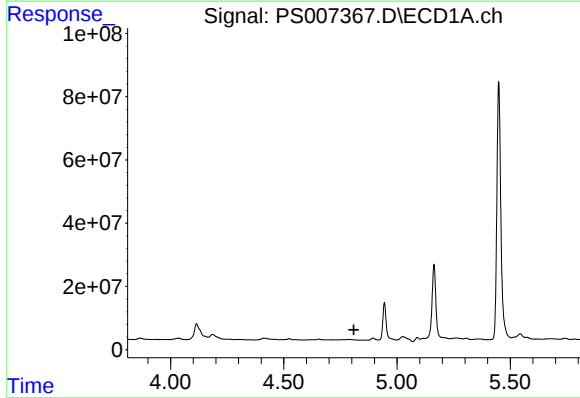


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

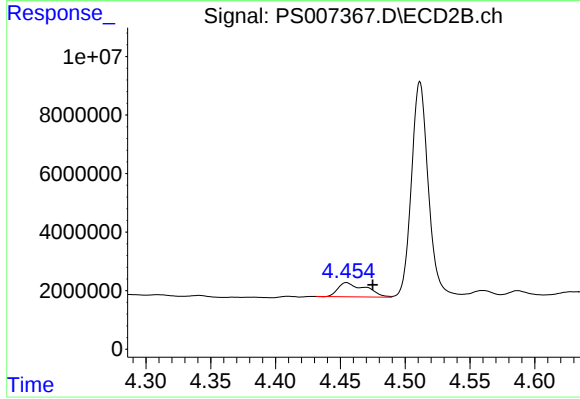

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.455 min
Delta R.T.: -0.020 min
Response: 7159007
Conc: 8.32 ng/ml

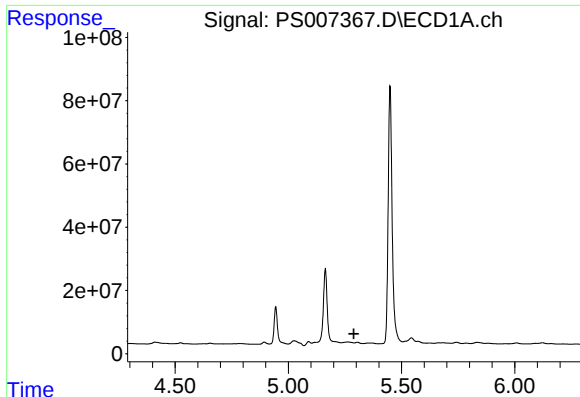

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

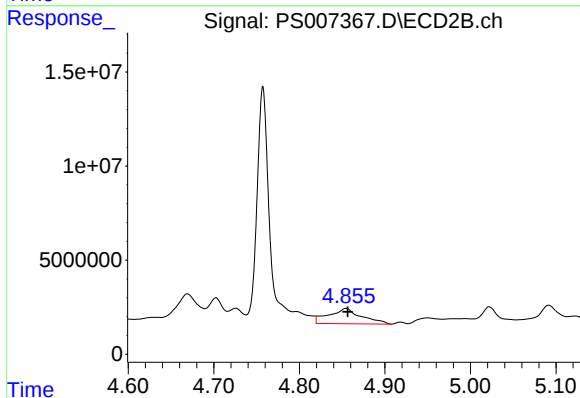


#3 4-Nitrophenol

R.T.: 4.855 min
Delta R.T.: -0.002 min
Response: 21539374
Conc: 54.54 ng/ml

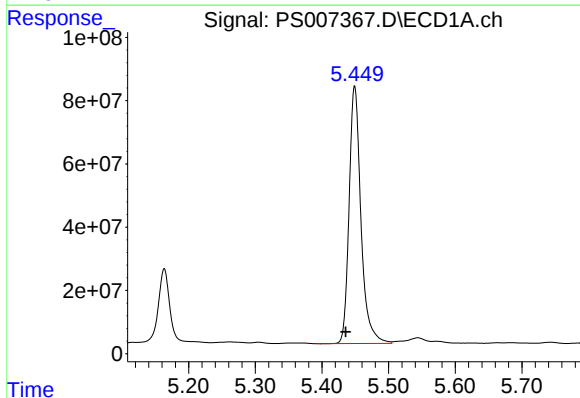


#4 2,4-DCAA

R.T.: 5.449 min
Delta R.T.: 0.014 min
Response: 1004956304
Conc: 734.26 ng/ml

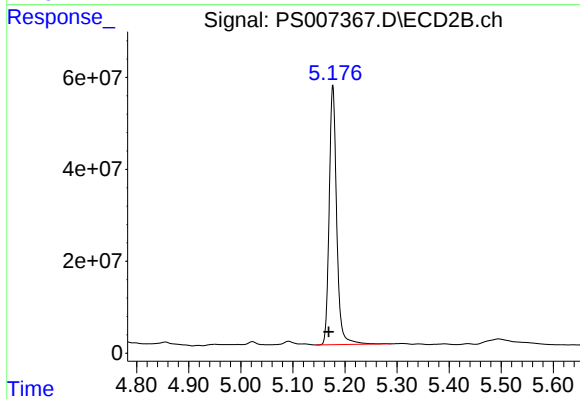

#4 2,4-DCAA


R.T.: 5.177 min
Delta R.T.: 0.008 min
Response: 562420408
Conc: 799.68 ng/ml

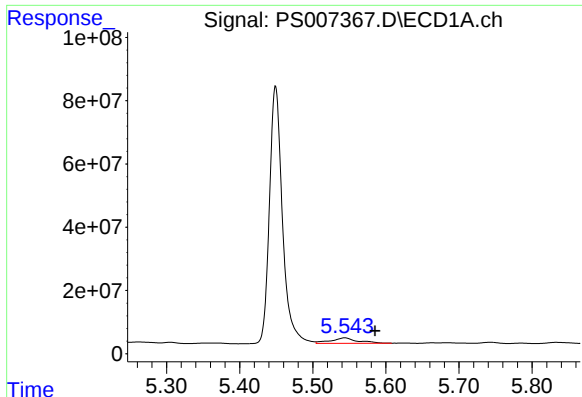

#5 DICAMBA


R.T.: 5.544 min
Delta R.T.: -0.042 min
Response: 44065510
Conc: 8.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

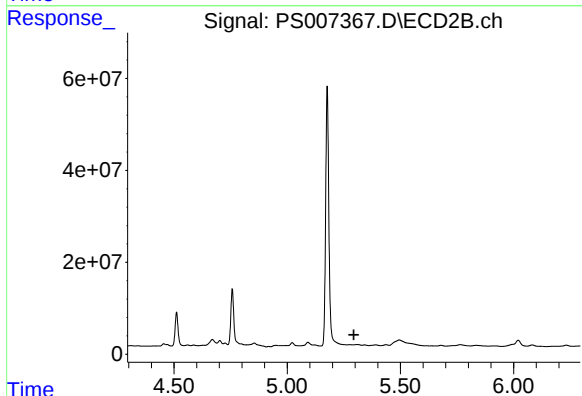


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

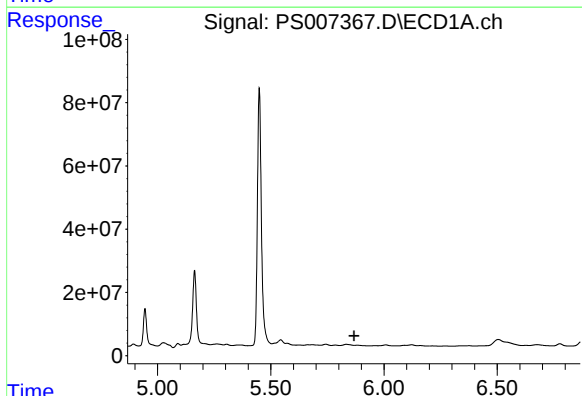


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

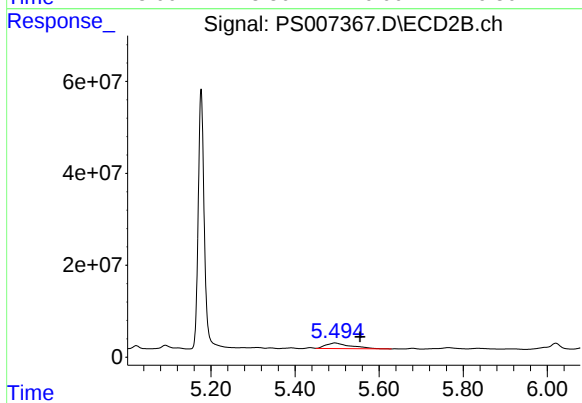

#7 MCPA


R.T.: 5.495 min
Delta R.T.: -0.060 min
Response: 49222060
Conc: 16.93 ug/ml

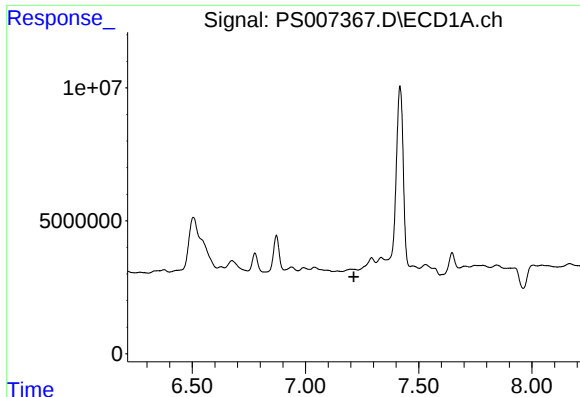

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

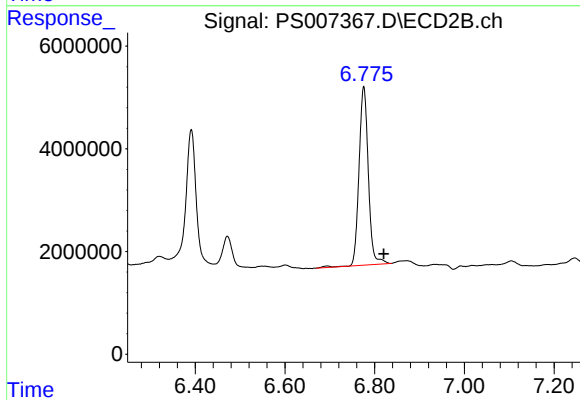


#11 2,4,5-TP (SILVEX)

R.T.: 6.776 min
Delta R.T.: -0.045 min
Response: 50242945
Conc: 13.21 ng/ml

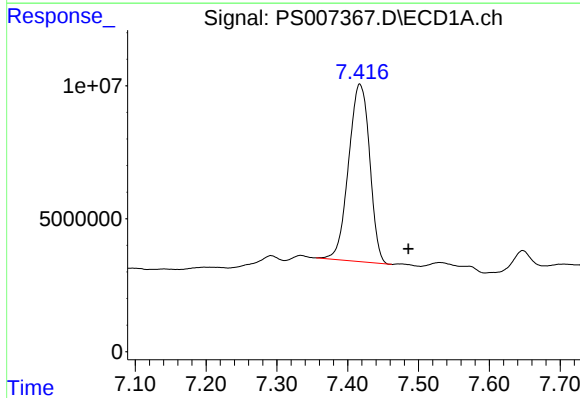


#12 2,4,5-T

R.T.: 7.417 min
Delta R.T.: -0.068 min
Response: 138019712
Conc: 18.05 ng/ml

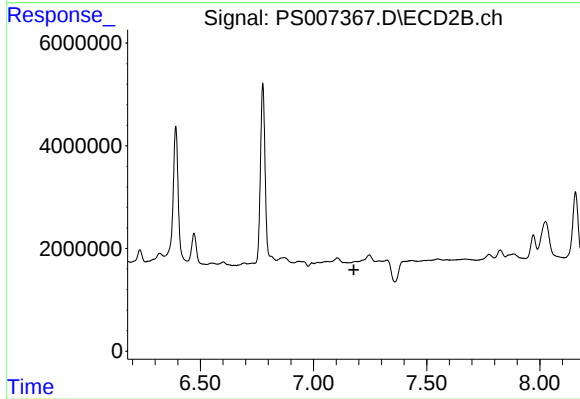

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.178 min
Response: 0
Conc: N.D.

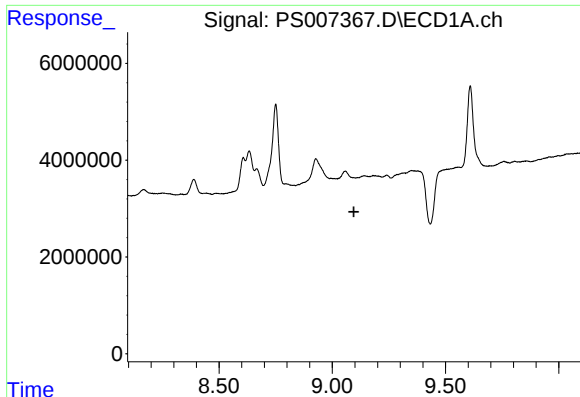

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

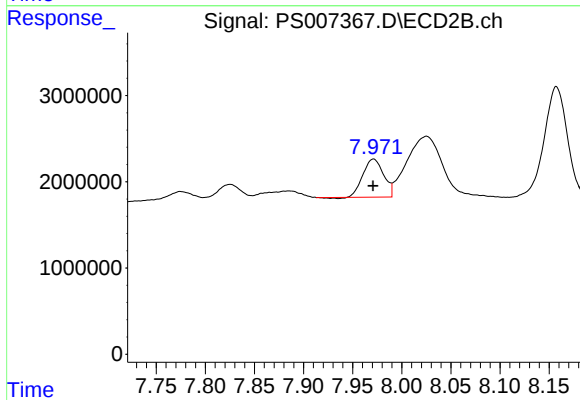


#14 DINOSEB

R.T.: 7.971 min
Delta R.T.: 0.000 min
Response: 6507621
Conc: 2.32 ng/ml

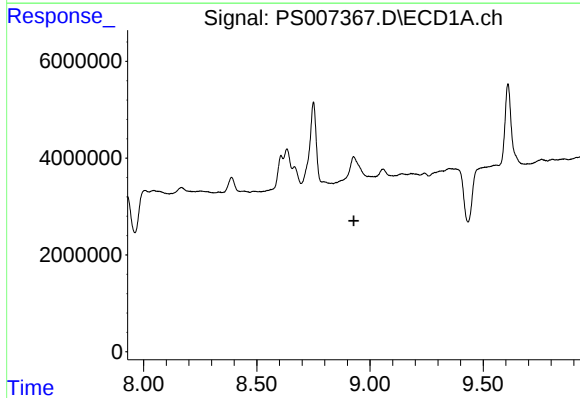


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

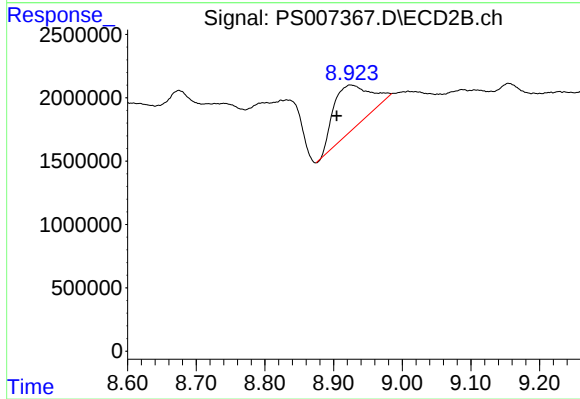

#15 Picloram


R.T.: 8.925 min
Delta R.T.: 0.021 min
Response: 13075376
Conc: 2.13 ng/ml

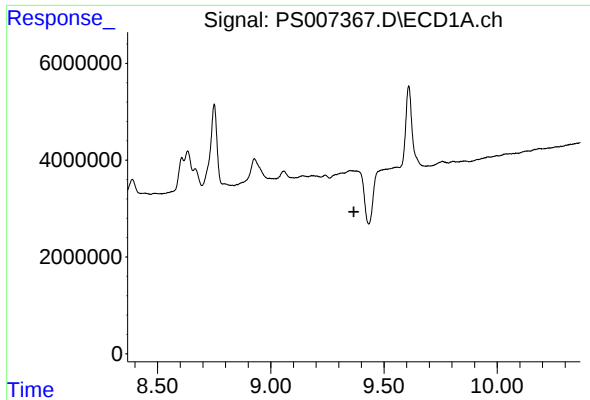

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

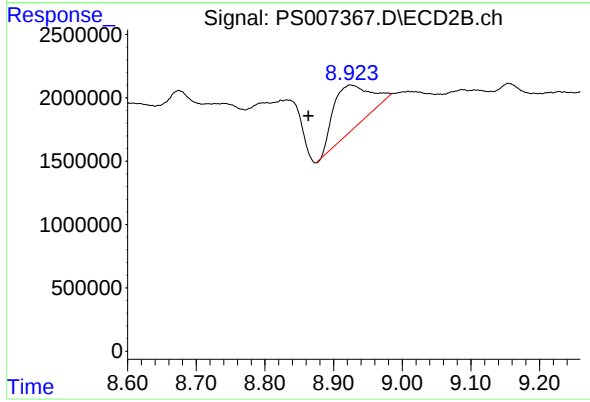

#16 DCPA

R.T.: 8.925 min
Delta R.T.: 0.062 min
Response: 13075376
Conc: 2.61 ng/ml