

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
 Data File : PS007370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2019 23:49
 Operator : SM\AJ
 Sample : K5494-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 01:16:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.449	5.176	1252.6E6	661.8E6	915.181	940.947
Target Compounds							
1) T	Dalapon	2.009	1.720	105.8E6	107.3E6	63.199	117.958 #
2) T	3,5-DICHL...	0.000	4.511	0	57851868	N.D.	67.236
5) T	DICAMBA	5.544	0.000	43950366	0	8.945	N.D. #
7) T	MCPA	0.000	5.547	0	18905295	N.D.	6.503
10) T	Pentachlo...	0.000	6.466	0	20026885	N.D.	2.083
11) T	2,4,5-TP ...	0.000	6.775	0	40847751	N.D.	10.739
12) T	2,4,5-T	7.417	0.000	150.1E6	0	19.632	N.D. #
14) T	DINOSEB	0.000	7.972	0	5486999	N.D.	1.955
15) T	Picloram	0.000	8.923	0	3885072	N.D.	<MDL
16) T	DCPA	0.000	8.923	0	3885072	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
Data File : PS007370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2019 23:49
Operator : SM\AJ
Sample : K5494-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 01:16:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

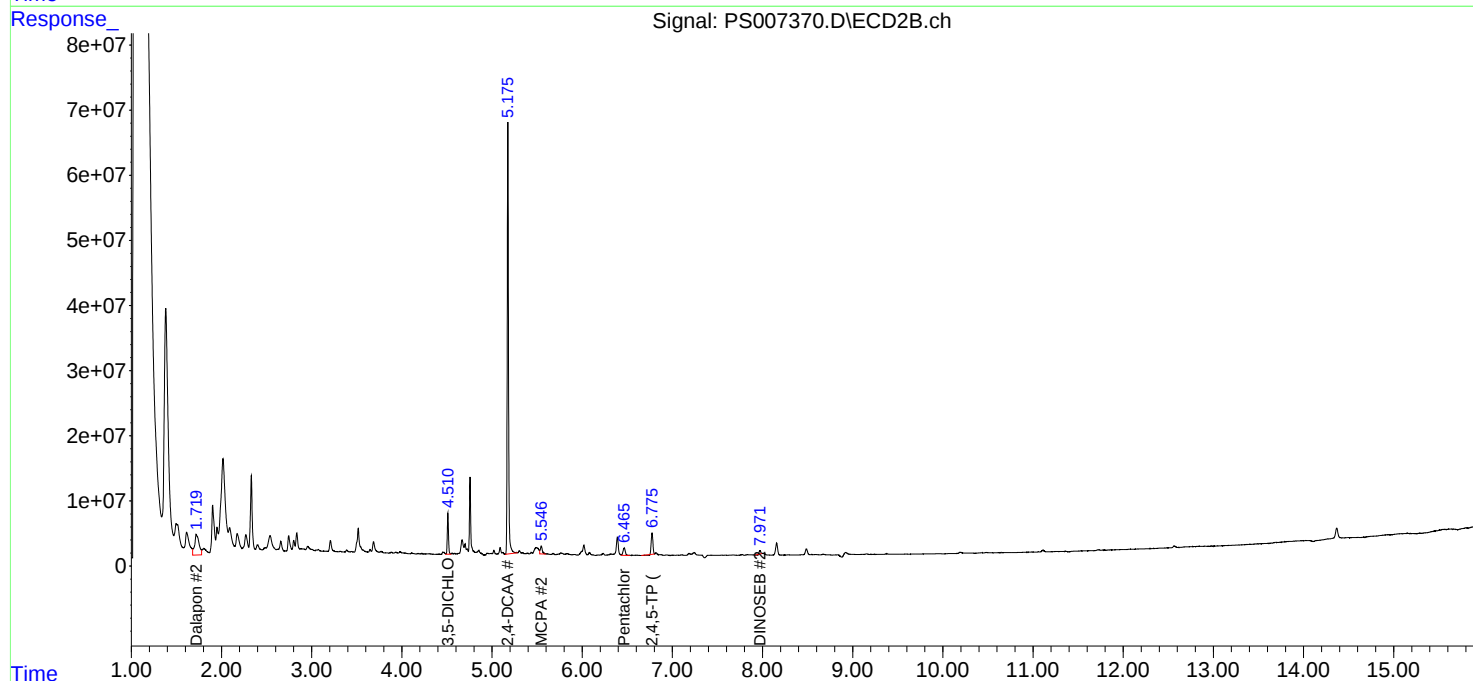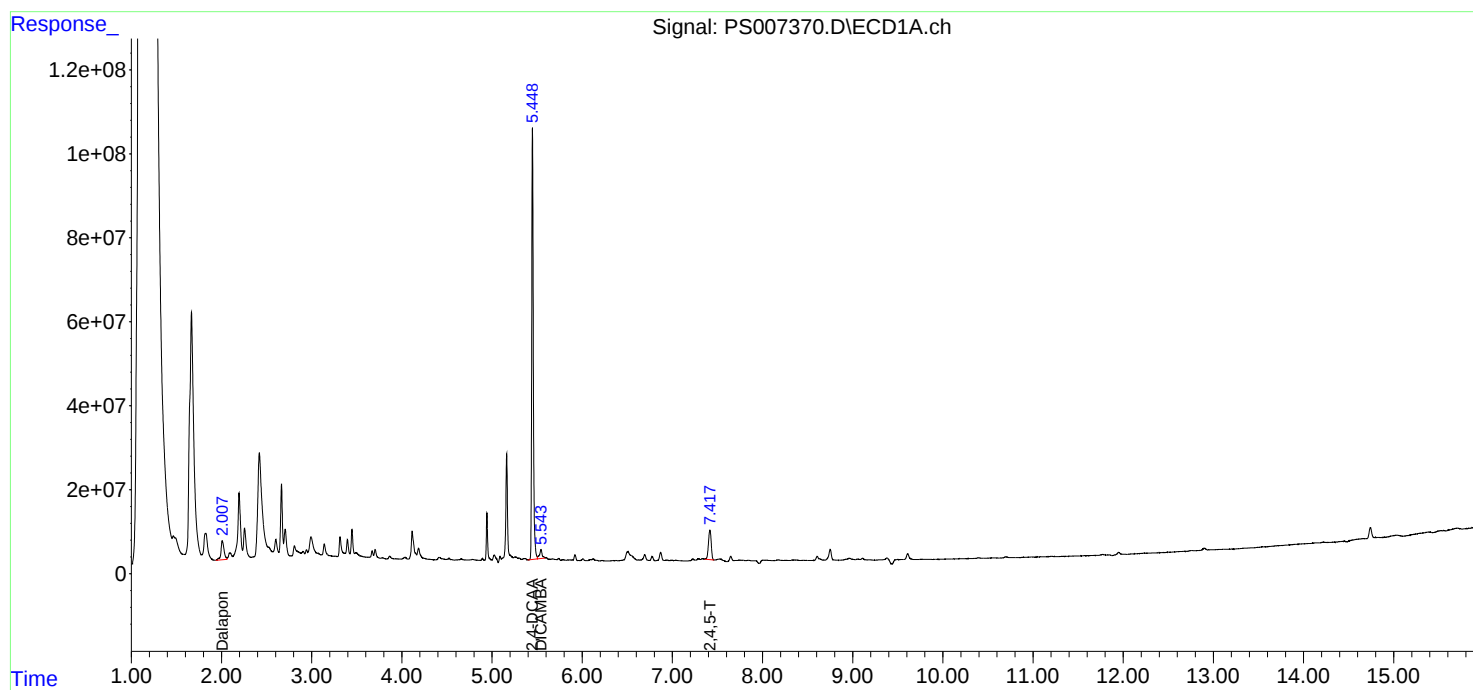


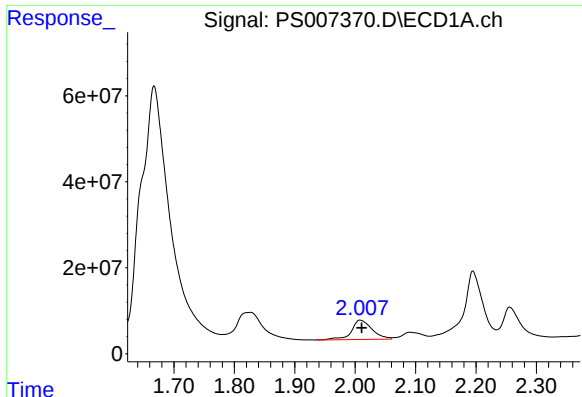

#1 Dalapon


R.T.: 2.009 min
Delta R.T.: -0.002 min
Response: 105750288
Conc: 63.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

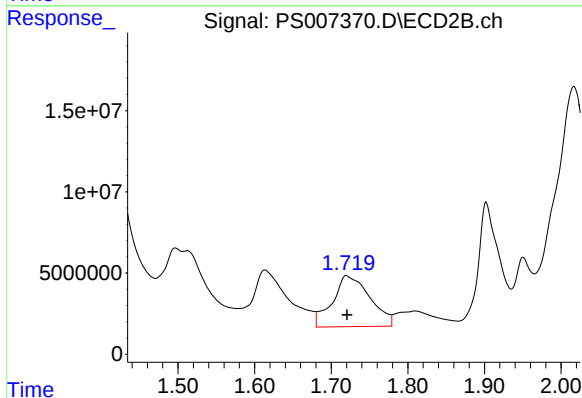


#1 Dalapon

R.T.: 1.720 min
Delta R.T.: 0.000 min
Response: 107342165
Conc: 117.96 ng/ml

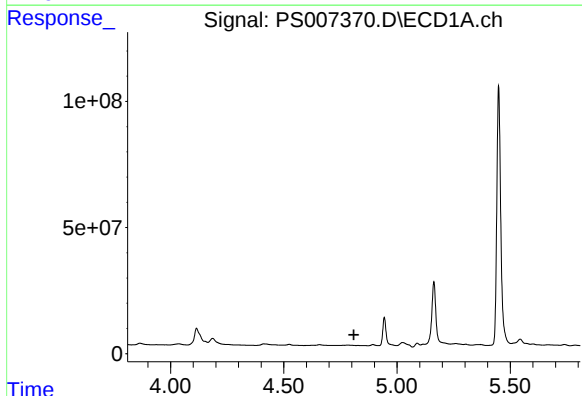


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

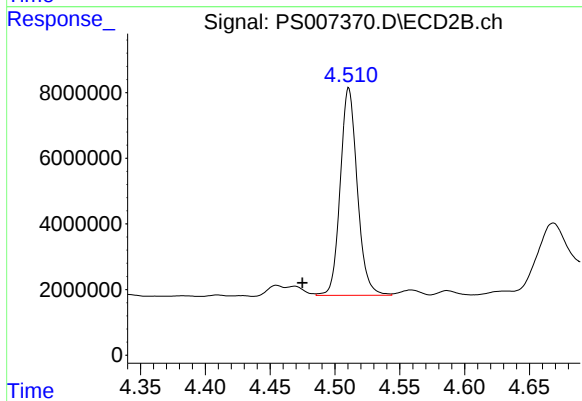

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.511 min
Delta R.T.: 0.036 min
Response: 57851868
Conc: 67.24 ng/ml

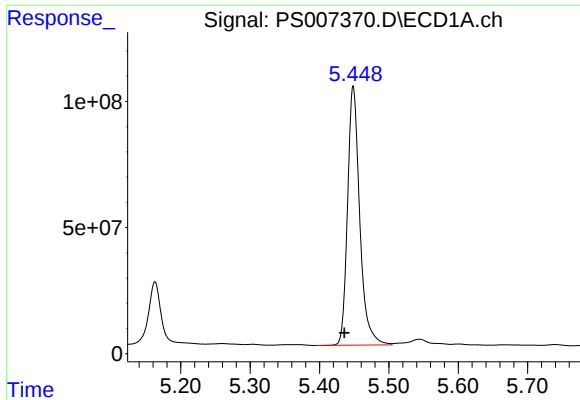

#4 2,4-DCAA


R.T.: 5.449 min
Delta R.T.: 0.013 min
Response: 1252579849
Conc: 915.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

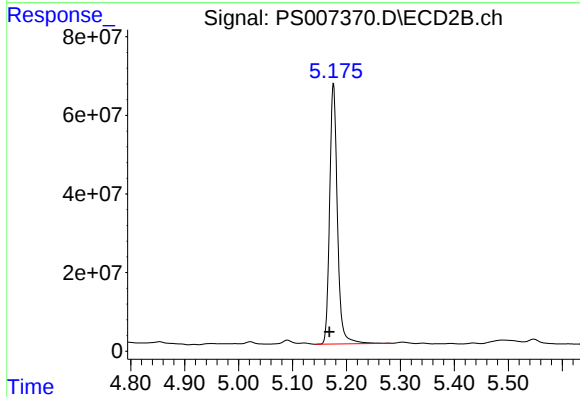


#4 2,4-DCAA

R.T.: 5.176 min
Delta R.T.: 0.007 min
Response: 661774208
Conc: 940.95 ng/ml

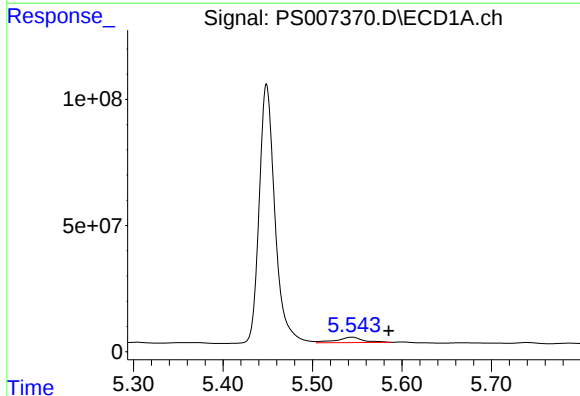


#5 DICAMBA

R.T.: 5.544 min
Delta R.T.: -0.042 min
Response: 43950366
Conc: 8.94 ng/ml

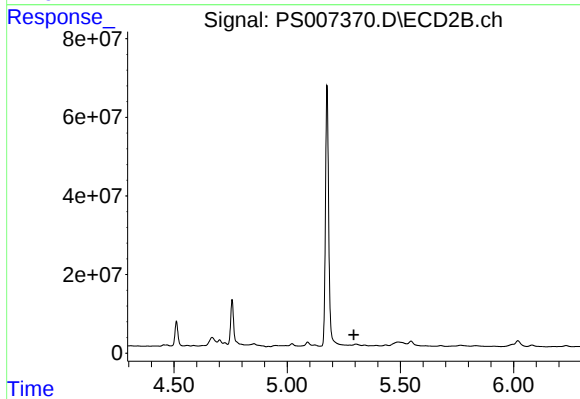

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

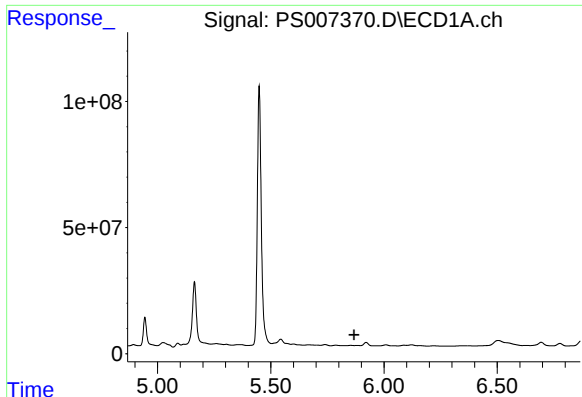

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

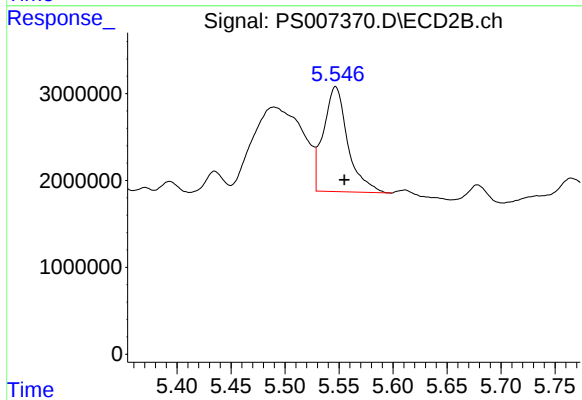


#7 MCPA

R.T.: 5.547 min
Delta R.T.: -0.008 min
Response: 18905295
Conc: 6.50 ug/ml

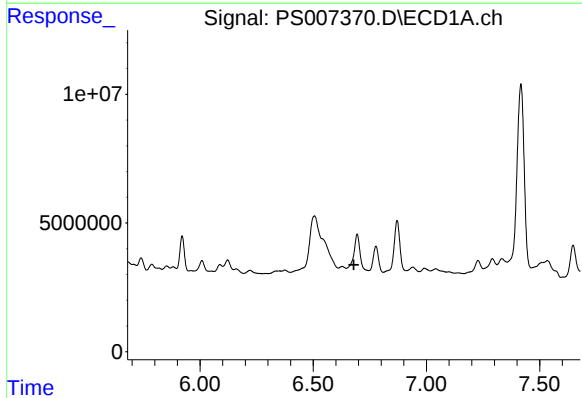


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

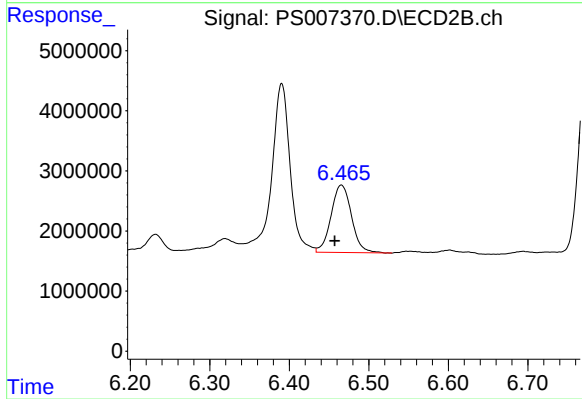

#10 Pentachlorophenol


R.T.: 6.466 min
Delta R.T.: 0.008 min
Response: 20026885
Conc: 2.08 ng/ml

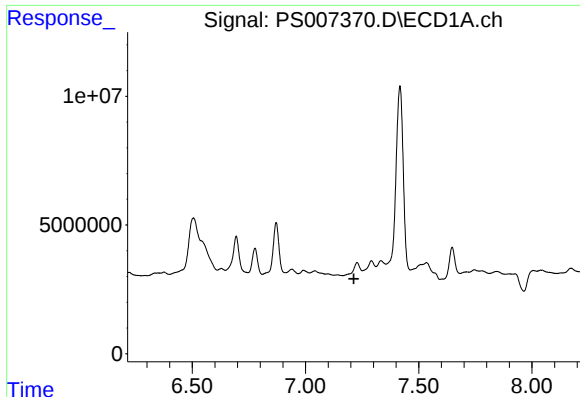

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

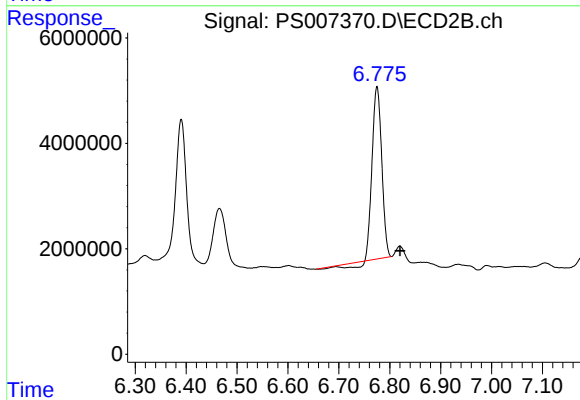


#11 2,4,5-TP (SILVEX)

R.T.: 6.775 min
Delta R.T.: -0.046 min
Response: 40847751
Conc: 10.74 ng/ml

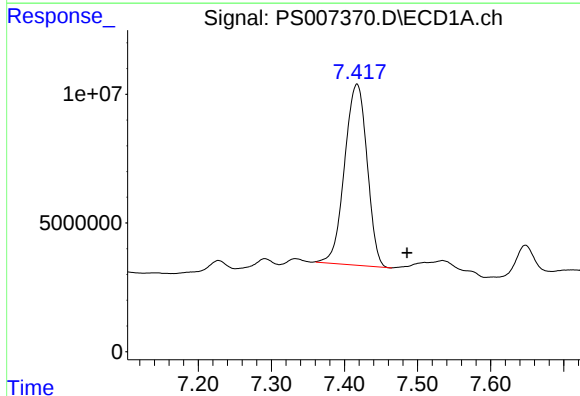


#12 2,4,5-T

R.T.: 7.417 min
Delta R.T.: -0.069 min
Response: 150083496
Conc: 19.63 ng/ml

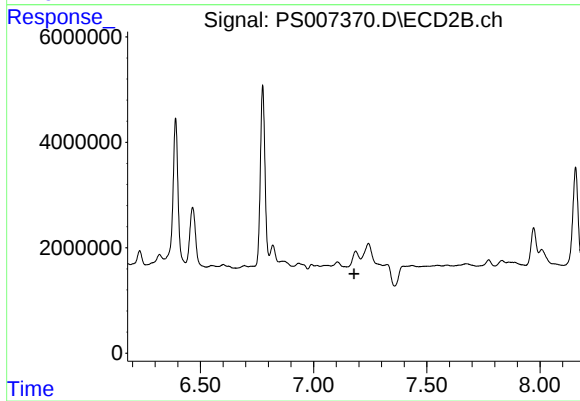

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.178 min
Response: 0
Conc: N.D.

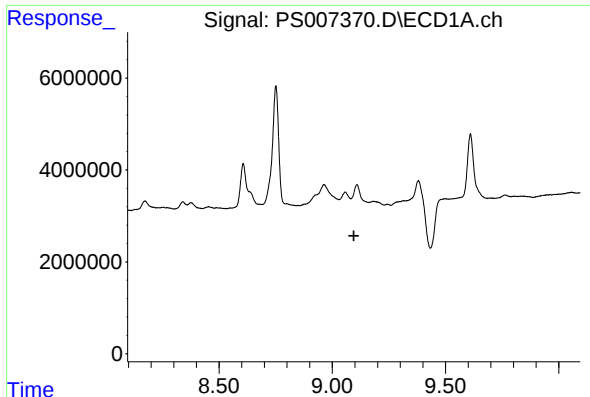

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

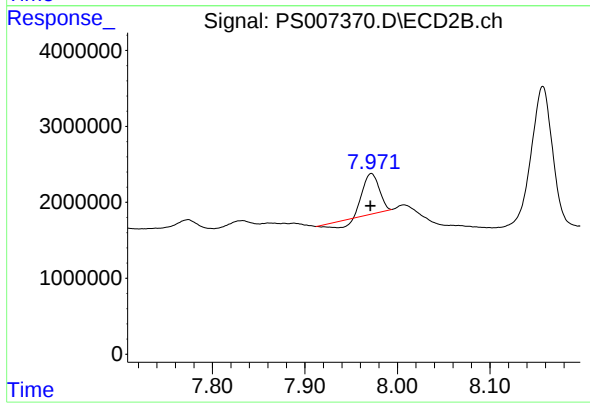

#14 DINOSEB

R.T.: 7.972 min
Delta R.T.: 0.001 min
Response: 5486999
Conc: 1.95 ng/ml